

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022819\
 Data File : PS003372.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2019 15:03
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 03:42:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.789	0	384817	N.D.	0.820 #
Target Compounds							
3) T	4-Nitroph...	0.000	9.914	0	68945	N.D.	0.307 #
5) T	DICAMBA	0.000	11.060	0	492686	N.D.	0.295 #
6) T	MCPD	0.000	11.317	0	82197	N.D.	0.070 #
7) T	MCPA	0.000	11.714	0	132326	N.D.	0.077 #
8) T	DICHLORPROP	0.000	12.193	0	50122	N.D.	0.121 #
9) T	2,4-D	0.000	12.677	0	228541	N.D.	0.435 #
10) T	Pentachlo...	0.000	13.193	0	230313	N.D.	0.035 #
11) T	2,4,5-TP ...	0.000	13.825	0	144868	N.D.	0.057 #
12) T	2,4,5-T	0.000	14.378	0	218510	N.D.	0.108 #
13) T	2,4-DB	0.000	14.997	0	739359	N.D.	2.895 #
14) T	DINOSEB	0.000	15.464	0	282822	N.D.	0.158 #
15) T	Picloram	0.000	16.680	0	735017	N.D.	0.290 #
16) T	DCPA	0.000	16.631	0	2622660	N.D.	0.843 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022819\
Data File : PS003372.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2019 15:03
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 03:42:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

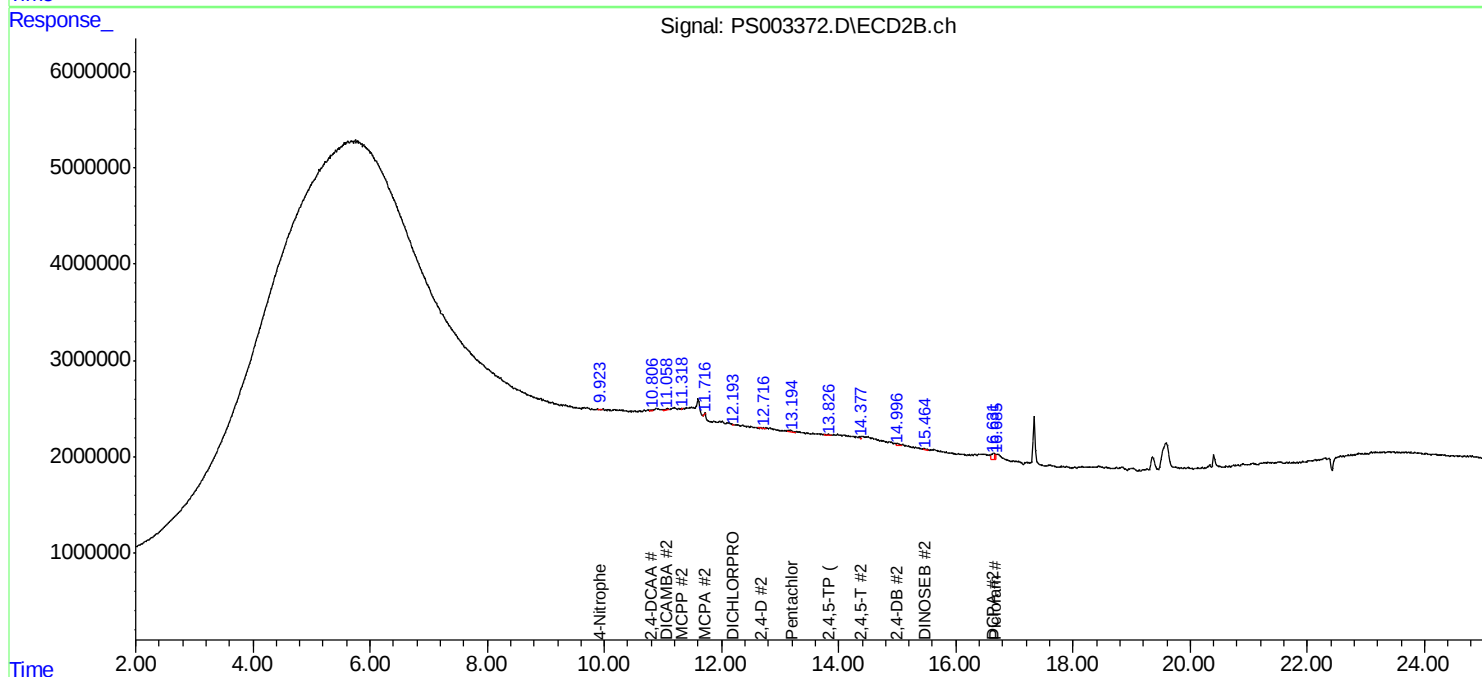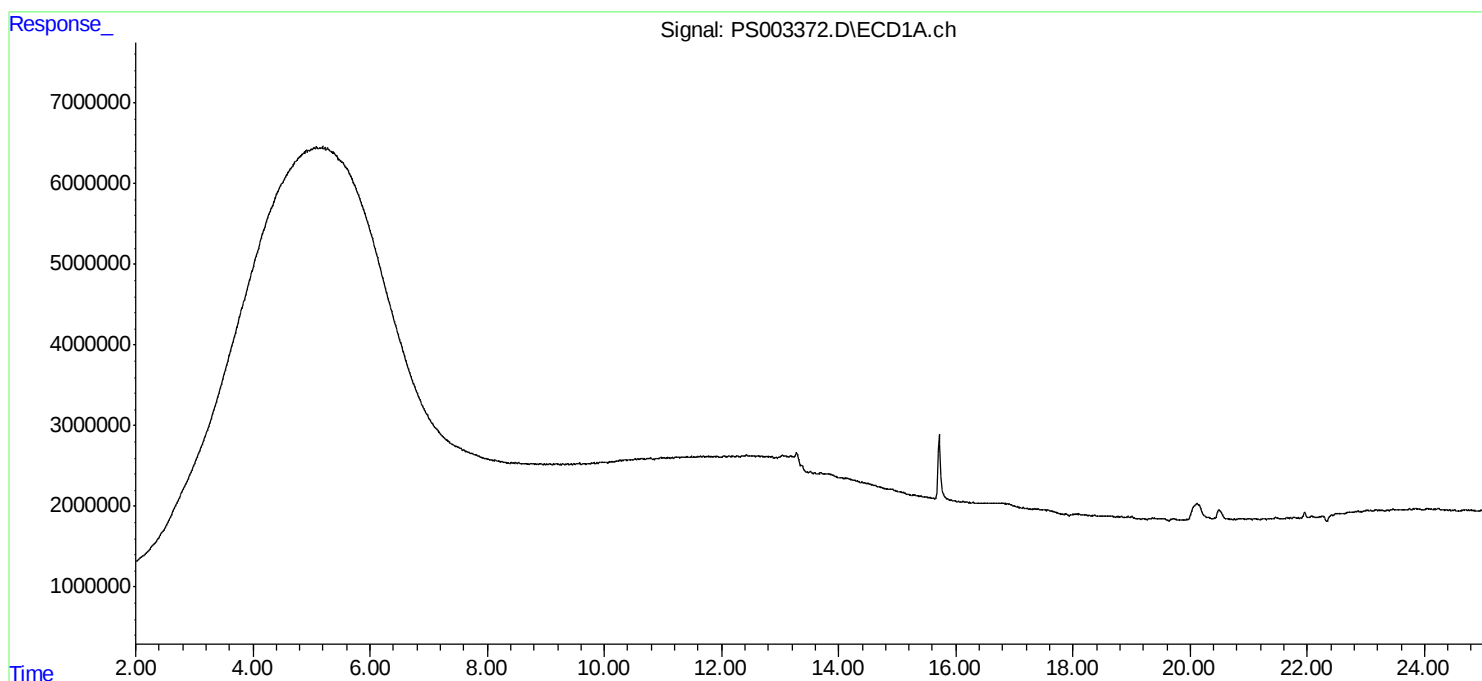


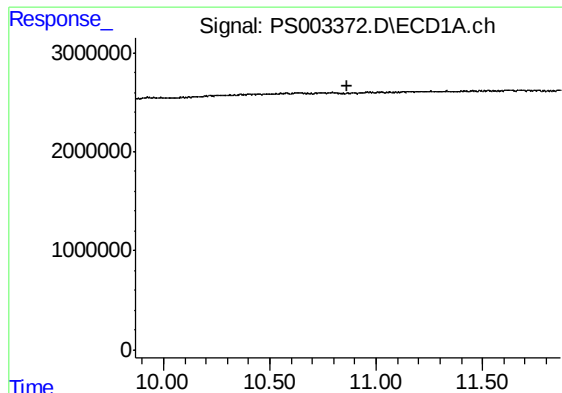

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

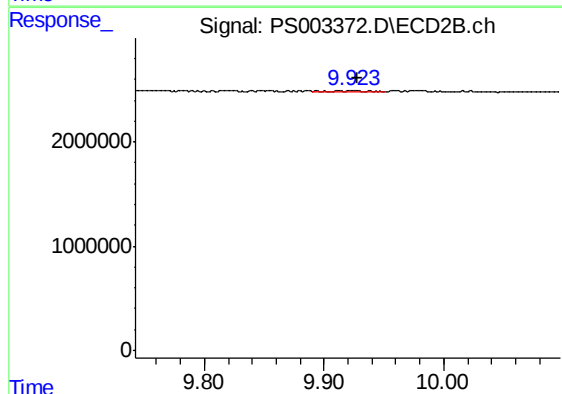


#3 4-Nitrophenol

R.T.: 9.914 min
Delta R.T.: -0.015 min
Response: 68945
Conc: 0.31 ng/ml

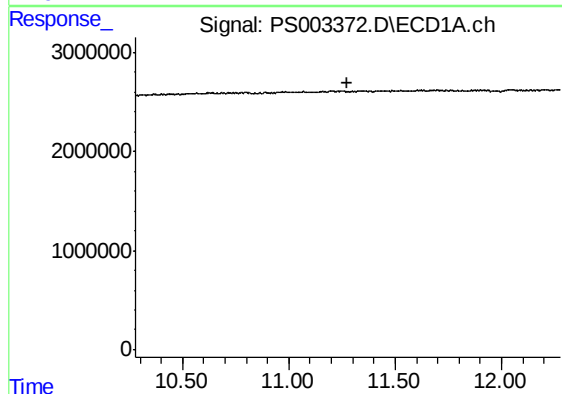


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 11.278 min
Response: 0
Conc: N.D.

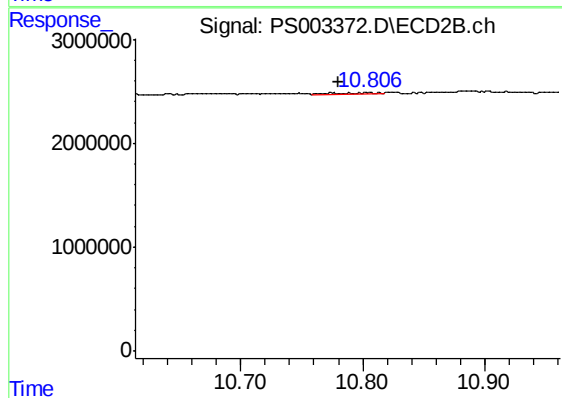

#4 2,4-DCAA


R.T.: 10.789 min
Delta R.T.: 0.010 min
Response: 384817
Conc: 0.82 ng/ml

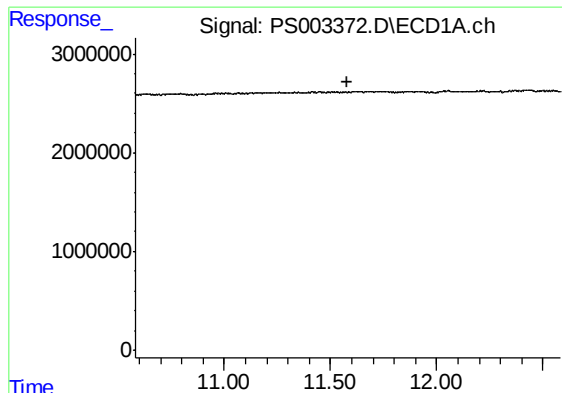

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

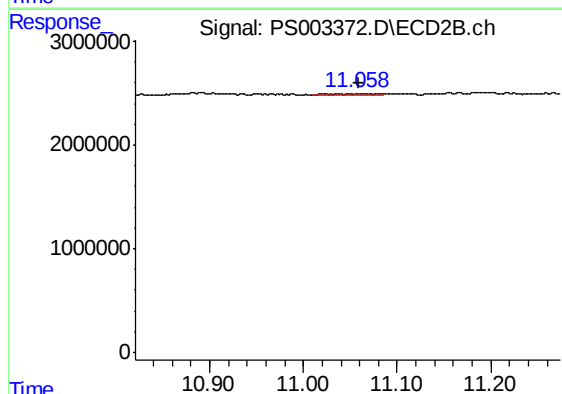


#5 DICAMBA

R.T.: 11.060 min
Delta R.T.: 0.000 min
Response: 492686
Conc: 0.29 ng/ml

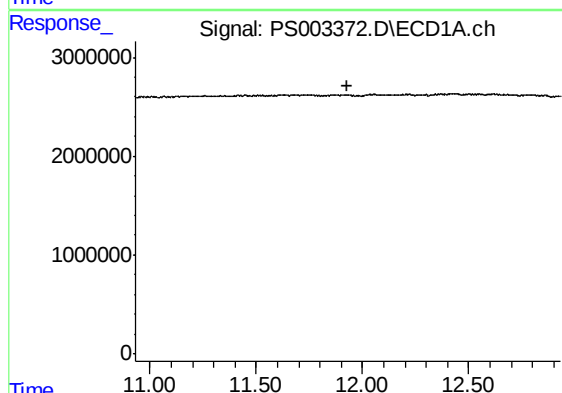


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.931 min
Response: 0
Conc: N.D.

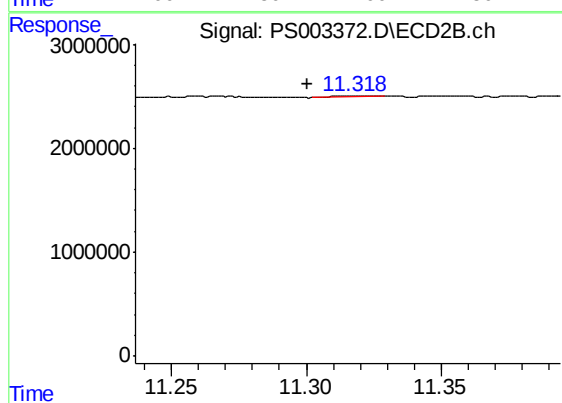

#6 MCPP


R.T.: 11.317 min
Delta R.T.: 0.017 min
Response: 82197
Conc: 0.07 ug/ml

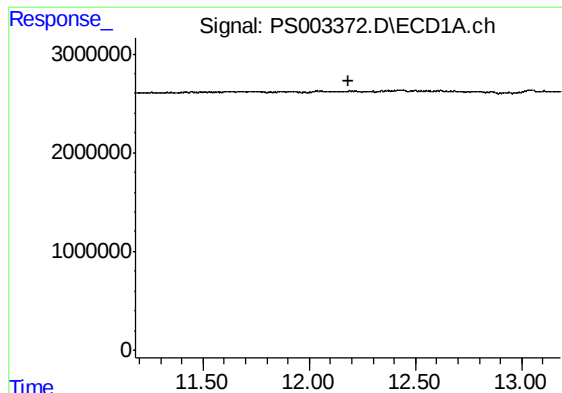

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

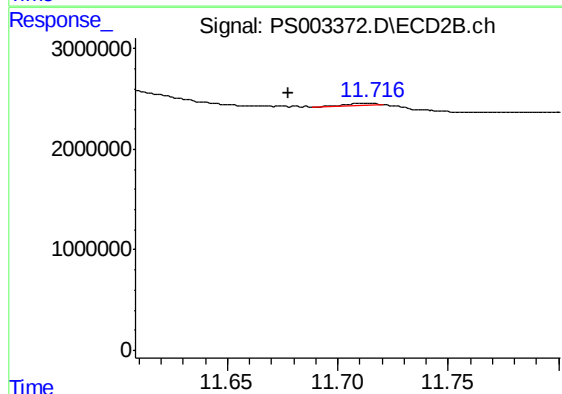


#7 MCPA

R.T.: 11.714 min
Delta R.T.: 0.037 min
Response: 132326
Conc: 0.08 ug/ml

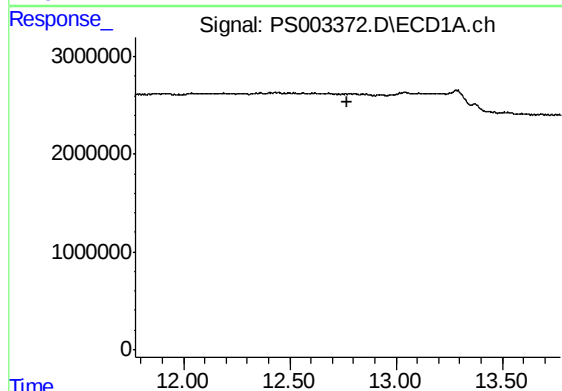


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.773 min
Response: 0
Conc: N.D.

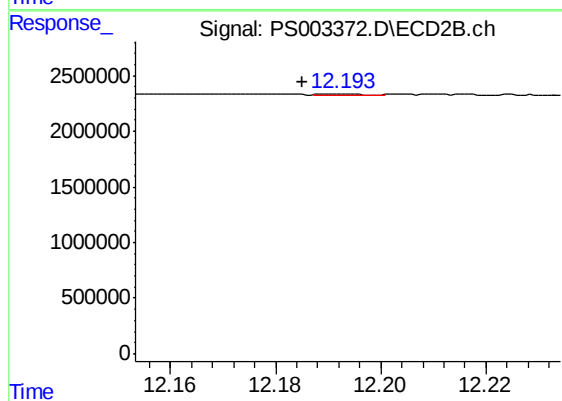

#8 DICHLORPROP


R.T.: 12.193 min
Delta R.T.: 0.008 min
Response: 50122
Conc: 0.12 ng/ml

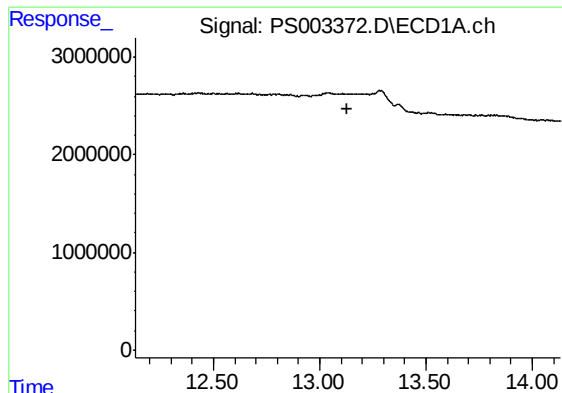

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 13.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

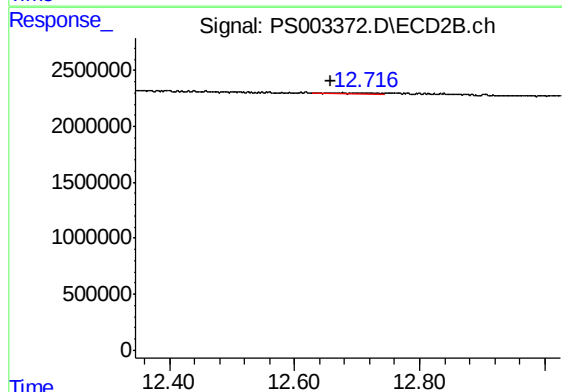


#9 2,4-D

R.T.: 12.677 min
Delta R.T.: 0.020 min
Response: 228541
Conc: 0.44 ng/ml

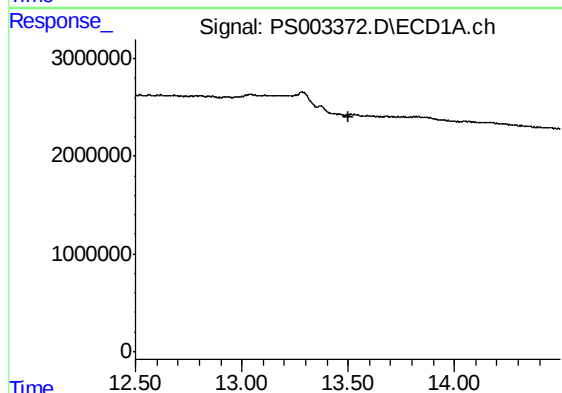


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.499 min
Response: 0
Conc: N.D.

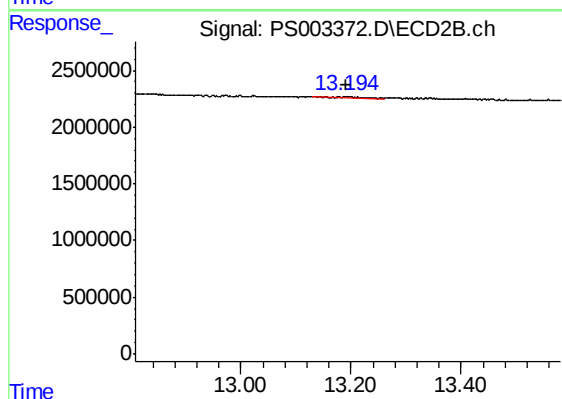

#10 Pentachlorophenol


R.T.: 13.193 min
Delta R.T.: 0.002 min
Response: 230313
Conc: 0.03 ng/ml

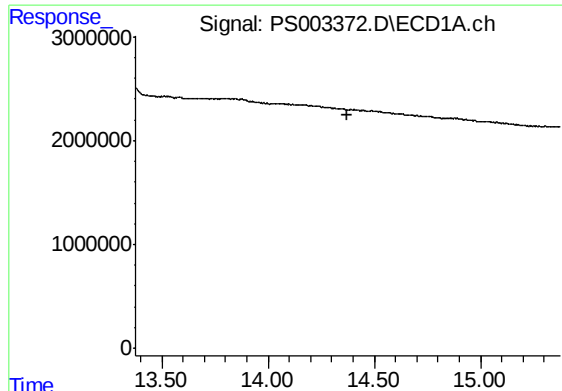

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

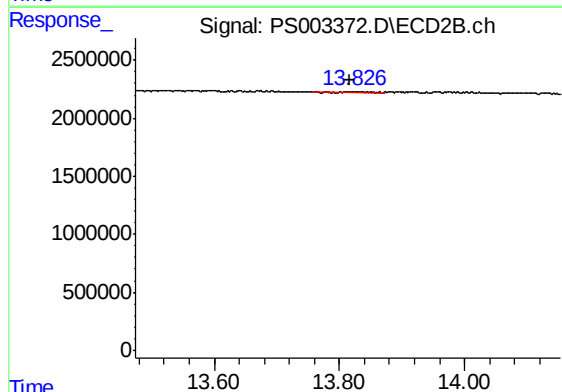


#11 2,4,5-TP (SILVEX)

R.T.: 13.825 min
Delta R.T.: 0.007 min
Response: 144868
Conc: 0.06 ng/ml

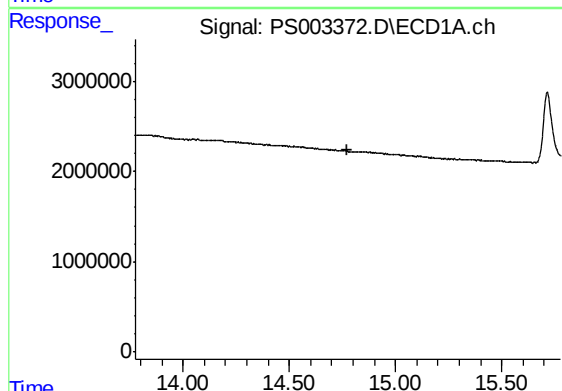


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

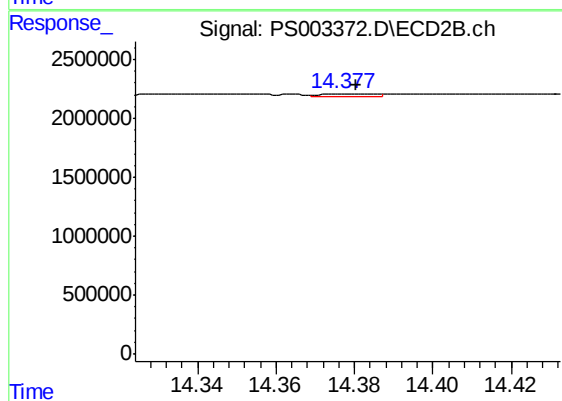

#12 2,4,5-T


R.T.: 14.378 min
Delta R.T.: -0.003 min
Response: 218510
Conc: 0.11 ng/ml

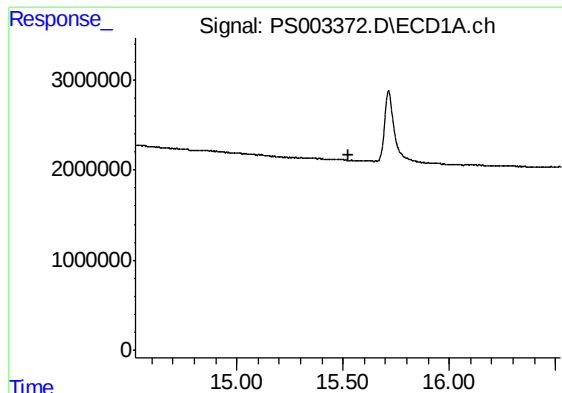

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

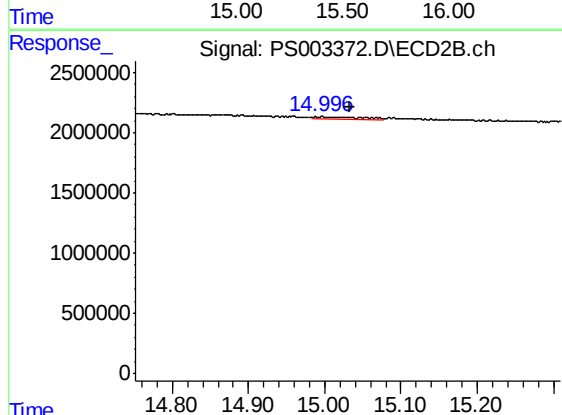


#13 2,4-DB

R.T.: 14.997 min
Delta R.T.: -0.036 min
Response: 739359
Conc: 2.90 ng/ml

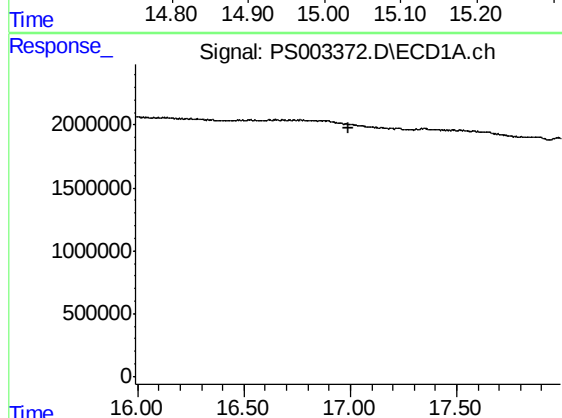


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

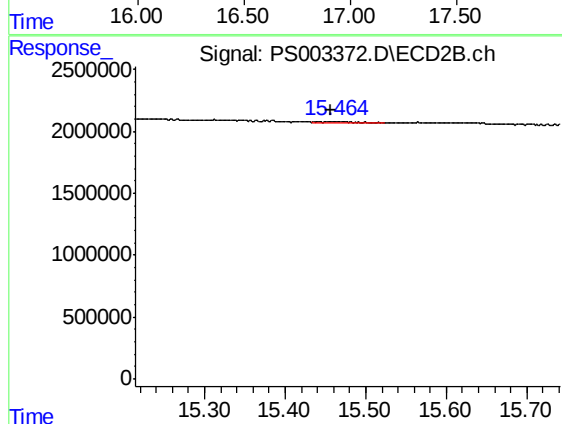

#14 DINOSEB


R.T.: 15.464 min
Delta R.T.: 0.007 min
Response: 282822
Conc: 0.16 ng/ml

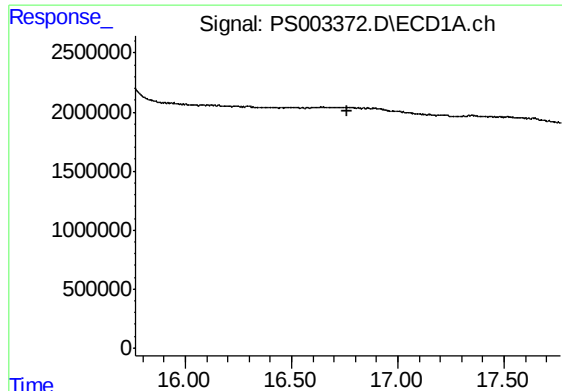

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

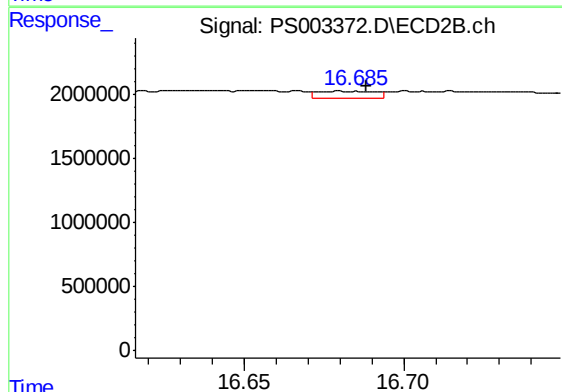


#15 Picloram

R.T.: 16.680 min
Delta R.T.: -0.008 min
Response: 735017
Conc: 0.29 ng/ml

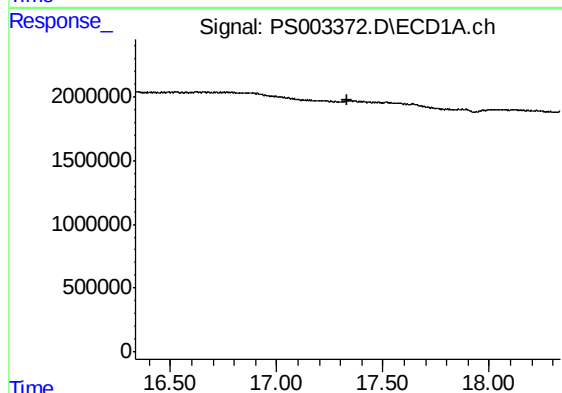

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

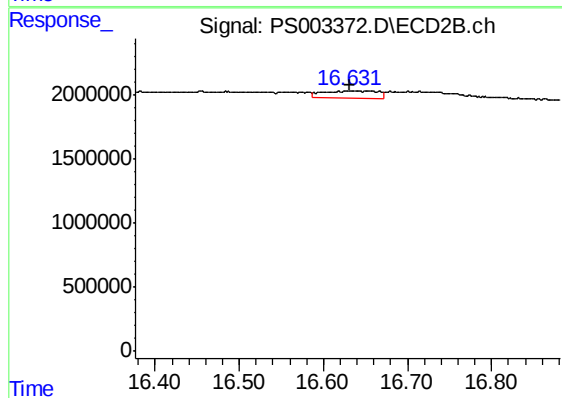

#16 DCPA

R.T.: 16.631 min
Delta R.T.: -0.001 min
Response: 2622660
Conc: 0.84 ng/ml