

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022819\
 Data File : PS003380.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2019 19:14
 Operator : EI\SJ
 Sample : K1596-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-14

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 03:44:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.276	10.777	40737463	42319345	92.791	90.124
Target Compounds							
1) T	Dalapon	2.792	2.275	40234986	2885299	61.905	4.557 #
2) T	3,5-DICHL...	0.000	8.938	0	160205	N.D.	0.259 #
3) T	4-Nitroph...	0.000	9.995	0	6191436	N.D.	27.539 #
5) T	DICAMBA	0.000	11.060	0	2723970	N.D.	1.630 #
6) T	MCPD	11.953	11.295	2734381	2206401	2.083	1.869
7) T	MCPA	0.000	11.676	0	544084	N.D.	0.315 #
8) T	DICHLORPROP	12.835	12.185	2502965	7794746	5.785	18.862 #
9) T	2,4-D	13.179	12.626	4506464	5787217	9.716	11.026
10) T	Pentachlo...	13.496	13.185	6729557	4160921	0.953	0.632 #
11) T	2,4,5-TP ...	0.000	13.784	0	2534996	N.D.	0.996 #
12) T	2,4,5-T	14.807	14.375	9387743	31195160	3.554	15.468 #
13) T	2,4-DB	15.549	15.033	196.0E6	125.6E6	827.534	491.665 #
14) T	DINOSEB	0.000	15.441	0	12277204	N.D.	6.879 #
15) T	Picloram	16.749	16.736	3140065	53257421	1.276	20.983 #
16) T	DCPA	17.291	0.000	15422002	0	4.680	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022819\
Data File : PS003380.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2019 19:14
Operator : EI\SJ
Sample : K1596-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-14

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 03:44:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

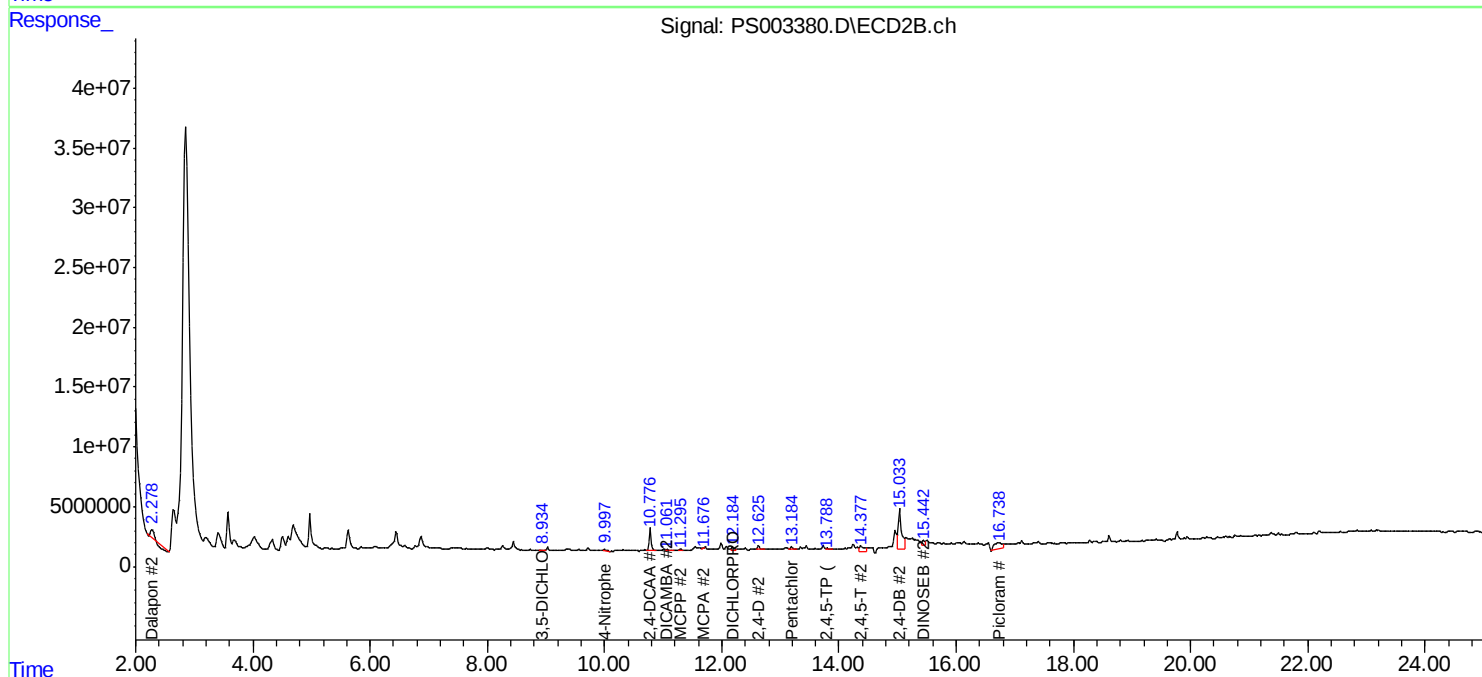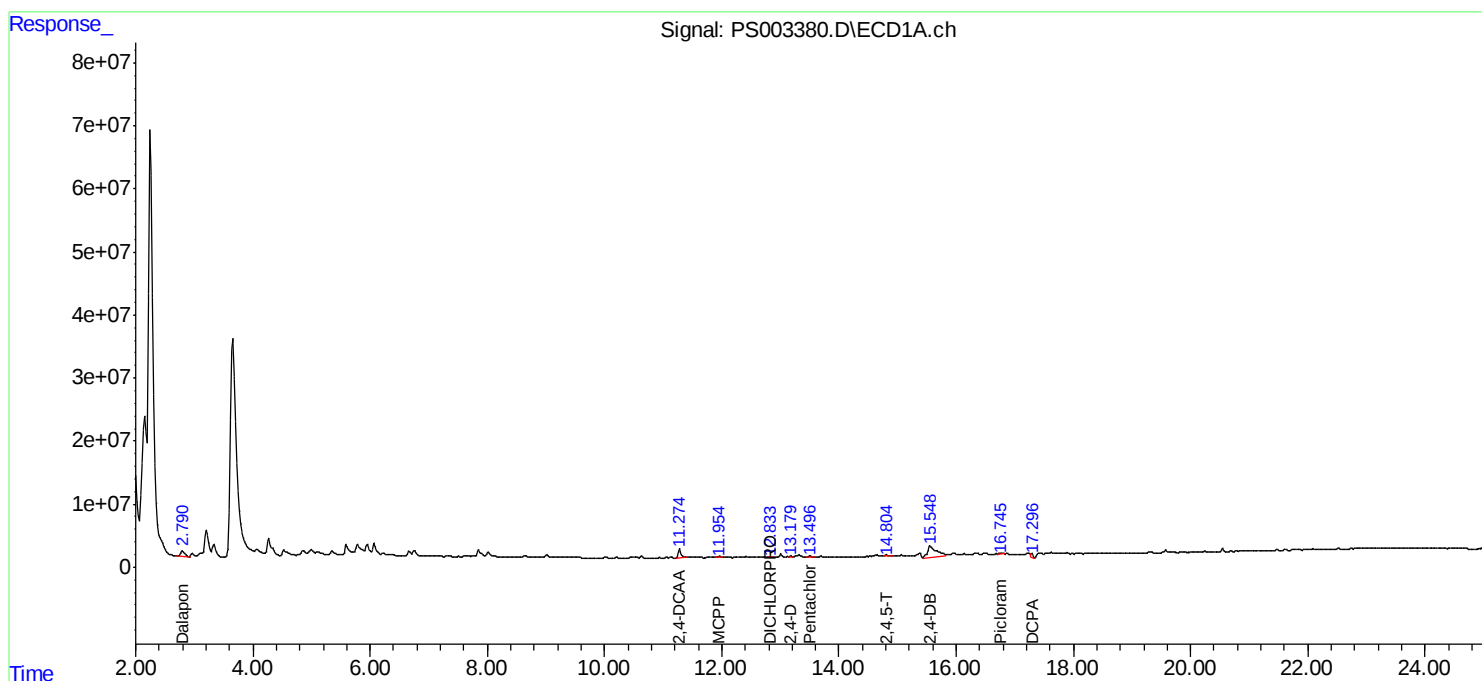


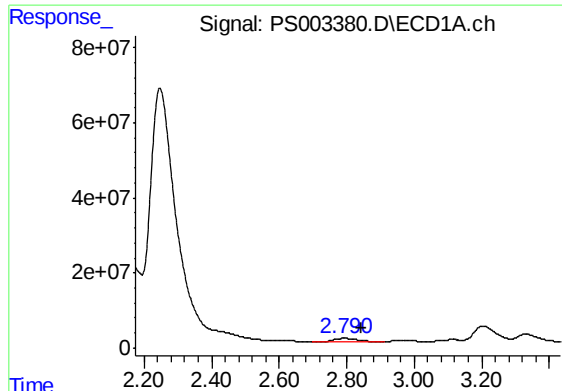

#1 Dalapon


R.T.: 2.792 min
Delta R.T.: -0.052 min
Response: 40234986
Conc: 61.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-14

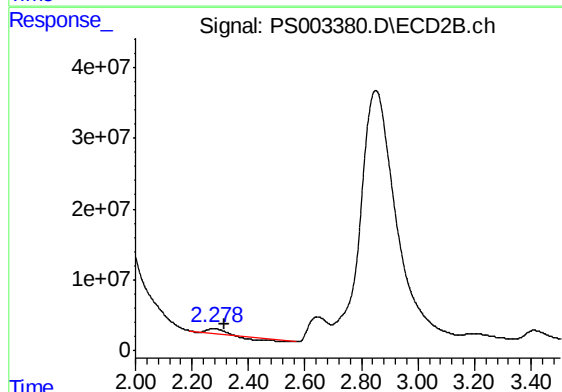


#1 Dalapon

R.T.: 2.275 min
Delta R.T.: -0.041 min
Response: 2885299
Conc: 4.56 ng/ml

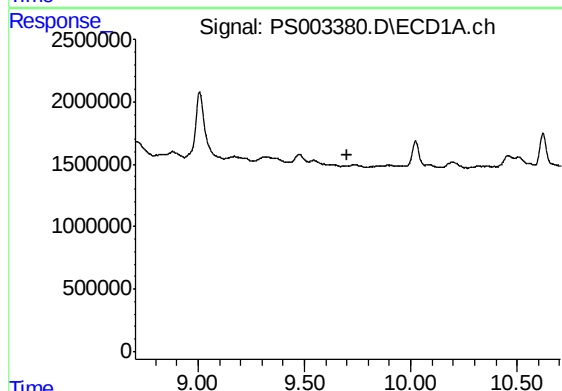


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

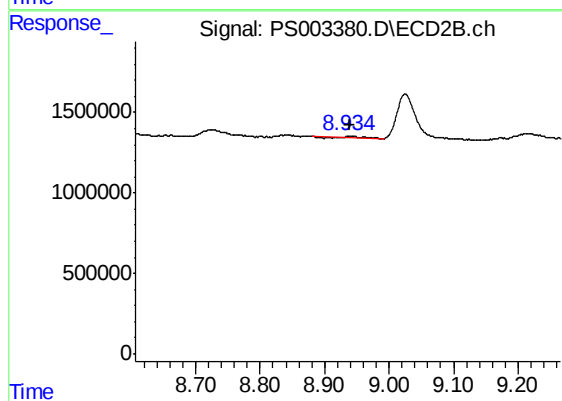

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.938 min
Delta R.T.: -0.002 min
Response: 160205
Conc: 0.26 ng/ml

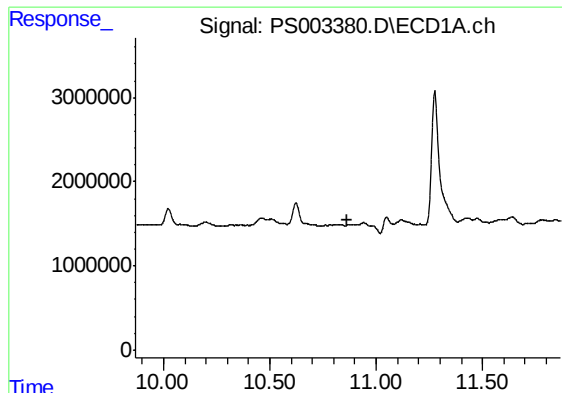

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-14

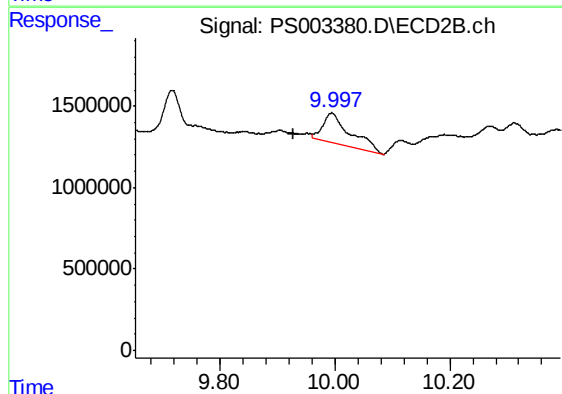


#3 4-Nitrophenol

R.T.: 9.995 min
Delta R.T.: 0.066 min
Response: 6191436
Conc: 27.54 ng/ml

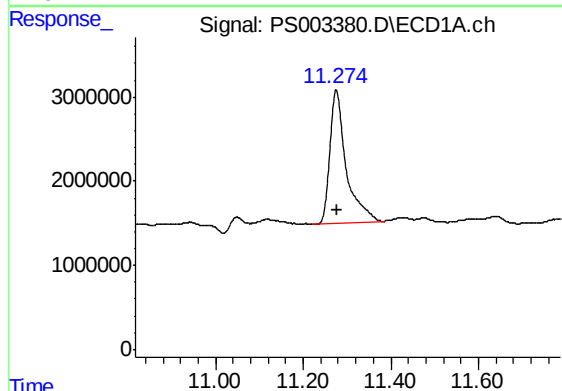


#4 2,4-DCAA

R.T.: 11.276 min
Delta R.T.: -0.002 min
Response: 40737463
Conc: 92.79 ng/ml

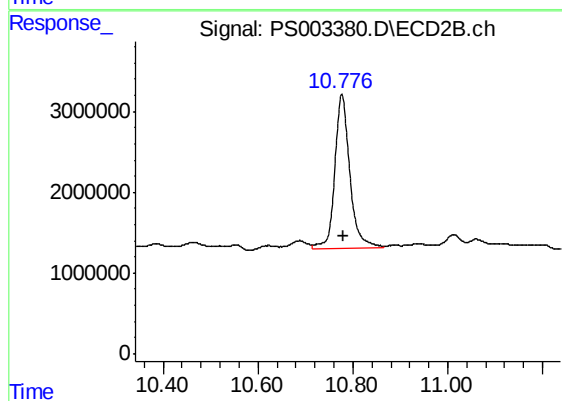

#4 2,4-DCAA


R.T.: 10.777 min
Delta R.T.: -0.003 min
Response: 42319345
Conc: 90.12 ng/ml

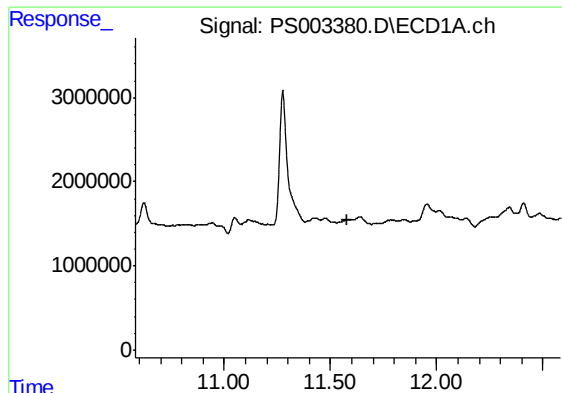

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-14

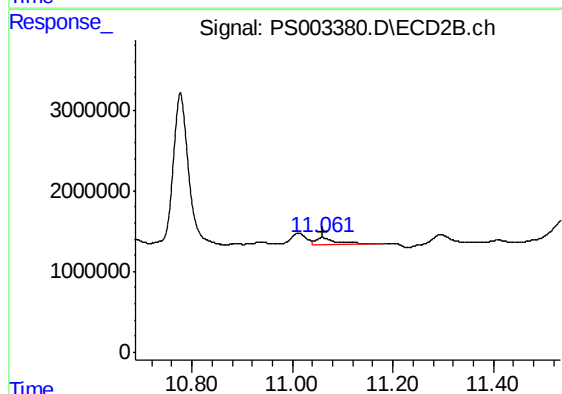


#5 DICAMBA

R.T.: 11.060 min
Delta R.T.: 0.000 min
Response: 2723970
Conc: 1.63 ng/ml

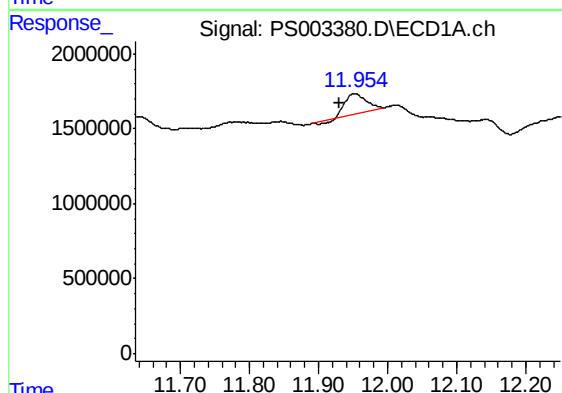


#6 MCPP

R.T.: 11.953 min
Delta R.T.: 0.022 min
Response: 2734381
Conc: 2.08 ug/ml

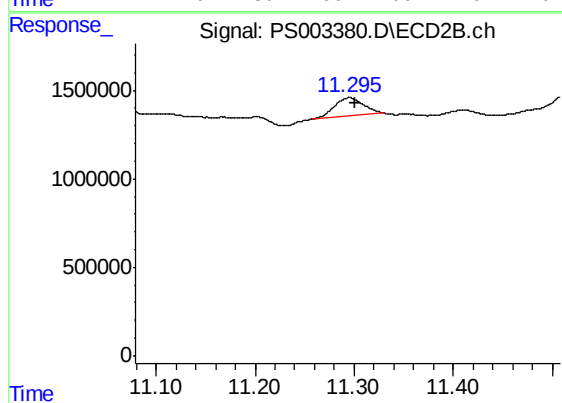

#6 MCPP


R.T.: 11.295 min
Delta R.T.: -0.005 min
Response: 2206401
Conc: 1.87 ug/ml

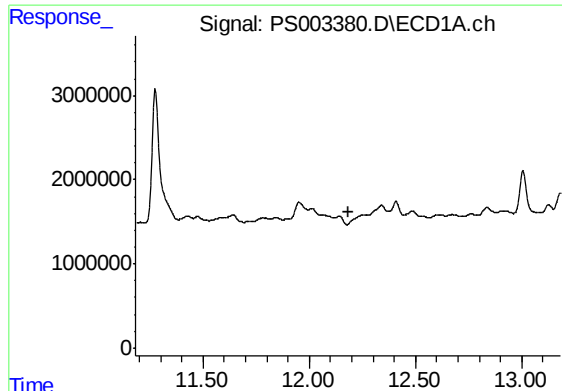

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-14

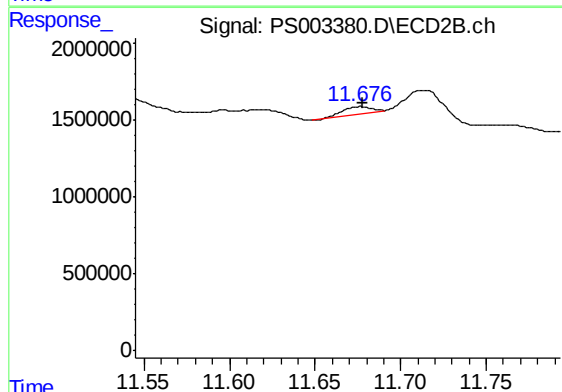


#7 MCPA

R.T.: 11.676 min
Delta R.T.: -0.001 min
Response: 544084
Conc: 0.32 ug/ml

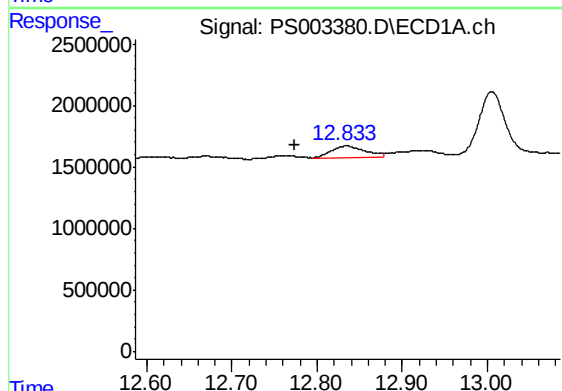


#8 DICHLORPROP

R.T.: 12.835 min
Delta R.T.: 0.061 min
Response: 2502965
Conc: 5.79 ng/ml

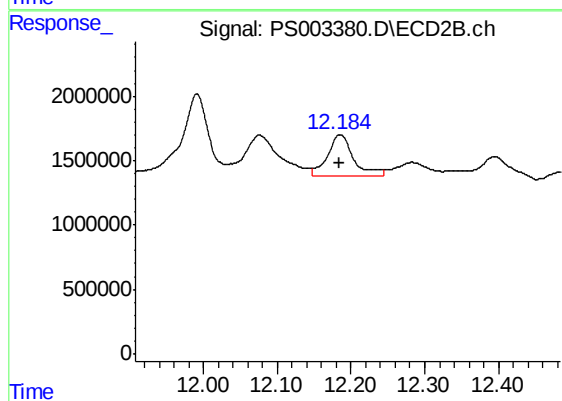

#8 DICHLORPROP


R.T.: 12.185 min
Delta R.T.: 0.000 min
Response: 7794746
Conc: 18.86 ng/ml

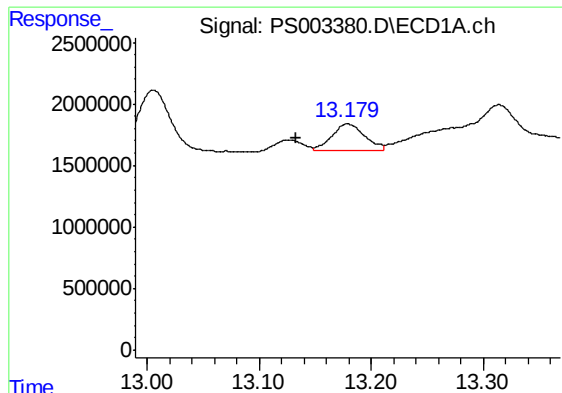

#9 2,4-D


R.T.: 13.179 min
Delta R.T.: 0.047 min
Response: 4506464
Conc: 9.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-14

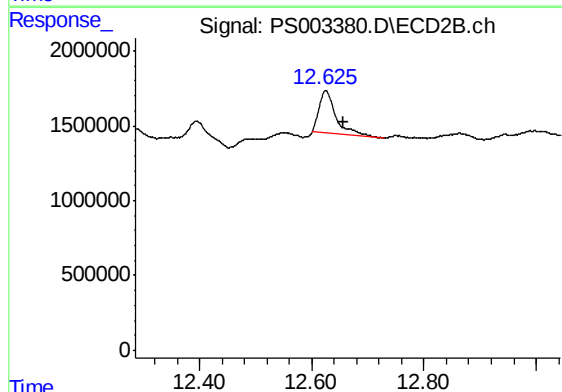


#9 2,4-D

R.T.: 12.626 min
Delta R.T.: -0.031 min
Response: 5787217
Conc: 11.03 ng/ml

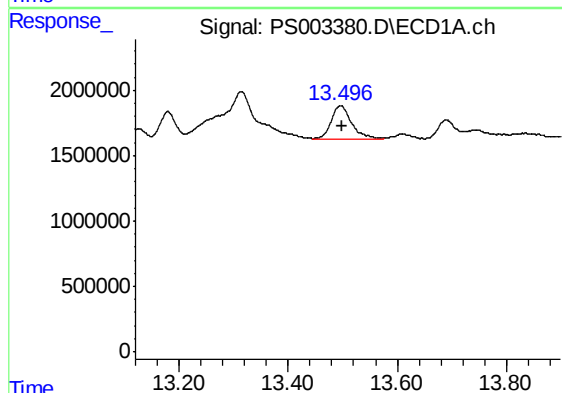


#10 Pentachlorophenol

R.T.: 13.496 min
Delta R.T.: -0.003 min
Response: 6729557
Conc: 0.95 ng/ml

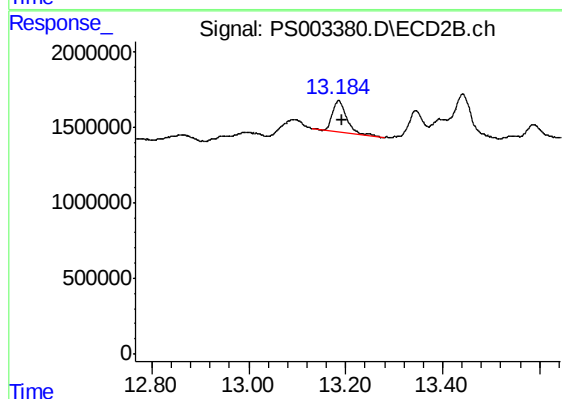

#10 Pentachlorophenol


R.T.: 13.185 min
Delta R.T.: -0.006 min
Response: 4160921
Conc: 0.63 ng/ml

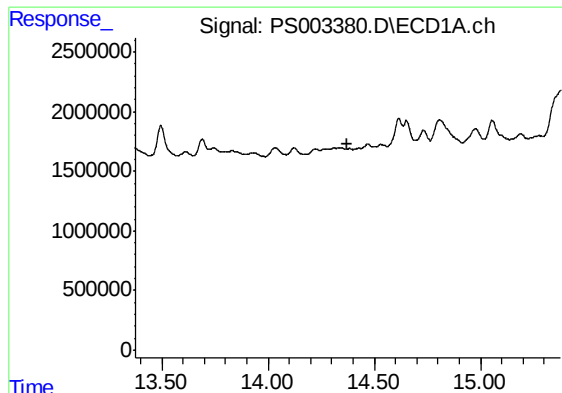

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-14

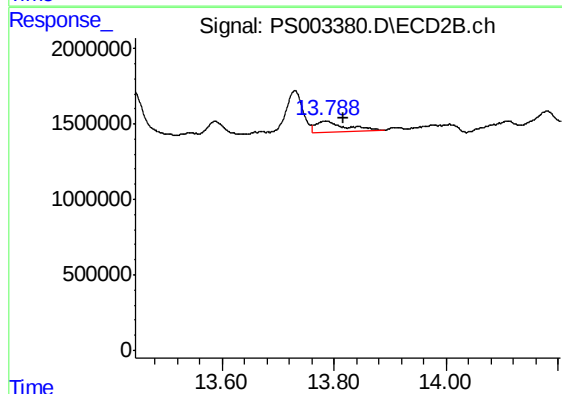


#11 2,4,5-TP (SILVEX)

R.T.: 13.784 min
Delta R.T.: -0.033 min
Response: 2534996
Conc: 1.00 ng/ml

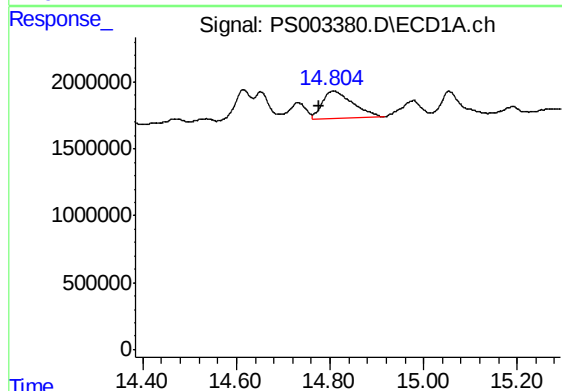


#12 2,4,5-T

R.T.: 14.807 min
Delta R.T.: 0.031 min
Response: 9387743
Conc: 3.55 ng/ml

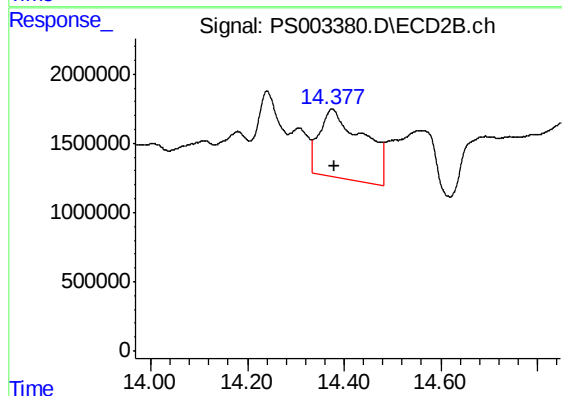

#12 2,4,5-T


R.T.: 14.375 min
Delta R.T.: -0.005 min
Response: 31195160
Conc: 15.47 ng/ml

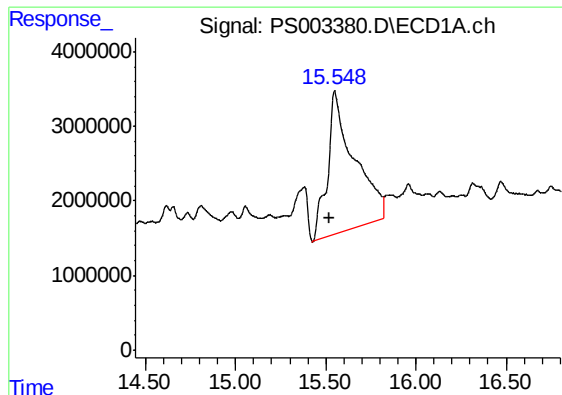

#13 2,4-DB


R.T.: 15.549 min
Delta R.T.: 0.026 min
Response: 195956455
Conc: 827.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-14

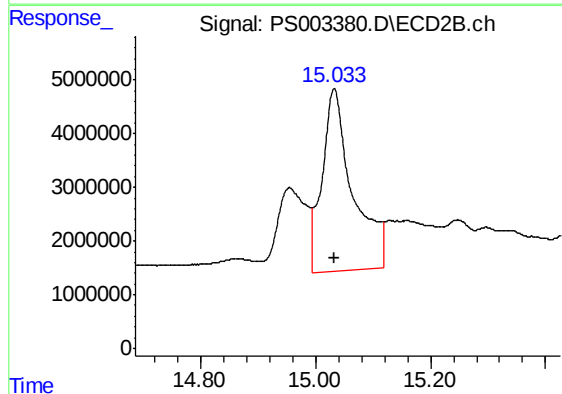


#13 2,4-DB

R.T.: 15.033 min
Delta R.T.: 0.000 min
Response: 125550029
Conc: 491.66 ng/ml

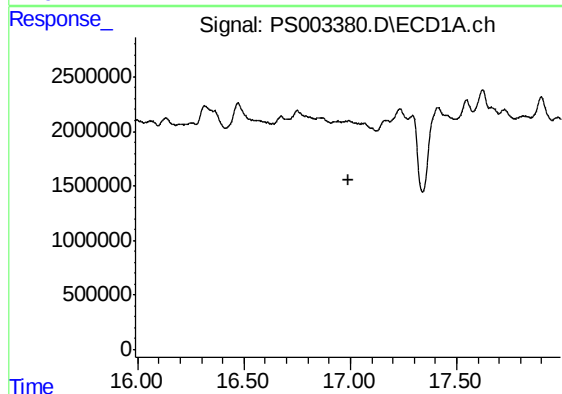


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

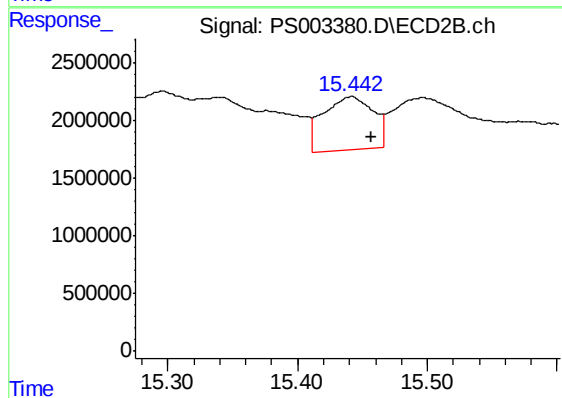

#14 DINOSEB


R.T.: 15.441 min
Delta R.T.: -0.016 min
Response: 12277204
Conc: 6.88 ng/ml

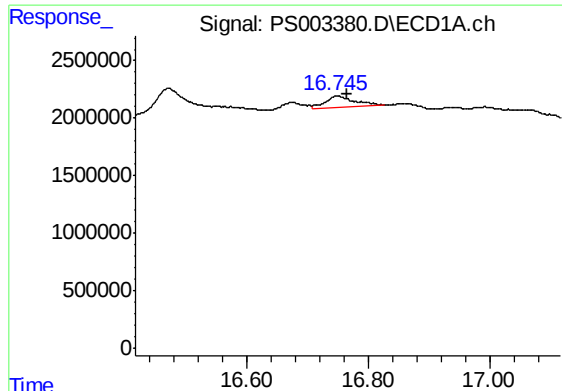

#15 Picloram


R.T.: 16.749 min
Delta R.T.: -0.016 min
Response: 3140065
Conc: 1.28 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-14

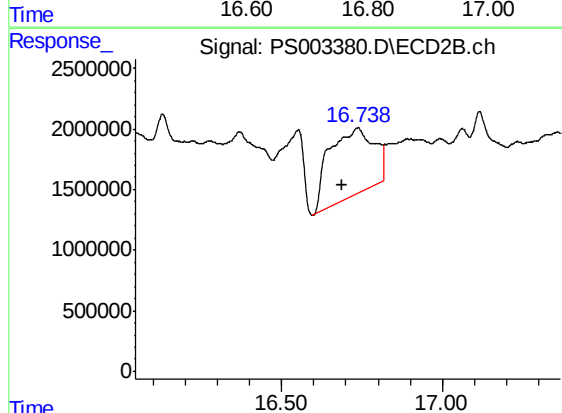


#15 Picloram

R.T.: 16.736 min
Delta R.T.: 0.048 min
Response: 53257421
Conc: 20.98 ng/ml

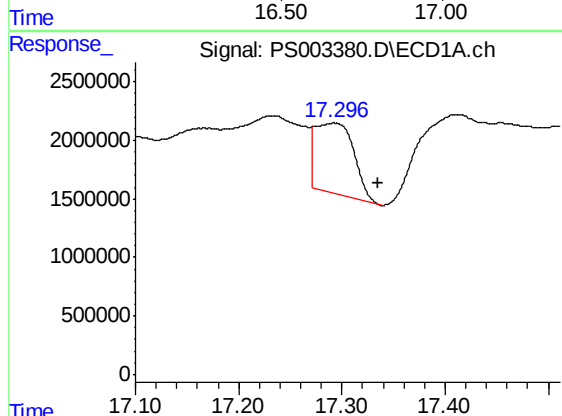

#16 DCPA

R.T.: 17.291 min
Delta R.T.: -0.044 min
Response: 15422002
Conc: 4.68 ng/ml

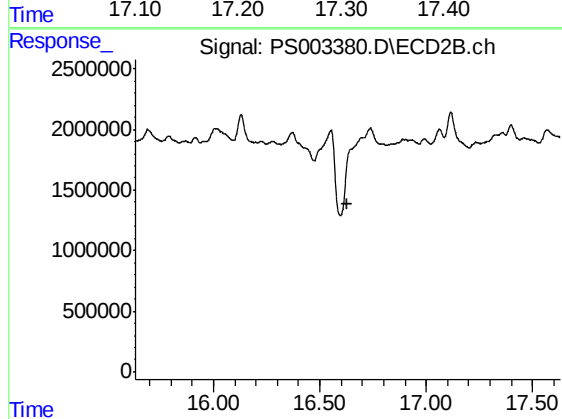

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 16.632 min
Response: 0
Conc: N.D.