

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022819\
 Data File : PS003381.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2019 19:45
 Operator : EI\SJ
 Sample : K1596-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-15

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 03:44:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.274	10.777	76609611	67958127	174.500	144.724
Target Compounds							
1) T	Dalapon	2.793	2.268	34249363	-18500342	52.696	N.D. #
2) T	3,5-DICHL...	0.000	8.954	0	320638	N.D.	0.519 #
3) T	4-Nitroph...	0.000	9.950	0	856868	N.D.	3.811 #
5) T	DICAMBA	11.636	11.062	9179969	2248256	5.208	1.346 #
6) T	MCPD	11.949	11.291	6915277	3807183	5.267	3.225 #
7) T	MCPA	0.000	11.678	0	1378319	N.D.	0.799 #
8) T	DICHLORPROP	12.834	12.186	5500068	8507459	12.712	20.587 #
9) T	2,4-D	13.127	12.625	2344583	5545661	5.055	10.565 #
10) T	Pentachlo...	13.498	13.187	9947269	5121724	1.408	0.778 #
11) T	2,4,5-TP ...	0.000	13.789	0	2155400	N.D.	0.846 #
12) T	2,4,5-T	14.799	14.374	10328752	19890510	3.910	9.863 #
13) T	2,4-DB	15.545	15.030	245.4E6	165.2E6	1036.151	646.759 #
14) T	DINOSEB	0.000	15.441	0	15404184	N.D.	8.630 #
15) T	Picloram	16.751	16.738	55127316	57312690	22.398	22.581
16) T	DCPA	17.290	0.000	19793566	0	6.007	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022819\
Data File : PS003381.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2019 19:45
Operator : EI\SJ
Sample : K1596-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-15

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 03:44:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

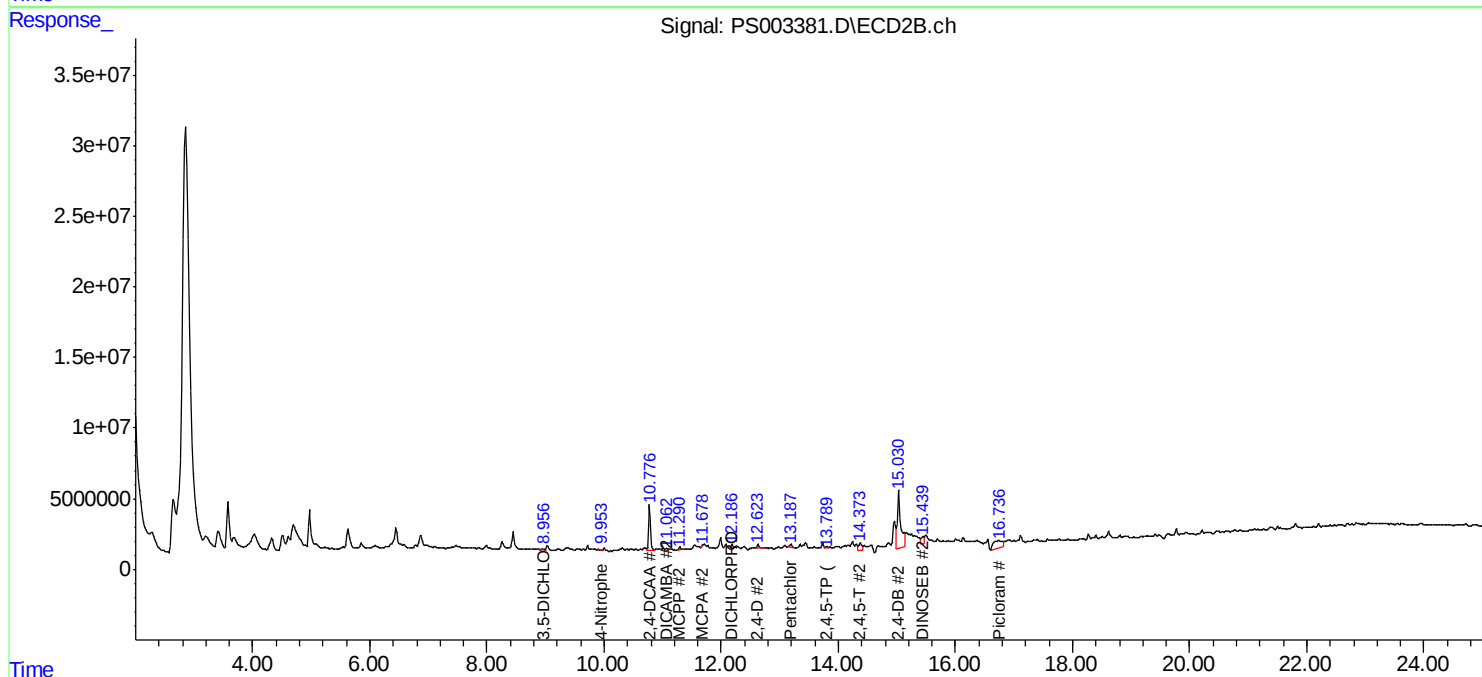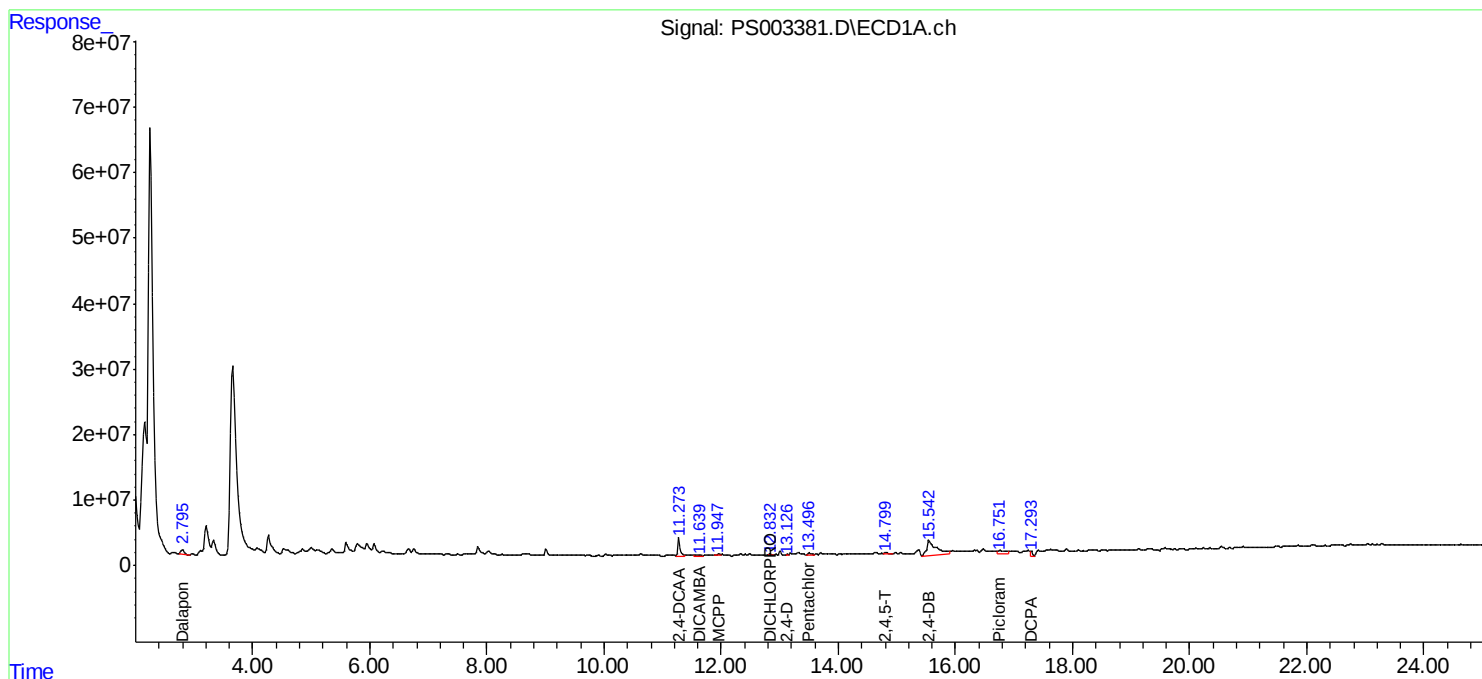


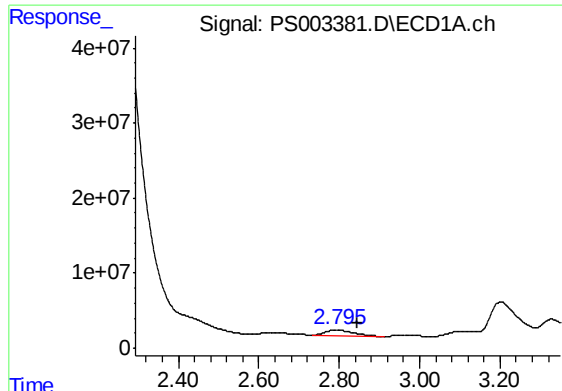

#1 Dalapon


R.T.: 2.793 min
Delta R.T.: -0.051 min
Response: 34249363
Conc: 52.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-15

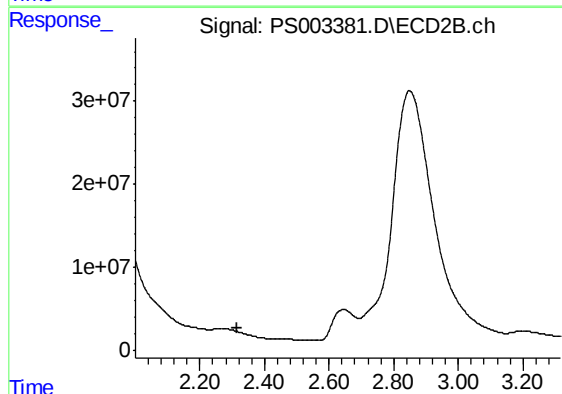


#1 Dalapon

R.T.: 2.268 min
Delta R.T.: -0.048 min
Response: -18500342
Conc: N.D.

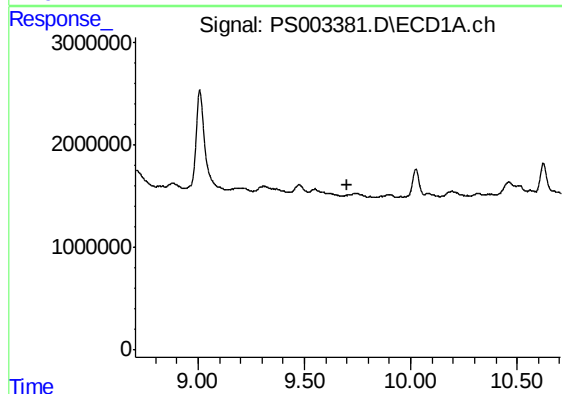


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

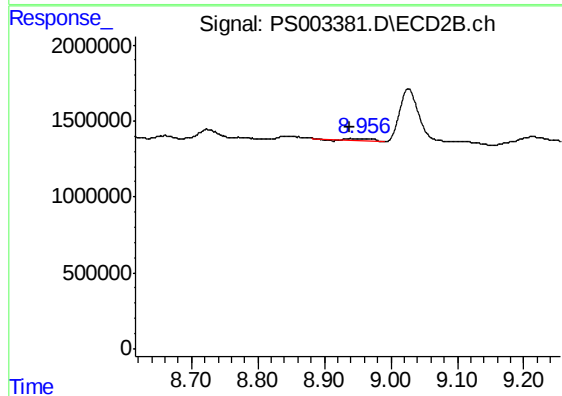

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.954 min
Delta R.T.: 0.015 min
Response: 320638
Conc: 0.52 ng/ml

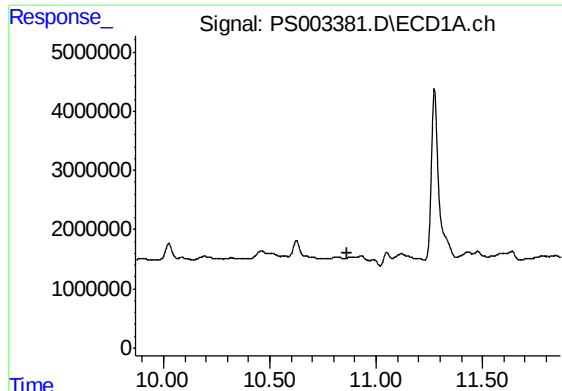

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-15

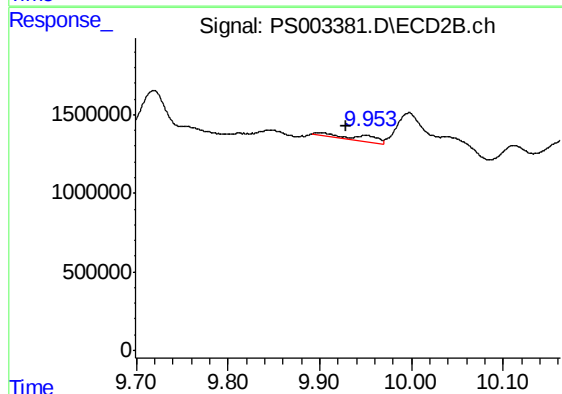


#3 4-Nitrophenol

R.T.: 9.950 min
Delta R.T.: 0.022 min
Response: 856868
Conc: 3.81 ng/ml

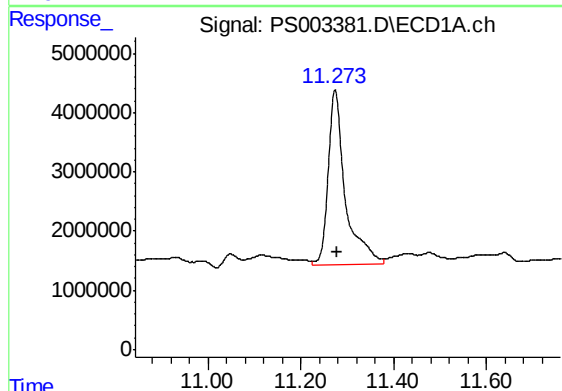


#4 2,4-DCAA

R.T.: 11.274 min
Delta R.T.: -0.003 min
Response: 76609611
Conc: 174.50 ng/ml

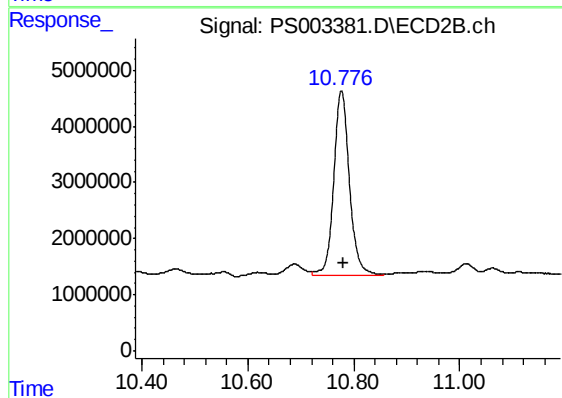

#4 2,4-DCAA


R.T.: 10.777 min
Delta R.T.: -0.003 min
Response: 67958127
Conc: 144.72 ng/ml

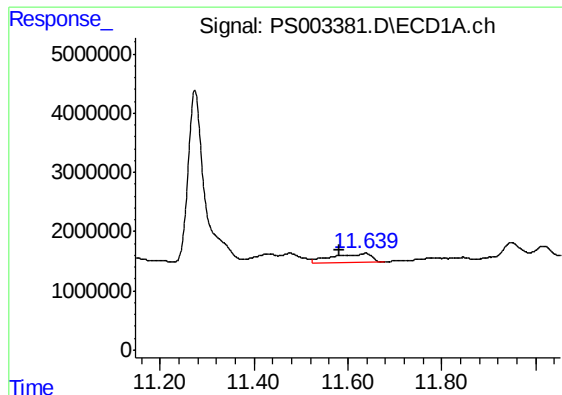

#5 DICAMBA


R.T.: 11.636 min
Delta R.T.: 0.054 min
Response: 9179969
Conc: 5.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-15

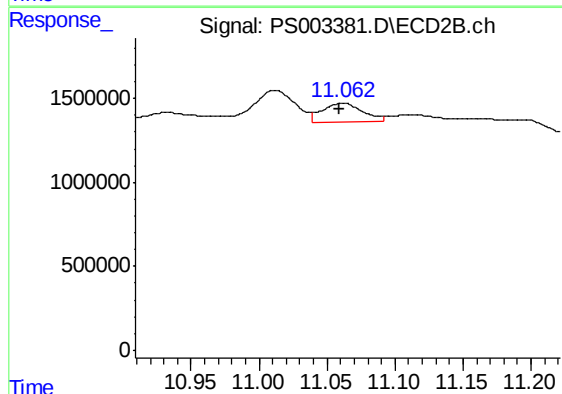


#5 DICAMBA

R.T.: 11.062 min
Delta R.T.: 0.002 min
Response: 2248256
Conc: 1.35 ng/ml

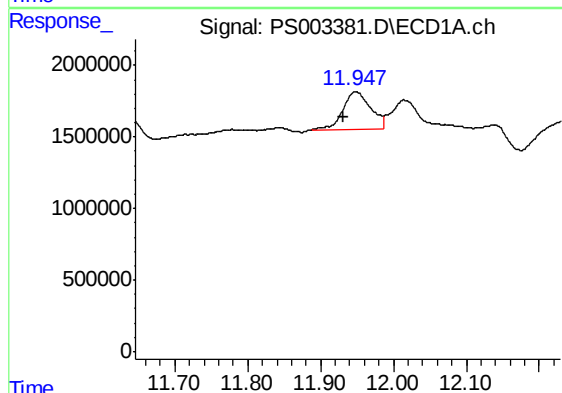


#6 MCPP

R.T.: 11.949 min
Delta R.T.: 0.018 min
Response: 6915277
Conc: 5.27 ug/ml

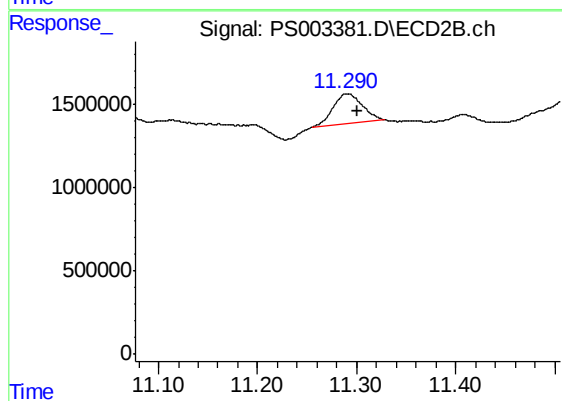

#6 MCPP


R.T.: 11.291 min
Delta R.T.: -0.010 min
Response: 3807183
Conc: 3.23 ug/ml

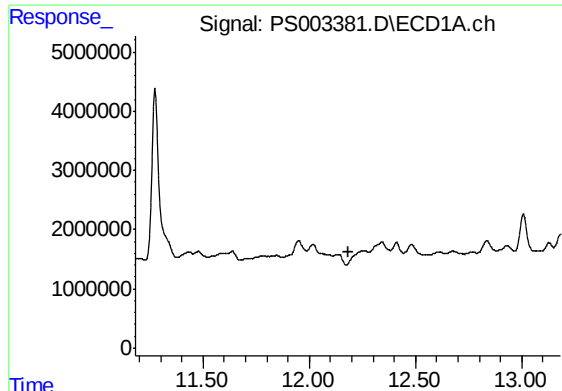

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-15

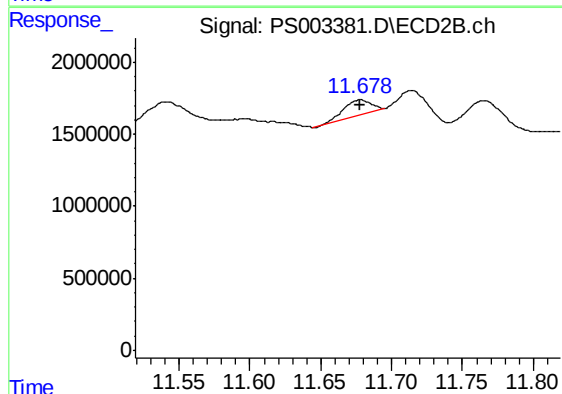


#7 MCPA

R.T.: 11.678 min
Delta R.T.: 0.000 min
Response: 1378319
Conc: 0.80 ug/ml

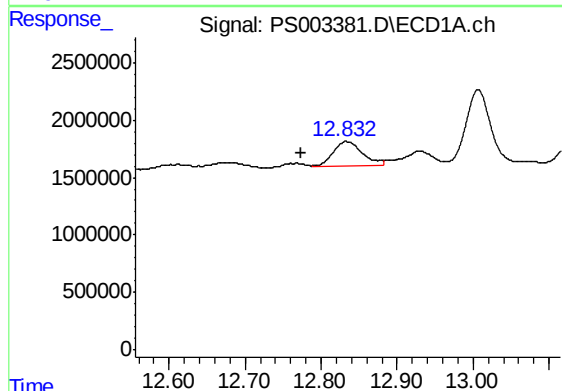


#8 DICHLORPROP

R.T.: 12.834 min
Delta R.T.: 0.061 min
Response: 5500068
Conc: 12.71 ng/ml

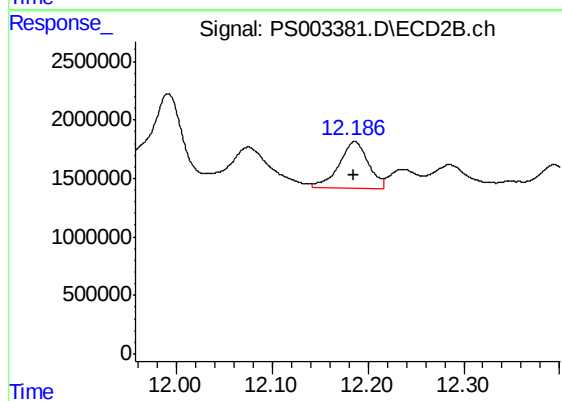

#8 DICHLORPROP


R.T.: 12.186 min
Delta R.T.: 0.001 min
Response: 8507459
Conc: 20.59 ng/ml

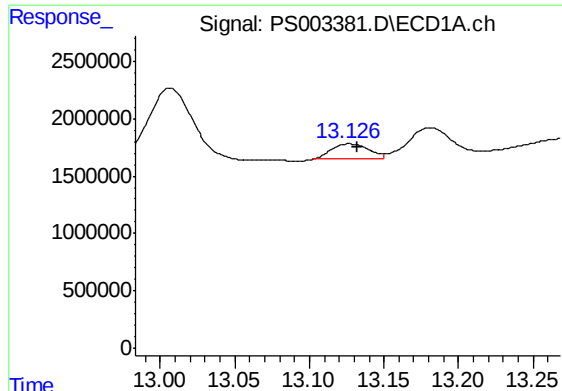

#9 2,4-D


R.T.: 13.127 min
Delta R.T.: -0.005 min
Response: 2344583
Conc: 5.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-15

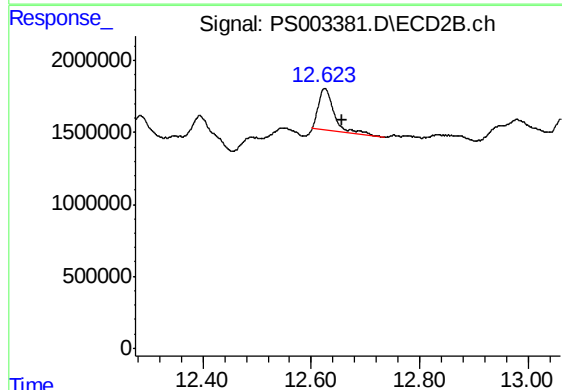


#9 2,4-D

R.T.: 12.625 min
Delta R.T.: -0.032 min
Response: 5545661
Conc: 10.57 ng/ml

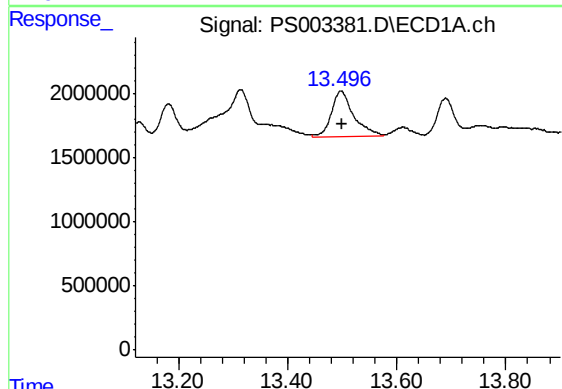


#10 Pentachlorophenol

R.T.: 13.498 min
Delta R.T.: -0.001 min
Response: 9947269
Conc: 1.41 ng/ml

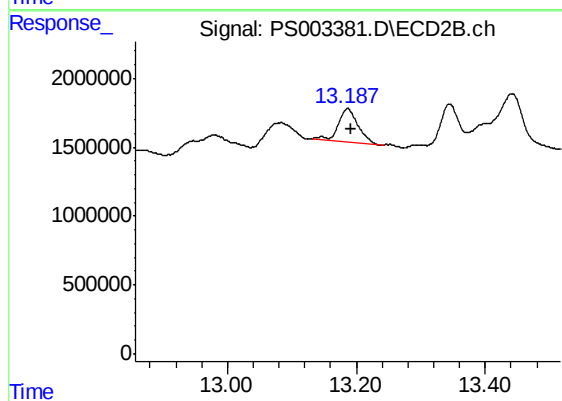

#10 Pentachlorophenol


R.T.: 13.187 min
Delta R.T.: -0.005 min
Response: 5121724
Conc: 0.78 ng/ml

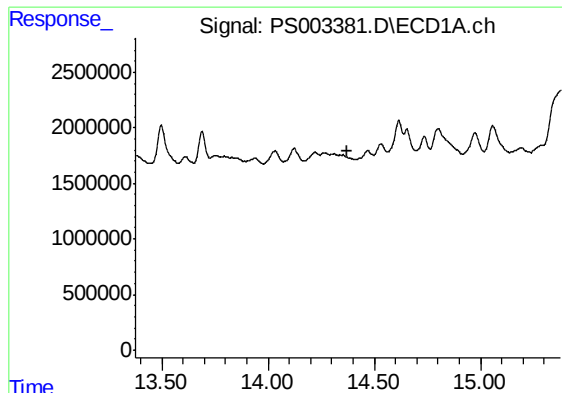

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-15

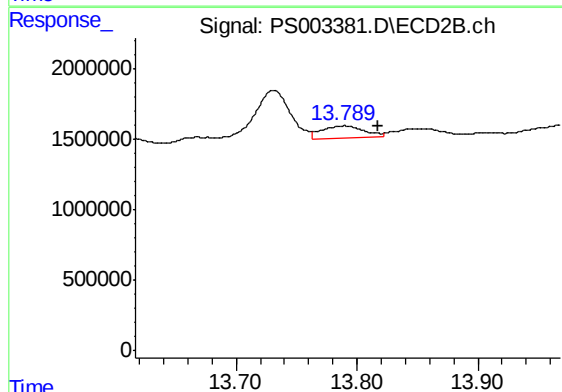


#11 2,4,5-TP (SILVEX)

R.T.: 13.789 min
Delta R.T.: -0.029 min
Response: 2155400
Conc: 0.85 ng/ml

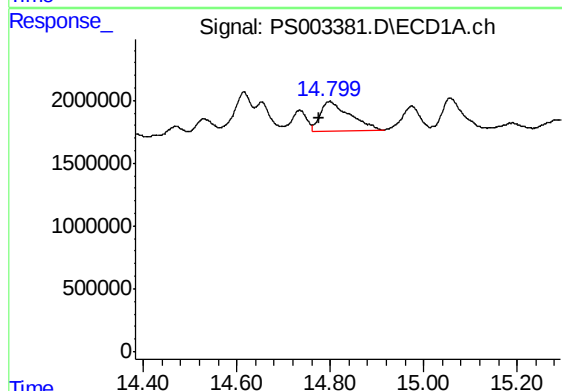


#12 2,4,5-T

R.T.: 14.799 min
Delta R.T.: 0.023 min
Response: 10328752
Conc: 3.91 ng/ml

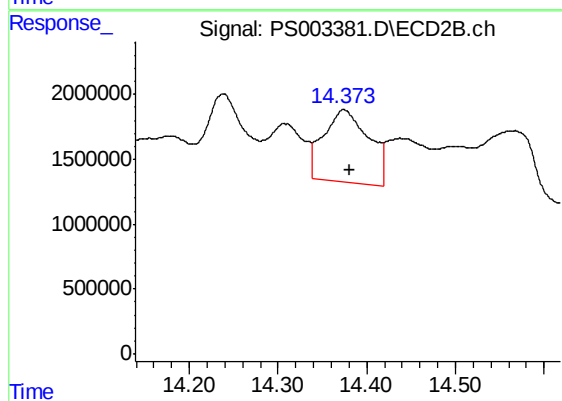

#12 2,4,5-T


R.T.: 14.374 min
Delta R.T.: -0.006 min
Response: 19890510
Conc: 9.86 ng/ml

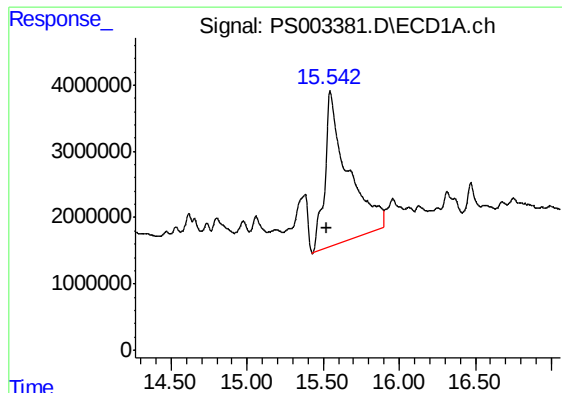

#13 2,4-DB


R.T.: 15.545 min
Delta R.T.: 0.022 min
Response: 245356185
Conc: 1036.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-15

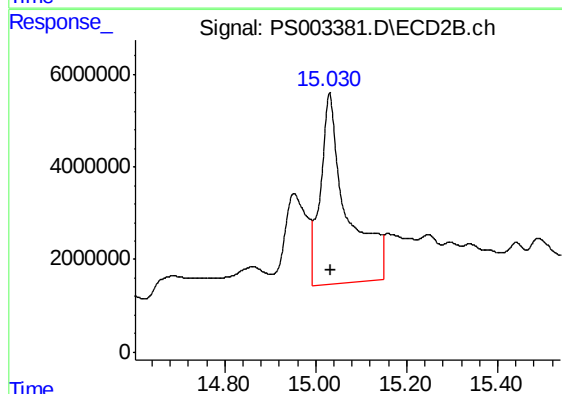


#13 2,4-DB

R.T.: 15.030 min
Delta R.T.: -0.003 min
Response: 165154472
Conc: 646.76 ng/ml

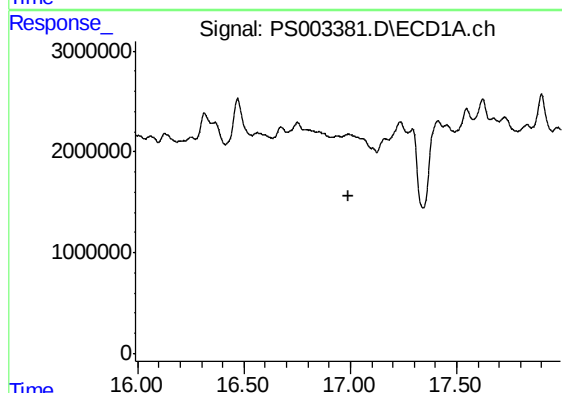


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

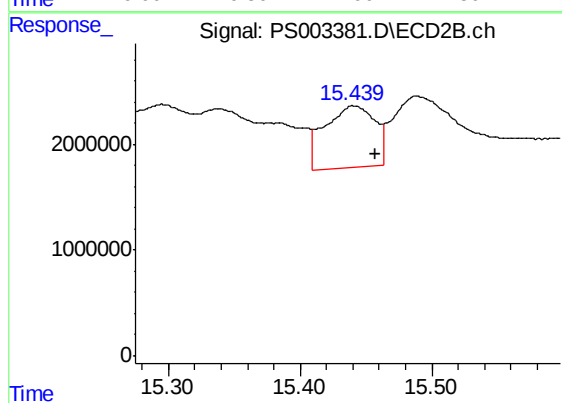

#14 DINOSEB


R.T.: 15.441 min
Delta R.T.: -0.016 min
Response: 15404184
Conc: 8.63 ng/ml

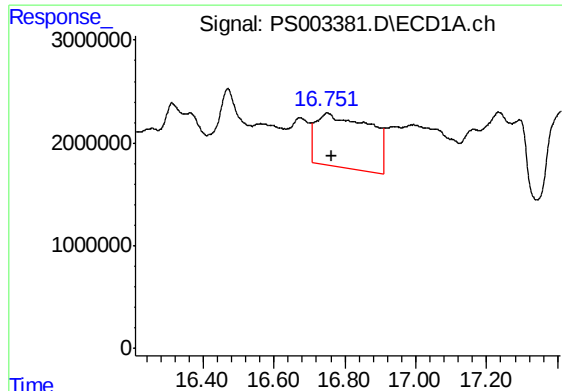

#15 Picloram


R.T.: 16.751 min
Delta R.T.: -0.014 min
Response: 55127316
Conc: 22.40 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-15

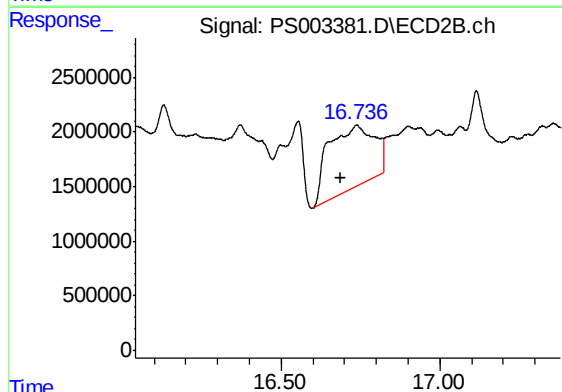


#15 Picloram

R.T.: 16.738 min
Delta R.T.: 0.049 min
Response: 57312690
Conc: 22.58 ng/ml

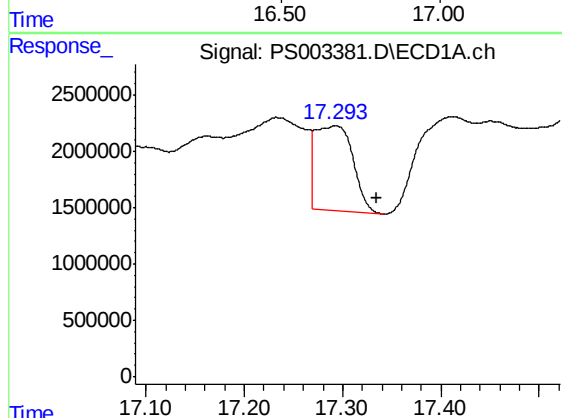

#16 DCPA

R.T.: 17.290 min
Delta R.T.: -0.045 min
Response: 19793566
Conc: 6.01 ng/ml

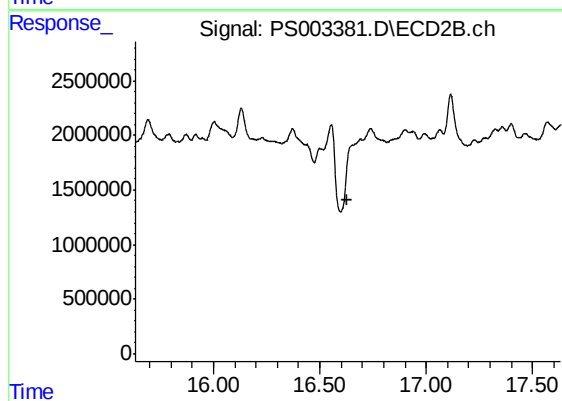

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 16.632 min
Response: 0
Conc: N.D.