

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022819\
 Data File : PS003382.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2019 20:16
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 03:45:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.277	10.779	234.1E6	225.6E6	533.268	480.421
Target Compounds							
7) T	MCPA	0.000	11.667	0	385595	N.D.	0.224 #
8) T	DICHLORPROP	0.000	12.145	0	289982	N.D.	0.702 #
10) T	Pentachlo...	0.000	13.194	0	1014007	N.D.	0.154 #
11) T	2,4,5-TP ...	0.000	13.813	0	69520	N.D.	0.027 #
12) T	2,4,5-T	0.000	14.340	0	68991	N.D.	0.034 #
13) T	2,4-DB	0.000	15.001	0	80690	N.D.	0.316 #
14) T	DINOSEB	0.000	15.409	0	166241	N.D.	0.093 #
15) T	Picloram	0.000	16.631	0	497582	N.D.	0.196 #
16) T	DCPA	0.000	16.631	0	497582	N.D.	0.160 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022819\
Data File : PS003382.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2019 20:16
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 03:45:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

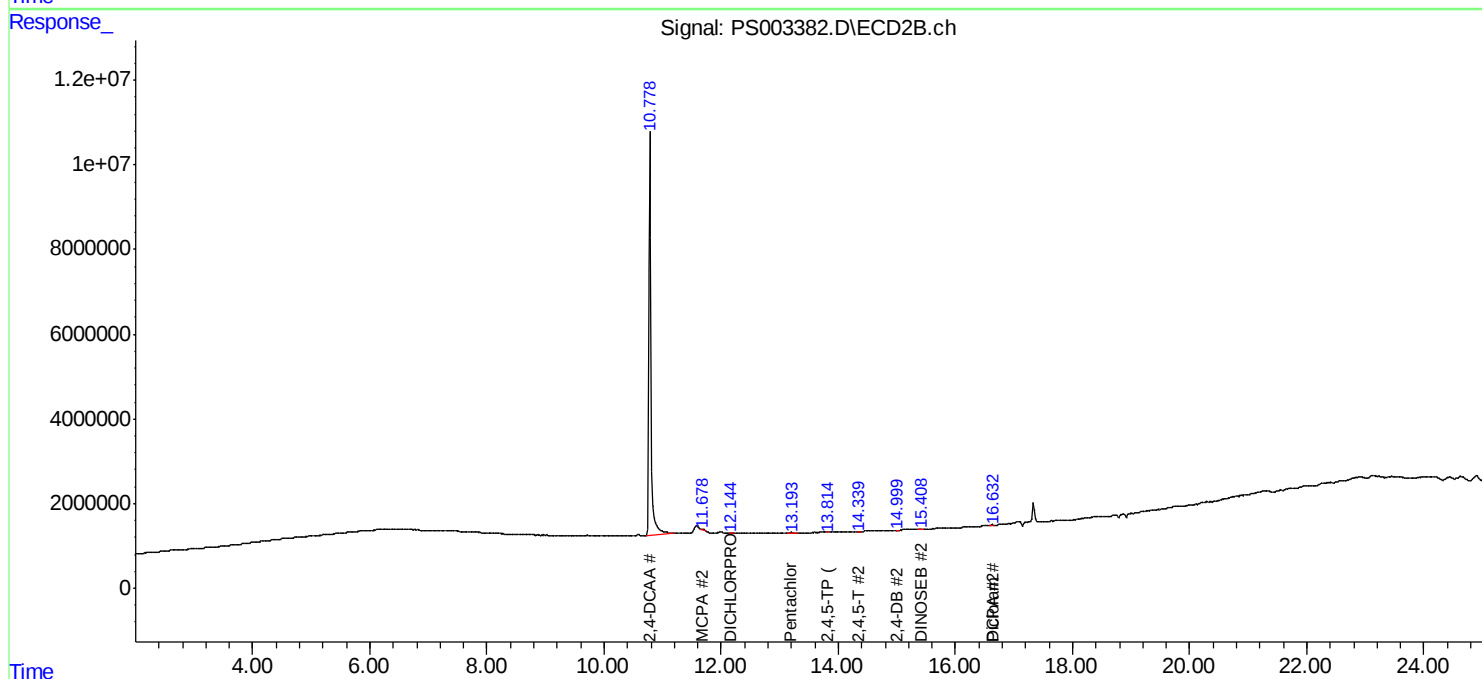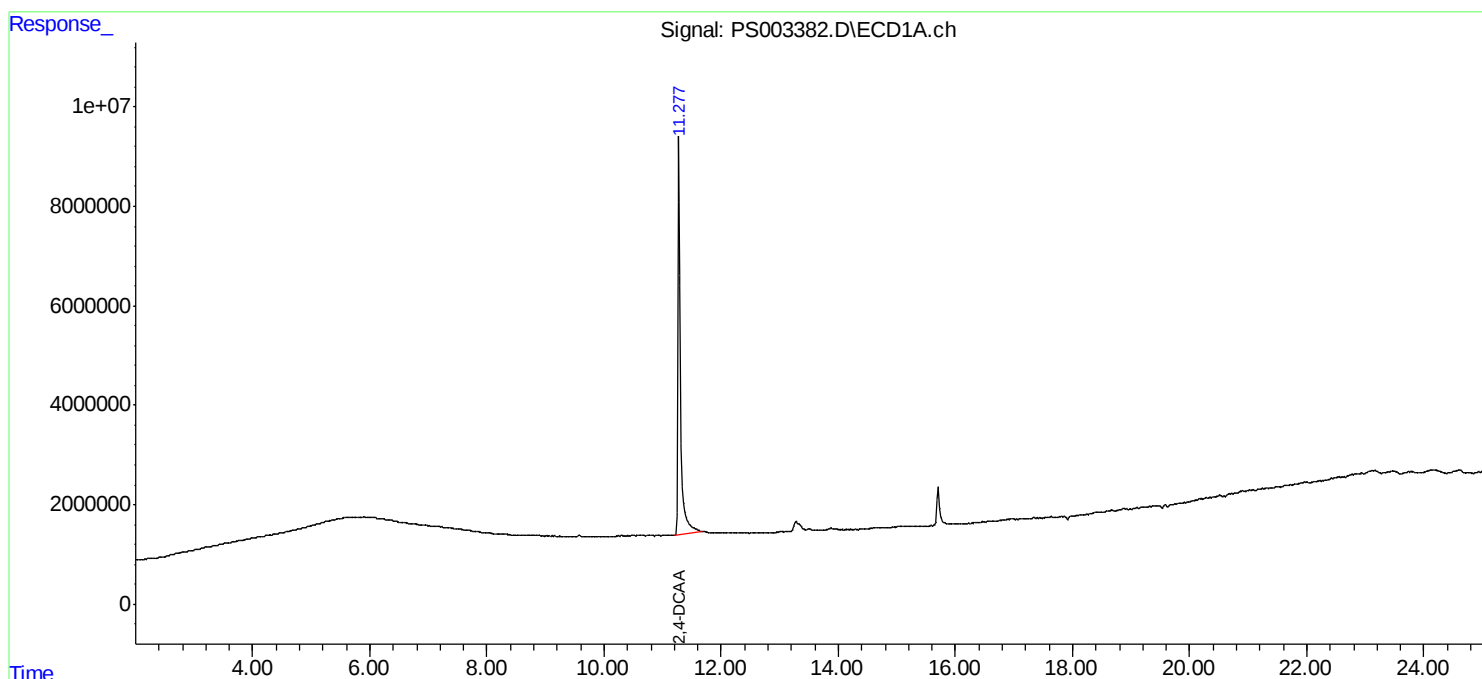


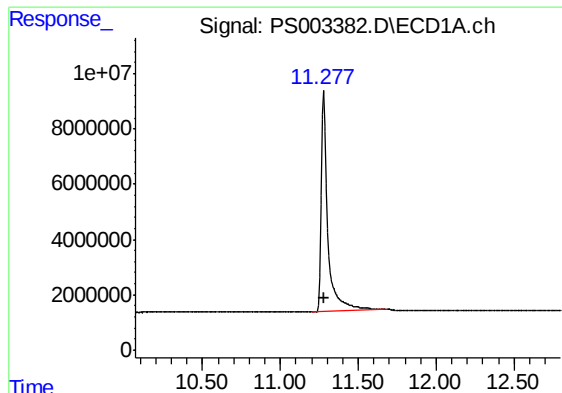

#4 2,4-DCAA


R.T.: 11.277 min
Delta R.T.: 0.000 min
Response: 234117553
Conc: 533.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

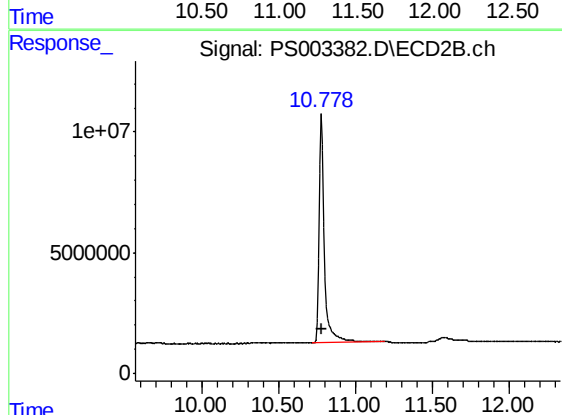


#4 2,4-DCAA

R.T.: 10.779 min
Delta R.T.: -0.001 min
Response: 225590895
Conc: 480.42 ng/ml

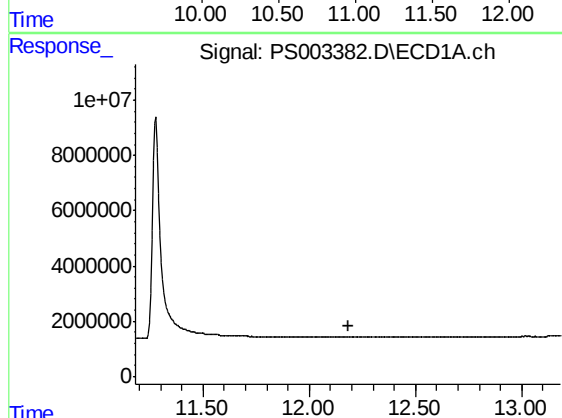


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

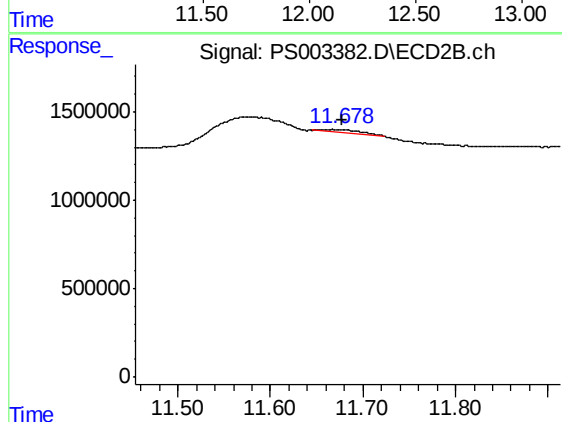

#7 MCPA


R.T.: 11.667 min
Delta R.T.: -0.010 min
Response: 385595
Conc: 0.22 ug/ml

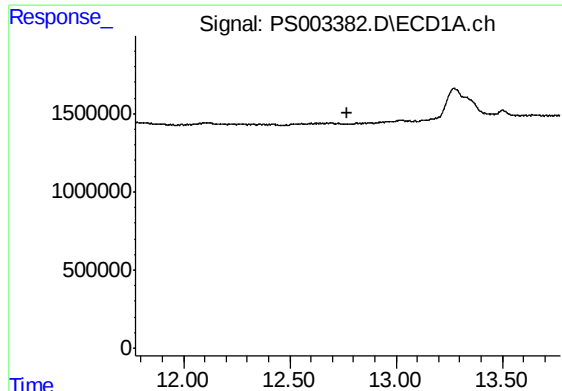

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

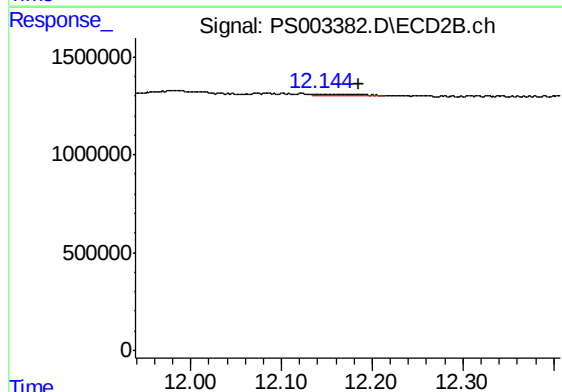


#8 DICHLORPROP

R.T.: 12.145 min
Delta R.T.: -0.040 min
Response: 289982
Conc: 0.70 ng/ml

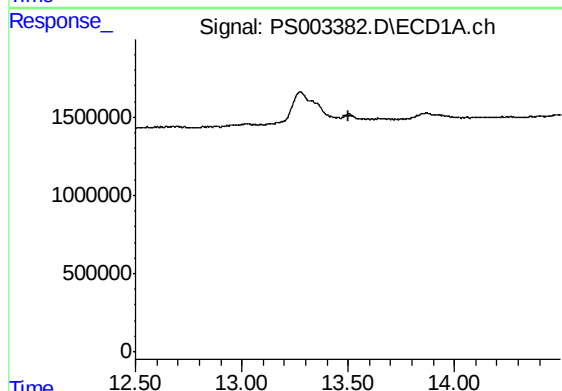


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.499 min
Response: 0
Conc: N.D.

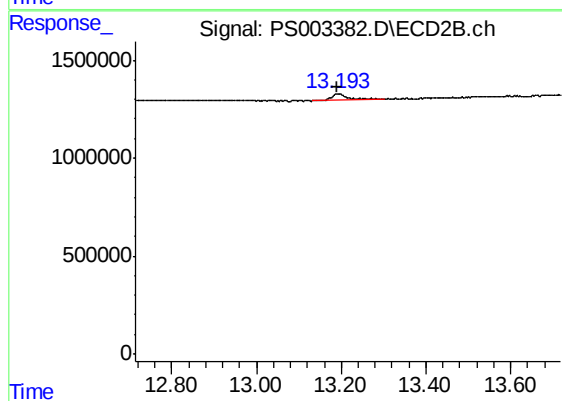

#10 Pentachlorophenol


R.T.: 13.194 min
Delta R.T.: 0.003 min
Response: 1014007
Conc: 0.15 ng/ml

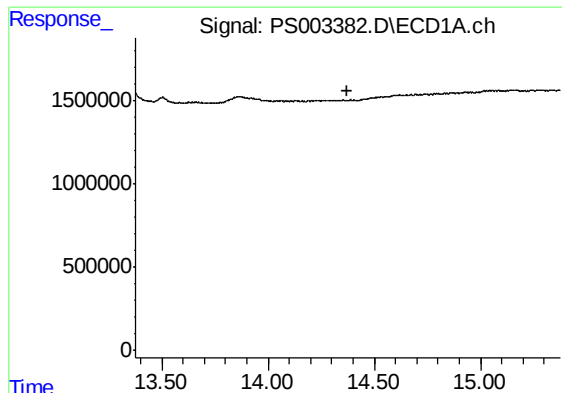

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

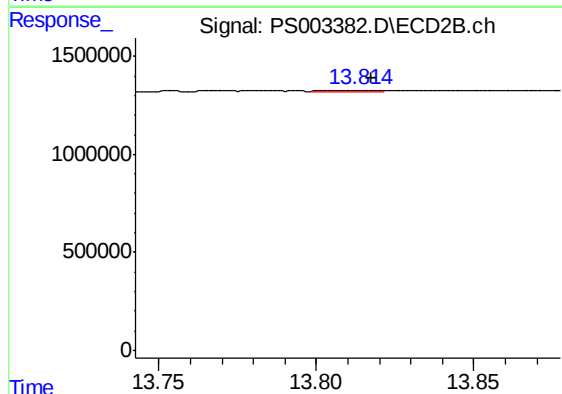


#11 2,4,5-TP (SILVEX)

R.T.: 13.813 min
Delta R.T.: -0.005 min
Response: 69520
Conc: 0.03 ng/ml

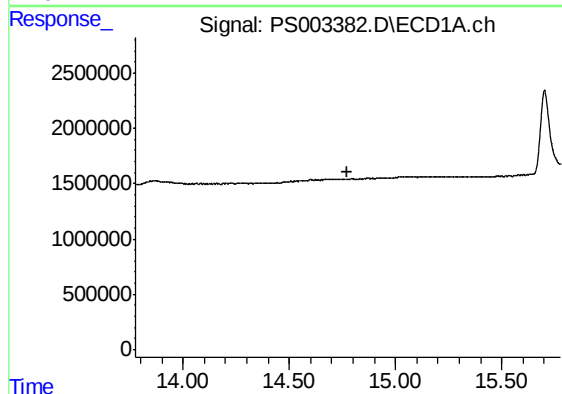


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

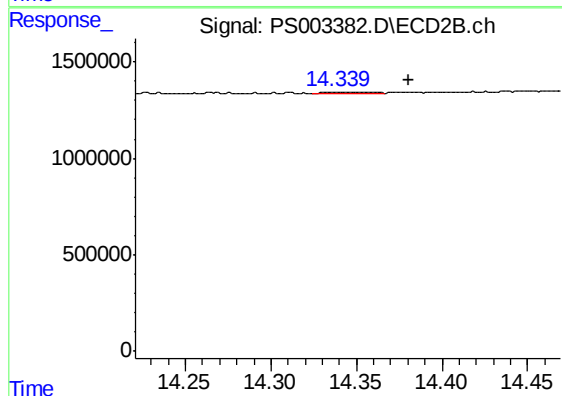

#12 2,4,5-T


R.T.: 14.340 min
Delta R.T.: -0.041 min
Response: 68991
Conc: 0.03 ng/ml

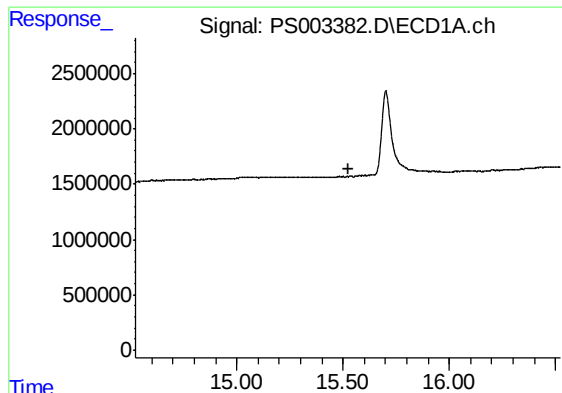

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

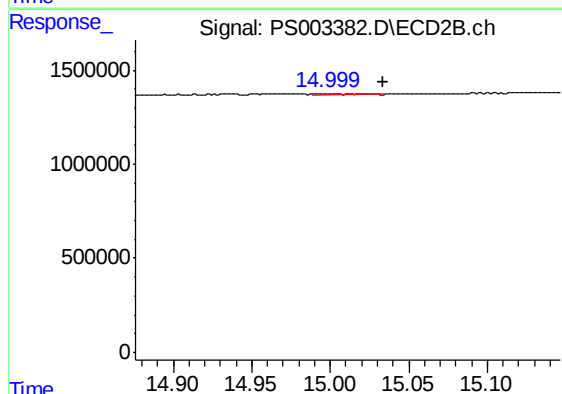


#13 2,4-DB

R.T.: 15.001 min
Delta R.T.: -0.033 min
Response: 80690
Conc: 0.32 ng/ml

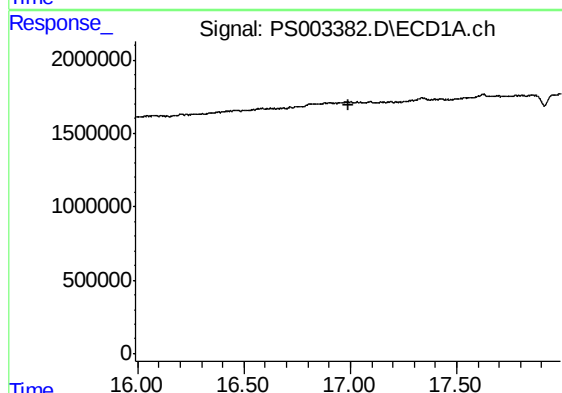


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

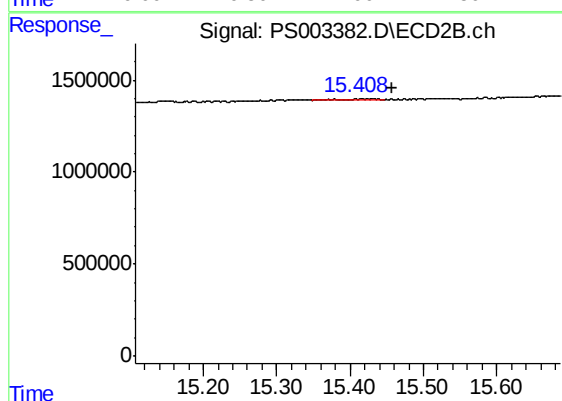

#14 DINOSEB


R.T.: 15.409 min
Delta R.T.: -0.048 min
Response: 166241
Conc: 0.09 ng/ml

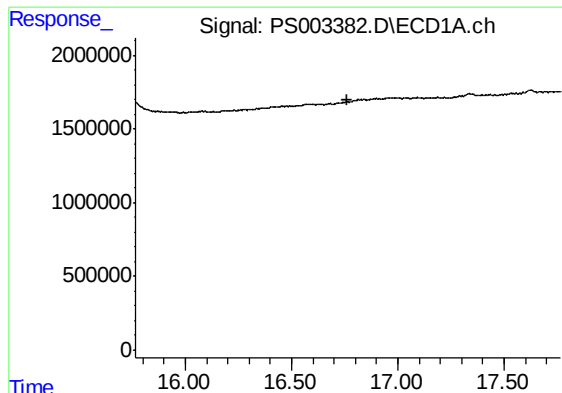

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

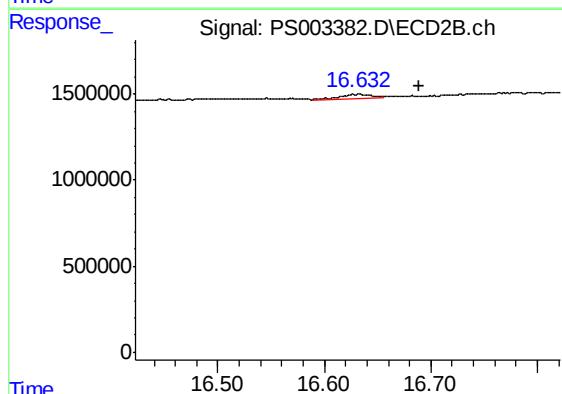


#15 Picloram

R.T.: 16.631 min
Delta R.T.: -0.057 min
Response: 497582
Conc: 0.20 ng/ml

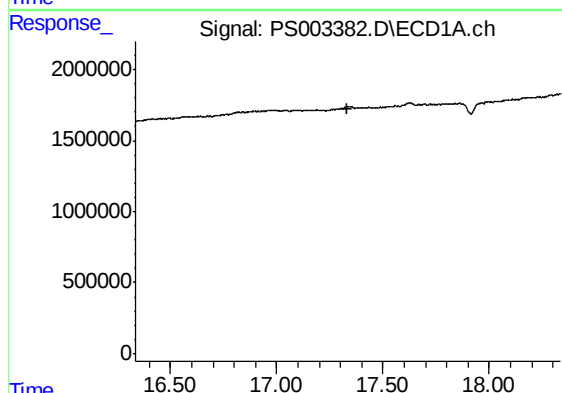

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

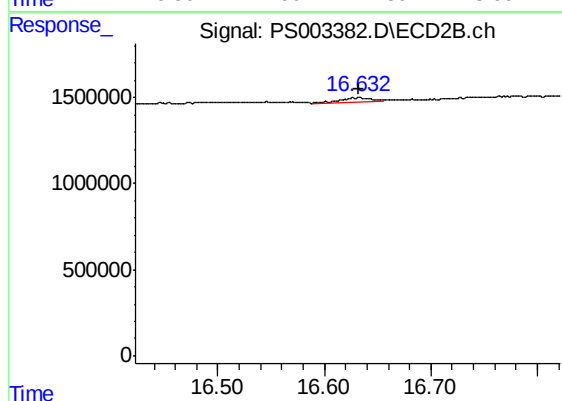

#16 DCPA

R.T.: 16.631 min
Delta R.T.: 0.000 min
Response: 497582
Conc: 0.16 ng/ml