

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022819\
 Data File : PS003387.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2019 22:51
 Operator : EI\SJ
 Sample : K1340-02
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 BU-03-022719

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 03:46:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.283	10.783	153.8E6	154.8E6	350.293	329.622
Target Compounds							
1) T	Dalapon	2.801	2.288	38618710	55291152	59.419	87.322 #
5) T	DICAMBA	0.000	11.022	0	5382398	N.D.	3.222 #
6) T	MCPD	11.988	11.322	6695864	-46995	5.100	N.D. #
7) T	MCPA	12.219	11.689	46561881	-788288	23.474	N.D. #
9) T	2,4-D	0.000	12.684	0	242789	N.D.	0.463 #
10) T	Pentachlo...	0.000	13.193	0	873784	N.D.	0.133 #
11) T	2,4,5-TP ...	0.000	13.827	0	525943	N.D.	0.207 #
12) T	2,4,5-T	0.000	14.384	0	7993638	N.D.	3.964 #
14) T	DINOSEB	0.000	15.520	0	6811973	N.D.	3.817 #
15) T	Picloram	16.764	16.723	4331324	24013948	1.760	9.461 #
16) T	DCPA	17.306	0.000	26644667	0	8.086	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022819\
Data File : PS003387.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2019 22:51
Operator : EI\SJ
Sample : K1340-02
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
BU-03-022719

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 03:46:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

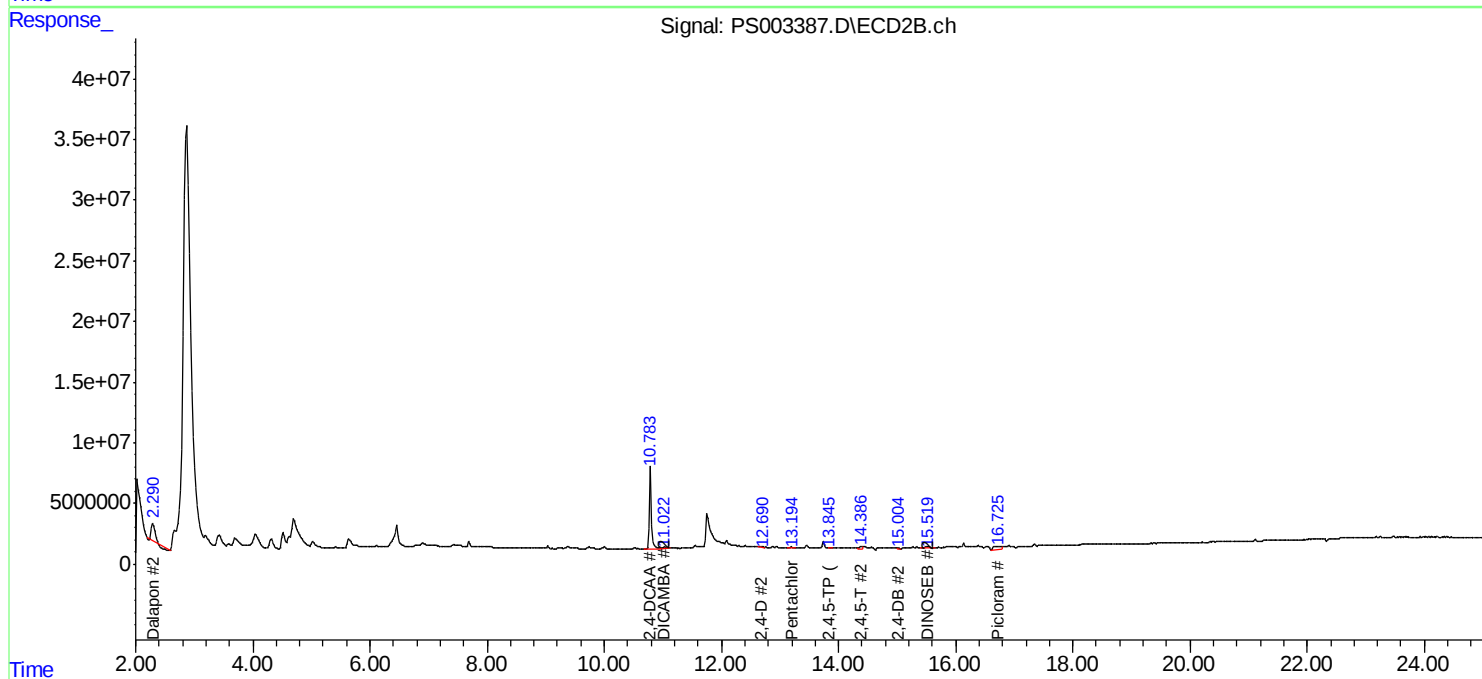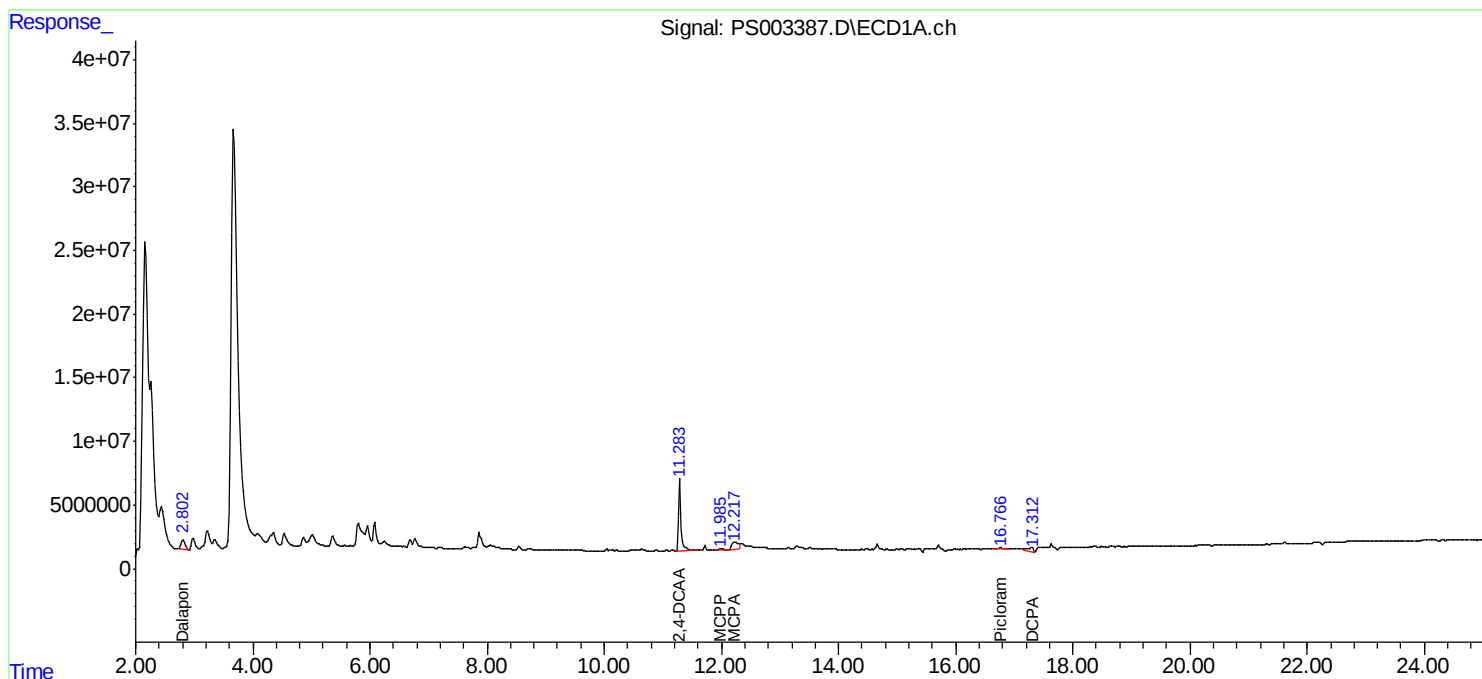


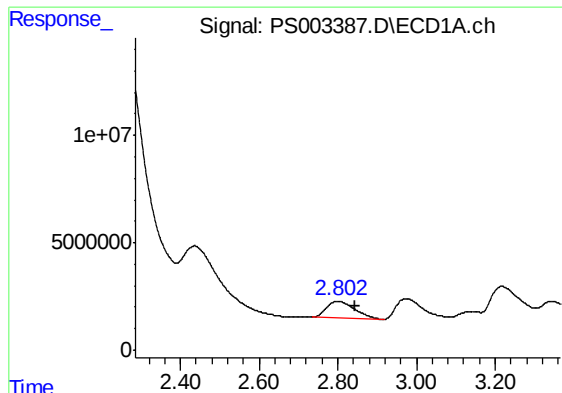

#1 Dalapon


R.T.: 2.801 min
Delta R.T.: -0.043 min
Response: 38618710
Conc: 59.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
BU-03-022719

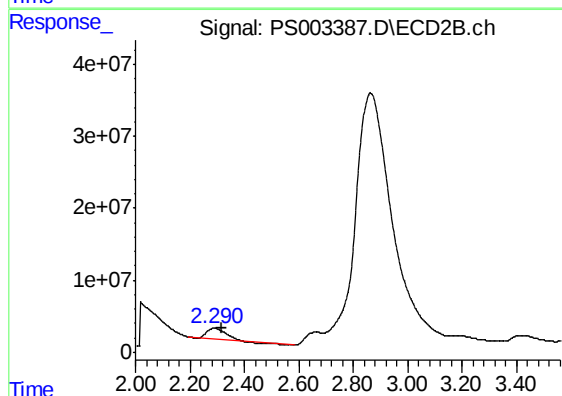


#1 Dalapon

R.T.: 2.288 min
Delta R.T.: -0.028 min
Response: 55291152
Conc: 87.32 ng/ml

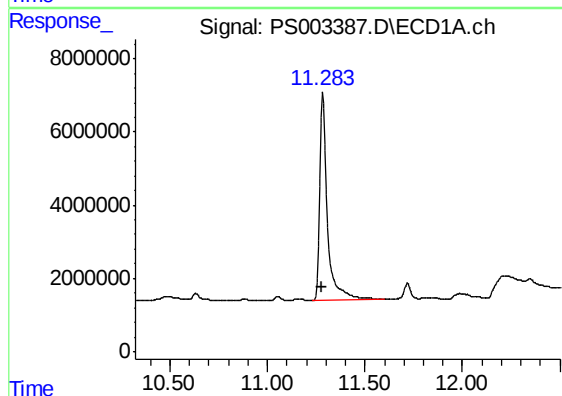


#4 2,4-DCAA

R.T.: 11.283 min
Delta R.T.: 0.006 min
Response: 153787376
Conc: 350.29 ng/ml

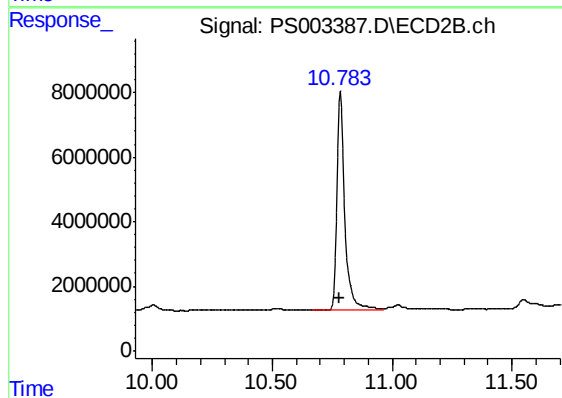

#4 2,4-DCAA


R.T.: 10.783 min
Delta R.T.: 0.004 min
Response: 154780430
Conc: 329.62 ng/ml

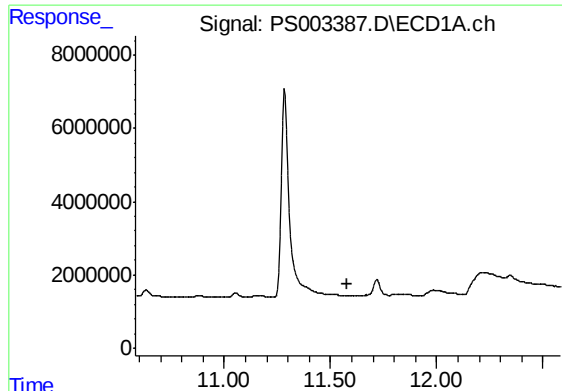

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BU-03-022719

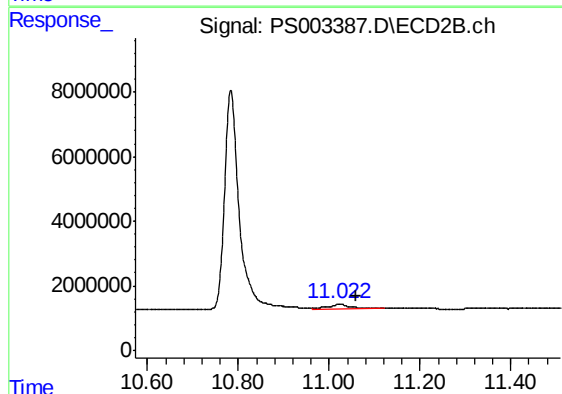


#5 DICAMBA

R.T.: 11.022 min
Delta R.T.: -0.037 min
Response: 5382398
Conc: 3.22 ng/ml

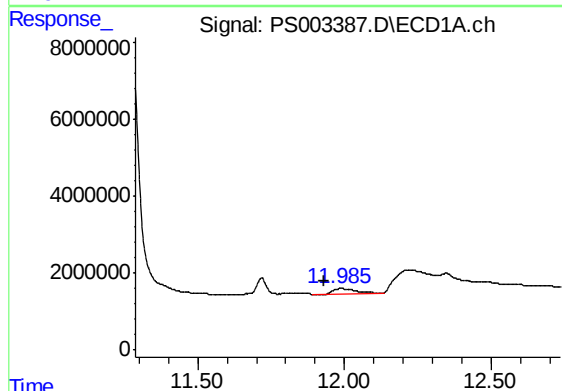


#6 MCPP

R.T.: 11.988 min
Delta R.T.: 0.057 min
Response: 6695864
Conc: 5.10 ug/ml

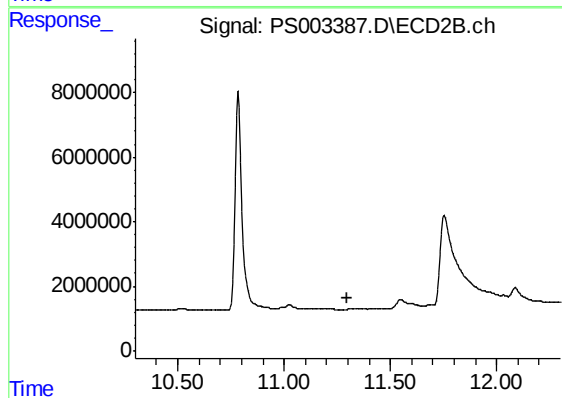

#6 MCPP


R.T.: 11.322 min
Delta R.T.: 0.022 min
Response: -46995
Conc: N.D.

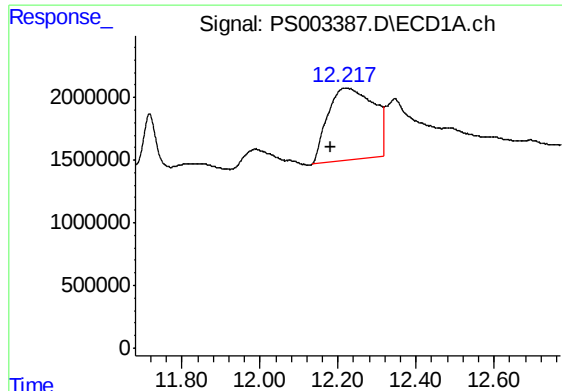

#7 MCPA


R.T.: 12.219 min
Delta R.T.: 0.037 min
Response: 46561881
Conc: 23.47 ug/ml

Instrument :
ECD_S
ClientSampleId :
BU-03-022719

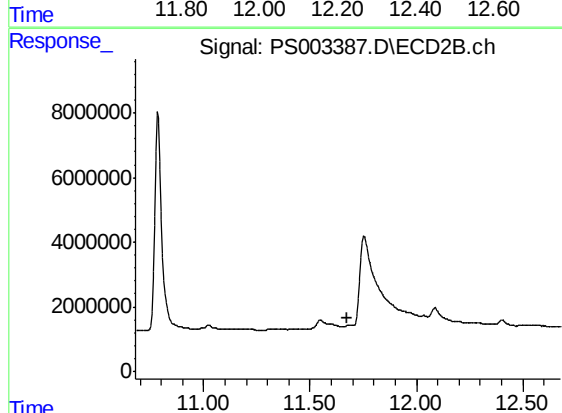


#7 MCPA

R.T.: 11.689 min
Delta R.T.: 0.011 min
Response: -788288
Conc: N.D.

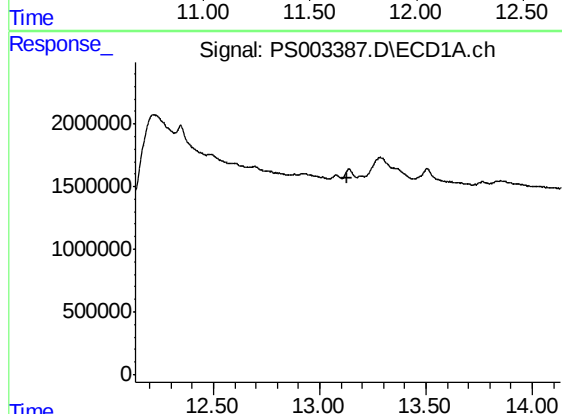


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.133 min
Response: 0
Conc: N.D.

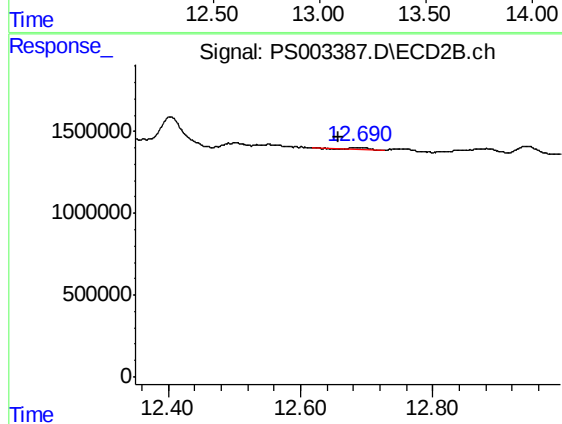

#9 2,4-D


R.T.: 12.684 min
Delta R.T.: 0.027 min
Response: 242789
Conc: 0.46 ng/ml

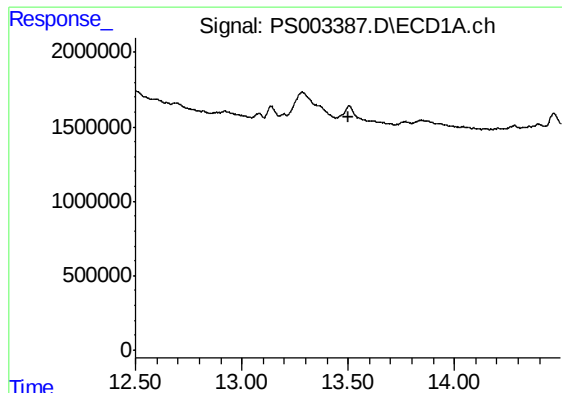

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BU-03-022719

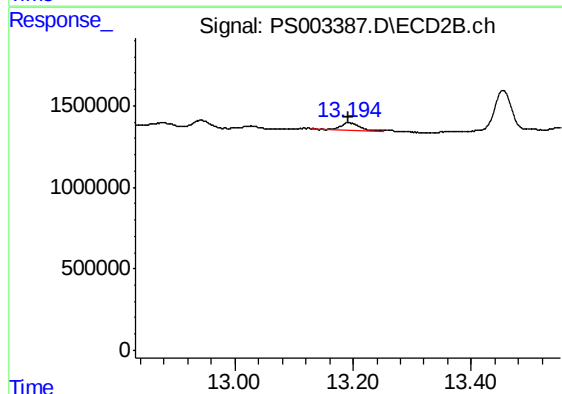


#10 Pentachlorophenol

R.T.: 13.193 min
Delta R.T.: 0.002 min
Response: 873784
Conc: 0.13 ng/ml

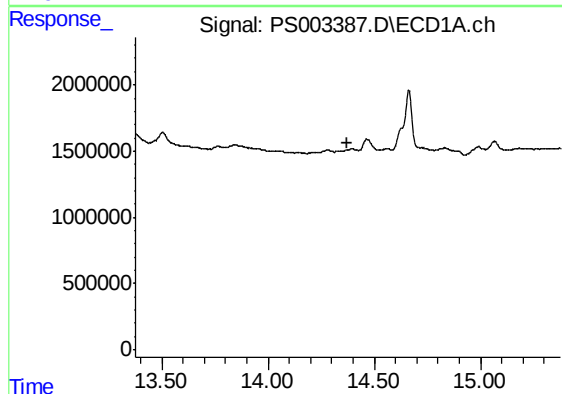


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

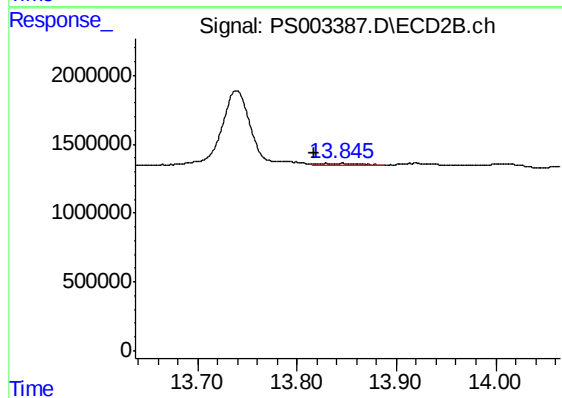

#11 2,4,5-TP (SILVEX)


R.T.: 13.827 min
Delta R.T.: 0.010 min
Response: 525943
Conc: 0.21 ng/ml

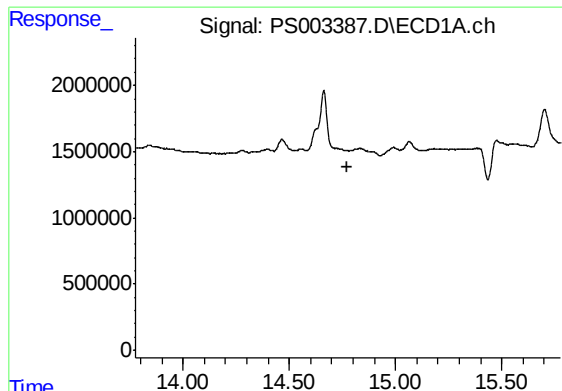

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BU-03-022719

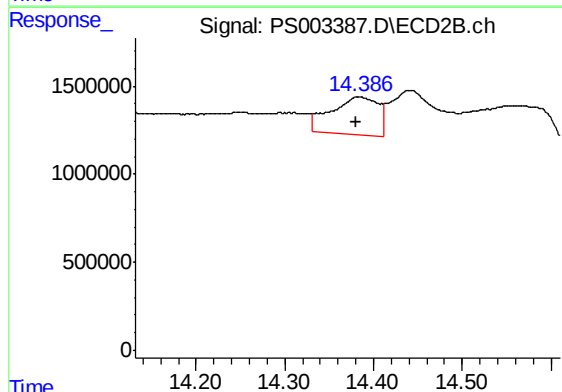


#12 2,4,5-T

R.T.: 14.384 min
Delta R.T.: 0.004 min
Response: 7993638
Conc: 3.96 ng/ml

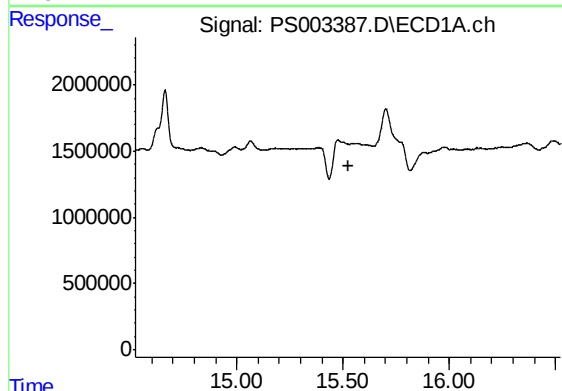


#13 2,4-DB

R.T.: 15.476 min
Delta R.T.: -0.047 min
Response: -4207311
Conc: N.D.

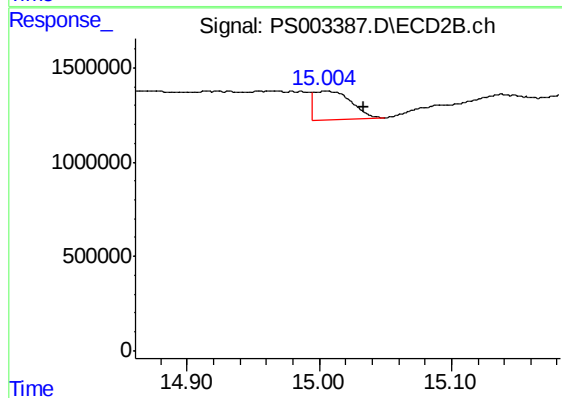

#13 2,4-DB


R.T.: 15.005 min
Delta R.T.: -0.028 min
Response: 2977883
Conc: 11.66 ng/ml

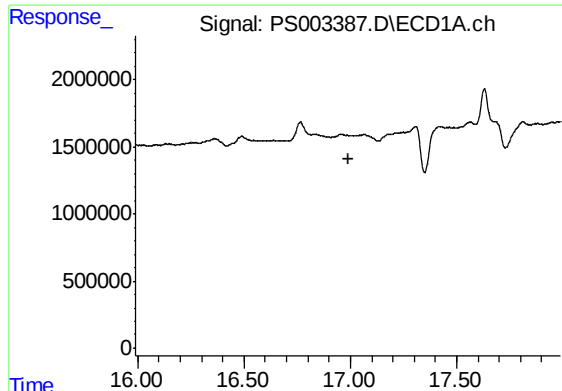

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BU-03-022719

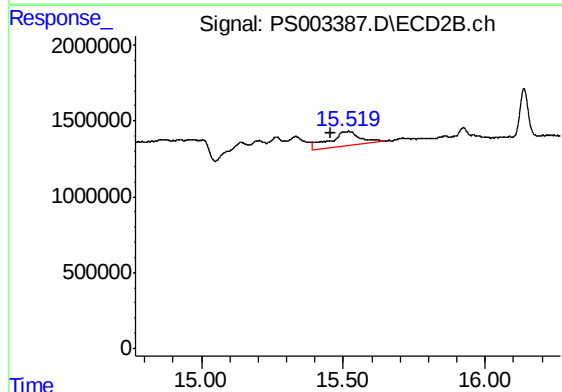


#14 DINOSEB

R.T.: 15.520 min
Delta R.T.: 0.063 min
Response: 6811973
Conc: 3.82 ng/ml

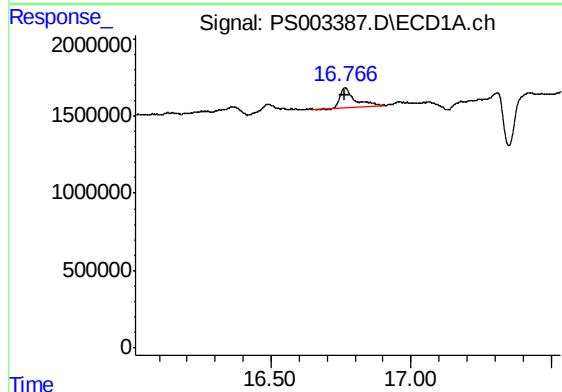


#15 Picloram

R.T.: 16.764 min
Delta R.T.: -0.001 min
Response: 4331324
Conc: 1.76 ng/ml

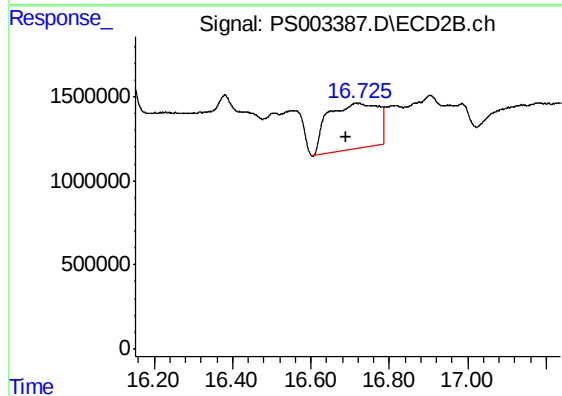

#15 Picloram


R.T.: 16.723 min
Delta R.T.: 0.035 min
Response: 24013948
Conc: 9.46 ng/ml

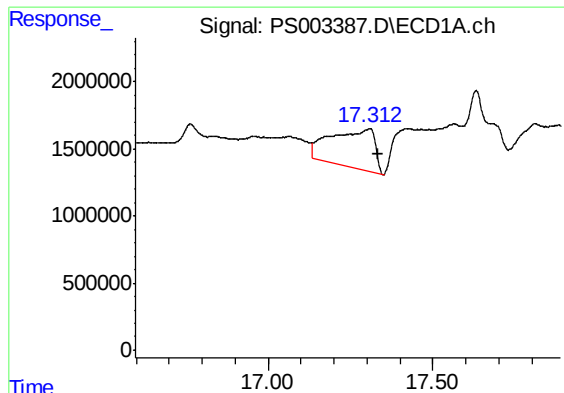

#16 DCPA

R.T.: 17.306 min
Delta R.T.: -0.029 min
Response: 26644667
Conc: 8.09 ng/ml

Instrument :
ECD_S
ClientSampleId :
BU-03-022719

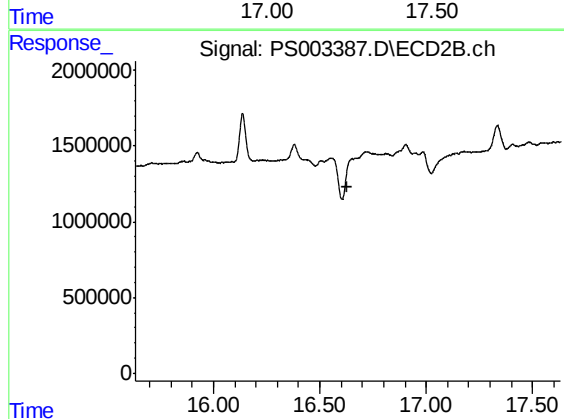

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 16.632 min
Response: 0
Conc: N.D.