

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022819\
 Data File : PS003390.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Mar 2019 00:24
 Operator : EI\SJ
 Sample : K1341-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HR-06-022719-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 03:46:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.294	10.795	157.7E6	158.4E6	359.153	337.270
Target Compounds							
1) T	Dalapon	2.810	2.299	39081584	26954665	60.131	42.570 #
5) T	DICAMBA	0.000	11.034	0	5061686	N.D.	3.030 #
6) T	MCP	11.994	0.000	3096145	0	2.358	N.D. #
7) T	MCPA	12.167	11.612	36737589	-59040	18.521	N.D. #
9) T	2,4-D	0.000	12.699	0	587717	N.D.	1.120 #
10) T	Pentachlo...	0.000	13.205	0	1169372	N.D.	0.178 #
11) T	2,4,5-TP ...	0.000	13.831	0	1789241	N.D.	0.703 #
12) T	2,4,5-T	0.000	14.412	0	9956185	N.D.	4.937 #
13) T	2,4-DB	15.488	0.000	10031101	0	42.362	N.D. #
14) T	DINOSEB	0.000	15.510	0	4460744	N.D.	2.499 #
15) T	Picloram	16.774	16.655	375633	6640770	0.153	2.616 #
16) T	DCPA	0.000	16.655	0	6640770	N.D.	2.135 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022819\
Data File : PS003390.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Mar 2019 00:24
Operator : EI\SJ
Sample : K1341-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HR-06-022719-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 03:46:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

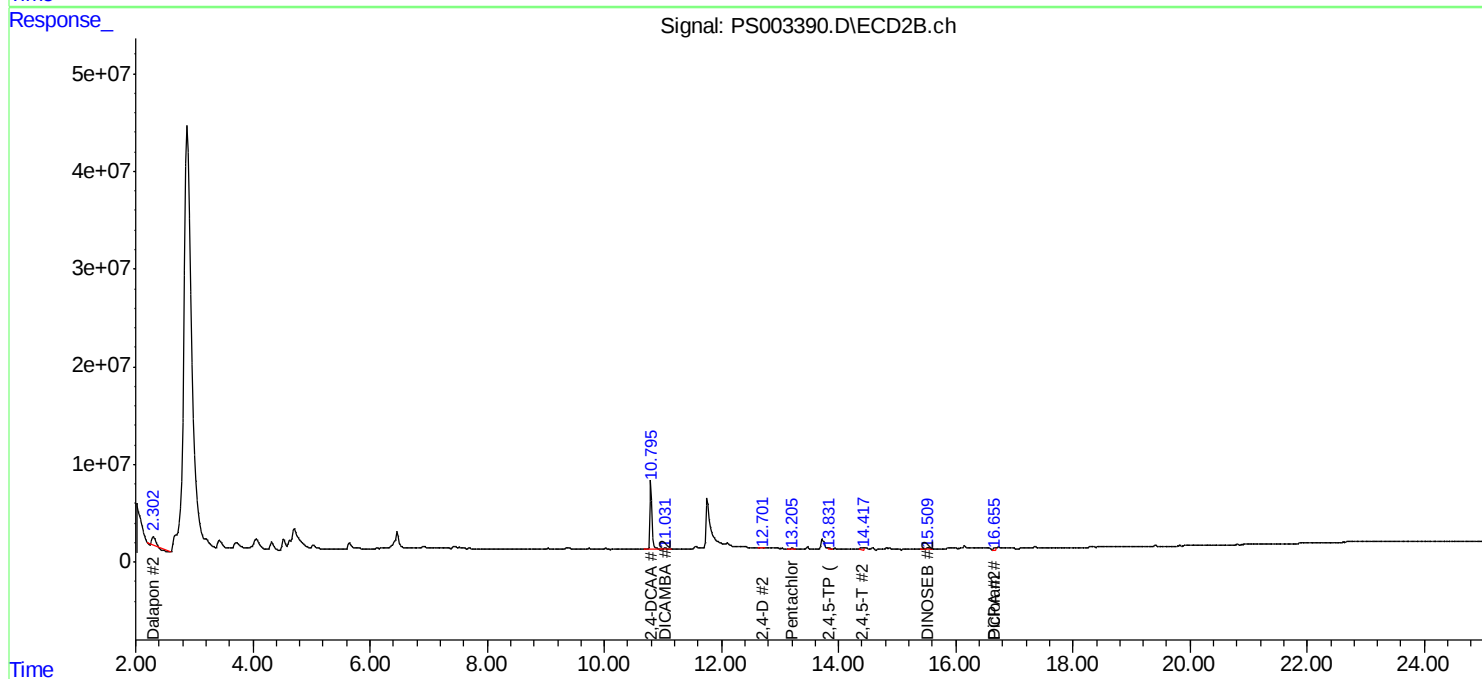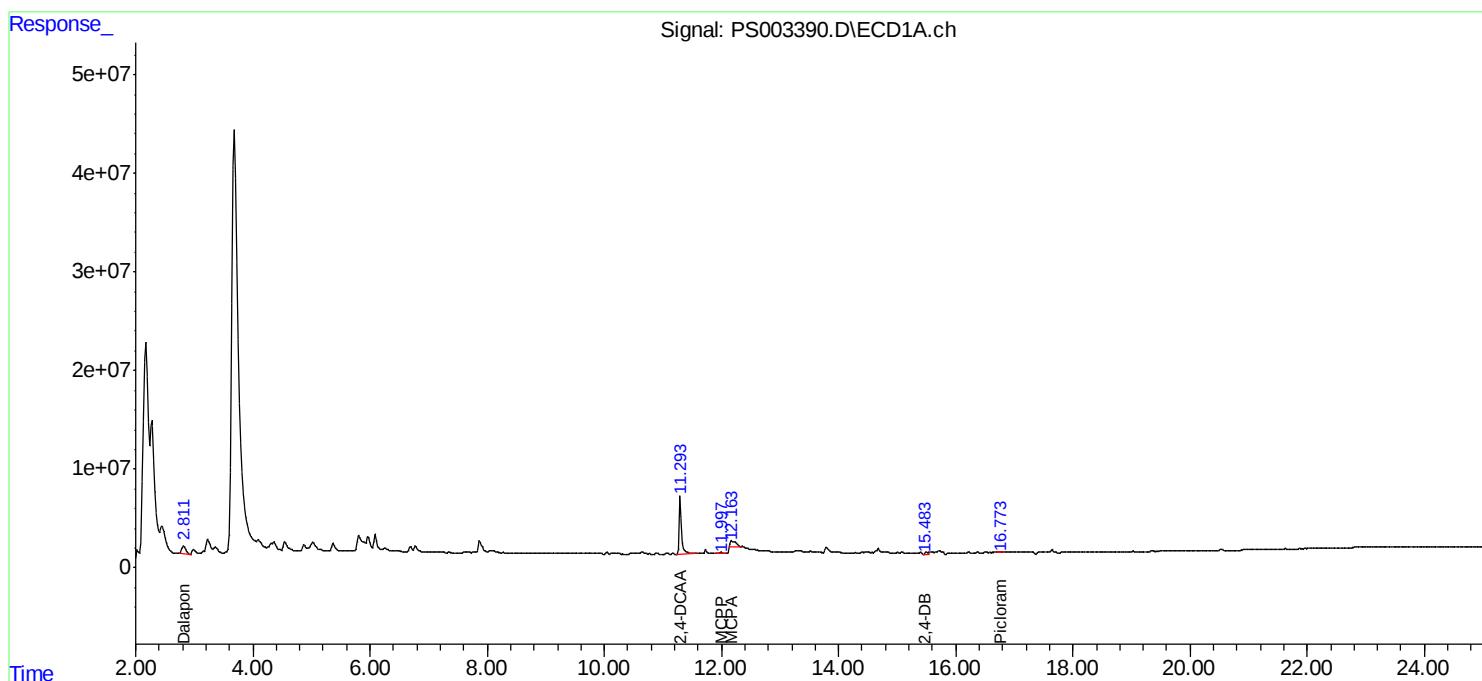


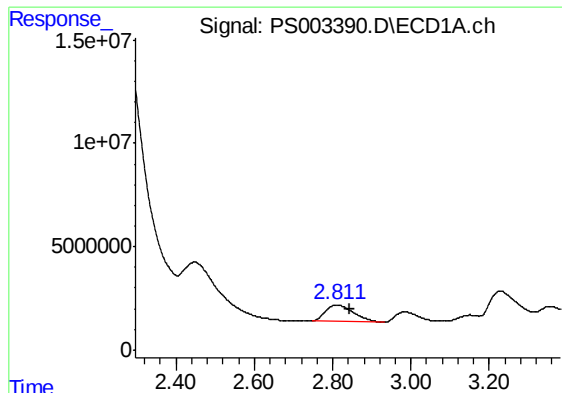

#1 Dalapon


R.T.: 2.810 min
Delta R.T.: -0.034 min
Response: 39081584
Conc: 60.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
HR-06-022719-A

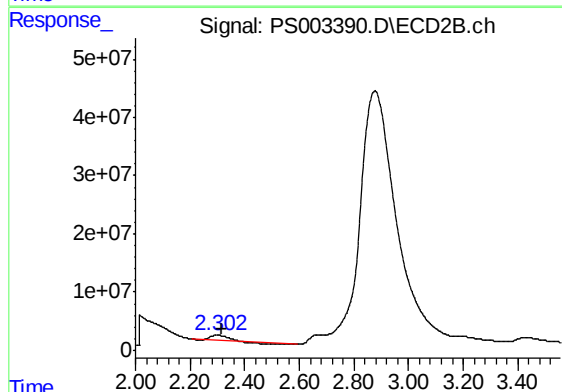


#1 Dalapon

R.T.: 2.299 min
Delta R.T.: -0.017 min
Response: 26954665
Conc: 42.57 ng/ml

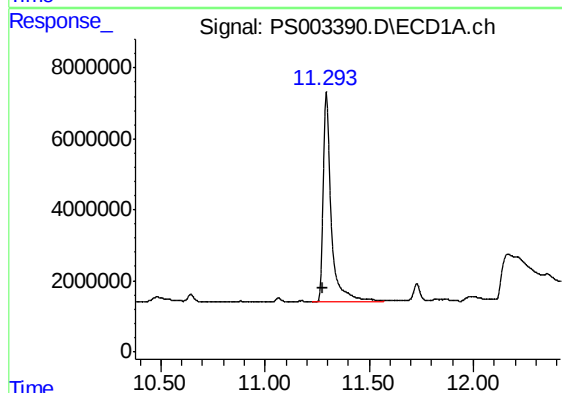


#4 2,4-DCAA

R.T.: 11.294 min
Delta R.T.: 0.017 min
Response: 157676834
Conc: 359.15 ng/ml

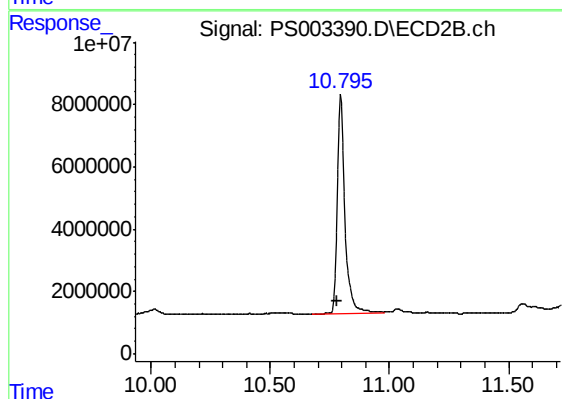

#4 2,4-DCAA


R.T.: 10.795 min
Delta R.T.: 0.016 min
Response: 158371365
Conc: 337.27 ng/ml

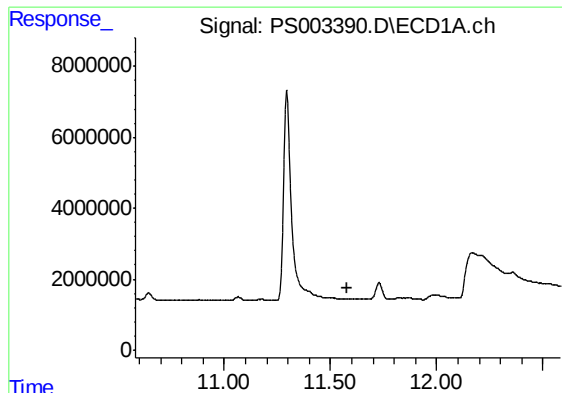

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HR-06-022719-A

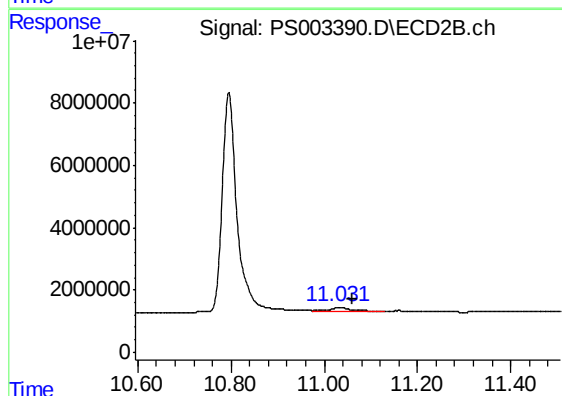


#5 DICAMBA

R.T.: 11.034 min
Delta R.T.: -0.026 min
Response: 5061686
Conc: 3.03 ng/ml

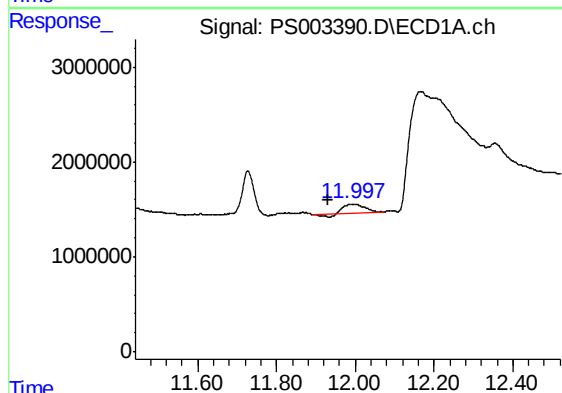


#6 MCPP

R.T.: 11.994 min
Delta R.T.: 0.063 min
Response: 3096145
Conc: 2.36 ug/ml

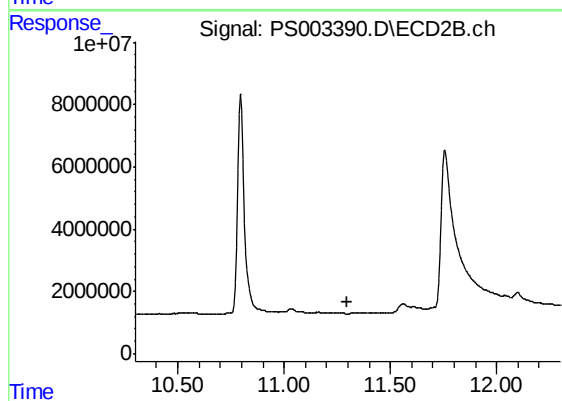

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 11.300 min
Response: 0
Conc: N.D.

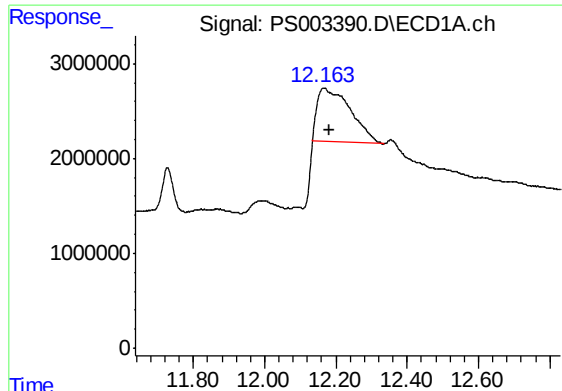

#7 MCPA


R.T.: 12.167 min
Delta R.T.: -0.015 min
Response: 36737589
Conc: 18.52 ug/ml

Instrument :
ECD_S
ClientSampleId :
HR-06-022719-A

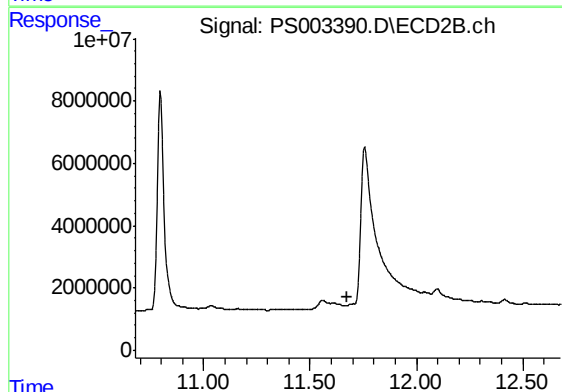


#7 MCPA

R.T.: 11.612 min
Delta R.T.: -0.066 min
Response: -59040
Conc: N.D.

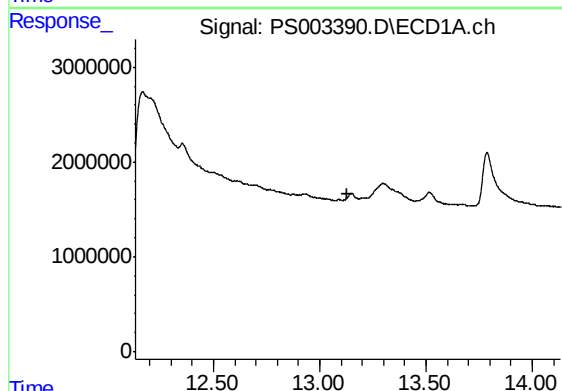


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.133 min
Response: 0
Conc: N.D.

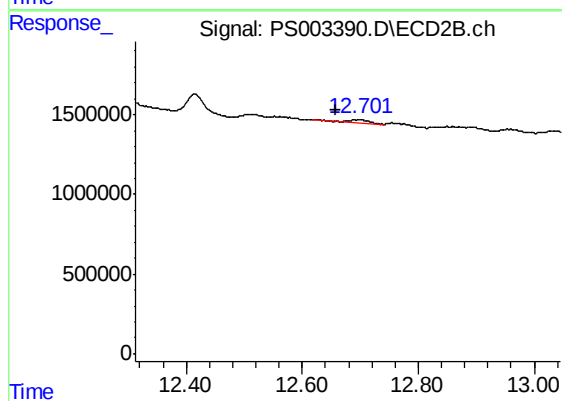

#9 2,4-D


R.T.: 12.699 min
Delta R.T.: 0.042 min
Response: 587717
Conc: 1.12 ng/ml

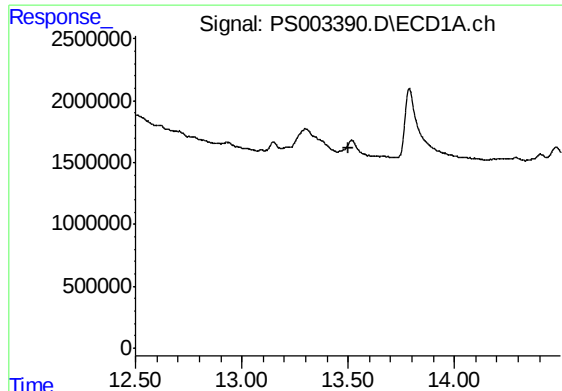

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HR-06-022719-A

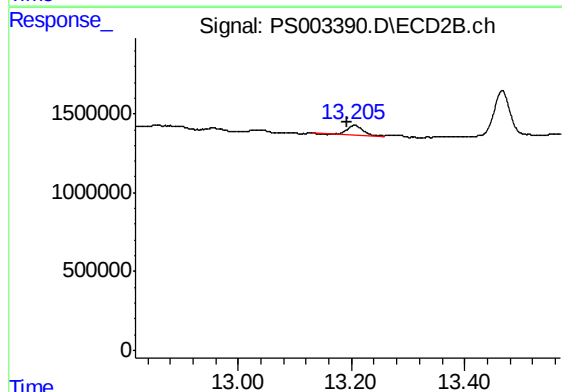


#10 Pentachlorophenol

R.T.: 13.205 min
Delta R.T.: 0.014 min
Response: 1169372
Conc: 0.18 ng/ml

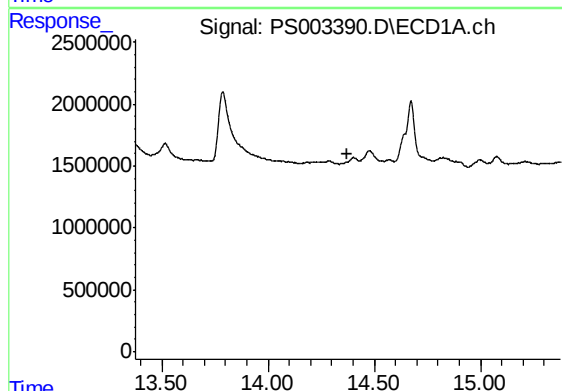


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

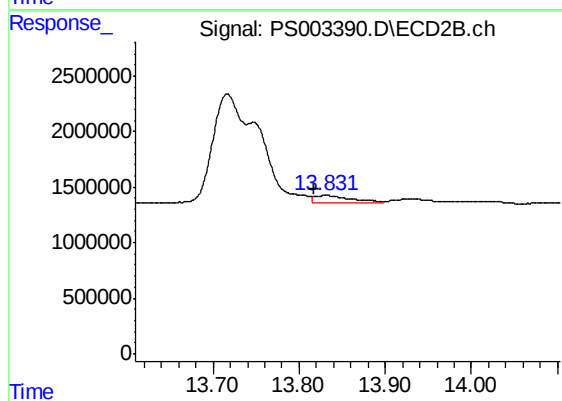

#11 2,4,5-TP (SILVEX)


R.T.: 13.831 min
Delta R.T.: 0.013 min
Response: 1789241
Conc: 0.70 ng/ml

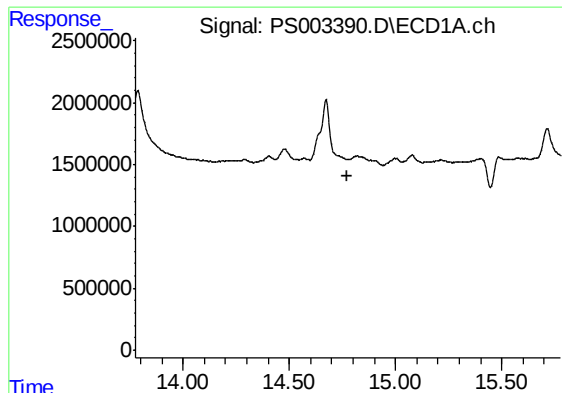

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HR-06-022719-A

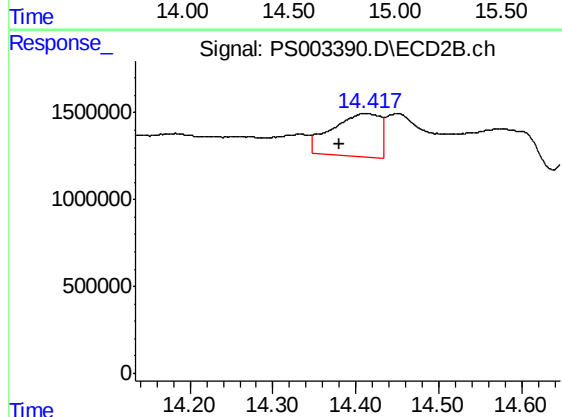


#12 2,4,5-T

R.T.: 14.412 min
Delta R.T.: 0.032 min
Response: 9956185
Conc: 4.94 ng/ml

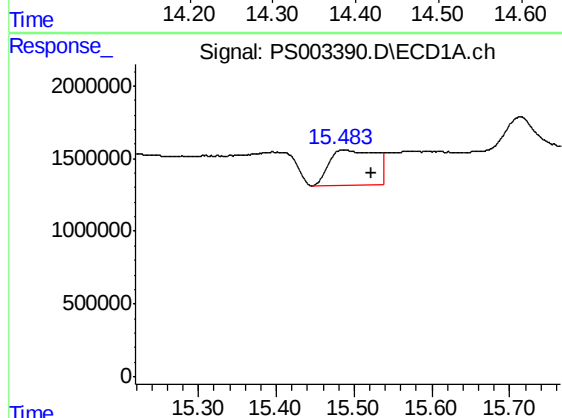


#13 2,4-DB

R.T.: 15.488 min
Delta R.T.: -0.035 min
Response: 10031101
Conc: 42.36 ng/ml

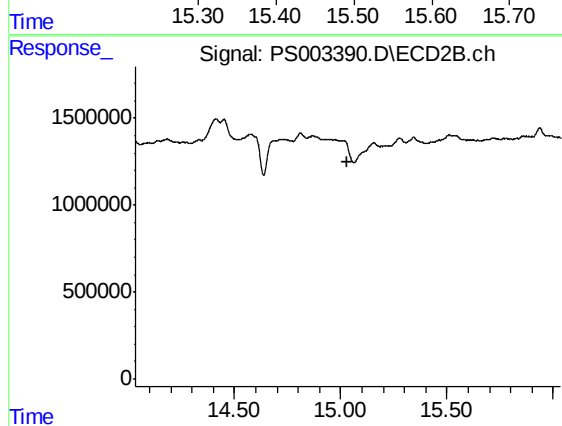

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.033 min
Response: 0
Conc: N.D.

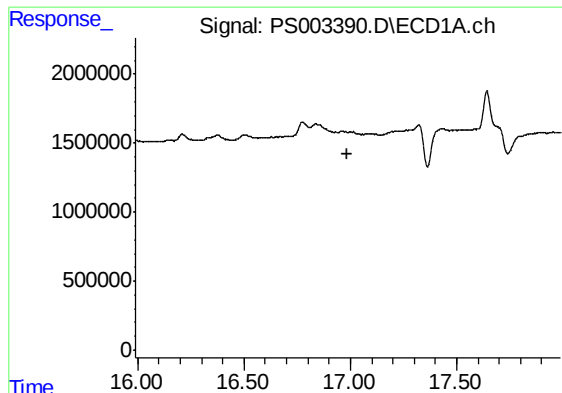

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HR-06-022719-A

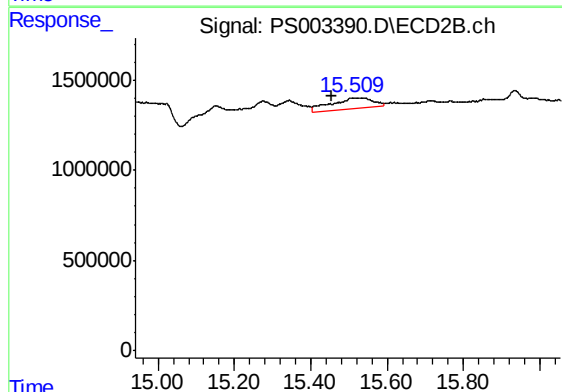


#14 DINOSEB

R.T.: 15.510 min
Delta R.T.: 0.053 min
Response: 4460744
Conc: 2.50 ng/ml

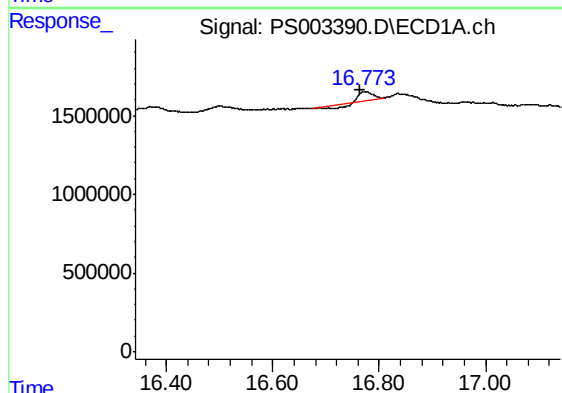


#15 Picloram

R.T.: 16.774 min
Delta R.T.: 0.009 min
Response: 375633
Conc: 0.15 ng/ml

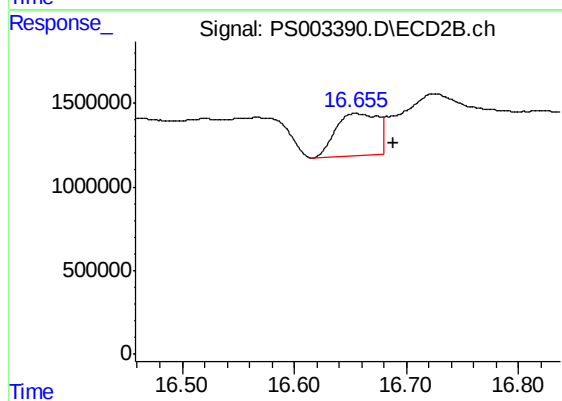

#15 Picloram


R.T.: 16.655 min
Delta R.T.: -0.033 min
Response: 6640770
Conc: 2.62 ng/ml

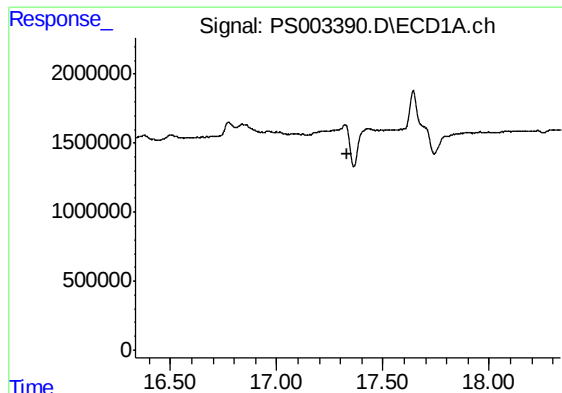

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HR-06-022719-A

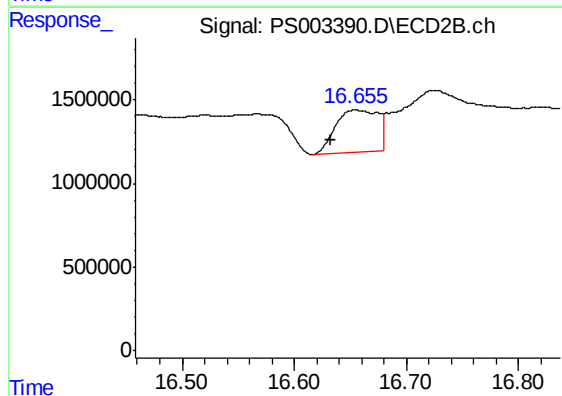

#16 DCPA

R.T.: 16.655 min
Delta R.T.: 0.023 min
Response: 6640770
Conc: 2.14 ng/ml