

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022819\
 Data File : PS003391.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Mar 2019 00:55
 Operator : EI\SJ
 Sample : K1341-10
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HR-06-022719-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 03:47:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.276	10.777	187.3E6	186.6E6	426.682	397.483
Target Compounds							
1) T	Dalapon	2.796	2.284	46075363	50558392	70.891	79.848
3) T	4-Nitroph...	0.000	9.996	0	6734630	N.D.	29.955 #
5) T	DICAMBA	0.000	11.017	0	5744906	N.D.	3.439 #
6) T	MCPD	11.969	11.316	4013546	138660	3.057	0.117 #
7) T	MCPA	0.000	11.740	0	19828855	N.D.	11.496 #
9) T	2,4-D	0.000	12.681	0	309588	N.D.	0.590 #
10) T	Pentachlo...	0.000	13.191	0	607411	N.D.	0.092 #
11) T	2,4,5-TP ...	0.000	13.819	0	1338157	N.D.	0.526 #
12) T	2,4,5-T	0.000	14.381	0	7991509	N.D.	3.963 #
15) T	Picloram	16.759	16.714	5215063	17910424	2.119	7.057 #
16) T	DCPA	0.000	16.639	0	7345298	N.D.	2.362 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022819\
Data File : PS003391.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Mar 2019 00:55
Operator : EI\SJ
Sample : K1341-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HR-06-022719-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 03:47:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

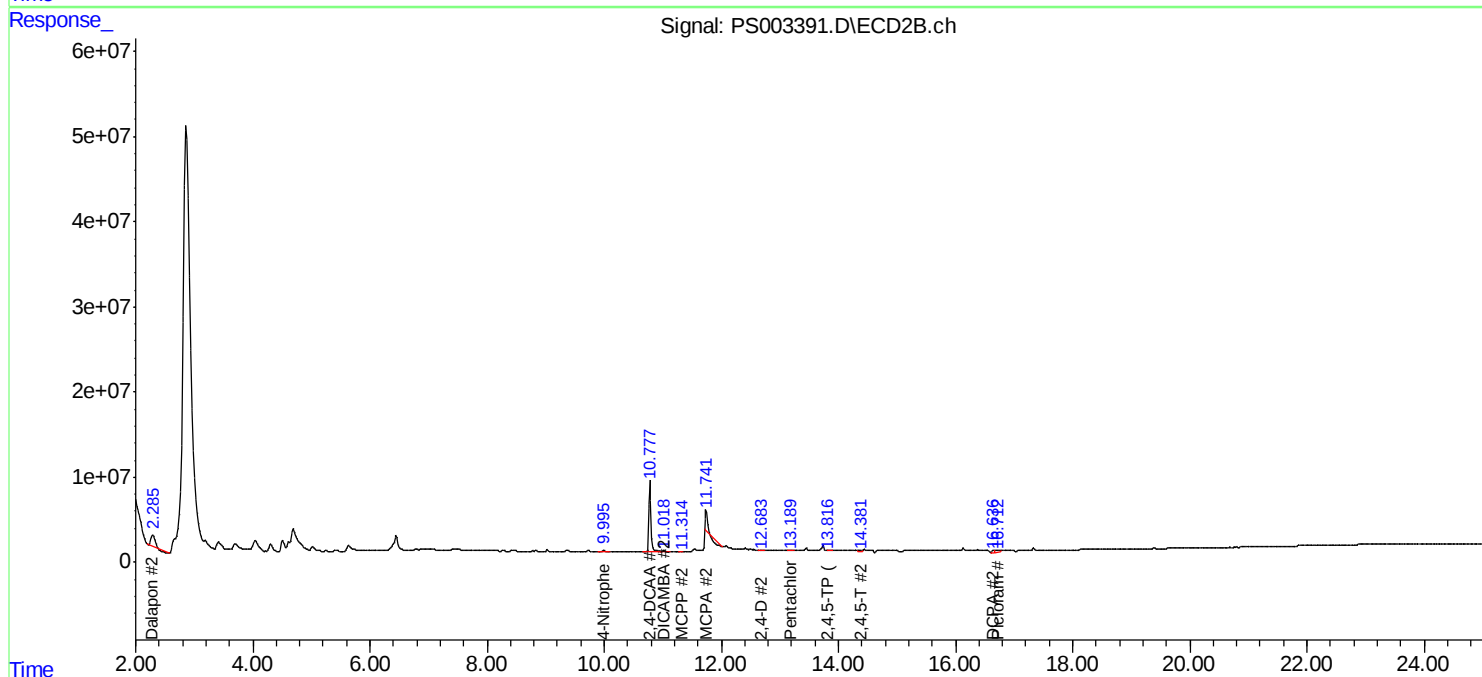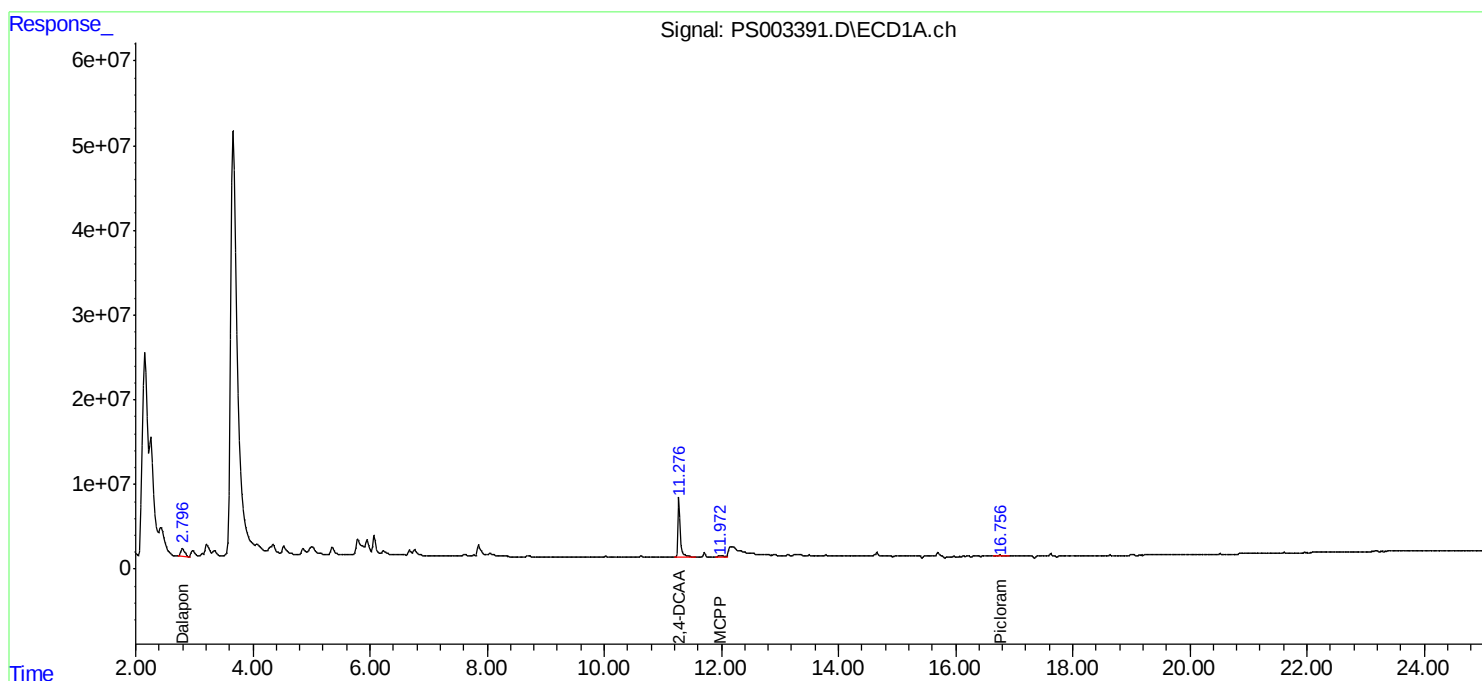


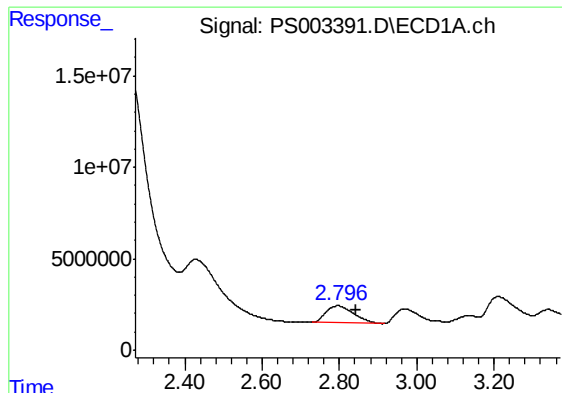

#1 Dalapon


R.T.: 2.796 min
Delta R.T.: -0.048 min
Response: 46075363
Conc: 70.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
HR-06-022719-B

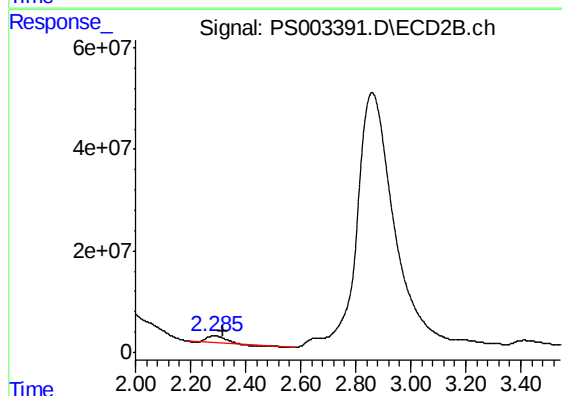


#1 Dalapon

R.T.: 2.284 min
Delta R.T.: -0.033 min
Response: 50558392
Conc: 79.85 ng/ml

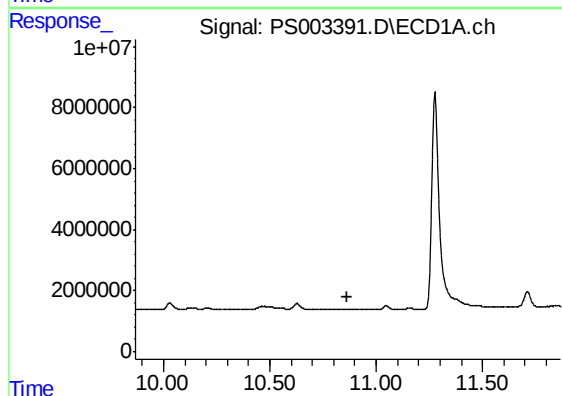


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 10.867 min
Response: 0
Conc: N.D.

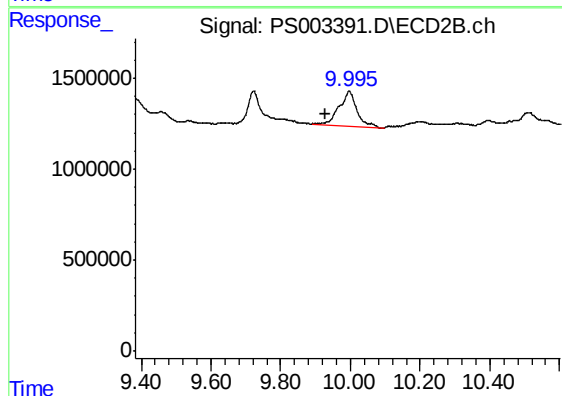

#3 4-Nitrophenol


R.T.: 9.996 min
Delta R.T.: 0.068 min
Response: 6734630
Conc: 29.95 ng/ml

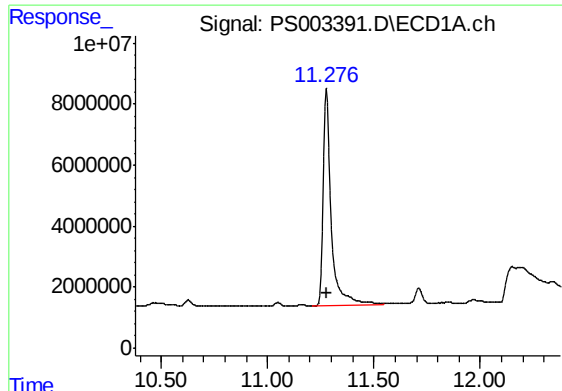

#4 2,4-DCAA


R.T.: 11.276 min
Delta R.T.: -0.001 min
Response: 187323702
Conc: 426.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
HR-06-022719-B

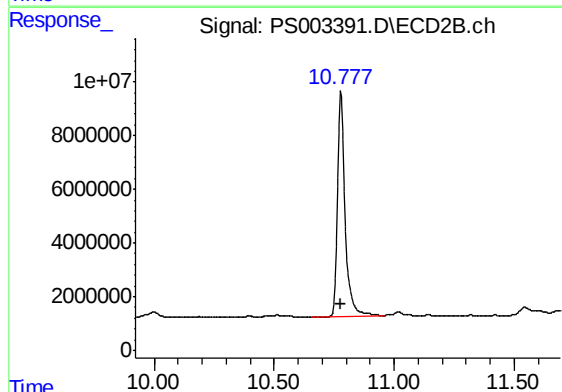


#4 2,4-DCAA

R.T.: 10.777 min
Delta R.T.: -0.002 min
Response: 186645532
Conc: 397.48 ng/ml

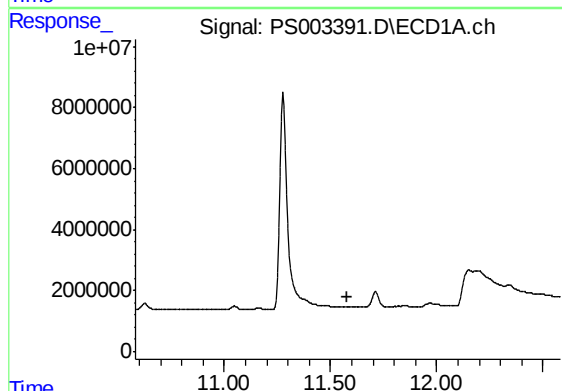


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

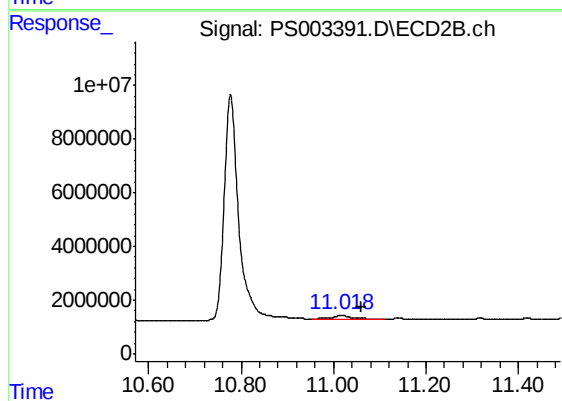

#5 DICAMBA


R.T.: 11.017 min
Delta R.T.: -0.042 min
Response: 5744906
Conc: 3.44 ng/ml

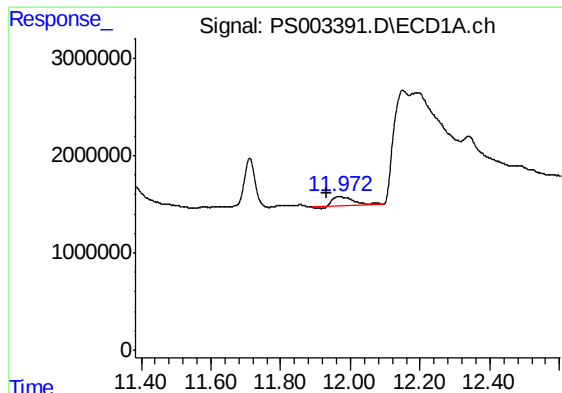

#6 MCPP


R.T.: 11.969 min
Delta R.T.: 0.038 min
Response: 4013546
Conc: 3.06 ug/ml

Instrument :
ECD_S
ClientSampleId :
HR-06-022719-B

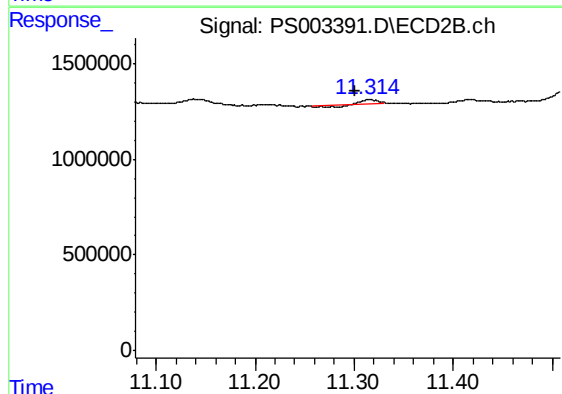


#6 MCPP

R.T.: 11.316 min
Delta R.T.: 0.016 min
Response: 138660
Conc: 0.12 ug/ml

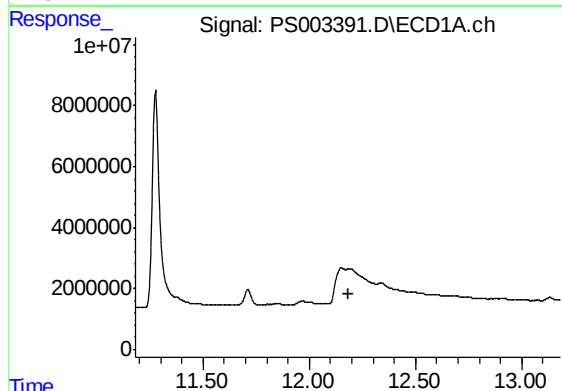


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

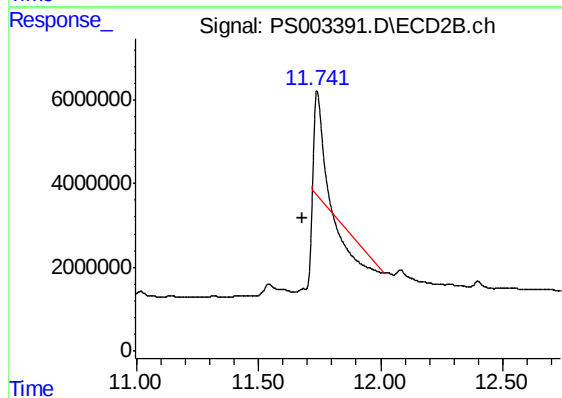

#7 MCPA


R.T.: 11.740 min
Delta R.T.: 0.062 min
Response: 19828855
Conc: 11.50 ug/ml

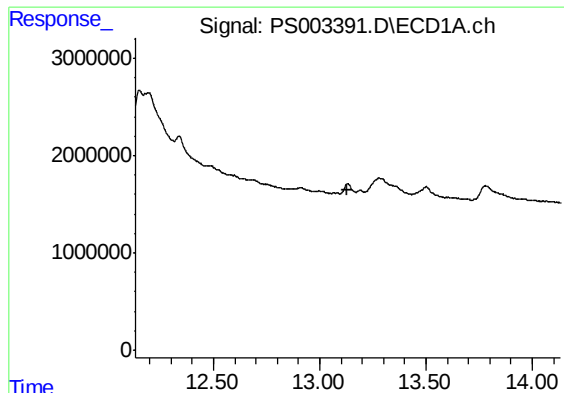

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HR-06-022719-B

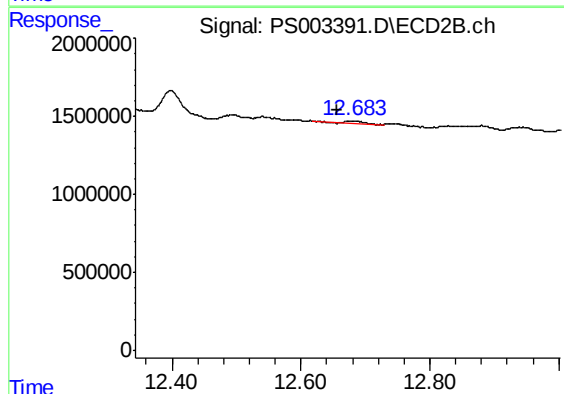


#9 2,4-D

R.T.: 12.681 min
Delta R.T.: 0.024 min
Response: 309588
Conc: 0.59 ng/ml

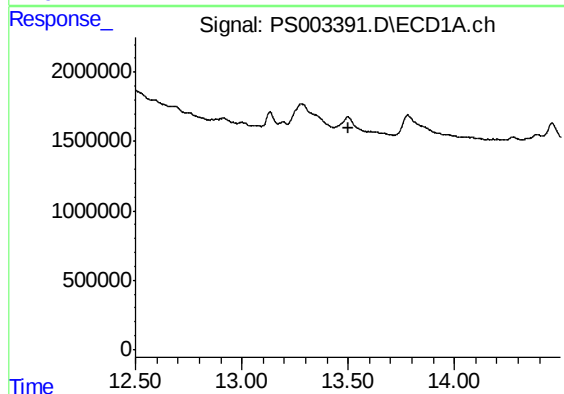


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

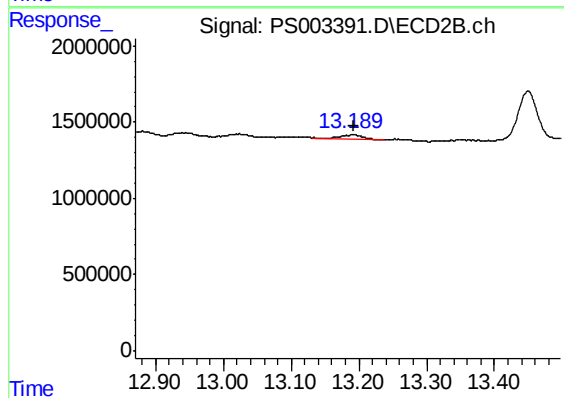

#10 Pentachlorophenol


R.T.: 13.191 min
Delta R.T.: 0.000 min
Response: 607411
Conc: 0.09 ng/ml

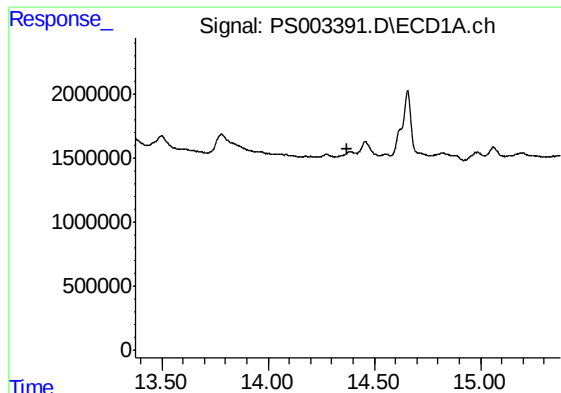

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HR-06-022719-B

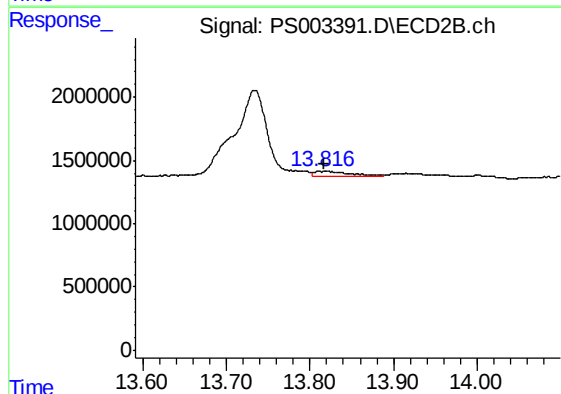


#11 2,4,5-TP (SILVEX)

R.T.: 13.819 min
Delta R.T.: 0.001 min
Response: 1338157
Conc: 0.53 ng/ml

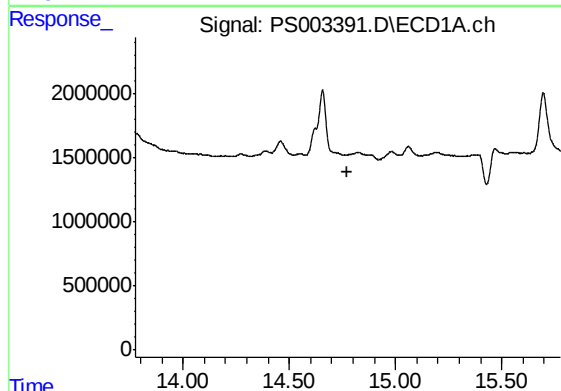


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

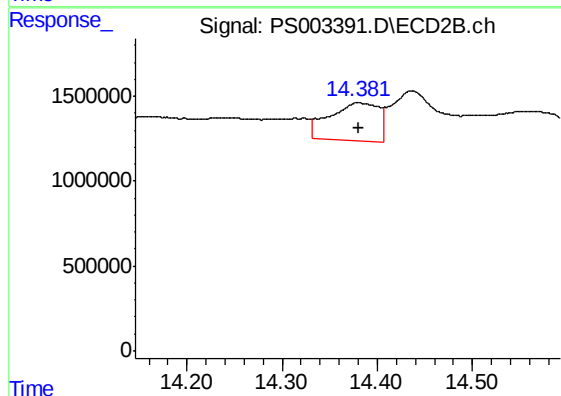

#12 2,4,5-T


R.T.: 14.381 min
Delta R.T.: 0.000 min
Response: 7991509
Conc: 3.96 ng/ml

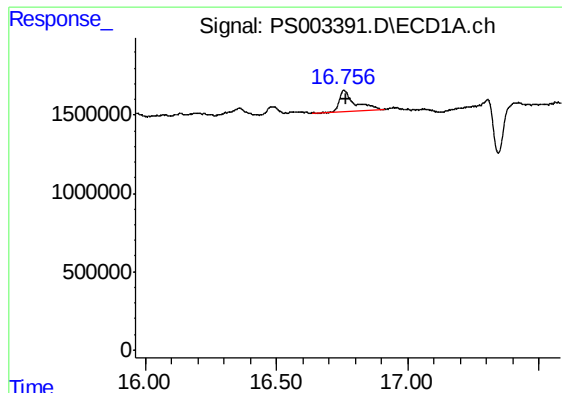

#15 Picloram


R.T.: 16.759 min
Delta R.T.: -0.007 min
Response: 5215063
Conc: 2.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
HR-06-022719-B

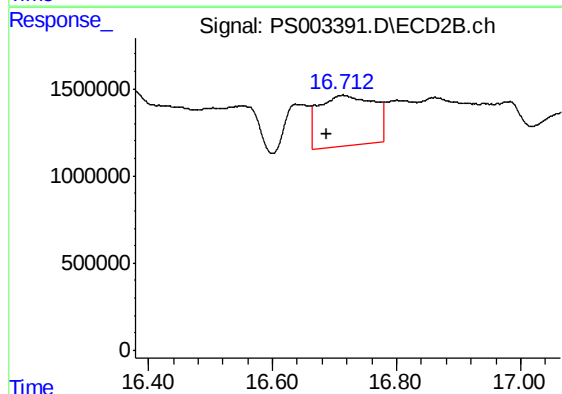


#15 Picloram

R.T.: 16.714 min
Delta R.T.: 0.025 min
Response: 17910424
Conc: 7.06 ng/ml

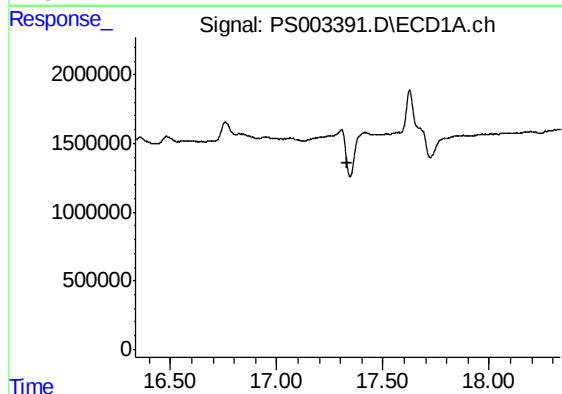

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

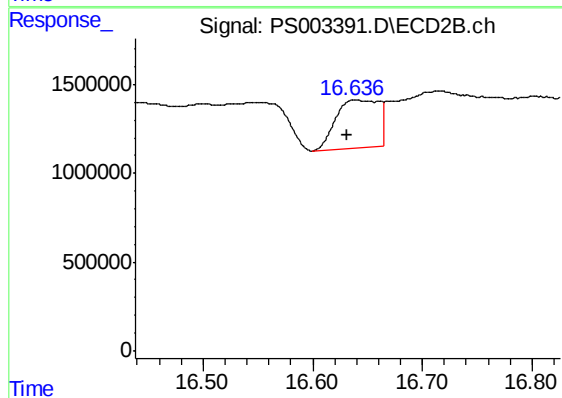

#16 DCPA

R.T.: 16.639 min
Delta R.T.: 0.007 min
Response: 7345298
Conc: 2.36 ng/ml