

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022819\
 Data File : PS003394.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Mar 2019 02:28
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 03:47:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.310	10.811	238.1E6	227.2E6	542.321	483.770
Target Compounds							
3) T	4-Nitroph...	0.000	9.978	0	123382	N.D.	0.549 #
7) T	MCPA	0.000	11.692	0	389908	N.D.	0.226 #
10) T	Pentachlo...	0.000	13.227	0	1181983	N.D.	0.179 #
11) T	2,4,5-TP ...	0.000	13.842	0	308347	N.D.	0.121 #
15) T	Picloram	0.000	16.665	0	426050	N.D.	0.168 #
16) T	DCPA	0.000	16.665	0	426050	N.D.	0.137 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022819\
Data File : PS003394.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Mar 2019 02:28
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 03:47:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

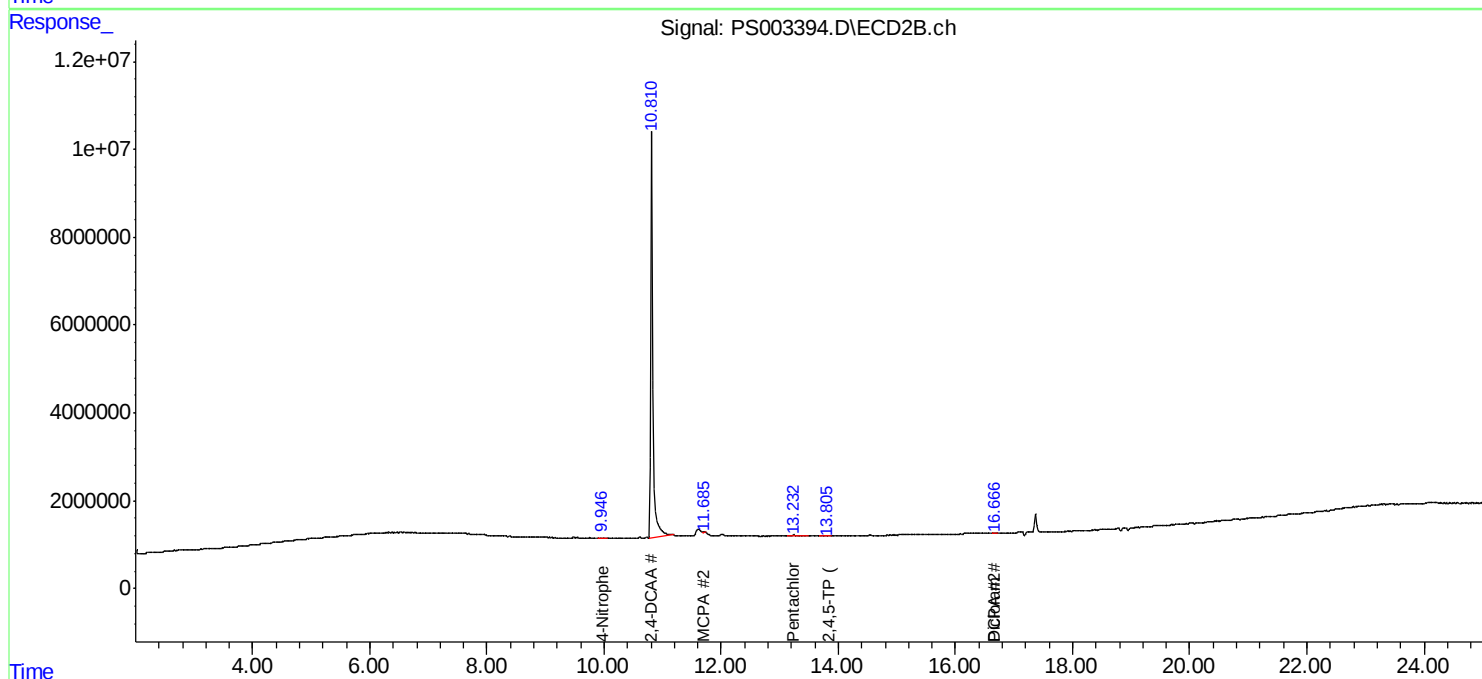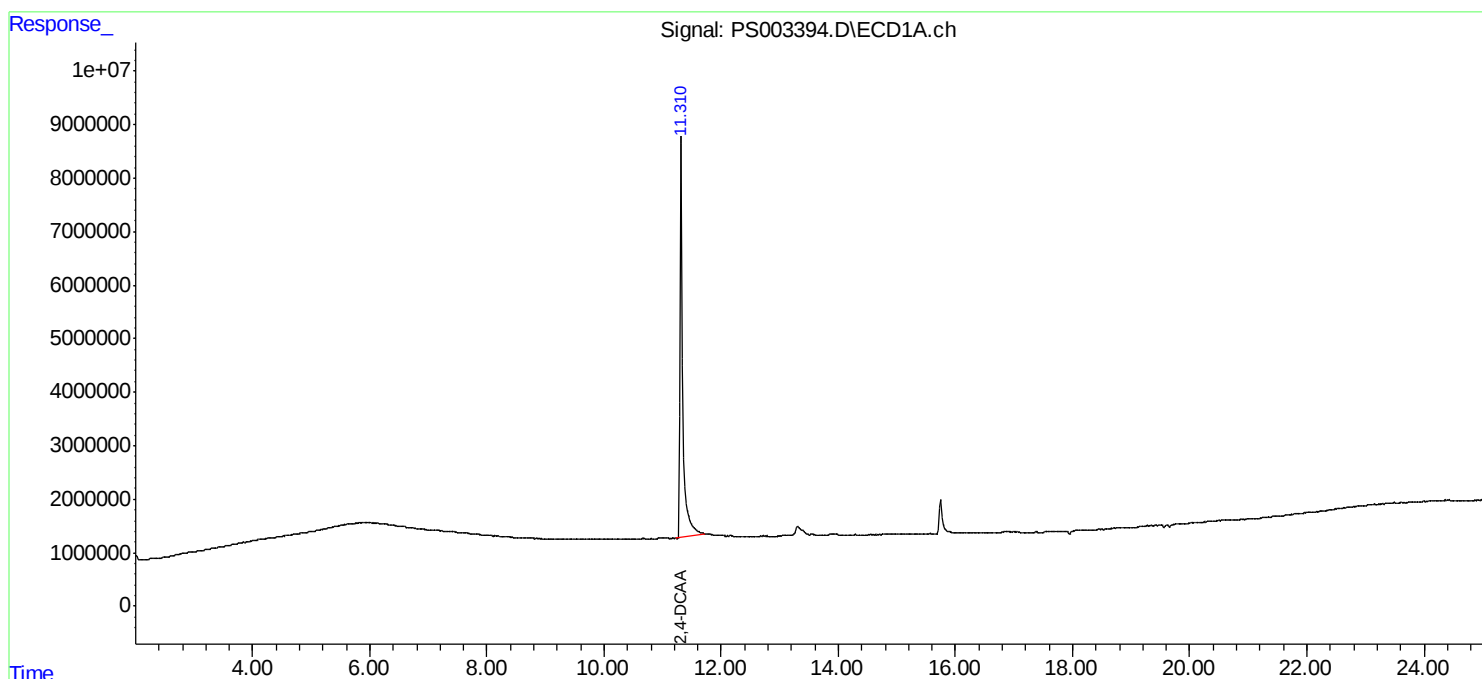


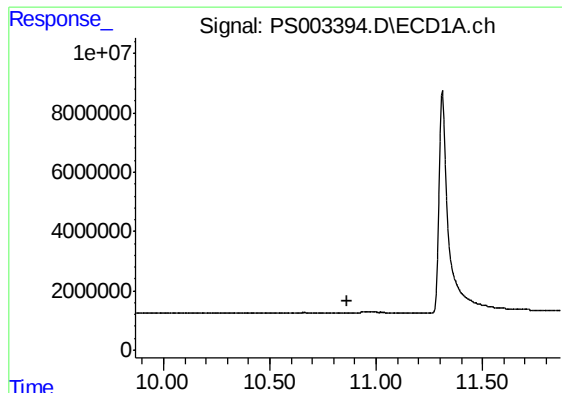

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

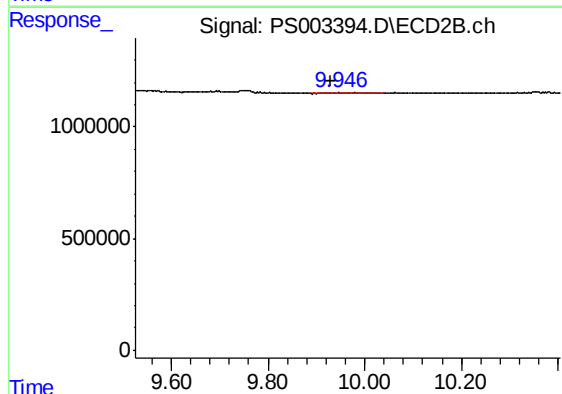


#3 4-Nitrophenol

R.T.: 9.978 min
Delta R.T.: 0.050 min
Response: 123382
Conc: 0.55 ng/ml

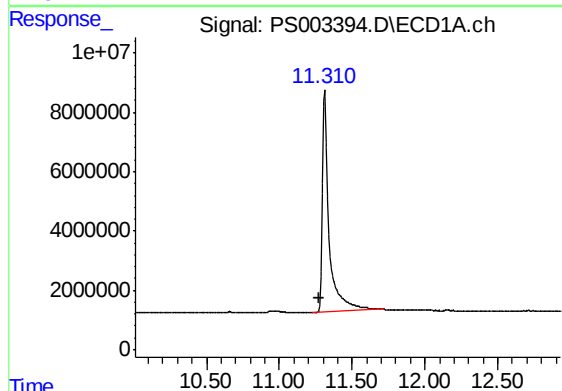


#4 2,4-DCAA

R.T.: 11.310 min
Delta R.T.: 0.033 min
Response: 238092223
Conc: 542.32 ng/ml

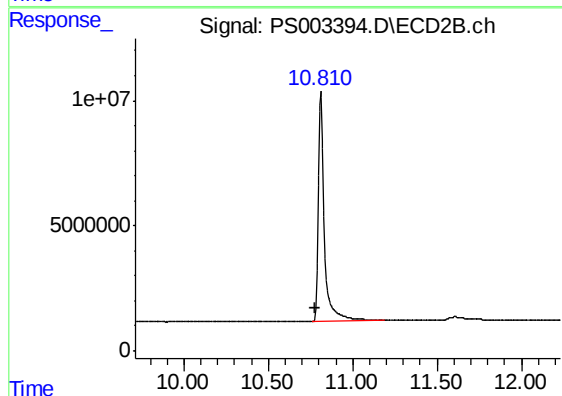

#4 2,4-DCAA


R.T.: 10.811 min
Delta R.T.: 0.031 min
Response: 227163584
Conc: 483.77 ng/ml

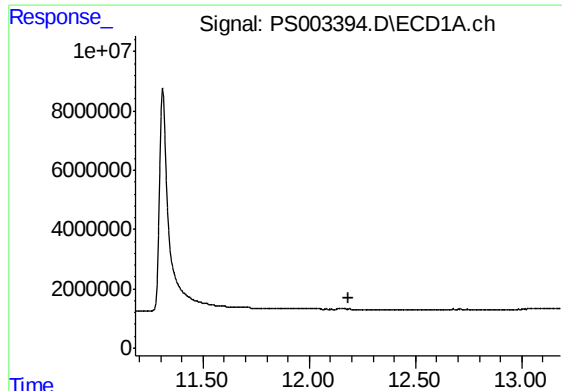

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

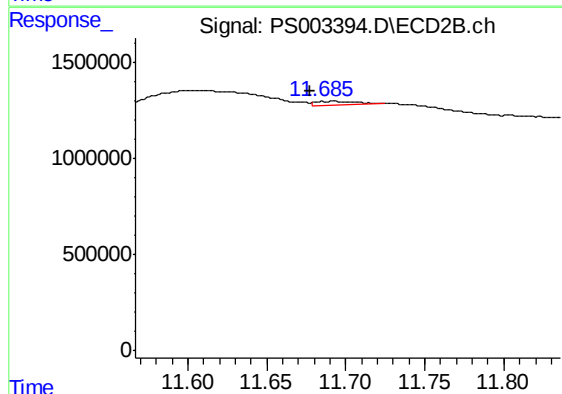


#7 MCPA

R.T.: 11.692 min
Delta R.T.: 0.015 min
Response: 389908
Conc: 0.23 ug/ml

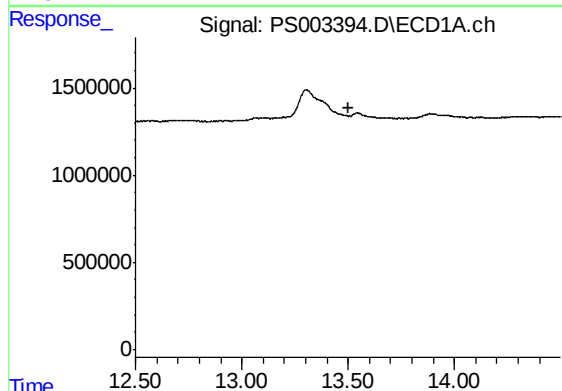


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.499 min
Response: 0
Conc: N.D.

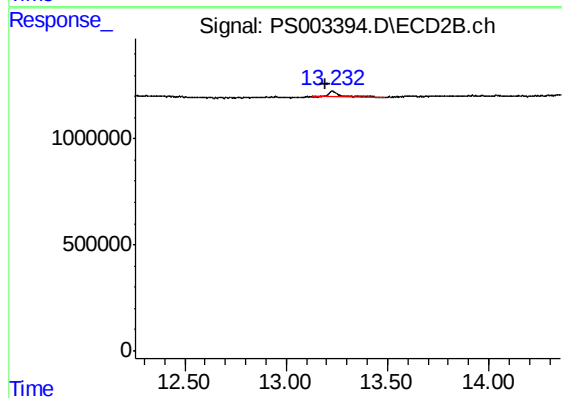

#10 Pentachlorophenol


R.T.: 13.227 min
Delta R.T.: 0.036 min
Response: 1181983
Conc: 0.18 ng/ml

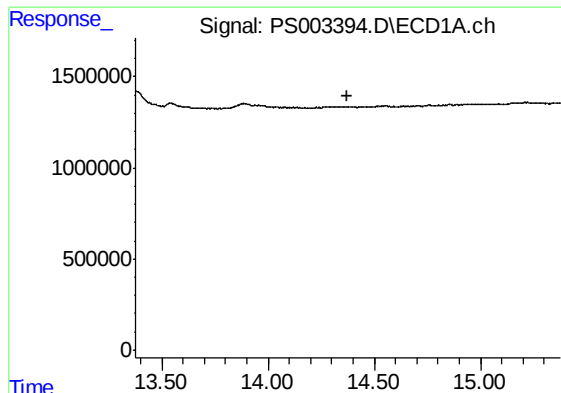

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 14.376 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

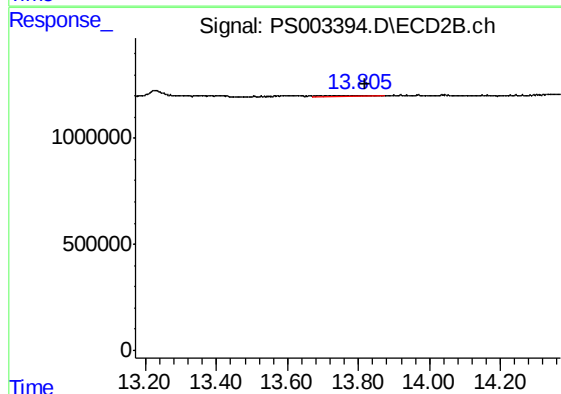


#11 2,4,5-TP (SILVEX)

R.T.: 13.842 min
Delta R.T.: 0.025 min
Response: 308347
Conc: 0.12 ng/ml

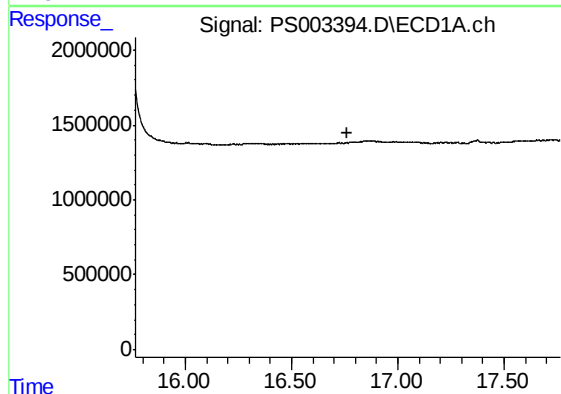


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

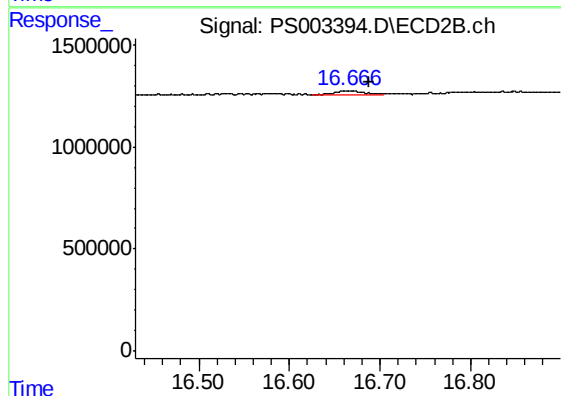

#15 Picloram


R.T.: 16.665 min
Delta R.T.: -0.023 min
Response: 426050
Conc: 0.17 ng/ml

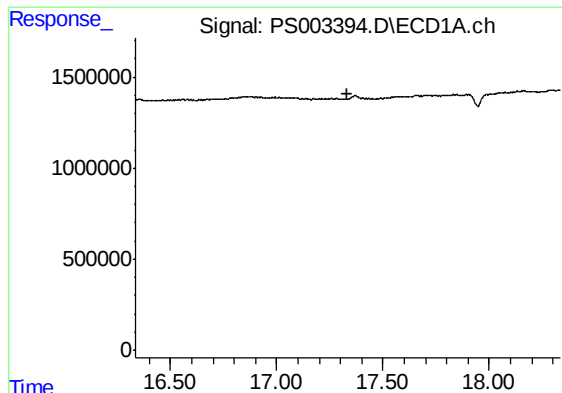

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

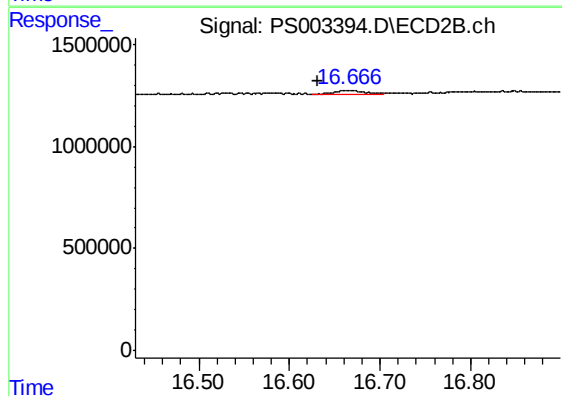

#16 DCPA

R.T.: 16.665 min
Delta R.T.: 0.033 min
Response: 426050
Conc: 0.14 ng/ml