

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
 Data File : PS009045.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2020 12:41
 Operator : DD\AJ
 Sample : L1656-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 29 00:10:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.251	6.939	759.1E6	328.2E6	347.181	340.664
Target Compounds							
1) T	Dalapon	3.006	2.586	118.5E6	181.8E6	39.617	124.361 #
2) T	3,5-DICHL...	0.000	6.113	0	80997246	N.D.	55.505
5) T	DICAMBA	7.371	0.000	113.7E6	0	13.995	N.D. #
7) T	MCPA	7.803	7.407	243.7E6	128.5E6	30.297	29.048
8) T	DICHLORPROP	0.000	7.759	0	60409769	N.D.	60.293
10) T	Pentachlo...	0.000	8.464	0	19939415	N.D.	1.403
11) T	2,4,5-TP ...	0.000	8.827	0	14741797	N.D.	2.721
12) T	2,4,5-T	9.460	9.207	212.7E6	30054969	19.890	5.552 #
13) T	2,4-DB	0.000	9.709	0	17247958	N.D.	24.554
14) T	DINOSEB	0.000	10.053	0	29474343	N.D.	7.454
15) T	Picloram	11.049	11.031	1223.9E6	643.4E6	89.396	88.542
16) T	DCPA	11.504	10.982	65218693	31693437	4.746	4.580



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
Data File : PS009045.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2020 12:41
Operator : DD\AJ
Sample : L1656-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 29 00:10:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

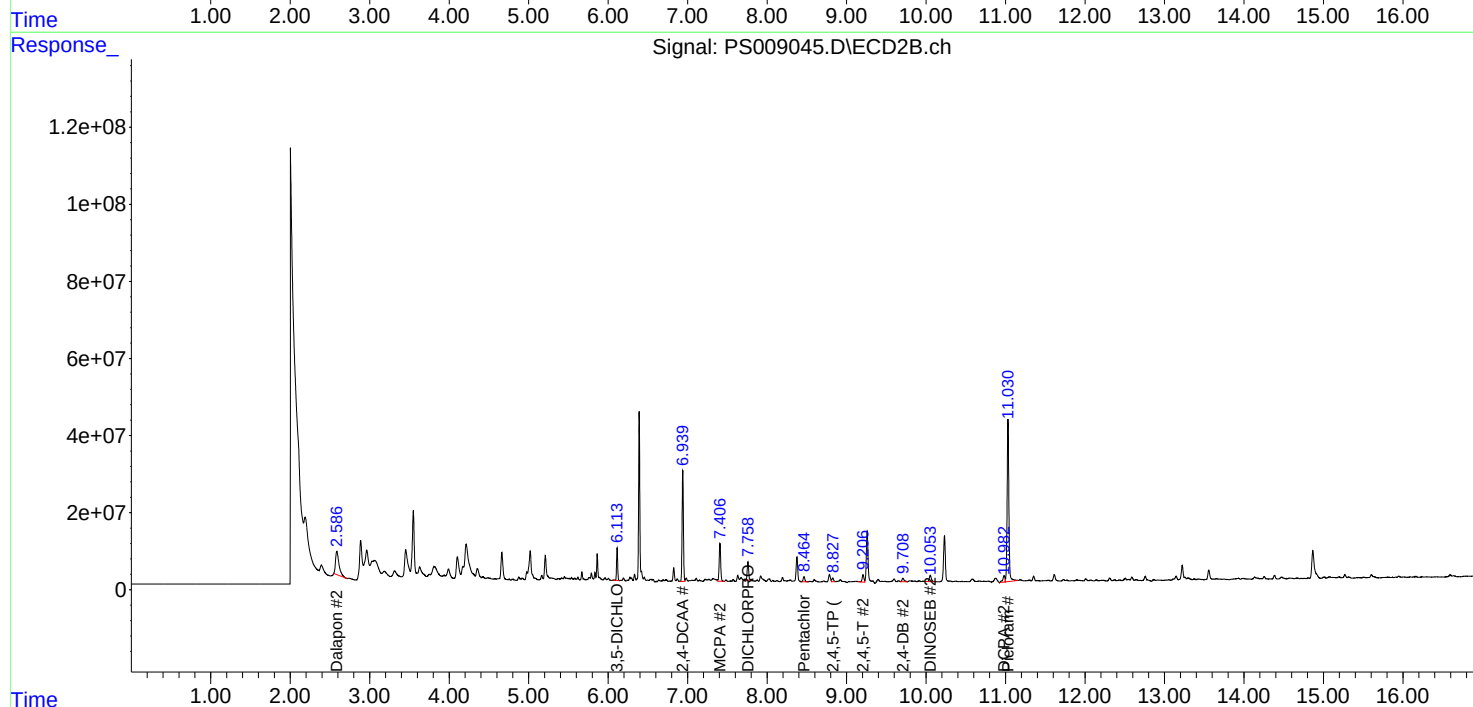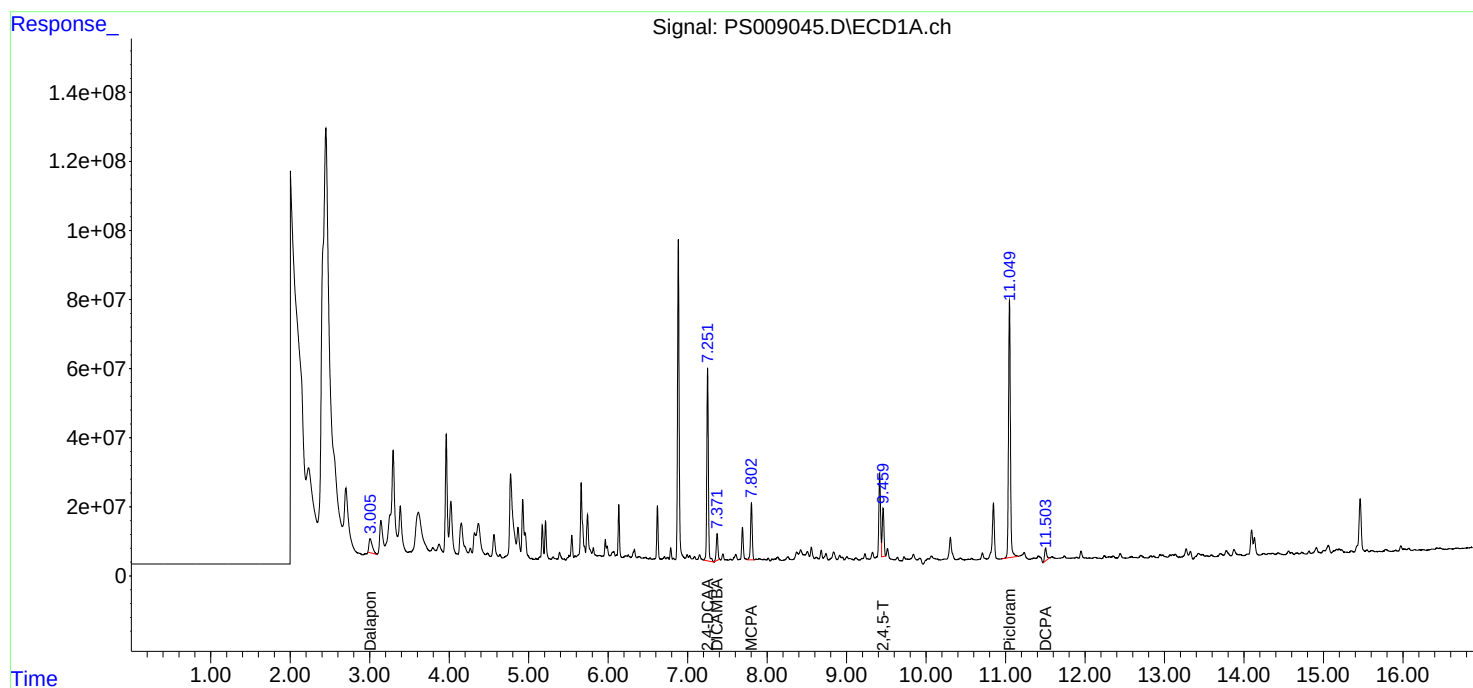


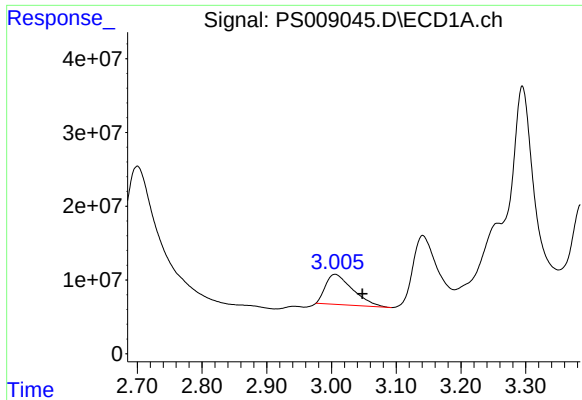

#1 Dalapon


R.T.: 3.006 min
Delta R.T.: -0.042 min
Response: 118525264
Conc: 39.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

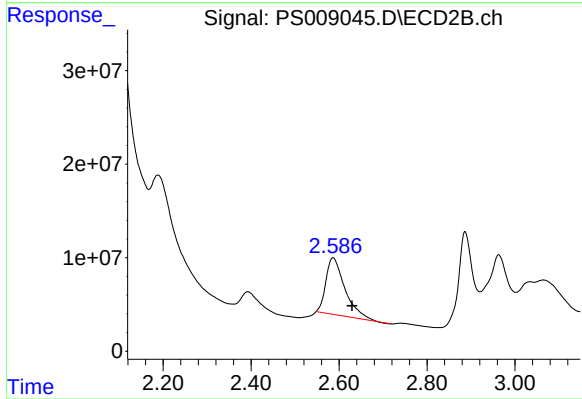


#1 Dalapon

R.T.: 2.586 min
Delta R.T.: -0.043 min
Response: 181843715
Conc: 124.36 ng/ml

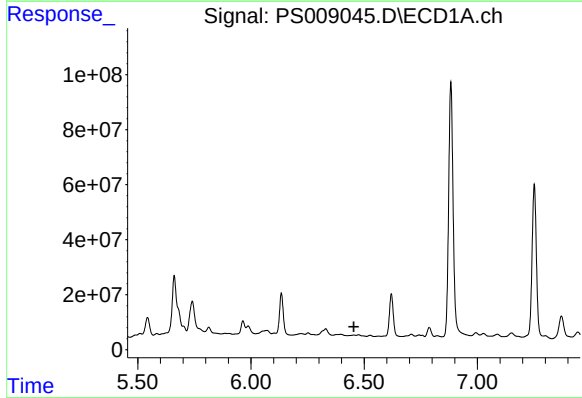


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.455 min
Response: 0
Conc: N.D.

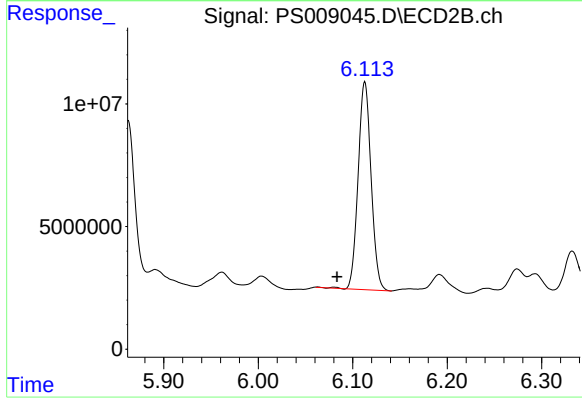

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.113 min
Delta R.T.: 0.029 min
Response: 80997246
Conc: 55.51 ng/ml

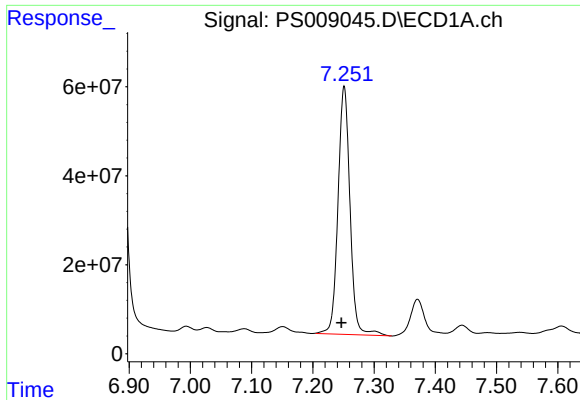

#4 2,4-DCAA


R.T.: 7.251 min
Delta R.T.: 0.004 min
Response: 759143249
Conc: 347.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

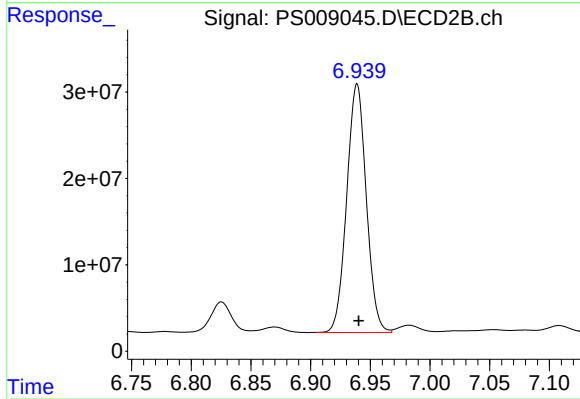


#4 2,4-DCAA

R.T.: 6.939 min
Delta R.T.: -0.002 min
Response: 328248362
Conc: 340.66 ng/ml

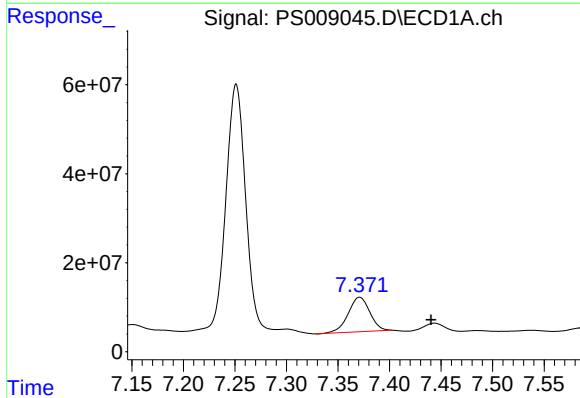


#5 DICAMBA

R.T.: 7.371 min
Delta R.T.: -0.069 min
Response: 113694618
Conc: 14.00 ng/ml

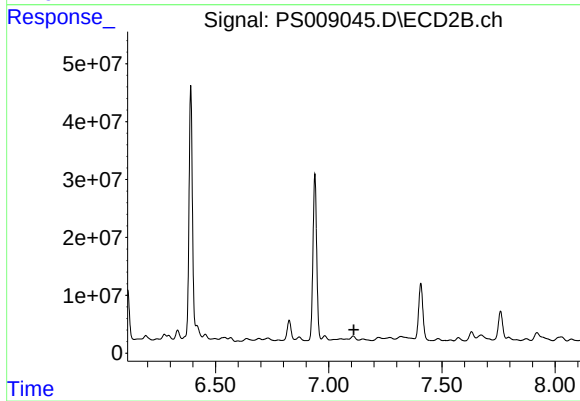

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.111 min
Response: 0
Conc: N.D.

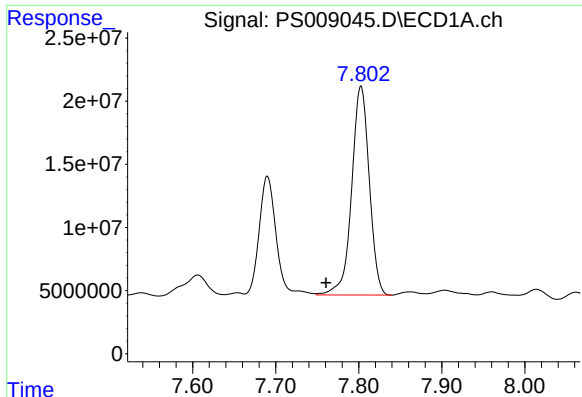

#7 MCPA


R.T.: 7.803 min
Delta R.T.: 0.042 min
Response: 243709948
Conc: 30.30 ug/ml

Instrument :
ECD_S
ClientSampleId :

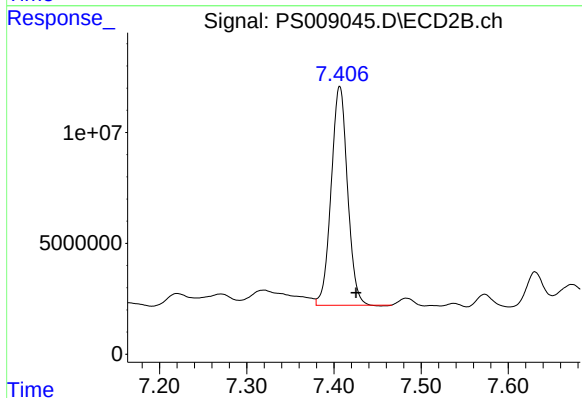


#7 MCPA

R.T.: 7.407 min
Delta R.T.: -0.019 min
Response: 128517235
Conc: 29.05 ug/ml

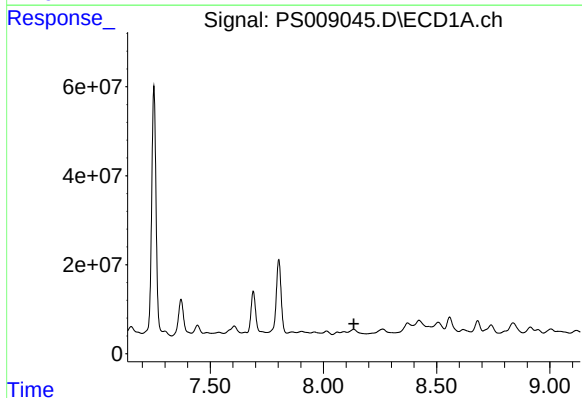


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

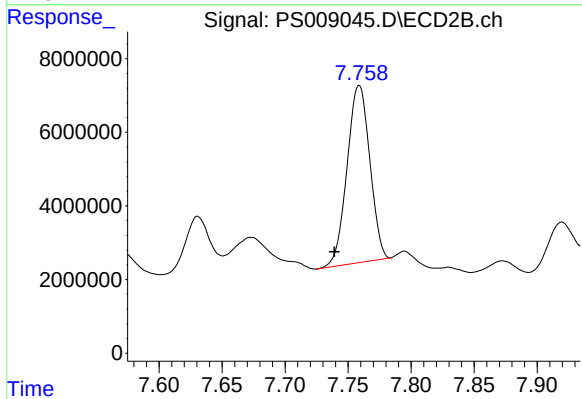

#8 DICHLORPROP


R.T.: 7.759 min
Delta R.T.: 0.020 min
Response: 60409769
Conc: 60.29 ng/ml

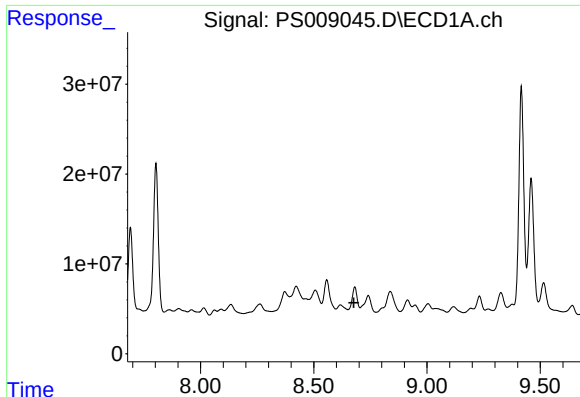

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.677 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

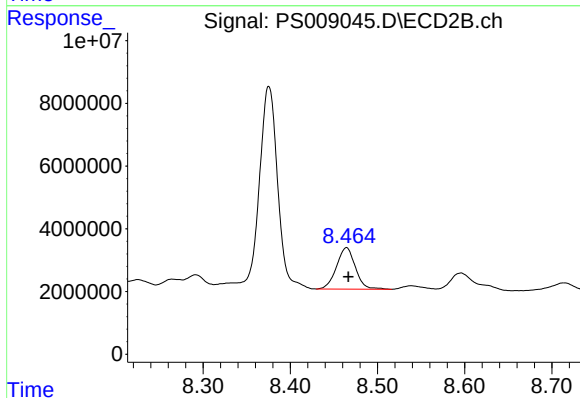


#10 Pentachlorophenol

R.T.: 8.464 min
Delta R.T.: -0.002 min
Response: 19939415
Conc: 1.40 ng/ml

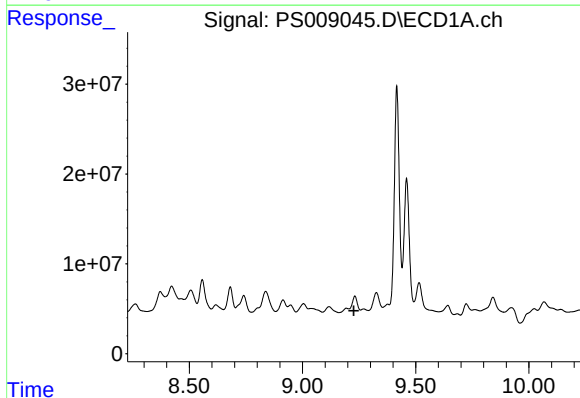


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

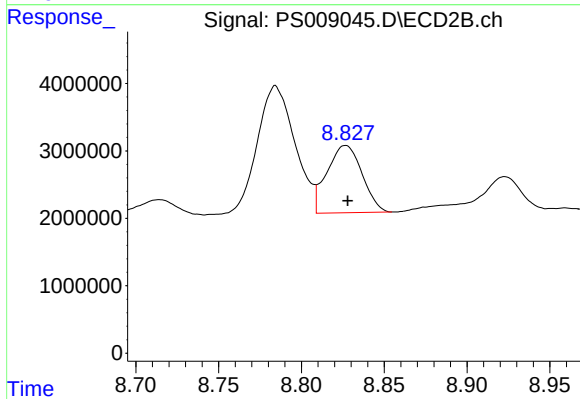

#11 2,4,5-TP (SILVEX)


R.T.: 8.827 min
Delta R.T.: -0.001 min
Response: 14741797
Conc: 2.72 ng/ml

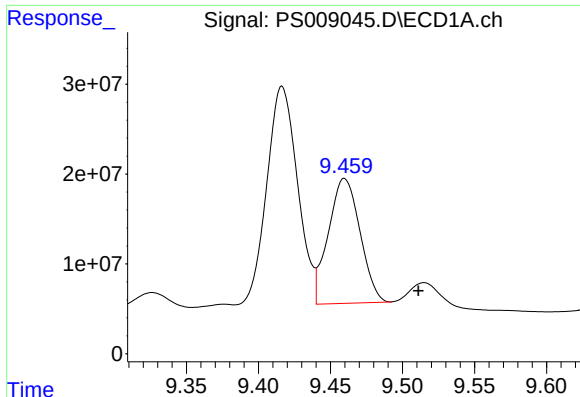

#12 2,4,5-T


R.T.: 9.460 min
Delta R.T.: -0.051 min
Response: 212663555
Conc: 19.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

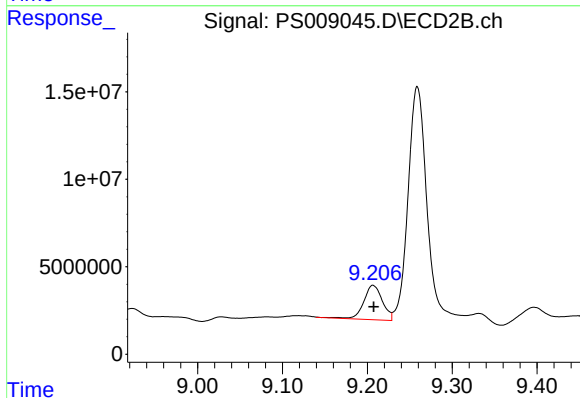


#12 2,4,5-T

R.T.: 9.207 min
Delta R.T.: 0.000 min
Response: 30054969
Conc: 5.55 ng/ml

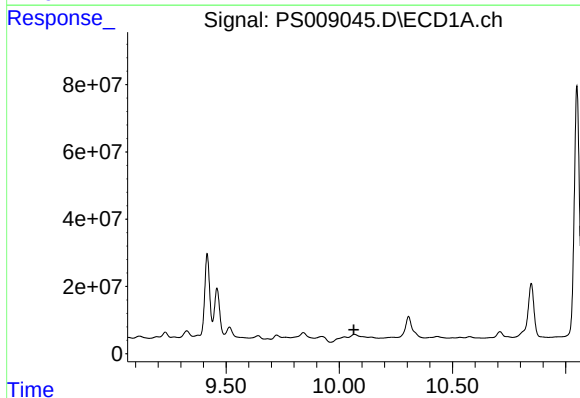


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.064 min
Response: 0
Conc: N.D.

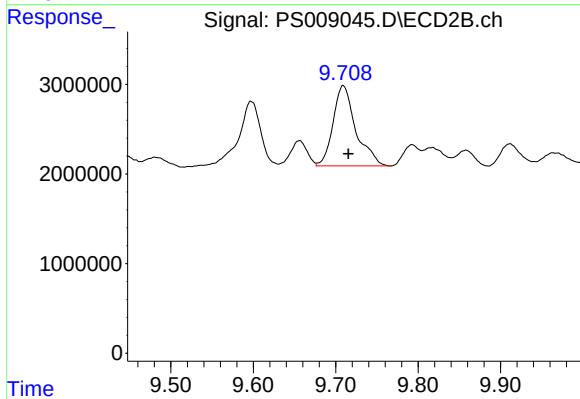

#13 2,4-DB


R.T.: 9.709 min
Delta R.T.: -0.006 min
Response: 17247958
Conc: 24.55 ng/ml

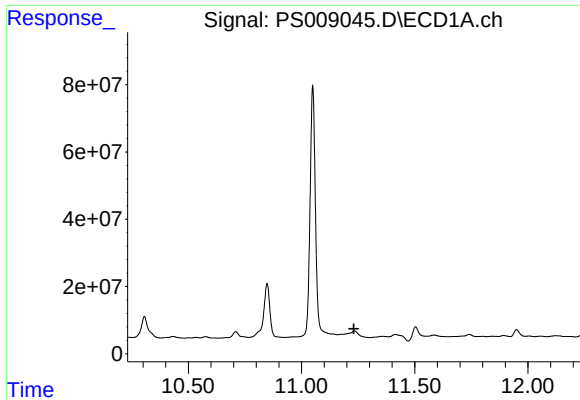

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

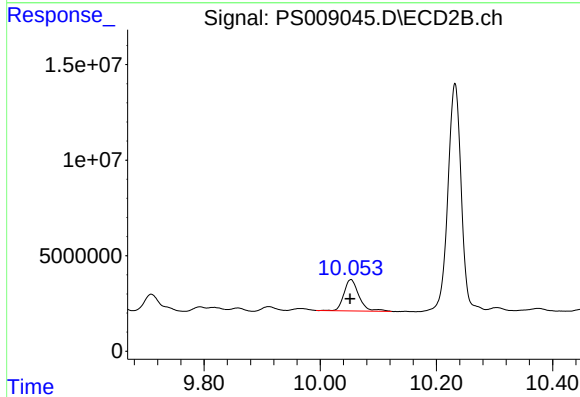


#14 DINOSEB

R.T.: 10.053 min
Delta R.T.: 0.001 min
Response: 29474343
Conc: 7.45 ng/ml

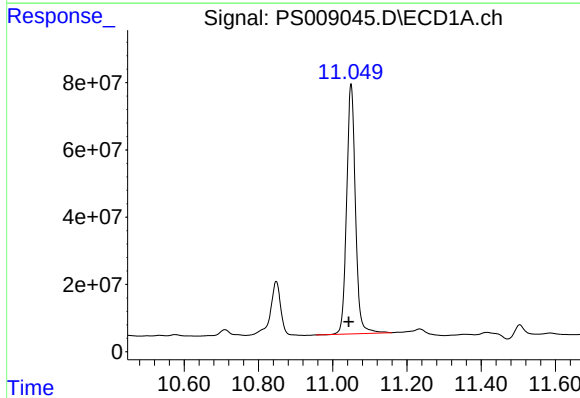


#15 Picloram

R.T.: 11.049 min
Delta R.T.: 0.006 min
Response: 1223914992
Conc: 89.40 ng/ml

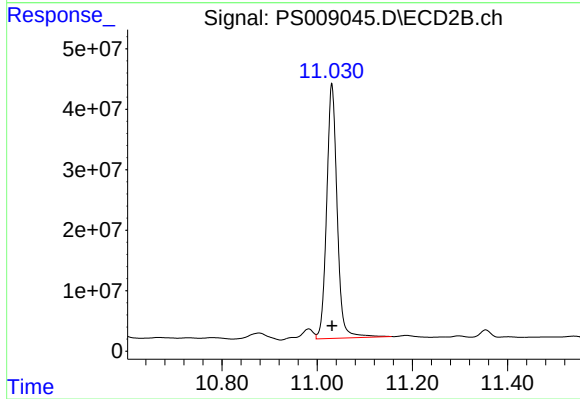

#15 Picloram


R.T.: 11.031 min
Delta R.T.: 0.000 min
Response: 643392547
Conc: 88.54 ng/ml

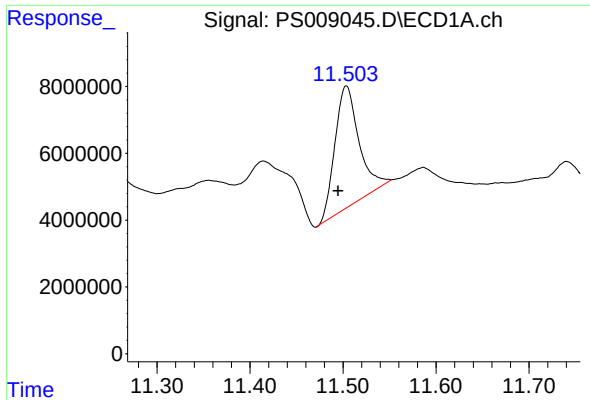

#16 DCPA

R.T.: 11.504 min
Delta R.T.: 0.009 min
Response: 65218693
Conc: 4.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

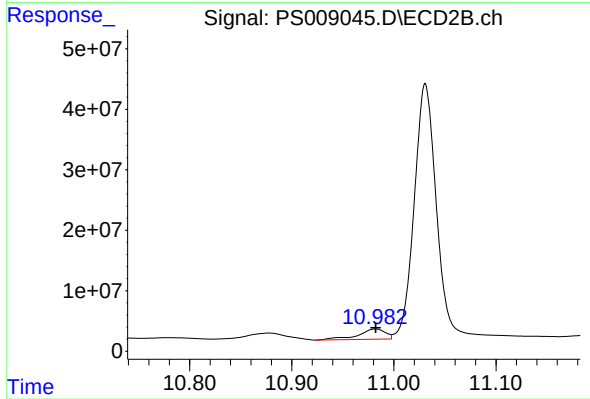

#16 DCPA

R.T.: 10.982 min
Delta R.T.: 0.000 min
Response: 31693437
Conc: 4.58 ng/ml