

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
 Data File : PS009046.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2020 13:03
 Operator : DD\AJ
 Sample : L1681-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 29 00:11:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.248	6.939	854.0E6	365.7E6	390.576	379.549
Target Compounds							
1) T	Dalapon	0.000	2.591	0 50321229		N.D.	34.414
2) T	3,5-DICHL...	0.000	6.114	0 76324169		N.D.	52.303
5) T	DICAMBA	0.000	7.074	0 15790780		N.D.	3.815
7) T	MCPA	7.800	7.407	67853024 45770867		8.435	10.345
8) T	DICHLORPROP	0.000	7.760	0 17643702		N.D.	17.610
11) T	2,4,5-TP ...	0.000	8.795	0 211.3E6		N.D.	38.998
12) T	2,4,5-T	9.458	0.000	123.1E6	0	11.511	N.D. #
13) T	2,4-DB	0.000	9.655	0 23189070		N.D.	33.012
14) T	DINOSEB	0.000	10.062	0 15665071		N.D.	3.962
15) T	Picloram	0.000	11.029	0 40787829		N.D.	5.613
16) T	DCPA	0.000	11.029	0 40787829		N.D.	5.895



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
Data File : PS009046.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2020 13:03
Operator : DD\AJ
Sample : L1681-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 29 00:11:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

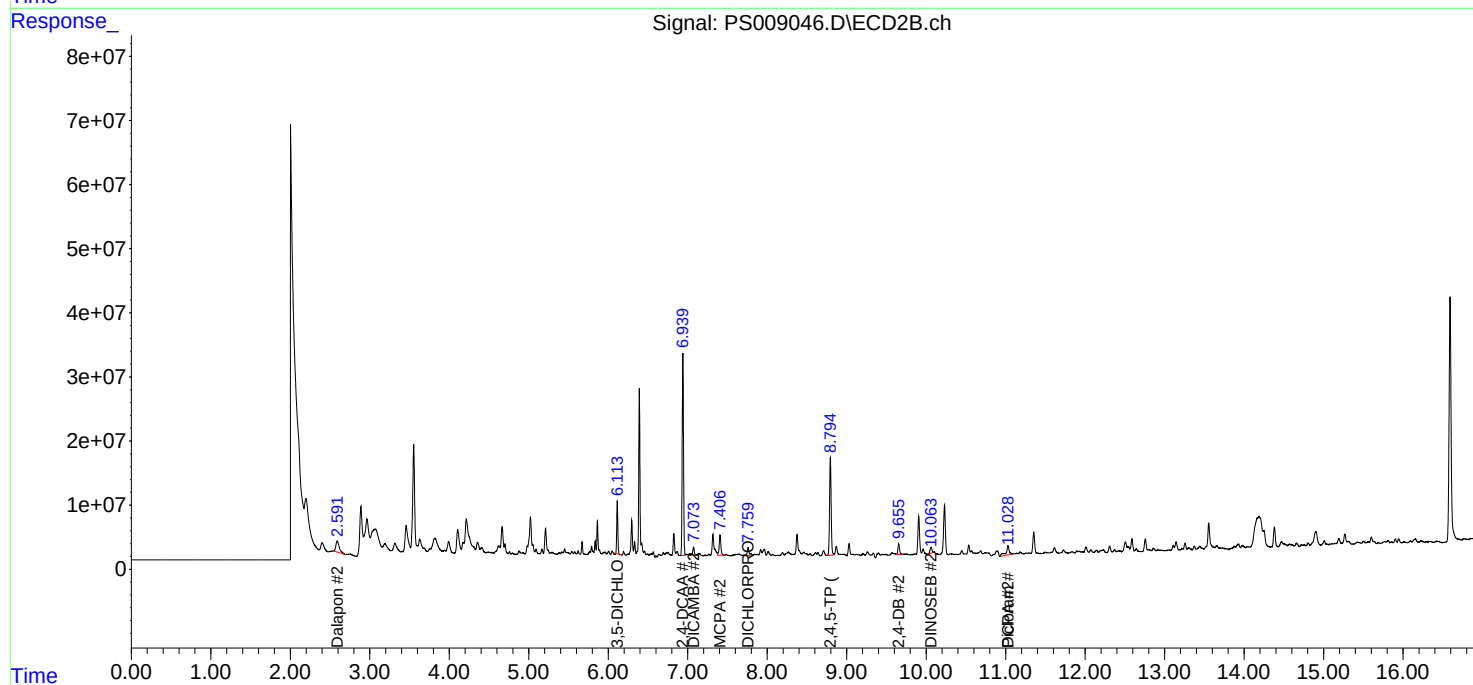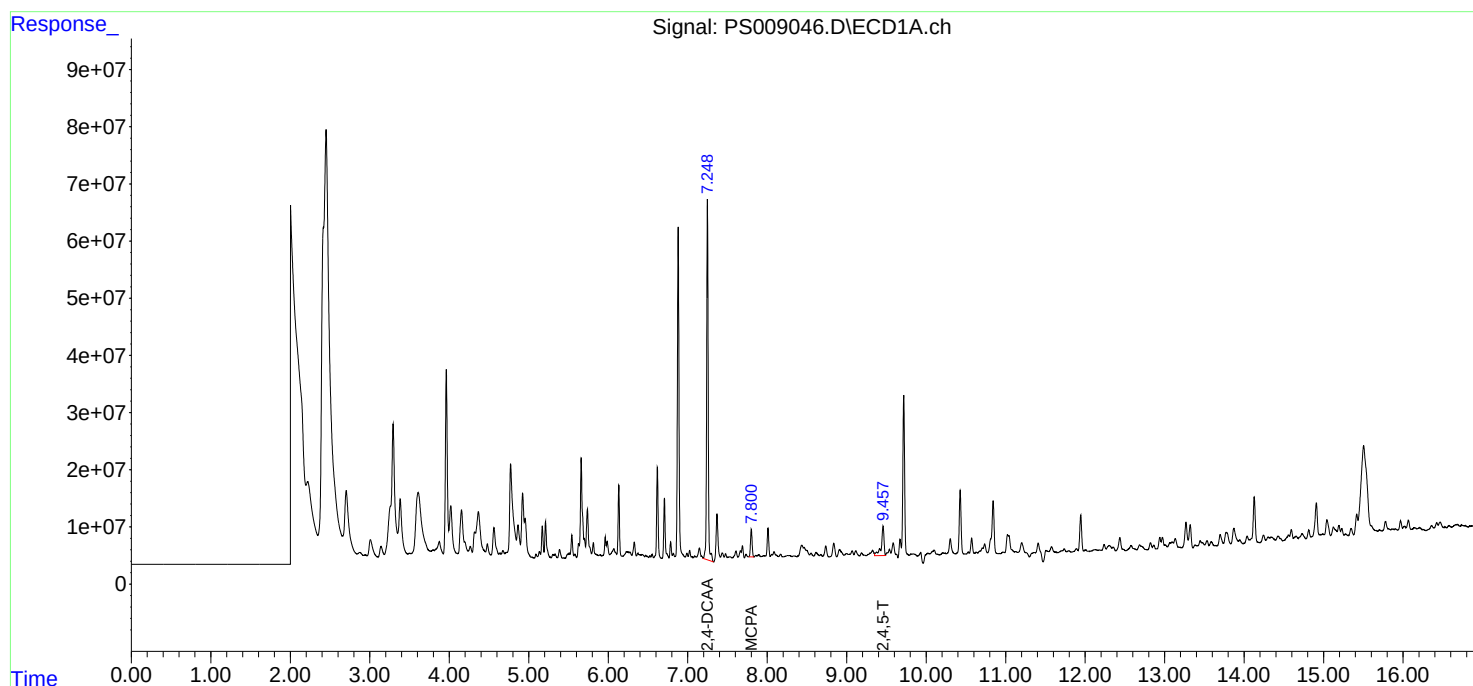


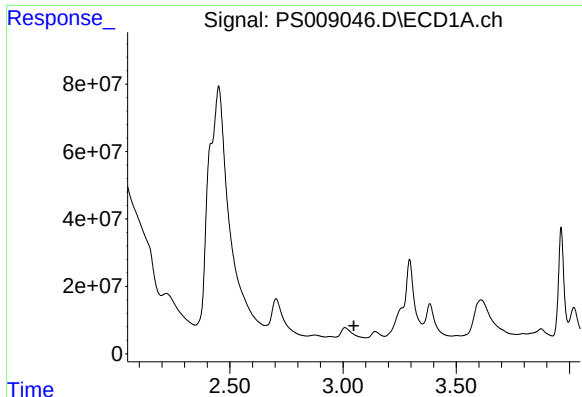

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

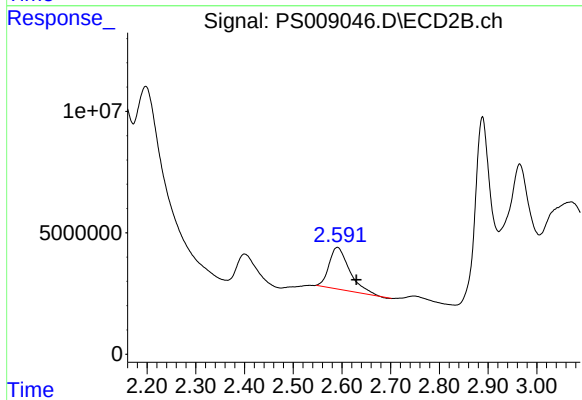


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.039 min
Response: 50321229
Conc: 34.41 ng/ml

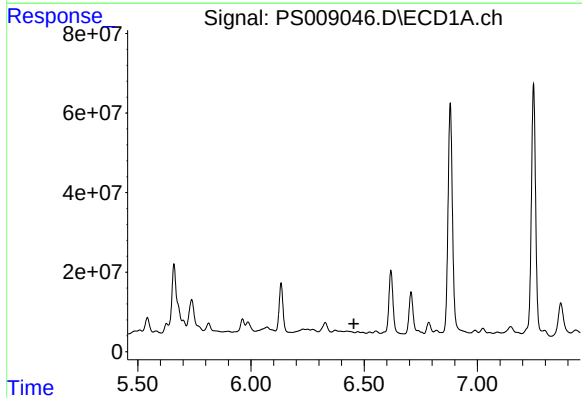


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

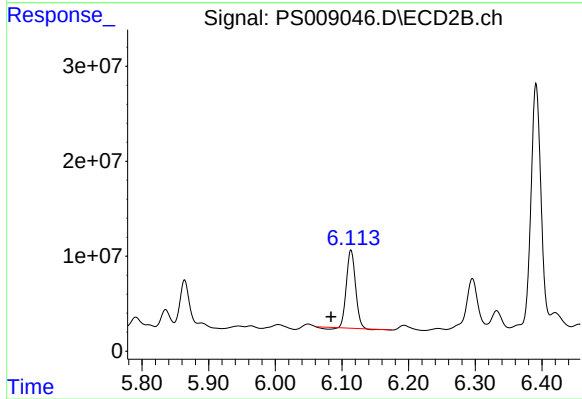

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.030 min
Response: 76324169
Conc: 52.30 ng/ml

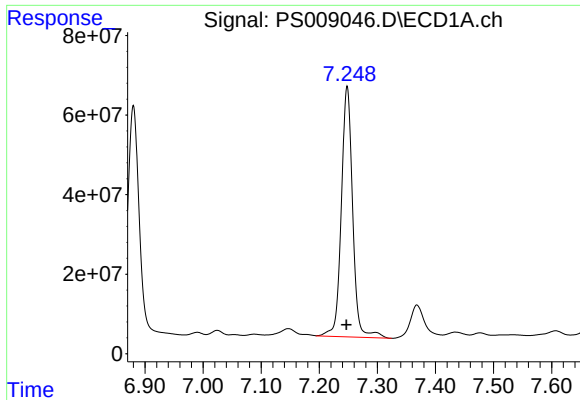

#4 2,4-DCAA


R.T.: 7.248 min
Delta R.T.: 0.001 min
Response: 854030679
Conc: 390.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

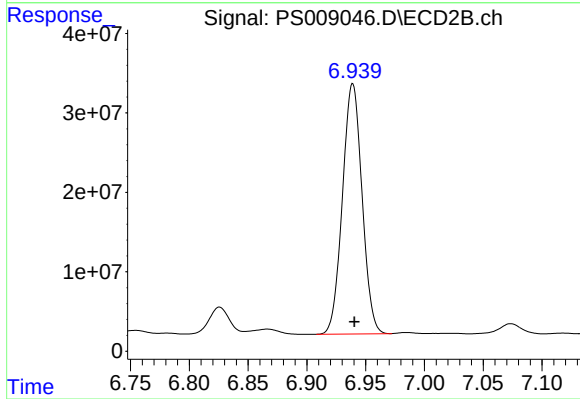


#4 2,4-DCAA

R.T.: 6.939 min
Delta R.T.: -0.001 min
Response: 365716494
Conc: 379.55 ng/ml

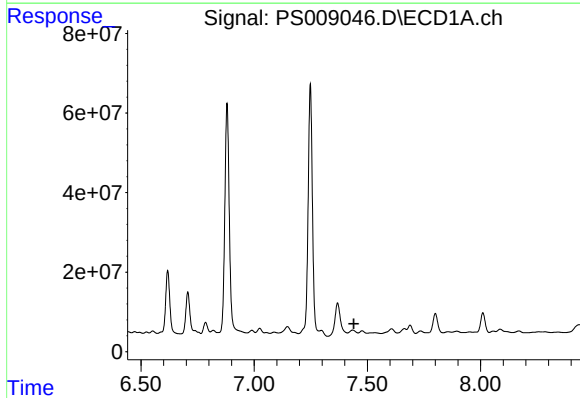


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.

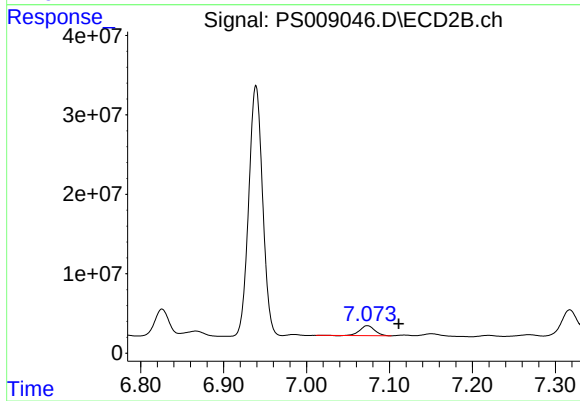

#5 DICAMBA


R.T.: 7.074 min
Delta R.T.: -0.038 min
Response: 15790780
Conc: 3.81 ng/ml

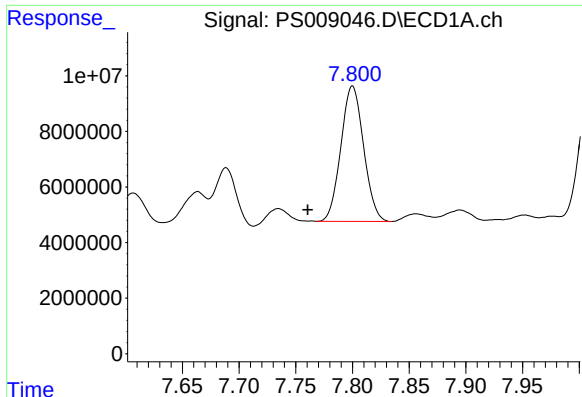

#7 MCPA


R.T.: 7.800 min
Delta R.T.: 0.039 min
Response: 67853024
Conc: 8.44 ug/ml

Instrument :
ECD_S
ClientSampleId :

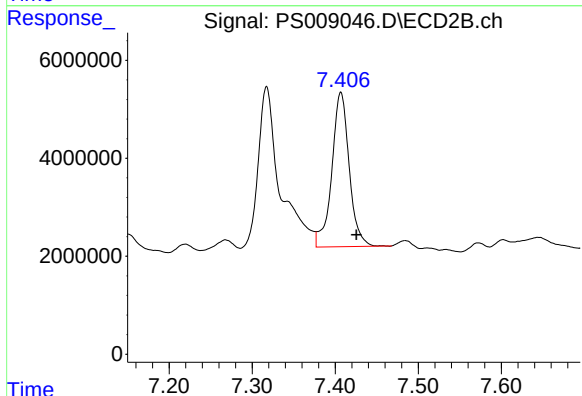


#7 MCPA

R.T.: 7.407 min
Delta R.T.: -0.019 min
Response: 45770867
Conc: 10.35 ug/ml

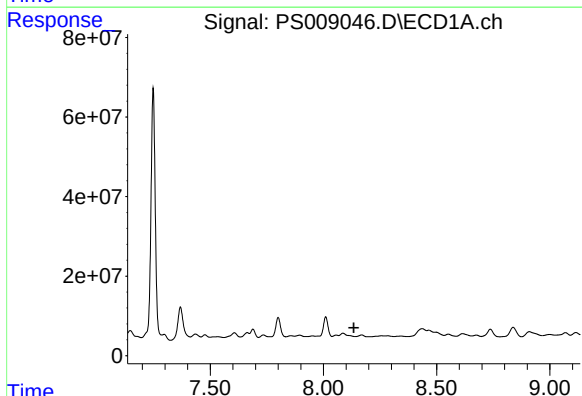


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

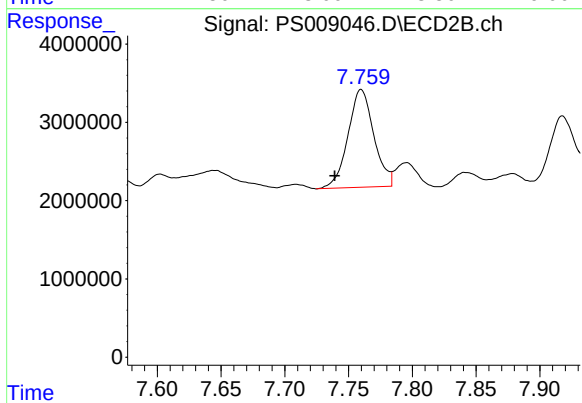

#8 DICHLORPROP


R.T.: 7.760 min
Delta R.T.: 0.021 min
Response: 17643702
Conc: 17.61 ng/ml

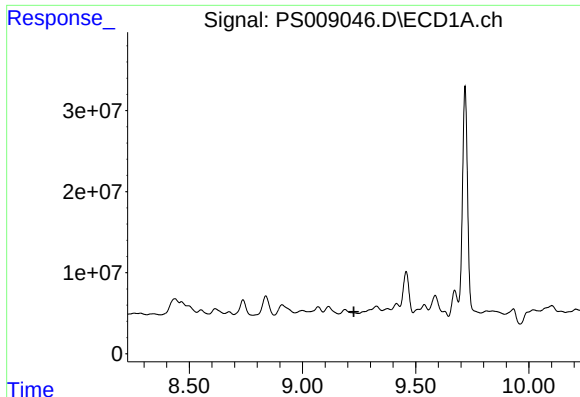

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

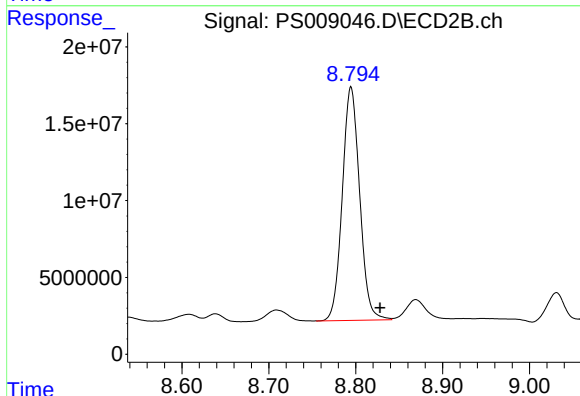


#11 2,4,5-TP (SILVEX)

R.T.: 8.795 min
Delta R.T.: -0.033 min
Response: 211251225
Conc: 39.00 ng/ml

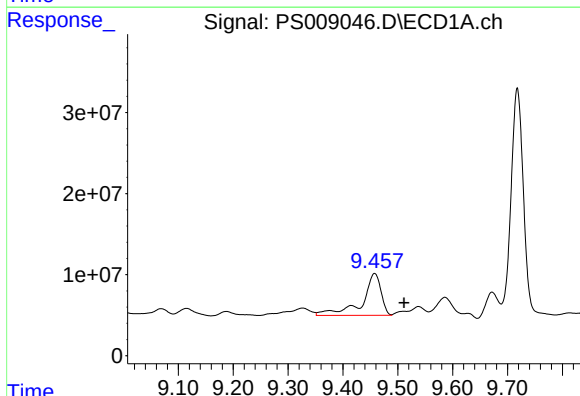


#12 2,4,5-T

R.T.: 9.458 min
Delta R.T.: -0.053 min
Response: 123080721
Conc: 11.51 ng/ml

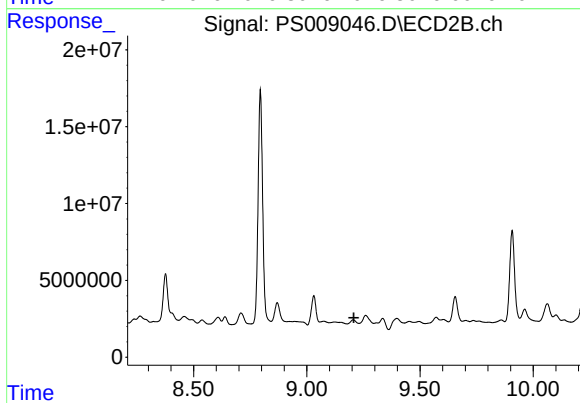

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.208 min
Response: 0
Conc: N.D.

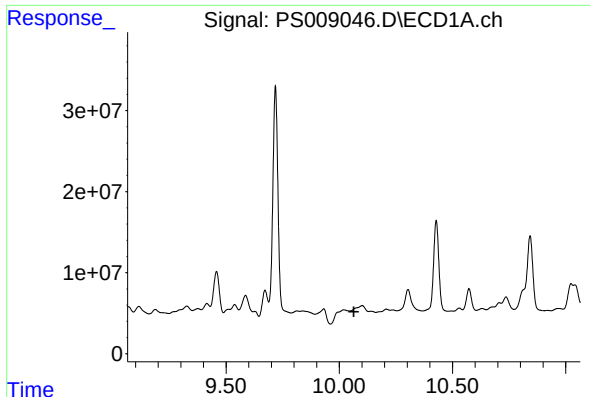

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

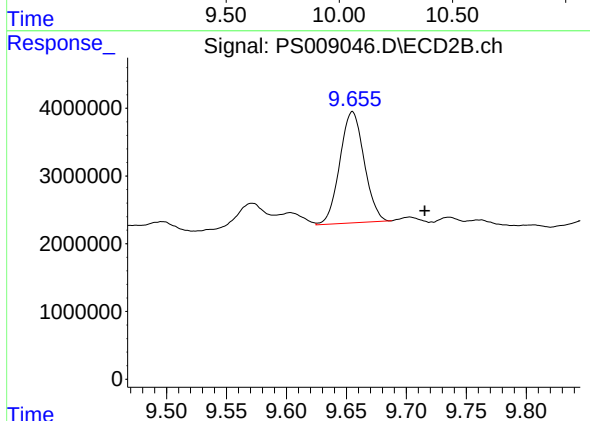


#13 2,4-DB

R.T.: 9.655 min
Delta R.T.: -0.060 min
Response: 23189070
Conc: 33.01 ng/ml

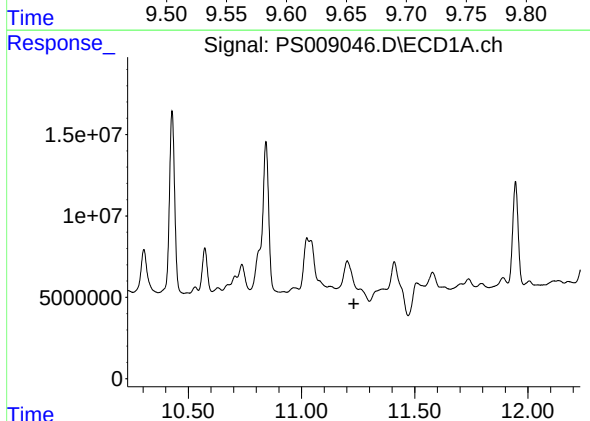


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

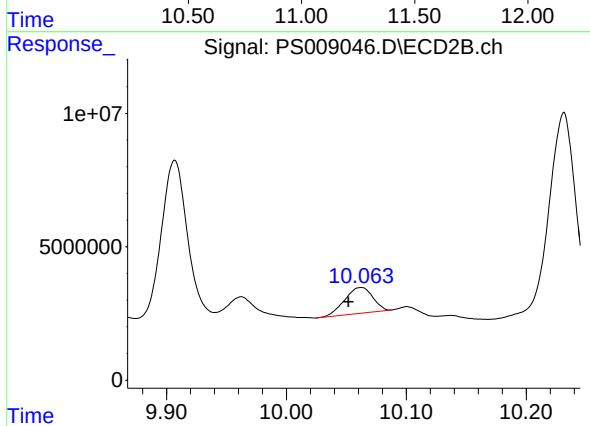

#14 DINOSEB


R.T.: 10.062 min
Delta R.T.: 0.010 min
Response: 15665071
Conc: 3.96 ng/ml

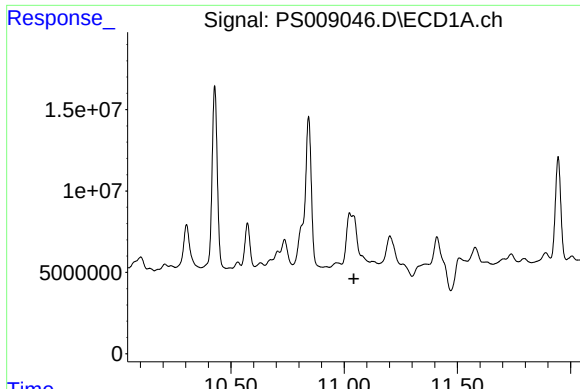

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 11.043 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

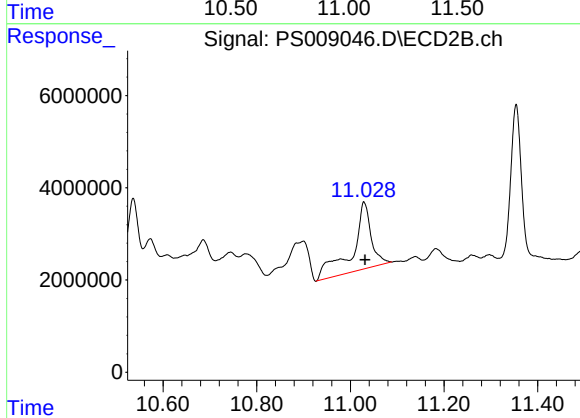


#15 Picloram

R.T.: 11.029 min
Delta R.T.: -0.002 min
Response: 40787829
Conc: 5.61 ng/ml

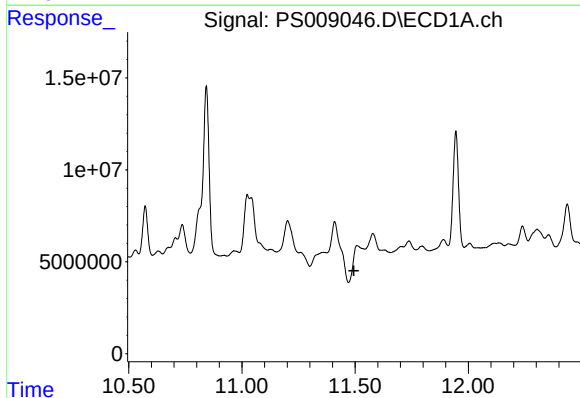

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.

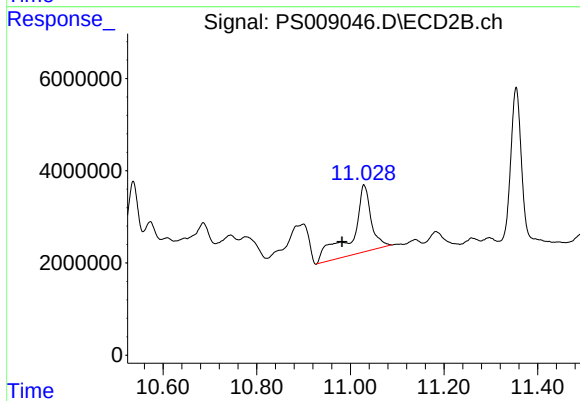

#16 DCPA

R.T.: 11.029 min
Delta R.T.: 0.047 min
Response: 40787829
Conc: 5.89 ng/ml