

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
 Data File : PS009048.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2020 13:49
 Operator : DD\AJ
 Sample : L1696-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 29 00:11:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.248	6.939	812.2E6	337.6E6	371.452	350.319
Target Compounds							
2) T	3,5-DICHL...	0.000	6.114	0	94465030	N.D.	64.734
5) T	DICAMBA	7.372	7.074	142.6E6	26271579	17.554	6.347 #
7) T	MCPA	7.800	7.432	75500995	27441612	9.386	6.203 #
8) T	DICHLORPROP	8.150	7.741	74392285	39259320	38.297	39.184
9) T	2,4-D	0.000	8.014	0	17007782	N.D.	14.355
11) T	2,4,5-TP ...	0.000	8.794	0	154.6E6	N.D.	28.546
12) T	2,4,5-T	9.457	9.197	190.5E6	16949252	17.819	3.131 #
13) T	2,4-DB	0.000	9.733	0	38715363	N.D.	55.116
14) T	DINOSEB	0.000	10.064	0	56853207	N.D.	14.378
15) T	Picloram	11.022	11.030	136.7E6	42275963	9.987	5.818 #
16) T	DCPA	0.000	11.030	0	42275963	N.D.	6.110



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
Data File : PS009048.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2020 13:49
Operator : DD\AJ
Sample : L1696-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 29 00:11:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

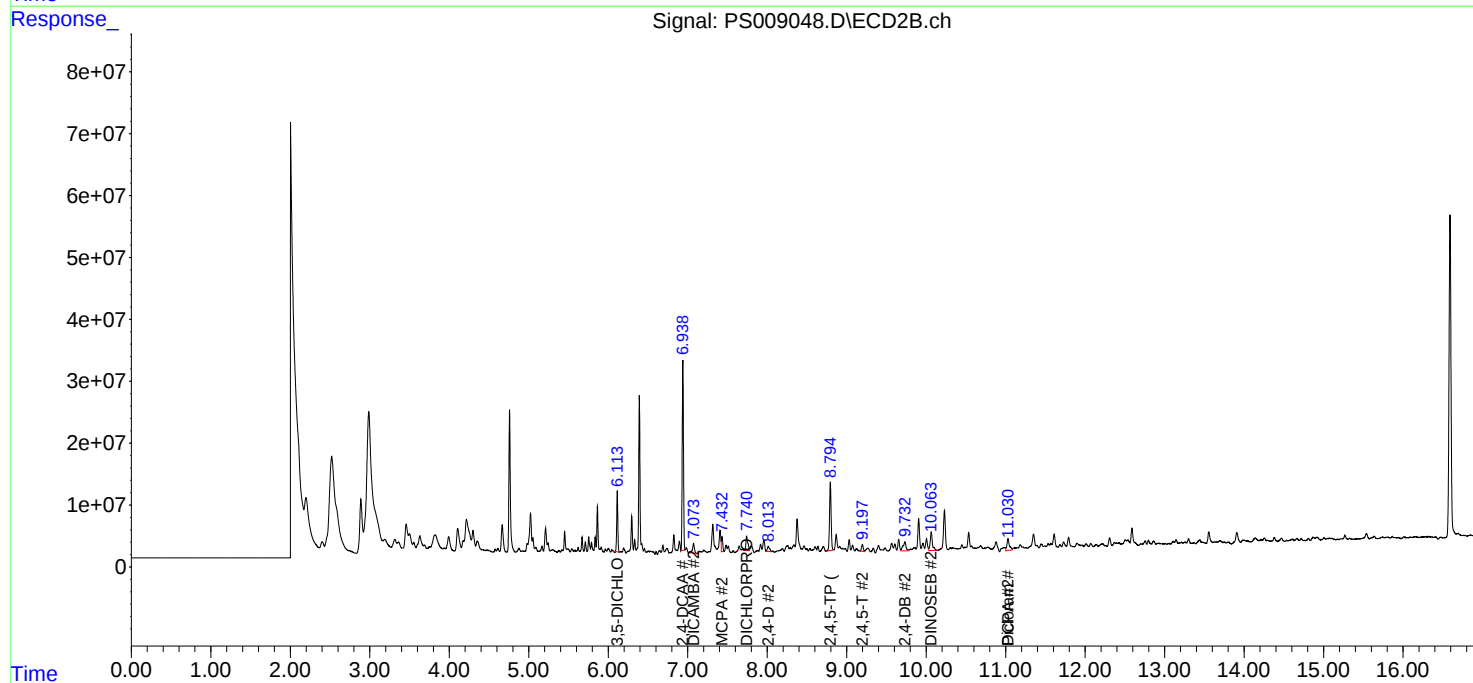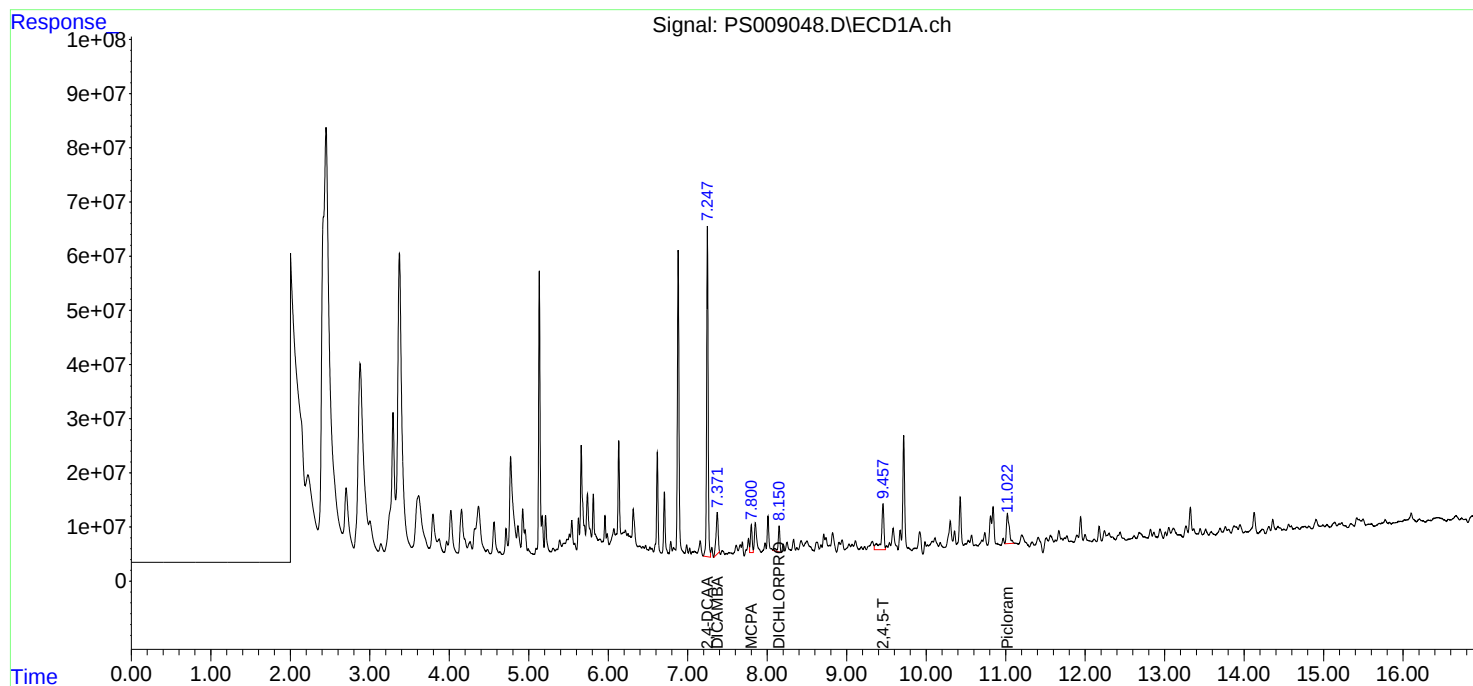


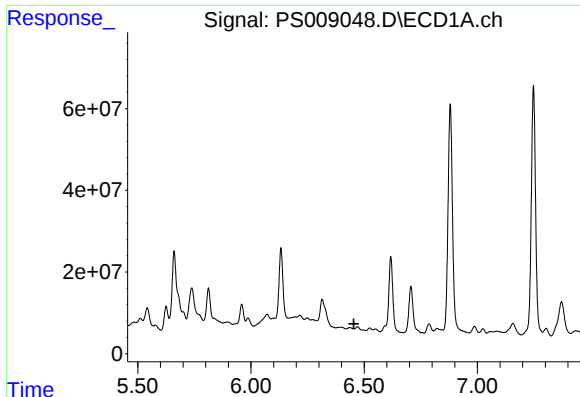

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

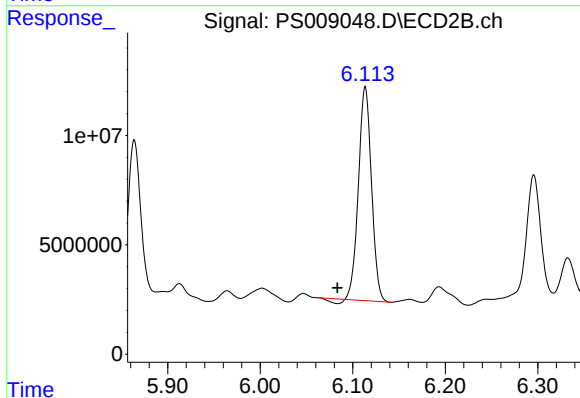


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.114 min
Delta R.T.: 0.030 min
Response: 94465030
Conc: 64.73 ng/ml

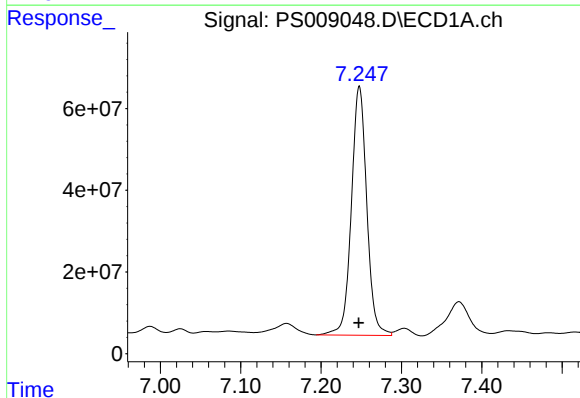


#4 2,4-DCAA

R.T.: 7.248 min
Delta R.T.: 0.000 min
Response: 812215027
Conc: 371.45 ng/ml

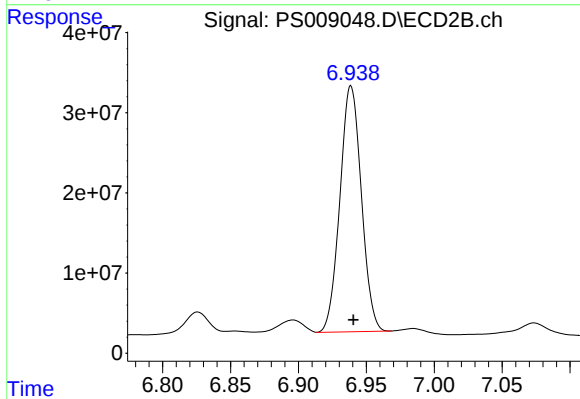

#4 2,4-DCAA


R.T.: 6.939 min
Delta R.T.: -0.002 min
Response: 337551759
Conc: 350.32 ng/ml

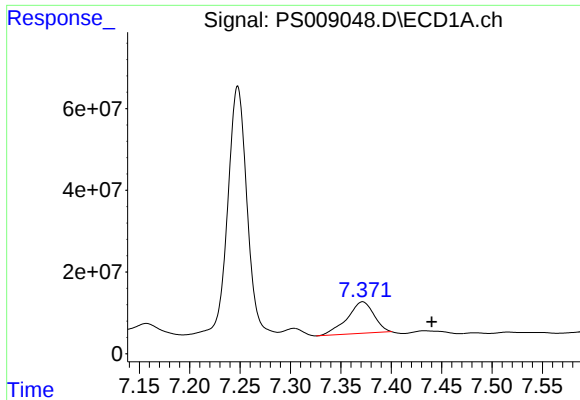

#5 DICAMBA


R.T.: 7.372 min
Delta R.T.: -0.069 min
Response: 142603585
Conc: 17.55 ng/ml

Instrument :
ECD_S
ClientSampleId :

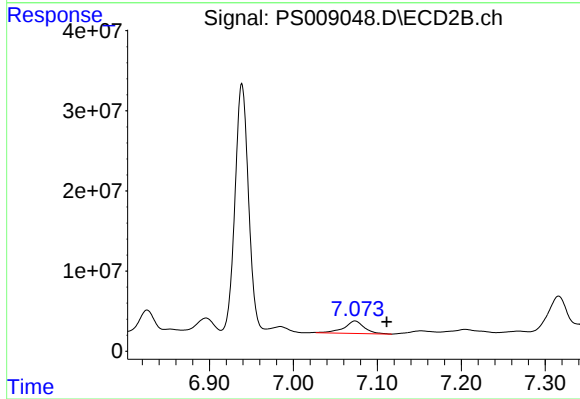


#5 DICAMBA

R.T.: 7.074 min
Delta R.T.: -0.038 min
Response: 26271579
Conc: 6.35 ng/ml

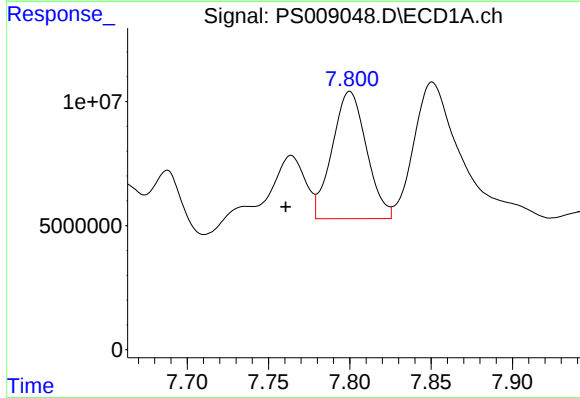


#7 MCPA

R.T.: 7.800 min
Delta R.T.: 0.039 min
Response: 75500995
Conc: 9.39 ug/ml

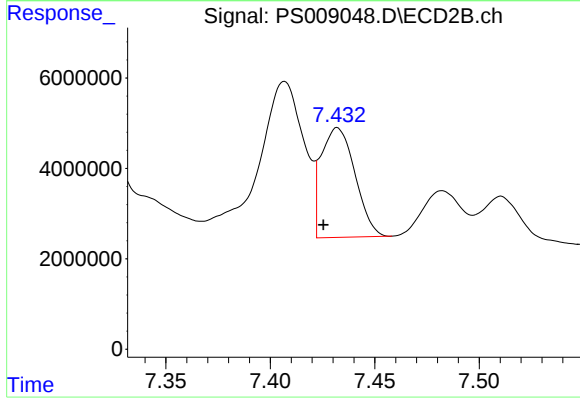

#7 MCPA


R.T.: 7.432 min
Delta R.T.: 0.007 min
Response: 27441612
Conc: 6.20 ug/ml

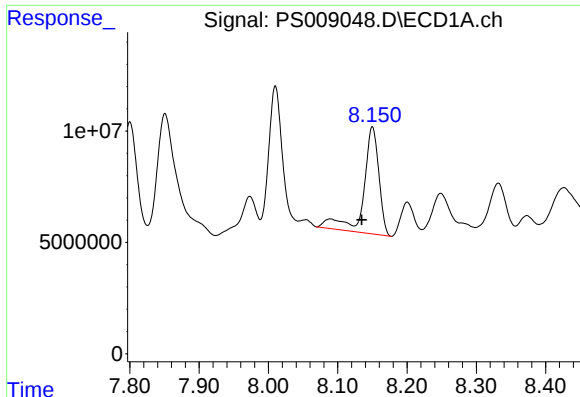

#8 DICHLORPROP


R.T.: 8.150 min
Delta R.T.: 0.015 min
Response: 74392285
Conc: 38.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

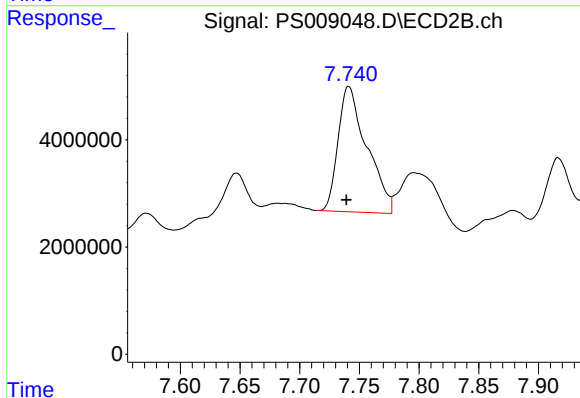


#8 DICHLORPROP

R.T.: 7.741 min
Delta R.T.: 0.002 min
Response: 39259320
Conc: 39.18 ng/ml

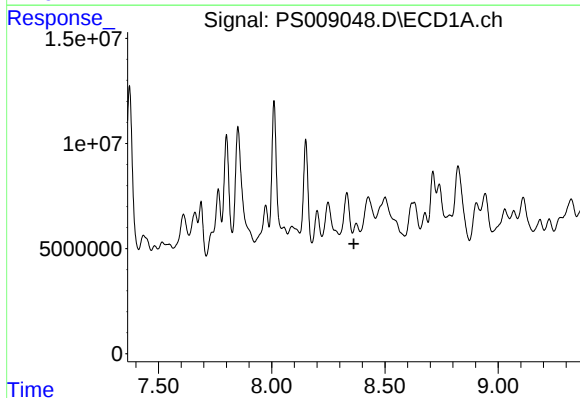


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.363 min
Response: 0
Conc: N.D.

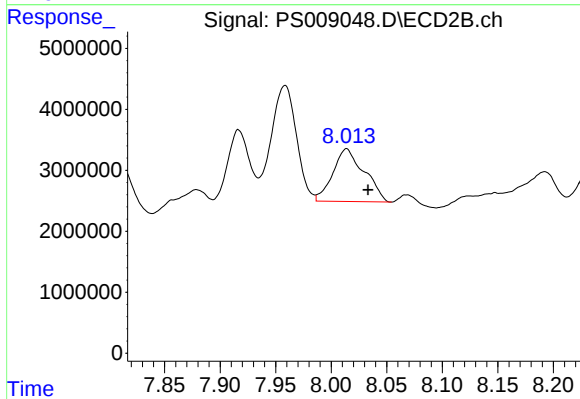

#9 2,4-D


R.T.: 8.014 min
Delta R.T.: -0.019 min
Response: 17007782
Conc: 14.35 ng/ml

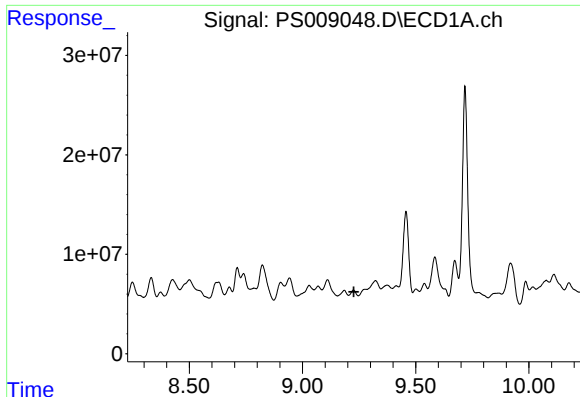

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

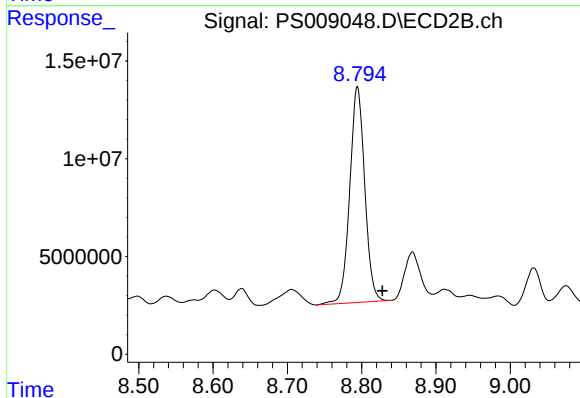


#11 2,4,5-TP (SILVEX)

R.T.: 8.794 min
Delta R.T.: -0.034 min
Response: 154628803
Conc: 28.55 ng/ml

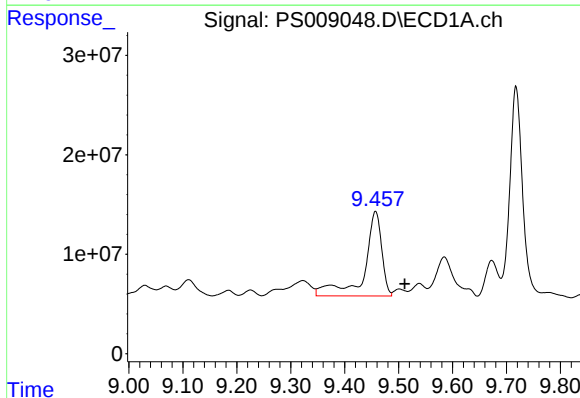


#12 2,4,5-T

R.T.: 9.457 min
Delta R.T.: -0.054 min
Response: 190520714
Conc: 17.82 ng/ml

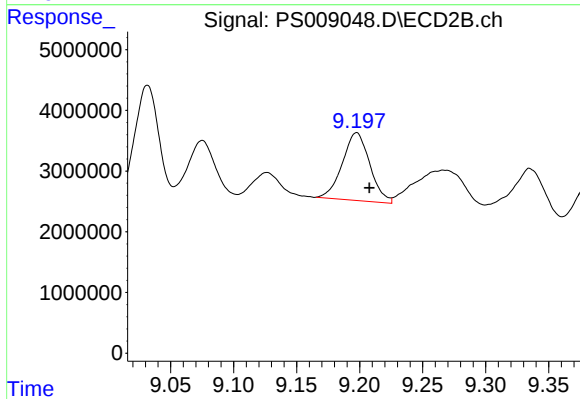

#12 2,4,5-T


R.T.: 9.197 min
Delta R.T.: -0.010 min
Response: 16949252
Conc: 3.13 ng/ml

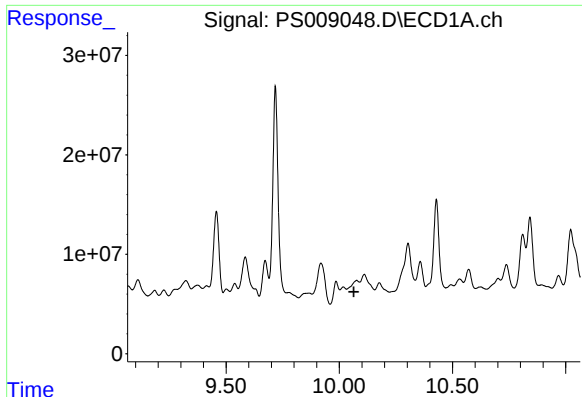

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

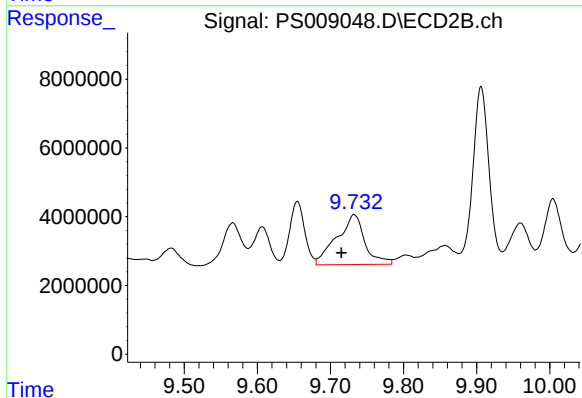


#13 2,4-DB

R.T.: 9.733 min
Delta R.T.: 0.017 min
Response: 38715363
Conc: 55.12 ng/ml

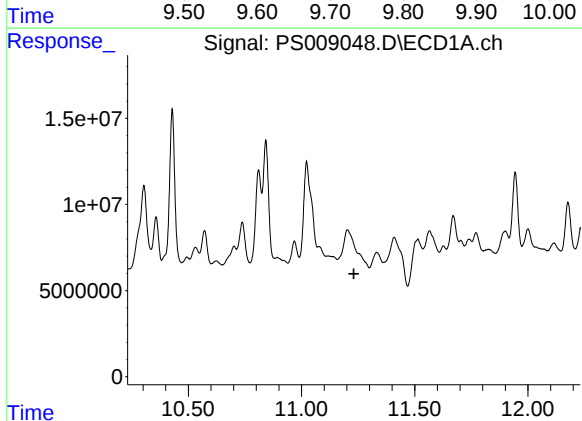


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

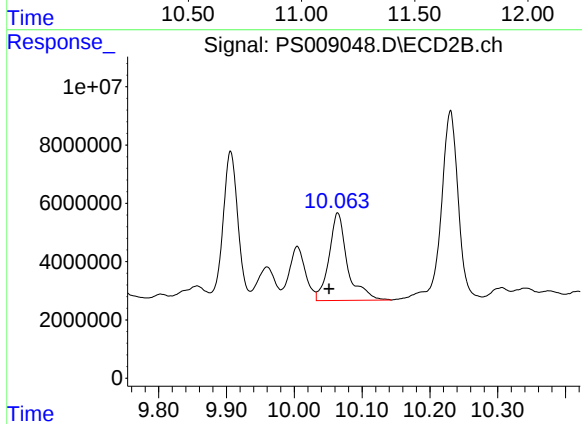

#14 DINOSEB


R.T.: 10.064 min
Delta R.T.: 0.013 min
Response: 56853207
Conc: 14.38 ng/ml

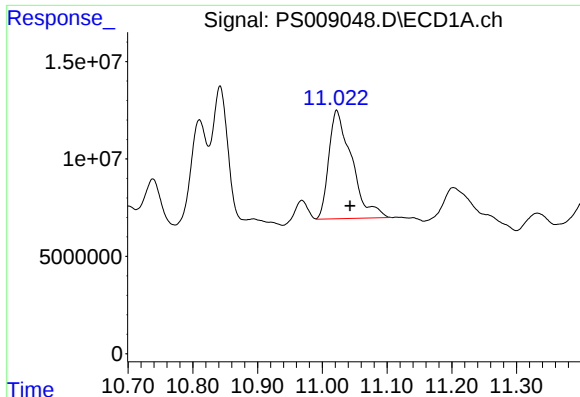

#15 Picloram


R.T.: 11.022 min
Delta R.T.: -0.021 min
Response: 136735544
Conc: 9.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

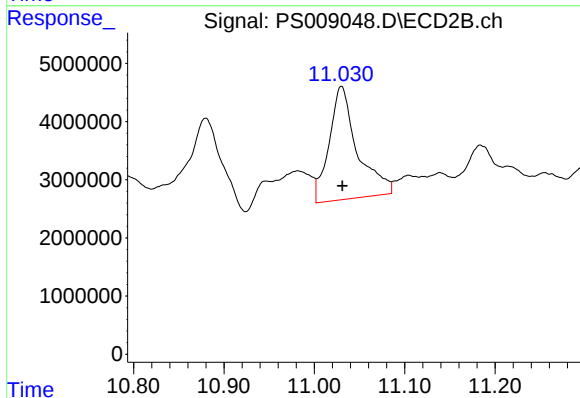


#15 Picloram

R.T.: 11.030 min
Delta R.T.: -0.001 min
Response: 42275963
Conc: 5.82 ng/ml

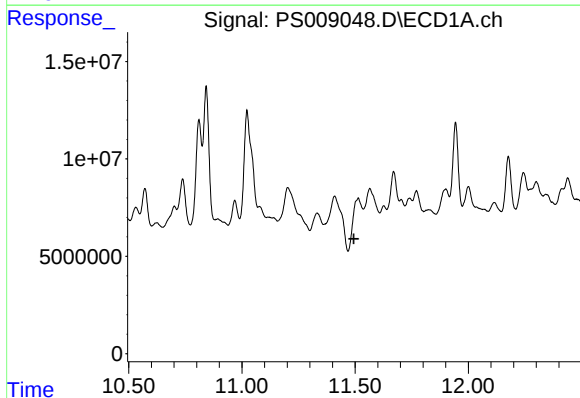

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.

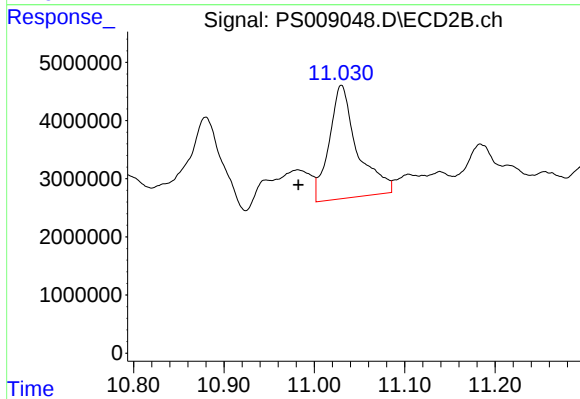

#16 DCPA

R.T.: 11.030 min
Delta R.T.: 0.048 min
Response: 42275963
Conc: 6.11 ng/ml