

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
 Data File : PS009049.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2020 14:12
 Operator : DD\AJ
 Sample : L1697-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 29 00:11:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.248	6.939	877.0E6	389.1E6	401.059	403.854
Target Compounds							
2) T	3,5-DICHL...	0.000	6.114	0	107.6E6	N.D.	73.717
5) T	DICAMBA	7.374	7.074	145.8E6	27719403	17.948	6.697 #
7) T	MCPA	7.800	7.432	74237842	33303250	9.229	7.527
8) T	DICHLORPROP	0.000	7.742	0	37479780	N.D.	37.408
11) T	2,4,5-TP ...	0.000	8.794	0	109.9E6	N.D.	20.282
12) T	2,4,5-T	9.456	9.197	195.2E6	19860586	18.259	3.669 #
13) T	2,4-DB	0.000	9.733	0	55431486	N.D.	78.913
14) T	DINOSEB	0.000	10.064	0	59456993	N.D.	15.037
15) T	Picloram	11.022	11.030	139.6E6	53155331	10.193	7.315 #
16) T	DCPA	0.000	11.030	0	53155331	N.D.	7.682



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
Data File : PS009049.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2020 14:12
Operator : DD\AJ
Sample : L1697-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 29 00:11:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

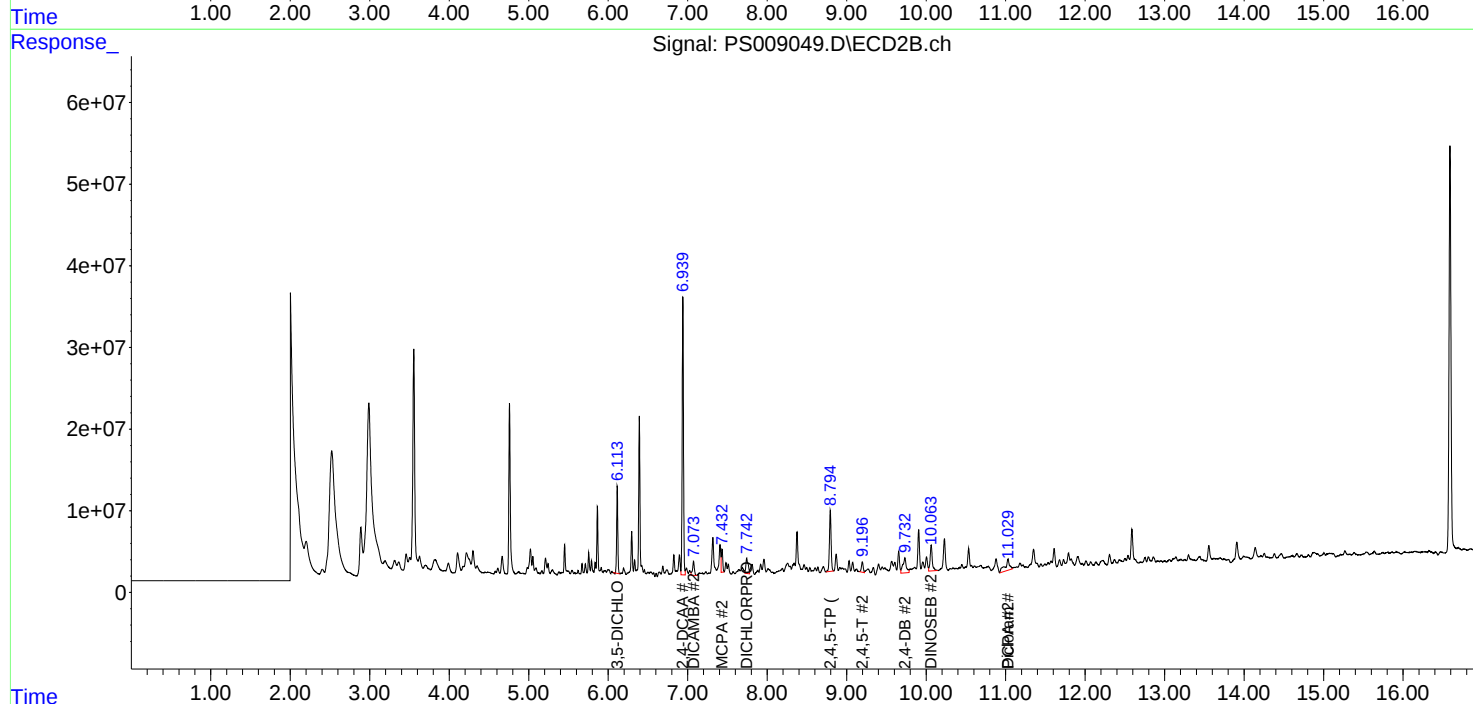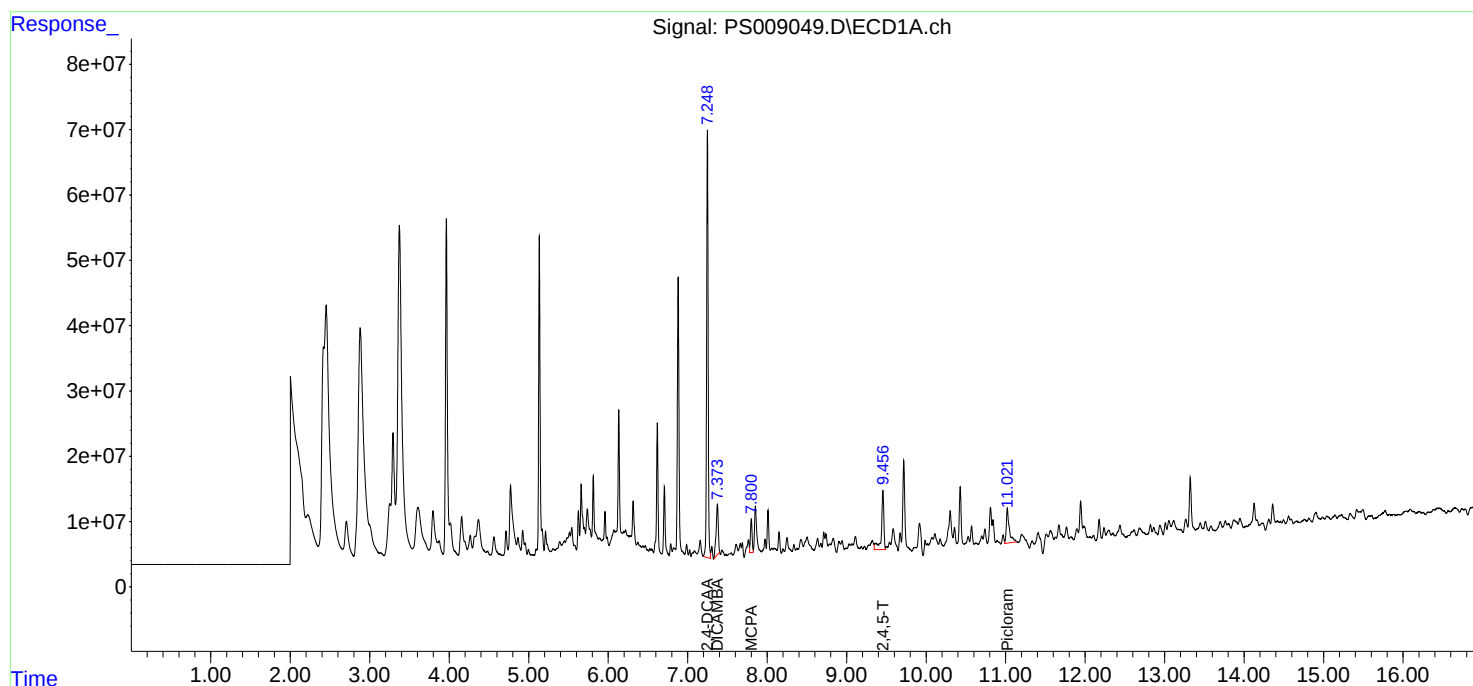


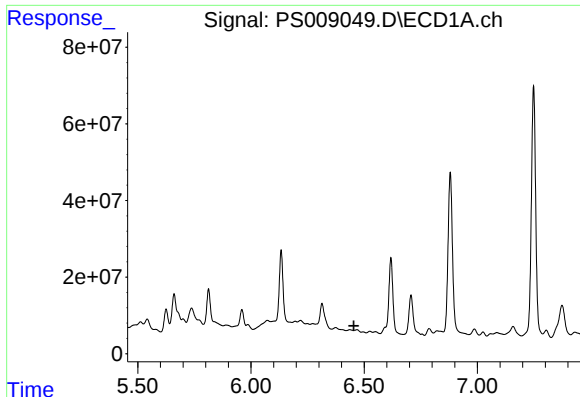

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

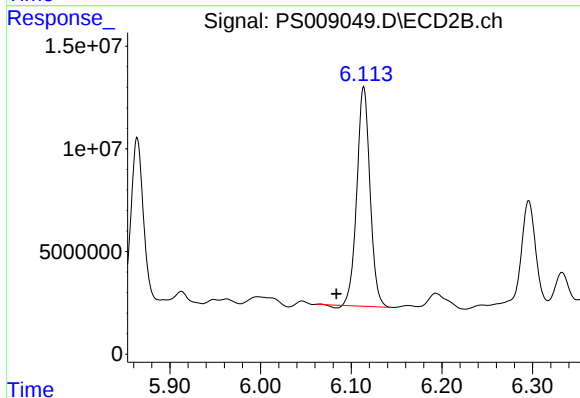


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.114 min
Delta R.T.: 0.030 min
Response: 107572524
Conc: 73.72 ng/ml

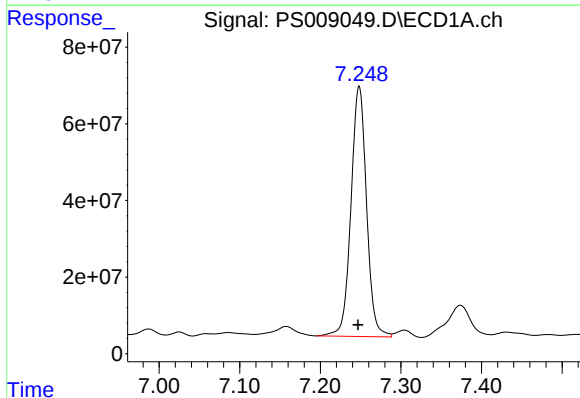


#4 2,4-DCAA

R.T.: 7.248 min
Delta R.T.: 0.001 min
Response: 876952726
Conc: 401.06 ng/ml

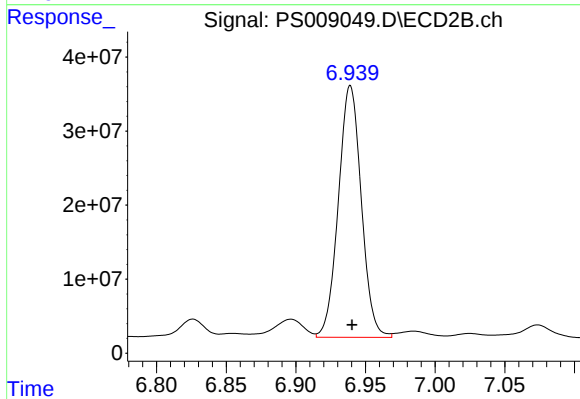

#4 2,4-DCAA


R.T.: 6.939 min
Delta R.T.: -0.001 min
Response: 389136091
Conc: 403.85 ng/ml

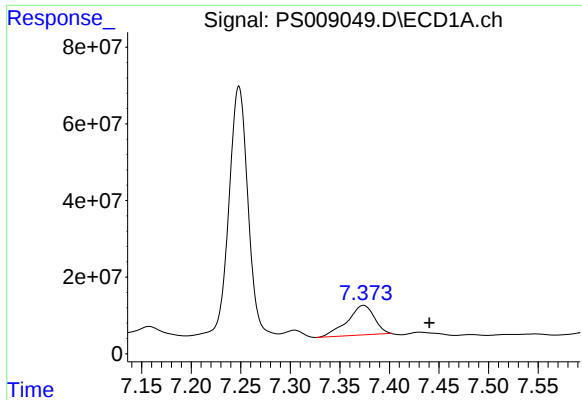

#5 DICAMBA


R.T.: 7.374 min
Delta R.T.: -0.067 min
Response: 145804921
Conc: 17.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

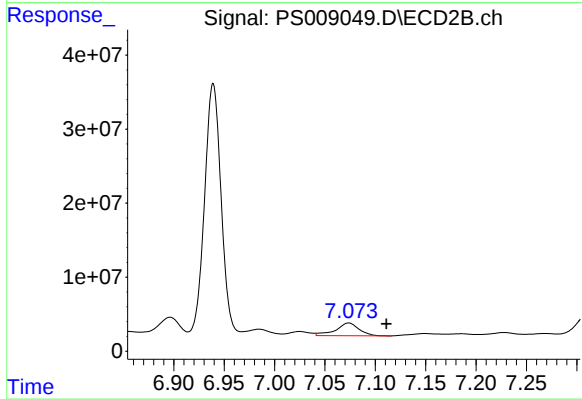


#5 DICAMBA

R.T.: 7.074 min
Delta R.T.: -0.038 min
Response: 27719403
Conc: 6.70 ng/ml

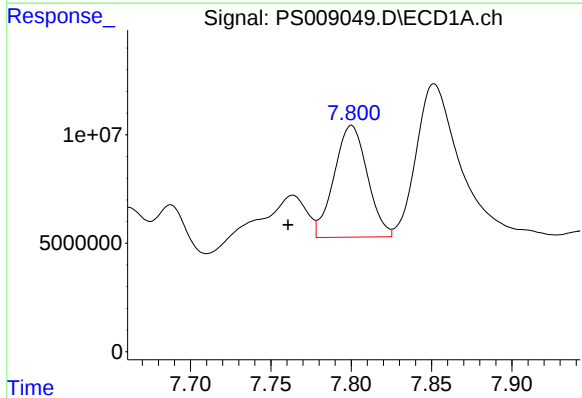


#7 MCPA

R.T.: 7.800 min
Delta R.T.: 0.039 min
Response: 74237842
Conc: 9.23 ug/ml

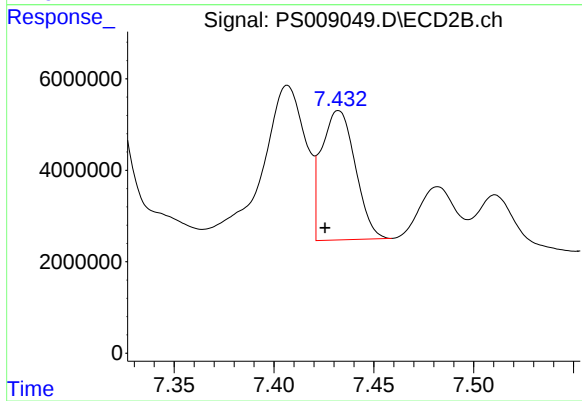

#7 MCPA


R.T.: 7.432 min
Delta R.T.: 0.007 min
Response: 33303250
Conc: 7.53 ug/ml

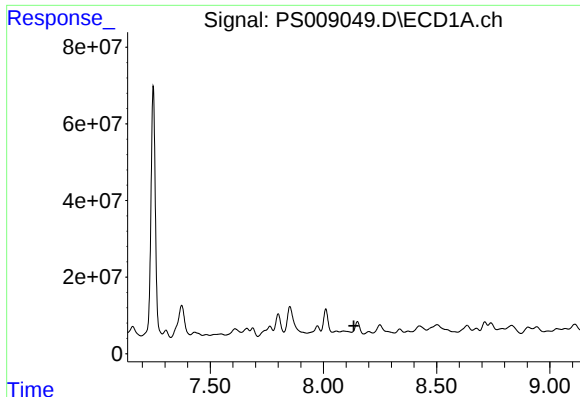

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

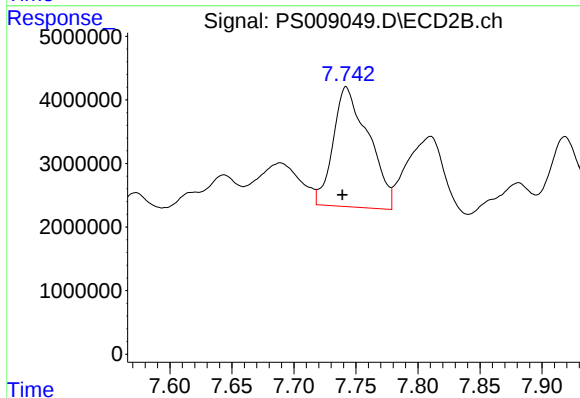


#8 DICHLORPROP

R.T.: 7.742 min
Delta R.T.: 0.003 min
Response: 37479780
Conc: 37.41 ng/ml

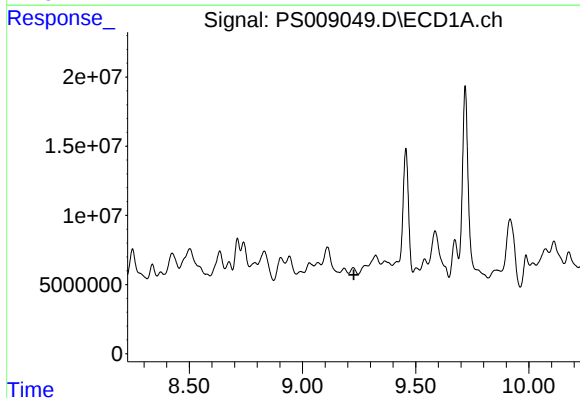


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

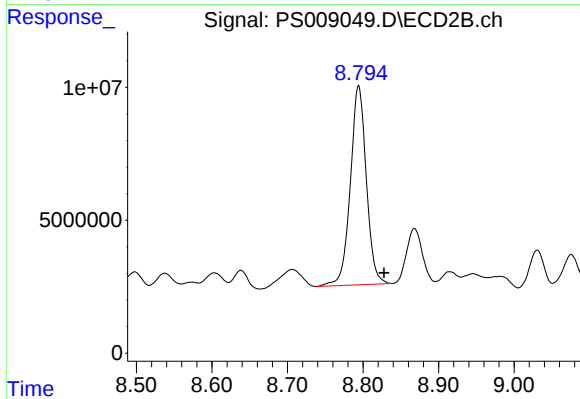

#11 2,4,5-TP (SILVEX)


R.T.: 8.794 min
Delta R.T.: -0.034 min
Response: 109863499
Conc: 20.28 ng/ml

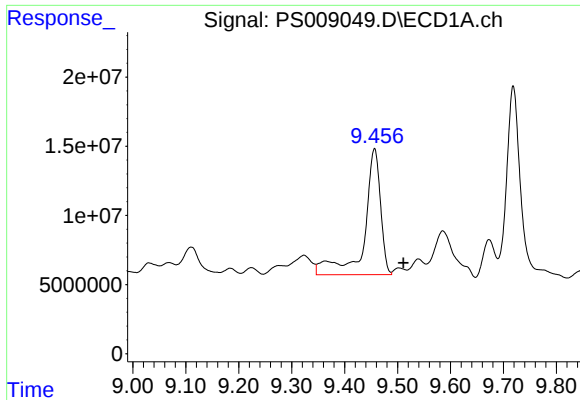

#12 2,4,5-T


R.T.: 9.456 min
Delta R.T.: -0.055 min
Response: 195230854
Conc: 18.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

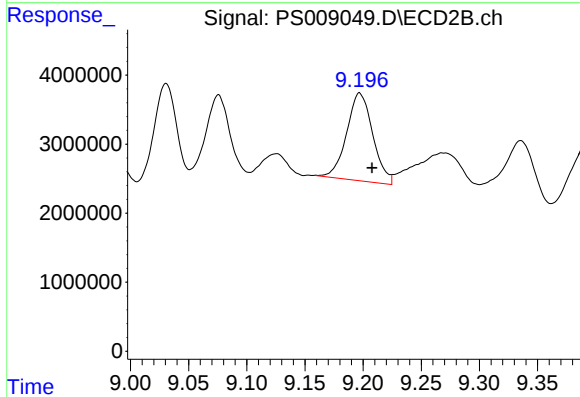


#12 2,4,5-T

R.T.: 9.197 min
Delta R.T.: -0.011 min
Response: 19860586
Conc: 3.67 ng/ml

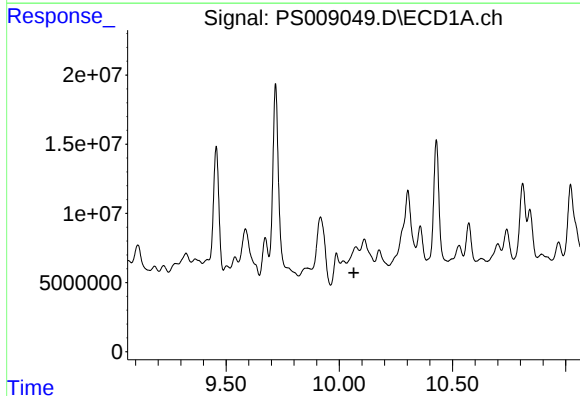


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.064 min
Response: 0
Conc: N.D.

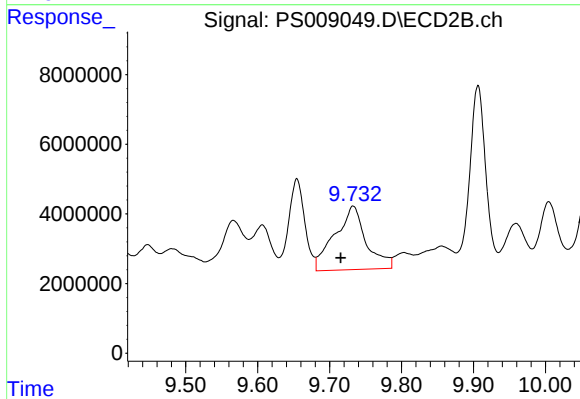

#13 2,4-DB


R.T.: 9.733 min
Delta R.T.: 0.018 min
Response: 55431486
Conc: 78.91 ng/ml

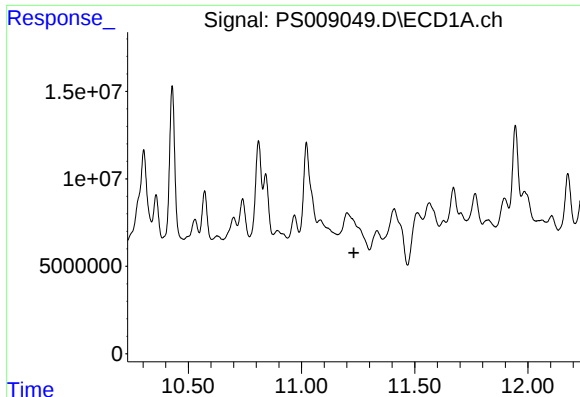

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

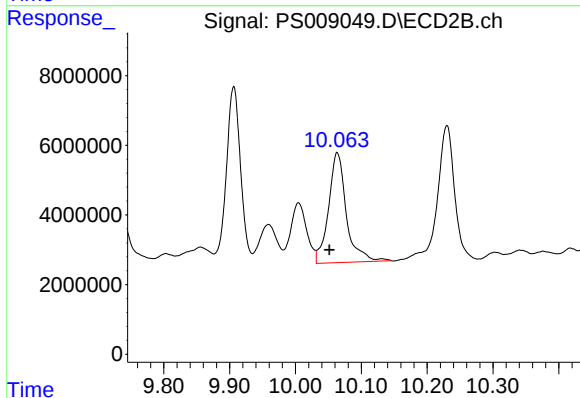


#14 DINOSEB

R.T.: 10.064 min
Delta R.T.: 0.012 min
Response: 59456993
Conc: 15.04 ng/ml

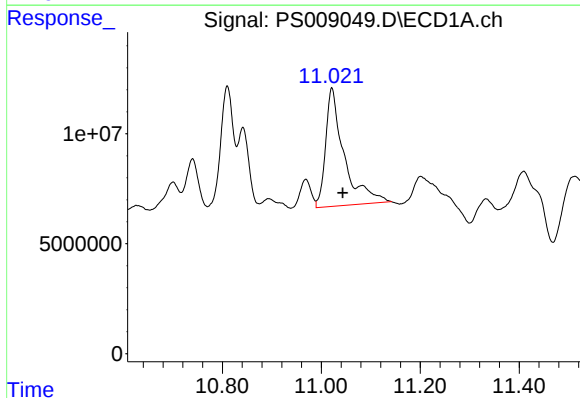


#15 Picloram

R.T.: 11.022 min
Delta R.T.: -0.022 min
Response: 139550238
Conc: 10.19 ng/ml

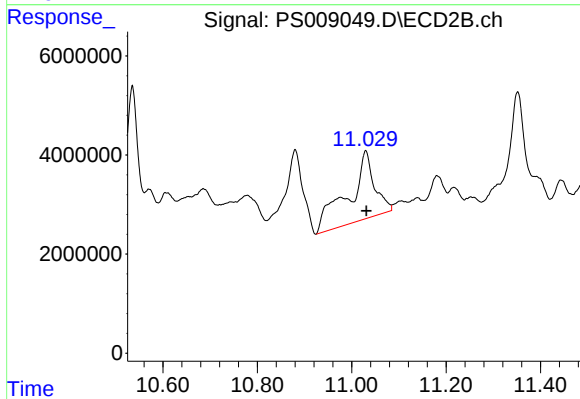

#15 Picloram


R.T.: 11.030 min
Delta R.T.: -0.001 min
Response: 53155331
Conc: 7.32 ng/ml

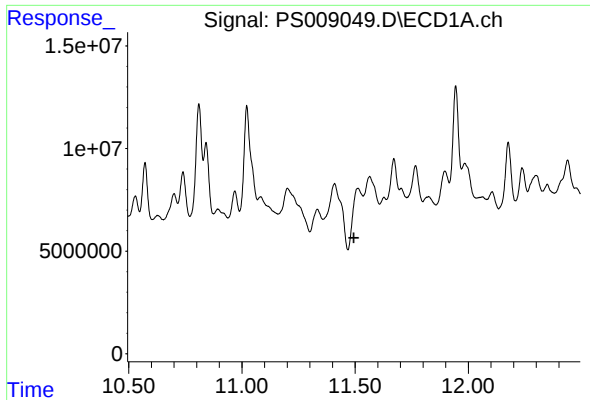

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

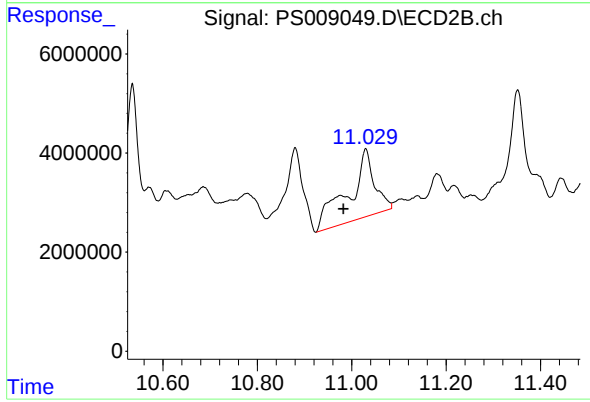

#16 DCPA

R.T.: 11.030 min
Delta R.T.: 0.047 min
Response: 53155331
Conc: 7.68 ng/ml