

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
 Data File : PS009050.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2020 14:35
 Operator : DD\AJ
 Sample : L1697-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 29 00:11:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.248	6.940	1037.4E6	466.1E6	474.436	483.734
Target Compounds							
2) T	3,5-DICHL...	0.000	6.114	0	119.6E6	N.D.	81.977
5) T	DICAMBA	7.373	7.074	147.9E6	29138518	18.201	7.039 #
7) T	MCPA	7.800	7.432	71796136	35100770	8.925	7.934
8) T	DICHLORPROP	0.000	7.743	0	31585390	N.D.	31.524
10) T	Pentachlo...	0.000	8.466	0	21084567	N.D.	1.484
11) T	2,4,5-TP ...	0.000	8.795	0	147.9E6	N.D.	27.296
12) T	2,4,5-T	9.457	9.198	163.0E6	18480537	15.248	3.414 #
13) T	2,4-DB	0.000	9.733	0	33118302	N.D.	47.148
14) T	DINOSEB	0.000	10.064	0	52283723	N.D.	13.223
15) T	Picloram	11.022	11.030	170.6E6	41941437	12.464	5.772 #
16) T	DCPA	0.000	11.030	0	41941437	N.D.	6.061



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
Data File : PS009050.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2020 14:35
Operator : DD\AJ
Sample : L1697-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 29 00:11:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

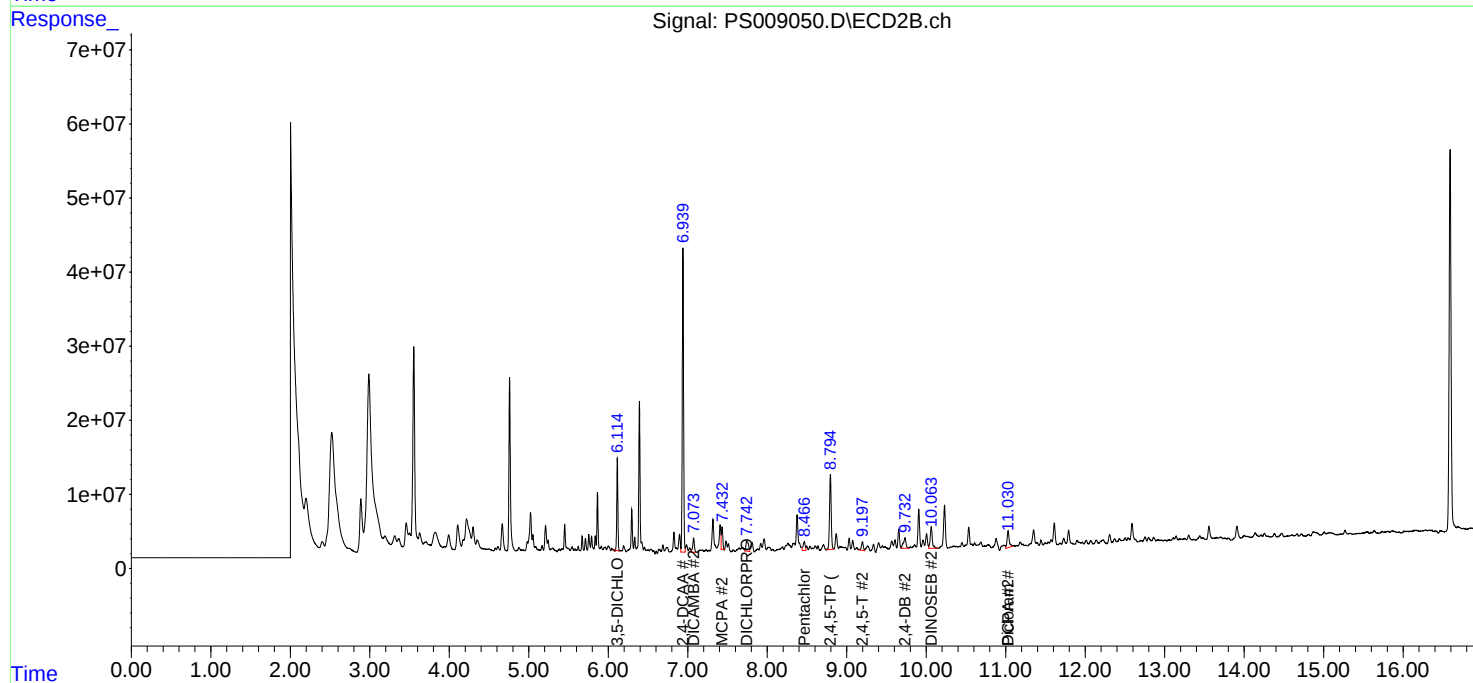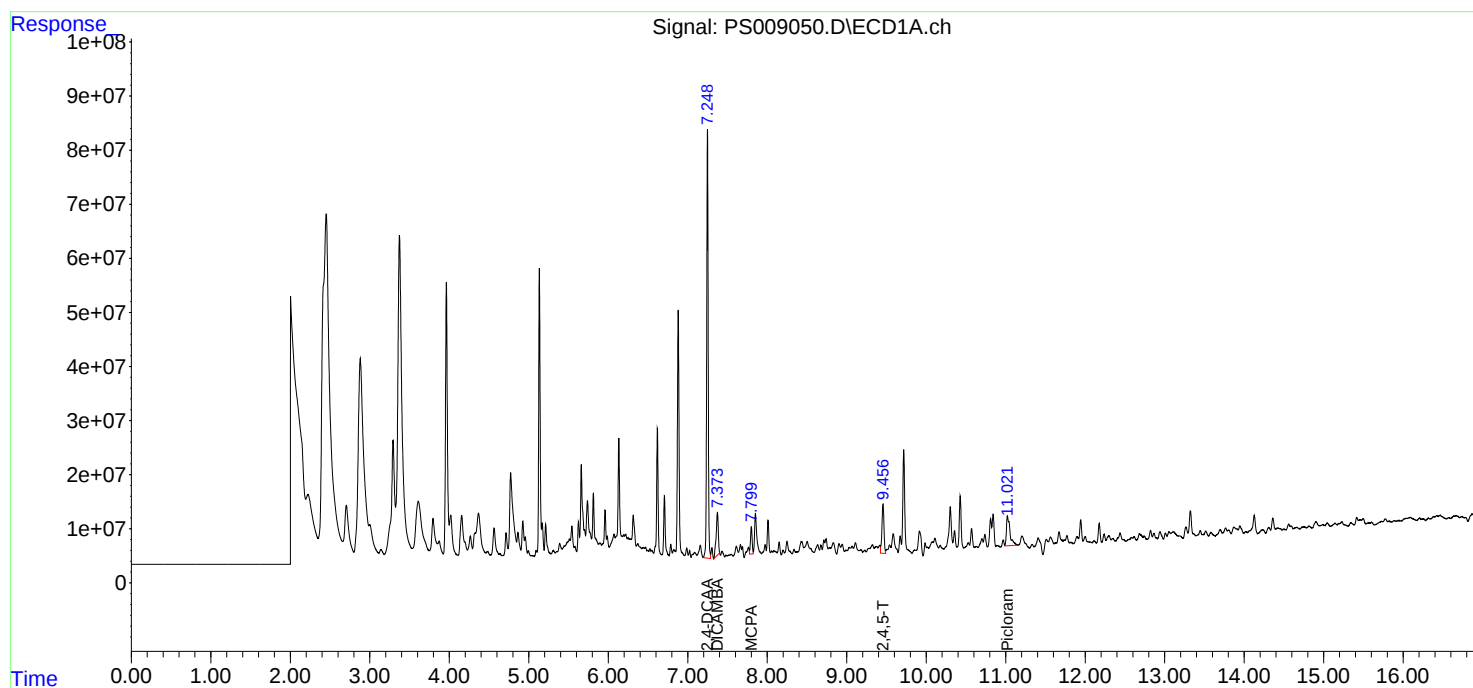


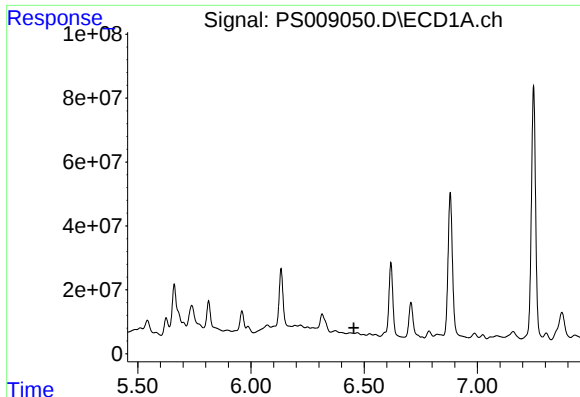

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

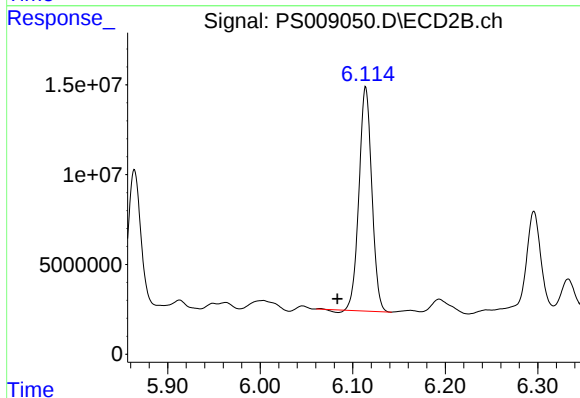


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.114 min
Delta R.T.: 0.031 min
Response: 119627173
Conc: 81.98 ng/ml

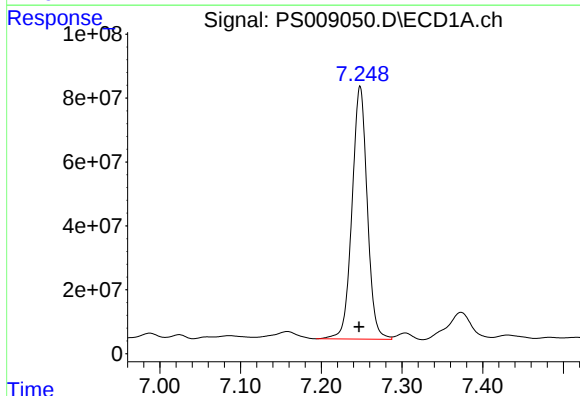


#4 2,4-DCAA

R.T.: 7.248 min
Delta R.T.: 0.001 min
Response: 1037397565
Conc: 474.44 ng/ml

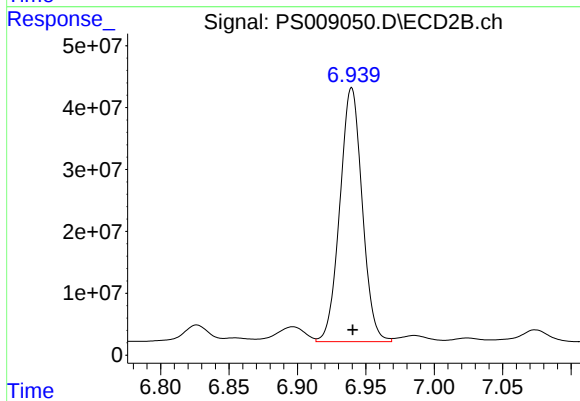

#4 2,4-DCAA


R.T.: 6.940 min
Delta R.T.: 0.000 min
Response: 466104058
Conc: 483.73 ng/ml

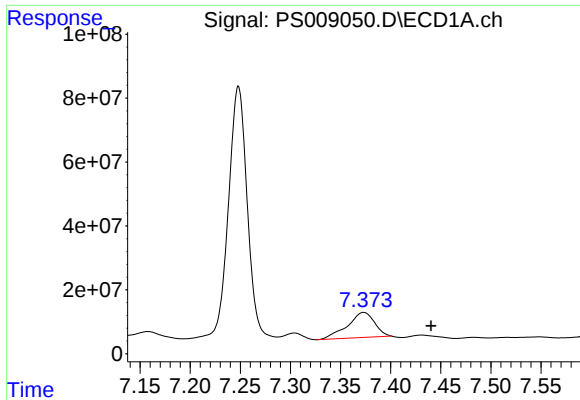

#5 DICAMBA


R.T.: 7.373 min
Delta R.T.: -0.067 min
Response: 147861213
Conc: 18.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

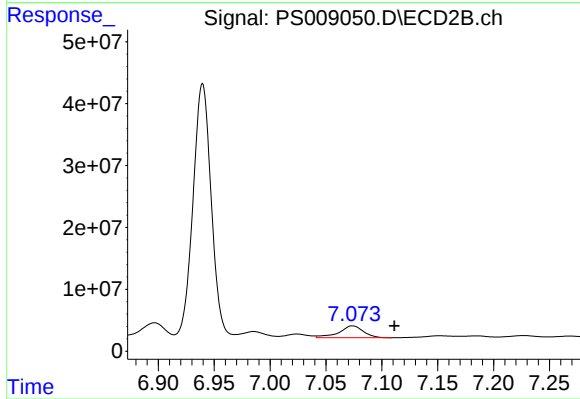


#5 DICAMBA

R.T.: 7.074 min
Delta R.T.: -0.037 min
Response: 29138518
Conc: 7.04 ng/ml

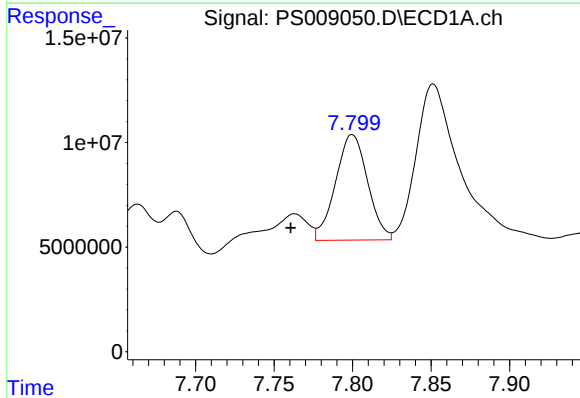


#7 MCPA

R.T.: 7.800 min
Delta R.T.: 0.039 min
Response: 71796136
Conc: 8.93 ug/ml

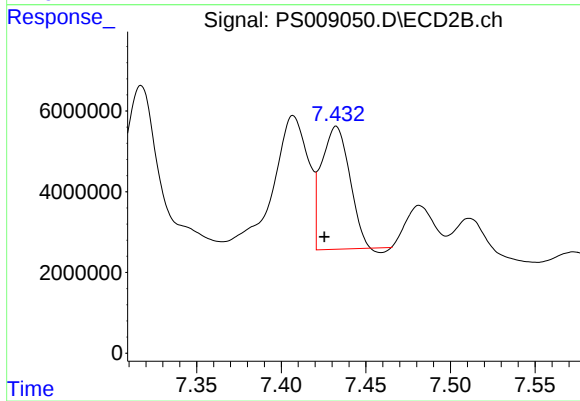

#7 MCPA


R.T.: 7.432 min
Delta R.T.: 0.007 min
Response: 35100770
Conc: 7.93 ug/ml

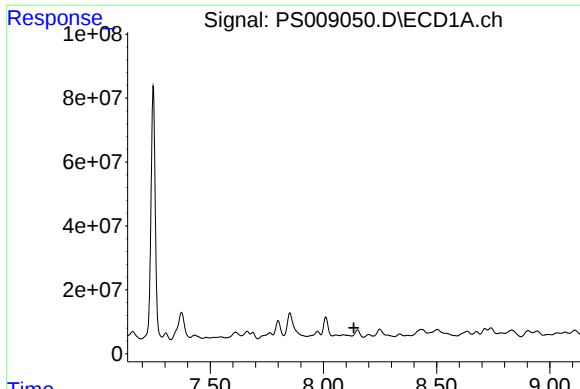

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

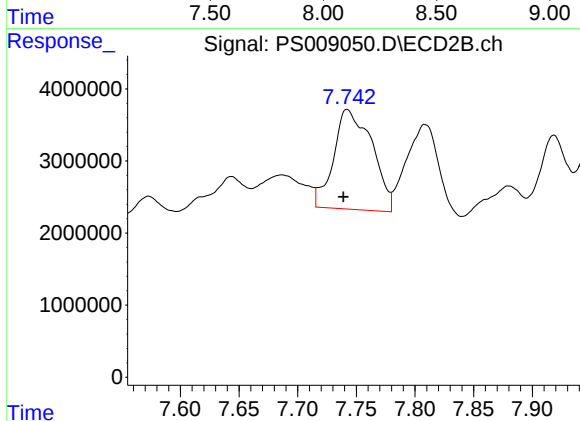


#8 DICHLORPROP

R.T.: 7.743 min
Delta R.T.: 0.003 min
Response: 31585390
Conc: 31.52 ng/ml

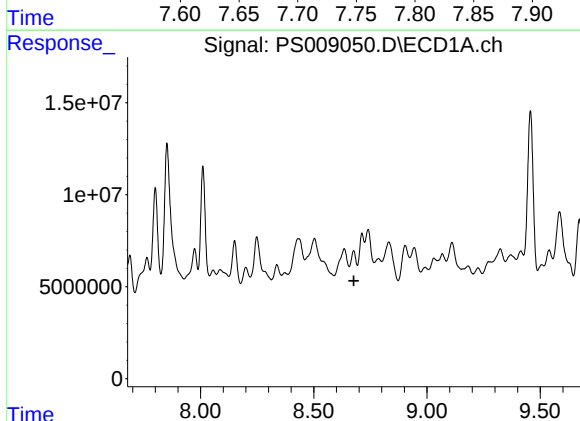


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 8.677 min
Response: 0
Conc: N.D.

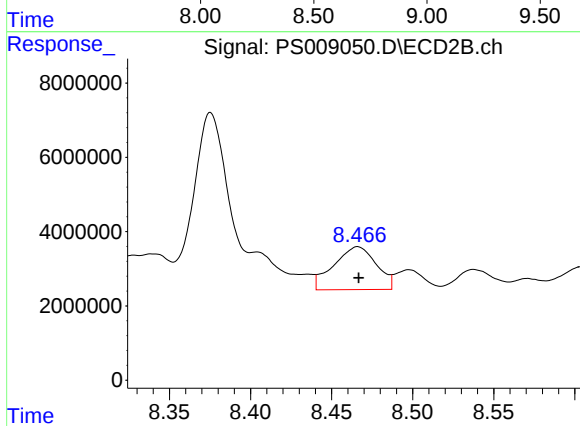

#10 Pentachlorophenol


R.T.: 8.466 min
Delta R.T.: 0.000 min
Response: 21084567
Conc: 1.48 ng/ml

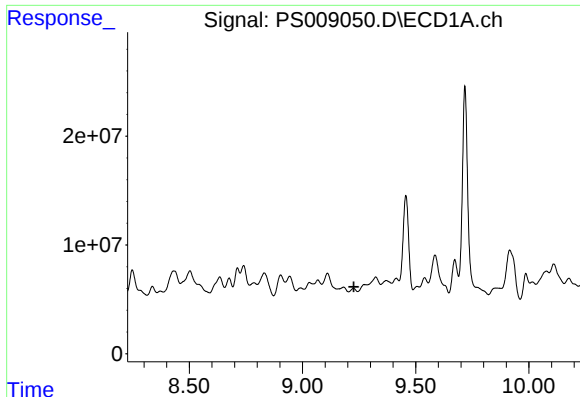

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

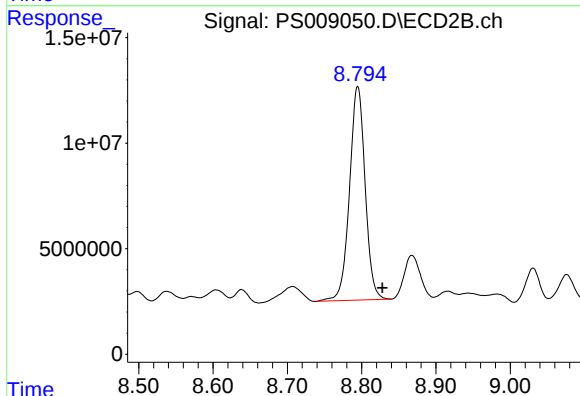


#11 2,4,5-TP (SILVEX)

R.T.: 8.795 min
Delta R.T.: -0.033 min
Response: 147860658
Conc: 27.30 ng/ml

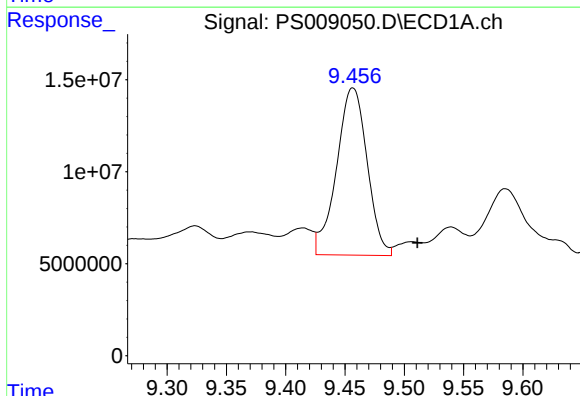


#12 2,4,5-T

R.T.: 9.457 min
Delta R.T.: -0.055 min
Response: 163032212
Conc: 15.25 ng/ml

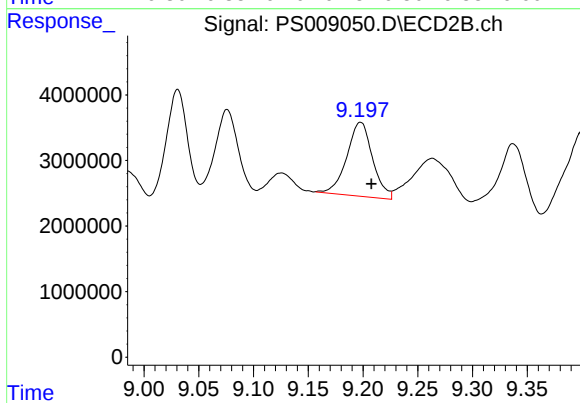

#12 2,4,5-T


R.T.: 9.198 min
Delta R.T.: -0.010 min
Response: 18480537
Conc: 3.41 ng/ml

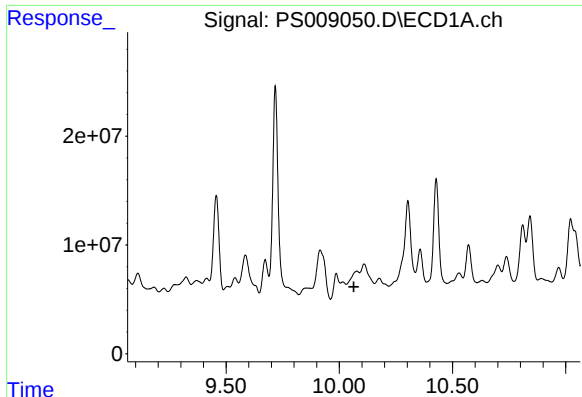

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

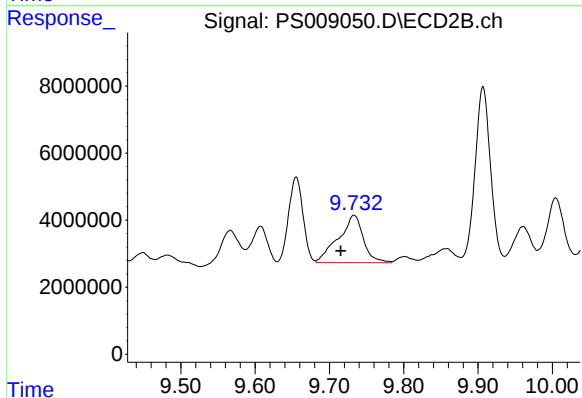


#13 2,4-DB

R.T.: 9.733 min
Delta R.T.: 0.018 min
Response: 33118302
Conc: 47.15 ng/ml

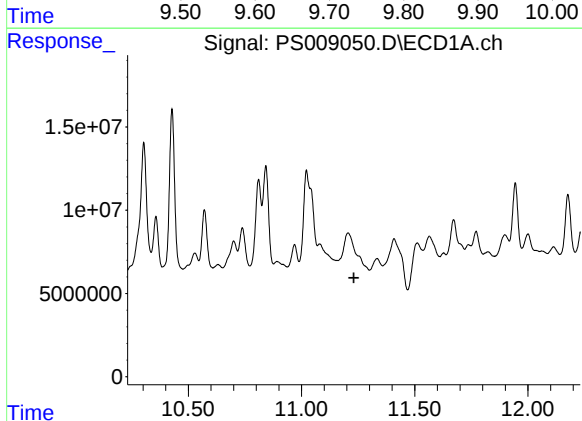


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

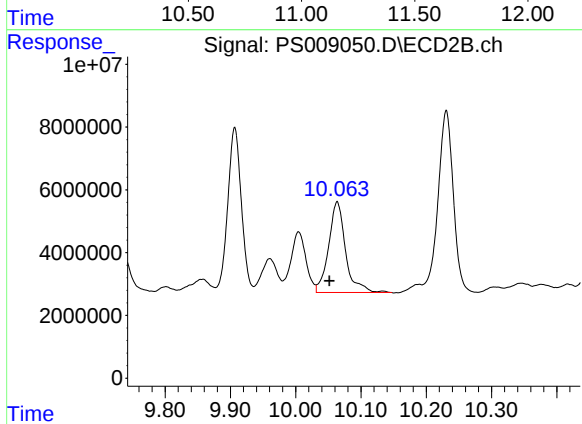

#14 DINOSEB


R.T.: 10.064 min
Delta R.T.: 0.012 min
Response: 52283723
Conc: 13.22 ng/ml

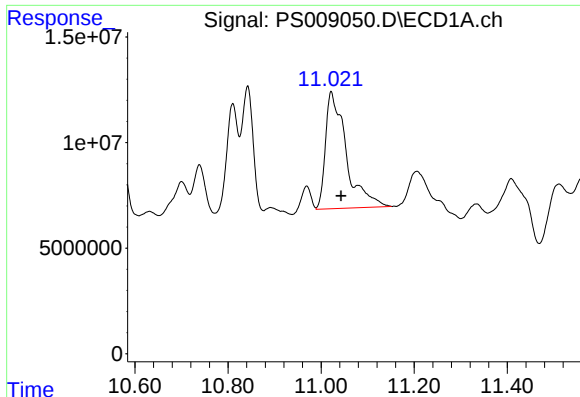

#15 Picloram


R.T.: 11.022 min
Delta R.T.: -0.021 min
Response: 170648303
Conc: 12.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

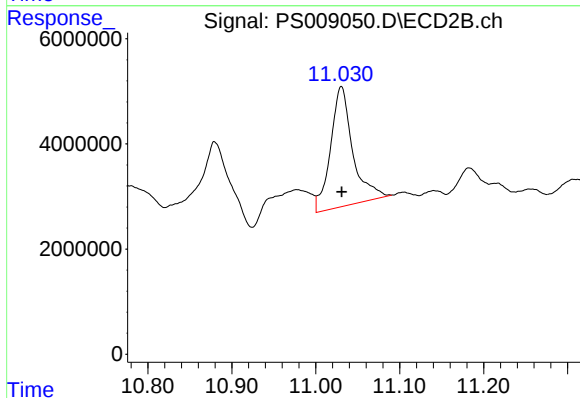


#15 Picloram

R.T.: 11.030 min
Delta R.T.: 0.000 min
Response: 41941437
Conc: 5.77 ng/ml

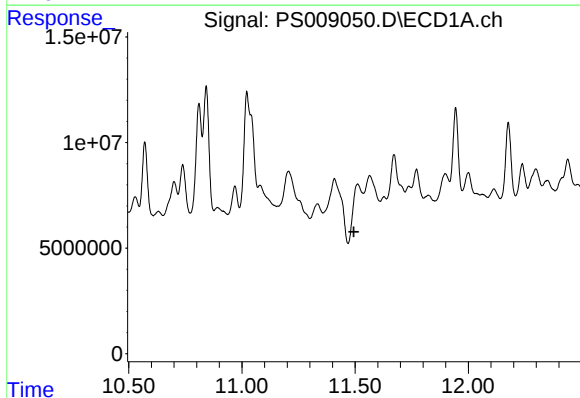

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.

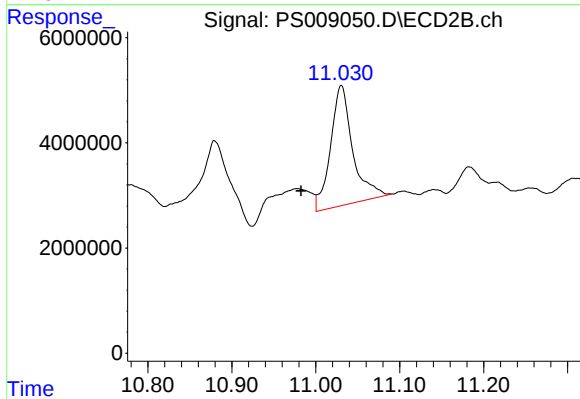

#16 DCPA

R.T.: 11.030 min
Delta R.T.: 0.048 min
Response: 41941437
Conc: 6.06 ng/ml