

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
 Data File : PS009051.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2020 14:57
 Operator : DD\AJ
 Sample : L1700-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 29 00:12:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.248	6.939	1310.2E6	590.3E6	599.200	612.659
Target Compounds							
2) T	3,5-DICHL...	0.000	6.114	0	108.5E6	N.D.	74.379
5) T	DICAMBA	0.000	7.073	0	24399917	N.D.	5.895
7) T	MCPA	7.800	7.405	71231701	69405418	8.855	15.688 #
8) T	DICHLORPROP	0.000	7.760	0	19050269	N.D.	19.014
10) T	Pentachlo...	0.000	8.463	0	19985873	N.D.	1.407
11) T	2,4,5-TP ...	0.000	8.794	0	177.9E6	N.D.	32.835
12) T	2,4,5-T	9.456	0.000	140.1E6	0	13.101	N.D. #
13) T	2,4-DB	0.000	9.654	0	27283654	N.D.	38.841
14) T	DINOSEB	0.000	10.063	0	43219490	N.D.	10.930
15) T	Picloram	11.022	11.030	153.6E6	54896077	11.222	7.555 #
16) T	DCPA	0.000	11.030	0	54896077	N.D.	7.934



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
Data File : PS009051.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2020 14:57
Operator : DD\AJ
Sample : L1700-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 29 00:12:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

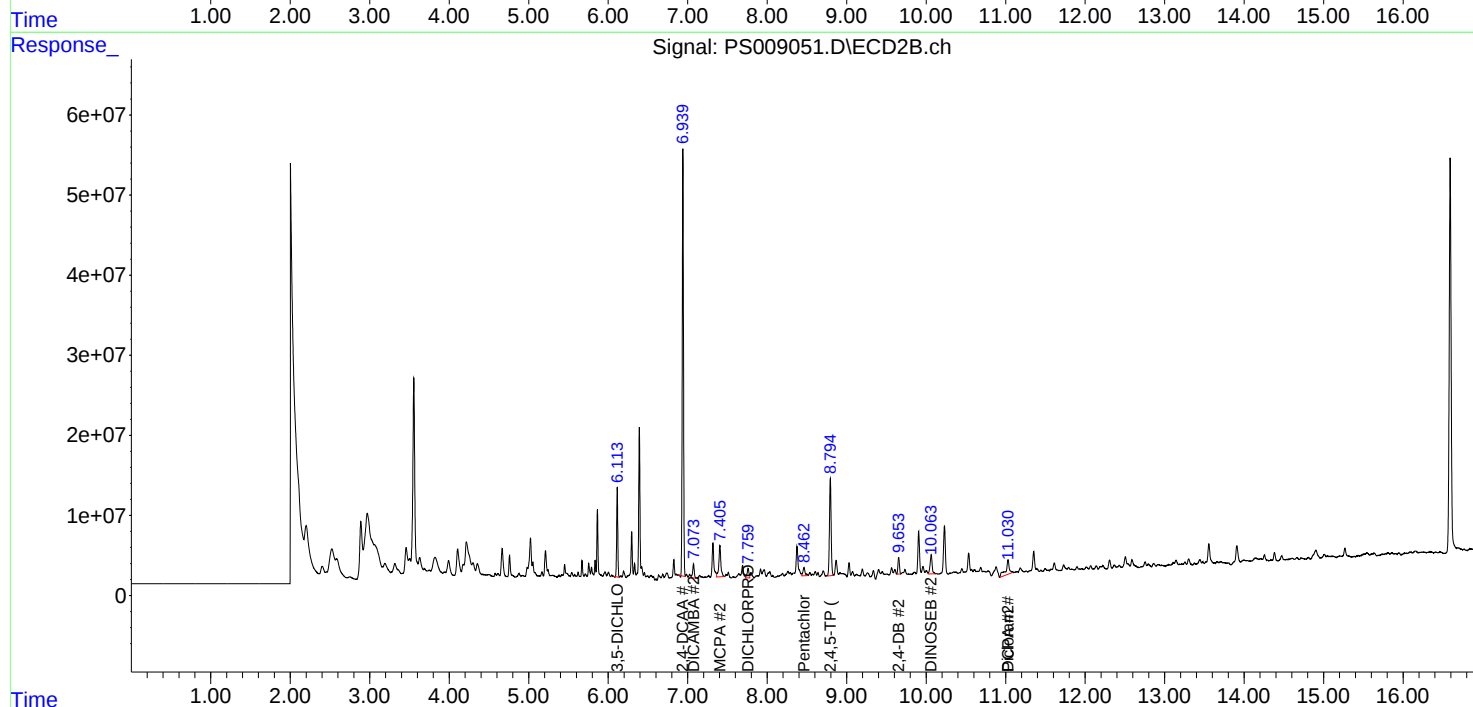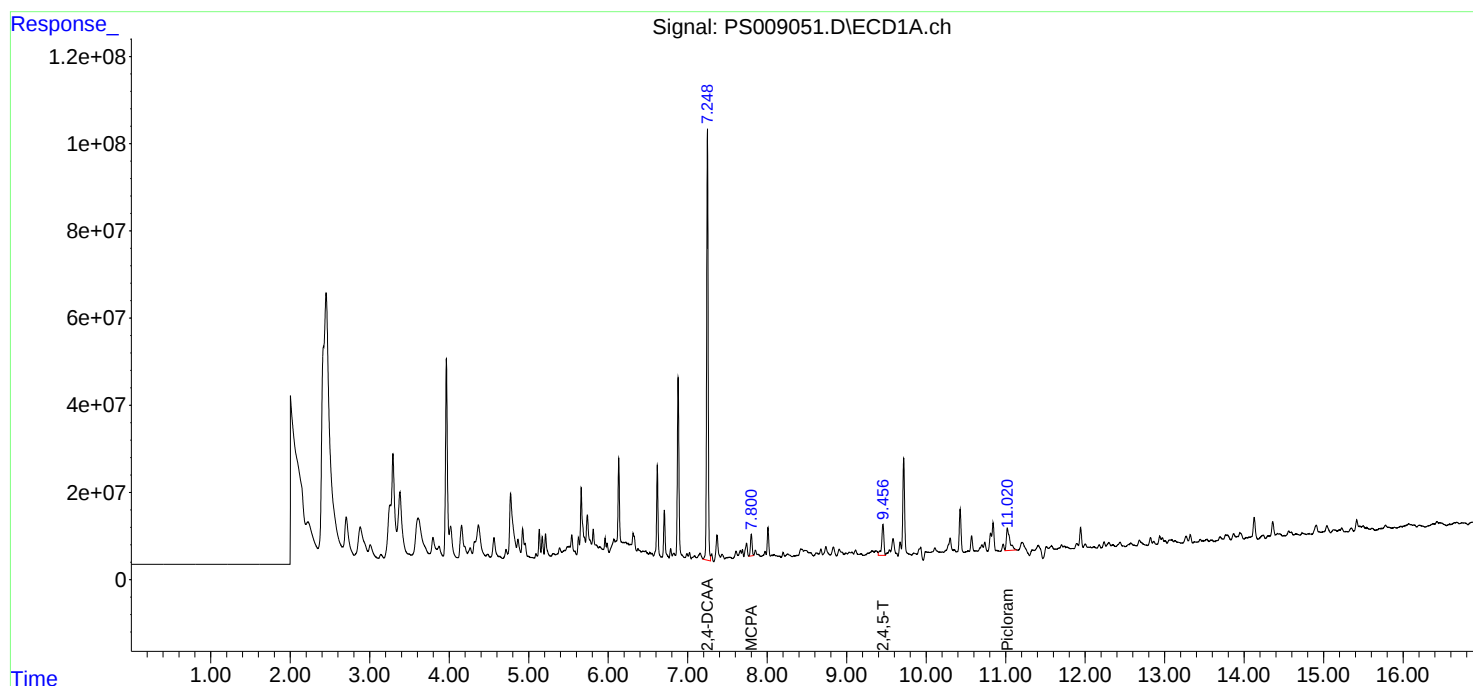


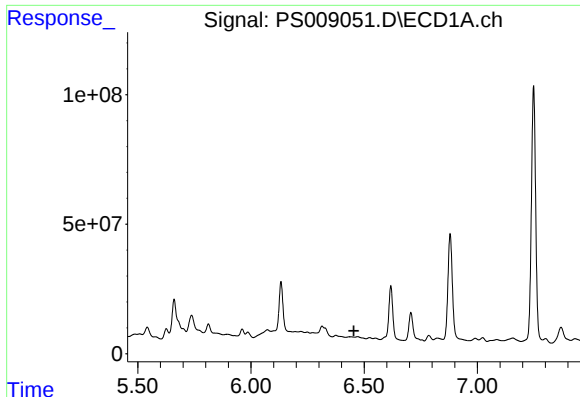

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

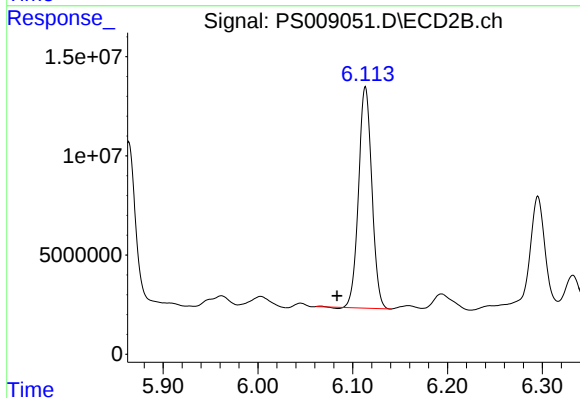


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.114 min
Delta R.T.: 0.030 min
Response: 108539541
Conc: 74.38 ng/ml

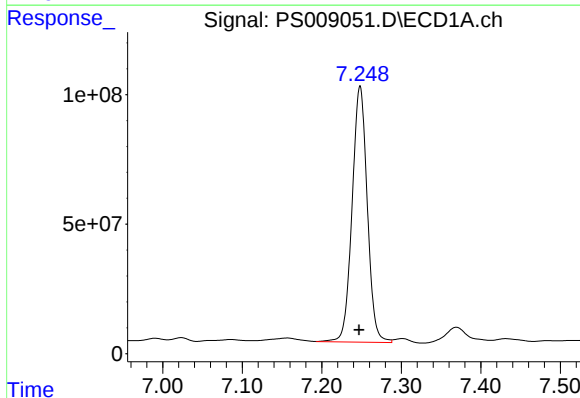


#4 2,4-DCAA

R.T.: 7.248 min
Delta R.T.: 0.001 min
Response: 1310205051
Conc: 599.20 ng/ml

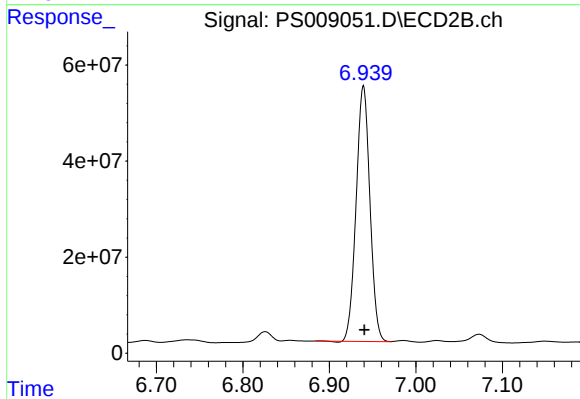

#4 2,4-DCAA


R.T.: 6.939 min
Delta R.T.: -0.001 min
Response: 590331354
Conc: 612.66 ng/ml

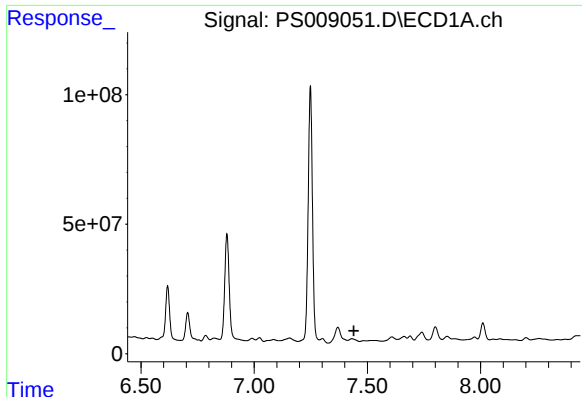

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

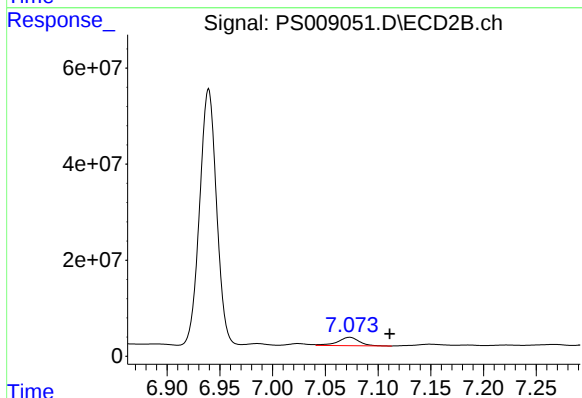


#5 DICAMBA

R.T.: 7.073 min
Delta R.T.: -0.038 min
Response: 24399917
Conc: 5.89 ng/ml

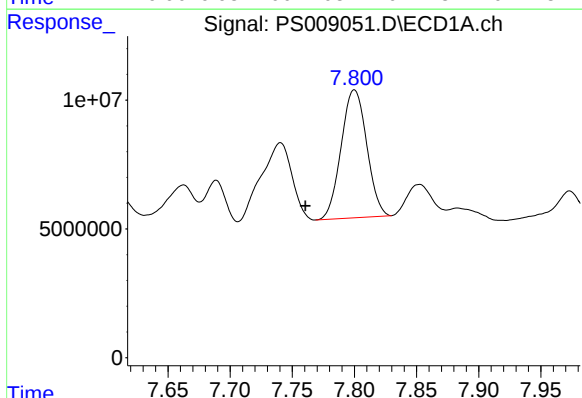


#7 MCPA

R.T.: 7.800 min
Delta R.T.: 0.039 min
Response: 71231701
Conc: 8.86 ug/ml

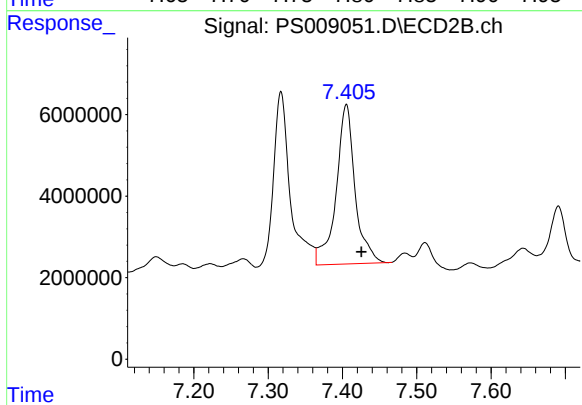

#7 MCPA


R.T.: 7.405 min
Delta R.T.: -0.020 min
Response: 69405418
Conc: 15.69 ug/ml

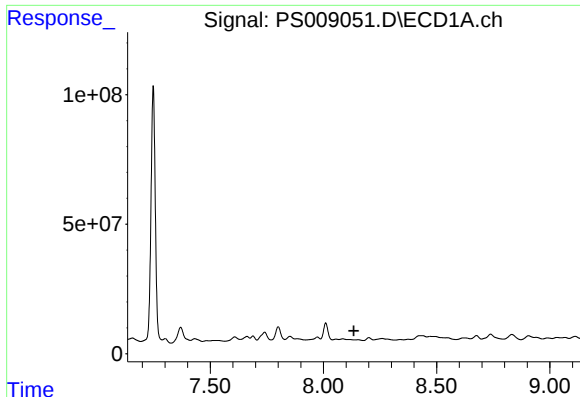

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

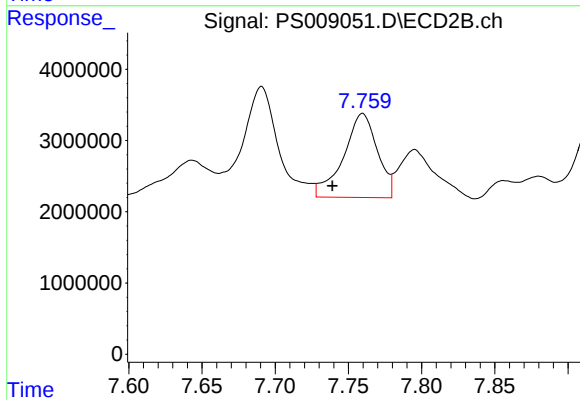


#8 DICHLORPROP

R.T.: 7.760 min
Delta R.T.: 0.021 min
Response: 19050269
Conc: 19.01 ng/ml

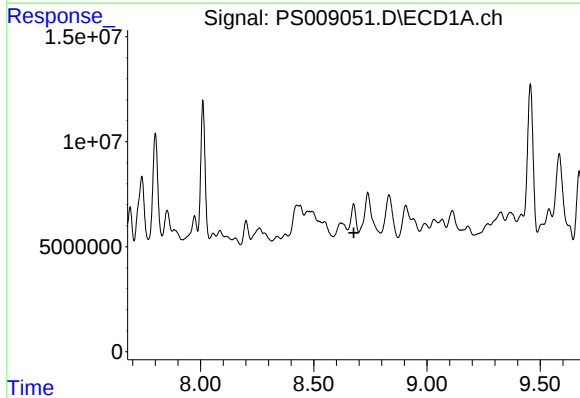


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 8.677 min
Response: 0
Conc: N.D.

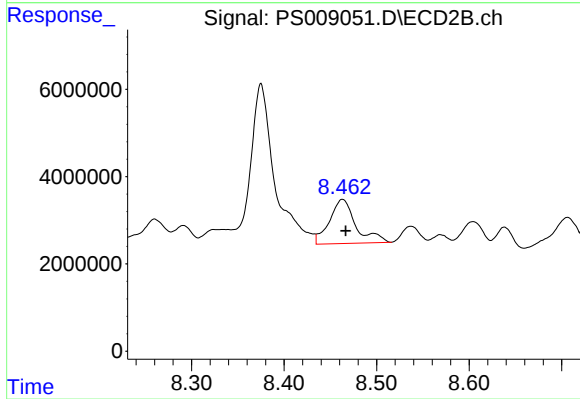

#10 Pentachlorophenol


R.T.: 8.463 min
Delta R.T.: -0.004 min
Response: 19985873
Conc: 1.41 ng/ml

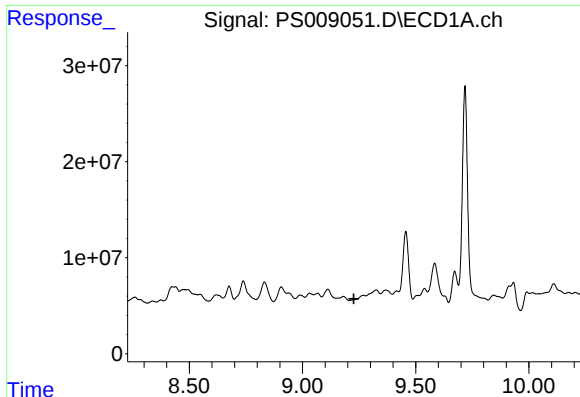

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

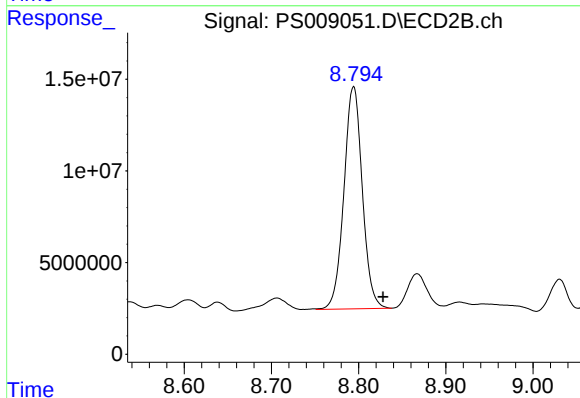


#11 2,4,5-TP (SILVEX)

R.T.: 8.794 min
Delta R.T.: -0.034 min
Response: 177862334
Conc: 32.83 ng/ml

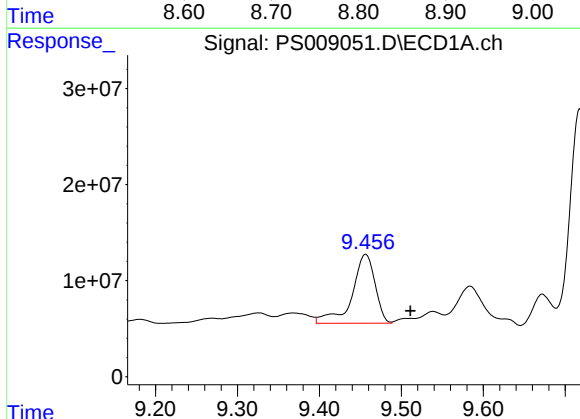


#12 2,4,5-T

R.T.: 9.456 min
Delta R.T.: -0.055 min
Response: 140078201
Conc: 13.10 ng/ml

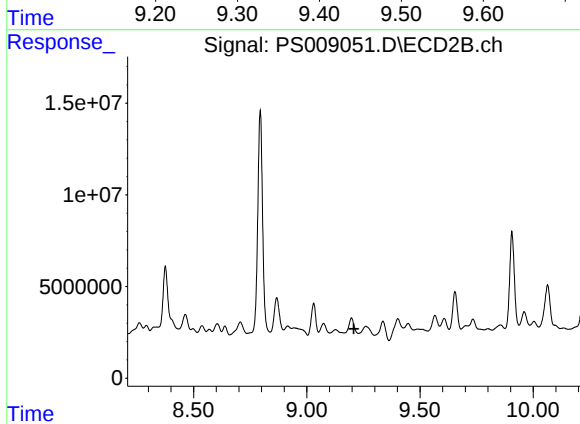

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.208 min
Response: 0
Conc: N.D.

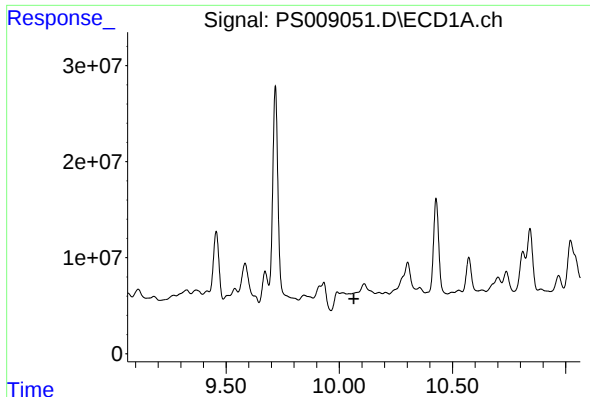

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

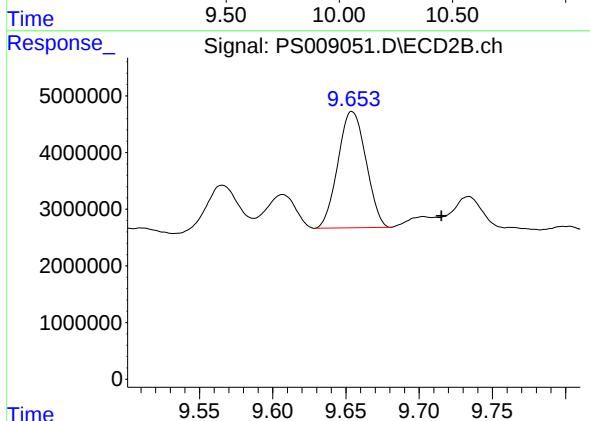


#13 2,4-DB

R.T.: 9.654 min
Delta R.T.: -0.061 min
Response: 27283654
Conc: 38.84 ng/ml

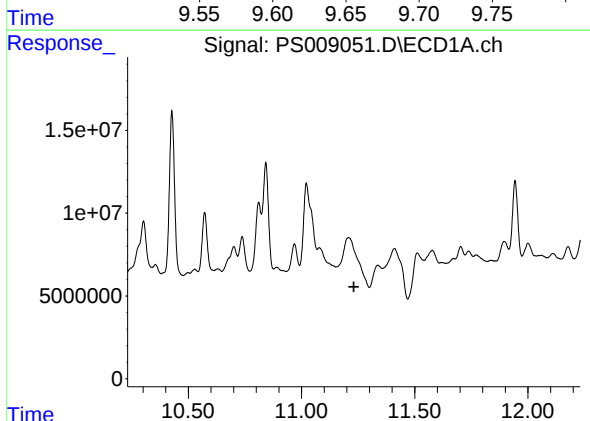


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

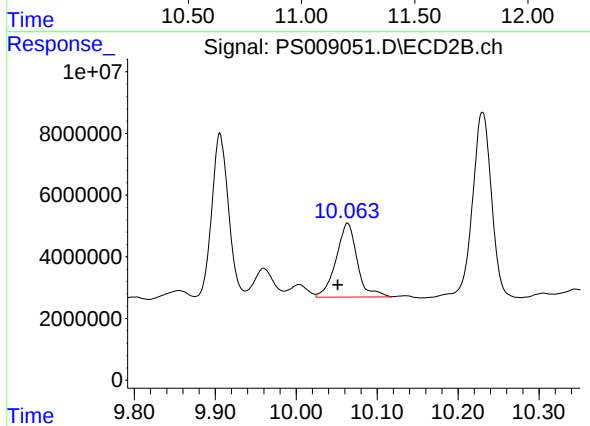

#14 DINOSEB


R.T.: 10.063 min
Delta R.T.: 0.012 min
Response: 43219490
Conc: 10.93 ng/ml

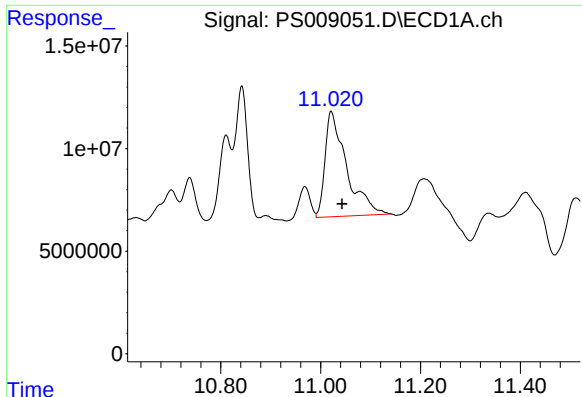

#15 Picloram


R.T.: 11.022 min
Delta R.T.: -0.022 min
Response: 153637053
Conc: 11.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

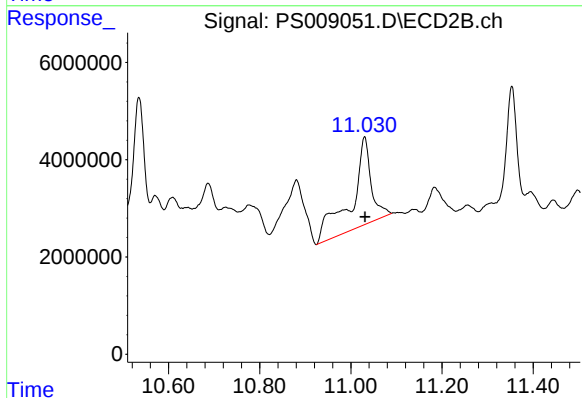


#15 Picloram

R.T.: 11.030 min
Delta R.T.: 0.000 min
Response: 54896077
Conc: 7.55 ng/ml

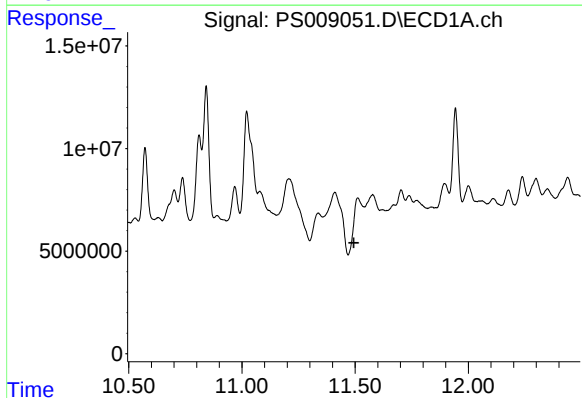

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.

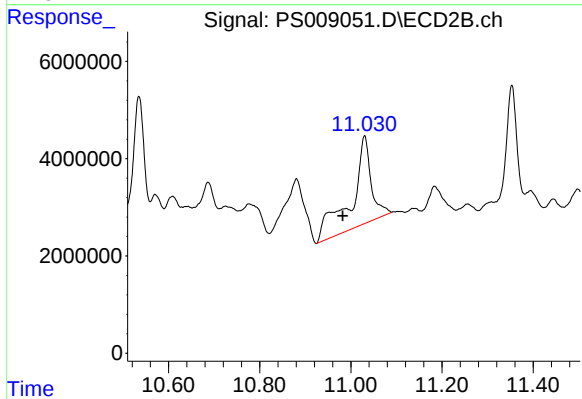

#16 DCPA

R.T.: 11.030 min
Delta R.T.: 0.048 min
Response: 54896077
Conc: 7.93 ng/ml