

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
 Data File : PS009052.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2020 15:20
 Operator : DD\AJ
 Sample : L1700-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 29 00:12:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.248	6.939	1581.5E6	713.8E6	723.281	740.789
Target Compounds							
2) T	3,5-DICHL...	0.000	6.114	0	116.3E6	N.D.	79.722
5) T	DICAMBA	0.000	7.073	0	27423414	N.D.	6.625
7) T	MCPA	7.800	7.405	70158740	71648776	8.722	16.195 #
8) T	DICHLORPROP	0.000	7.759	0	25700887	N.D.	25.651
10) T	Pentachlo...	0.000	8.464	0	34555777	N.D.	2.432
11) T	2,4,5-TP ...	0.000	8.794	0	157.3E6	N.D.	29.041
12) T	2,4,5-T	9.456	0.000	167.5E6	0	15.664	N.D. #
13) T	2,4-DB	0.000	9.654	0	28945297	N.D.	41.207
14) T	DINOSEB	0.000	10.063	0	47775935	N.D.	12.083
15) T	Picloram	11.022	11.029	111.2E6	53209548	8.124	7.323
16) T	DCPA	0.000	11.029	0	53209548	N.D.	7.690



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
Data File : PS009052.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2020 15:20
Operator : DD\AJ
Sample : L1700-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 29 00:12:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

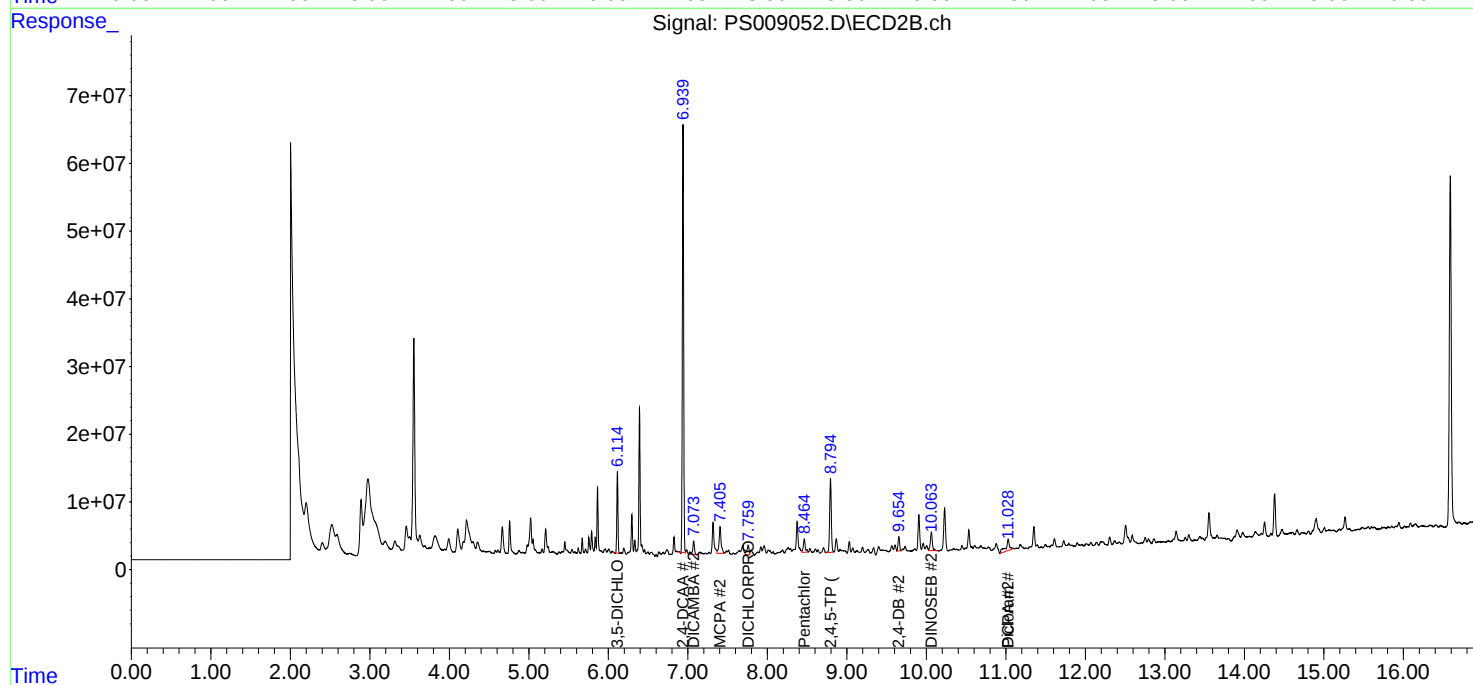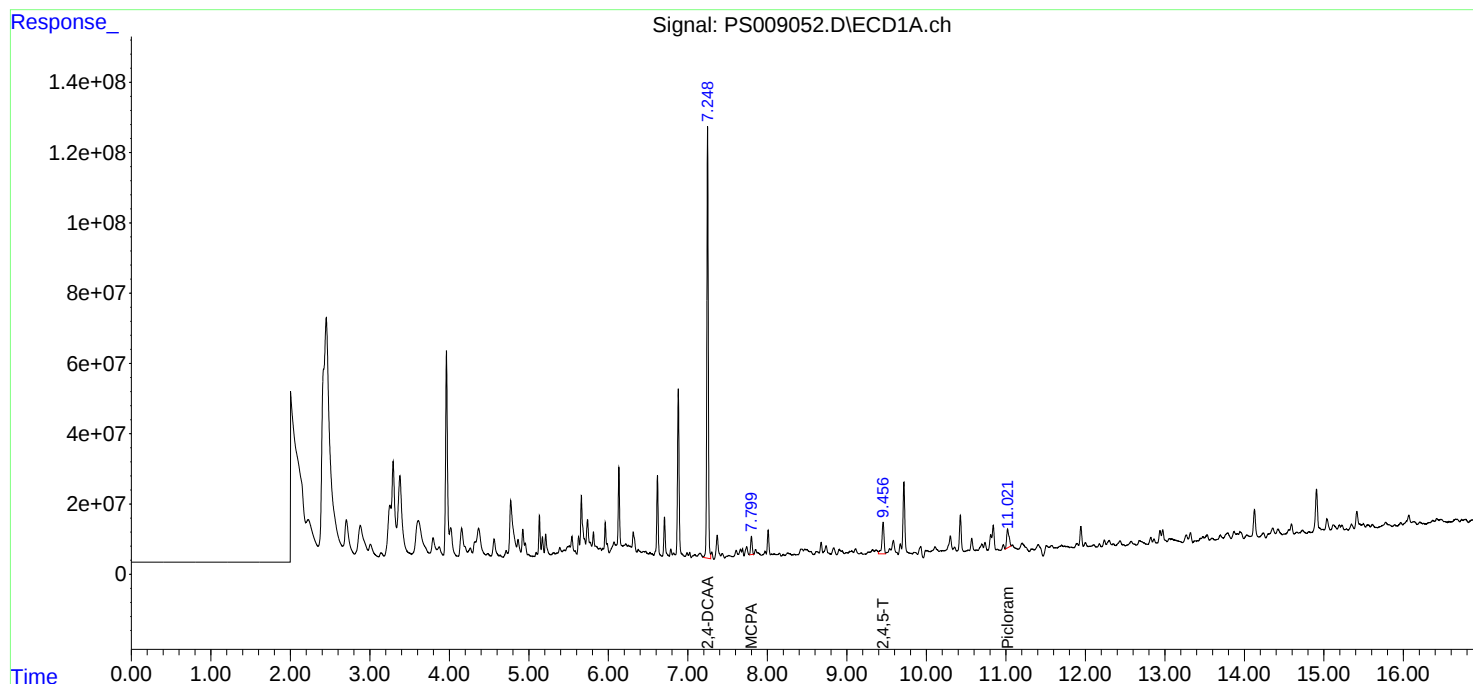


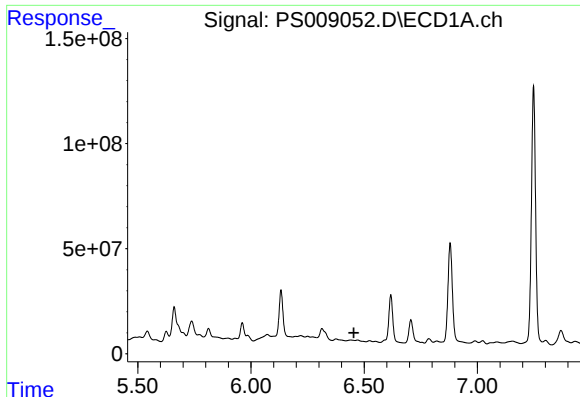

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

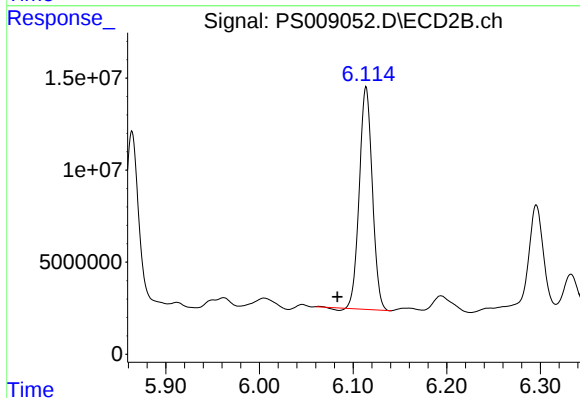


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.114 min
Delta R.T.: 0.030 min
Response: 116335657
Conc: 79.72 ng/ml

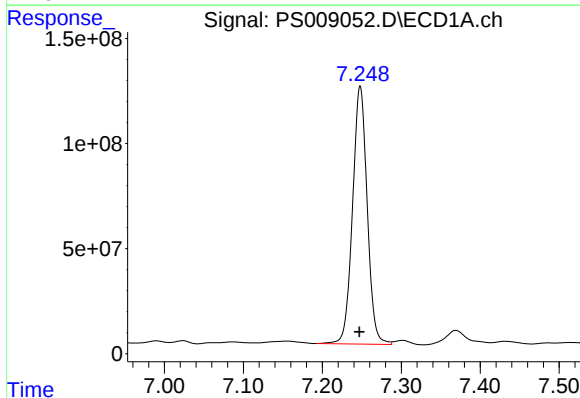


#4 2,4-DCAA

R.T.: 7.248 min
Delta R.T.: 0.001 min
Response: 1581519981
Conc: 723.28 ng/ml

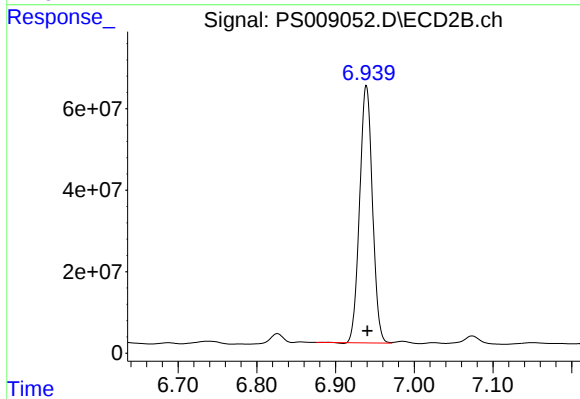

#4 2,4-DCAA


R.T.: 6.939 min
Delta R.T.: -0.001 min
Response: 713791287
Conc: 740.79 ng/ml

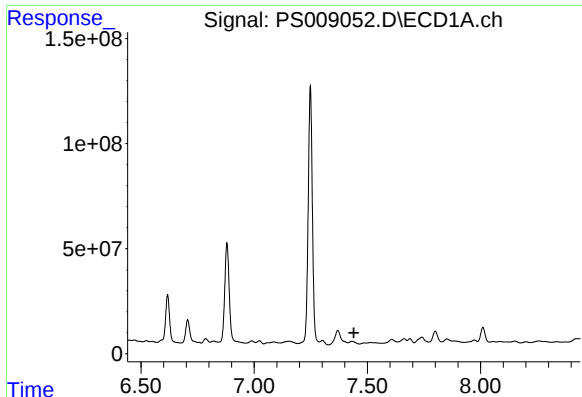

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

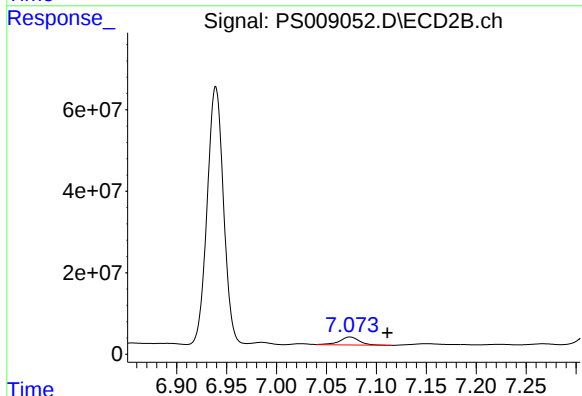


#5 DICAMBA

R.T.: 7.073 min
Delta R.T.: -0.038 min
Response: 27423414
Conc: 6.63 ng/ml

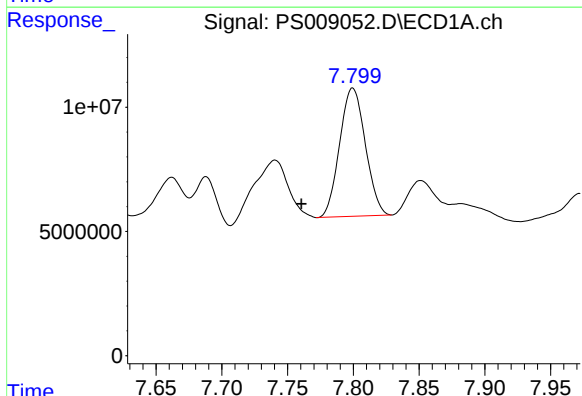


#7 MCPA

R.T.: 7.800 min
Delta R.T.: 0.039 min
Response: 70158740
Conc: 8.72 ug/ml

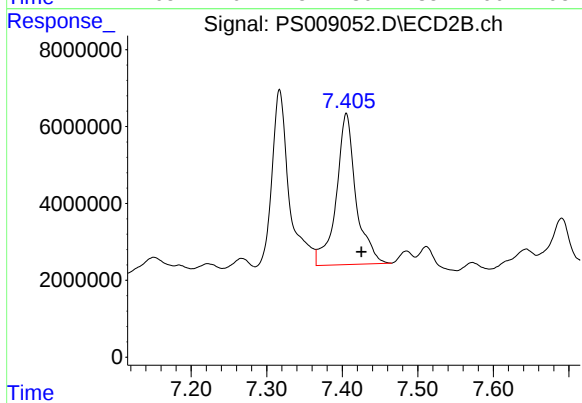

#7 MCPA


R.T.: 7.405 min
Delta R.T.: -0.020 min
Response: 71648776
Conc: 16.19 ug/ml

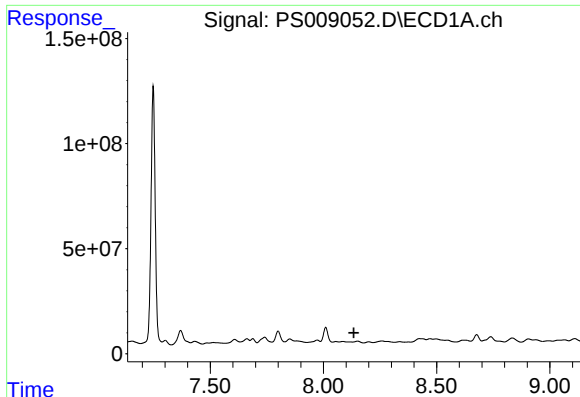

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

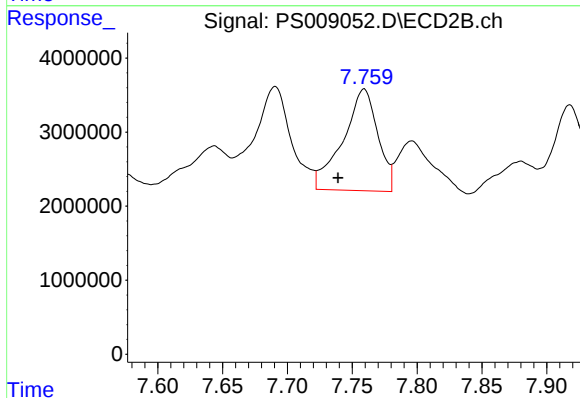


#8 DICHLORPROP

R.T.: 7.759 min
Delta R.T.: 0.020 min
Response: 25700887
Conc: 25.65 ng/ml

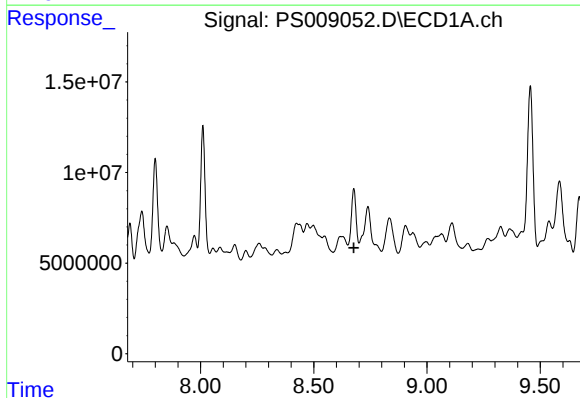


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 8.677 min
Response: 0
Conc: N.D.

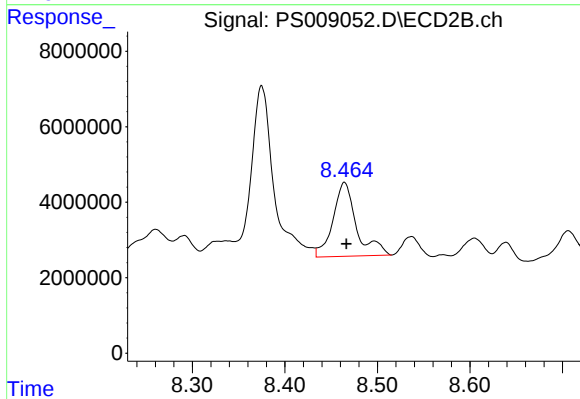

#10 Pentachlorophenol


R.T.: 8.464 min
Delta R.T.: -0.002 min
Response: 34555777
Conc: 2.43 ng/ml

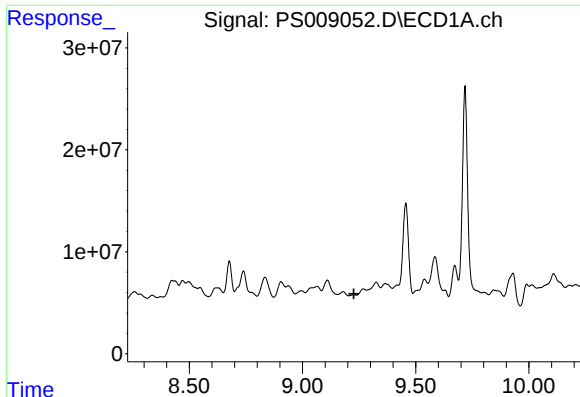

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

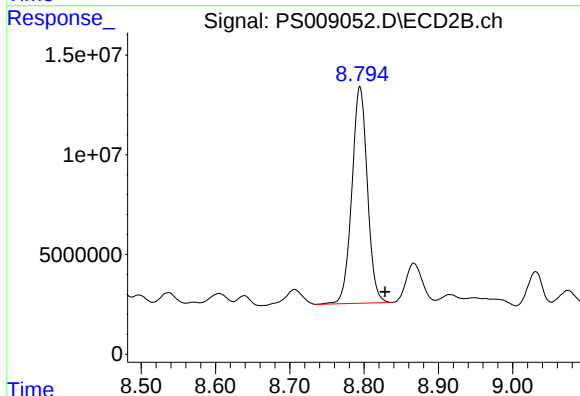


#11 2,4,5-TP (SILVEX)

R.T.: 8.794 min
Delta R.T.: -0.034 min
Response: 157312094
Conc: 29.04 ng/ml

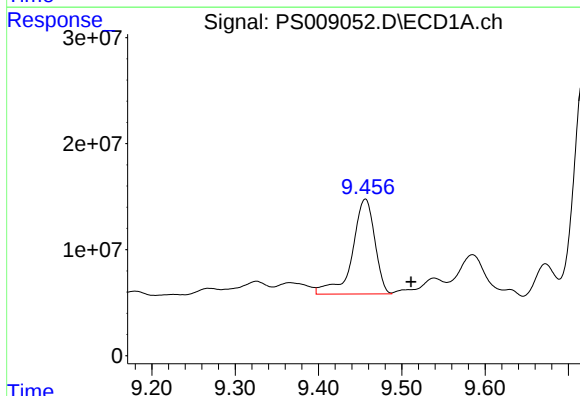


#12 2,4,5-T

R.T.: 9.456 min
Delta R.T.: -0.055 min
Response: 167477395
Conc: 15.66 ng/ml

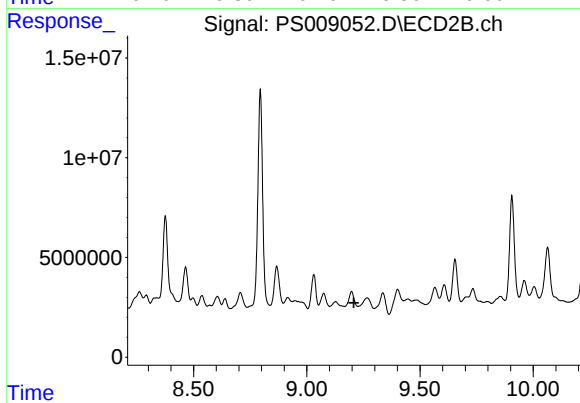

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.208 min
Response: 0
Conc: N.D.

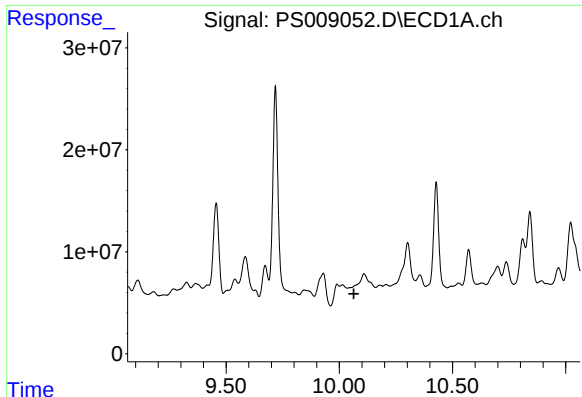

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

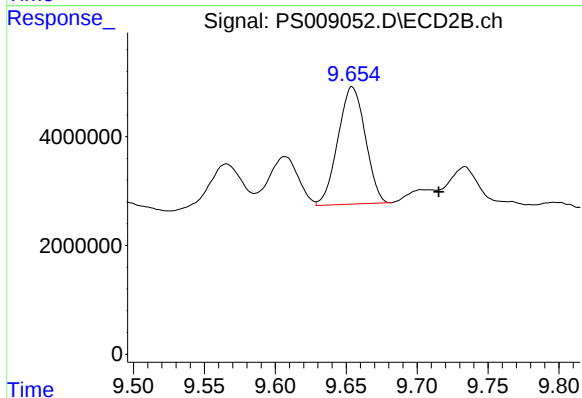


#13 2,4-DB

R.T.: 9.654 min
Delta R.T.: -0.061 min
Response: 28945297
Conc: 41.21 ng/ml

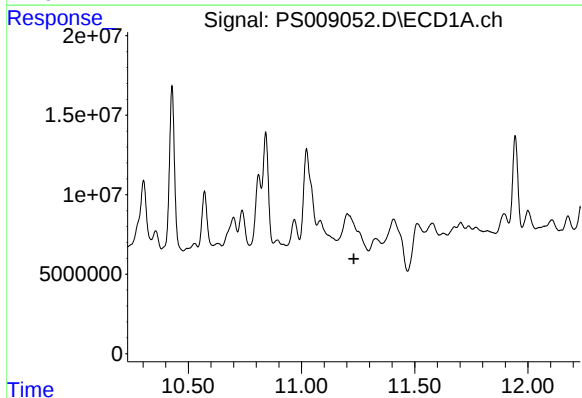


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

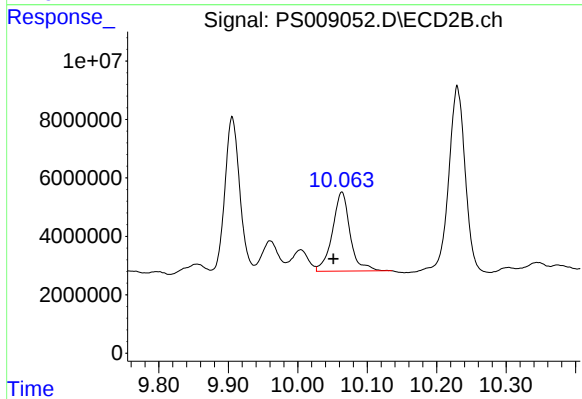

#14 DINOSEB


R.T.: 10.063 min
Delta R.T.: 0.012 min
Response: 47775935
Conc: 12.08 ng/ml

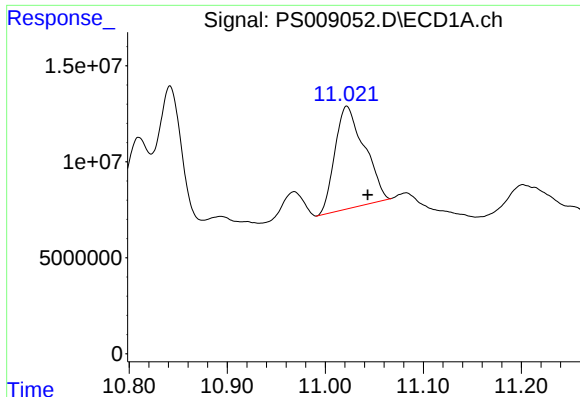

#15 Picloram


R.T.: 11.022 min
Delta R.T.: -0.021 min
Response: 111221675
Conc: 8.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

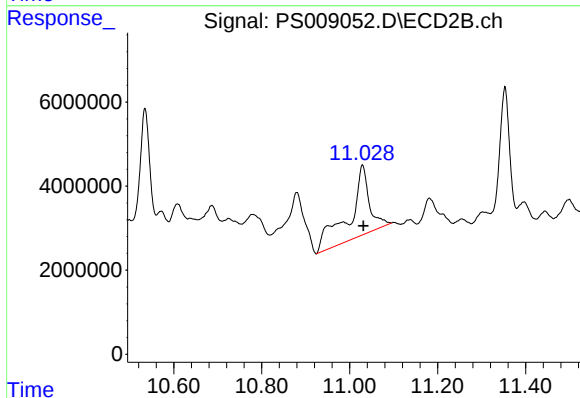


#15 Picloram

R.T.: 11.029 min
Delta R.T.: -0.002 min
Response: 53209548
Conc: 7.32 ng/ml

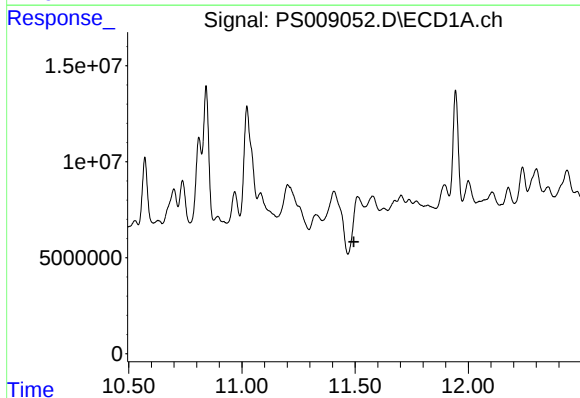

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.

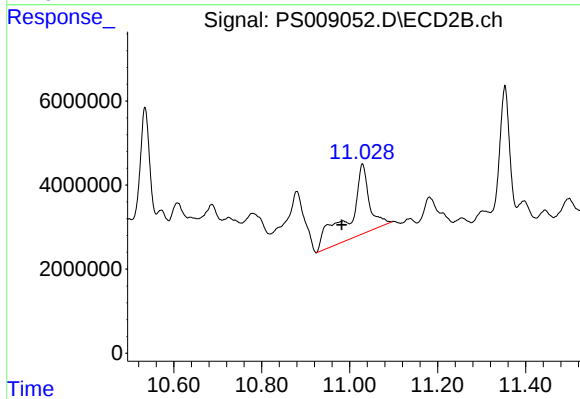

#16 DCPA

R.T.: 11.029 min
Delta R.T.: 0.047 min
Response: 53209548
Conc: 7.69 ng/ml