

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
 Data File : PS009057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2020 18:14
 Operator : DD\AJ
 Sample : PB127152TB
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 29 00:13:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.939	763.0E6	371.6E6	348.932	385.671
Target Compounds							
1) T	Dalapon	0.000	2.591	0	46207665	N.D.	31.601
2) T	3,5-DICHL...	0.000	6.114	0	139.5E6	N.D.	95.596
5) T	DICAMBA	0.000	7.074	0	37970681	N.D.	9.173
7) T	MCPA	7.692	0.000	191.3E6	0	23.785	N.D. #
8) T	DICHLORPROP	0.000	7.760	0	28198605	N.D.	28.144
10) T	Pentachlo...	0.000	8.463	0	19965755	N.D.	1.405
11) T	2,4,5-TP ...	0.000	8.793	0	114.2E6	N.D.	21.081
12) T	2,4,5-T	9.454	9.262	128.3E6	21866755	11.996	4.040 #
14) T	DINOSEB	0.000	10.097	0	27673943	N.D.	6.999
15) T	Picloram	11.023	11.031	153.8E6	36548488	11.237	5.030 #
16) T	DCPA	0.000	11.031	0	36548488	N.D.	5.282



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
Data File : PS009057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2020 18:14
Operator : DD\AJ
Sample : PB127152TB
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 29 00:13:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

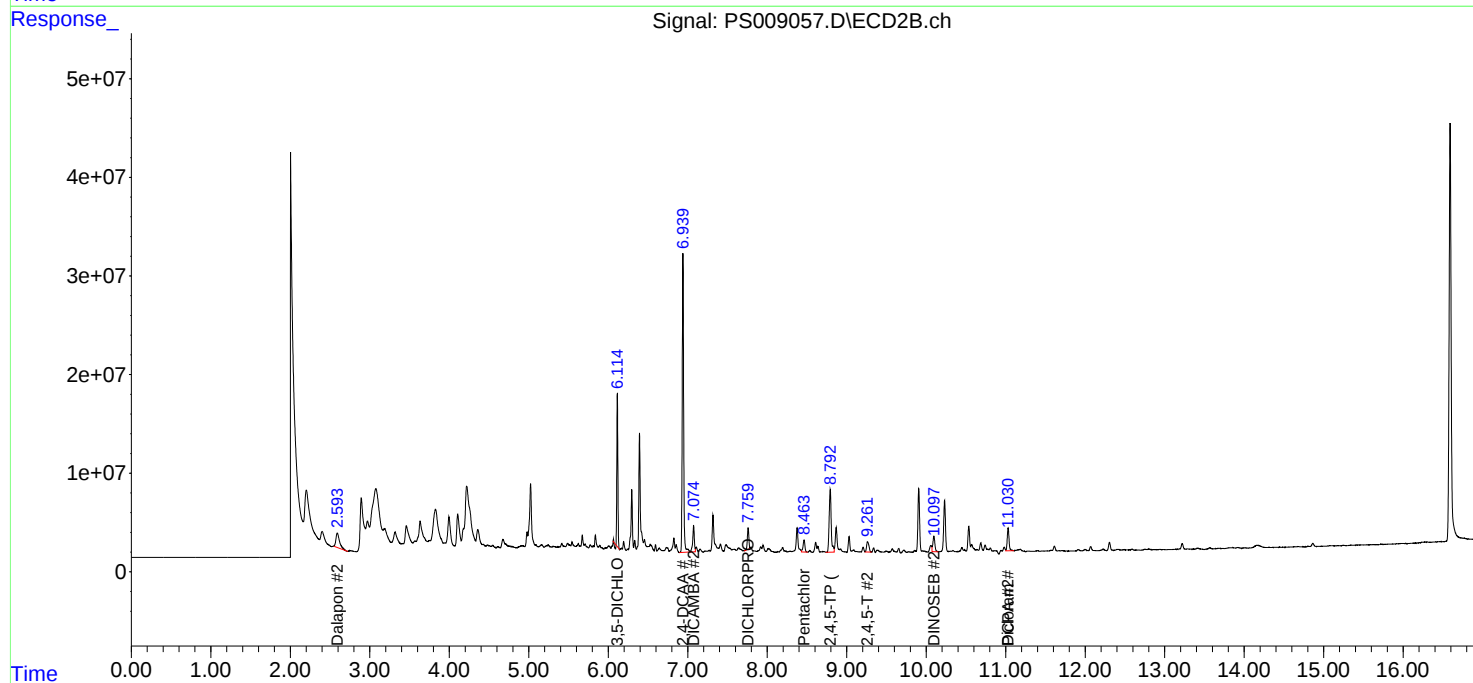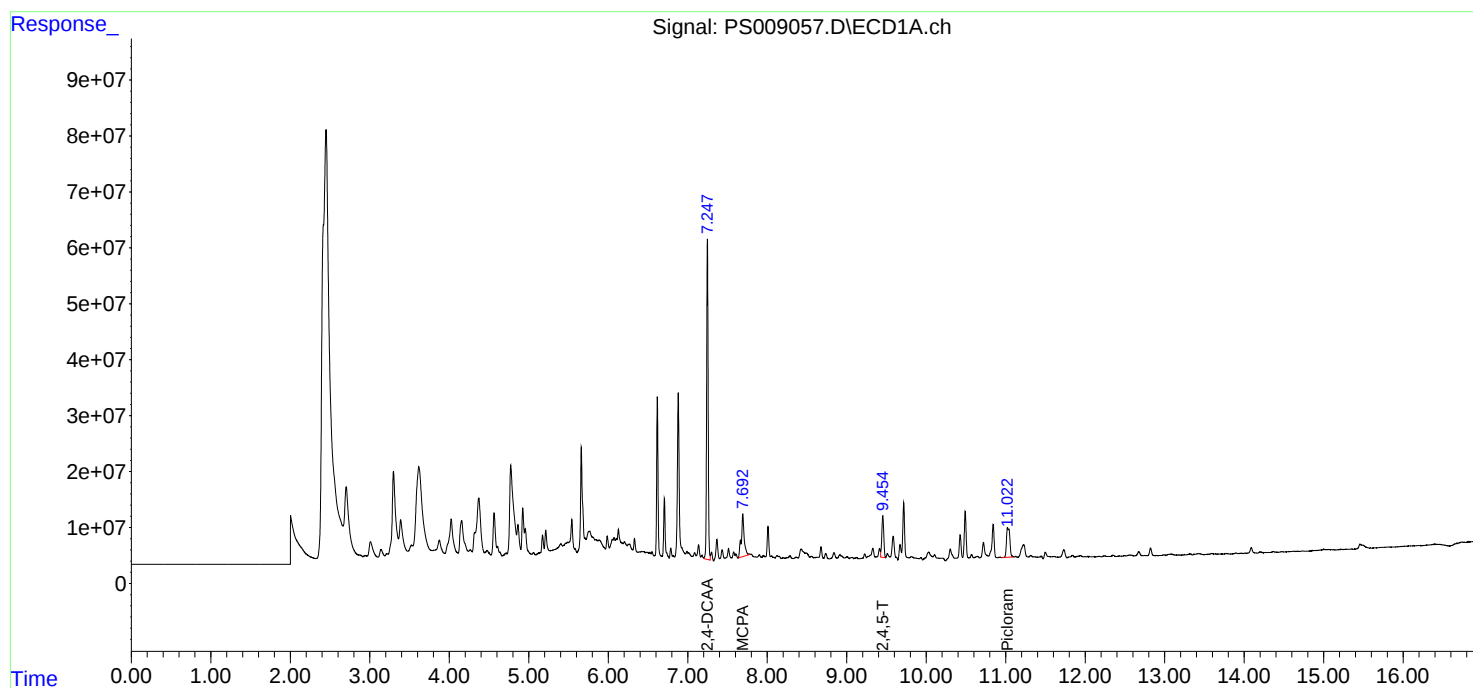


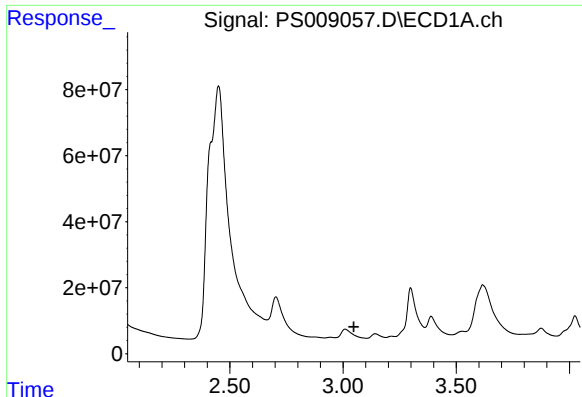

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

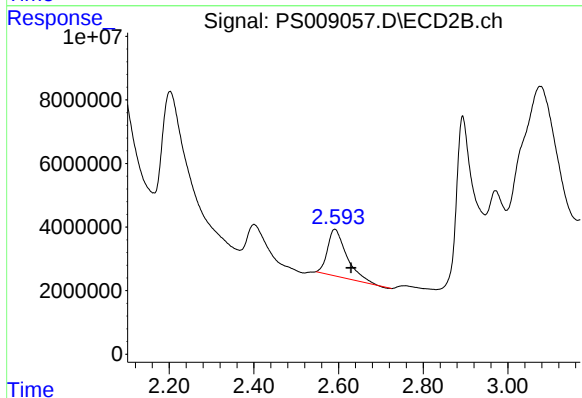


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.039 min
Response: 46207665
Conc: 31.60 ng/ml

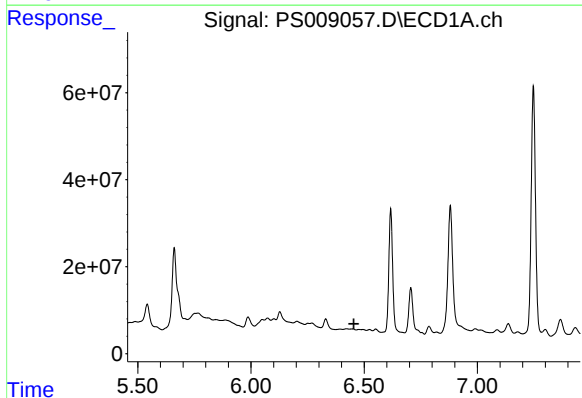


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

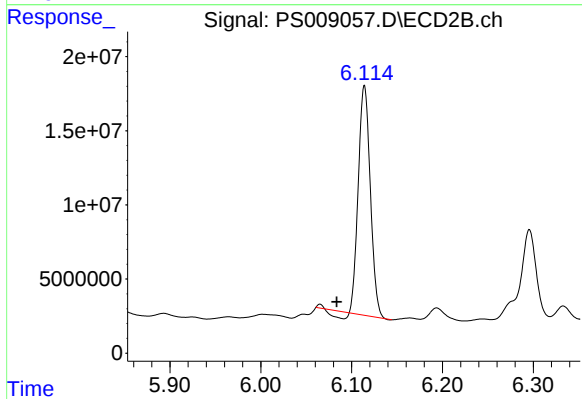

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.031 min
Response: 139499722
Conc: 95.60 ng/ml

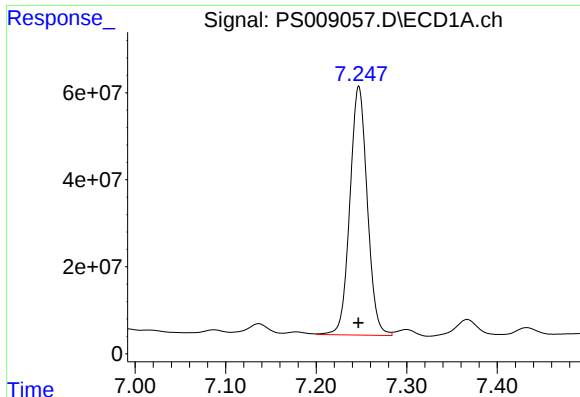

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 762972063
Conc: 348.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

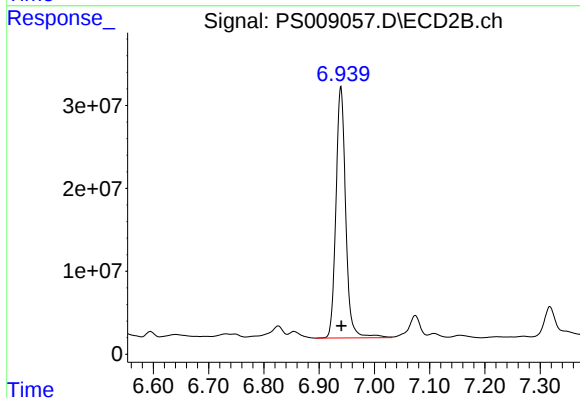


#4 2,4-DCAA

R.T.: 6.939 min
Delta R.T.: -0.001 min
Response: 371615401
Conc: 385.67 ng/ml

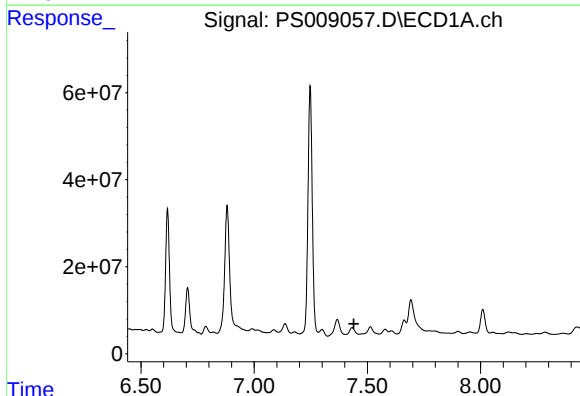


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.

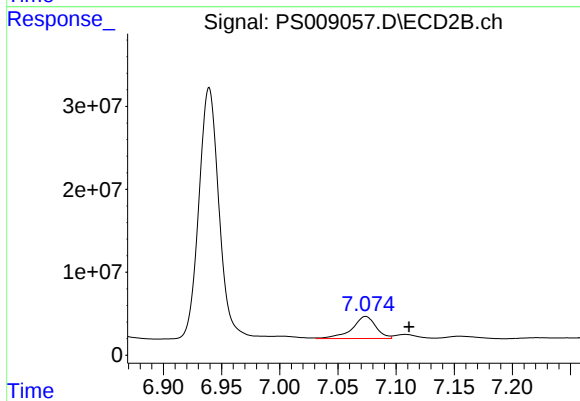

#5 DICAMBA


R.T.: 7.074 min
Delta R.T.: -0.037 min
Response: 37970681
Conc: 9.17 ng/ml

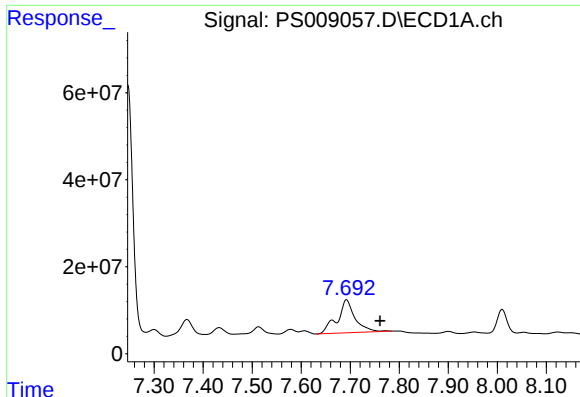

#7 MCPA


R.T.: 7.692 min
Delta R.T.: -0.068 min
Response: 191327980
Conc: 23.79 ug/ml

Instrument :
ECD_S
ClientSampleId :

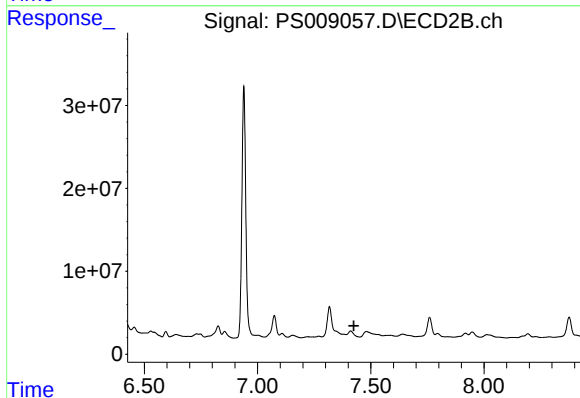


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.425 min
Response: 0
Conc: N.D.

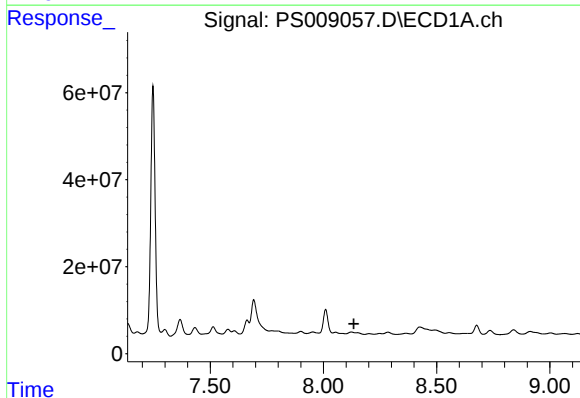


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

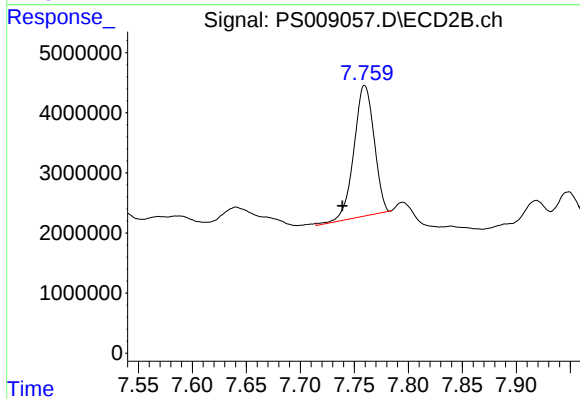

#8 DICHLORPROP


R.T.: 7.760 min
Delta R.T.: 0.021 min
Response: 28198605
Conc: 28.14 ng/ml

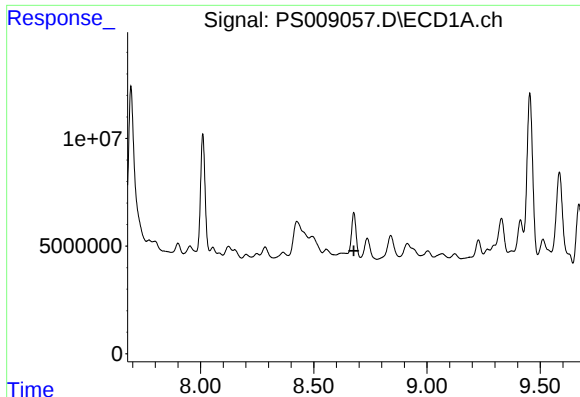

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.677 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

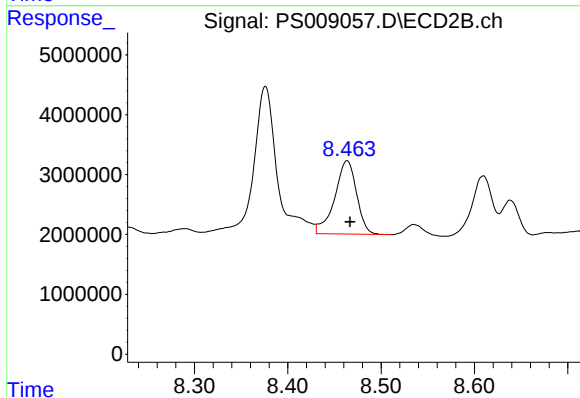


#10 Pentachlorophenol

R.T.: 8.463 min
Delta R.T.: -0.003 min
Response: 19965755
Conc: 1.41 ng/ml

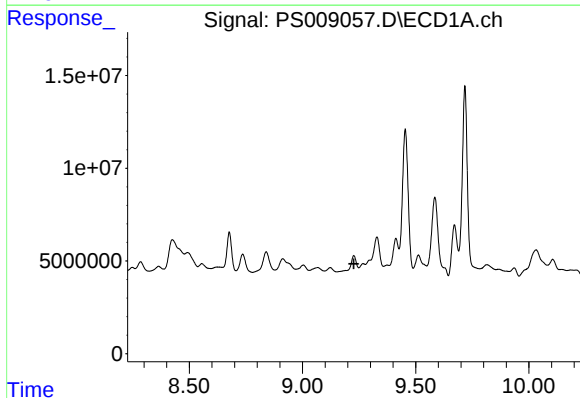


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

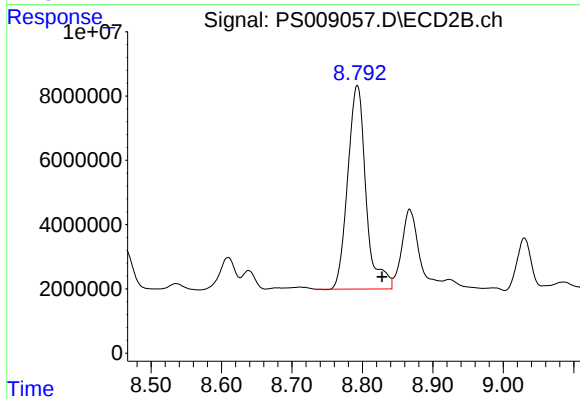

#11 2,4,5-TP (SILVEX)


R.T.: 8.793 min
Delta R.T.: -0.035 min
Response: 114192739
Conc: 21.08 ng/ml

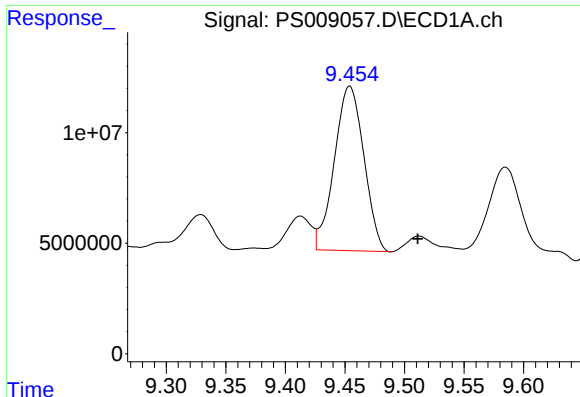

#12 2,4,5-T


R.T.: 9.454 min
Delta R.T.: -0.057 min
Response: 128265053
Conc: 12.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

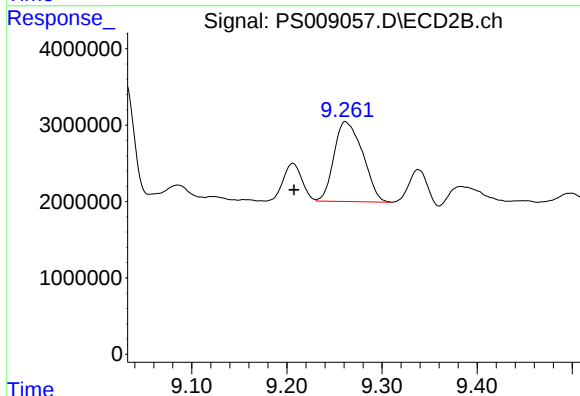


#12 2,4,5-T

R.T.: 9.262 min
Delta R.T.: 0.054 min
Response: 21866755
Conc: 4.04 ng/ml

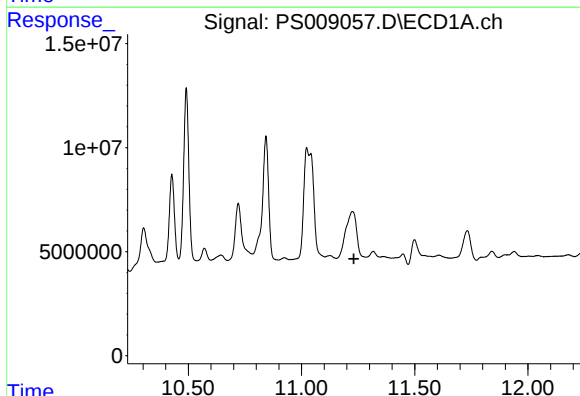


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

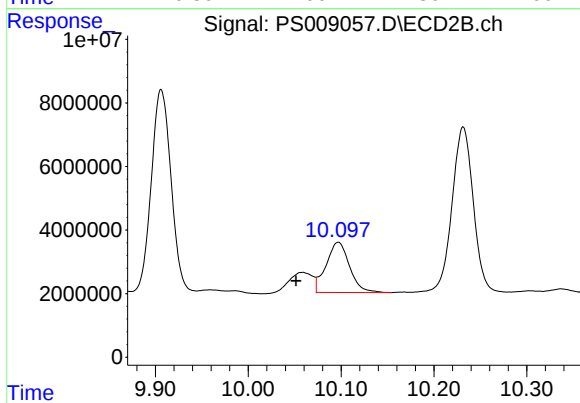

#14 DINOSEB


R.T.: 10.097 min
Delta R.T.: 0.045 min
Response: 27673943
Conc: 7.00 ng/ml

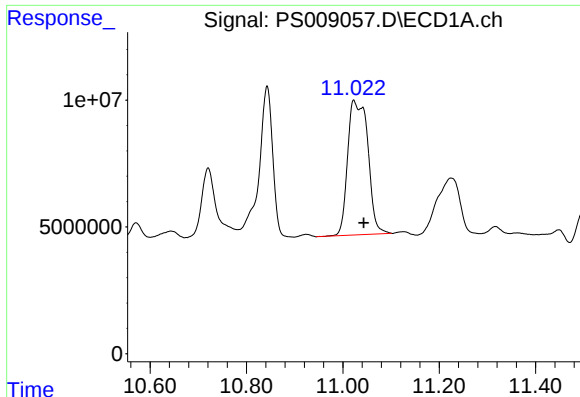

#15 Picloram


R.T.: 11.023 min
Delta R.T.: -0.020 min
Response: 153848525
Conc: 11.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

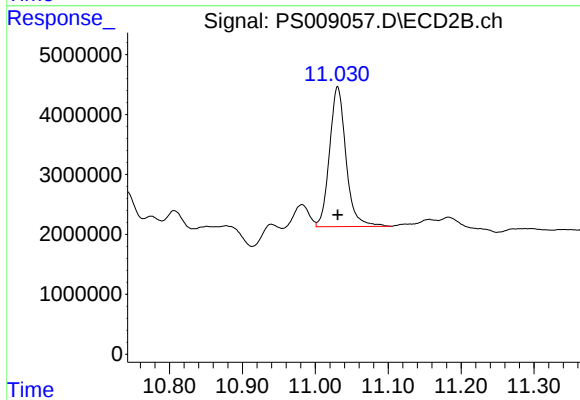


#15 Picloram

R.T.: 11.031 min
Delta R.T.: 0.000 min
Response: 36548488
Conc: 5.03 ng/ml

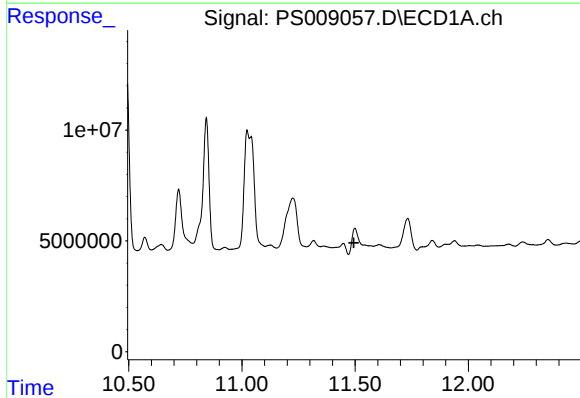

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.

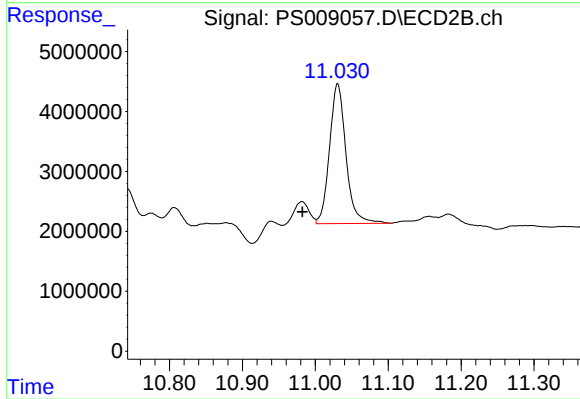

#16 DCPA

R.T.: 11.031 min
Delta R.T.: 0.048 min
Response: 36548488
Conc: 5.28 ng/ml