

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
 Data File : PS009058.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2020 18:37
 Operator : DD\AJ
 Sample : L1363-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 29 00:13:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.248	6.939	807.5E6	379.9E6	369.279	394.295
Target Compounds							
1) T	Dalapon	0.000	2.590	0	46747749	N.D.	31.970
2) T	3,5-DICHL...	0.000	6.114	0	164.3E6	N.D.	112.587
5) T	DICAMBA	0.000	7.074	0	32844400	N.D.	7.935
7) T	MCPA	7.693	0.000	218.5E6	0	27.165	N.D. #
8) T	DICHLORPROP	0.000	7.759	0	27908014	N.D.	27.854
11) T	2,4,5-TP ...	0.000	8.791	0	113.8E6	N.D.	21.015
12) T	2,4,5-T	9.454	0.000	166.3E6	0	15.555	N.D. #
14) T	DINOSEB	0.000	10.096	0	33394064	N.D.	8.446
15) T	Picloram	11.021	11.030	127.0E6	16370038	9.275	2.253 #
16) T	DCPA	0.000	11.030	0	16370038	N.D.	2.366



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
Data File : PS009058.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2020 18:37
Operator : DD\AJ
Sample : L1363-10
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 29 00:13:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

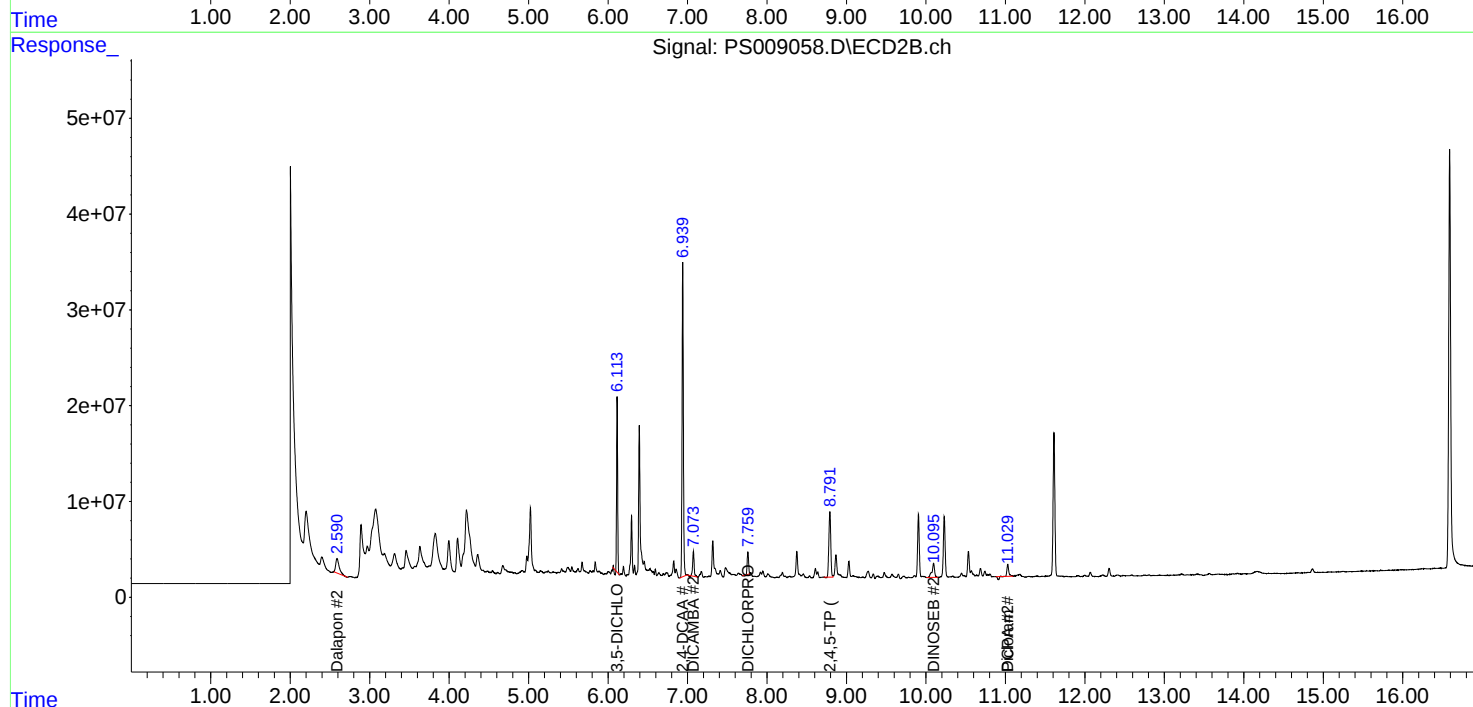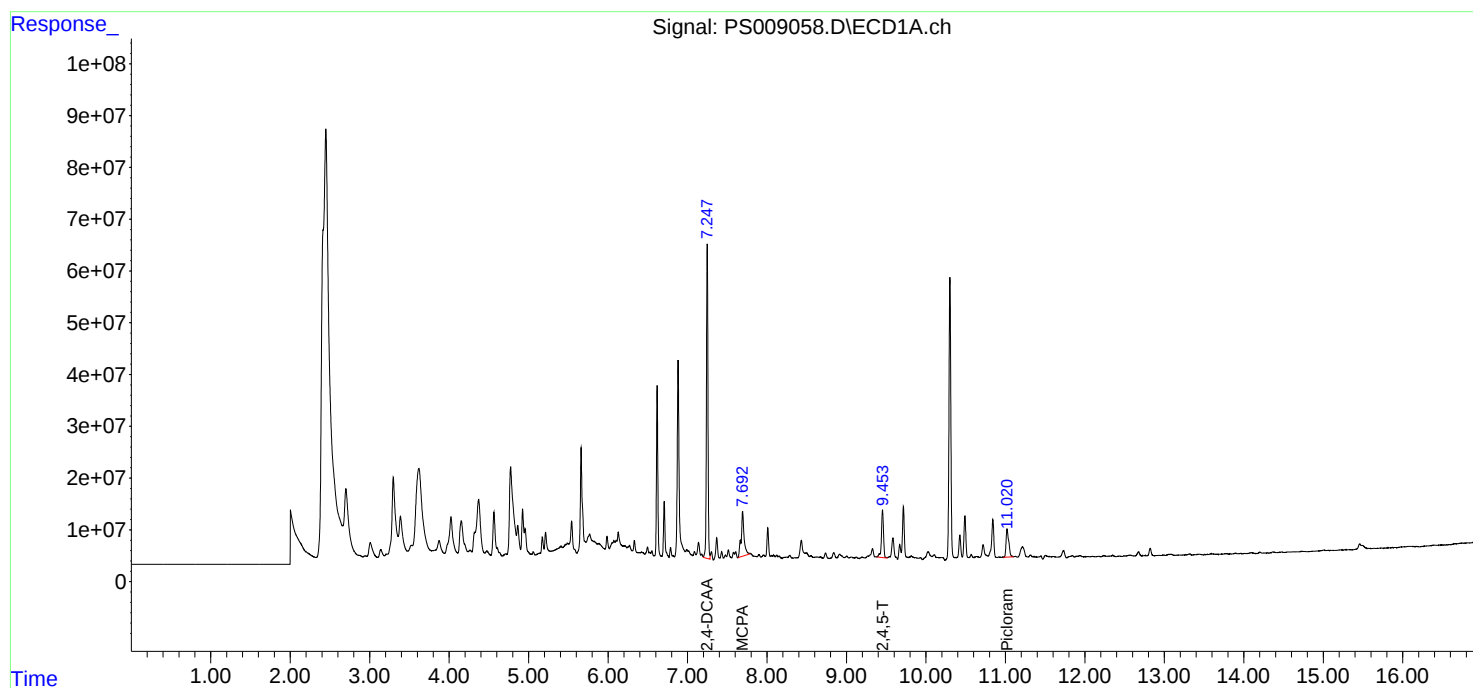


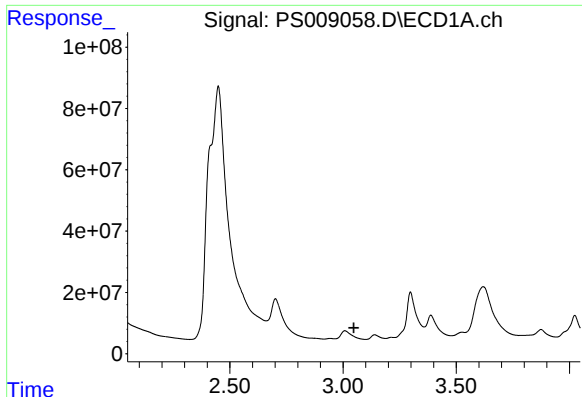

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

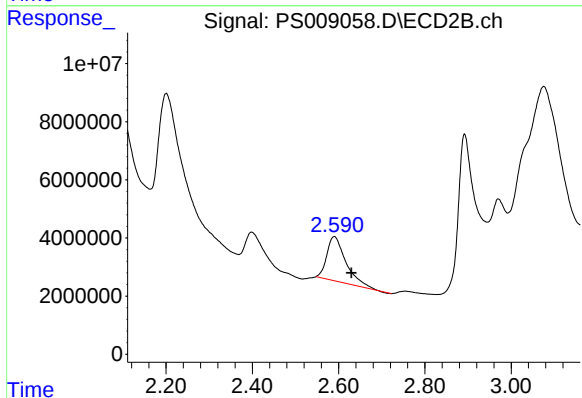


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.040 min
Response: 46747749
Conc: 31.97 ng/ml

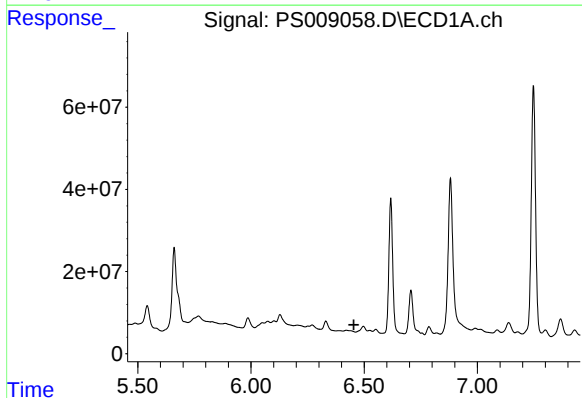


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

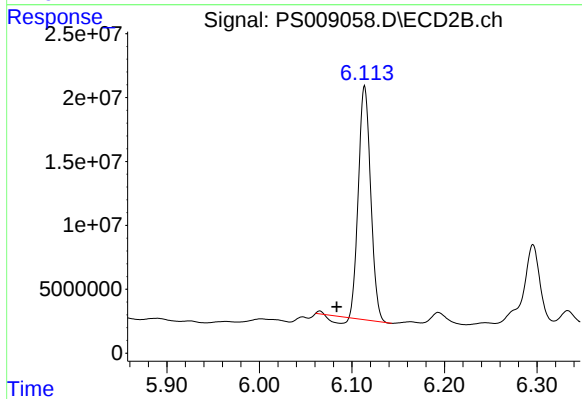

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.030 min
Response: 164294698
Conc: 112.59 ng/ml

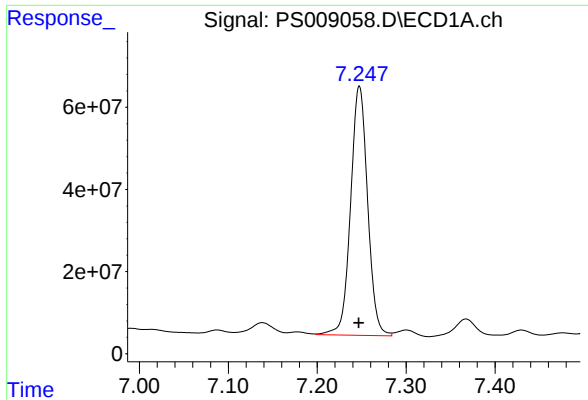

#4 2,4-DCAA


R.T.: 7.248 min
Delta R.T.: 0.000 min
Response: 807462900
Conc: 369.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

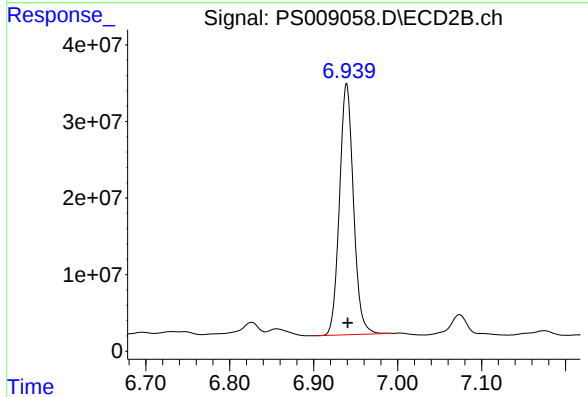


#4 2,4-DCAA

R.T.: 6.939 min
Delta R.T.: -0.001 min
Response: 379924710
Conc: 394.29 ng/ml

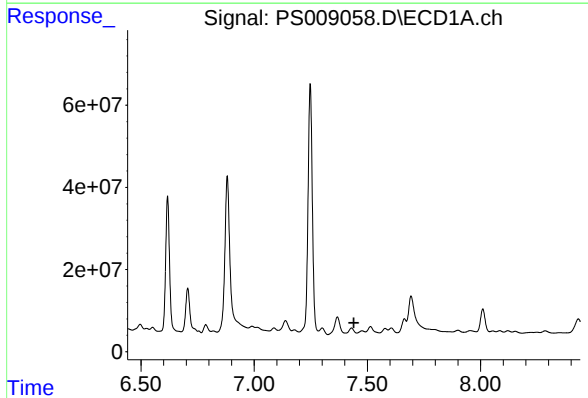


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.

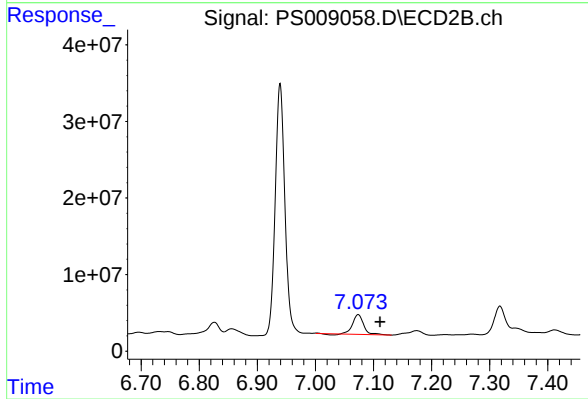

#5 DICAMBA


R.T.: 7.074 min
Delta R.T.: -0.037 min
Response: 32844400
Conc: 7.93 ng/ml

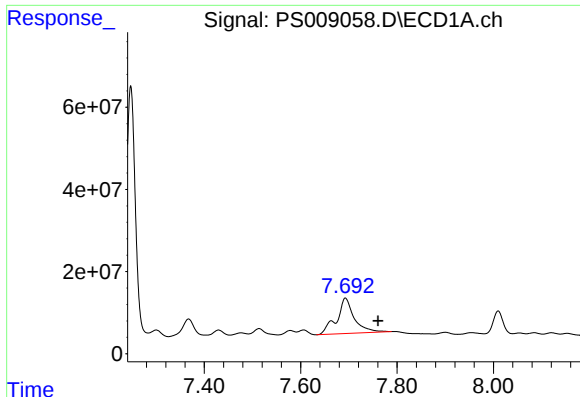

#7 MCPA


R.T.: 7.693 min
Delta R.T.: -0.068 min
Response: 218513169
Conc: 27.16 ug/ml

Instrument :
ECD_S
ClientSampleId :

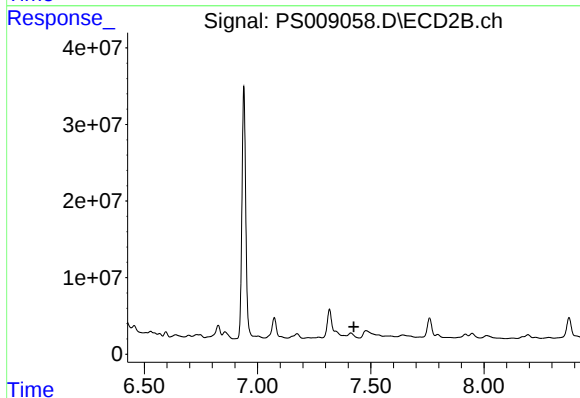


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.425 min
Response: 0
Conc: N.D.

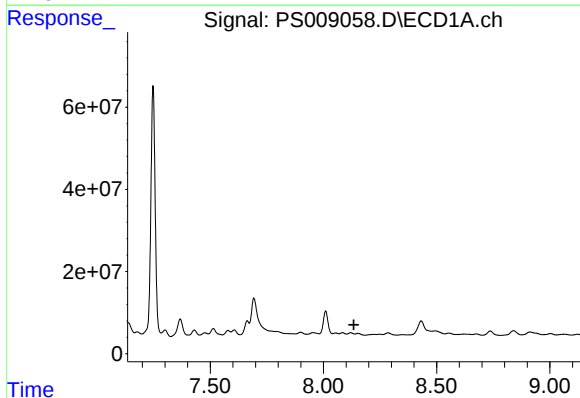


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

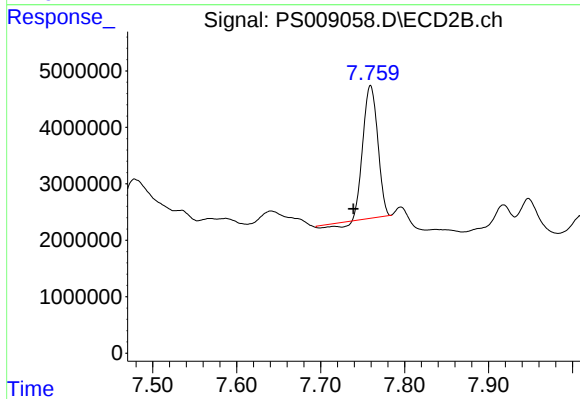

#8 DICHLORPROP


R.T.: 7.759 min
Delta R.T.: 0.020 min
Response: 27908014
Conc: 27.85 ng/ml

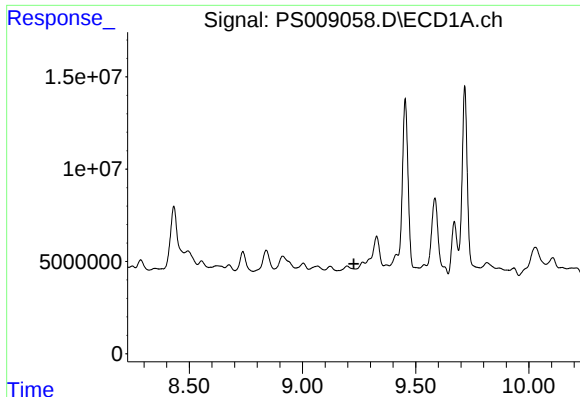

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

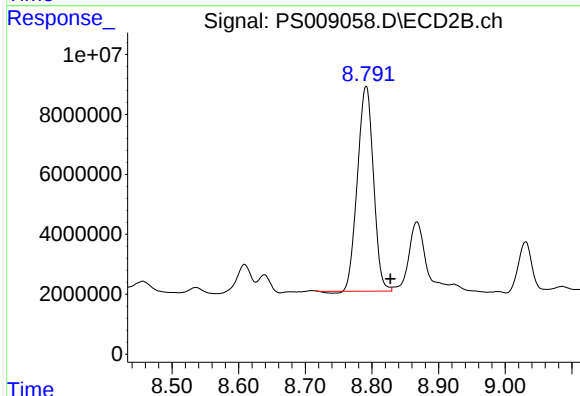


#11 2,4,5-TP (SILVEX)

R.T.: 8.791 min
Delta R.T.: -0.037 min
Response: 113835087
Conc: 21.01 ng/ml

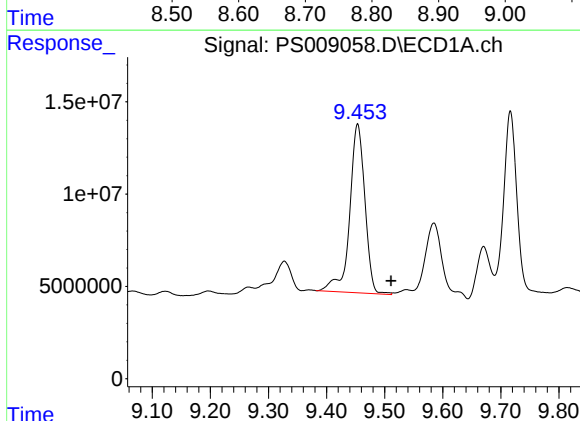


#12 2,4,5-T

R.T.: 9.454 min
Delta R.T.: -0.058 min
Response: 166313691
Conc: 15.55 ng/ml

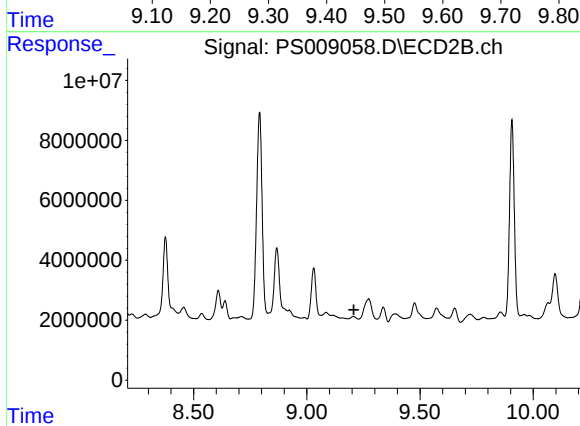

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.208 min
Response: 0
Conc: N.D.

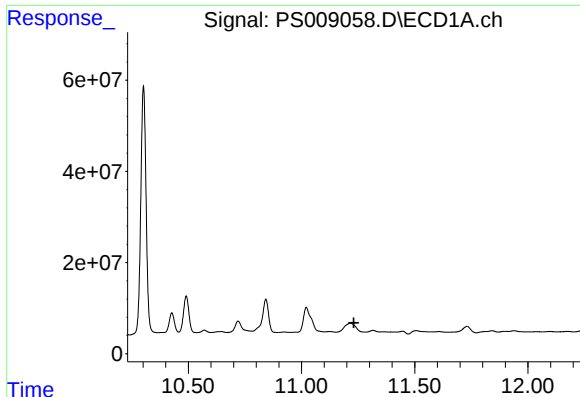

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

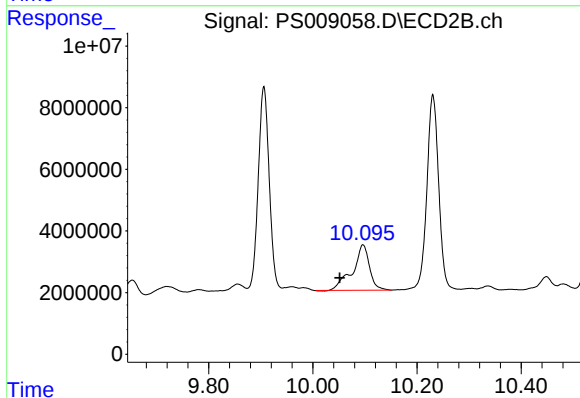


#14 DINOSEB

R.T.: 10.096 min
Delta R.T.: 0.045 min
Response: 33394064
Conc: 8.45 ng/ml

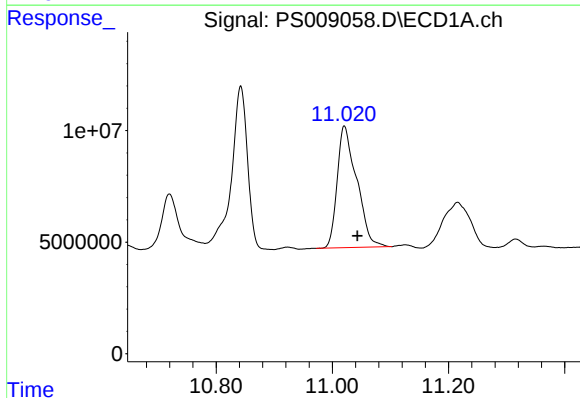


#15 Picloram

R.T.: 11.021 min
Delta R.T.: -0.022 min
Response: 126984744
Conc: 9.28 ng/ml

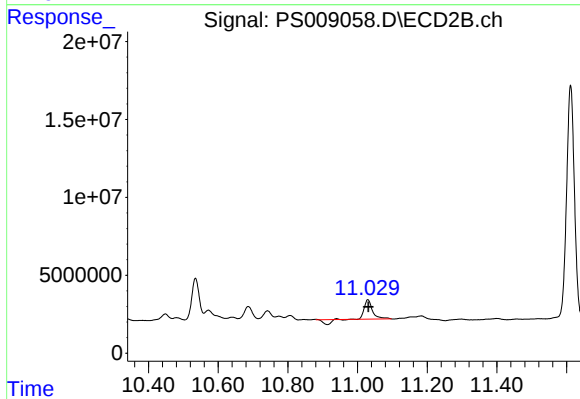

#15 Picloram


R.T.: 11.030 min
Delta R.T.: -0.001 min
Response: 16370038
Conc: 2.25 ng/ml

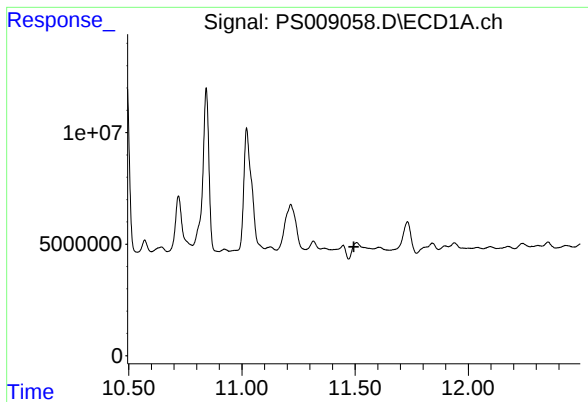

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

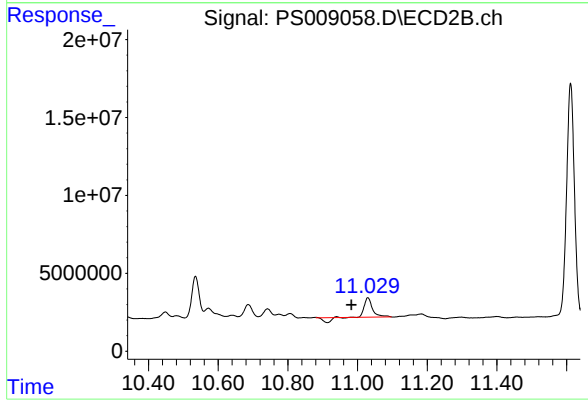

#16 DCPA

R.T.: 11.030 min
Delta R.T.: 0.047 min
Response: 16370038
Conc: 2.37 ng/ml