

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
 Data File : PS009061.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2020 19:46
 Operator : DD\AJ
 Sample : L1373-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 29 00:13:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.939	736.6E6	355.5E6	336.883	368.994
Target Compounds							
1) T	Dalapon	0.000	2.590	0 50648018		N.D.	34.638
2) T	3,5-DICHL...	0.000	6.114	0 129.4E6		N.D.	88.709
5) T	DICAMBA	0.000	7.073	0 28614840		N.D.	6.913
7) T	MCPA	7.693	0.000	102.0E6	0	12.686	N.D. #
8) T	DICHLORPROP	0.000	7.760	0 31363182		N.D.	31.303
10) T	Pentachlo...	0.000	8.463	0 15703440		N.D.	1.105
11) T	2,4,5-TP ...	0.000	8.798	0 201.8E6		N.D.	37.263
12) T	2,4,5-T	9.454	0.000	130.7E6	0	12.228	N.D. #
14) T	DINOSEB	0.000	10.095	0 72224474		N.D.	18.266
15) T	Picloram	11.022	11.030	119.9E6	18649512	8.756	2.566 #
16) T	DCPA	0.000	11.030	0 18649512		N.D.	2.695



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
Data File : PS009061.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2020 19:46
Operator : DD\AJ
Sample : L1373-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 29 00:13:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

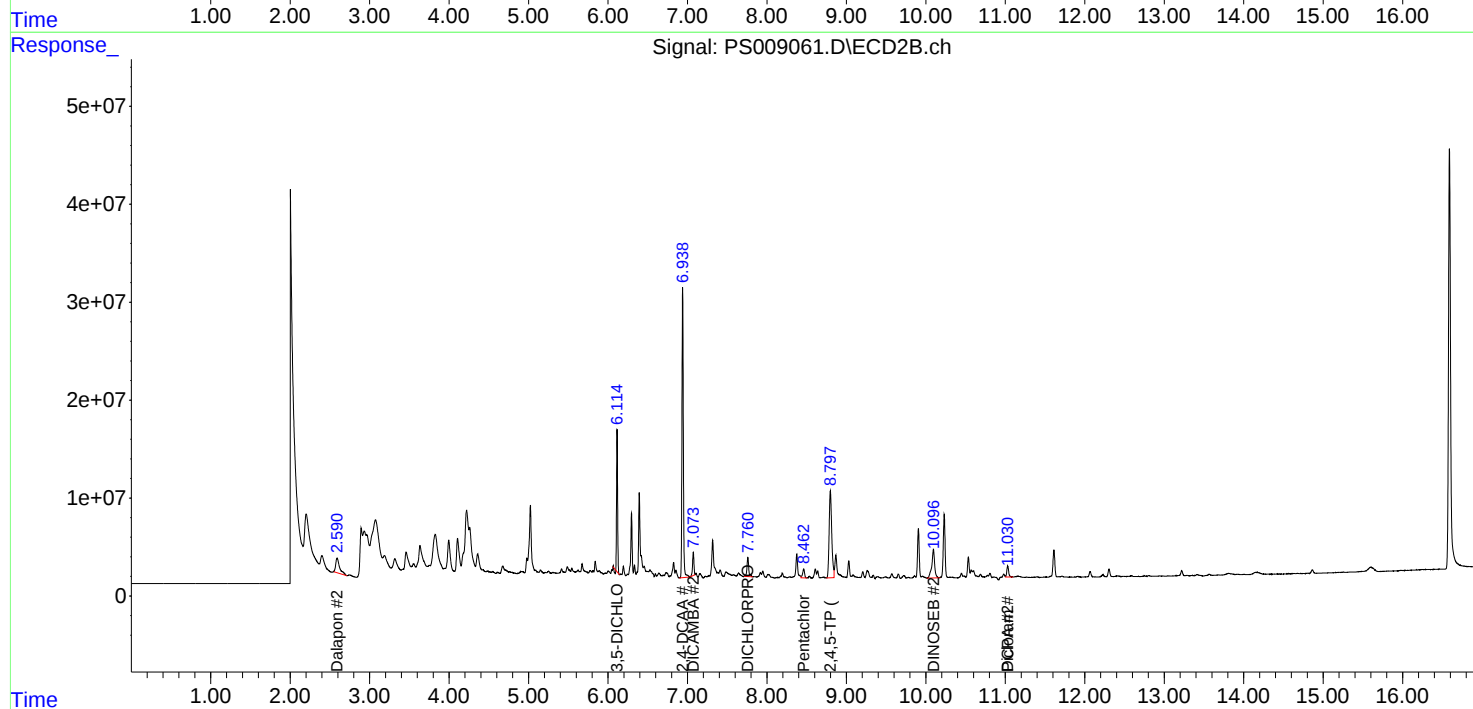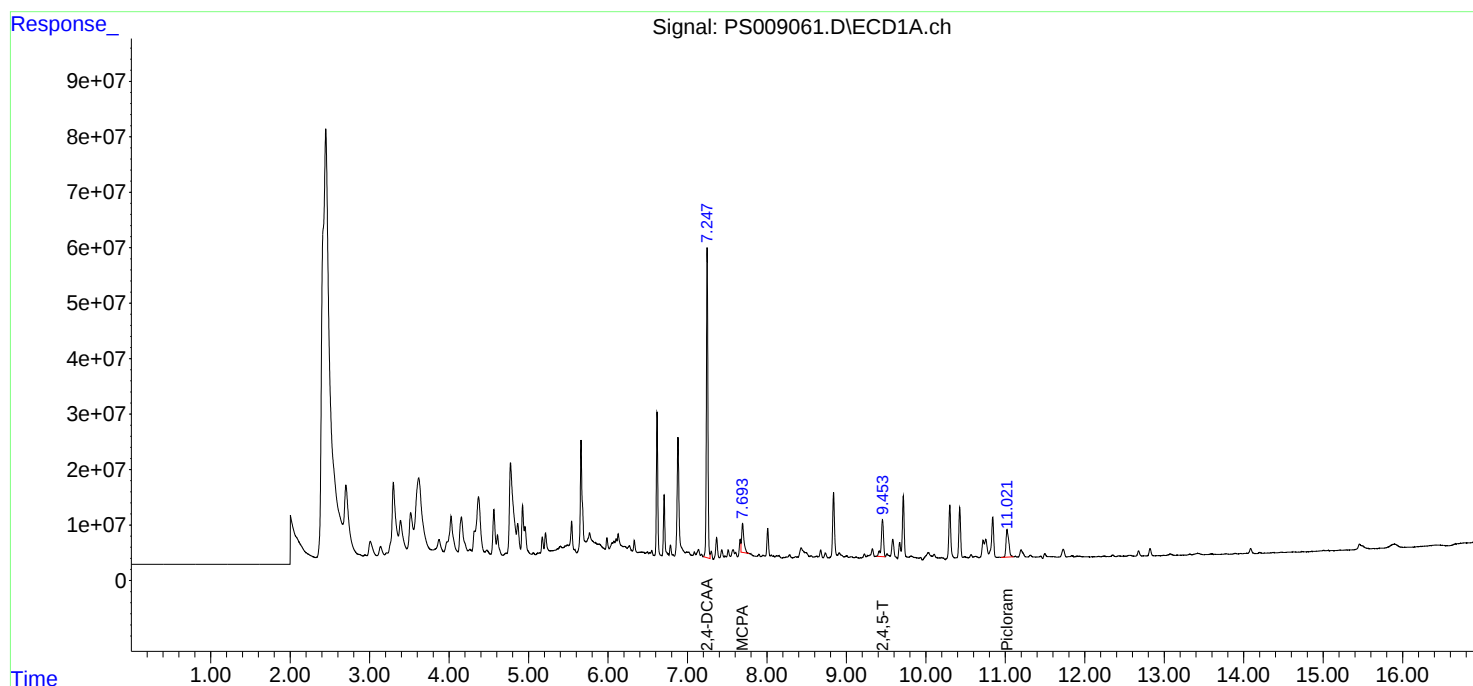


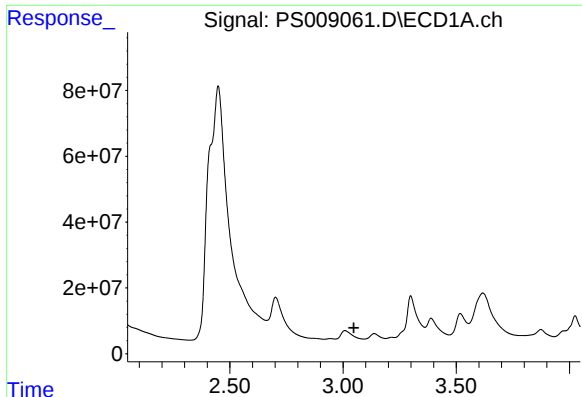

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

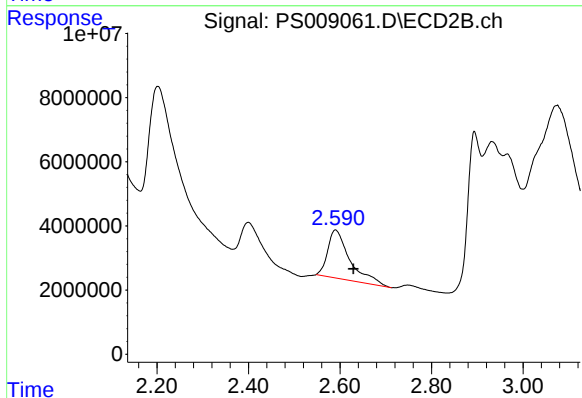


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.040 min
Response: 50648018
Conc: 34.64 ng/ml

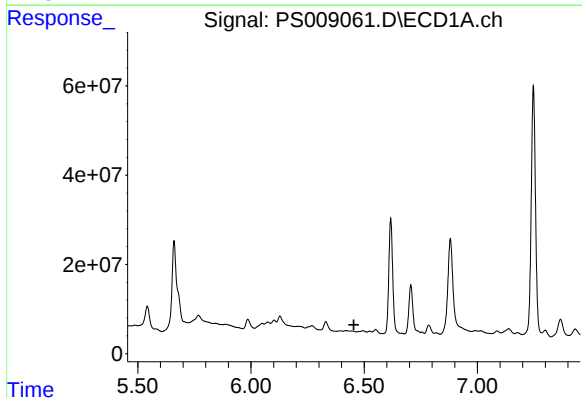


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

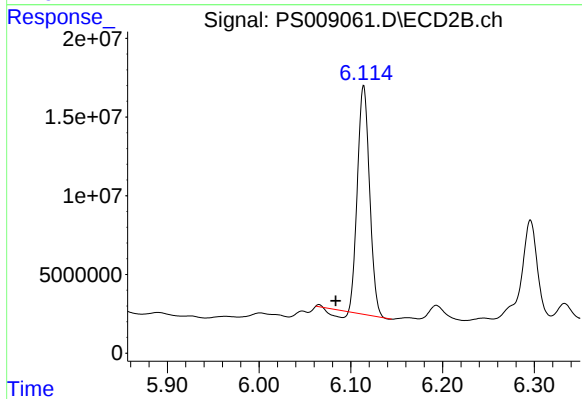

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.031 min
Response: 129449714
Conc: 88.71 ng/ml

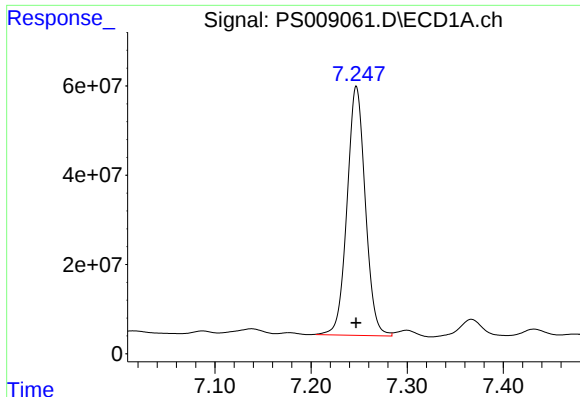

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 736625713
Conc: 336.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

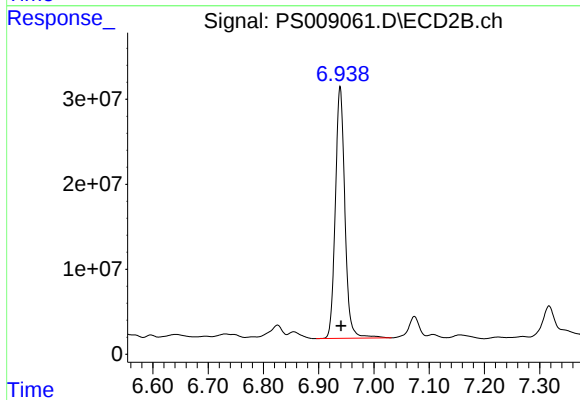


#4 2,4-DCAA

R.T.: 6.939 min
Delta R.T.: -0.002 min
Response: 355545888
Conc: 368.99 ng/ml

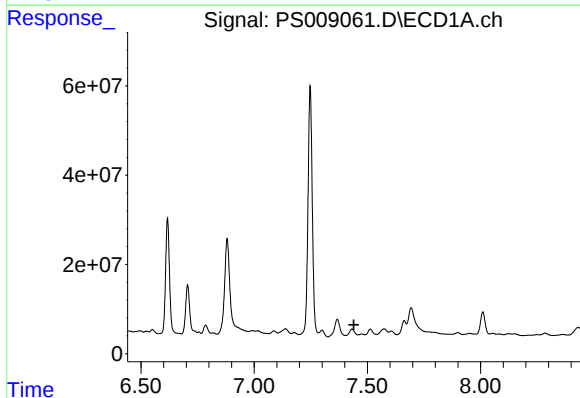


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.

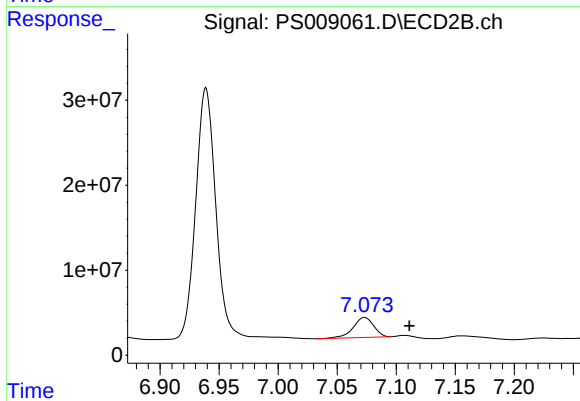

#5 DICAMBA


R.T.: 7.073 min
Delta R.T.: -0.038 min
Response: 28614840
Conc: 6.91 ng/ml

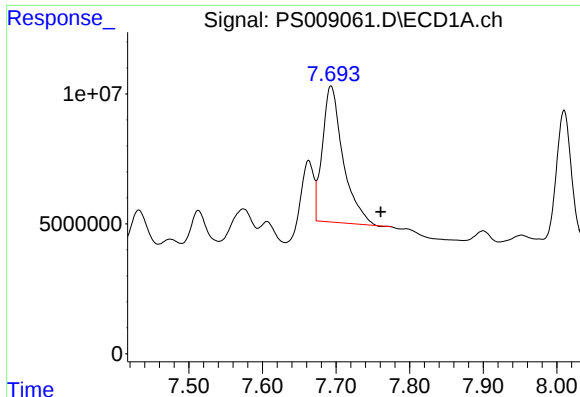

#7 MCPA


R.T.: 7.693 min
Delta R.T.: -0.067 min
Response: 102044287
Conc: 12.69 ug/ml

Instrument :
ECD_S
ClientSampleId :

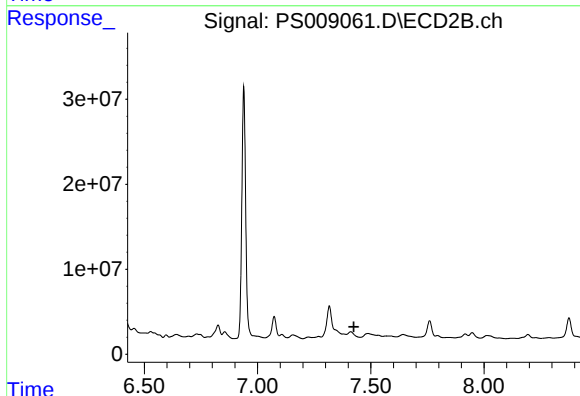


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.425 min
Response: 0
Conc: N.D.

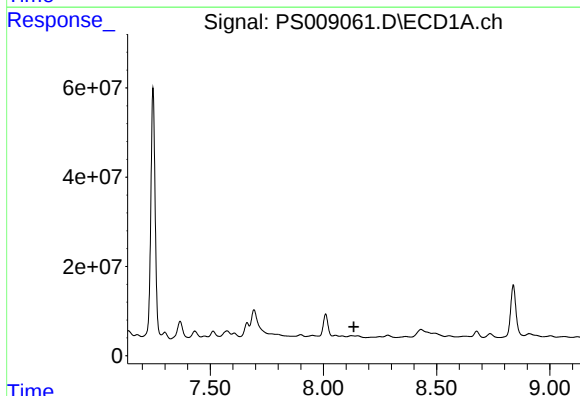


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

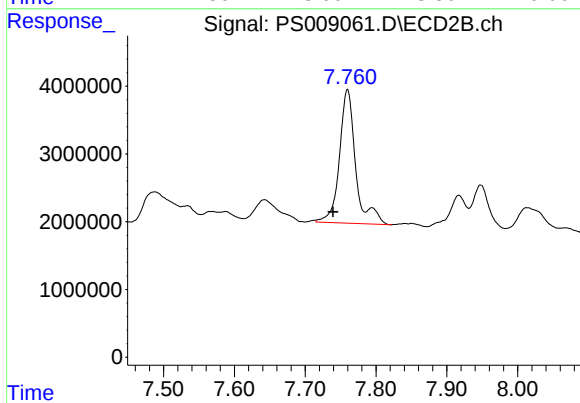

#8 DICHLORPROP


R.T.: 7.760 min
Delta R.T.: 0.021 min
Response: 31363182
Conc: 31.30 ng/ml

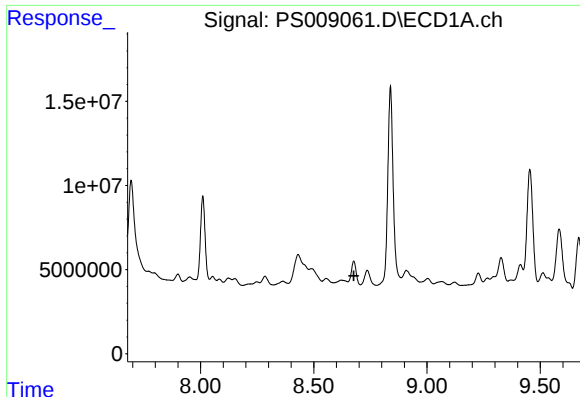

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.677 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

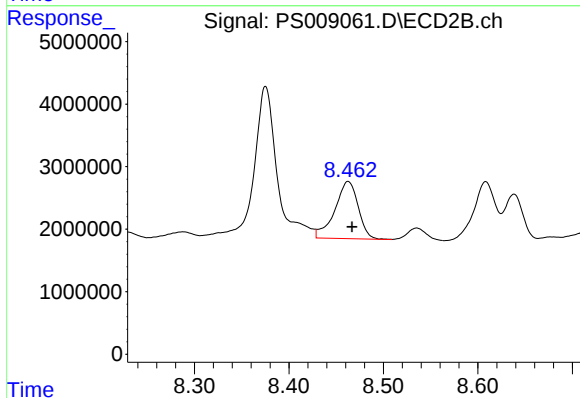


#10 Pentachlorophenol

R.T.: 8.463 min
Delta R.T.: -0.004 min
Response: 15703440
Conc: 1.11 ng/ml

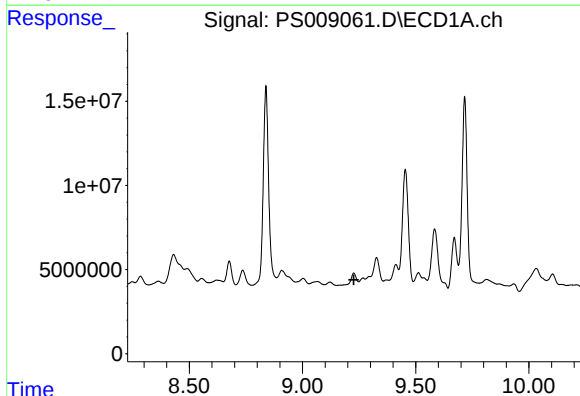


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

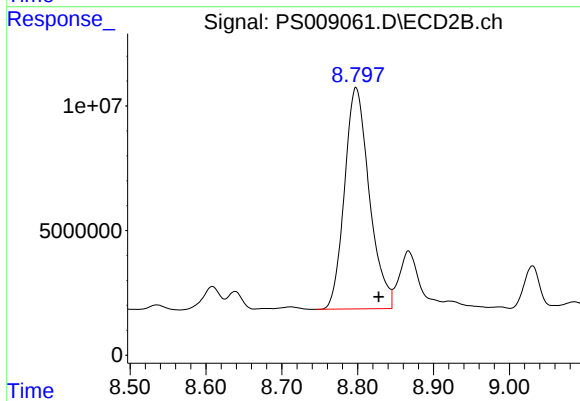

#11 2,4,5-TP (SILVEX)


R.T.: 8.798 min
Delta R.T.: -0.030 min
Response: 201847945
Conc: 37.26 ng/ml

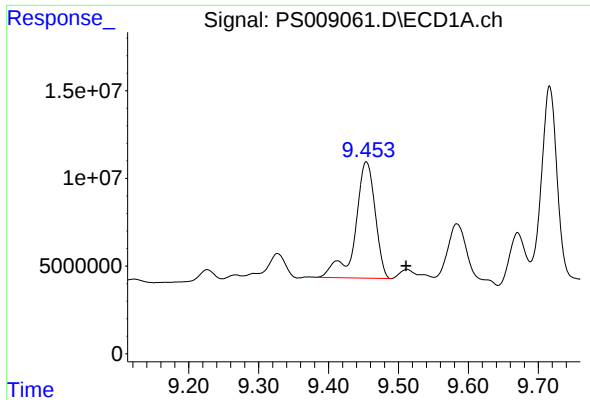

#12 2,4,5-T


R.T.: 9.454 min
Delta R.T.: -0.057 min
Response: 130737407
Conc: 12.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

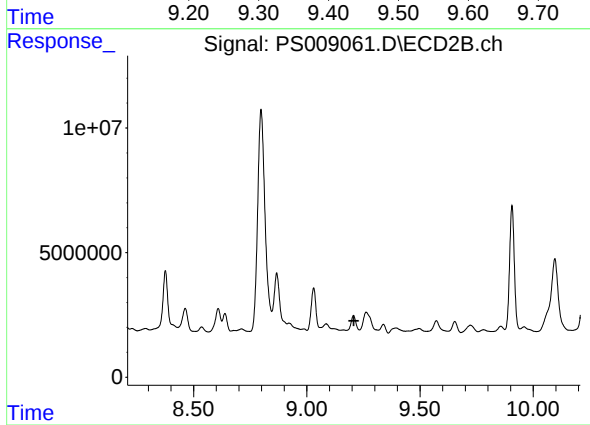


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.208 min
Response: 0
Conc: N.D.

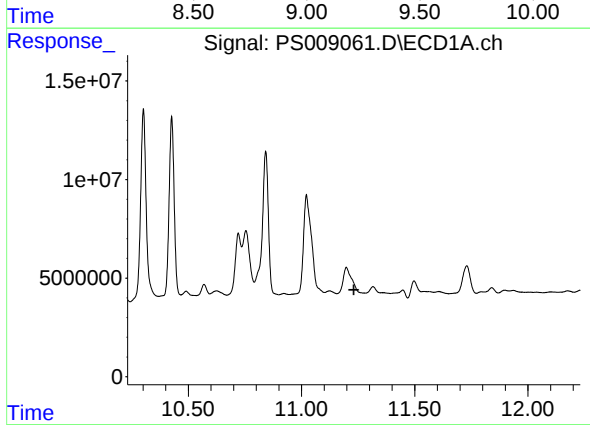


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

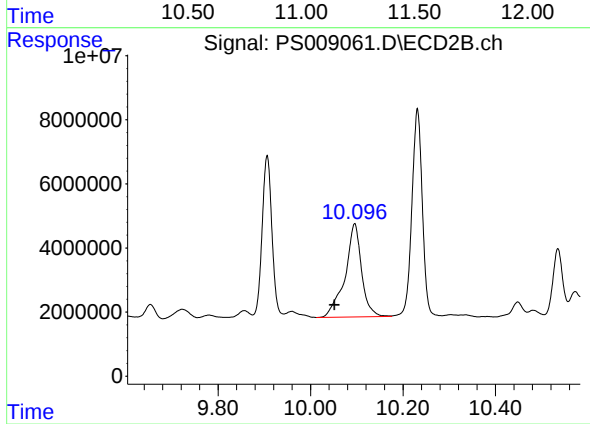

#14 DINOSEB


R.T.: 10.095 min
Delta R.T.: 0.044 min
Response: 72224474
Conc: 18.27 ng/ml

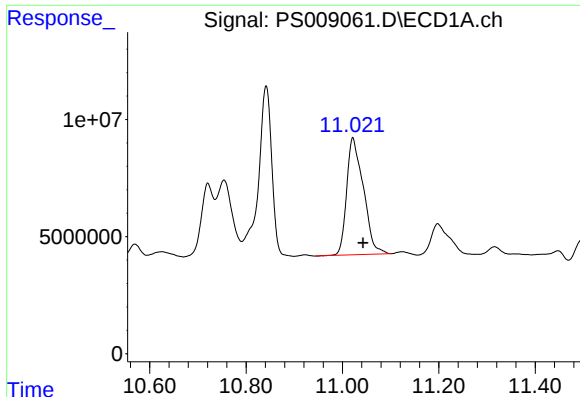

#15 Picloram


R.T.: 11.022 min
Delta R.T.: -0.021 min
Response: 119876041
Conc: 8.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

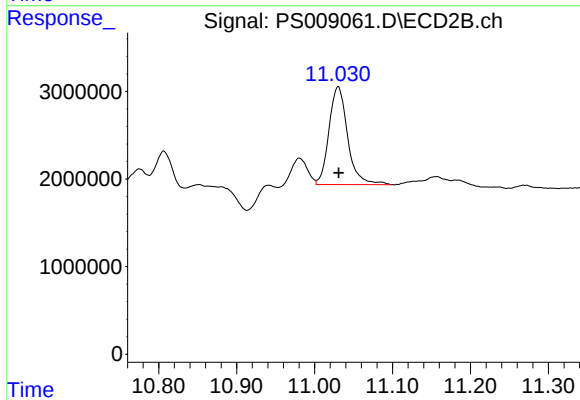


#15 Picloram

R.T.: 11.030 min
Delta R.T.: 0.000 min
Response: 18649512
Conc: 2.57 ng/ml

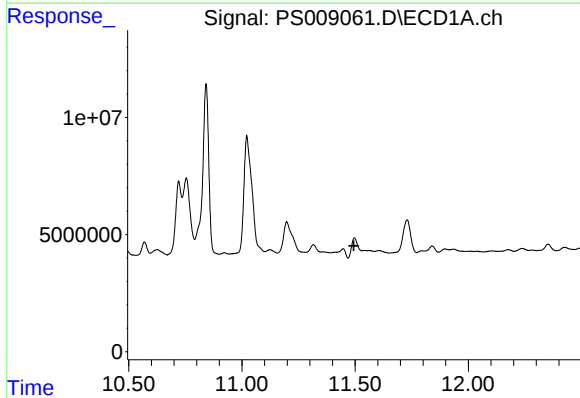

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.

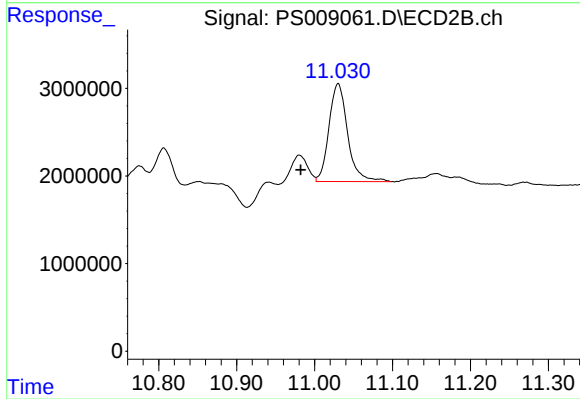

#16 DCPA

R.T.: 11.030 min
Delta R.T.: 0.048 min
Response: 18649512
Conc: 2.70 ng/ml