

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
 Data File : PS009067.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2020 22:03
 Operator : DD\AJ
 Sample : L1718-12
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 29 00:15:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.939	657.4E6	334.0E6	300.650	346.616
Target Compounds							
1) T	Dalapon	0.000	2.590	0	32118450	N.D.	21.966
2) T	3,5-DICHL...	0.000	6.114	0	140.1E6	N.D.	96.031
5) T	DICAMBA	0.000	7.073	0	35170189	N.D.	8.497
7) T	MCPA	7.692	0.000	74029615	0	9.203	N.D. #
8) T	DICHLORPROP	0.000	7.759	0	33349367	N.D.	33.285
10) T	Pentachlo...	0.000	8.464	0	30788886	N.D.	2.167
11) T	2,4,5-TP ...	0.000	8.793	0	120.8E6	N.D.	22.292
12) T	2,4,5-T	9.453	9.207	111.8E6	16455868	10.457	3.040 #
14) T	DINOSEB	0.000	10.096	0	54258179	N.D.	13.722
15) T	Picloram	11.044	11.030	458.8E6	218.4E6	33.510	30.057
16) T	DCPA	0.000	10.980	0	22562210	N.D.	3.261



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
Data File : PS009067.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2020 22:03
Operator : DD\AJ
Sample : L1718-12
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 29 00:15:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

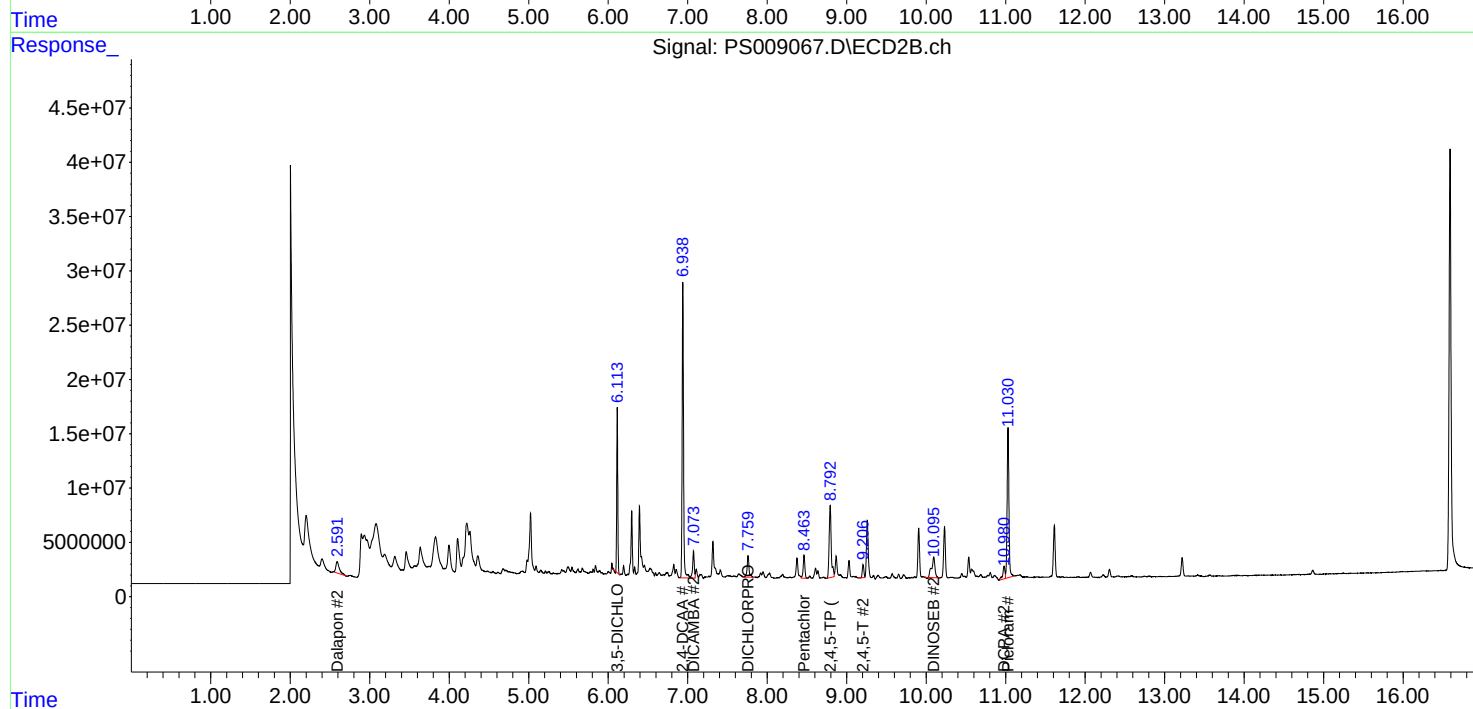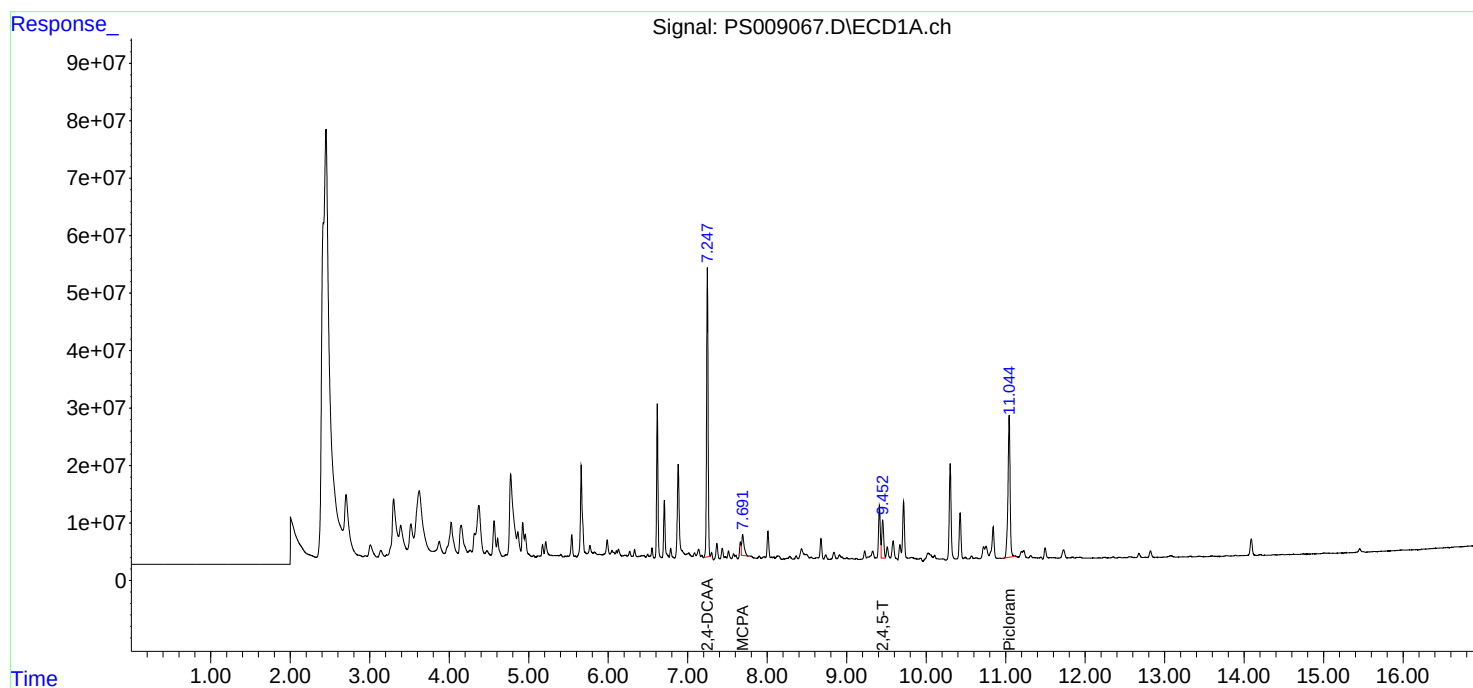


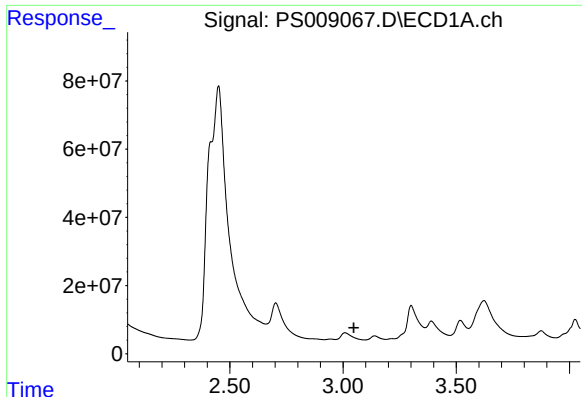

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

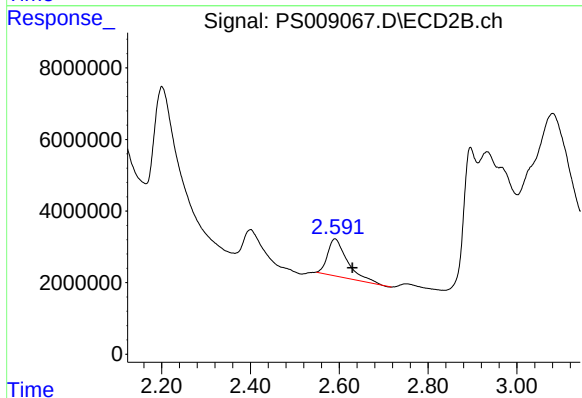


#1 Dalapon

R.T.: 2.590 min
Delta R.T.: -0.040 min
Response: 32118450
Conc: 21.97 ng/ml

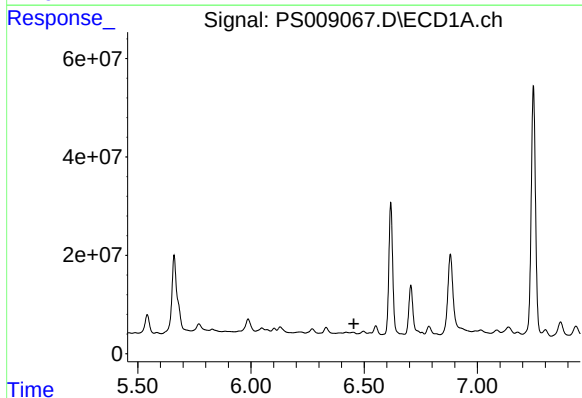


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

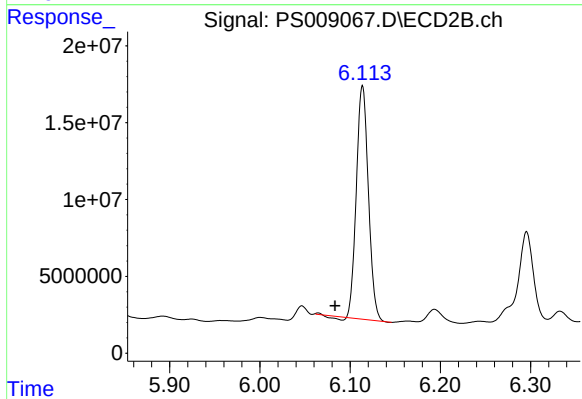

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.030 min
Response: 140134852
Conc: 96.03 ng/ml

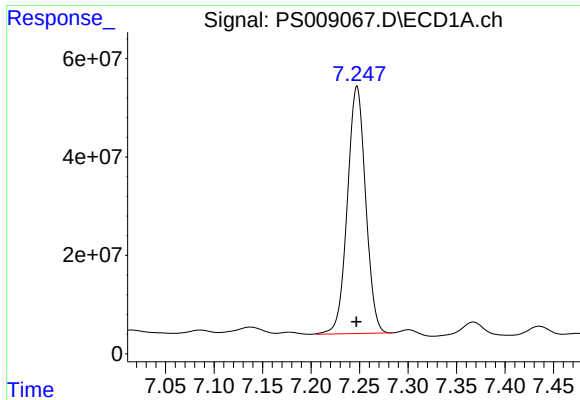

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 657399542
Conc: 300.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

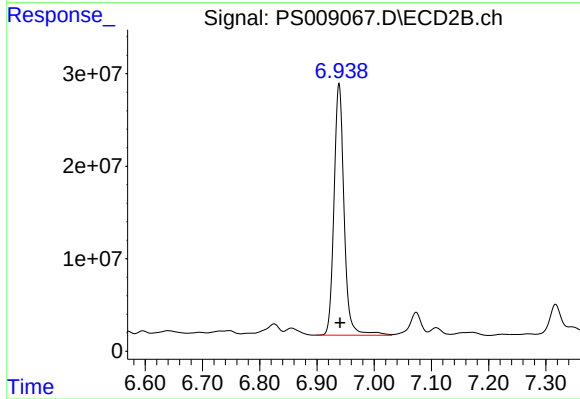


#4 2,4-DCAA

R.T.: 6.939 min
Delta R.T.: -0.002 min
Response: 333984138
Conc: 346.62 ng/ml

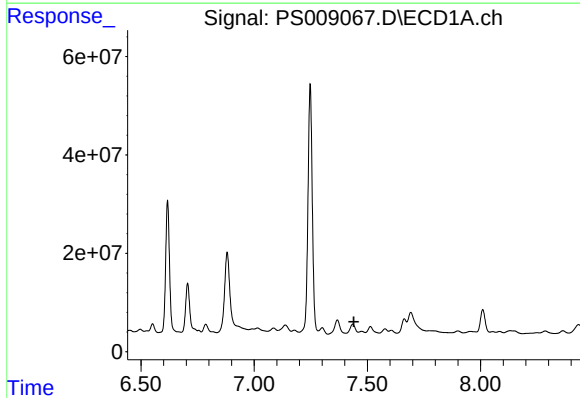


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.

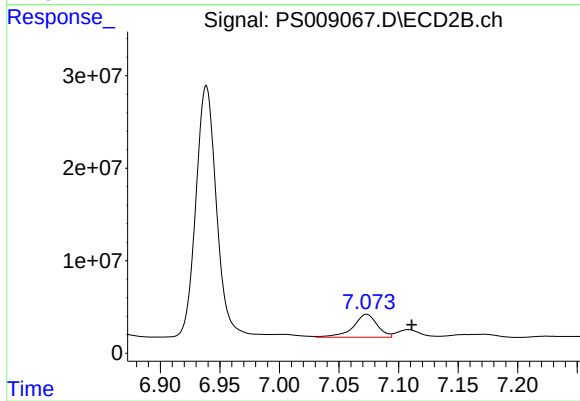

#5 DICAMBA


R.T.: 7.073 min
Delta R.T.: -0.038 min
Response: 35170189
Conc: 8.50 ng/ml

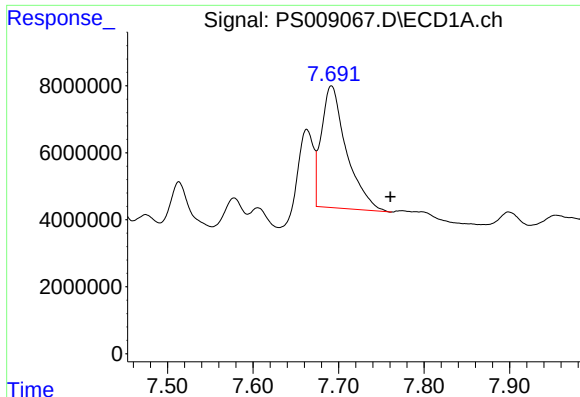

#7 MCPA


R.T.: 7.692 min
Delta R.T.: -0.069 min
Response: 74029615
Conc: 9.20 ug/ml

Instrument :
ECD_S
ClientSampleId :

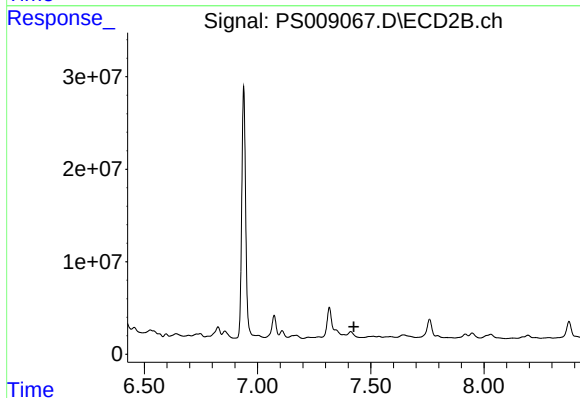


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.425 min
Response: 0
Conc: N.D.

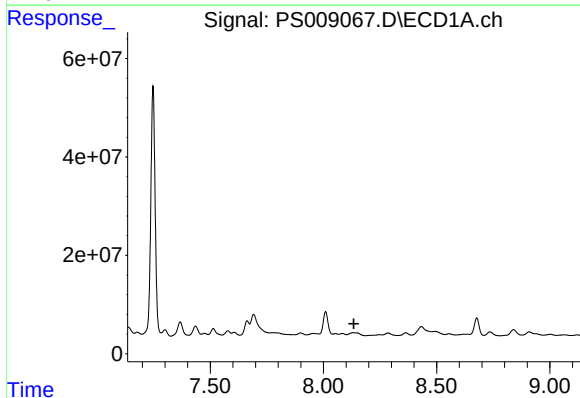


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

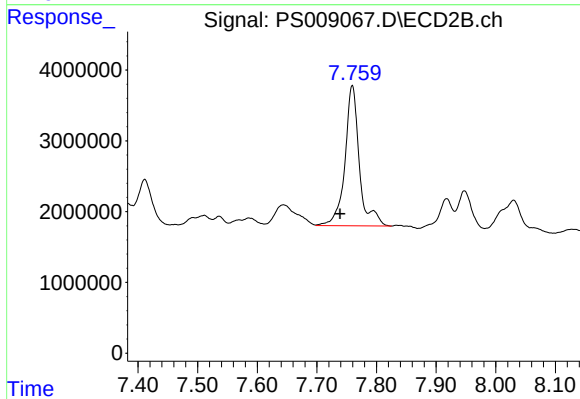

#8 DICHLORPROP


R.T.: 7.759 min
Delta R.T.: 0.020 min
Response: 33349367
Conc: 33.29 ng/ml

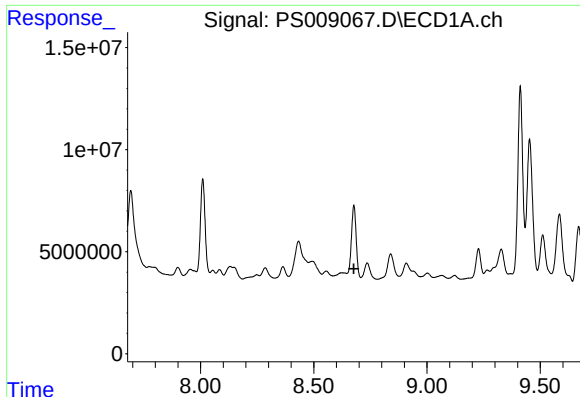

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.677 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

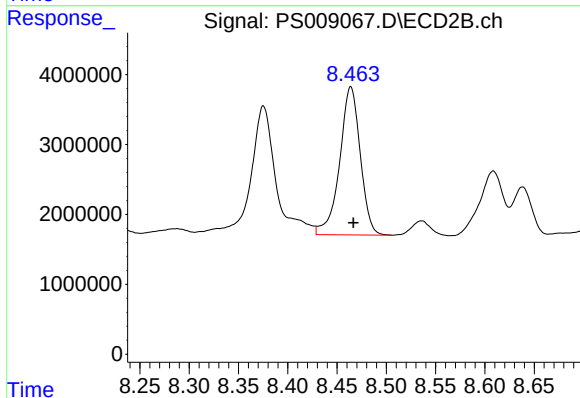


#10 Pentachlorophenol

R.T.: 8.464 min
Delta R.T.: -0.003 min
Response: 3078886
Conc: 2.17 ng/ml

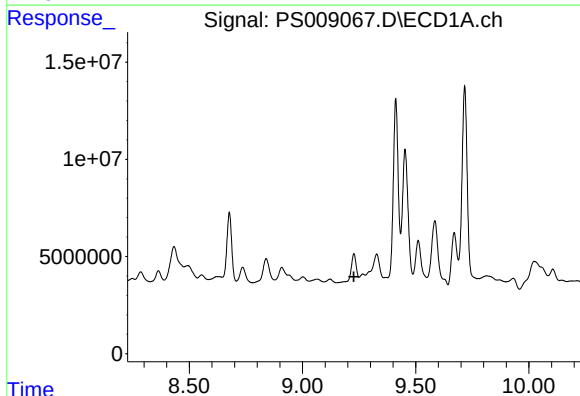


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

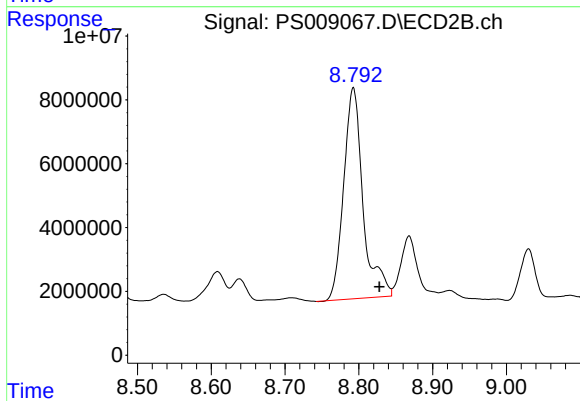

#11 2,4,5-TP (SILVEX)


R.T.: 8.793 min
Delta R.T.: -0.035 min
Response: 120756409
Conc: 22.29 ng/ml

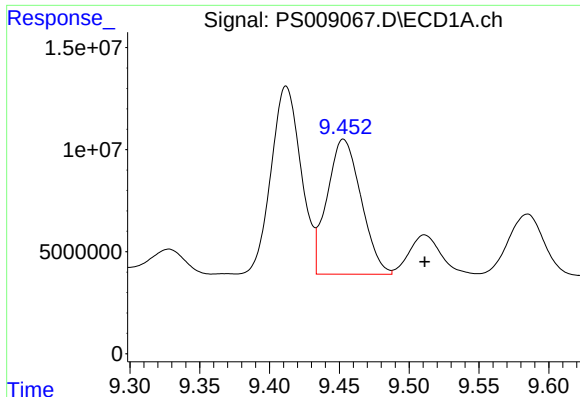

#12 2,4,5-T


R.T.: 9.453 min
Delta R.T.: -0.058 min
Response: 111807234
Conc: 10.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

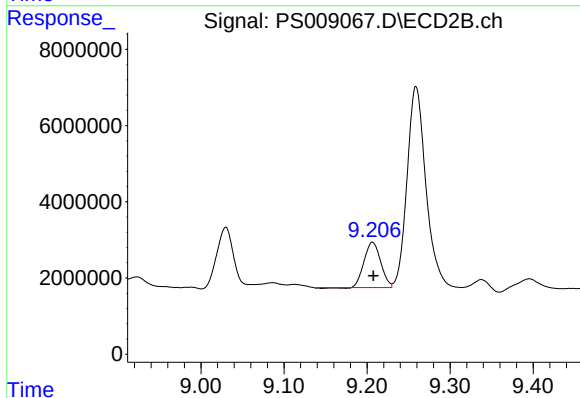


#12 2,4,5-T

R.T.: 9.207 min
Delta R.T.: -0.001 min
Response: 16455868
Conc: 3.04 ng/ml

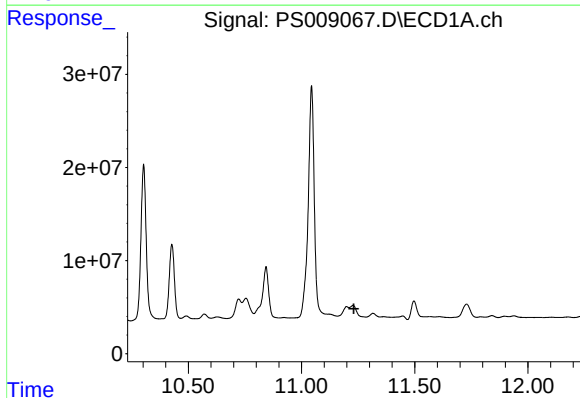


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.231 min
Response: 0
Conc: N.D.

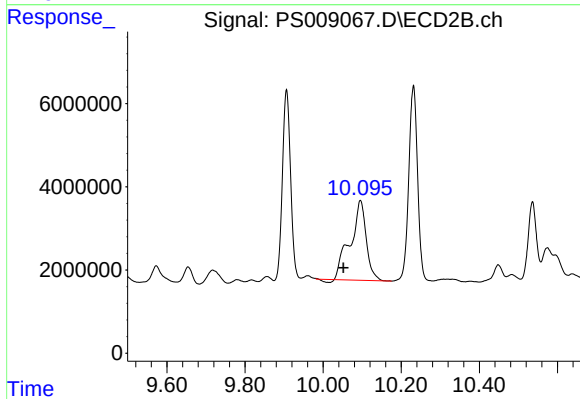

#14 DINOSEB


R.T.: 10.096 min
Delta R.T.: 0.044 min
Response: 54258179
Conc: 13.72 ng/ml

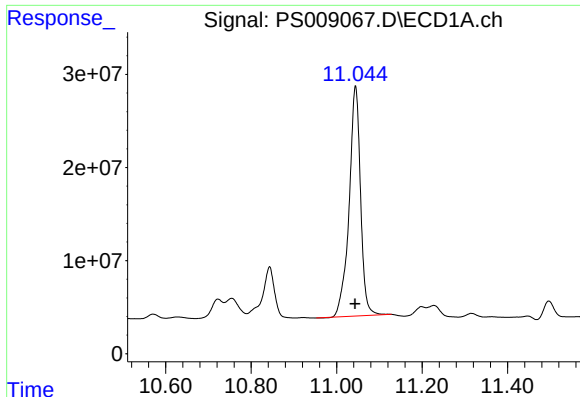

#15 Picloram


R.T.: 11.044 min
Delta R.T.: 0.001 min
Response: 458784403
Conc: 33.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

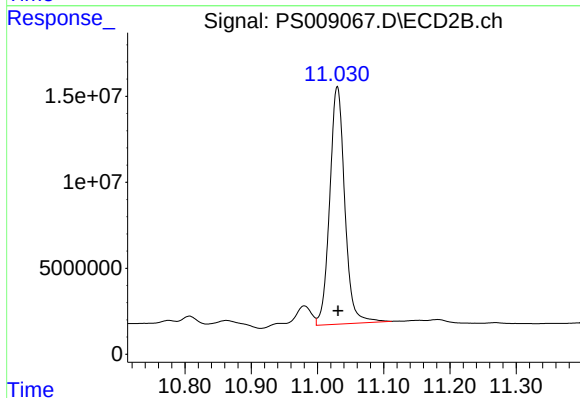


#15 Picloram

R.T.: 11.030 min
Delta R.T.: -0.001 min
Response: 218410126
Conc: 30.06 ng/ml

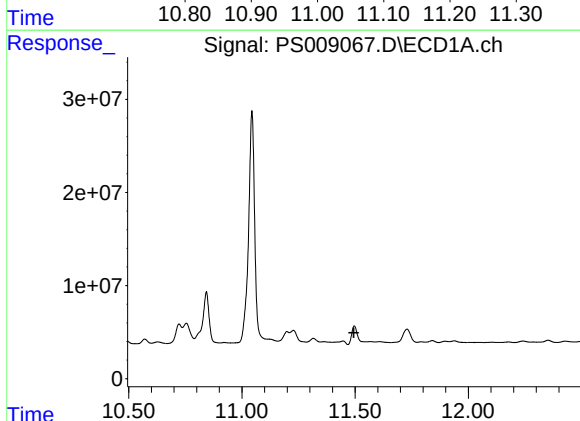

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.

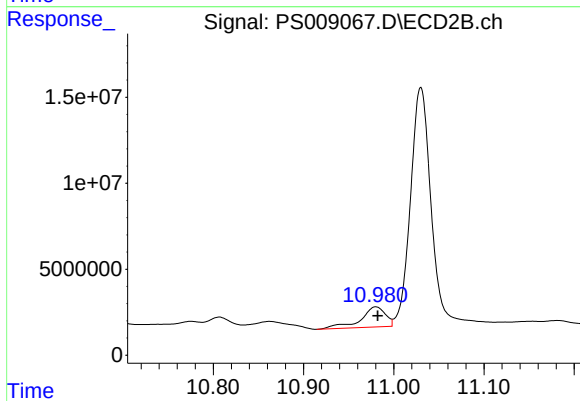

#16 DCPA

R.T.: 10.980 min
Delta R.T.: -0.002 min
Response: 22562210
Conc: 3.26 ng/ml