

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
 Data File : PS009068.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2020 22:26
 Operator : DD\AJ
 Sample : L1719-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 29 00:15:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.939	787.6E6	389.3E6	360.203	404.066
Target Compounds							
1) T	Dalapon	0.000	2.591	0	39583615	N.D.	27.071
2) T	3,5-DICHL...	0.000	6.114	0	141.0E6	N.D.	96.651
5) T	DICAMBA	0.000	7.073	0	37694066	N.D.	9.106
7) T	MCPA	7.691	0.000	148.5E6	0	18.462	N.D. #
8) T	DICHLORPROP	0.000	7.759	0	33631857	N.D.	33.567
11) T	2,4,5-TP ...	0.000	8.792	0	125.5E6	N.D.	23.170
12) T	2,4,5-T	9.454	0.000	131.8E6	0	12.324	N.D. #
14) T	DINOSEB	0.000	10.095	0	64524544	N.D.	16.319
15) T	Picloram	11.022	11.030	135.9E6	28571229	9.927	3.932 #
16) T	DCPA	0.000	11.030	0	28571229	N.D.	4.129



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022820\
Data File : PS009068.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2020 22:26
Operator : DD\AJ
Sample : L1719-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 29 00:15:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

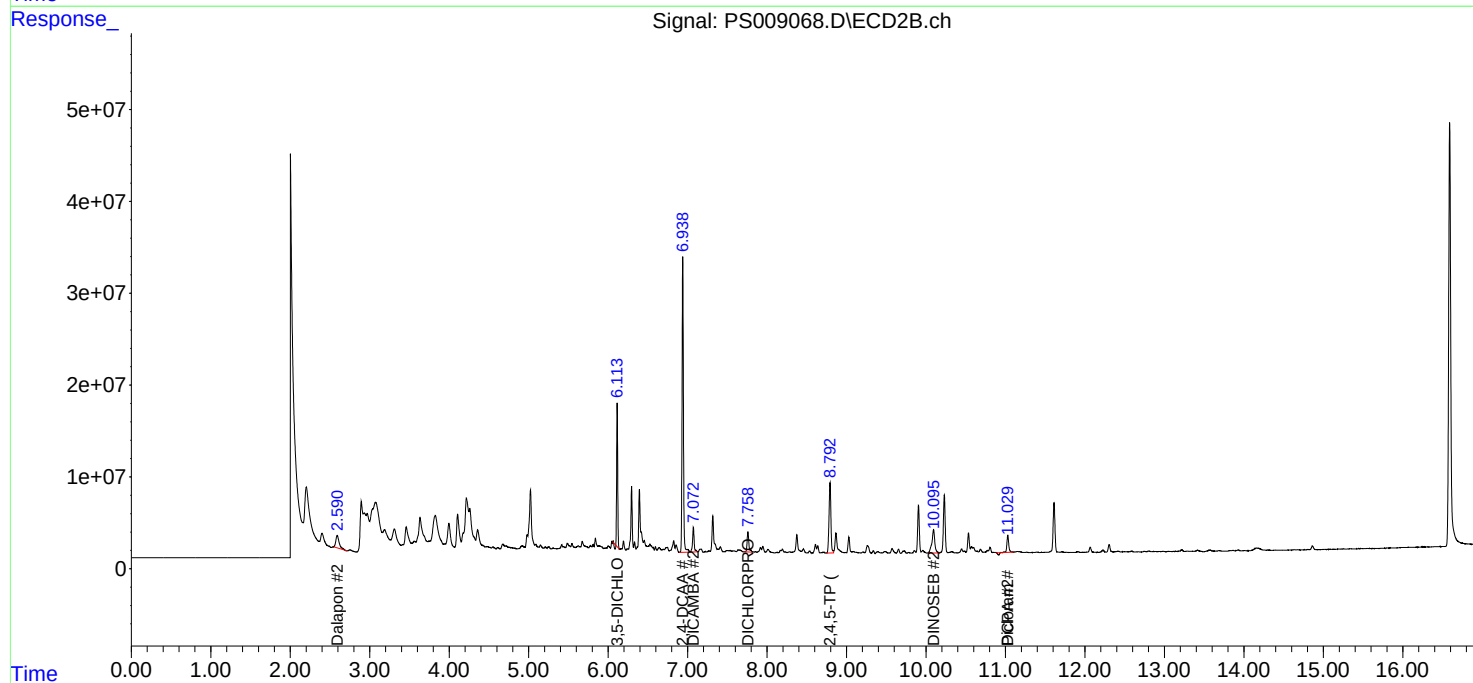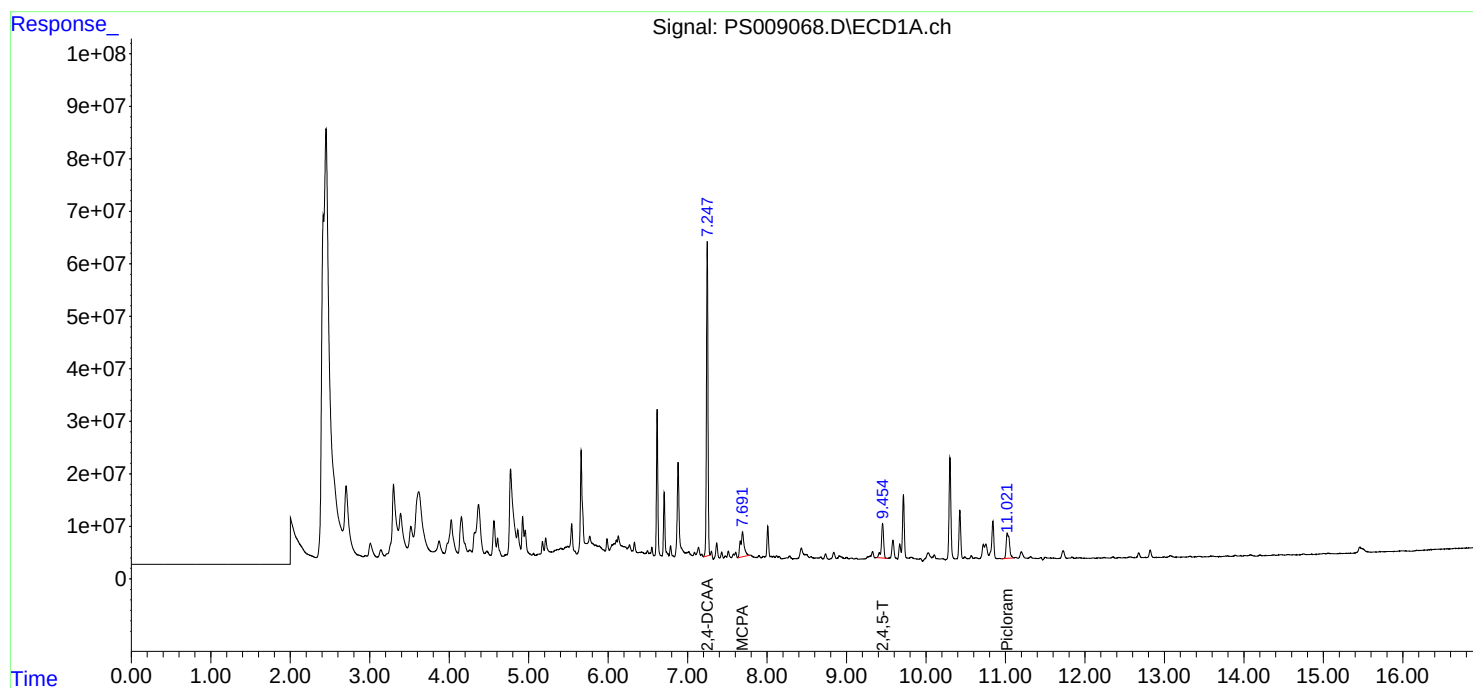


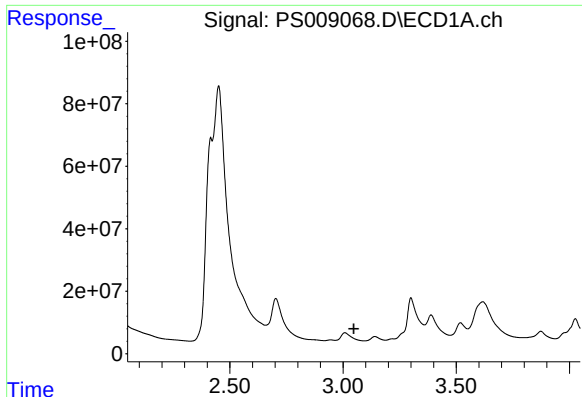

#1 Dalapon


R.T.: 0.000 min
Exp R.T. : 3.048 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

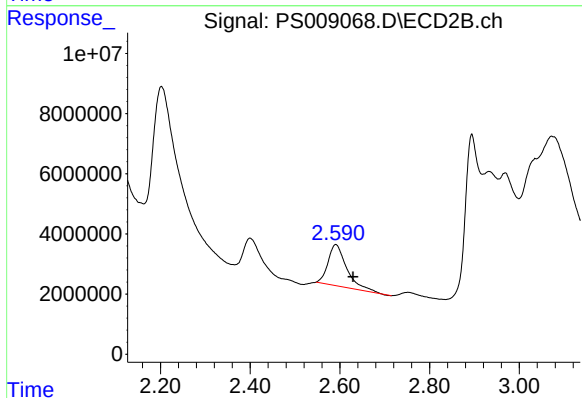


#1 Dalapon

R.T.: 2.591 min
Delta R.T.: -0.039 min
Response: 39583615
Conc: 27.07 ng/ml

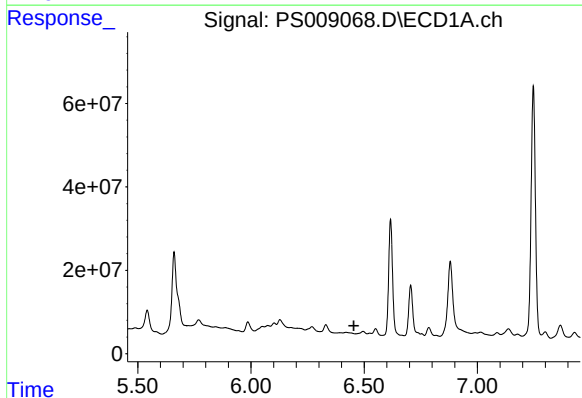


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.455 min
Response: 0
Conc: N.D.

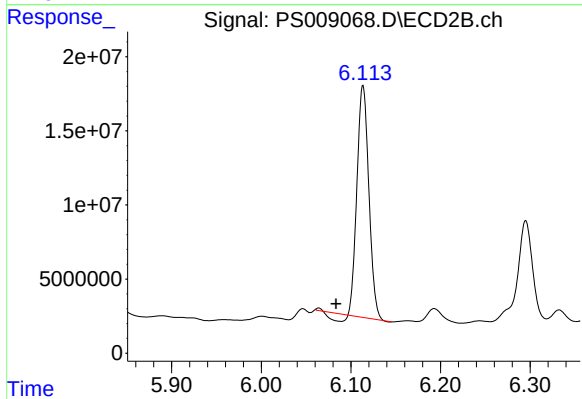

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.114 min
Delta R.T.: 0.030 min
Response: 141039528
Conc: 96.65 ng/ml

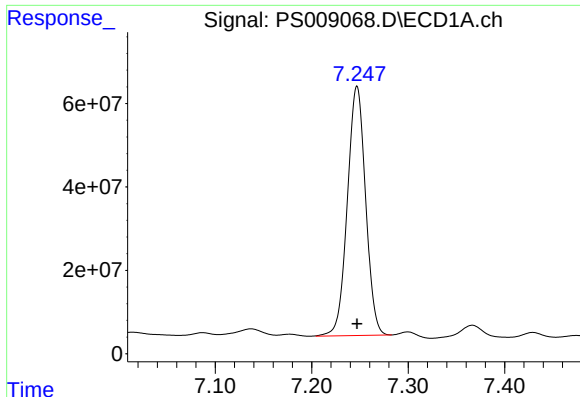

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 787616030
Conc: 360.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

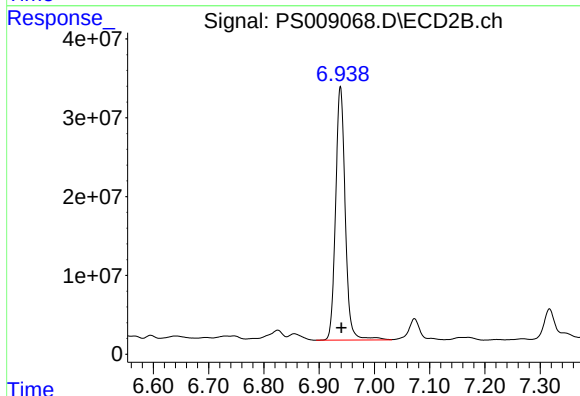


#4 2,4-DCAA

R.T.: 6.939 min
Delta R.T.: -0.002 min
Response: 389340379
Conc: 404.07 ng/ml

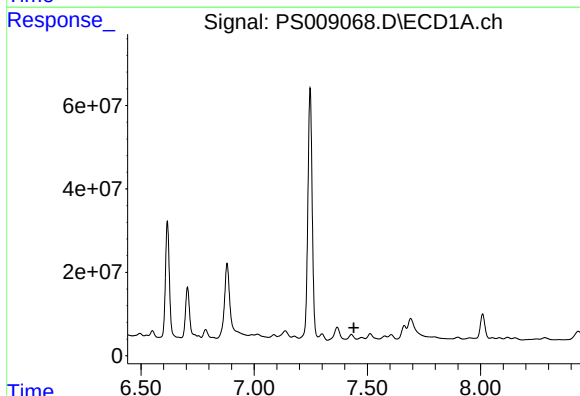


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.

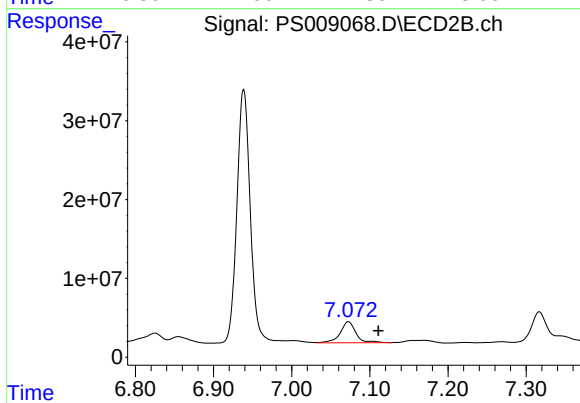

#5 DICAMBA


R.T.: 7.073 min
Delta R.T.: -0.039 min
Response: 37694066
Conc: 9.11 ng/ml

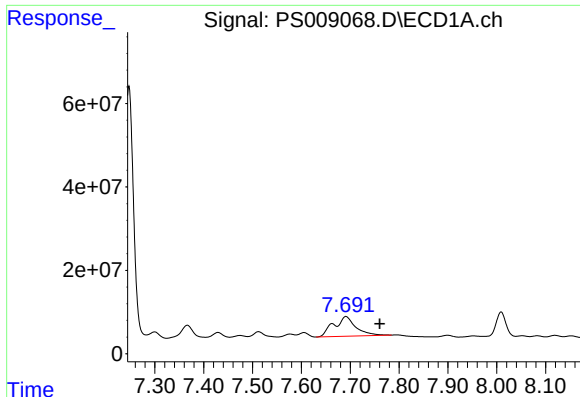

#7 MCPA


R.T.: 7.691 min
Delta R.T.: -0.069 min
Response: 148509281
Conc: 18.46 ug/ml

Instrument :
ECD_S
ClientSampleId :

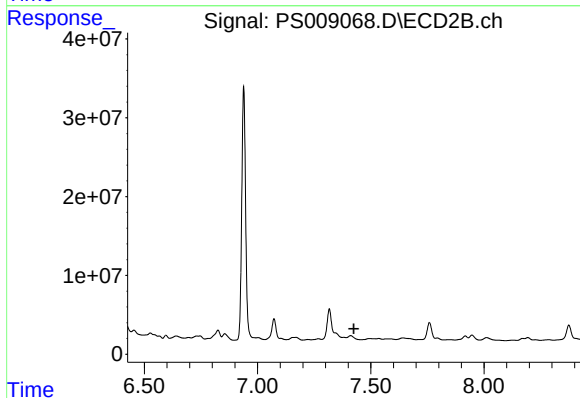


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.425 min
Response: 0
Conc: N.D.

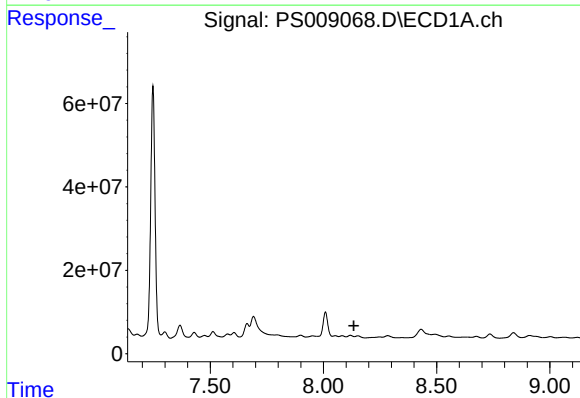


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.135 min
Response: 0
Conc: N.D.

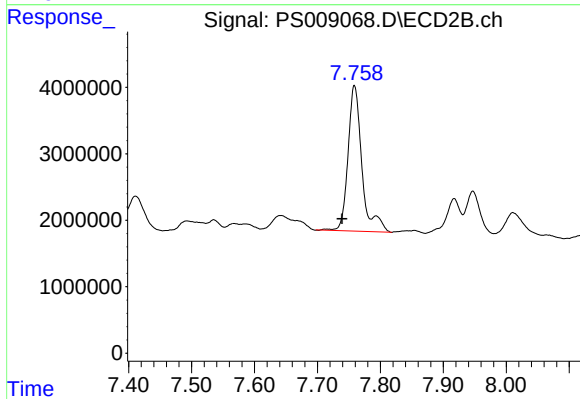

#8 DICHLORPROP


R.T.: 7.759 min
Delta R.T.: 0.020 min
Response: 33631857
Conc: 33.57 ng/ml

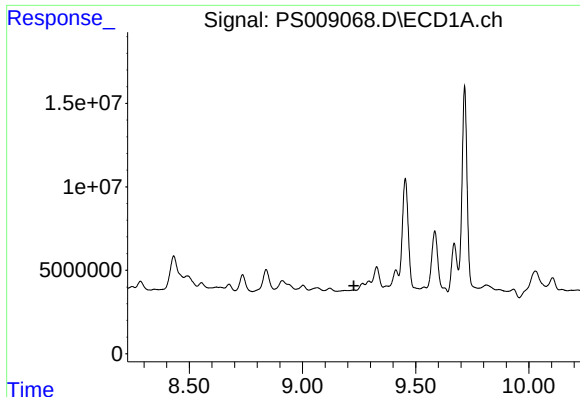

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.227 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

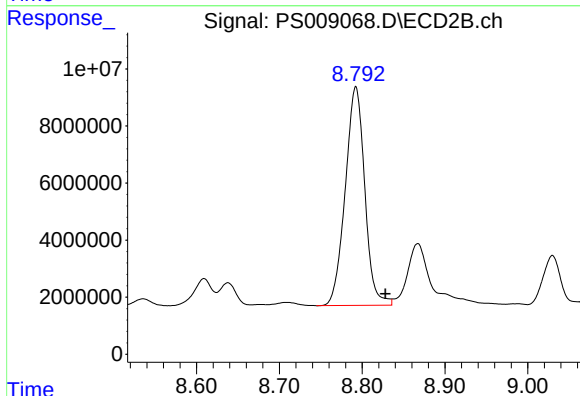


#11 2,4,5-TP (SILVEX)

R.T.: 8.792 min
Delta R.T.: -0.036 min
Response: 125510372
Conc: 23.17 ng/ml

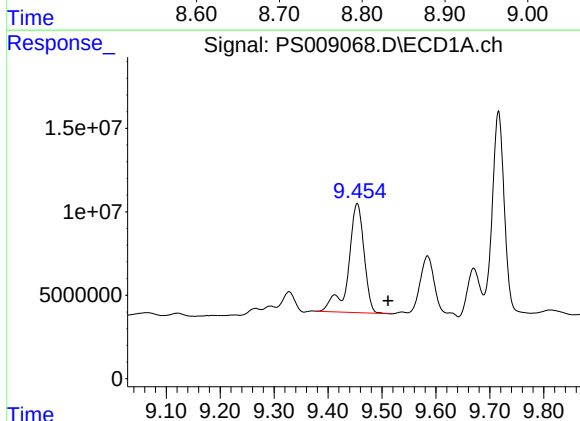


#12 2,4,5-T

R.T.: 9.454 min
Delta R.T.: -0.057 min
Response: 131773266
Conc: 12.32 ng/ml

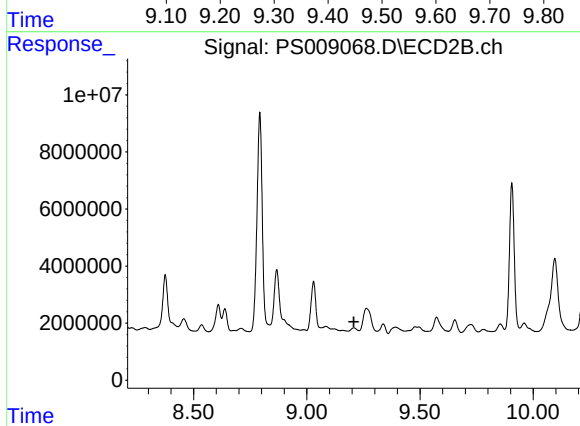

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.208 min
Response: 0
Conc: N.D.

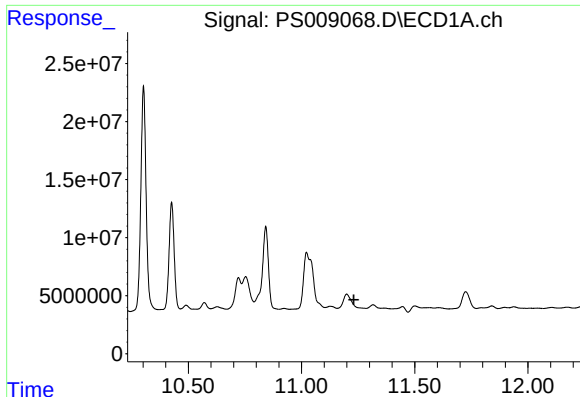

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

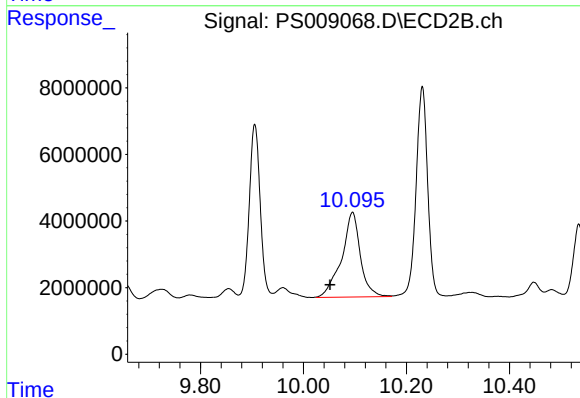


#14 DINOSEB

R.T.: 10.095 min
Delta R.T.: 0.044 min
Response: 64524544
Conc: 16.32 ng/ml

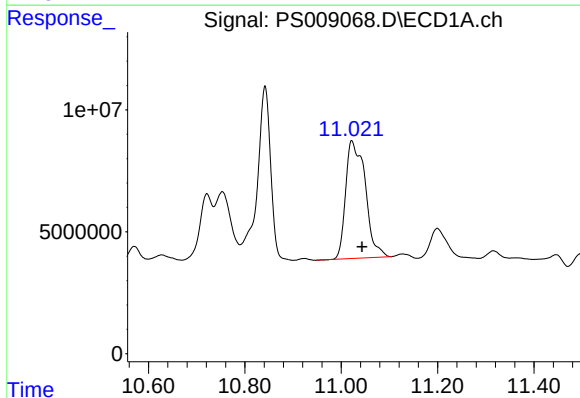


#15 Picloram

R.T.: 11.022 min
Delta R.T.: -0.021 min
Response: 135914296
Conc: 9.93 ng/ml

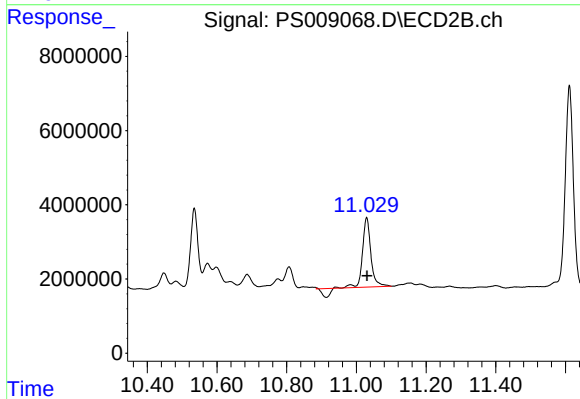

#15 Picloram


R.T.: 11.030 min
Delta R.T.: -0.002 min
Response: 28571229
Conc: 3.93 ng/ml

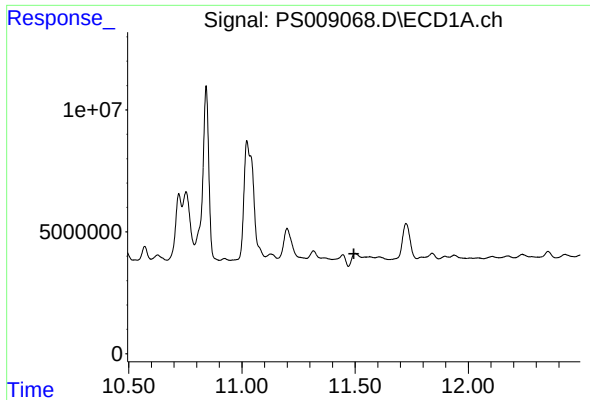

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

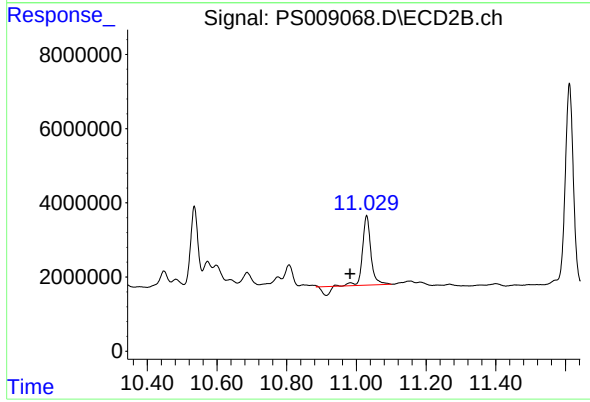

#16 DCPA

R.T.: 11.030 min
Delta R.T.: 0.047 min
Response: 28571229
Conc: 4.13 ng/ml