

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022822\
 Data File : PS018452.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2022 10:57
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 00:03:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
5) T	DICAMBA	7.211	6.786	7519336	3548178	1.144 1.264
8) T	DICHLORPROP	7.898	0.000	3039556	0	1.797 N.D. #
9) T	2,4-D	8.134	7.694	6775051	2801561	3.321 2.993
10) T	Pentachlo...	8.419	8.095	19008737	8714878	<MDL <MDL #
11) T	2,4,5-TP ...	8.969	8.458	13363375	6323641	1.404 1.532
12) T	2,4,5-T	9.257	8.841	26548439	12142214	2.639 3.085
13) T	2,4-DB	9.807	9.344	12187934	1960029	7.013 3.628 #
14) T	DINOSEB	10.939	9.656	20472779	5902282	2.635 2.030
15) T	Picloram	10.783	10.647	229.2E6	115.0E6	18.042 19.879
16) T	DCPA	11.207	10.580	21164037	9471155	1.760 1.907



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022822\
Data File : PS018452.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2022 10:57
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 00:03:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

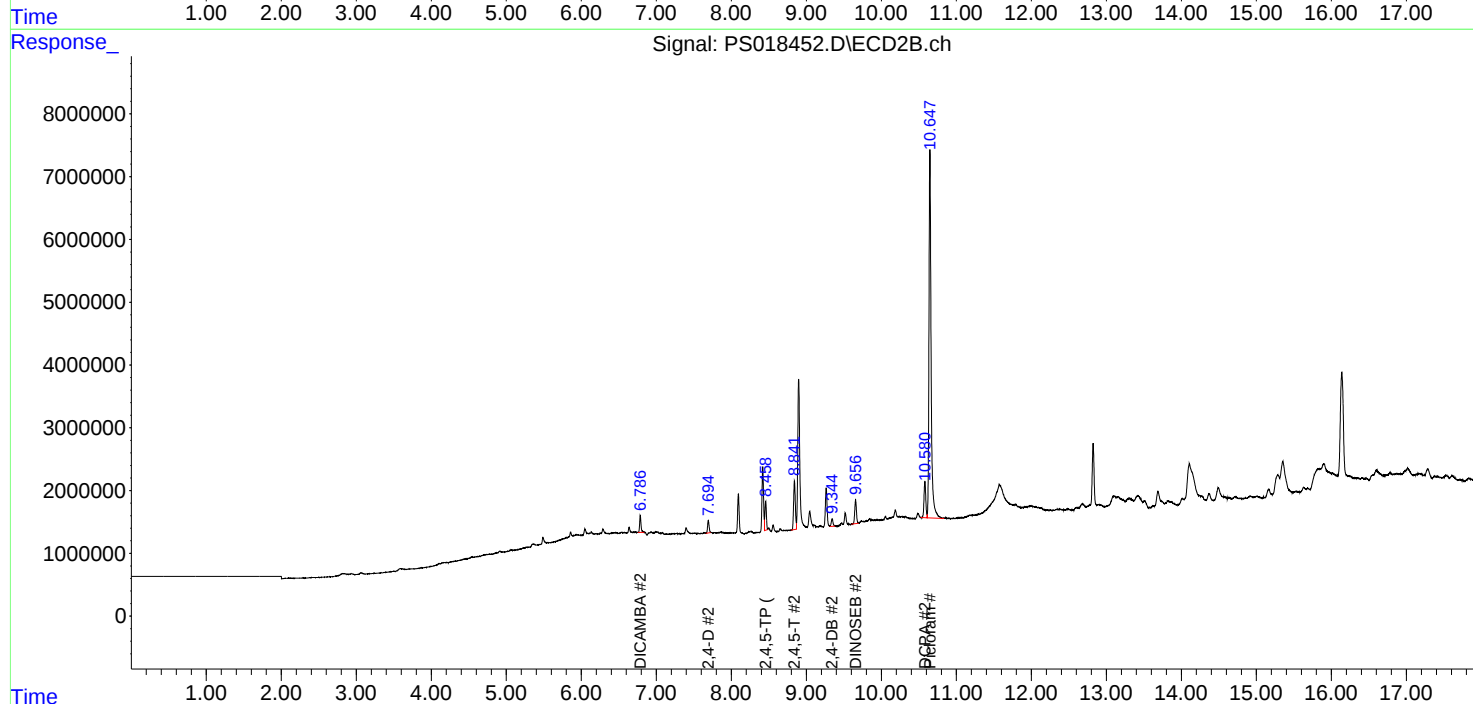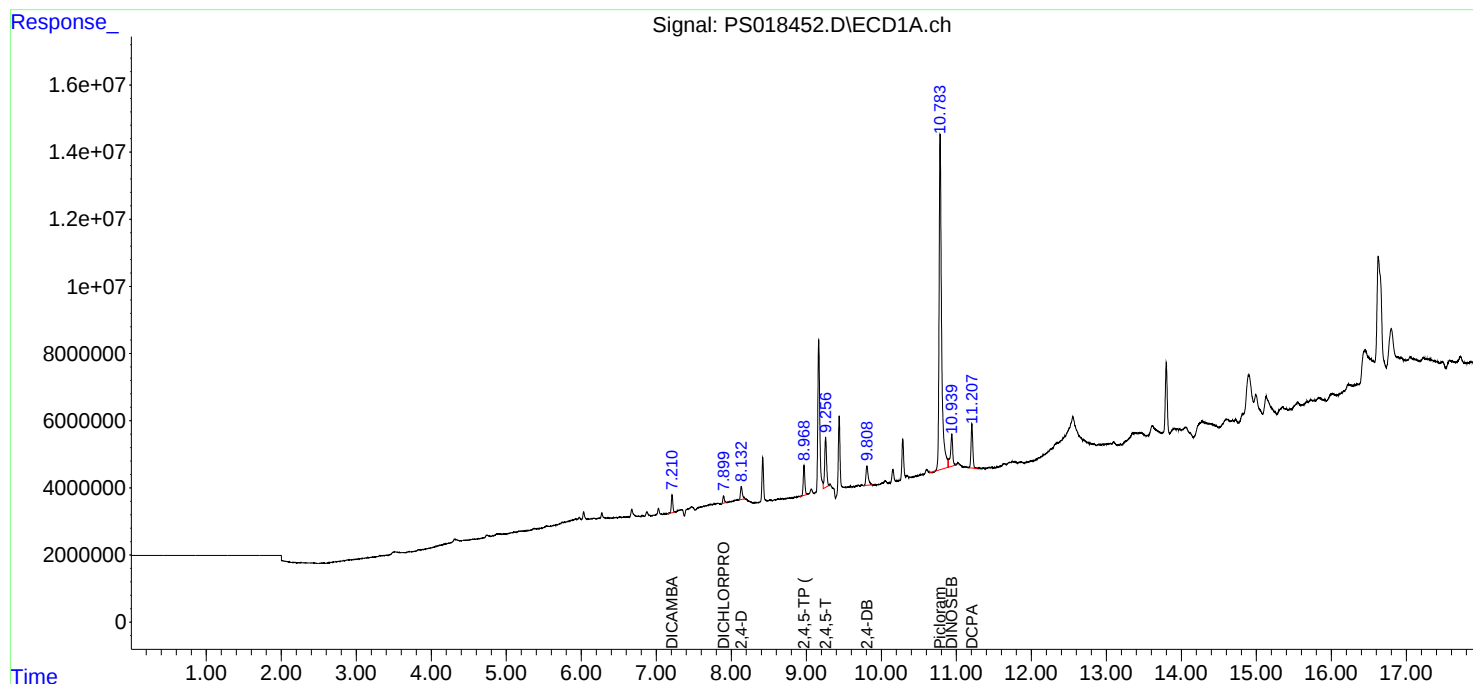


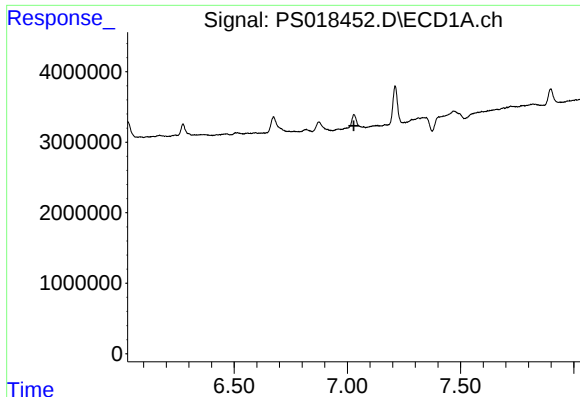

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.029 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

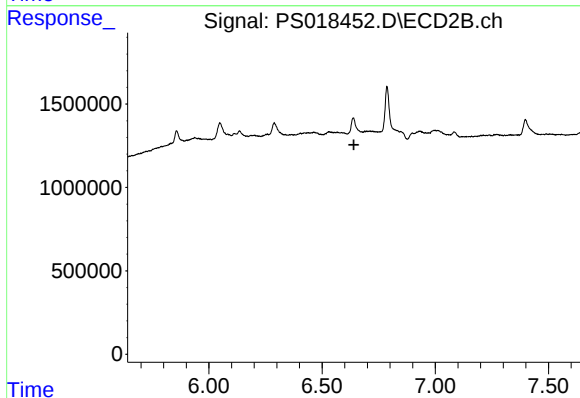


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

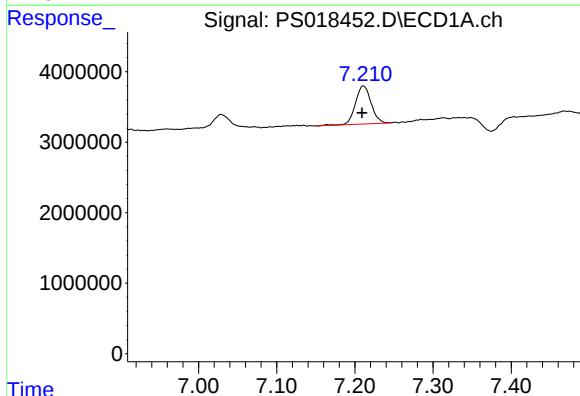


#5 DICAMBA

R.T.: 7.211 min
Delta R.T.: 0.001 min
Response: 7519336
Conc: 1.14 ng/ml

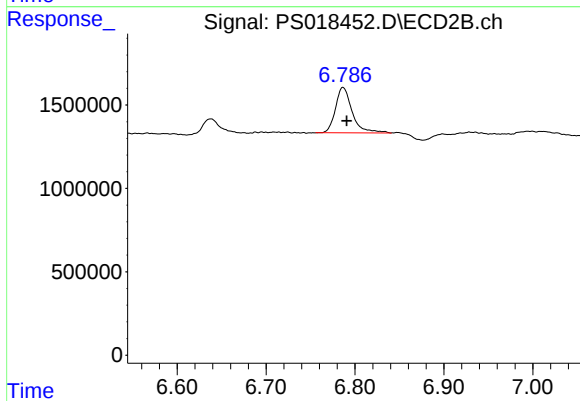

#5 DICAMBA


R.T.: 6.786 min
Delta R.T.: -0.005 min
Response: 3548178
Conc: 1.26 ng/ml

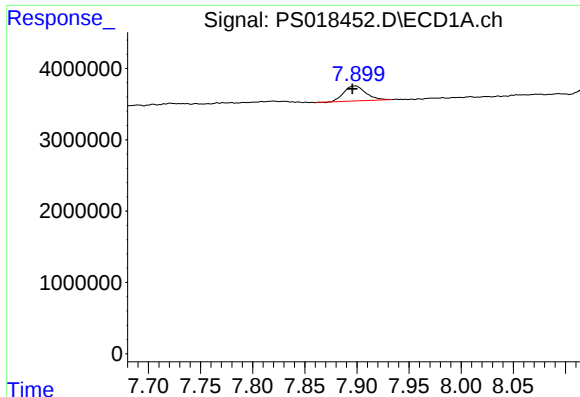

#8 DICHLORPROP


R.T.: 7.898 min
Delta R.T.: 0.002 min
Response: 3039556
Conc: 1.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

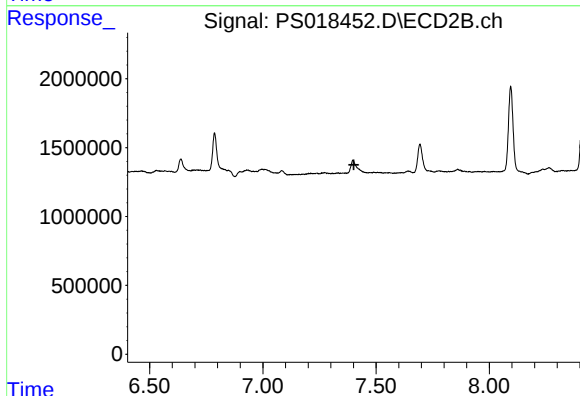


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.402 min
Response: 0
Conc: N.D.

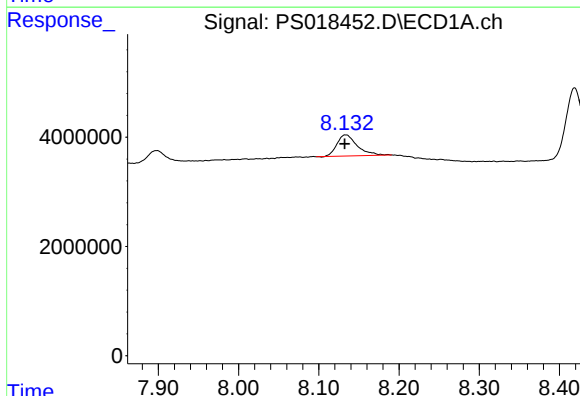


#9 2,4-D

R.T.: 8.134 min
Delta R.T.: 0.001 min
Response: 6775051
Conc: 3.32 ng/ml

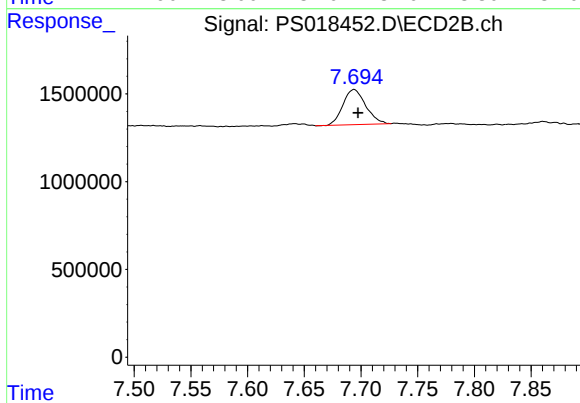

#9 2,4-D


R.T.: 7.694 min
Delta R.T.: -0.003 min
Response: 2801561
Conc: 2.99 ng/ml

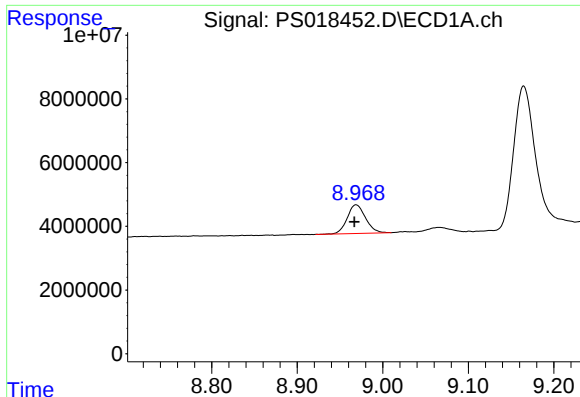

#11 2,4,5-TP (SILVEX)


R.T.: 8.969 min
Delta R.T.: 0.002 min
Response: 13363375
Conc: 1.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

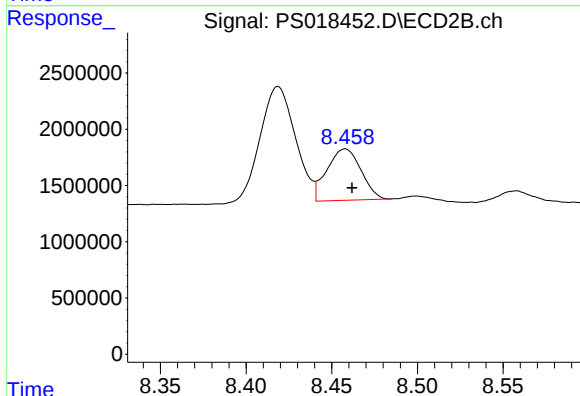


#11 2,4,5-TP (SILVEX)

R.T.: 8.458 min
Delta R.T.: -0.004 min
Response: 6323641
Conc: 1.53 ng/ml

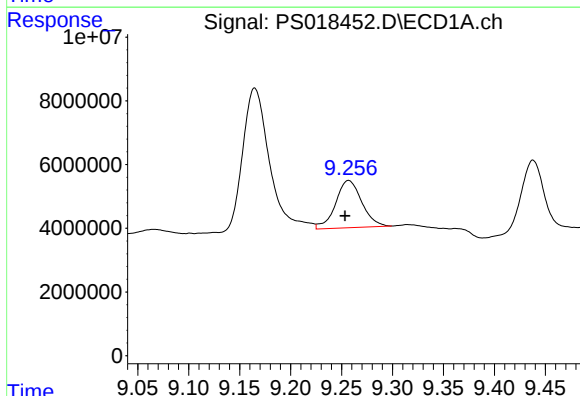


#12 2,4,5-T

R.T.: 9.257 min
Delta R.T.: 0.003 min
Response: 26548439
Conc: 2.64 ng/ml

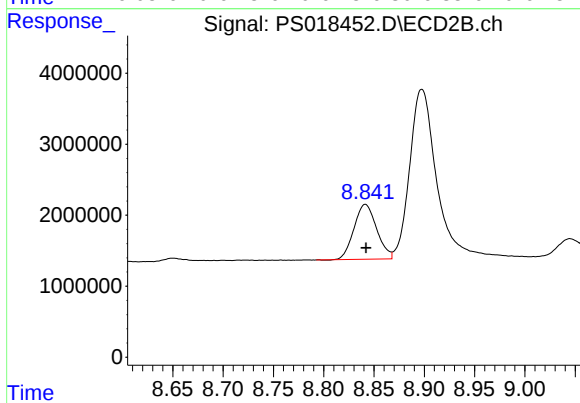

#12 2,4,5-T


R.T.: 8.841 min
Delta R.T.: 0.000 min
Response: 12142214
Conc: 3.08 ng/ml

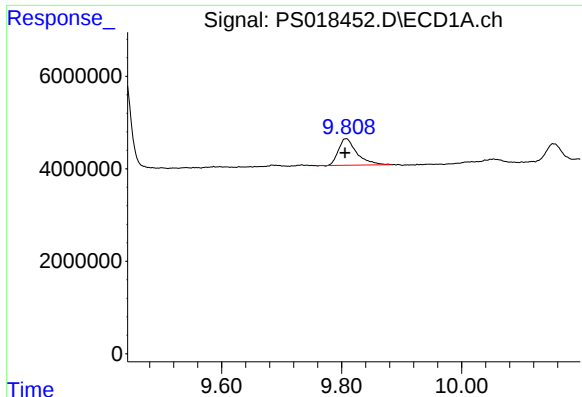

#13 2,4-DB


R.T.: 9.807 min
Delta R.T.: 0.002 min
Response: 12187934
Conc: 7.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

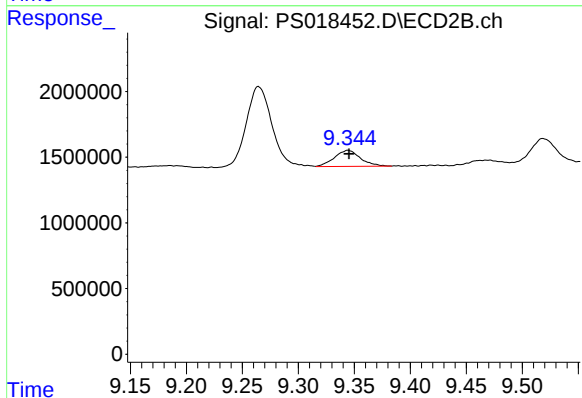


#13 2,4-DB

R.T.: 9.344 min
Delta R.T.: 0.000 min
Response: 1960029
Conc: 3.63 ng/ml

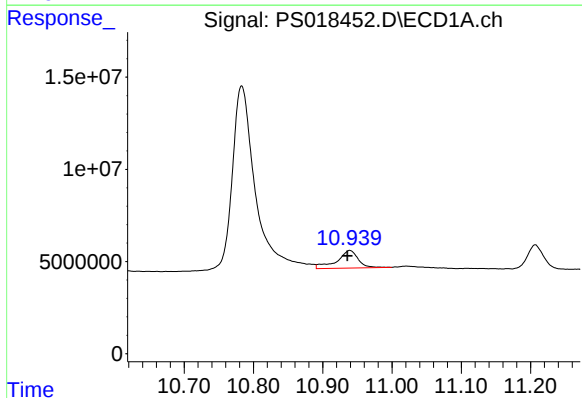


#14 DINOSEB

R.T.: 10.939 min
Delta R.T.: 0.003 min
Response: 20472779
Conc: 2.64 ng/ml

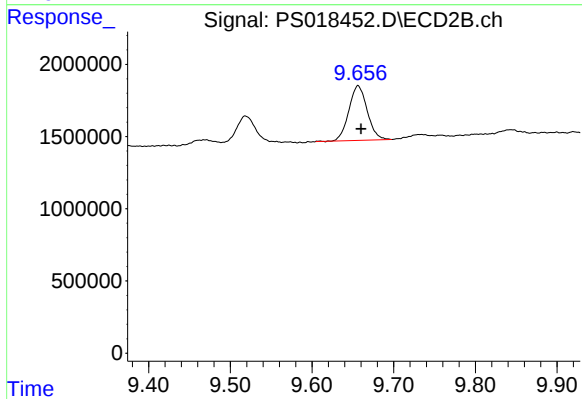

#14 DINOSEB


R.T.: 9.656 min
Delta R.T.: -0.004 min
Response: 5902282
Conc: 2.03 ng/ml

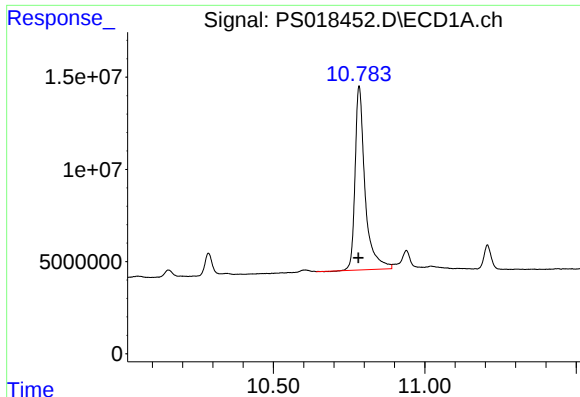

#15 Picloram


R.T.: 10.783 min
Delta R.T.: 0.002 min
Response: 229245863
Conc: 18.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

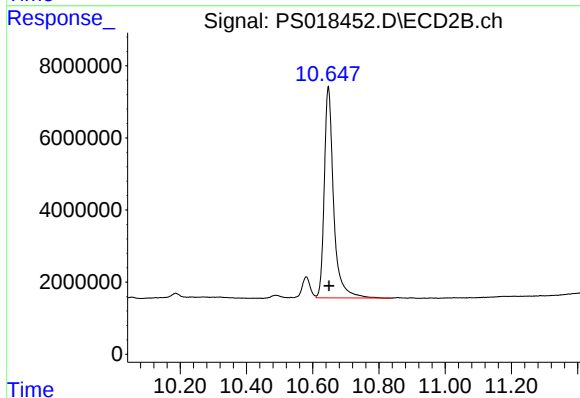


#15 Picloram

R.T.: 10.647 min
Delta R.T.: -0.002 min
Response: 114961353
Conc: 19.88 ng/ml

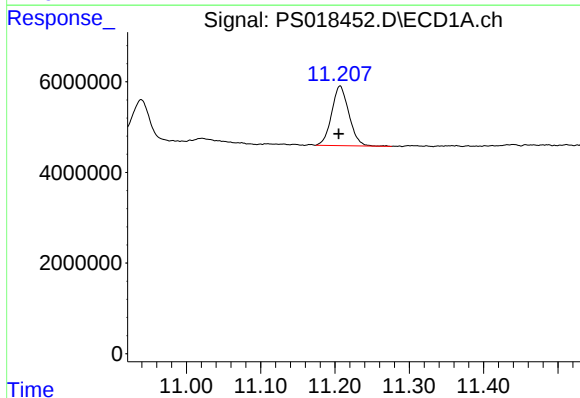

#16 DCPA

R.T.: 11.207 min
Delta R.T.: 0.002 min
Response: 21164037
Conc: 1.76 ng/ml

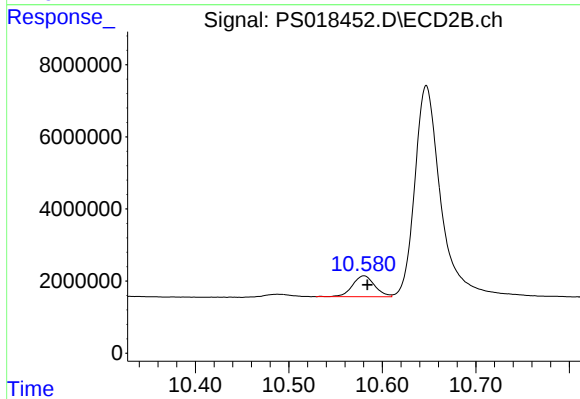

#16 DCPA

R.T.: 10.580 min
Delta R.T.: -0.004 min
Response: 9471155
Conc: 1.91 ng/ml