

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022822\
 Data File : PS018453.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2022 11:21
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 00:03:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.028	6.641	752.7E6	431.9E6	452.353	648.194 #
Target Compounds							
5) T	DICAMBA	0.000	6.796	0	2851931	N.D.	1.016
10) T	Pentachlo...	8.429	8.112	3642737	2181314	<MDL	<MDL #
11) T	2,4,5-TP ...	8.979	8.442	3513777	20012300	<MDL	4.847 #
12) T	2,4,5-T	9.226	8.898f	46476176	3617596	4.620	<MDL #
13) T	2,4-DB	0.000	9.289f	0	18052919	N.D.	33.415
14) T	DINOSEB	10.931	9.673	49988093	2224644	6.434	<MDL #
15) T	Picloram	10.775	10.701f	4558138	113.9E6	<MDL	19.689 #
16) T	DCPA	11.208	10.588	5971565	4966188	<MDL	1.000 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022822\
Data File : PS018453.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2022 11:21
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 00:03:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

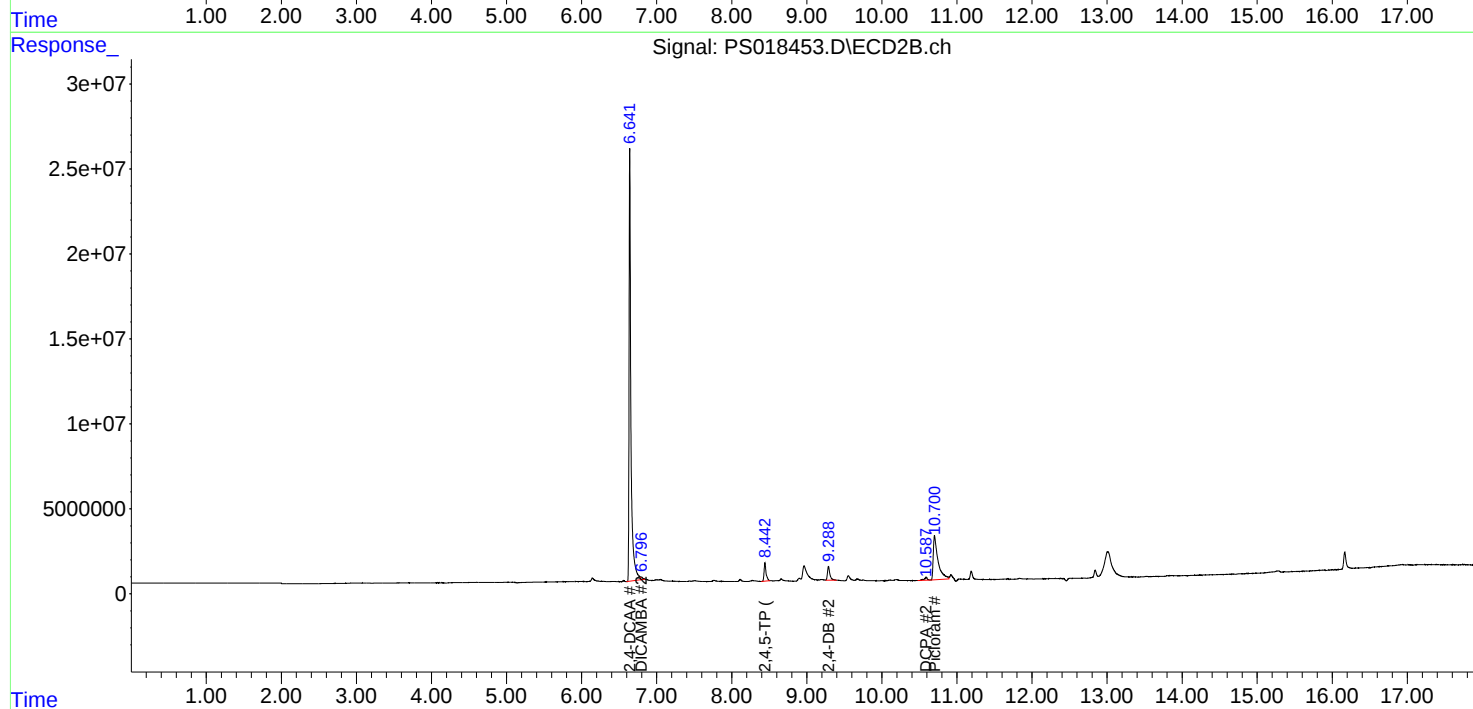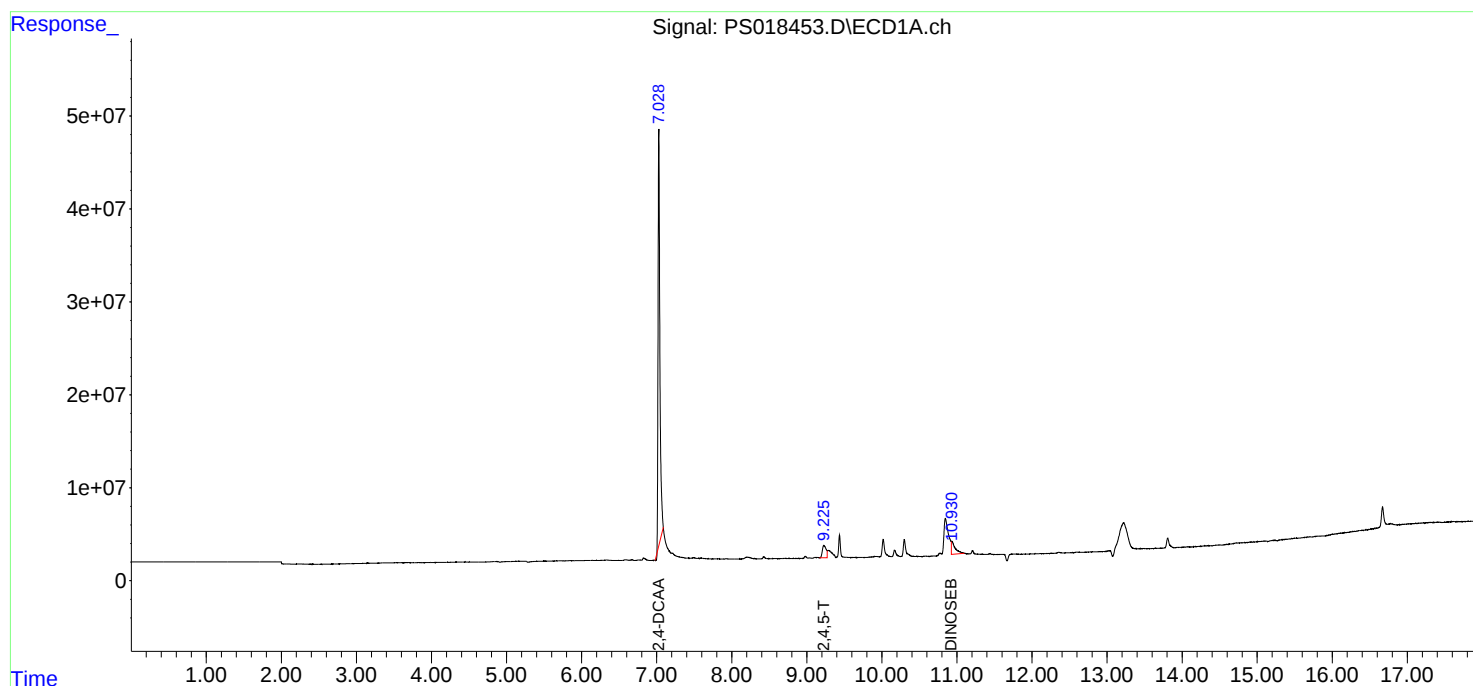


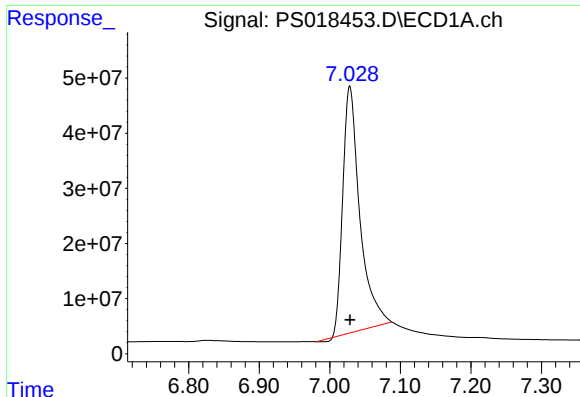

#4 2,4-DCAA


R.T.: 7.028 min
Delta R.T.: 0.000 min
Response: 752737970
Conc: 452.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

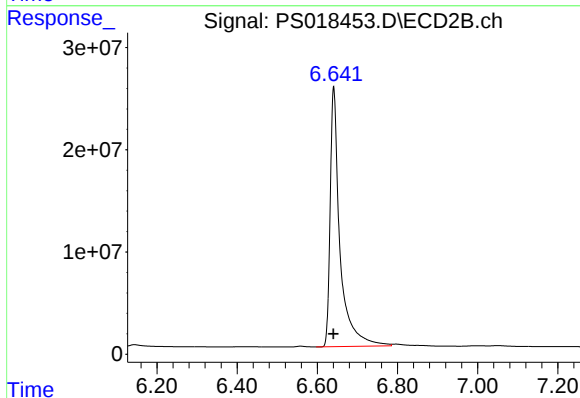


#4 2,4-DCAA

R.T.: 6.641 min
Delta R.T.: 0.000 min
Response: 431918978
Conc: 648.19 ng/ml

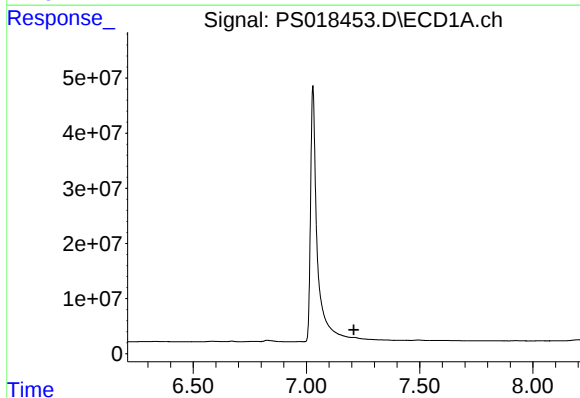


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.209 min
Response: 0
Conc: N.D.

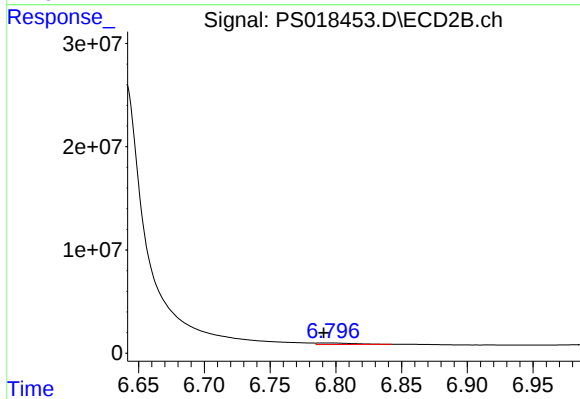

#5 DICAMBA


R.T.: 6.796 min
Delta R.T.: 0.005 min
Response: 2851931
Conc: 1.02 ng/ml

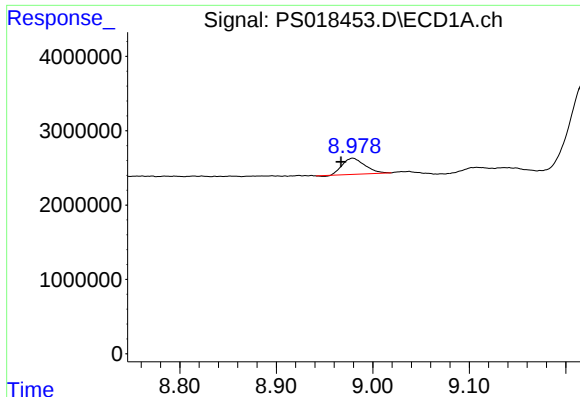

#11 2,4,5-TP (SILVEX)


R.T.: 8.979 min
Delta R.T.: 0.012 min
Response: 3513777
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

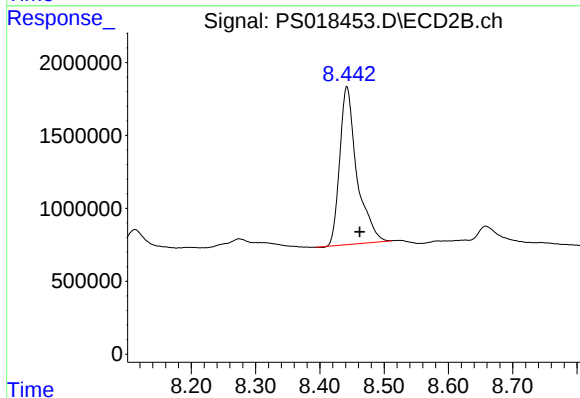


#11 2,4,5-TP (SILVEX)

R.T.: 8.442 min
Delta R.T.: -0.020 min
Response: 20012300
Conc: 4.85 ng/ml

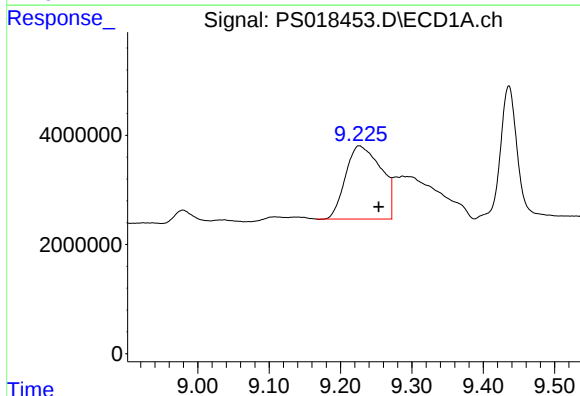


#12 2,4,5-T

R.T.: 9.226 min
Delta R.T.: -0.027 min
Response: 46476176
Conc: 4.62 ng/ml

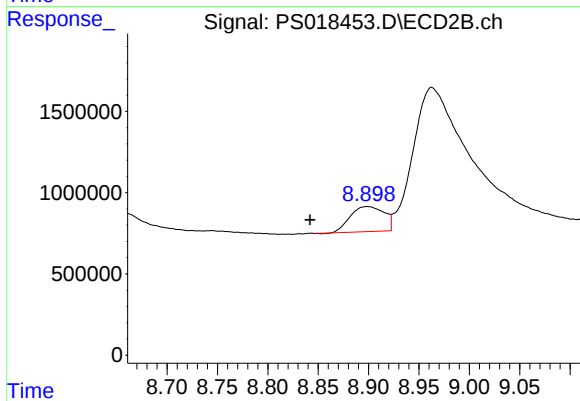

#12 2,4,5-T


R.T.: 8.898 min
Delta R.T.: 0.056 min
Response: 3617596
Conc: N.D.

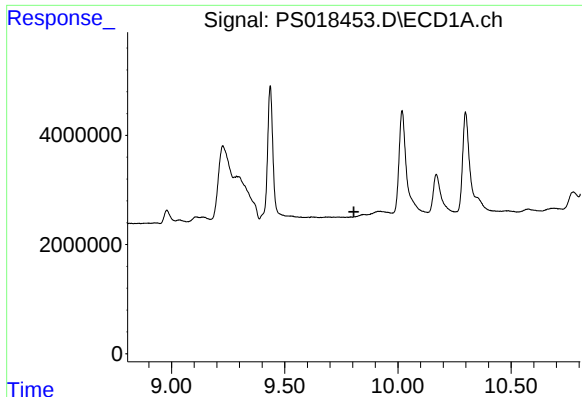

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

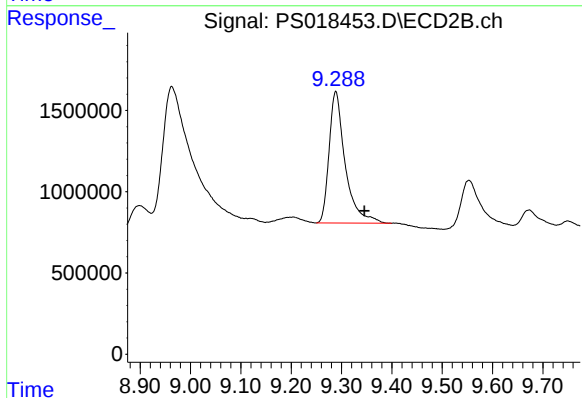


#13 2,4-DB

R.T.: 9.289 min
Delta R.T.: -0.057 min
Response: 18052919
Conc: 33.41 ng/ml

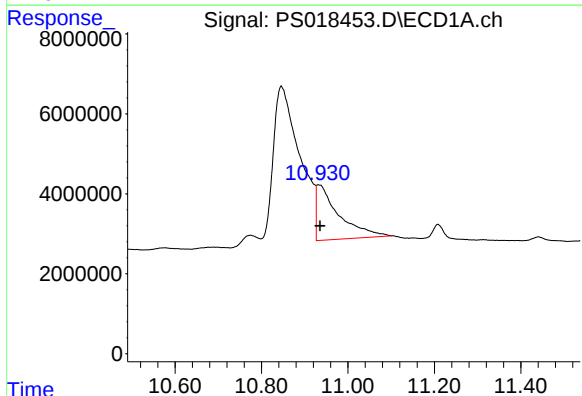


#14 DINOSEB

R.T.: 10.931 min
Delta R.T.: -0.005 min
Response: 49988093
Conc: 6.43 ng/ml

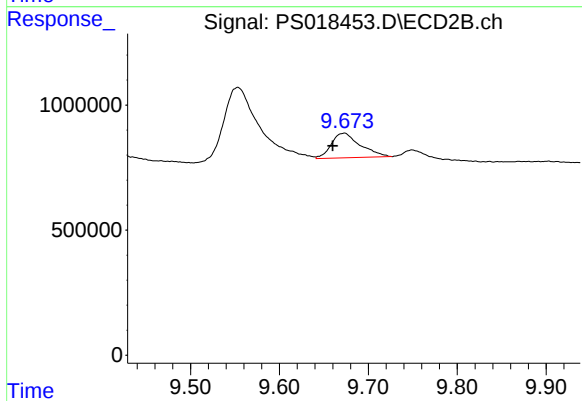

#14 DINOSEB


R.T.: 9.673 min
Delta R.T.: 0.013 min
Response: 2224644
Conc: N.D.

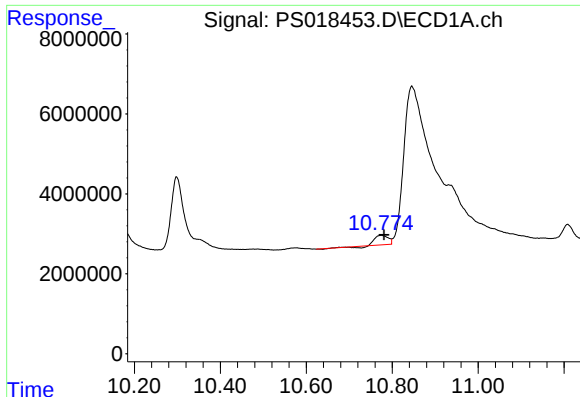

#15 Picloram


R.T.: 10.775 min
Delta R.T.: -0.006 min
Response: 4558138
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

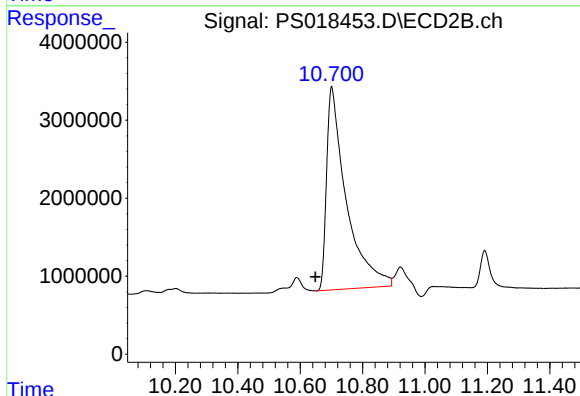


#15 Picloram

R.T.: 10.701 min
Delta R.T.: 0.052 min
Response: 113858794
Conc: 19.69 ng/ml

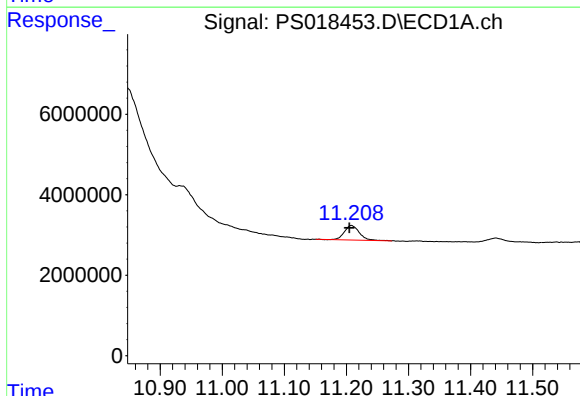

#16 DCPA

R.T.: 11.208 min
Delta R.T.: 0.003 min
Response: 5971565
Conc: N.D.

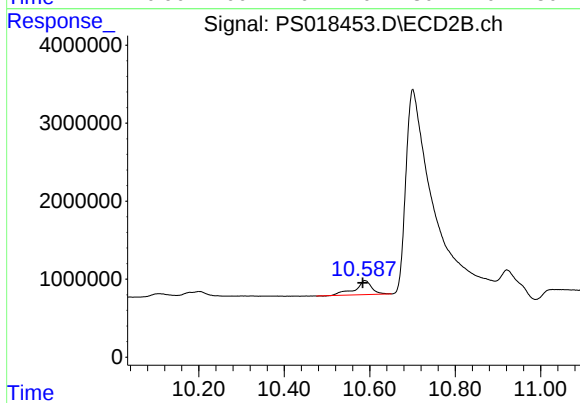

#16 DCPA

R.T.: 10.588 min
Delta R.T.: 0.004 min
Response: 4966188
Conc: 1.00 ng/ml