

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022822\
 Data File : PS018469.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2022 18:35
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 00:08:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.025	6.638	814.1E6	426.6E6	489.252	640.244 #
Target Compounds							
3) T	4-Nitroph...	6.819f	0.000	183309	0	<MDL	N.D. #
5) T	DICAMBA	0.000	6.792	0	1442970	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.469f	0	2022913	N.D.	2.747
9) T	2,4-D	8.195f	0.000	11964894	0	5.865	N.D. #
11) T	2,4,5-TP ...	9.024f	8.432	6707745	22121166	<MDL	5.358 #
12) T	2,4,5-T	9.279	8.877	7885437	2623701	<MDL	<MDL #
13) T	2,4-DB	0.000	9.357	0	3249181	N.D.	6.014
14) T	DINOSEB	10.915	9.677	35097639	7380704	4.518	2.539 #
15) T	Picloram	10.755	10.689f	13190423	39436622	1.038	6.819 #
16) T	DCPA	11.204	10.586	2825639	2786668	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS022822\
Data File : PS018469.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2022 18:35
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 00:08:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

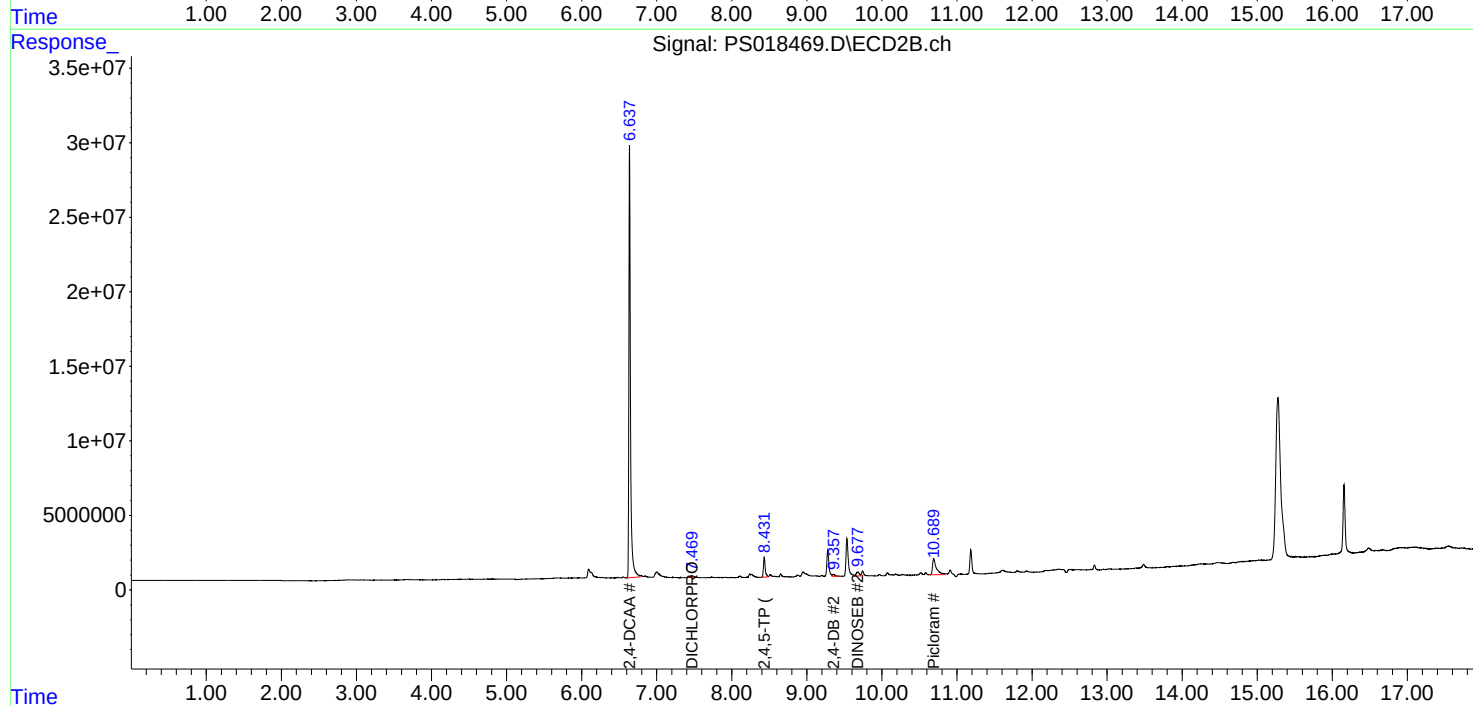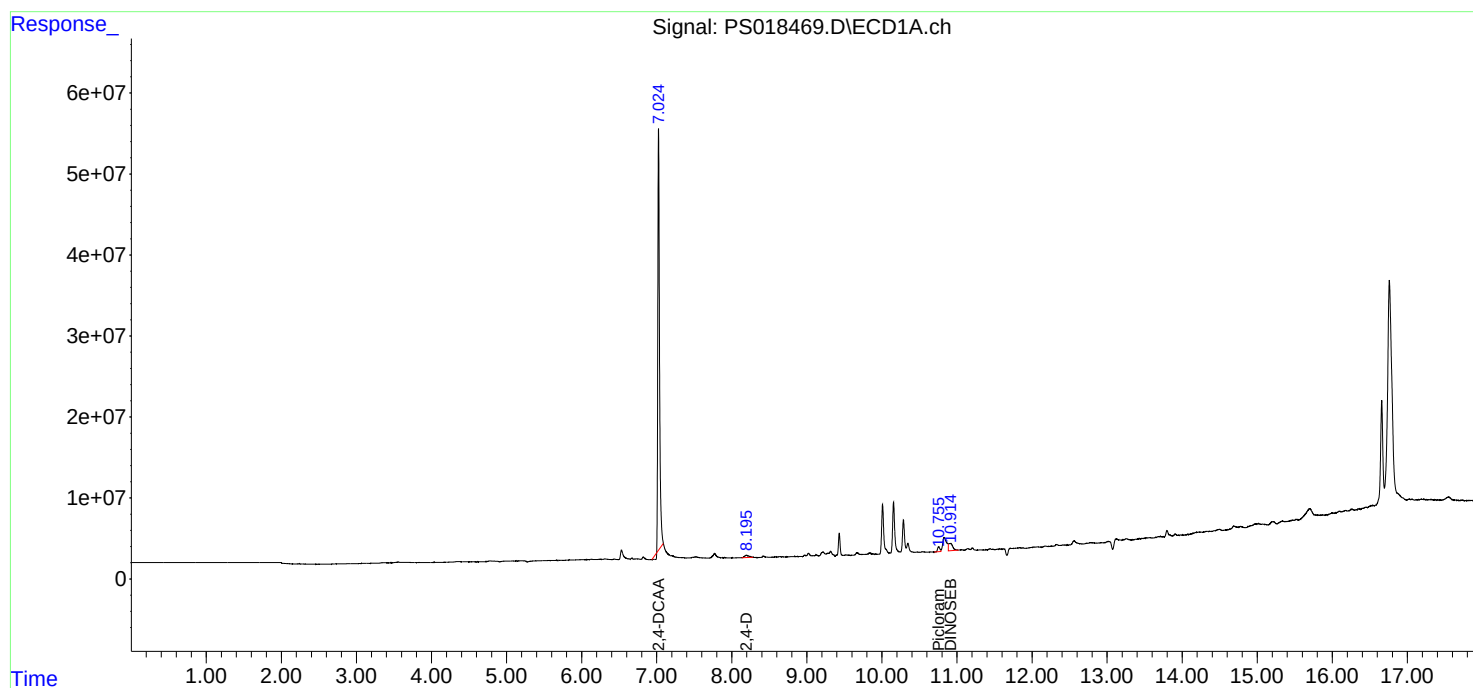


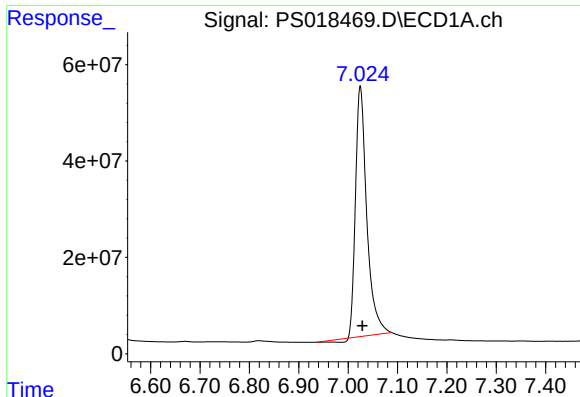

#4 2,4-DCAA


R.T.: 7.025 min
Delta R.T.: -0.004 min
Response: 814139746
Conc: 489.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

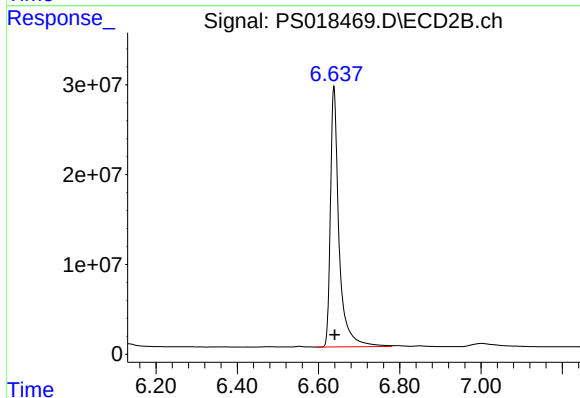


#4 2,4-DCAA

R.T.: 6.638 min
Delta R.T.: -0.002 min
Response: 426621584
Conc: 640.24 ng/ml

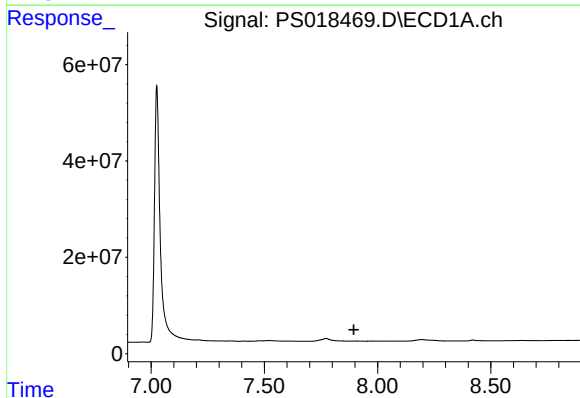


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.896 min
Response: 0
Conc: N.D.

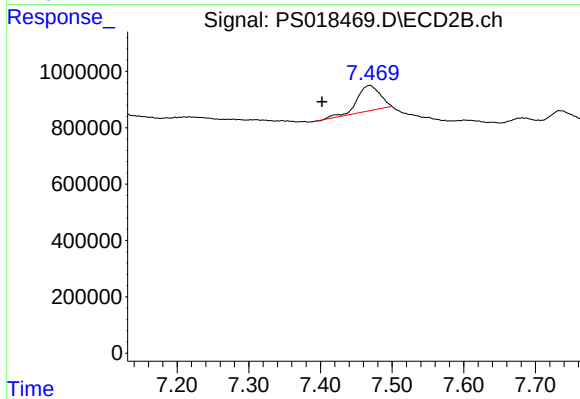

#8 DICHLORPROP


R.T.: 7.469 min
Delta R.T.: 0.067 min
Response: 2022913
Conc: 2.75 ng/ml

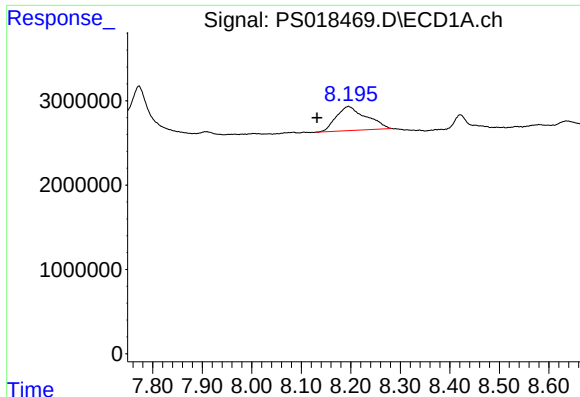

#9 2,4-D


R.T.: 8.195 min
Delta R.T.: 0.063 min
Response: 11964894
Conc: 5.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

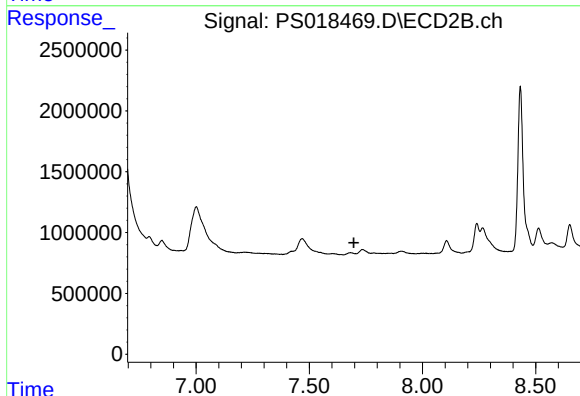


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.697 min
Response: 0
Conc: N.D.

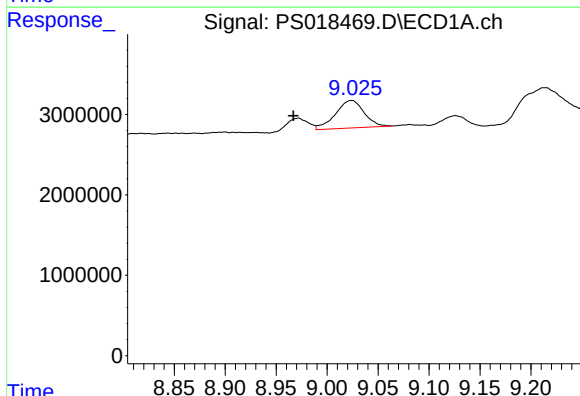


#11 2,4,5-TP (SILVEX)

R.T.: 9.024 min
Delta R.T.: 0.057 min
Response: 6707745
Conc: N.D.

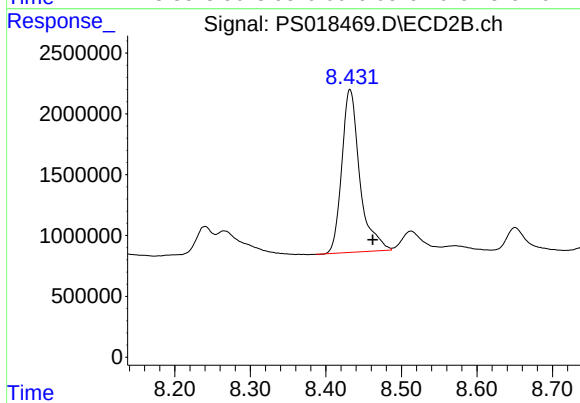

#11 2,4,5-TP (SILVEX)


R.T.: 8.432 min
Delta R.T.: -0.030 min
Response: 22121166
Conc: 5.36 ng/ml

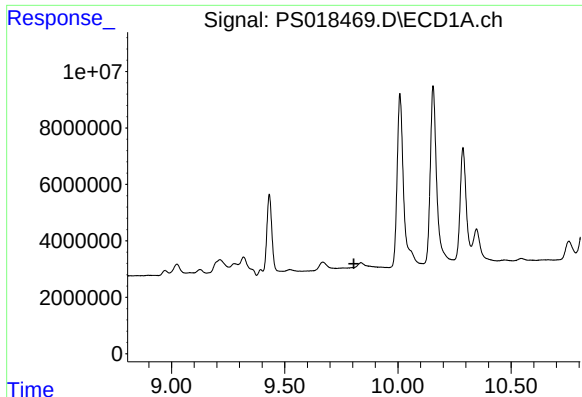

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.806 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

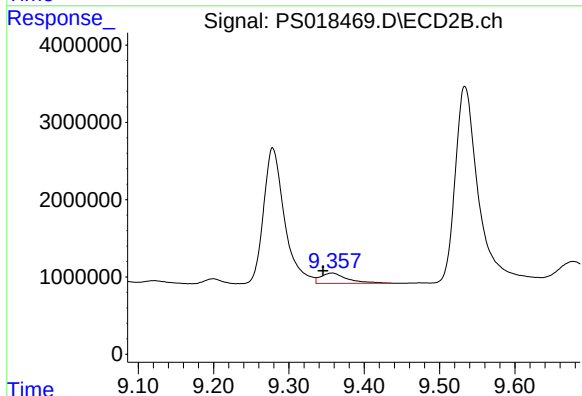


#13 2,4-DB

R.T.: 9.357 min
Delta R.T.: 0.012 min
Response: 3249181
Conc: 6.01 ng/ml

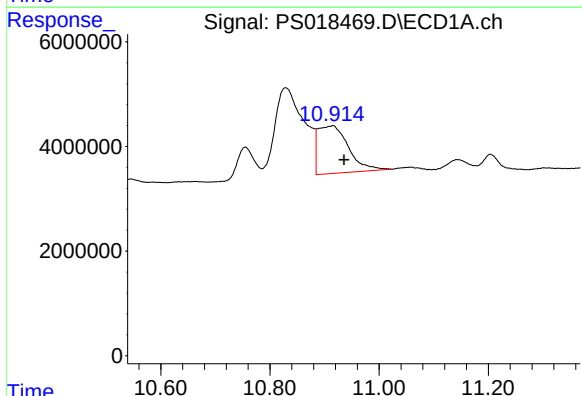


#14 DINOSEB

R.T.: 10.915 min
Delta R.T.: -0.020 min
Response: 35097639
Conc: 4.52 ng/ml

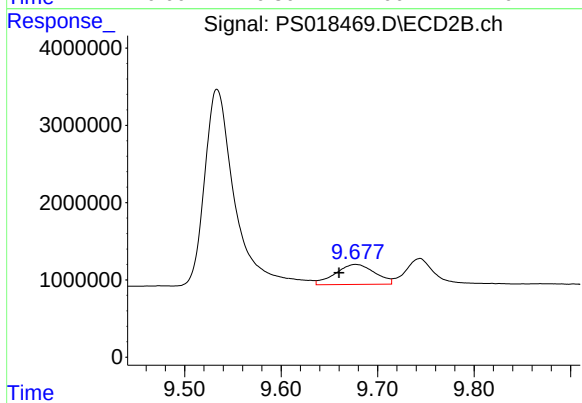

#14 DINOSEB


R.T.: 9.677 min
Delta R.T.: 0.017 min
Response: 7380704
Conc: 2.54 ng/ml

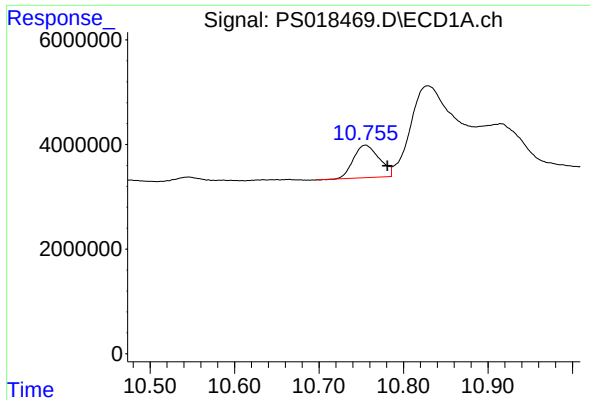

#15 Picloram

R.T.: 10.755 min
Delta R.T.: -0.026 min
Response: 13190423
Conc: 1.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

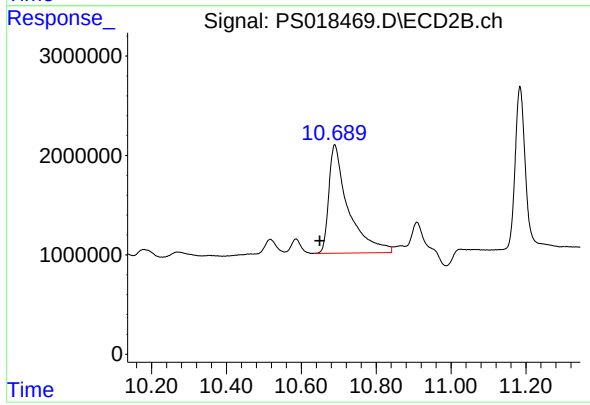

#15 Picloram

R.T.: 10.689 min
Delta R.T.: 0.040 min
Response: 39436622
Conc: 6.82 ng/ml