

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030123\
 Data File : PS022284.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Mar 2023 19:44
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 20:32:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
 Quant Title : 8080.M
 QLast Update : Mon Feb 20 13:26:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.300	6.723	1288.0E6	1161.6E6	519.617	553.434
Target Compounds							
1) T	Dalapon	2.411	2.519	332265	930841	<MDL	<MDL #
2) T	3,5-DICHL...	5.668	0.000	850941	0	<MDL	N.D. #
3) T	4-Nitroph...	6.153	6.349	7407062	2078664	5.821	1.556 #
5) T	DICAMBA	0.000	6.882	0	13150316	N.D.	1.361
6) T	MCP	6.613	6.932f	-907205	11192726	N.D.	1.466
7) T	MCPA	6.720	7.126f	4776706	28710873	<MDL	2.817 #
8) T	DICHLORPROP	7.029	7.569f	-190201	24708655	N.D.	10.051
9) T	2,4-D	7.220	0.000	4693922	0	1.432	N.D. #
10) T	Pentachlo...	7.449	8.213	10497352	7635143	<MDL	<MDL #
11) T	2,4,5-TP ...	7.987	8.583	7094497	2521533	<MDL	<MDL #
12) T	2,4,5-T	8.235	8.996f	8765070	3231950	<MDL	<MDL #
14) T	DINOSEB	9.778	9.778	16208206	6641724	1.179	<MDL #
15) T	Picloram	9.640	10.701f	8345088	15804420	<MDL	<MDL #
16) T	DCPA	10.045	10.701	7346680	15804420	<MDL	1.010 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030123\
Data File : PS022284.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Mar 2023 19:44
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 20:32:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
Quant Title : 8080.M
QLast Update : Mon Feb 20 13:26:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

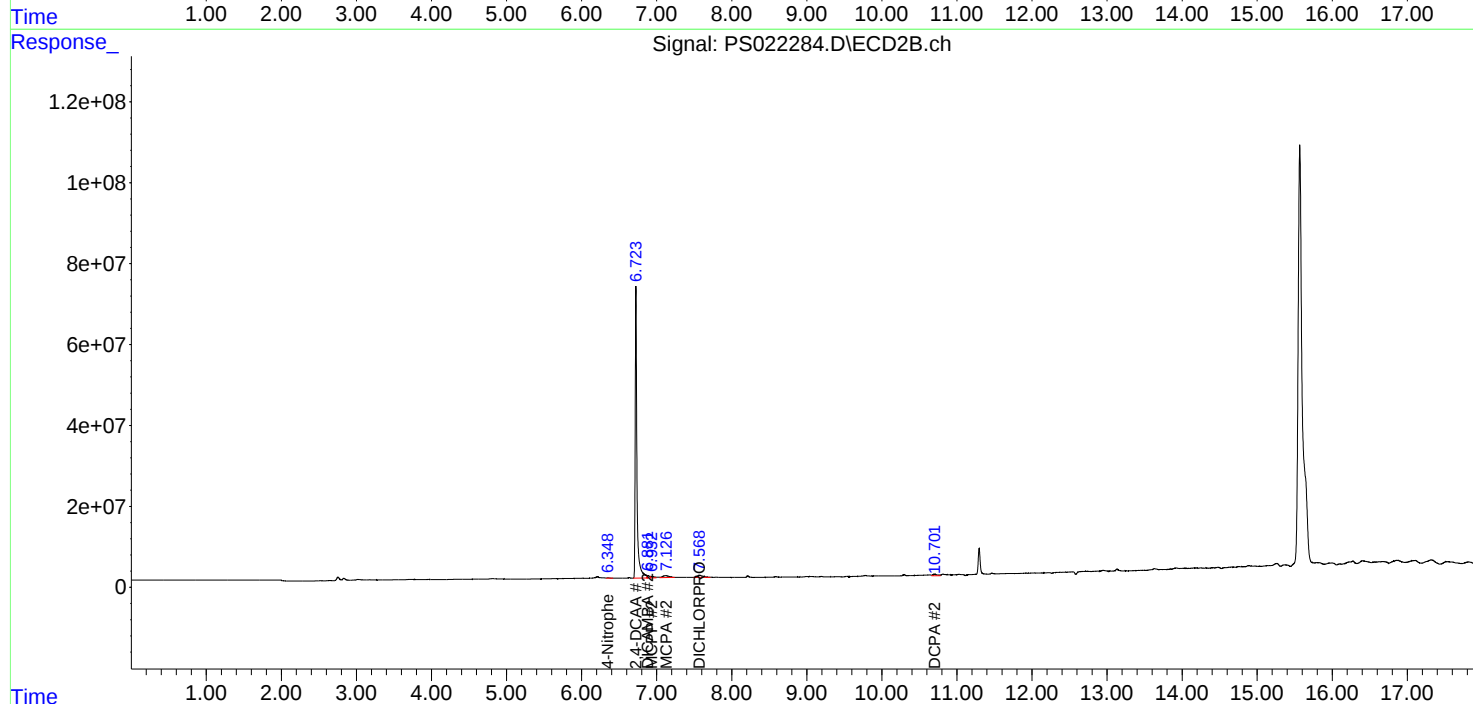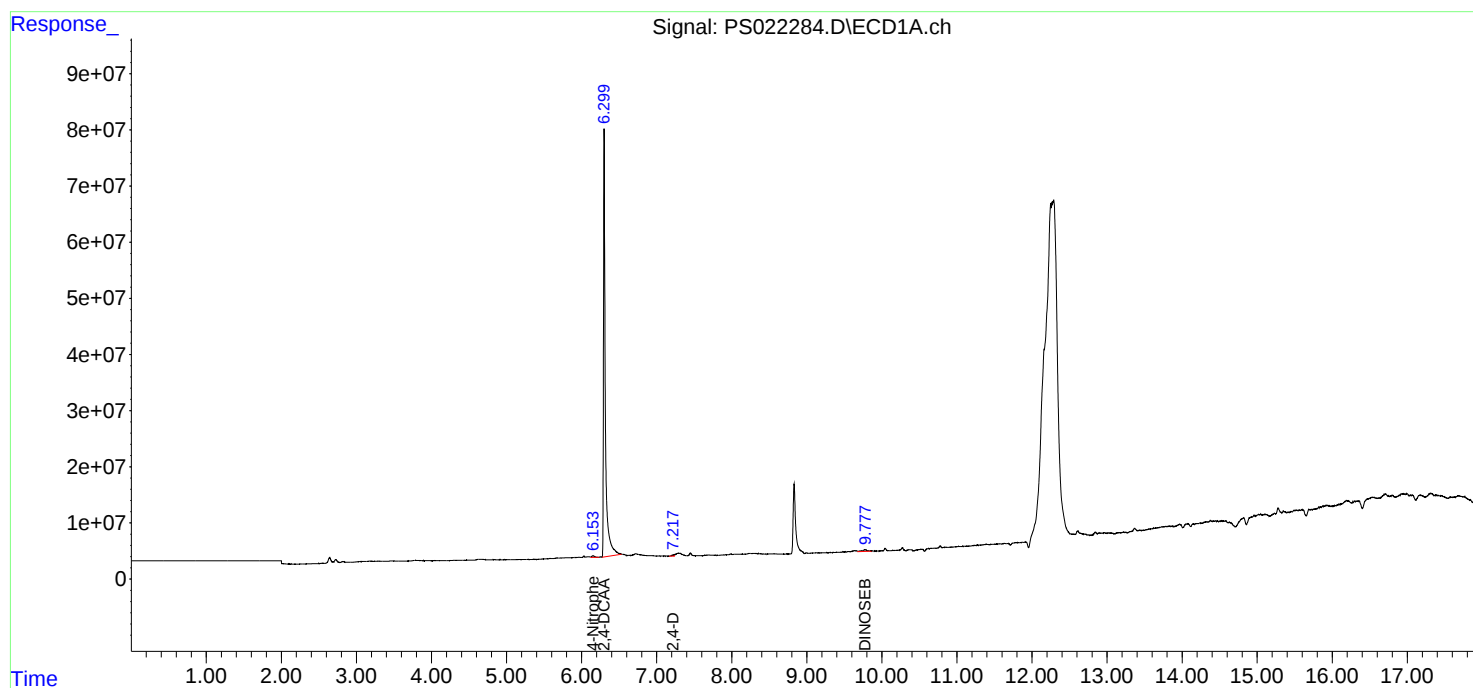


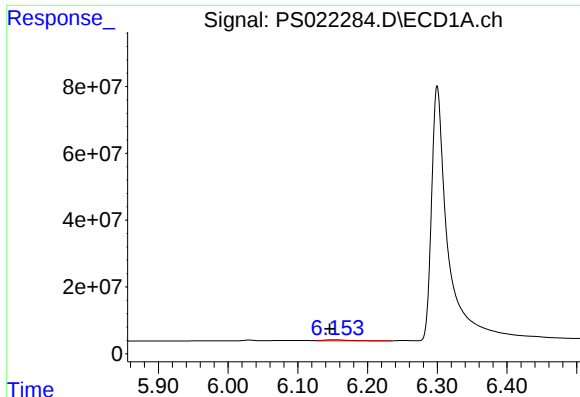

#3 4-Nitrophenol


R.T.: 6.153 min
Delta R.T.: 0.007 min
Response: 7407062
Conc: 5.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

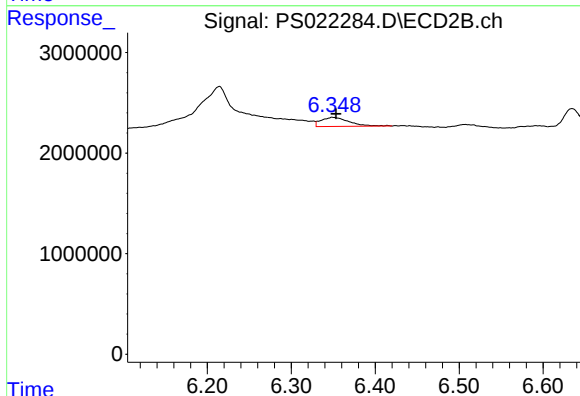


#3 4-Nitrophenol

R.T.: 6.349 min
Delta R.T.: -0.004 min
Response: 2078664
Conc: 1.56 ng/ml

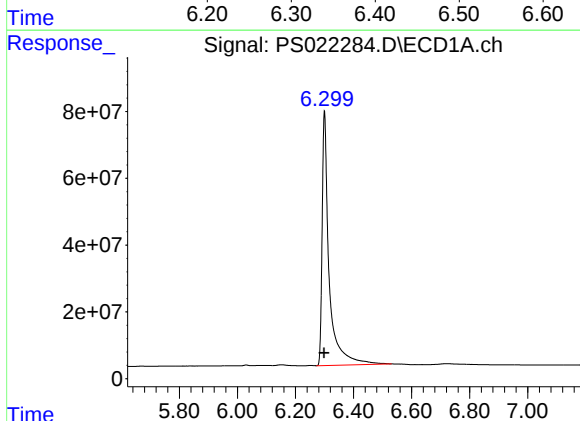


#4 2,4-DCAA

R.T.: 6.300 min
Delta R.T.: 0.002 min
Response: 1287970737
Conc: 519.62 ng/ml

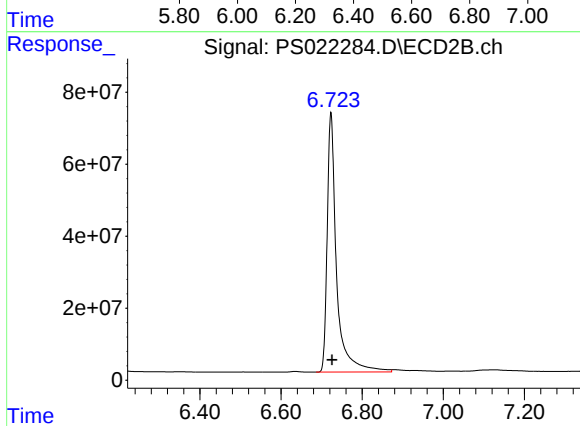

#4 2,4-DCAA


R.T.: 6.723 min
Delta R.T.: -0.003 min
Response: 1161637523
Conc: 553.43 ng/ml

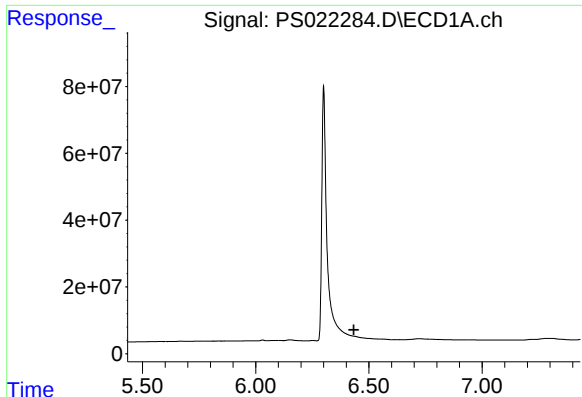

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

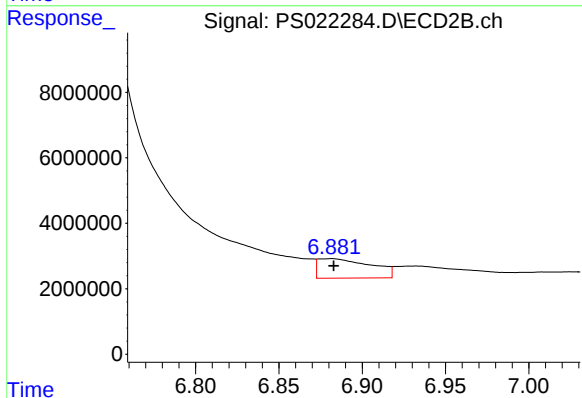


#5 DICAMBA

R.T.: 6.882 min
Delta R.T.: -0.002 min
Response: 13150316
Conc: 1.36 ng/ml

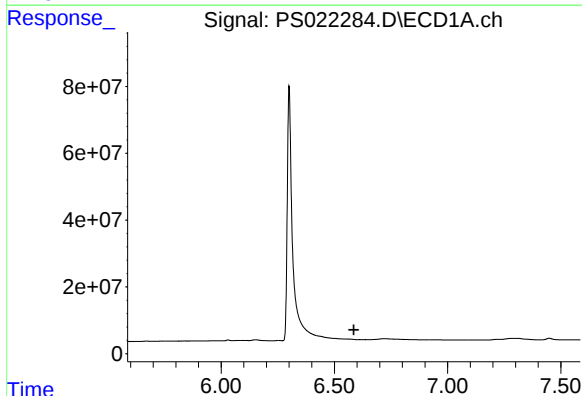


#6 MCP

R.T.: 6.613 min
Delta R.T.: 0.027 min
Response: -907205
Conc: N.D.

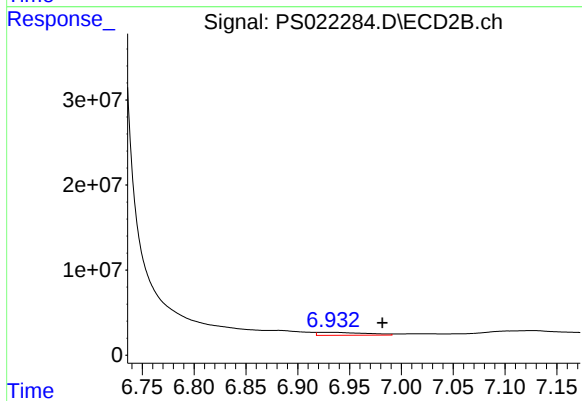

#6 MCP


R.T.: 6.932 min
Delta R.T.: -0.050 min
Response: 11192726
Conc: 1.47 ug/ml

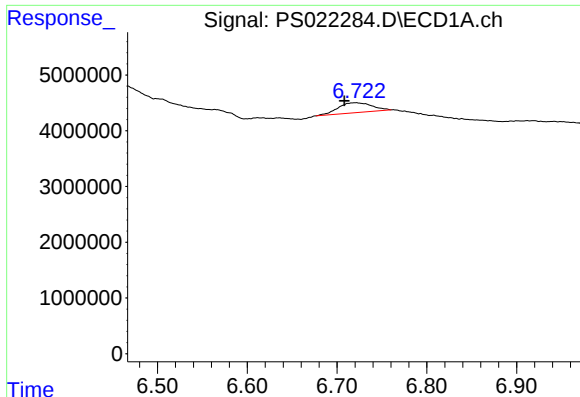

#7 MCPA


R.T.: 6.720 min
Delta R.T.: 0.012 min
Response: 4776706
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

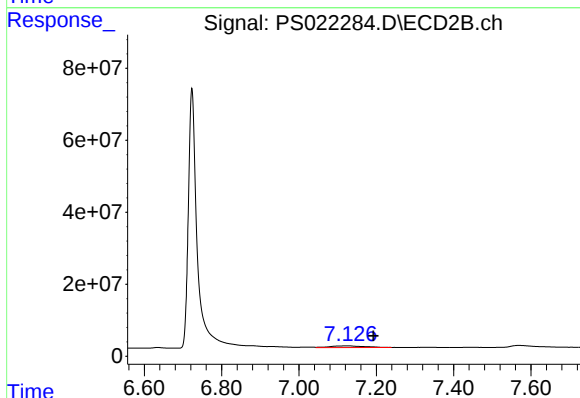


#7 MCPA

R.T.: 7.126 min
Delta R.T.: -0.066 min
Response: 28710873
Conc: 2.82 ug/ml

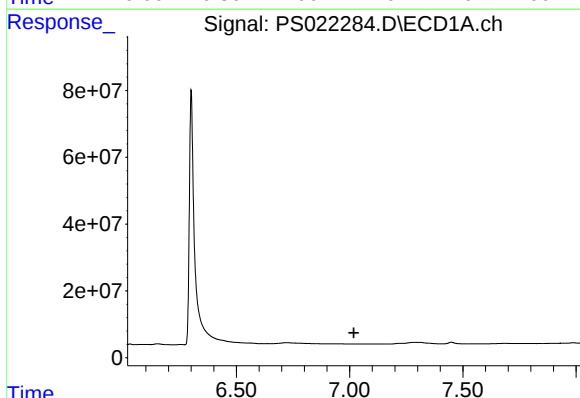


#8 DICHLORPROP

R.T.: 7.029 min
Delta R.T.: 0.011 min
Response: -190201
Conc: N.D.

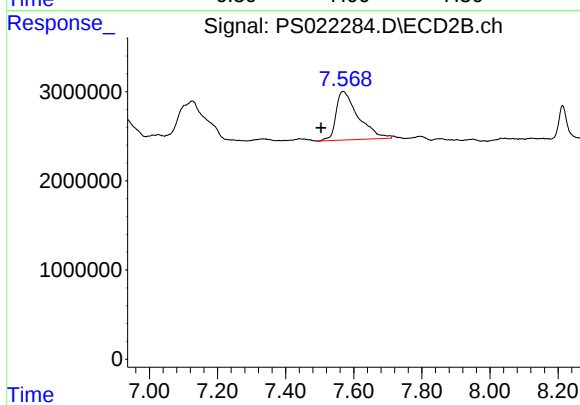

#8 DICHLORPROP


R.T.: 7.569 min
Delta R.T.: 0.064 min
Response: 24708655
Conc: 10.05 ng/ml

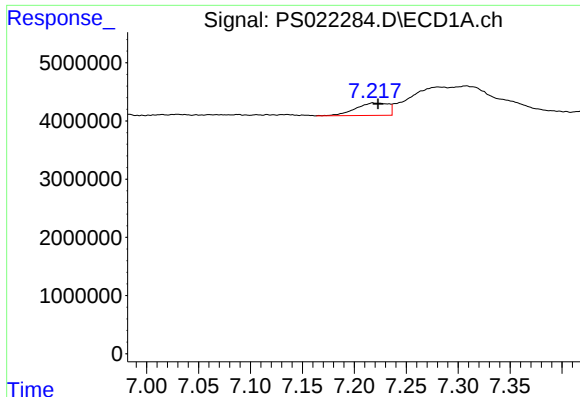

#9 2,4-D


R.T.: 7.220 min
Delta R.T.: -0.003 min
Response: 4693922
Conc: 1.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

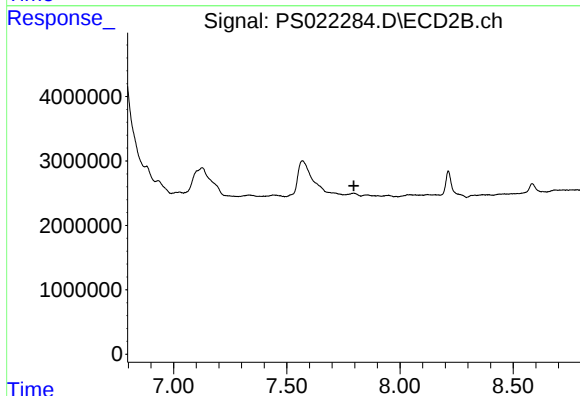


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.796 min
Response: 0
Conc: N.D.

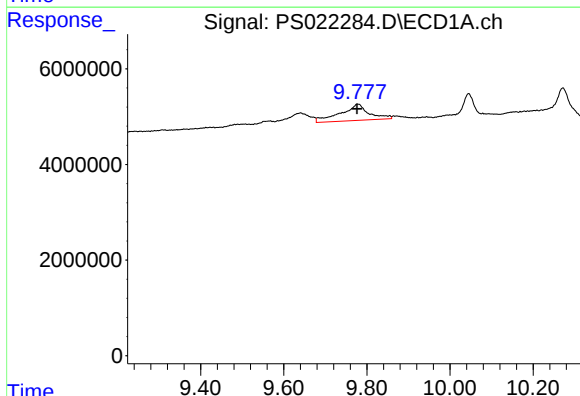


#14 DINOSEB

R.T.: 9.778 min
Delta R.T.: 0.002 min
Response: 16208206
Conc: 1.18 ng/ml

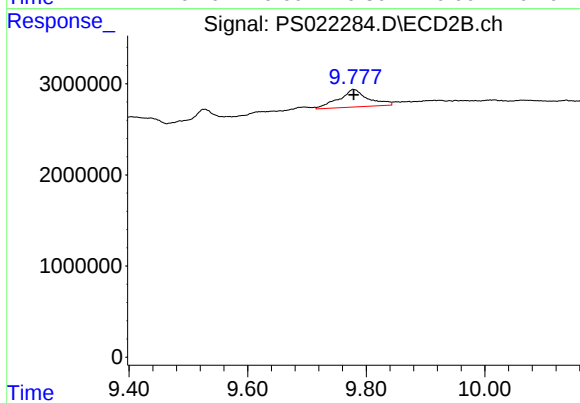

#14 DINOSEB


R.T.: 9.778 min
Delta R.T.: 0.000 min
Response: 6641724
Conc: N.D.

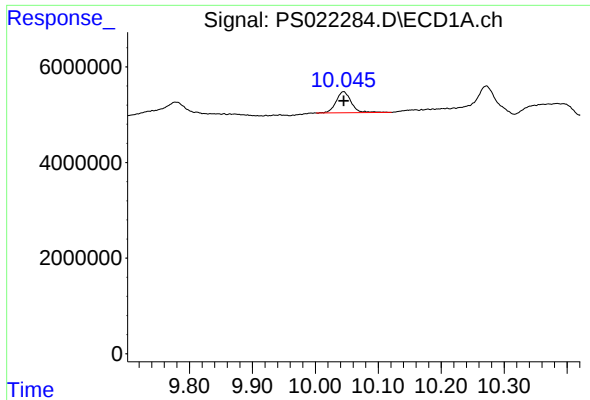

#16 DCPA

R.T.: 10.045 min
Delta R.T.: 0.000 min
Response: 7346680
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

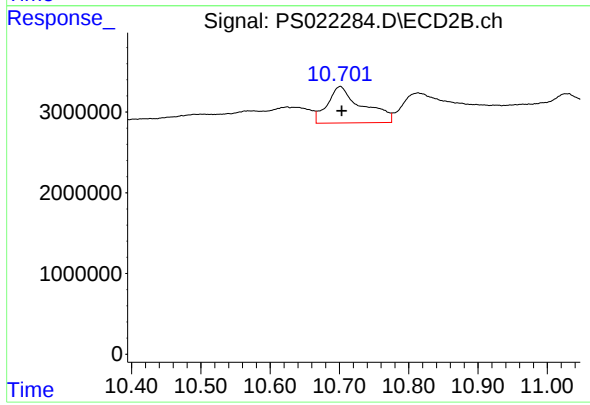

#16 DCPA

R.T.: 10.701 min
Delta R.T.: -0.002 min
Response: 15804420
Conc: 1.01 ng/ml