

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030222\
 Data File : PS018472.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2022 09:11
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 00:03:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.030	6.642	697.1E6	446.9E6	418.905	670.617 #
Target Compounds							
11) T	2,4,5-TP ...	0.000	8.442	0	27739369	N.D.	6.719
12) T	2,4,5-T	9.249	0.000	43863702	0	4.361	N.D. #
13) T	2,4-DB	0.000	9.291f	0	25658577	N.D.	47.492
14) T	DINOSEB	10.871f	0.000	183.4E6	0	23.609	N.D. #
15) T	Picloram	10.780	10.590f	19232211	3694831	1.514	<MDL #
16) T	DCPA	0.000	10.590	0	3694831	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030222\
Data File : PS018472.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2022 09:11
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 00:03:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

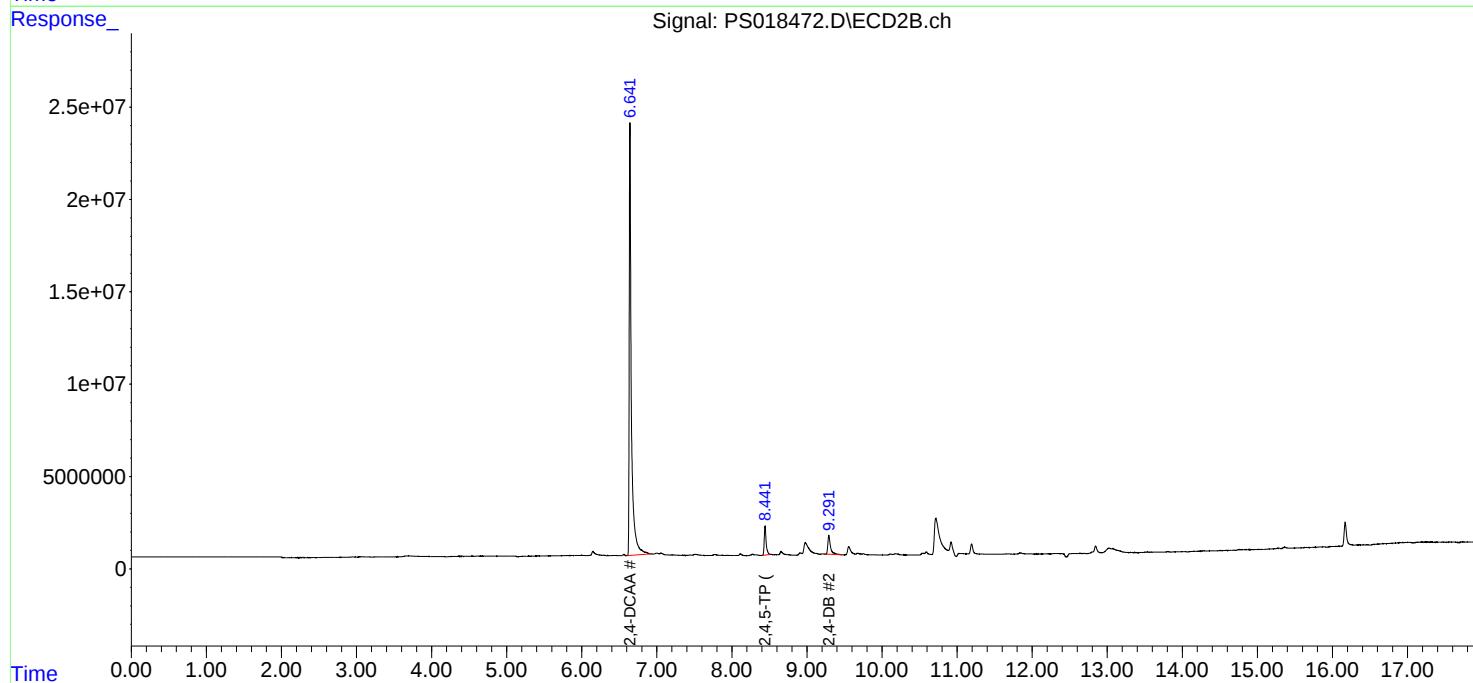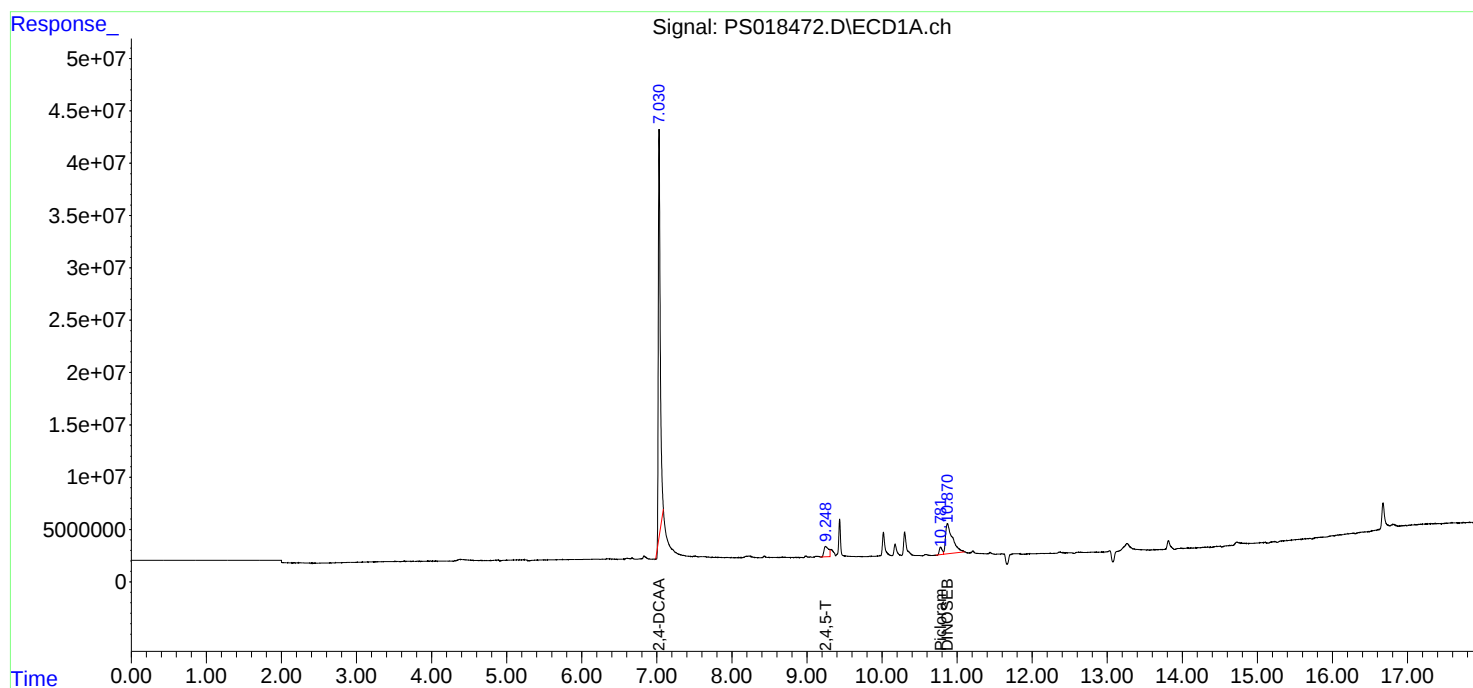


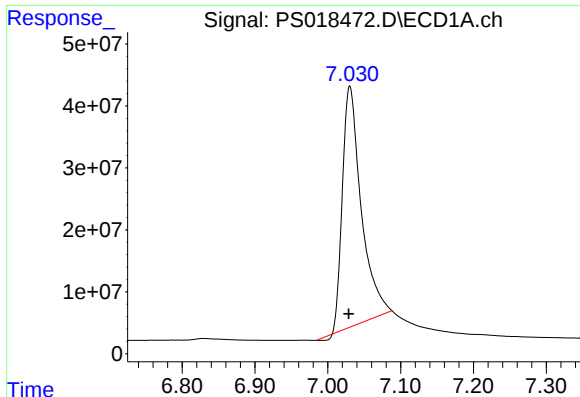

#4 2,4-DCAA


R.T.: 7.030 min
Delta R.T.: 0.002 min
Response: 697078002
Conc: 418.90 ng/ml

Instrument :
ECD_S
ClientSampleId :

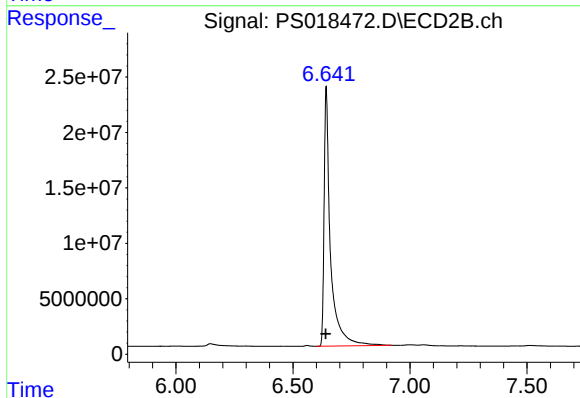


#4 2,4-DCAA

R.T.: 6.642 min
Delta R.T.: 0.002 min
Response: 446860326
Conc: 670.62 ng/ml

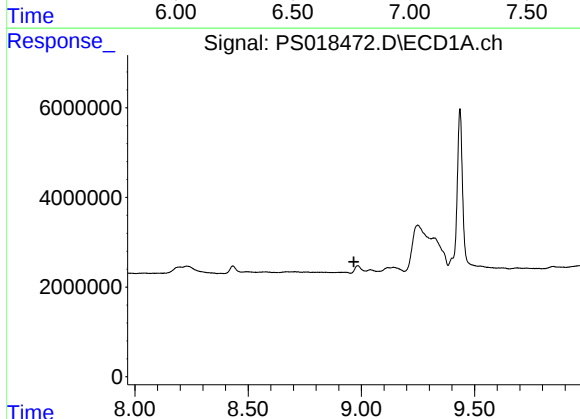


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.967 min
Response: 0
Conc: N.D.

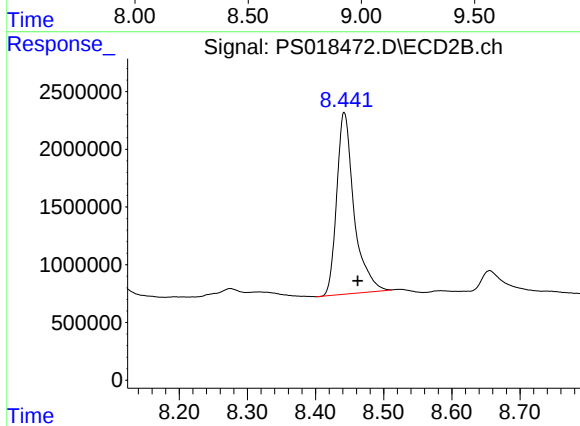

#11 2,4,5-TP (SILVEX)


R.T.: 8.442 min
Delta R.T.: -0.020 min
Response: 27739369
Conc: 6.72 ng/ml

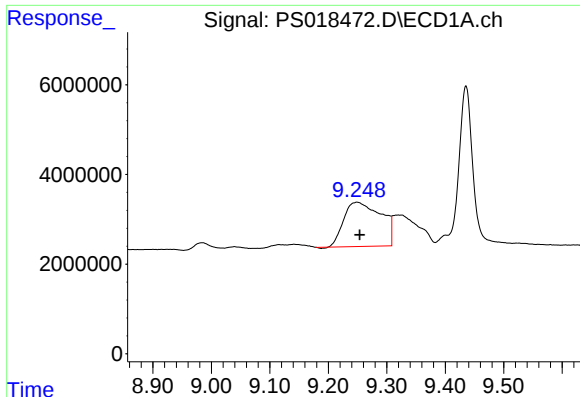

#12 2,4,5-T


R.T.: 9.249 min
Delta R.T.: -0.005 min
Response: 43863702
Conc: 4.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

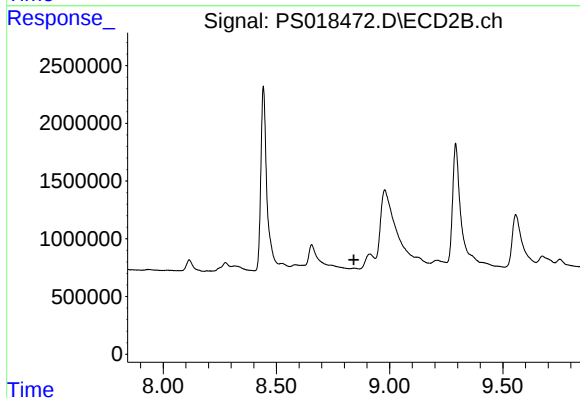


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.842 min
Response: 0
Conc: N.D.

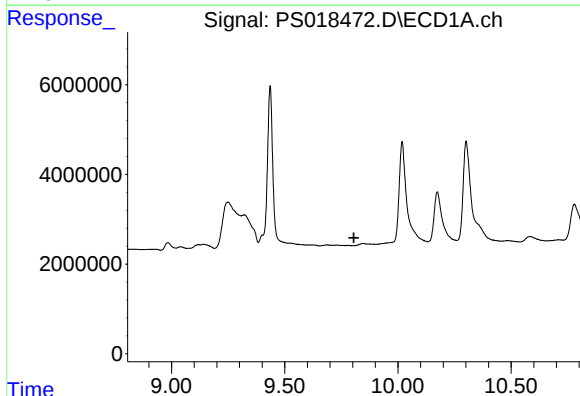


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.806 min
Response: 0
Conc: N.D.

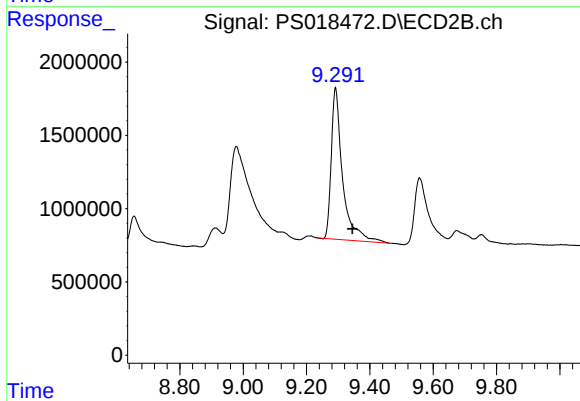

#13 2,4-DB


R.T.: 9.291 min
Delta R.T.: -0.054 min
Response: 25658577
Conc: 47.49 ng/ml

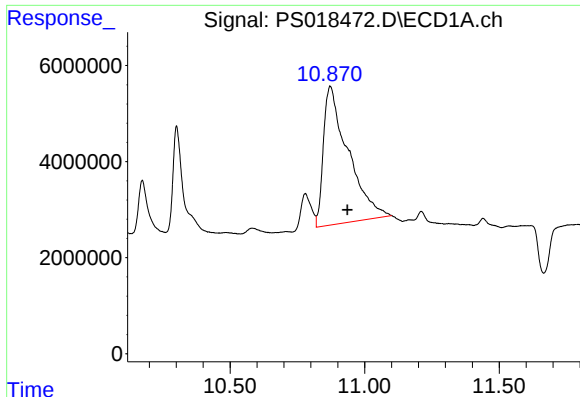

#14 DINOSEB


R.T.: 10.871 min
Delta R.T.: -0.064 min
Response: 183420127
Conc: 23.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

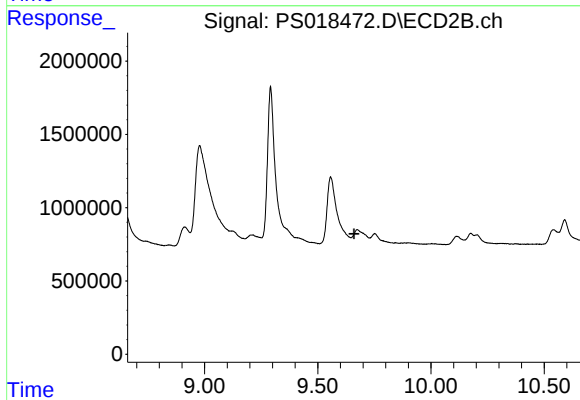


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.660 min
Response: 0
Conc: N.D.

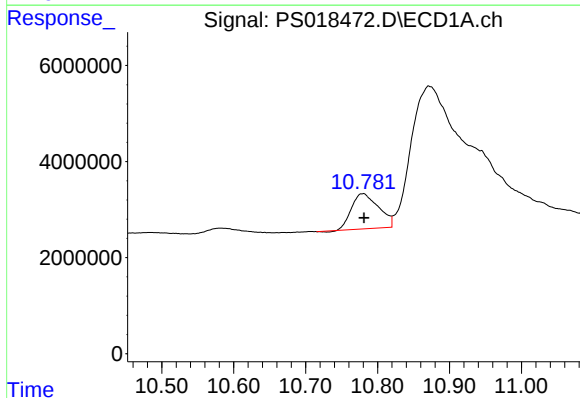

#15 Picloram

R.T.: 10.780 min
Delta R.T.: 0.000 min
Response: 19232211
Conc: 1.51 ng/ml

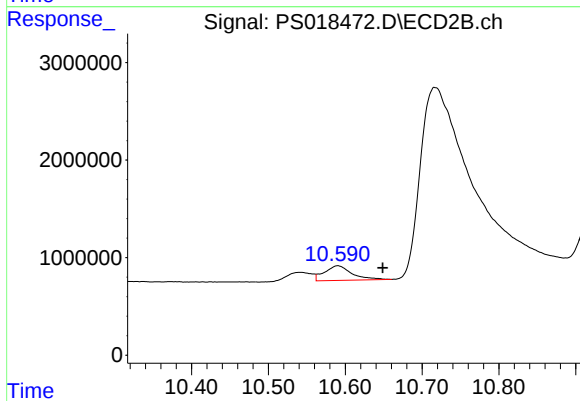

#15 Picloram

R.T.: 10.590 min
Delta R.T.: -0.058 min
Response: 3694831
Conc: N.D.