

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030223\
 Data File : PS022286.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2023 09:17
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 21:32:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
 Quant Title : 8080.M
 QLast Update : Mon Feb 20 13:26:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.314	0.000	524972	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.441	2.514	1050465	576243	<MDL	<MDL #
2) T	3,5-DICHL...	5.621f	0.000	128940	0	<MDL	N.D. #
3) T	4-Nitroph...	6.145	0.000	1873021	0	1.472	N.D. #
5) T	DICAMBA	6.442	6.931f	541242	5271924	<MDL	<MDL #
6) T	MCP	0.000	6.931f	0	5271924	N.D.	<MDL
8) T	DICHLORPROP	7.026	7.546f	2358542	6393814	<MDL	2.601 #
9) T	2,4-D	7.202	0.000	61521461	0	18.764	N.D. #
10) T	Pentachlo...	7.451	8.210	8246442	12850384	<MDL	<MDL #
11) T	2,4,5-TP ...	7.985	8.576	6600358	29114331	<MDL	2.164 #
12) T	2,4,5-T	8.209	8.975	11833349	4953737	<MDL	<MDL #
13) T	2,4-DB	8.729	0.000	2932071	0	1.082	N.D. #
14) T	DINOSEB	0.000	9.778	0	1467243	N.D.	<MDL
15) T	Picloram	9.616	10.704f	42006982	59949513	1.705	3.058 #
16) T	DCPA	10.053	10.704	1300160	59949513	<MDL	3.832 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030223\
Data File : PS022286.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2023 09:17
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 21:32:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
Quant Title : 8080.M
QLast Update : Mon Feb 20 13:26:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

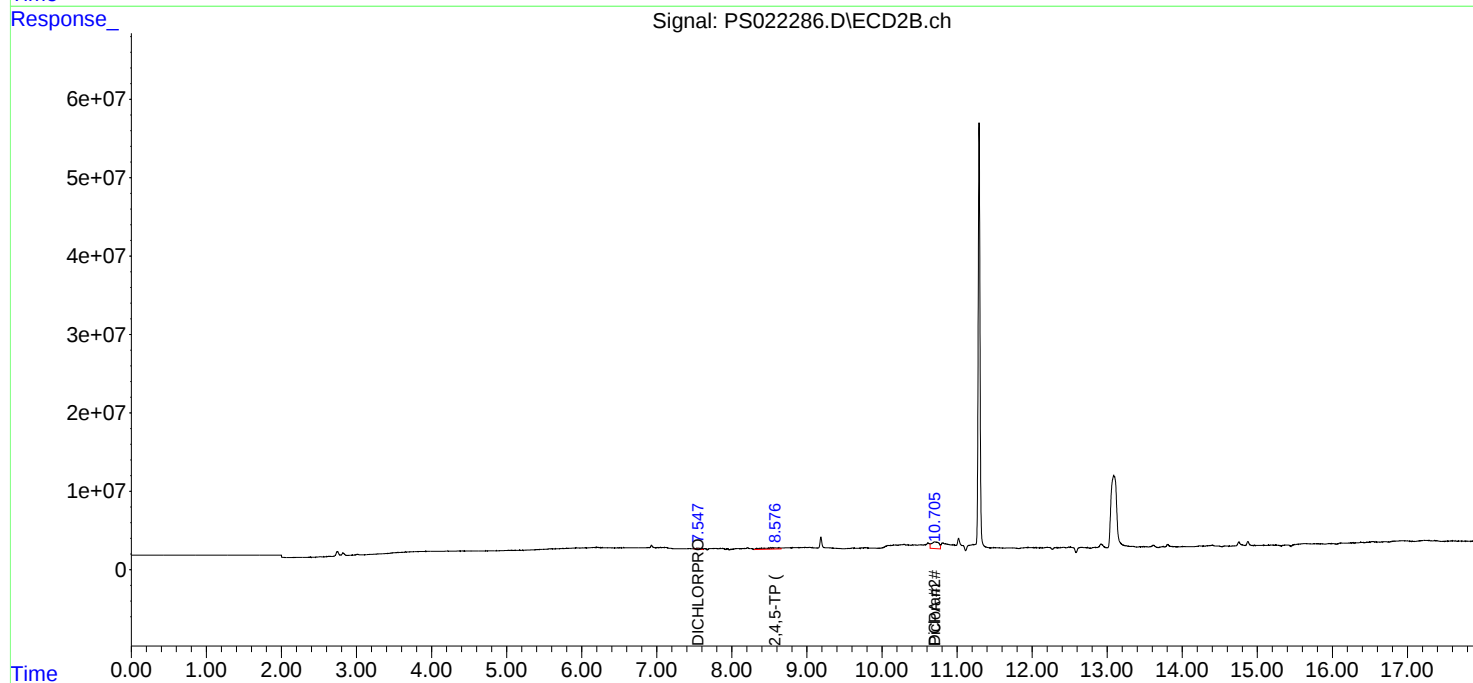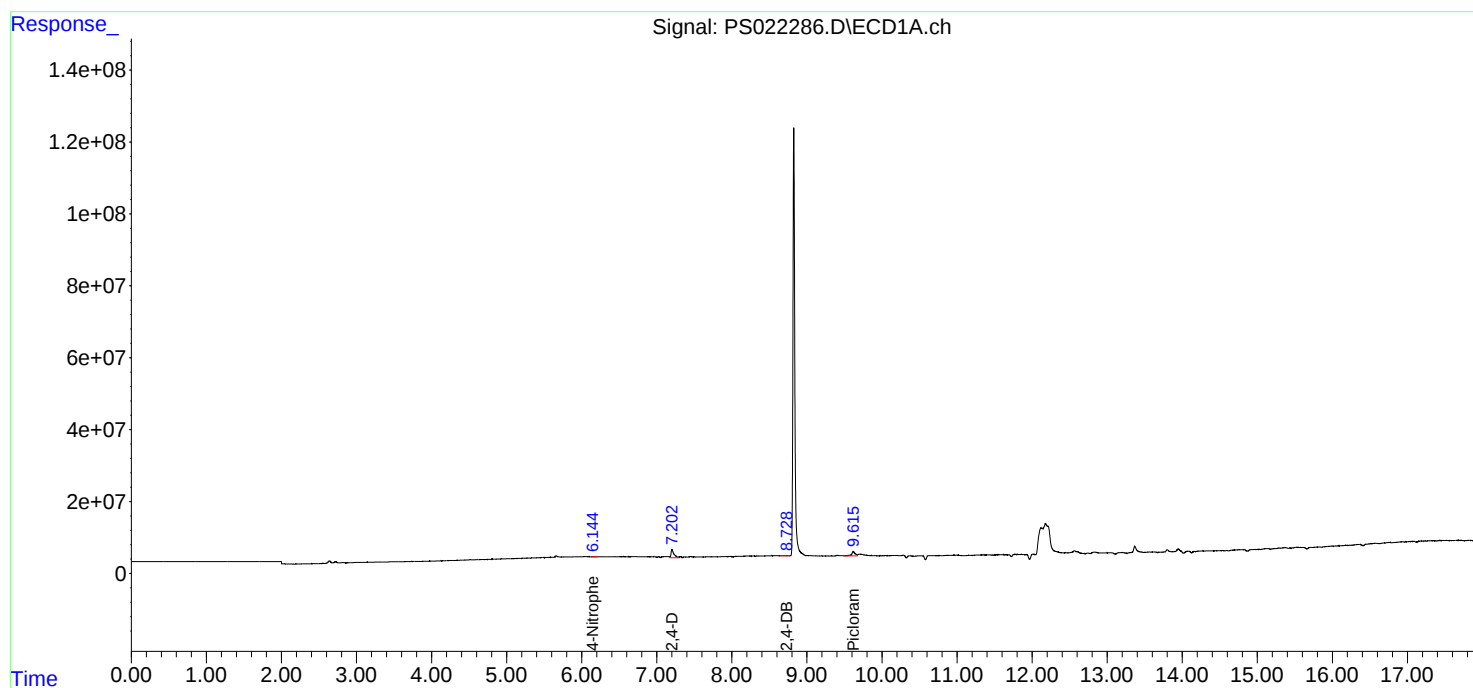


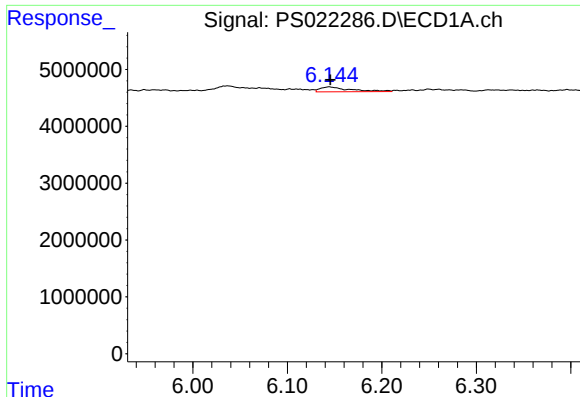

#3 4-Nitrophenol


R.T.: 6.145 min
Delta R.T.: -0.001 min
Response: 1873021
Conc: 1.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

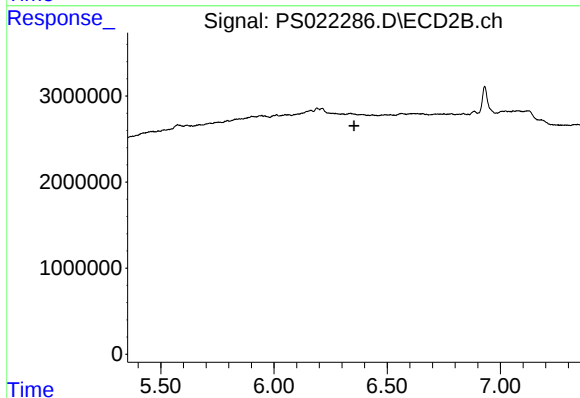


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.353 min
Response: 0
Conc: N.D.

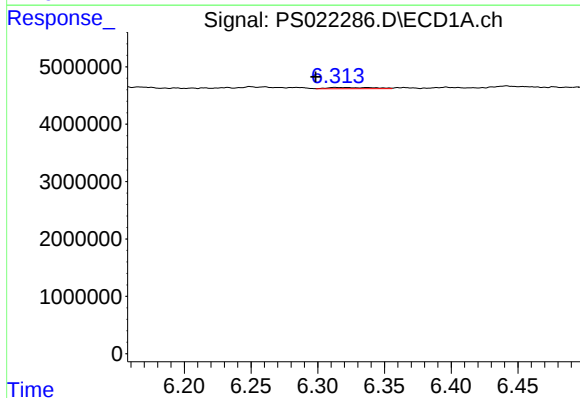


#4 2,4-DCAA

R.T.: 6.314 min
Delta R.T.: 0.016 min
Response: 524972
Conc: N.D.

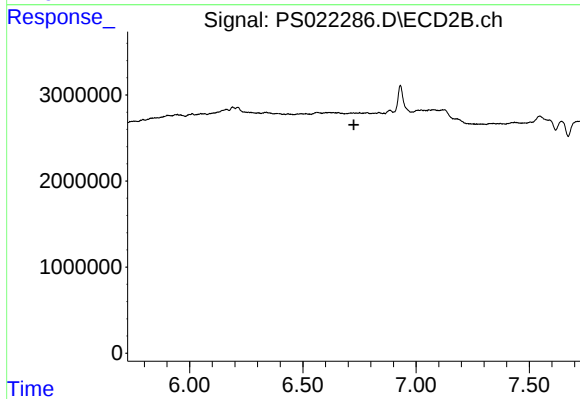

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.726 min
Response: 0
Conc: N.D.

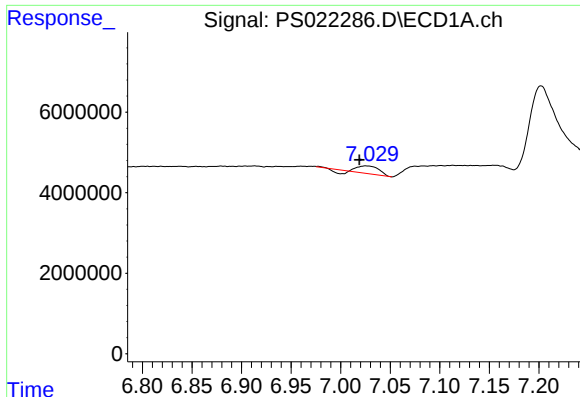

#8 DICHLORPROP


R.T.: 7.026 min
Delta R.T.: 0.007 min
Response: 2358542
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

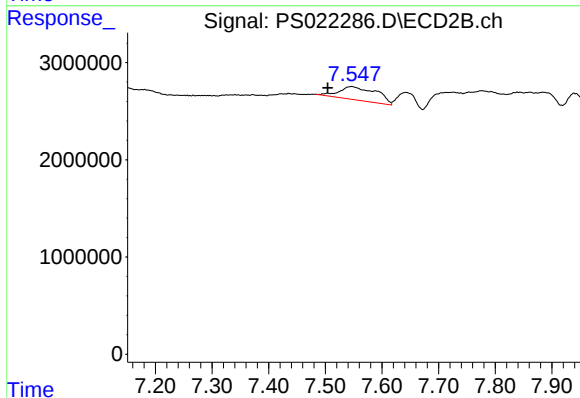


#8 DICHLORPROP

R.T.: 7.546 min
Delta R.T.: 0.042 min
Response: 6393814
Conc: 2.60 ng/ml

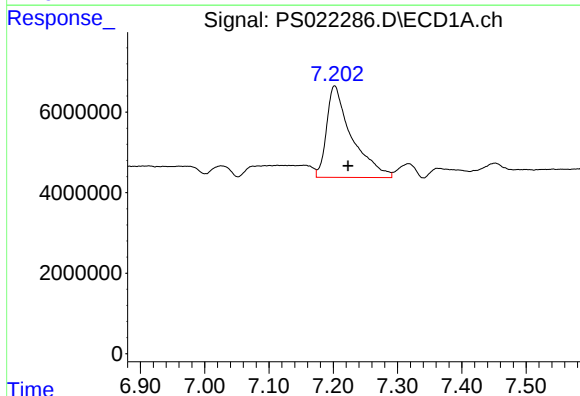


#9 2,4-D

R.T.: 7.202 min
Delta R.T.: -0.020 min
Response: 61521461
Conc: 18.76 ng/ml

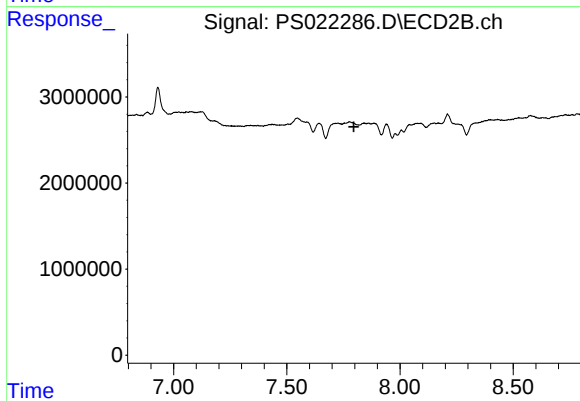

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.796 min
Response: 0
Conc: N.D.

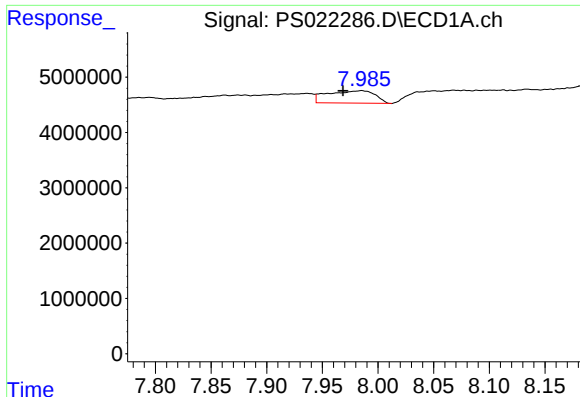

#11 2,4,5-TP (SILVEX)


R.T.: 7.985 min
Delta R.T.: 0.016 min
Response: 6600358
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

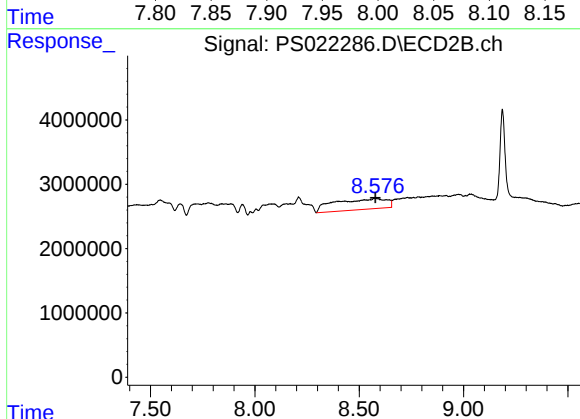


#11 2,4,5-TP (SILVEX)

R.T.: 8.576 min
Delta R.T.: -0.001 min
Response: 29114331
Conc: 2.16 ng/ml

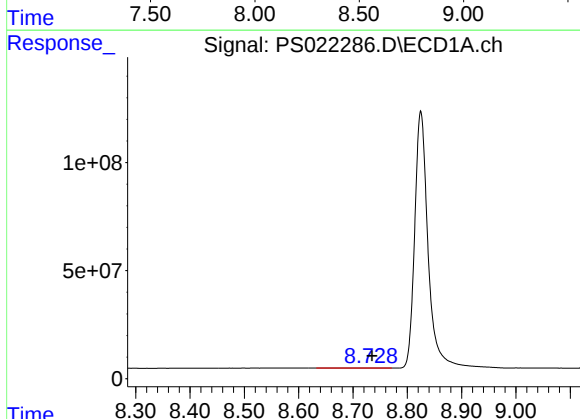


#13 2,4-DB

R.T.: 8.729 min
Delta R.T.: -0.006 min
Response: 2932071
Conc: 1.08 ng/ml

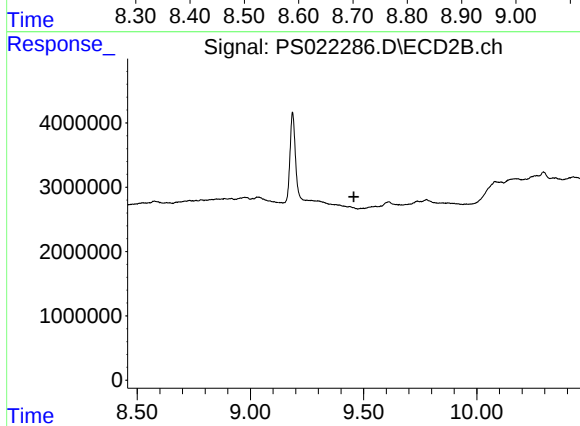

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.457 min
Response: 0
Conc: N.D.

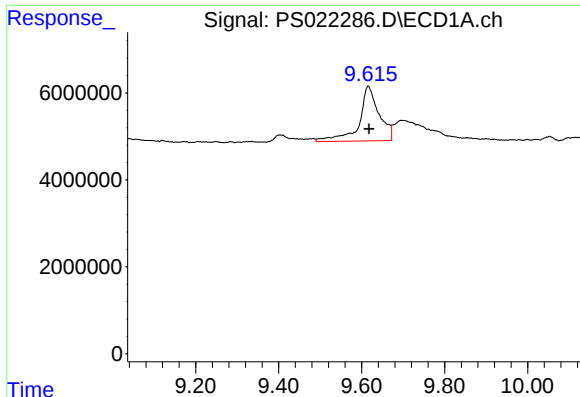

#15 Picloram


R.T.: 9.616 min
Delta R.T.: -0.002 min
Response: 42006982
Conc: 1.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

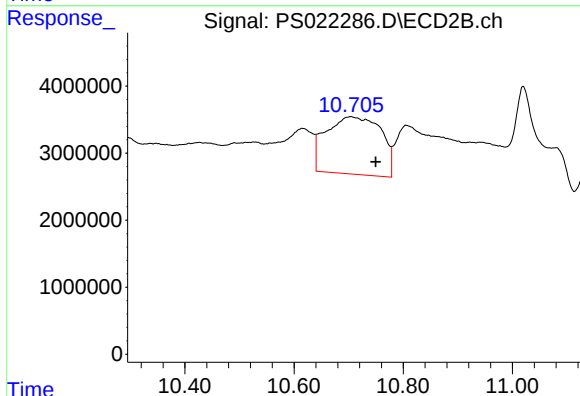


#15 Picloram

R.T.: 10.704 min
Delta R.T.: -0.046 min
Response: 59949513
Conc: 3.06 ng/ml

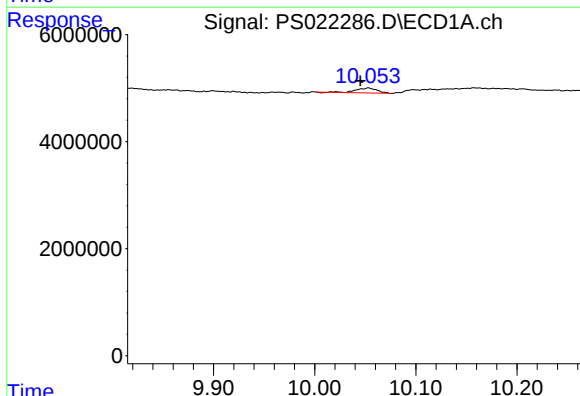

#16 DCPA

R.T.: 10.053 min
Delta R.T.: 0.007 min
Response: 1300160
Conc: N.D.

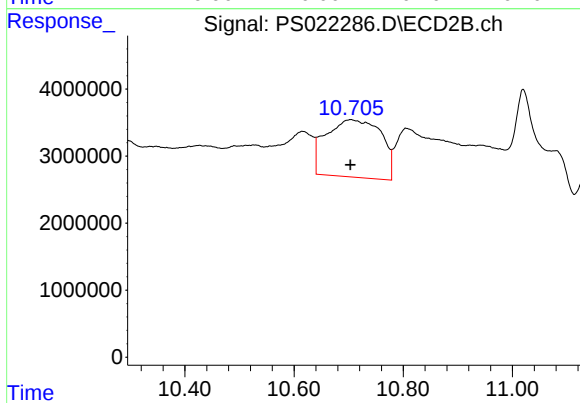

#16 DCPA

R.T.: 10.704 min
Delta R.T.: 0.000 min
Response: 59949513
Conc: 3.83 ng/ml