

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030223\
 Data File : PS022287.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2023 10:21
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 21:33:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
 Quant Title : 8080.M
 QLast Update : Mon Feb 20 13:26:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.305	6.723	1280.6E6	1184.5E6	516.653	564.303
Target Compounds							
1) T	Dalapon	2.439	2.516	1194233	871597	<MDL	<MDL #
2) T	3,5-DICHL...	5.672	0.000	30435831	0	8.187	N.D. #
3) T	4-Nitroph...	6.163	0.000	6333313	0	4.977	N.D. #
5) T	DICAMBA	0.000	6.937f	0	51981545	N.D.	5.379
6) T	MCP	0.000	6.937f	0	51981545	N.D.	6.809
7) T	MCPA	6.691	0.000	614351	0	<MDL	N.D. #
9) T	2,4-D	7.213	0.000	204.2E6	0	62.276	N.D. #
10) T	Pentachlo...	7.458	8.216	11919881	12115755	<MDL	<MDL #
11) T	2,4,5-TP ...	7.947	8.592	679059	2623397	<MDL	<MDL #
12) T	2,4,5-T	8.179f	9.016f	175455	2090587	<MDL	<MDL #
13) T	2,4-DB	8.684f	0.000	180640	0	<MDL	N.D. #
14) T	DINOSEB	9.788	9.783	13820688	3040739	1.006	<MDL #
15) T	Picloram	9.628	10.703f	70330804	28430995	2.855	1.450 #
16) T	DCPA	10.053	10.703	5759485	28430995	<MDL	1.817 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030223\
Data File : PS022287.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2023 10:21
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 21:33:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
Quant Title : 8080.M
QLast Update : Mon Feb 20 13:26:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

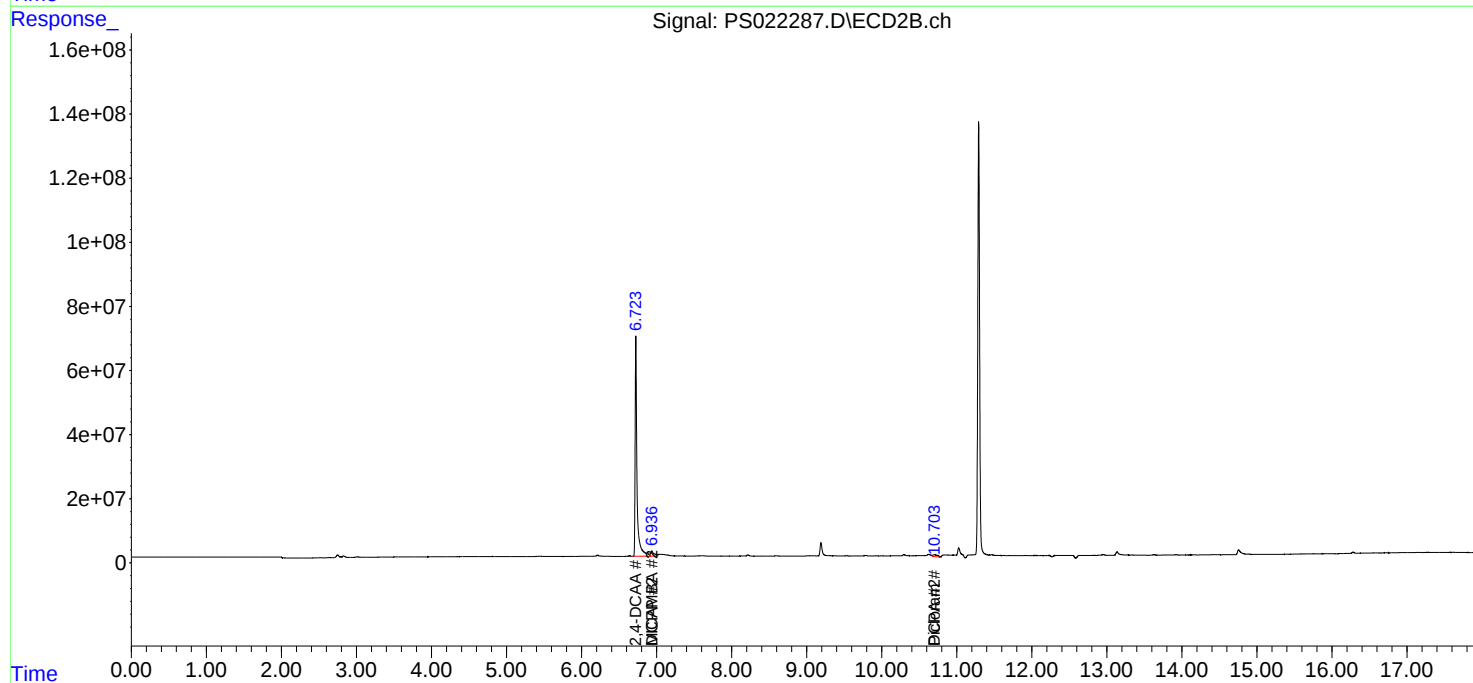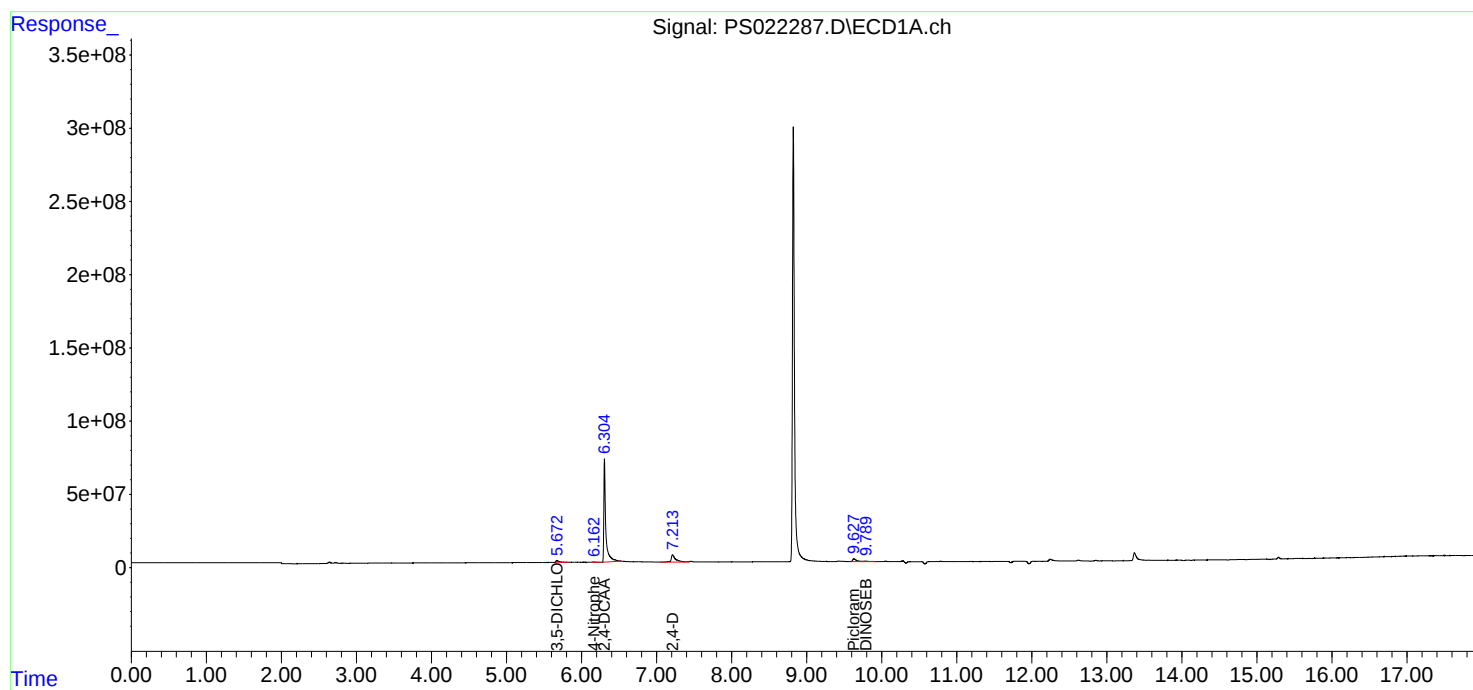


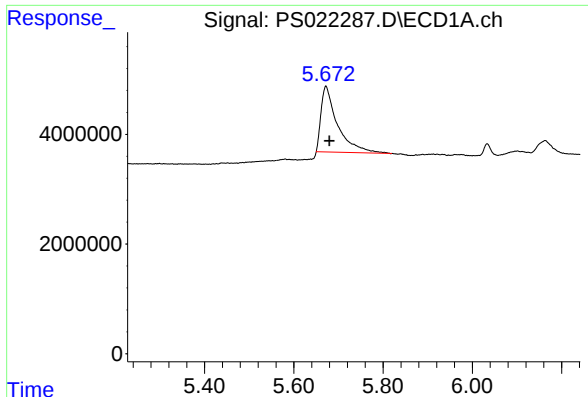

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.672 min
Delta R.T.: -0.008 min
Response: 30435831
Conc: 8.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

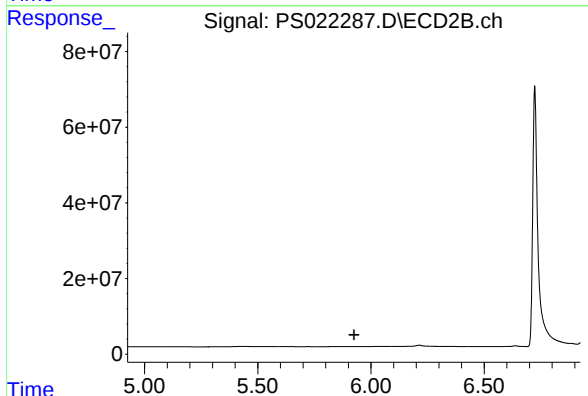


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.925 min
Response: 0
Conc: N.D.

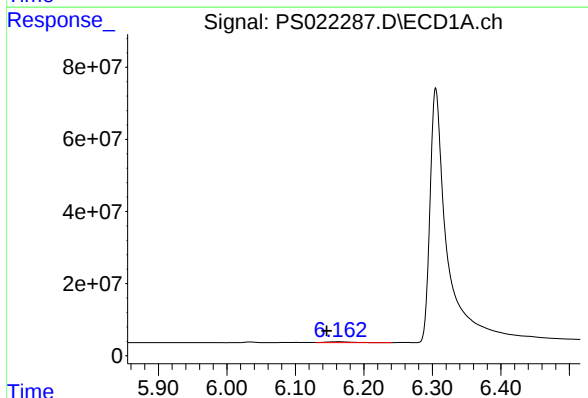


#3 4-Nitrophenol

R.T.: 6.163 min
Delta R.T.: 0.017 min
Response: 6333313
Conc: 4.98 ng/ml

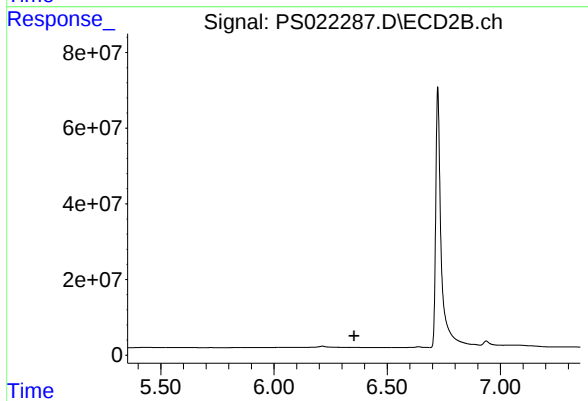

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.353 min
Response: 0
Conc: N.D.

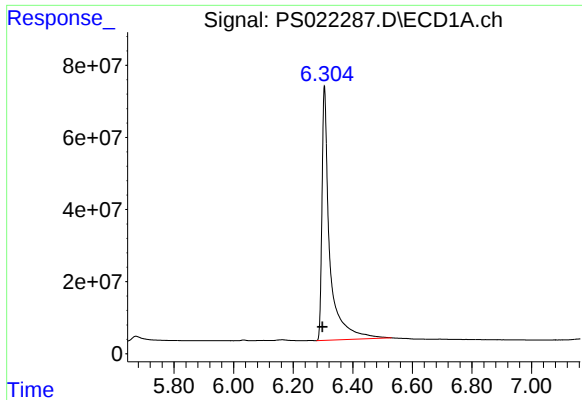

#4 2,4-DCAA


R.T.: 6.305 min
Delta R.T.: 0.007 min
Response: 1280623357
Conc: 516.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

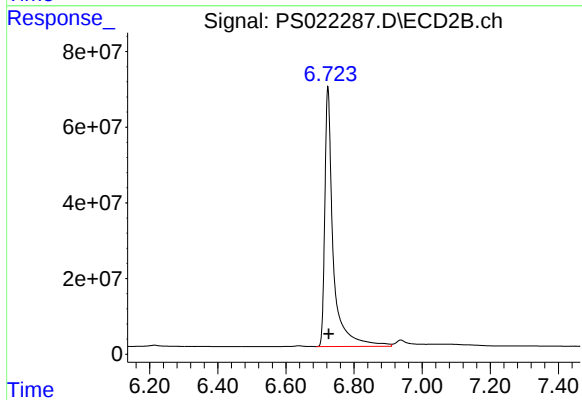


#4 2,4-DCAA

R.T.: 6.723 min
Delta R.T.: -0.002 min
Response: 1184451663
Conc: 564.30 ng/ml

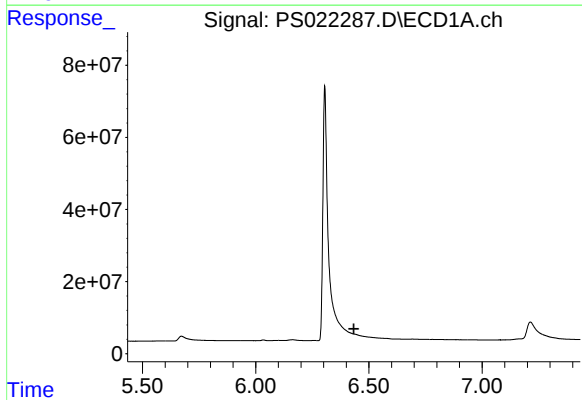


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

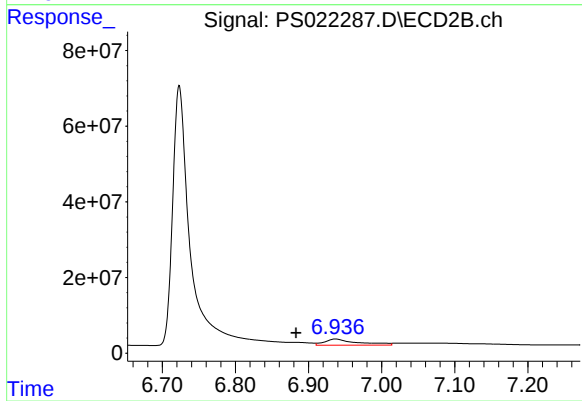

#5 DICAMBA


R.T.: 6.937 min
Delta R.T.: 0.054 min
Response: 51981545
Conc: 5.38 ng/ml

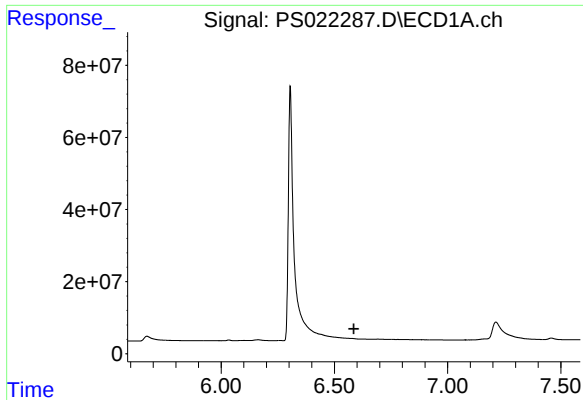

#6 MCP


R.T.: 0.000 min
Exp R.T.: 6.586 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

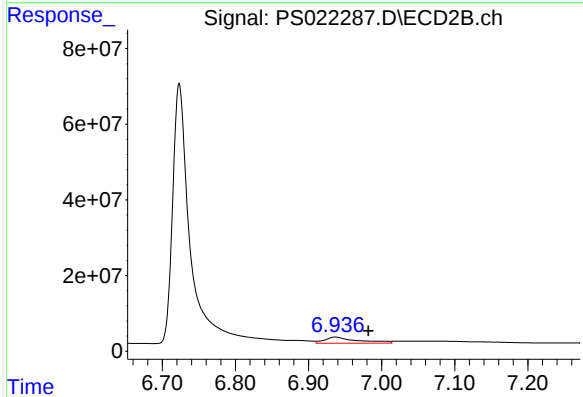


#6 MCP

R.T.: 6.937 min
Delta R.T.: -0.045 min
Response: 51981545
Conc: 6.81 ug/ml

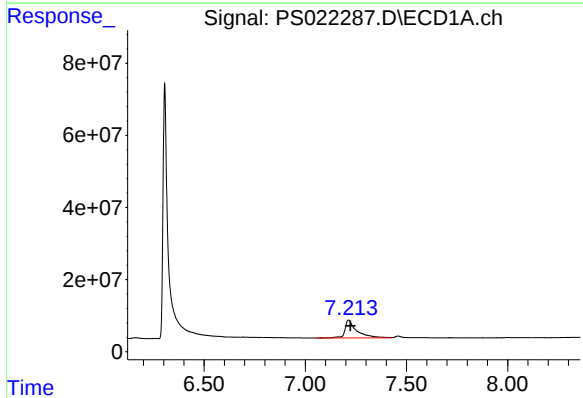


#9 2,4-D

R.T.: 7.213 min
Delta R.T.: -0.009 min
Response: 204184864
Conc: 62.28 ng/ml

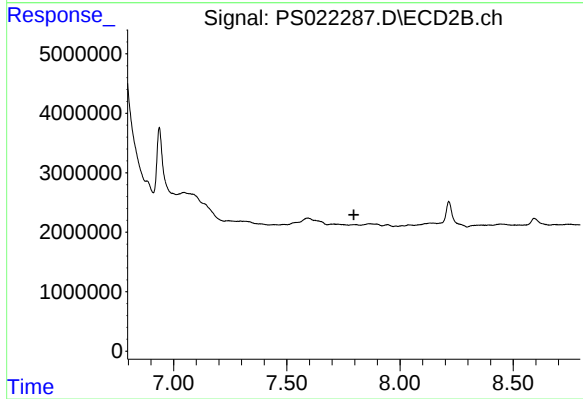

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.796 min
Response: 0
Conc: N.D.

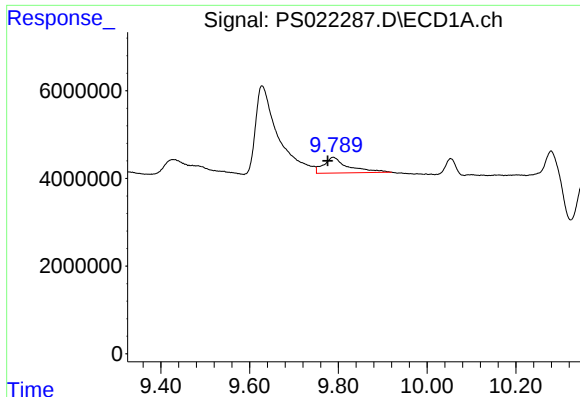

#14 DINOSEB


R.T.: 9.788 min
Delta R.T.: 0.012 min
Response: 13820688
Conc: 1.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

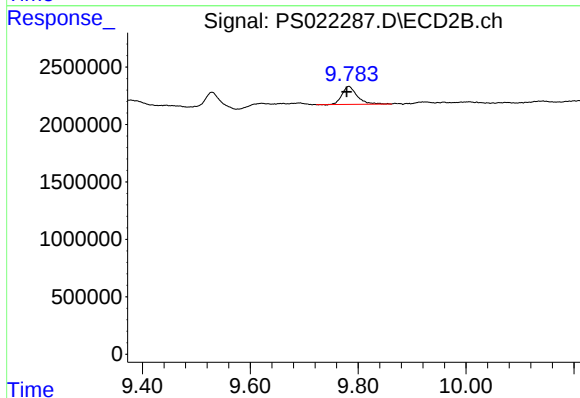


#14 DINOSEB

R.T.: 9.783 min
Delta R.T.: 0.004 min
Response: 3040739
Conc: N.D.

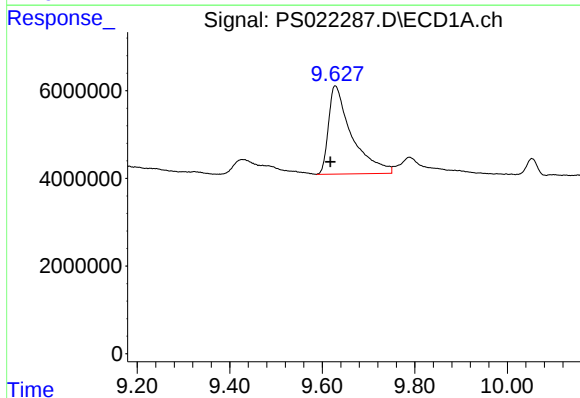


#15 Picloram

R.T.: 9.628 min
Delta R.T.: 0.011 min
Response: 70330804
Conc: 2.86 ng/ml

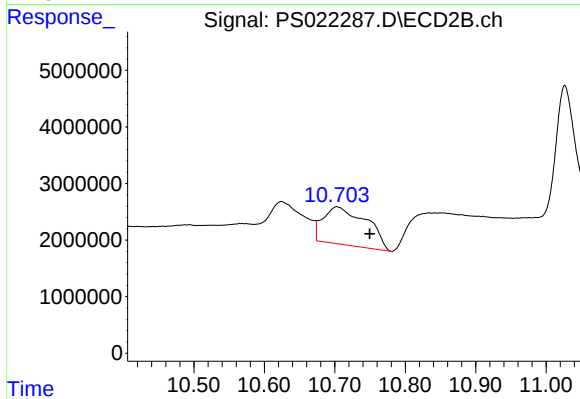

#15 Picloram


R.T.: 10.703 min
Delta R.T.: -0.047 min
Response: 28430995
Conc: 1.45 ng/ml

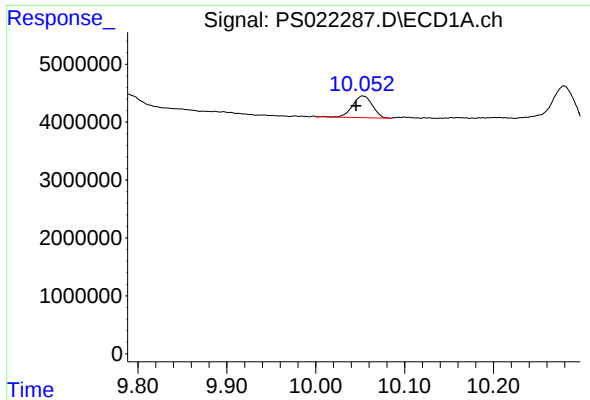

#16 DCPA

R.T.: 10.053 min
Delta R.T.: 0.008 min
Response: 5759485
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

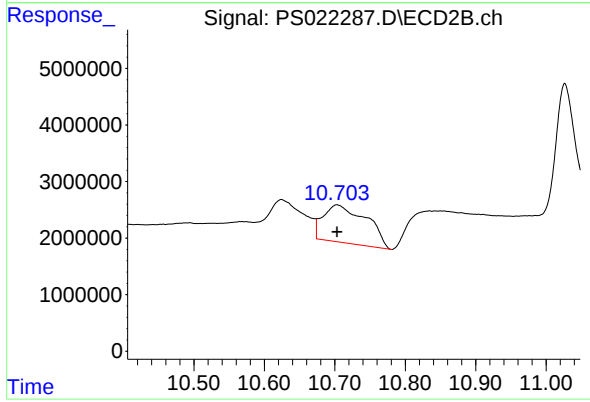

#16 DCPA

R.T.: 10.703 min
Delta R.T.: 0.000 min
Response: 28430995
Conc: 1.82 ng/ml