

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030321\
 Data File : PS014116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2021 12:56
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 15:33:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030321.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 03 15:10:33 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.207	6.900	441.4E6	189.5E6	443.594	501.694
Target Compounds							
5) T	DICAMBA	0.000	7.104	0	3281544	N.D.	2.063
6) T	MCPD	0.000	7.174	0	2681948	N.D.	2.077
13) T	2,4-DB	0.000	9.688	0	676098	N.D.	2.323



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030321\
Data File : PS014116.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2021 12:56
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 15:33:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030321.M
Quant Title : 8080.M
QLast Update : Wed Mar 03 15:10:33 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

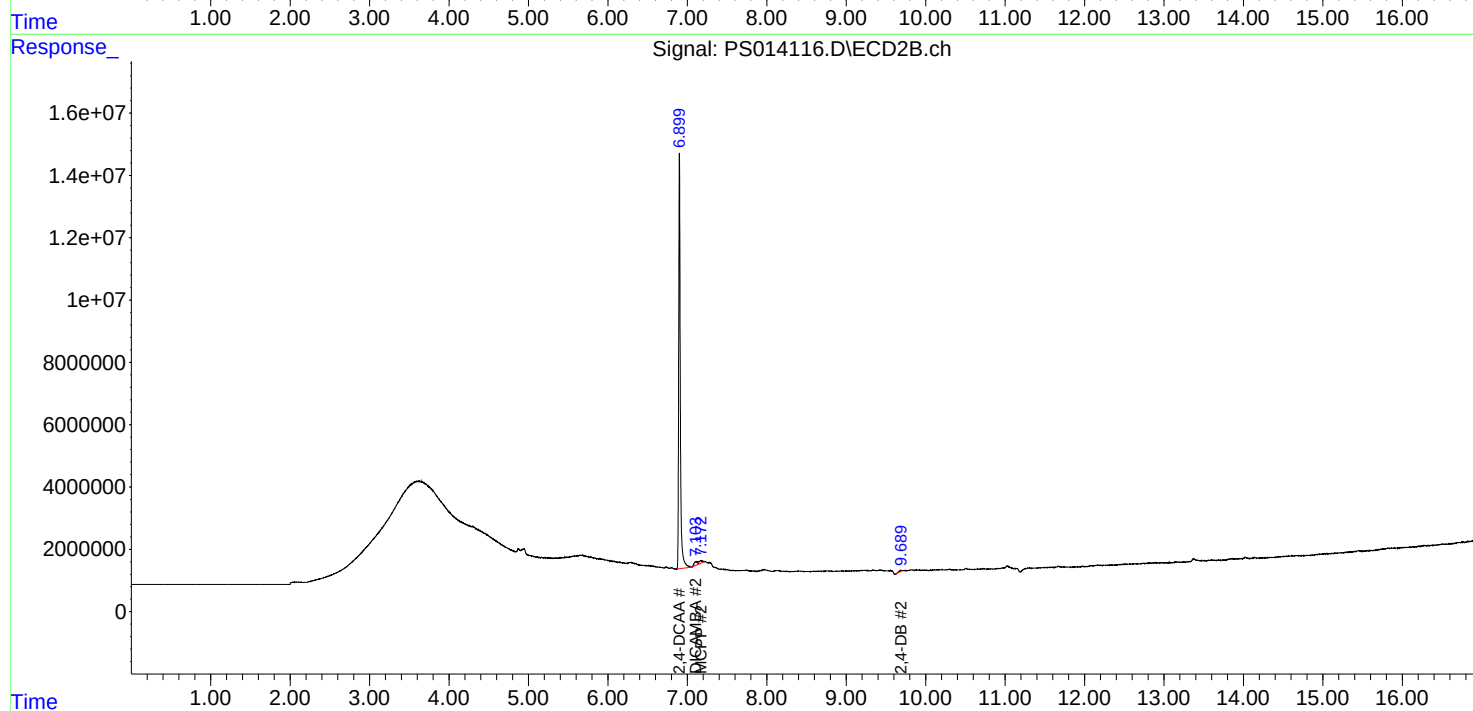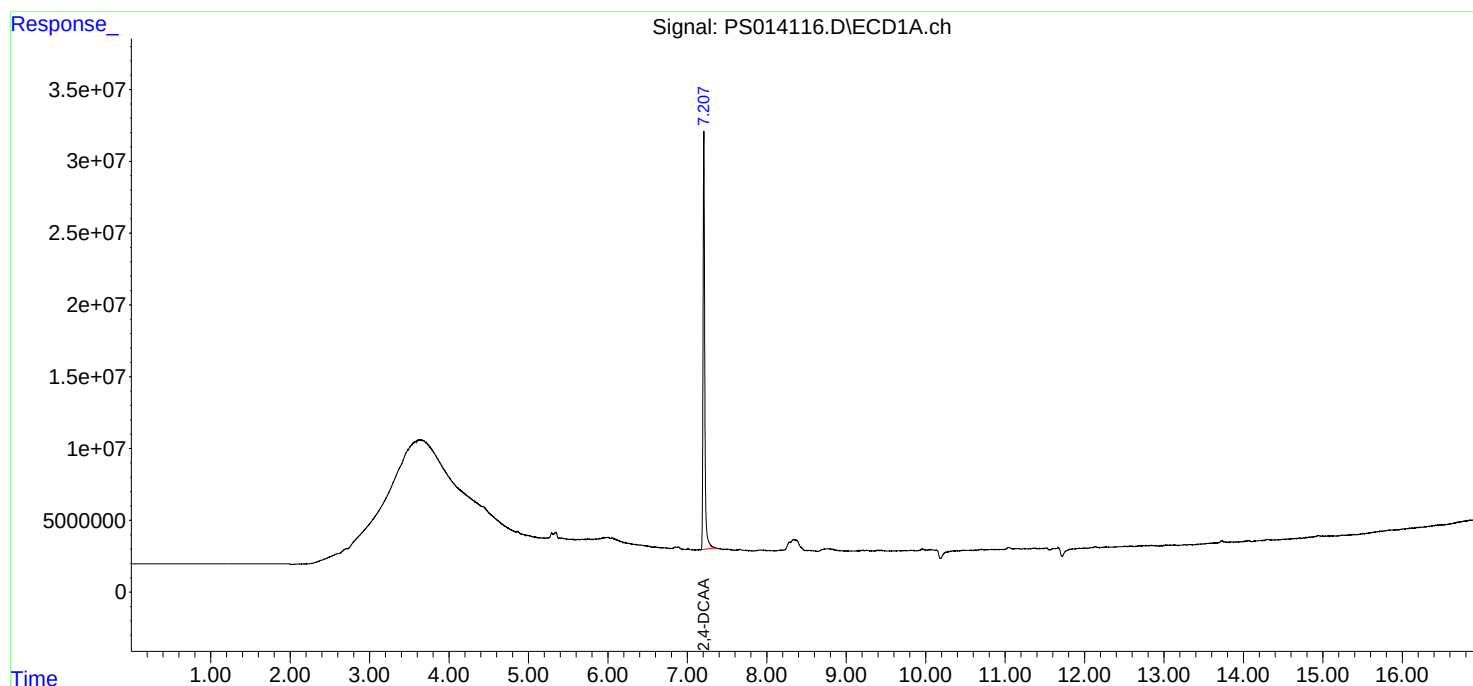


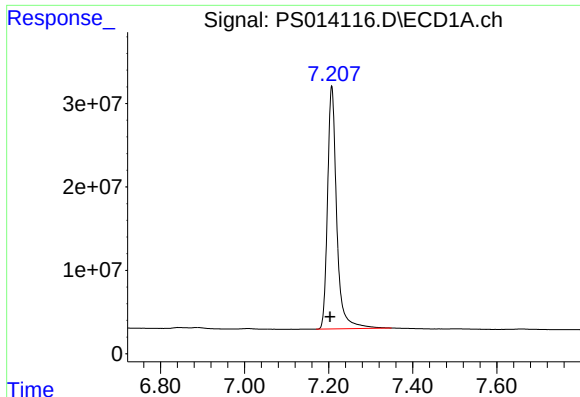

#4 2,4-DCAA


R.T.: 7.207 min
Delta R.T.: 0.004 min
Response: 441392956
Conc: 443.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

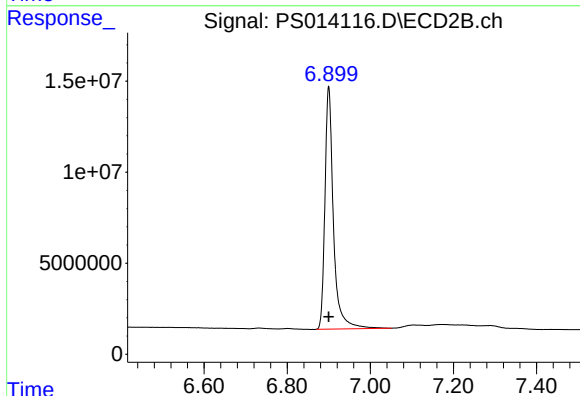


#4 2,4-DCAA

R.T.: 6.900 min
Delta R.T.: 0.000 min
Response: 189489684
Conc: 501.69 ng/ml

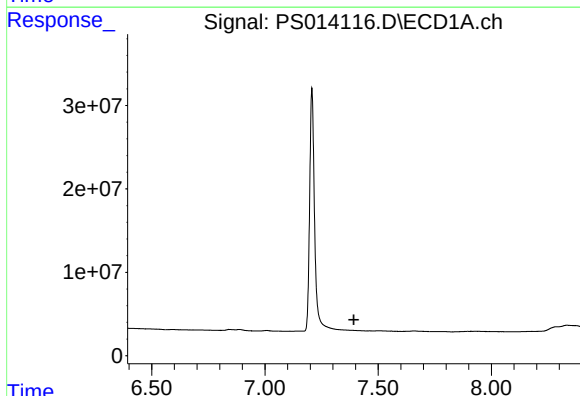


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.393 min
Response: 0
Conc: N.D.

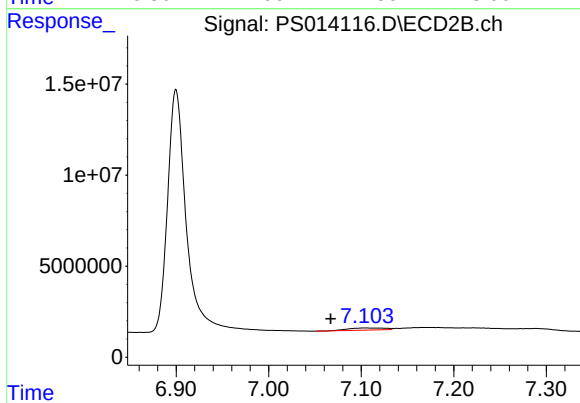

#5 DICAMBA


R.T.: 7.104 min
Delta R.T.: 0.037 min
Response: 3281544
Conc: 2.06 ng/ml

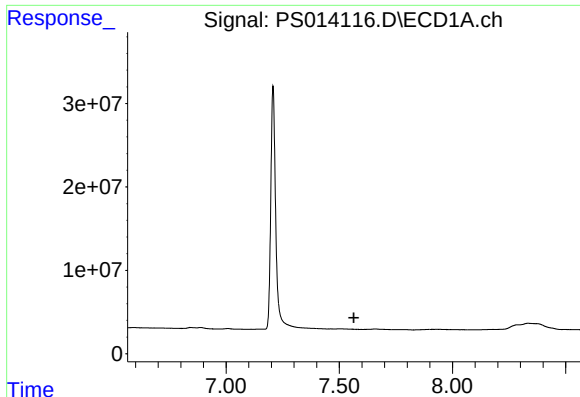

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.565 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

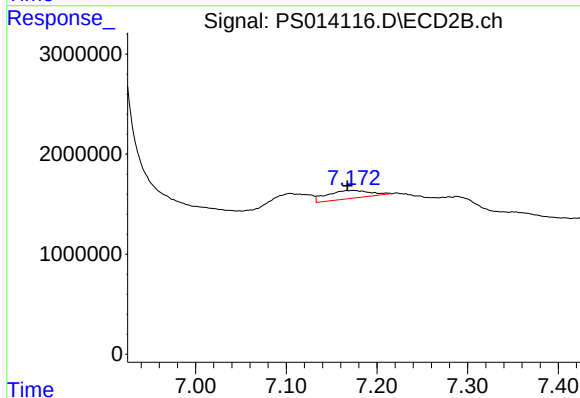


#6 MCPP

R.T.: 7.174 min
Delta R.T.: 0.006 min
Response: 2681948
Conc: 2.08 ug/ml

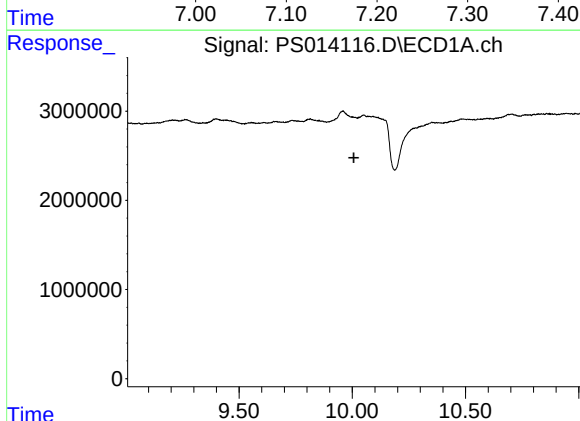

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.007 min
Response: 0
Conc: N.D.

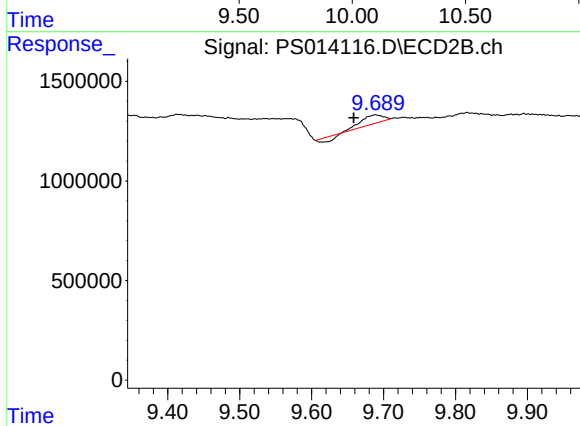

#13 2,4-DB

R.T.: 9.688 min
Delta R.T.: 0.030 min
Response: 676098
Conc: 2.32 ng/ml