

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030322\
 Data File : PS018484.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2022 10:44
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 00:10:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
5)	T	DICAMBA	7.211	6.787	7518044	2758040	1.144 <MDL #
8)	T	DICHLORPROP	7.899	7.422	3385747	3432267	2.002 4.662 #
9)	T	2,4-D	8.139	7.699	3830410	2655995	1.878 2.837 #
10)	T	Pentachlo...	8.419	8.096	22277678	9289863	<MDL <MDL #
11)	T	2,4,5-TP ...	8.970	8.457	31874514	7070625	3.348 1.713 #
12)	T	2,4,5-T	9.258	8.844	40816498	12173835	4.058 3.093
13)	T	2,4-DB	9.812	0.000	11300870	0	6.503 N.D. #
14)	T	DINOSEB	10.939	9.656	23540360	6388024	3.030 2.197 #
15)	T	Picloram	10.788	10.648	345.3E6	183.7E6	27.176 31.770
16)	T	DCPA	11.208	10.579	20320703	21468160	1.690 4.324 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030322\
Data File : PS018484.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2022 10:44
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 00:10:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

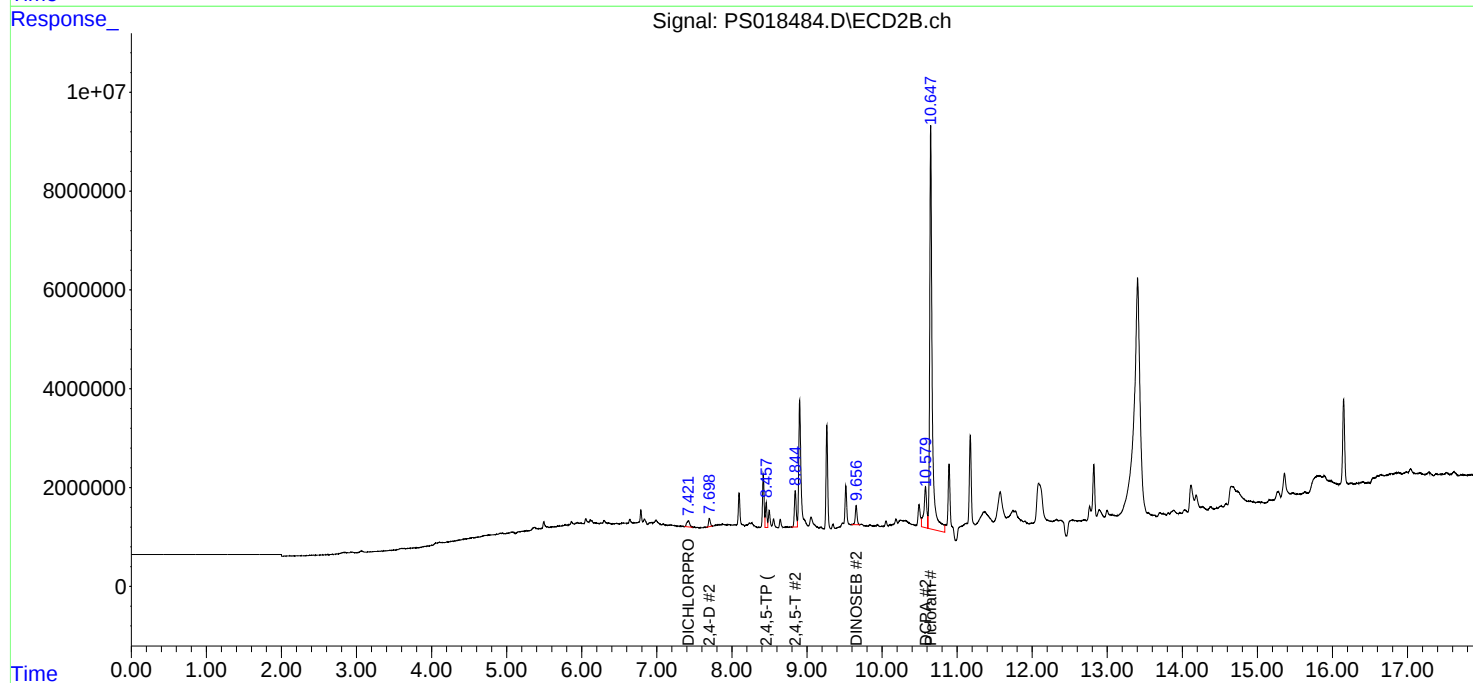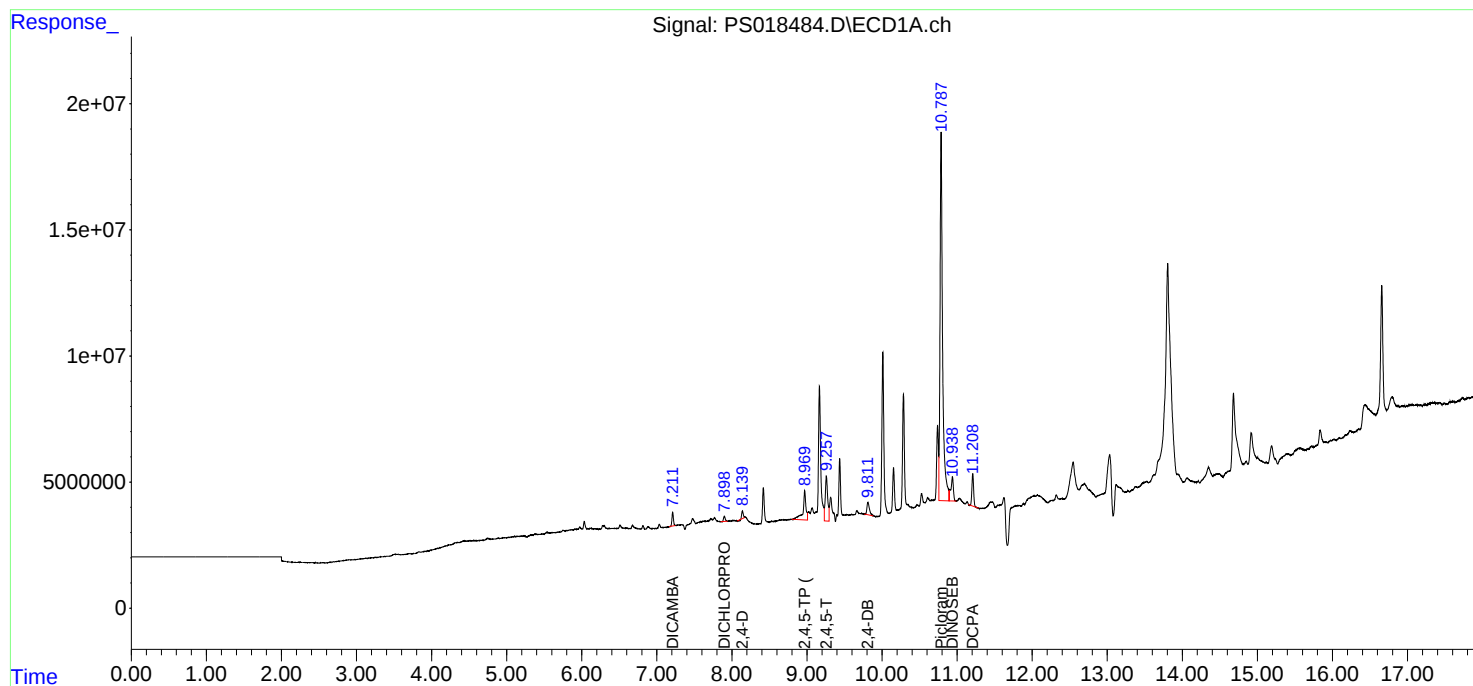


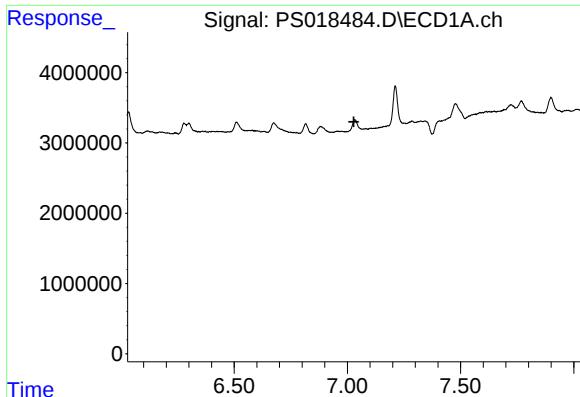

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.029 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

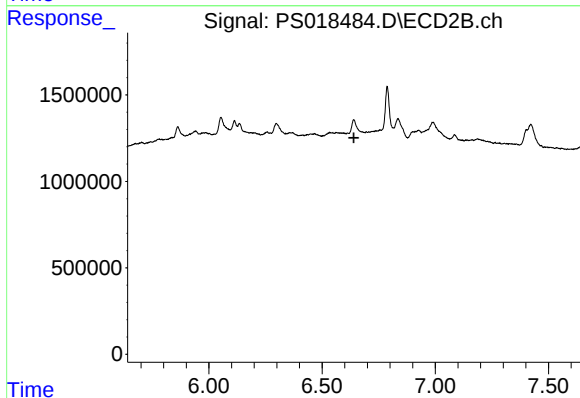


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

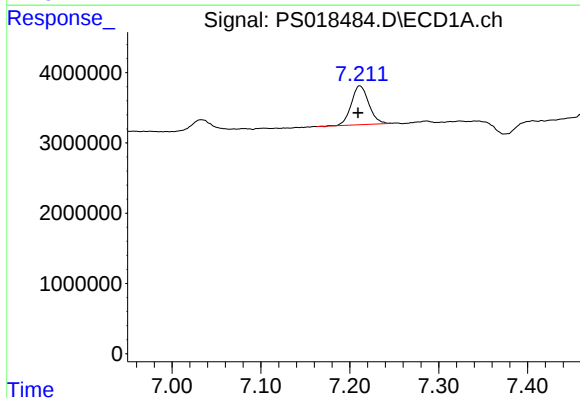


#5 DICAMBA

R.T.: 7.211 min
Delta R.T.: 0.002 min
Response: 7518044
Conc: 1.14 ng/ml

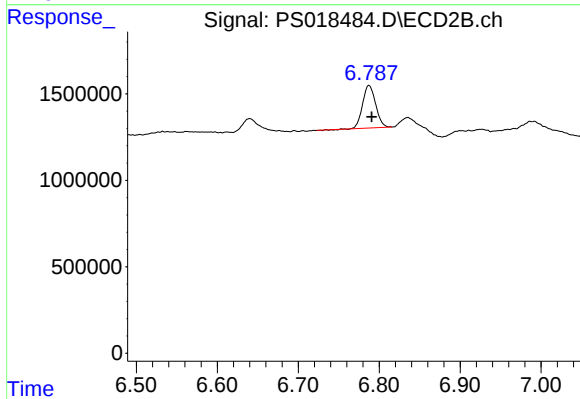

#5 DICAMBA


R.T.: 6.787 min
Delta R.T.: -0.004 min
Response: 2758040
Conc: N.D.

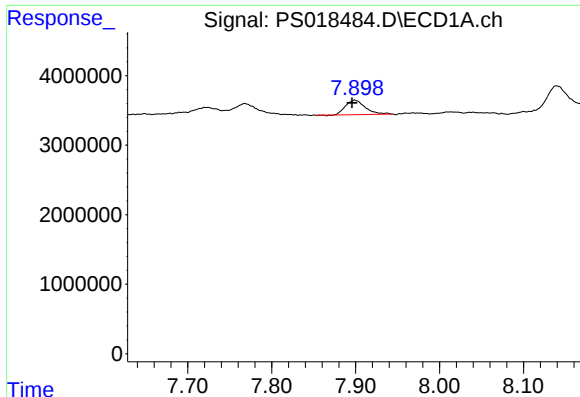

#8 DICHLORPROP


R.T.: 7.899 min
Delta R.T.: 0.003 min
Response: 3385747
Conc: 2.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

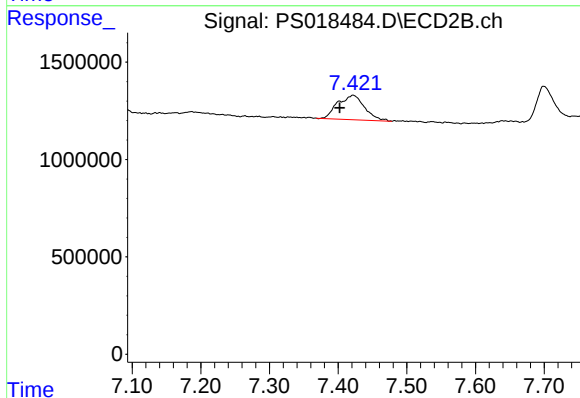


#8 DICHLORPROP

R.T.: 7.422 min
Delta R.T.: 0.019 min
Response: 3432267
Conc: 4.66 ng/ml

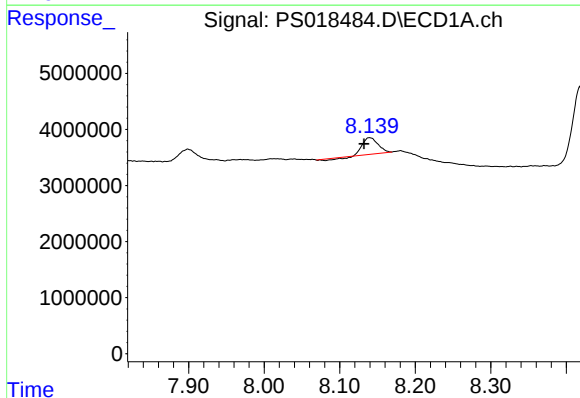


#9 2,4-D

R.T.: 8.139 min
Delta R.T.: 0.007 min
Response: 3830410
Conc: 1.88 ng/ml

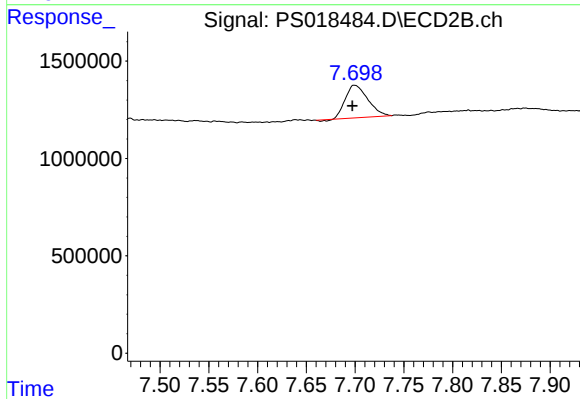

#9 2,4-D


R.T.: 7.699 min
Delta R.T.: 0.002 min
Response: 2655995
Conc: 2.84 ng/ml

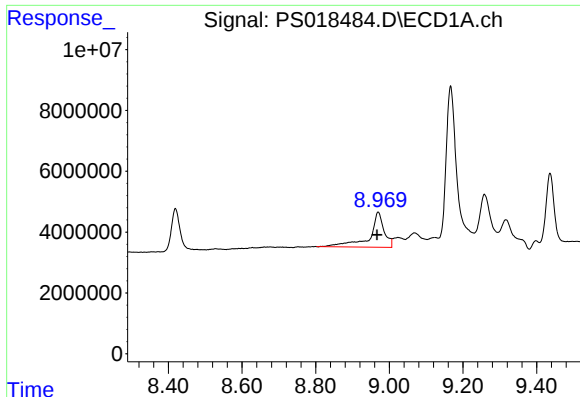

#11 2,4,5-TP (SILVEX)


R.T.: 8.970 min
Delta R.T.: 0.003 min
Response: 31874514
Conc: 3.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

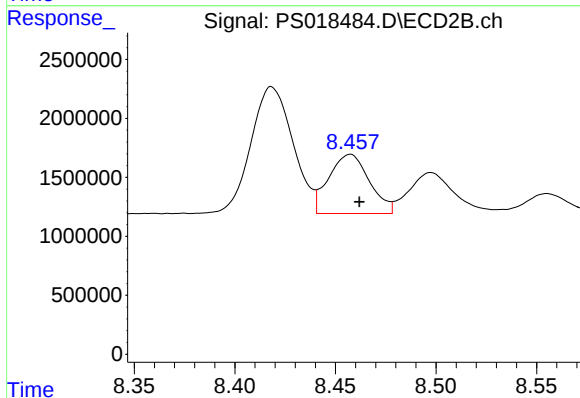


#11 2,4,5-TP (SILVEX)

R.T.: 8.457 min
Delta R.T.: -0.005 min
Response: 7070625
Conc: 1.71 ng/ml

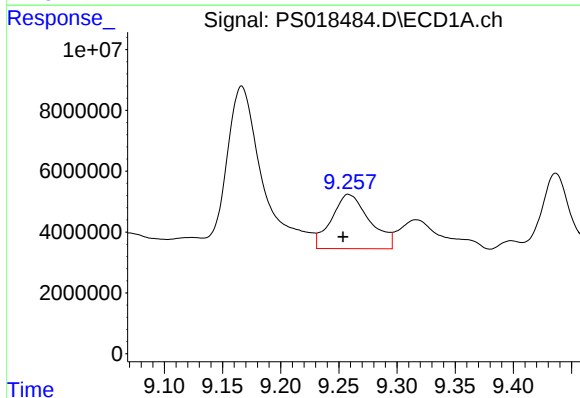


#12 2,4,5-T

R.T.: 9.258 min
Delta R.T.: 0.005 min
Response: 40816498
Conc: 4.06 ng/ml

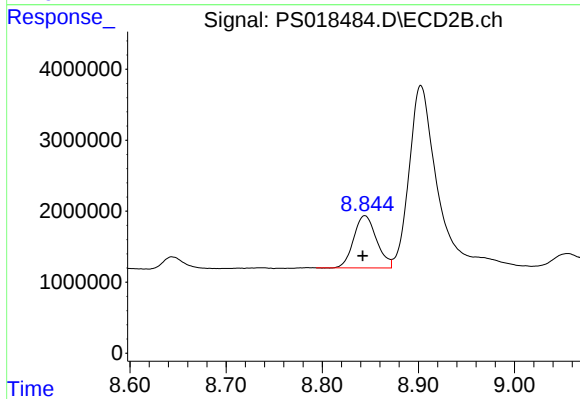

#12 2,4,5-T


R.T.: 8.844 min
Delta R.T.: 0.002 min
Response: 12173835
Conc: 3.09 ng/ml

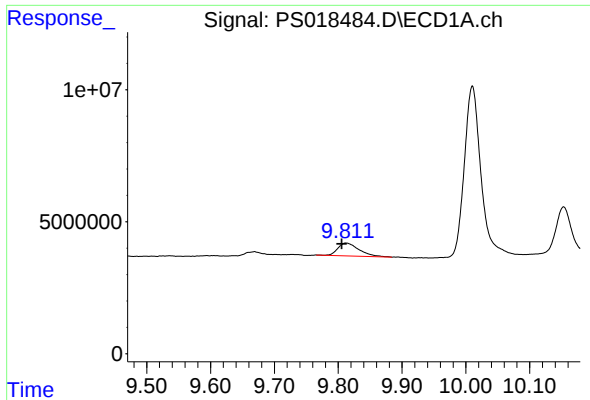

#13 2,4-DB


R.T.: 9.812 min
Delta R.T.: 0.006 min
Response: 11300870
Conc: 6.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

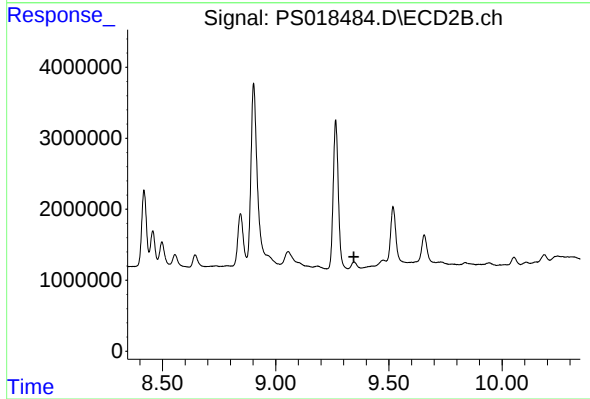


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.345 min
Response: 0
Conc: N.D.

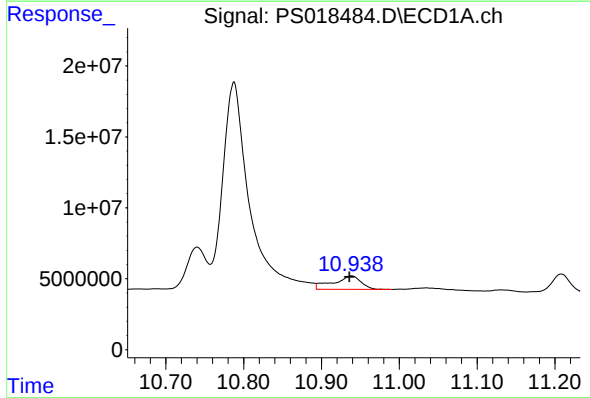


#14 DINOSEB

R.T.: 10.939 min
Delta R.T.: 0.003 min
Response: 23540360
Conc: 3.03 ng/ml

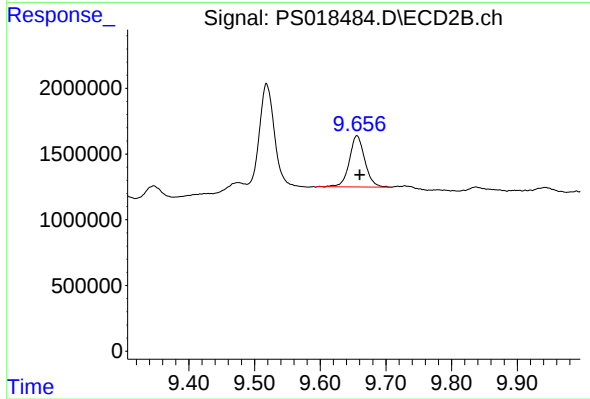

#14 DINOSEB


R.T.: 9.656 min
Delta R.T.: -0.004 min
Response: 6388024
Conc: 2.20 ng/ml

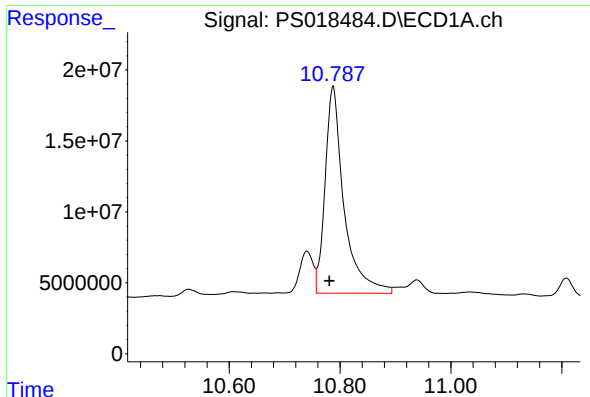

#15 Picloram


R.T.: 10.788 min
Delta R.T.: 0.007 min
Response: 345299762
Conc: 27.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

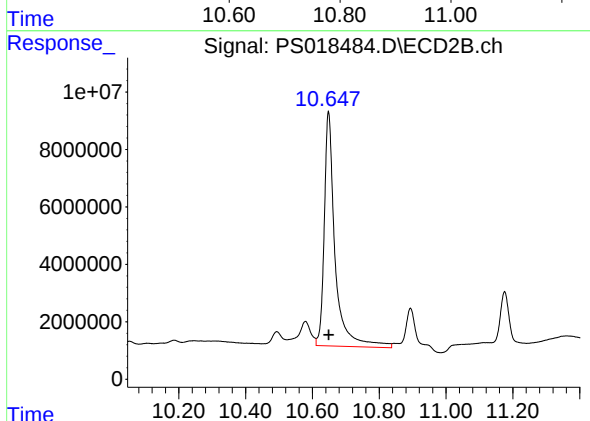


#15 Picloram

R.T.: 10.648 min
Delta R.T.: 0.000 min
Response: 183723351
Conc: 31.77 ng/ml

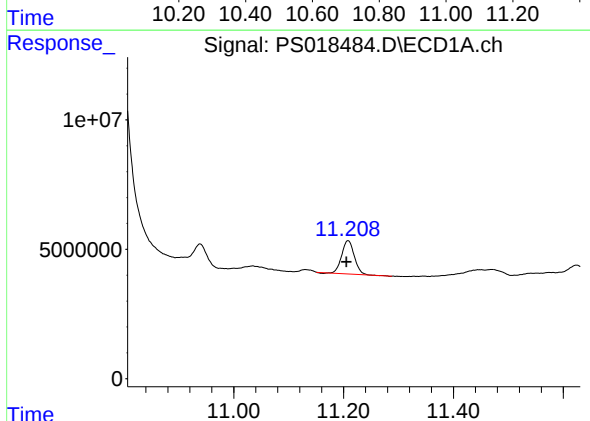

#16 DCPA

R.T.: 11.208 min
Delta R.T.: 0.003 min
Response: 20320703
Conc: 1.69 ng/ml

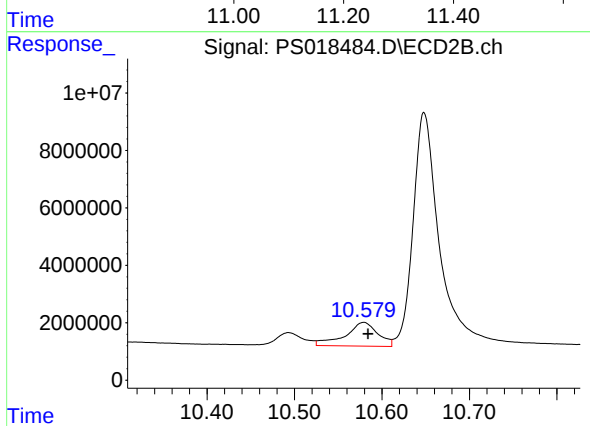

#16 DCPA

R.T.: 10.579 min
Delta R.T.: -0.005 min
Response: 21468160
Conc: 4.32 ng/ml