

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030322\
 Data File : PS018485.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2022 14:20
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 00:11:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.029	6.636	639.2E6	324.9E6	384.150	487.651 #
Target Compounds							
5) T	DICAMBA	7.216	6.793	8542198	4792726	1.299	1.707 #
8) T	DICHLORPROP	0.000	7.413	0	1588111	N.D.	2.157
9) T	2,4-D	8.171	7.727	12500121	3911641	6.128	4.179 #
10) T	Pentachlo...	8.426	8.103	20461916	9173652	<MDL	<MDL #
11) T	2,4,5-TP ...	8.975	8.460	15485083	8037253	1.626	1.947
12) T	2,4,5-T	9.277	8.863	39896720	12111600	3.966	3.077
13) T	2,4-DB	9.848f	9.275f	7812962	39572692	4.496	73.246 #
14) T	DINOSEB	10.940	9.663	59534707	7529759	7.663	2.590 #
15) T	Picloram	10.762	10.671	6334499	156.2E6	<MDL	27.003 #
16) T	DCPA	11.210	10.584	19481450	9930063	1.620	2.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030322\
Data File : PS018485.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2022 14:20
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 00:11:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

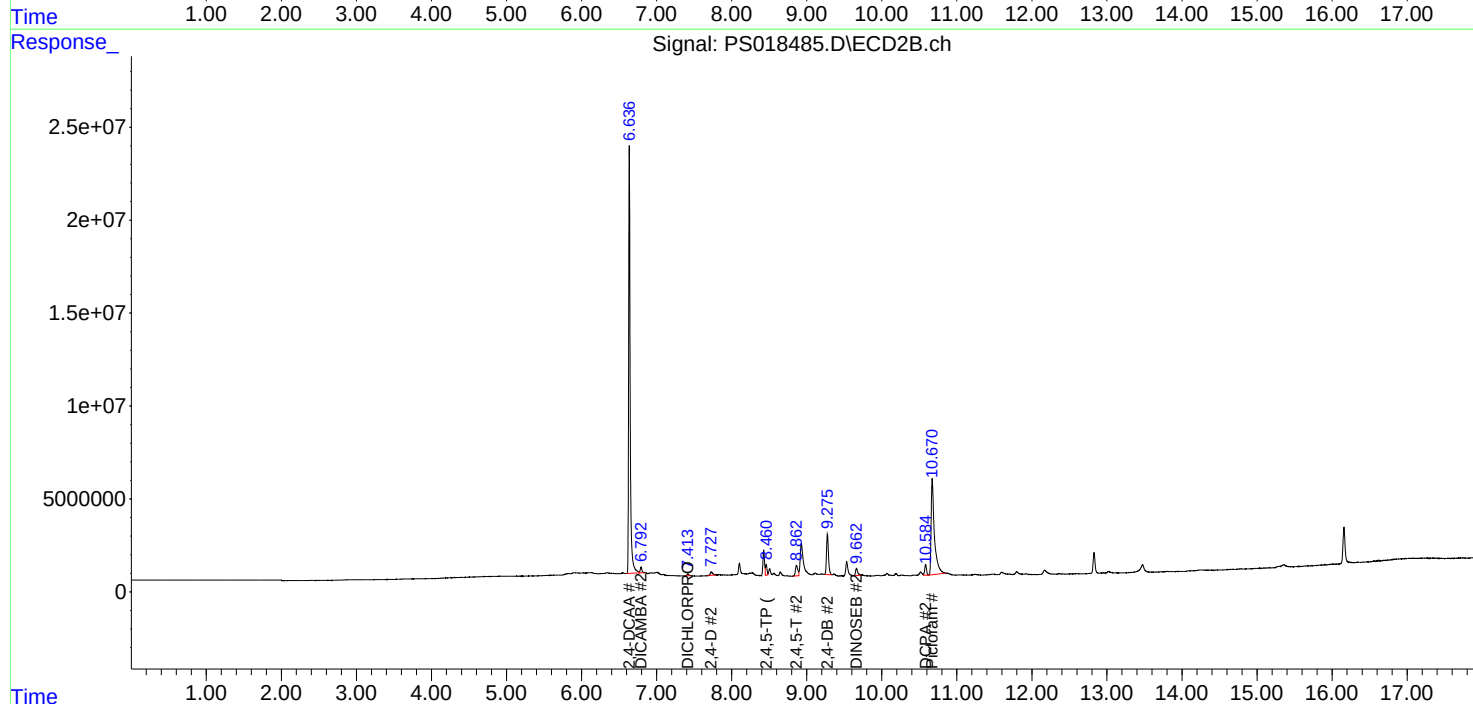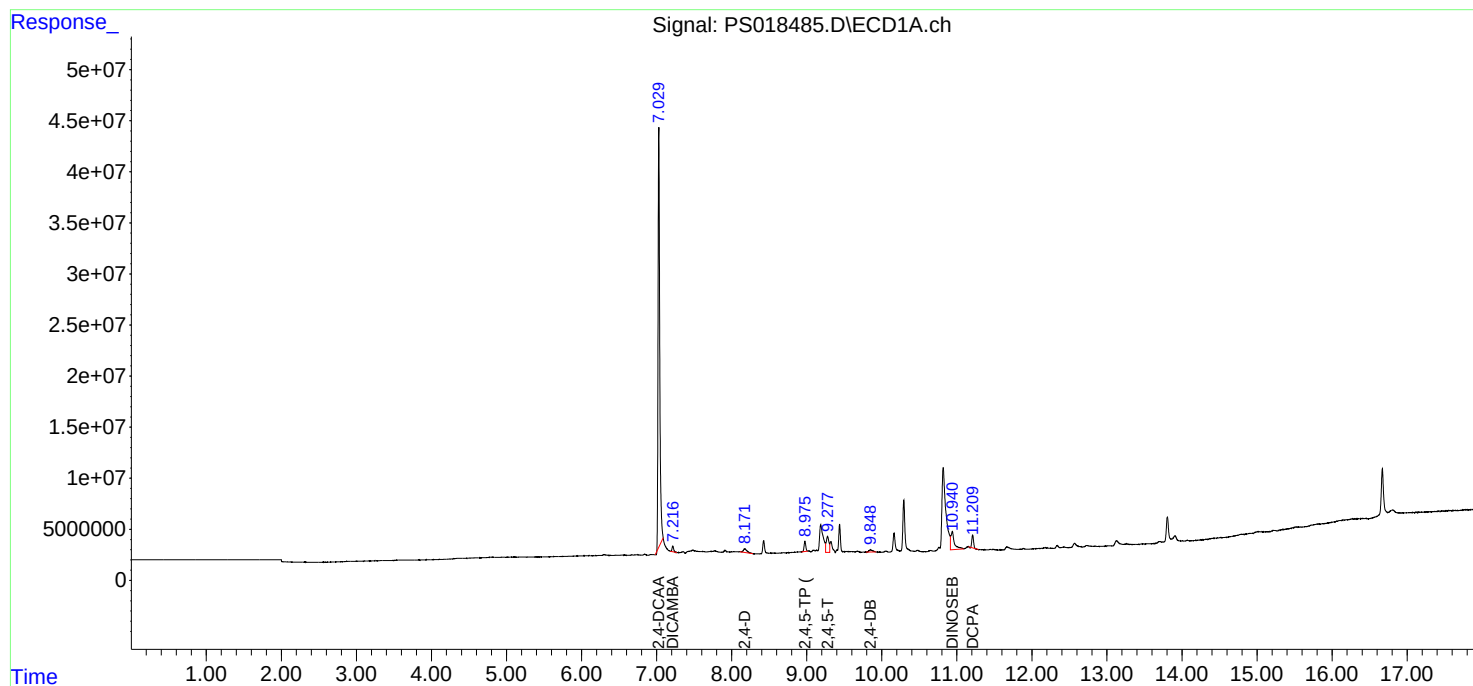


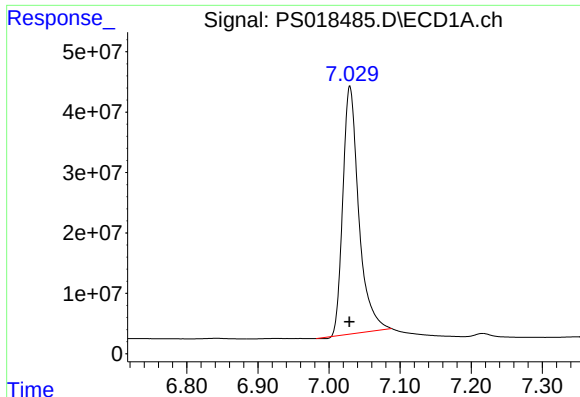

#4 2,4-DCAA


R.T.: 7.029 min
Delta R.T.: 0.000 min
Response: 639244479
Conc: 384.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

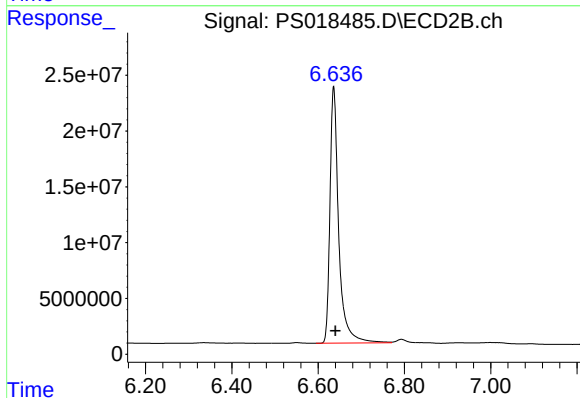


#4 2,4-DCAA

R.T.: 6.636 min
Delta R.T.: -0.004 min
Response: 324942219
Conc: 487.65 ng/ml

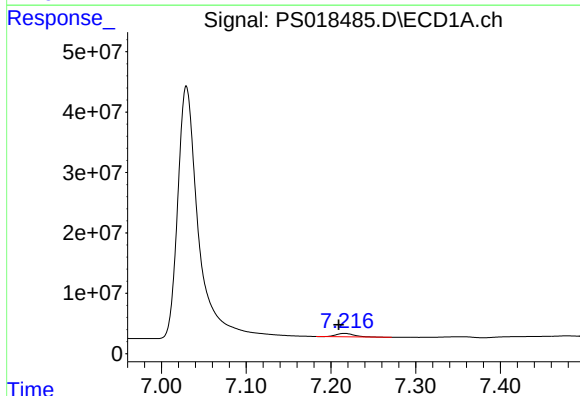


#5 DICAMBA

R.T.: 7.216 min
Delta R.T.: 0.007 min
Response: 8542198
Conc: 1.30 ng/ml

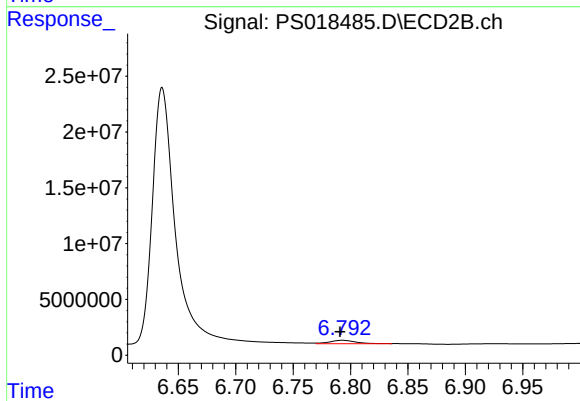

#5 DICAMBA


R.T.: 6.793 min
Delta R.T.: 0.002 min
Response: 4792726
Conc: 1.71 ng/ml

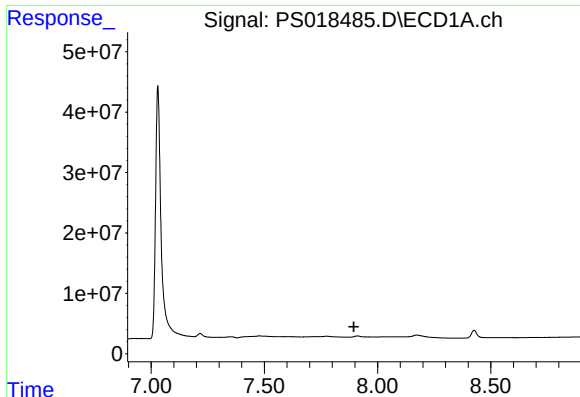

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.896 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

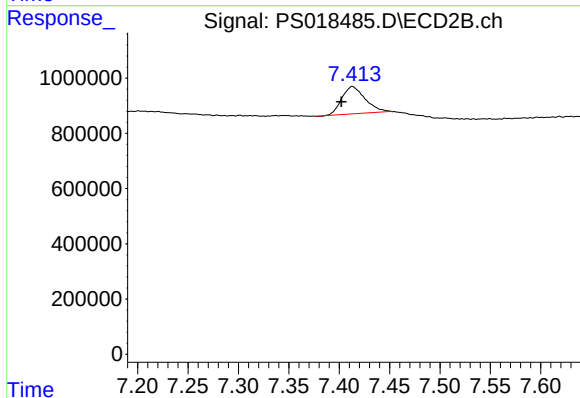


#8 DICHLORPROP

R.T.: 7.413 min
Delta R.T.: 0.011 min
Response: 1588111
Conc: 2.16 ng/ml

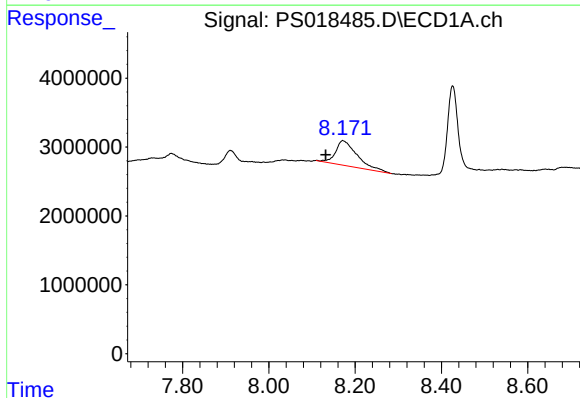


#9 2,4-D

R.T.: 8.171 min
Delta R.T.: 0.039 min
Response: 12500121
Conc: 6.13 ng/ml

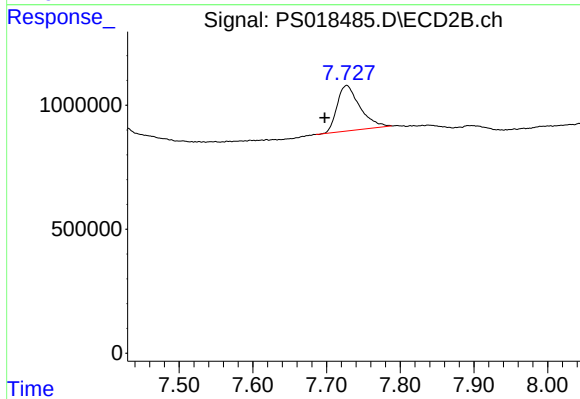

#9 2,4-D


R.T.: 7.727 min
Delta R.T.: 0.030 min
Response: 3911641
Conc: 4.18 ng/ml

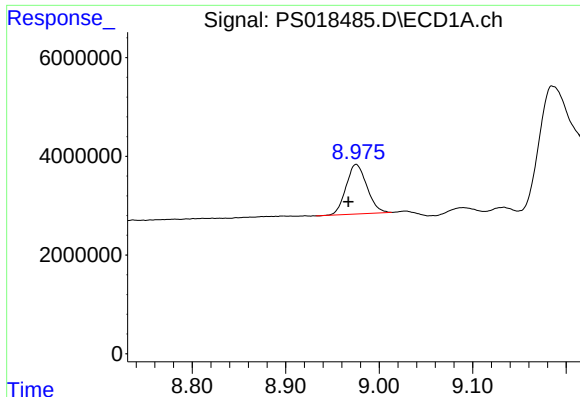

#11 2,4,5-TP (SILVEX)


R.T.: 8.975 min
Delta R.T.: 0.008 min
Response: 15485083
Conc: 1.63 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

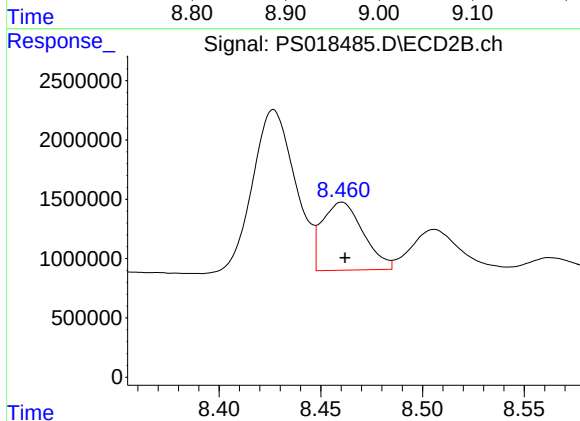


#11 2,4,5-TP (SILVEX)

R.T.: 8.460 min
Delta R.T.: -0.002 min
Response: 8037253
Conc: 1.95 ng/ml

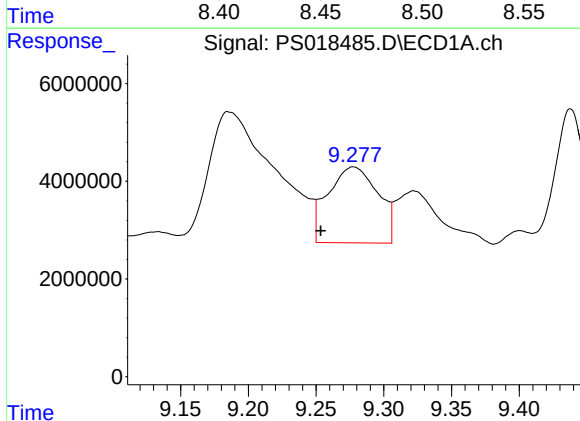


#12 2,4,5-T

R.T.: 9.277 min
Delta R.T.: 0.024 min
Response: 39896720
Conc: 3.97 ng/ml

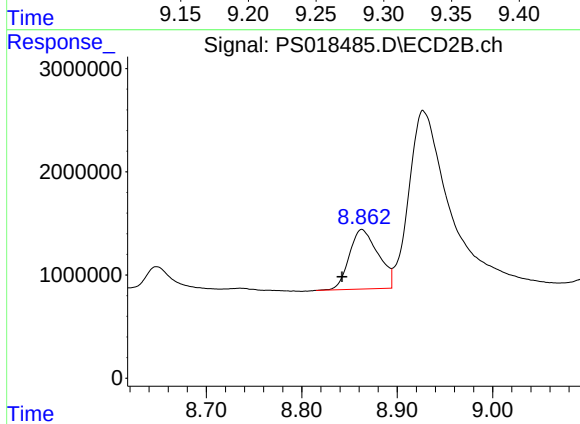

#12 2,4,5-T


R.T.: 8.863 min
Delta R.T.: 0.021 min
Response: 12111600
Conc: 3.08 ng/ml

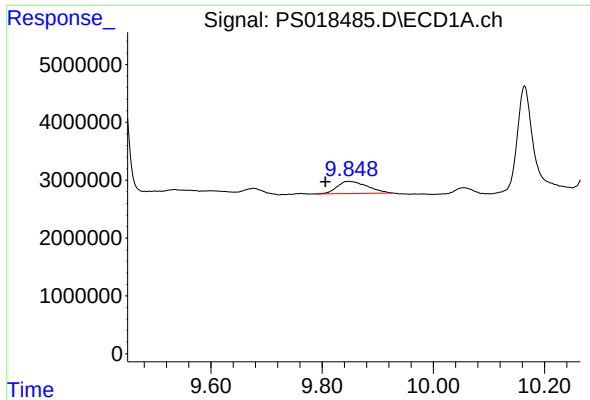

#13 2,4-DB


R.T.: 9.848 min
Delta R.T.: 0.043 min
Response: 7812962
Conc: 4.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

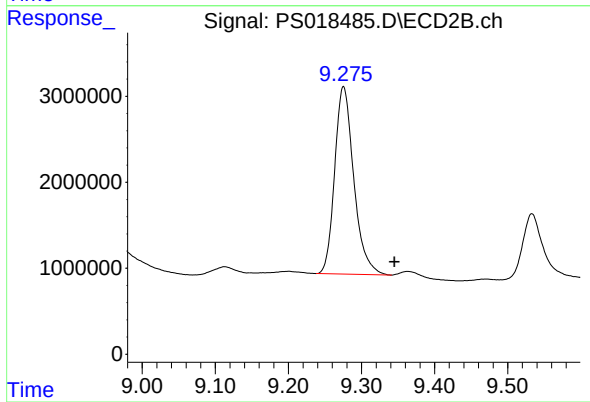


#13 2,4-DB

R.T.: 9.275 min
Delta R.T.: -0.070 min
Response: 39572692
Conc: 73.25 ng/ml

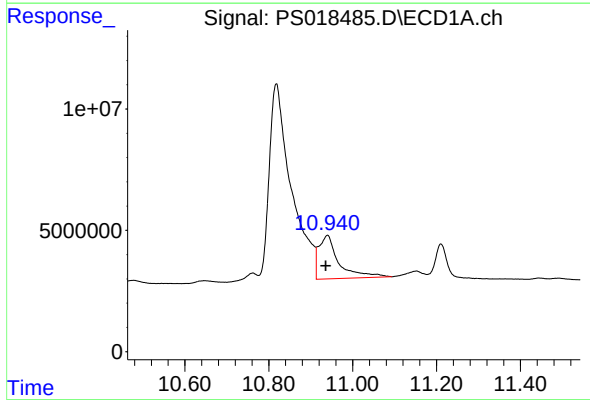


#14 DINOSEB

R.T.: 10.940 min
Delta R.T.: 0.004 min
Response: 59534707
Conc: 7.66 ng/ml

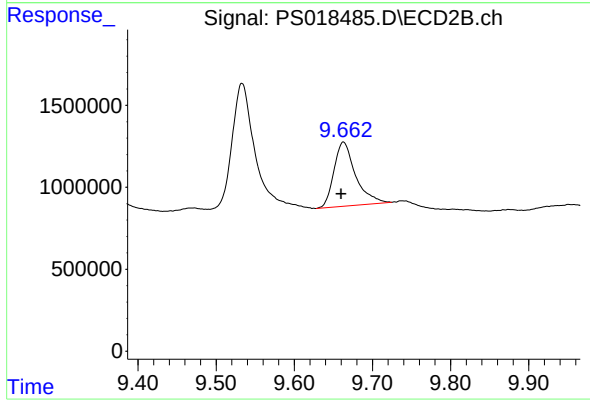

#14 DINOSEB


R.T.: 9.663 min
Delta R.T.: 0.003 min
Response: 7529759
Conc: 2.59 ng/ml

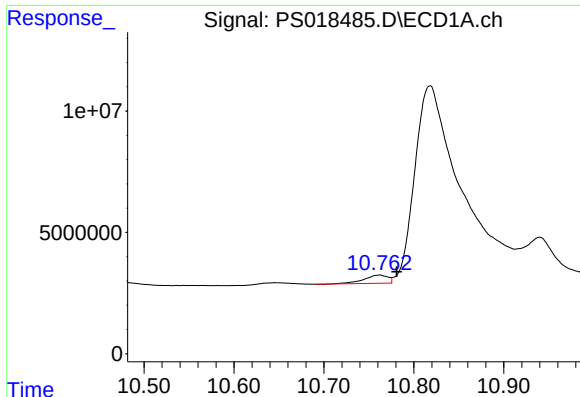

#15 Picloram


R.T.: 10.762 min
Delta R.T.: -0.019 min
Response: 6334499
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

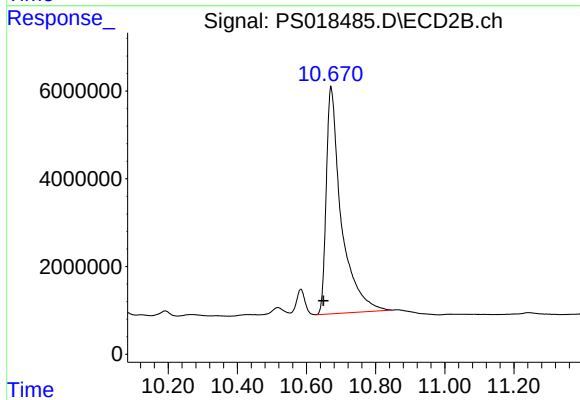


#15 Picloram

R.T.: 10.671 min
Delta R.T.: 0.022 min
Response: 156160182
Conc: 27.00 ng/ml

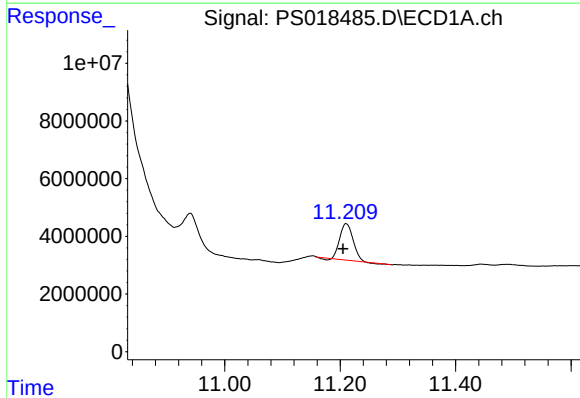

#16 DCPA

R.T.: 11.210 min
Delta R.T.: 0.005 min
Response: 19481450
Conc: 1.62 ng/ml

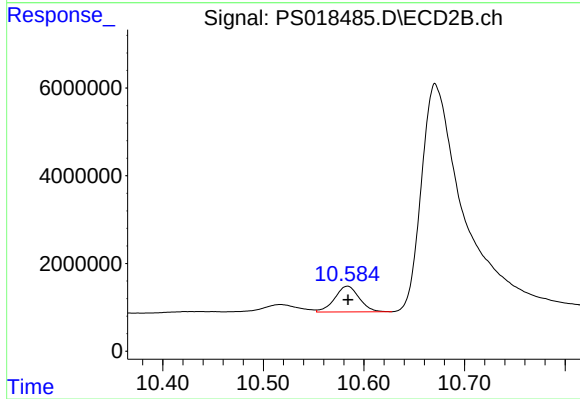

#16 DCPA

R.T.: 10.584 min
Delta R.T.: 0.000 min
Response: 9930063
Conc: 2.00 ng/ml