

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030322\
 Data File : PS018494.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2022 19:57
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 00:14:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.021	6.634	697.8E6	324.7E6	419.347	487.224
Target Compounds							
7) T	MCPA	7.471f	0.000	5717893	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.433	0	6554395	N.D.	8.902
9) T	2,4-D	8.171	0.000	423281	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.017f	8.496	48378406	12693815	5.081	3.075 #
12) T	2,4,5-T	9.252	8.839	11372160	3314187	1.131	<MDL #
13) T	2,4-DB	9.827	9.345	7722565	7029282	4.444	13.011 #
14) T	DINOSEB	10.870f	9.664	101.9E6	3383139	13.110	1.164 #
15) T	Picloram	10.805	10.666	84665595	45643379	6.663	7.893
16) T	DCPA	0.000	10.615	0	2994815	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030322\
Data File : PS018494.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2022 19:57
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 00:14:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

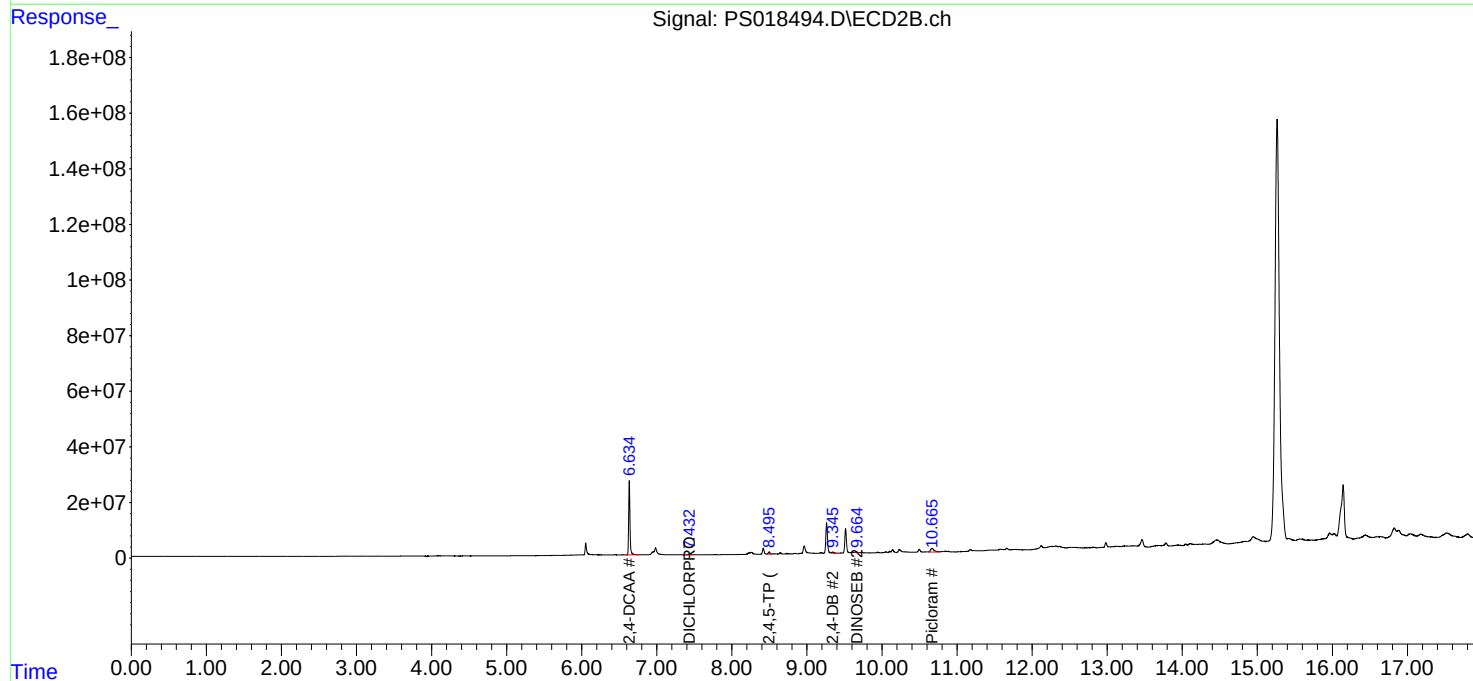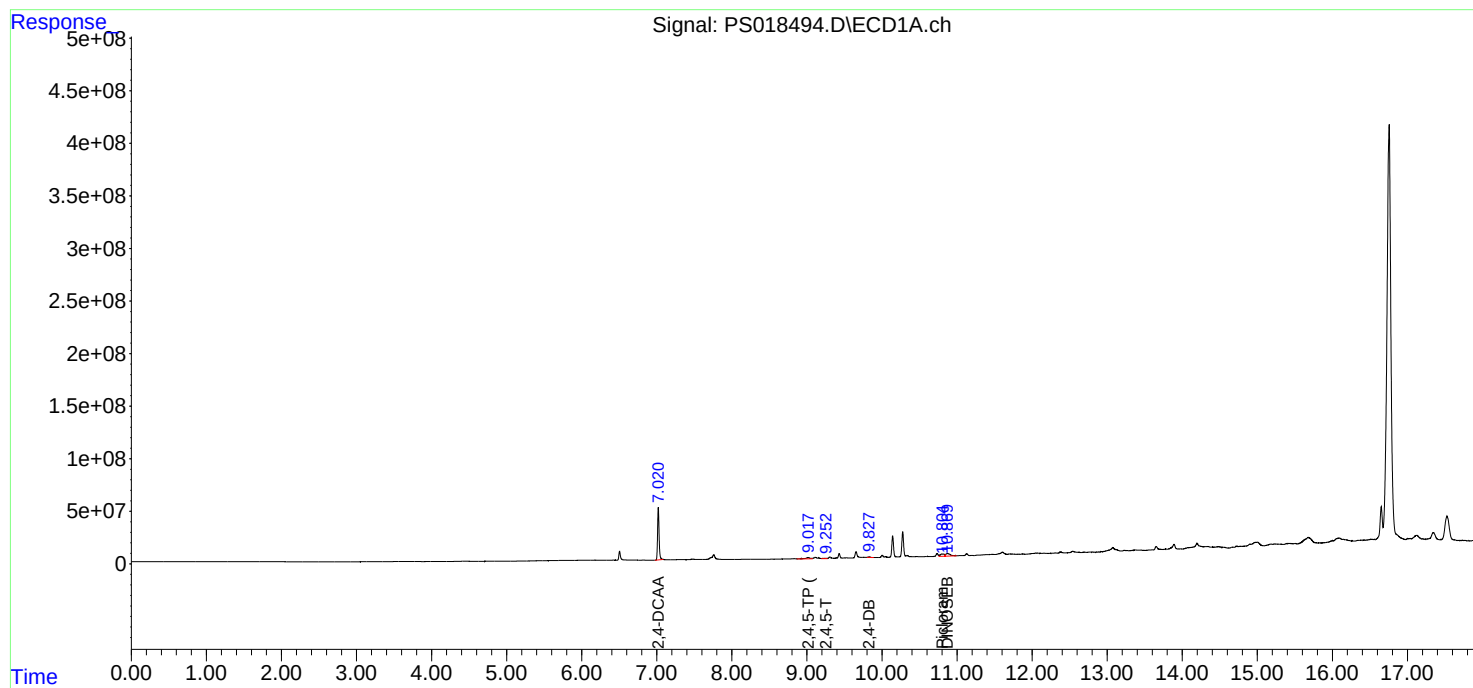


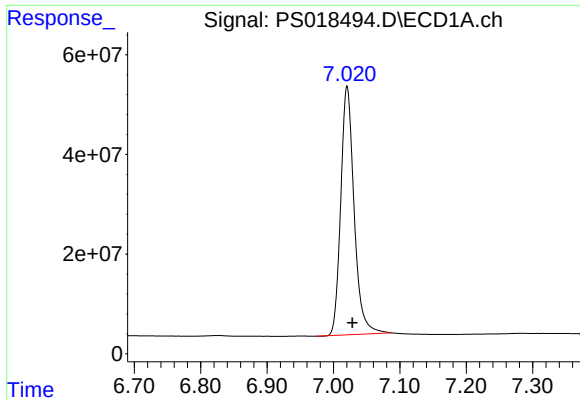

#4 2,4-DCAA


R.T.: 7.021 min
Delta R.T.: -0.008 min
Response: 697815067
Conc: 419.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

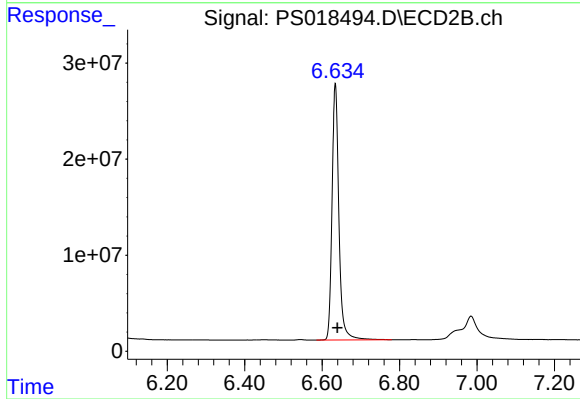


#4 2,4-DCAA

R.T.: 6.634 min
Delta R.T.: -0.006 min
Response: 324658091
Conc: 487.22 ng/ml

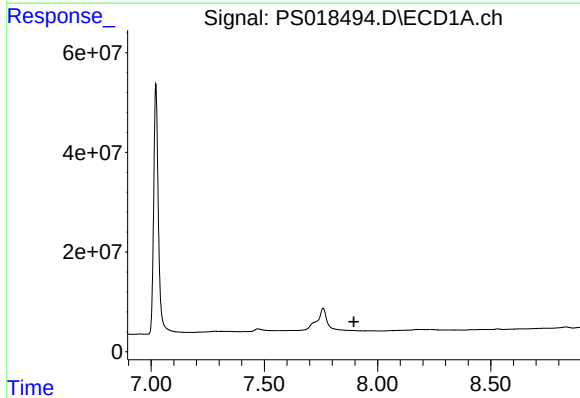


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.896 min
Response: 0
Conc: N.D.

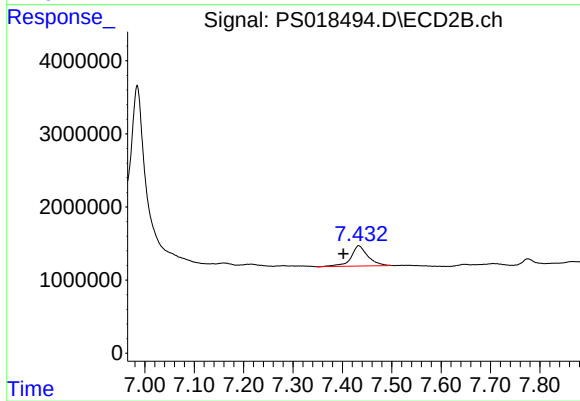

#8 DICHLORPROP


R.T.: 7.433 min
Delta R.T.: 0.030 min
Response: 6554395
Conc: 8.90 ng/ml

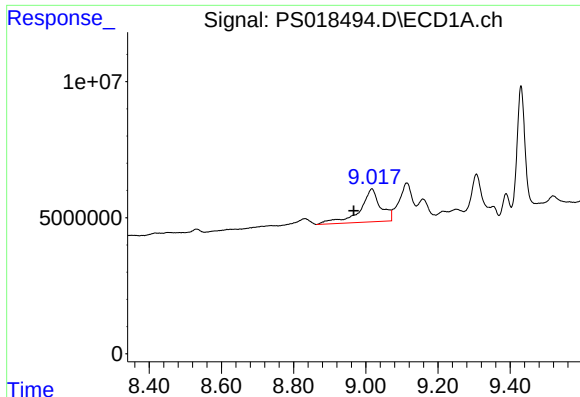

#11 2,4,5-TP (SILVEX)


R.T.: 9.017 min
Delta R.T.: 0.050 min
Response: 48378406
Conc: 5.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

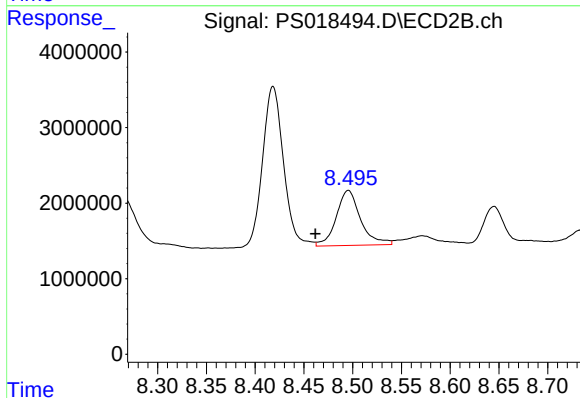


#11 2,4,5-TP (SILVEX)

R.T.: 8.496 min
Delta R.T.: 0.034 min
Response: 12693815
Conc: 3.07 ng/ml

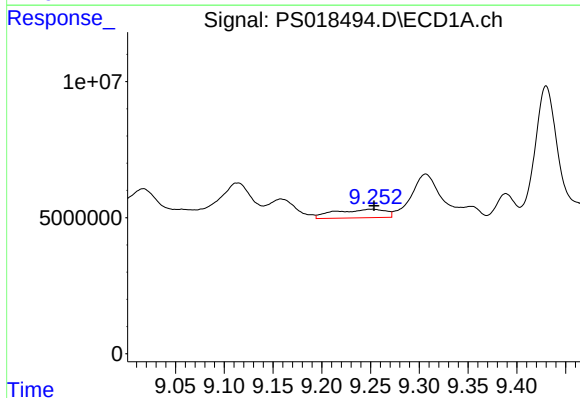


#12 2,4,5-T

R.T.: 9.252 min
Delta R.T.: -0.001 min
Response: 11372160
Conc: 1.13 ng/ml

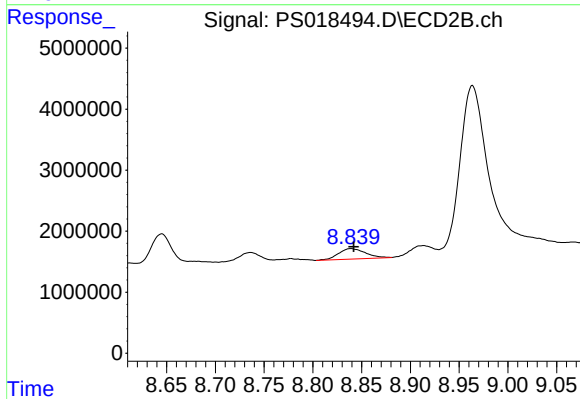

#12 2,4,5-T


R.T.: 8.839 min
Delta R.T.: -0.003 min
Response: 3314187
Conc: N.D.

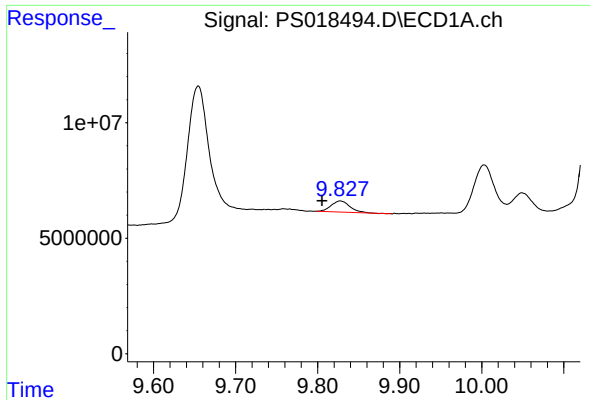

#13 2,4-DB


R.T.: 9.827 min
Delta R.T.: 0.022 min
Response: 7722565
Conc: 4.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

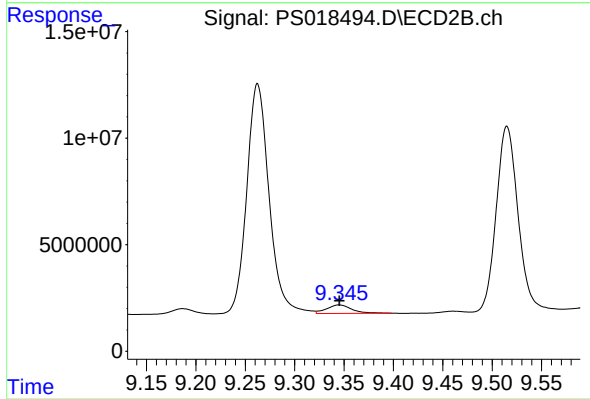


#13 2,4-DB

R.T.: 9.345 min
Delta R.T.: 0.000 min
Response: 7029282
Conc: 13.01 ng/ml

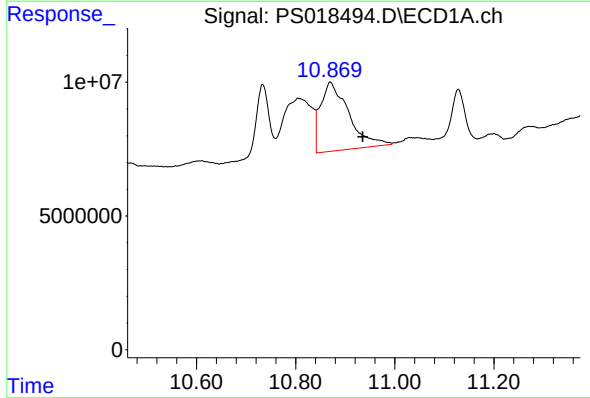


#14 DINOSEB

R.T.: 10.870 min
Delta R.T.: -0.066 min
Response: 101856129
Conc: 13.11 ng/ml

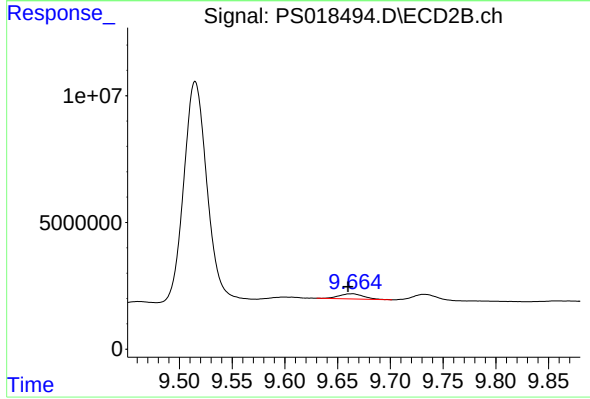

#14 DINOSEB


R.T.: 9.664 min
Delta R.T.: 0.004 min
Response: 3383139
Conc: 1.16 ng/ml

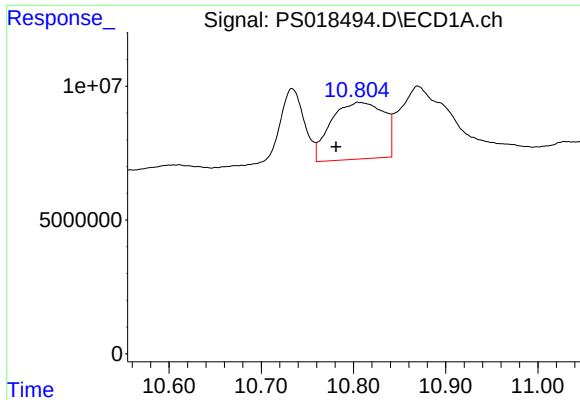

#15 Picloram

R.T.: 10.805 min
Delta R.T.: 0.024 min
Response: 84665595
Conc: 6.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

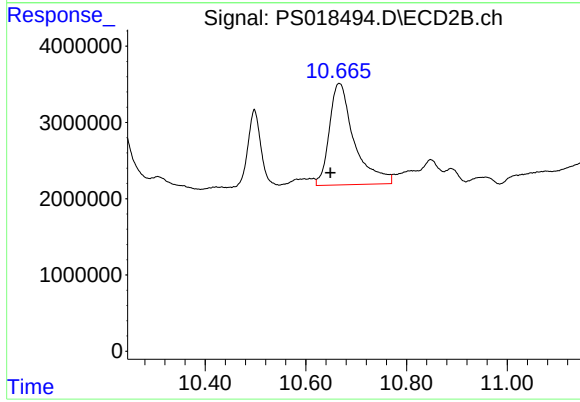

#15 Picloram

R.T.: 10.666 min
Delta R.T.: 0.017 min
Response: 45643379
Conc: 7.89 ng/ml