

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030322\
 Data File : PS018493.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2022 19:33
 Operator : AJ\MA
 Sample : N1731-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 VACLOT-TOPSOIL-GRILLO-01A

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/04/2022
 Supervised By :Ankita Jodhani 03/04/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 00:13:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.018	6.630	548.5E6	330.1E6	329.604	495.317m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030322\
Data File : PS018493.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2022 19:33
Operator : AJ\MA
Sample : N1731-02
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
VACLOT-TOPSOIL-GRILLO-01A


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/04/2022
Supervised By : Ankita Jodhani 03/04/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 00:13:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

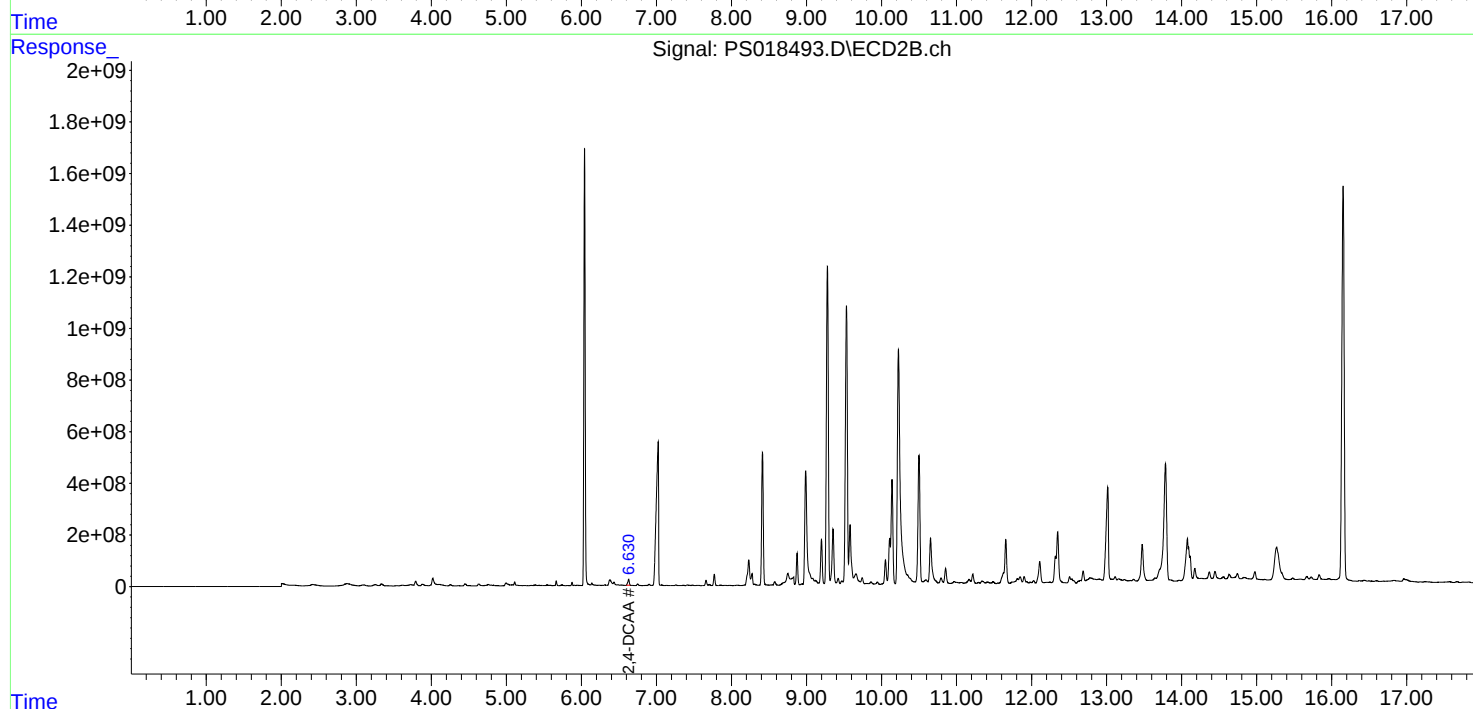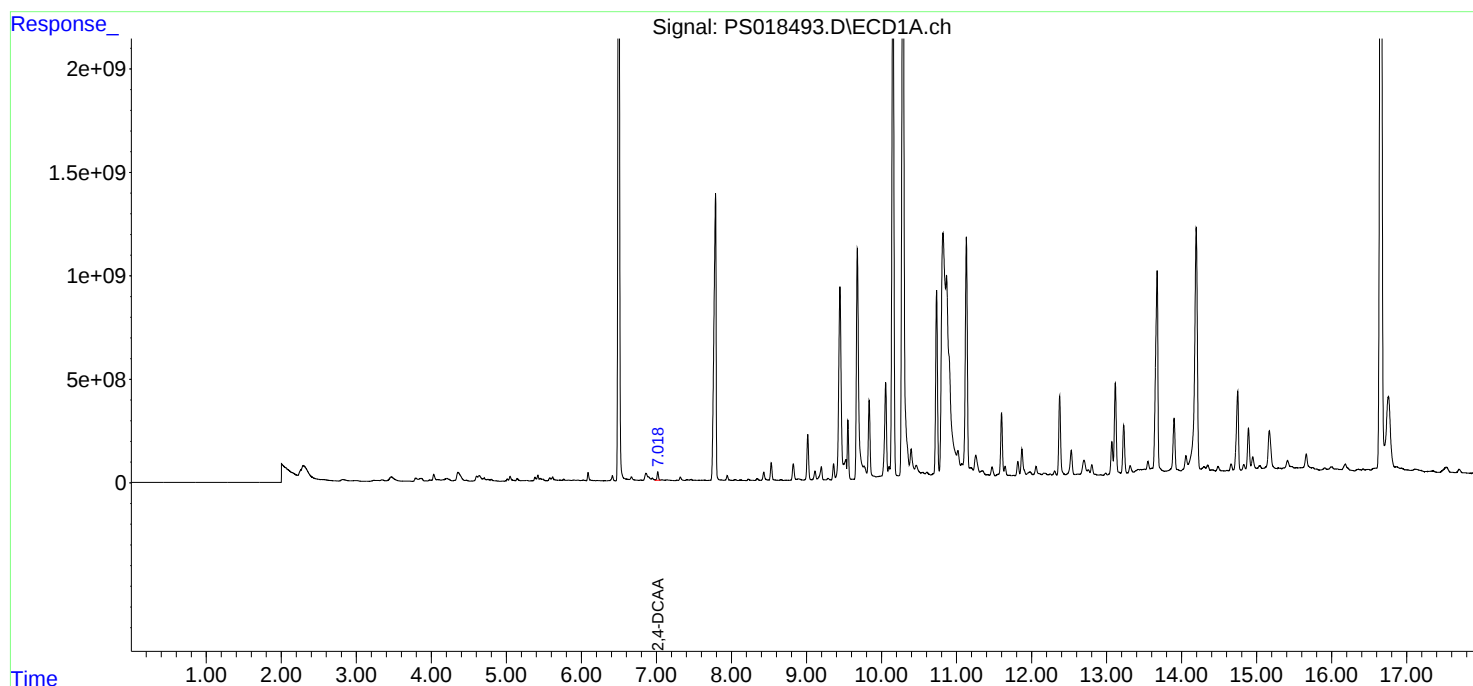

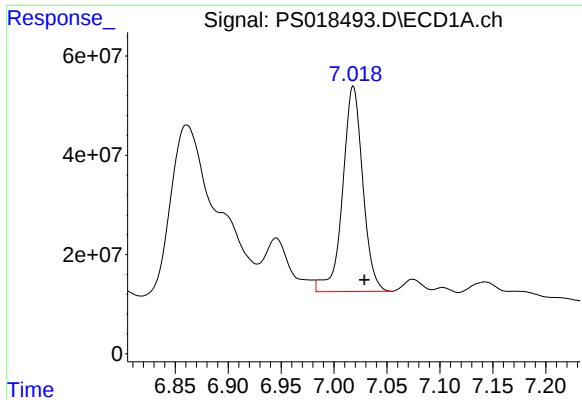


#4 2,4-DCAA

R.T.: 7.018 min
Delta R.T.: -0.011 min
Response: 548477182
Conc: 329.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
VACLOT-TOPSOIL-GRILLO-01A

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/04/2022
Supervised By :Ankita Jodhani 03/04/2022

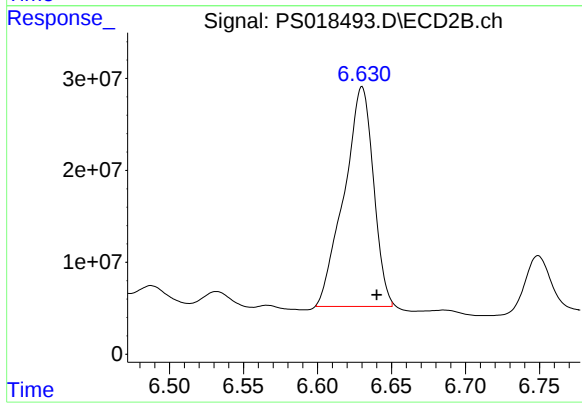

#4 2,4-DCAA

R.T.: 6.630 min
Delta R.T.: -0.010 min
Response: 330050531
Conc: 495.32 ng/ml m