

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030323\
 Data File : PS022301.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2023 08:13
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 12:04:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
 Quant Title : 8080.M
 QLast Update : Mon Feb 20 13:26:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.290	0.000	253671	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.368f	2.512	177383	506530	<MDL	<MDL #
3) T	4-Nitroph...	6.140	0.000	1890721	0	1.486	N.D. #
5) T	DICAMBA	6.398	6.928f	191727	3840697	<MDL	<MDL #
6) T	MCP	6.612	6.928f	16354	3840697	<MDL	<MDL #
7) T	MCPA	6.668f	0.000	233535	0	<MDL	N.D. #
8) T	DICHLORPROP	7.027	7.538	2883779	9951219	1.068	4.048 #
9) T	2,4-D	7.197	0.000	58105719	0	17.722	N.D. #
10) T	Pentachlo...	7.445	8.207	9591587	5577097	<MDL	<MDL #
11) T	2,4,5-TP ...	7.972	8.577	6420167	2963033	<MDL	<MDL #
12) T	2,4,5-T	8.209	0.000	10906912	0	<MDL	N.D. #
13) T	2,4-DB	8.717	0.000	1903980	0	<MDL	N.D. #
15) T	Picloram	9.609	10.704f	25779989	32981509	1.047	1.682 #
16) T	DCPA	10.049	10.704	900417	32981509	<MDL	2.108 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030323\
Data File : PS022301.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2023 08:13
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 12:04:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
Quant Title : 8080.M
QLast Update : Mon Feb 20 13:26:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

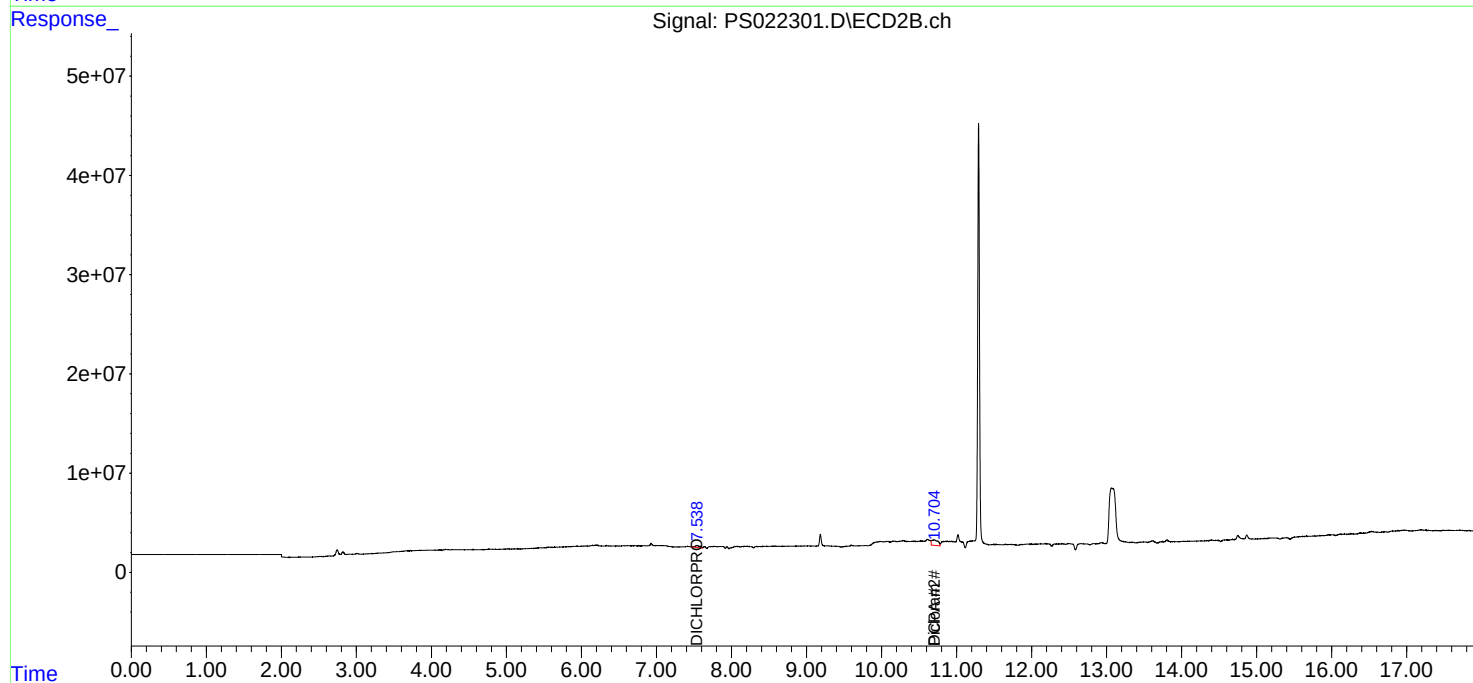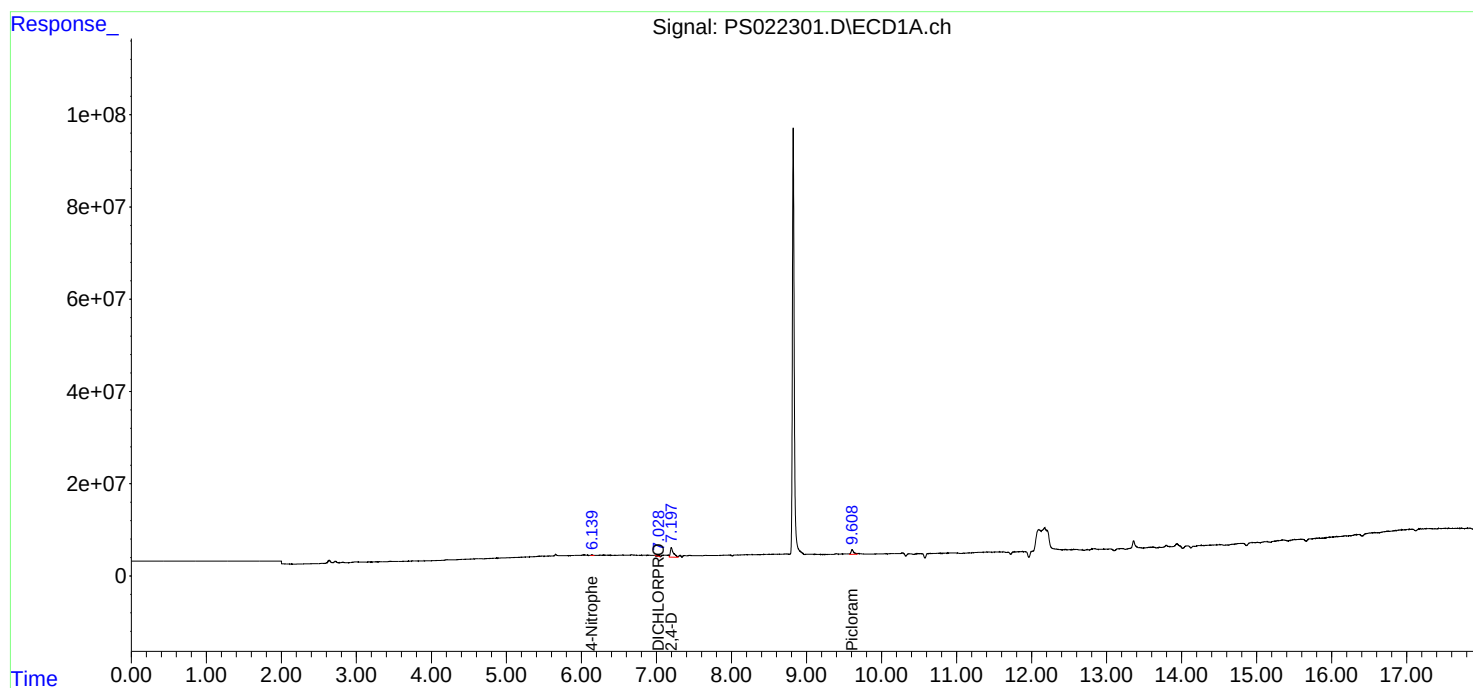


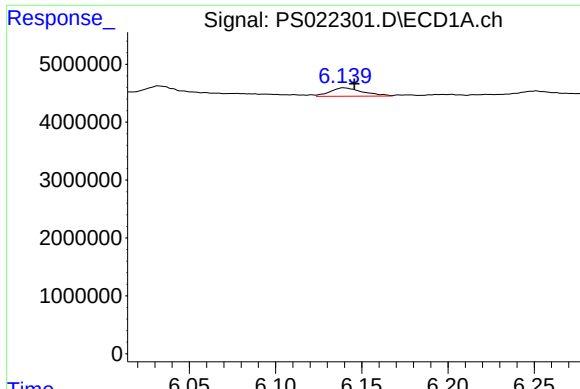

#3 4-Nitrophenol


R.T.: 6.140 min
Delta R.T.: -0.006 min
Response: 1890721
Conc: 1.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

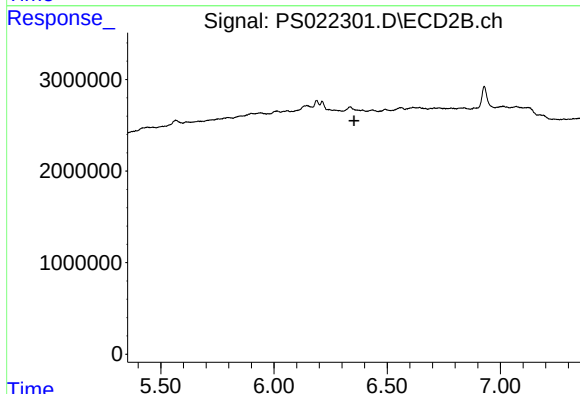


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.353 min
Response: 0
Conc: N.D.

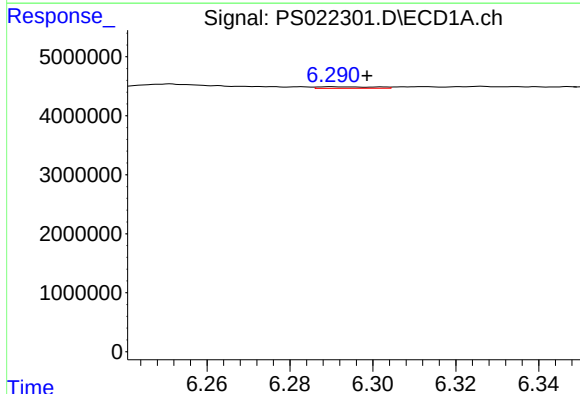


#4 2,4-DCAA

R.T.: 6.290 min
Delta R.T.: -0.008 min
Response: 253671
Conc: N.D.

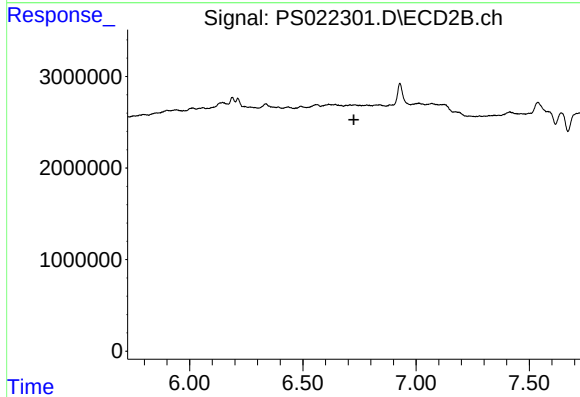

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.726 min
Response: 0
Conc: N.D.

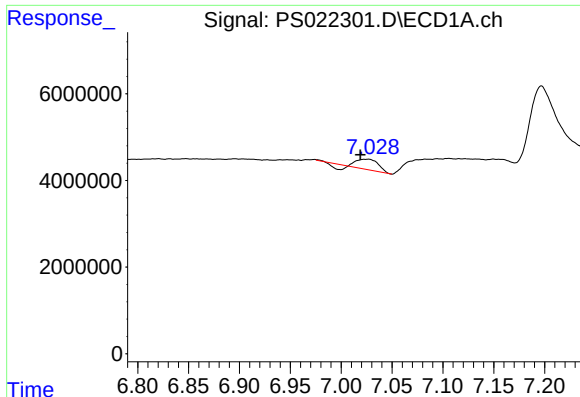

#8 DICHLORPROP


R.T.: 7.027 min
Delta R.T.: 0.008 min
Response: 2883779
Conc: 1.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

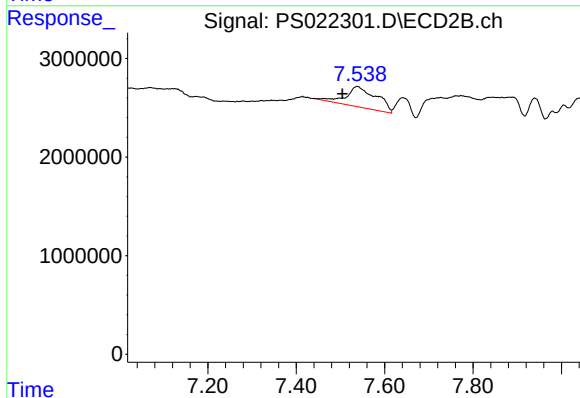


#8 DICHLORPROP

R.T.: 7.538 min
Delta R.T.: 0.034 min
Response: 9951219
Conc: 4.05 ng/ml

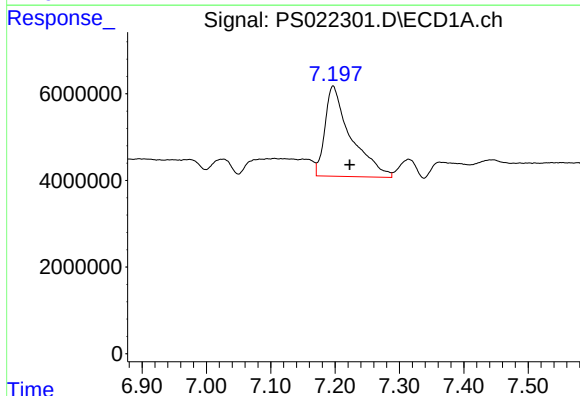


#9 2,4-D

R.T.: 7.197 min
Delta R.T.: -0.026 min
Response: 58105719
Conc: 17.72 ng/ml

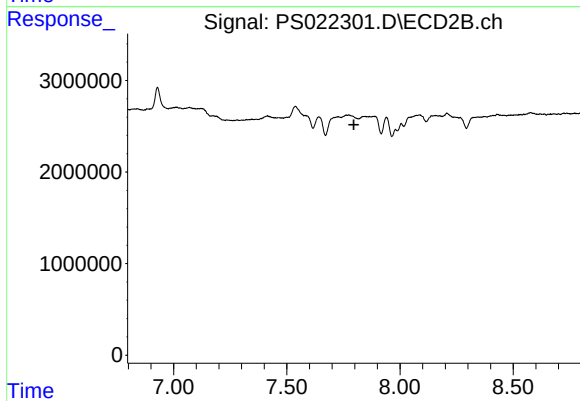

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.796 min
Response: 0
Conc: N.D.

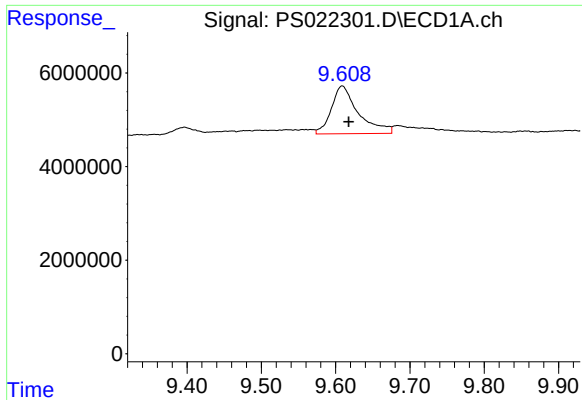

#15 Picloram


R.T.: 9.609 min
Delta R.T.: -0.009 min
Response: 25779989
Conc: 1.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

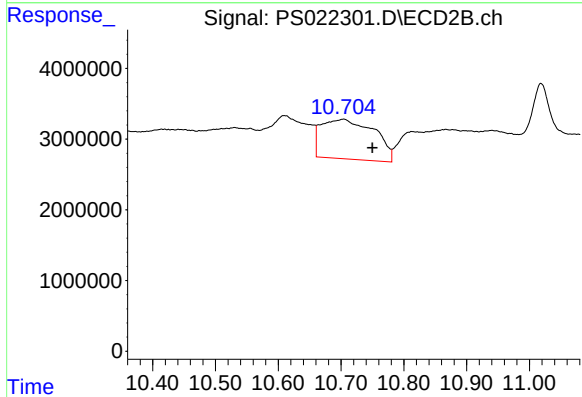


#15 Picloram

R.T.: 10.704 min
Delta R.T.: -0.046 min
Response: 32981509
Conc: 1.68 ng/ml

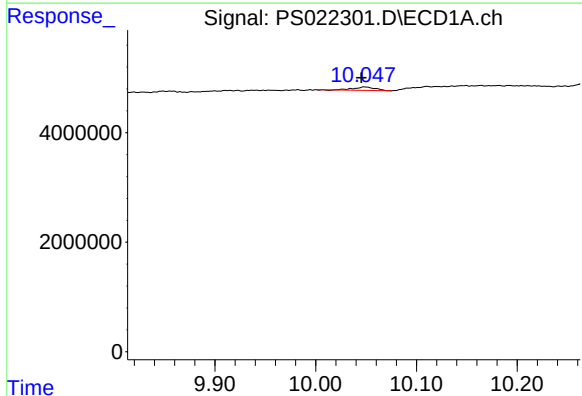

#16 DCPA

R.T.: 10.049 min
Delta R.T.: 0.004 min
Response: 900417
Conc: N.D.

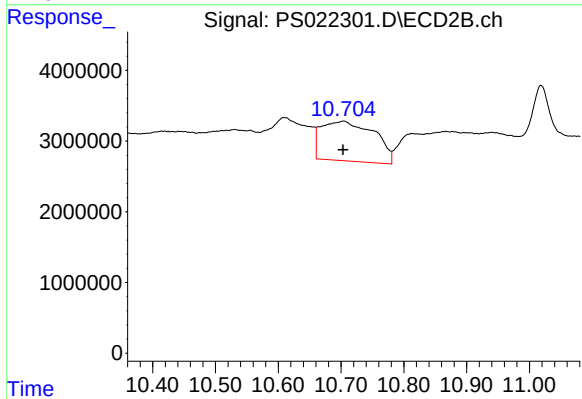

#16 DCPA

R.T.: 10.704 min
Delta R.T.: 0.000 min
Response: 32981509
Conc: 2.11 ng/ml