

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030323\
 Data File : PS022314.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2023 14:04
 Operator : AR\AJ
 Sample : PB151111TB
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 15:19:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
 Quant Title : 8080.M
 QLast Update : Mon Feb 20 13:26:02 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.324	0.000	603759	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.414	0.000	114454	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.706	0.000	85916	0	<MDL	N.D. #
3) T	4-Nitroph...	6.155	0.000	10416145	0	8.185	N.D. #
5) T	DICAMBA	6.389f	0.000	2861093	0	<MDL	N.D. #
6) T	MCP	6.588	0.000	694614	0	<MDL	N.D. #
8) T	DICHLORPROP	6.958f	0.000	380294	0	<MDL	N.D. #
10) T	Pentachlo...	7.459	0.000	1335147	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.010f	8.572	861671	2092269	<MDL	<MDL #
12) T	2,4,5-T	8.253	0.000	1255718	0	<MDL	N.D. #
13) T	2,4-DB	8.762	0.000	263988	0	<MDL	N.D. #
14) T	DINOSEB	9.788	0.000	5679740	0	<MDL	N.D. #
16) T	DCPA	10.045	0.000	652372	0	<MDL	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030323\
Data File : PS022314.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2023 14:04
Operator : AR\AJ
Sample : PB151111TB
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 15:19:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022023.M
Quant Title : 8080.M
QLast Update : Mon Feb 20 13:26:02 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

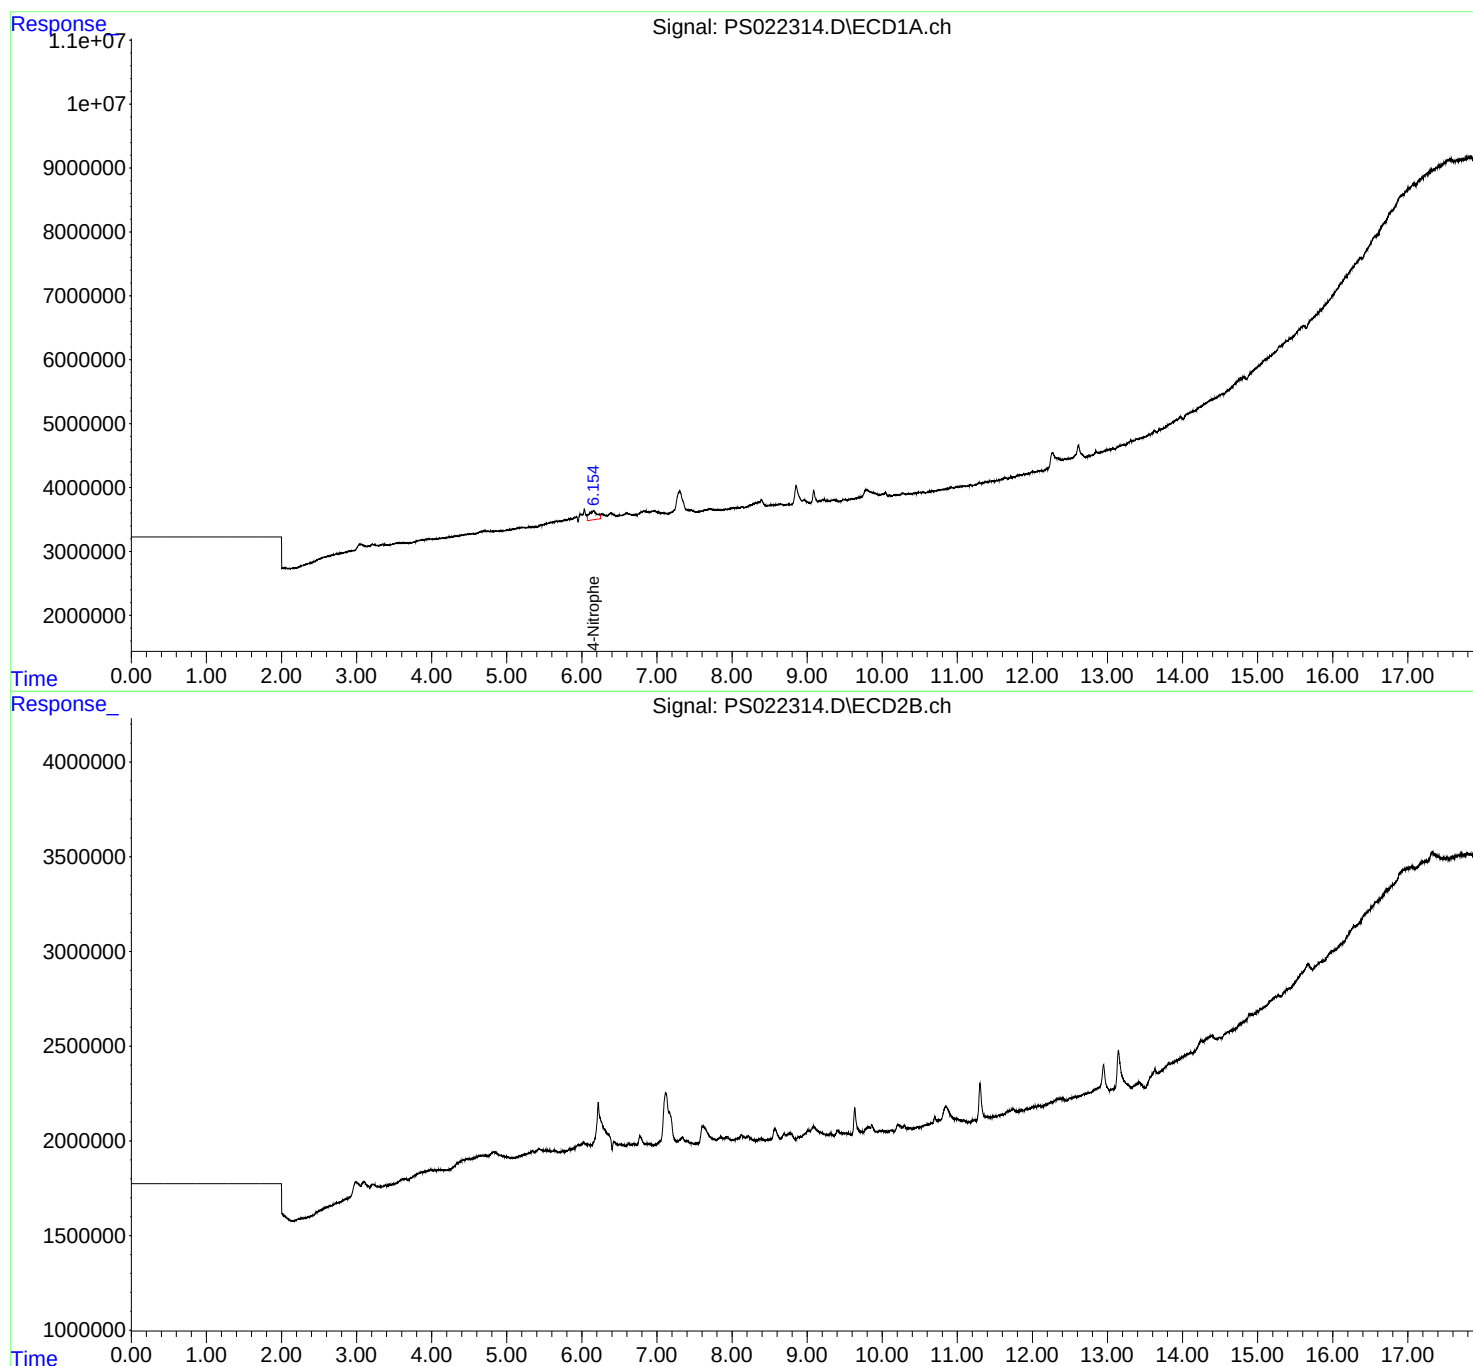


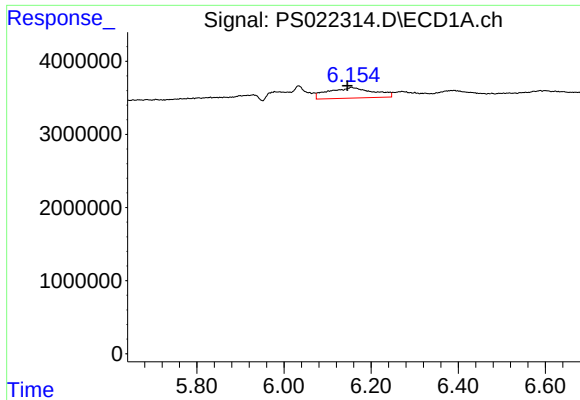

#3 4-Nitrophenol


R.T.: 6.155 min
Delta R.T.: 0.009 min
Response: 10416145
Conc: 8.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

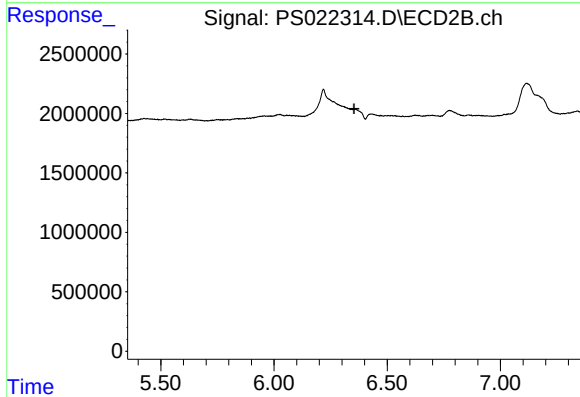


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.353 min
Response: 0
Conc: N.D.

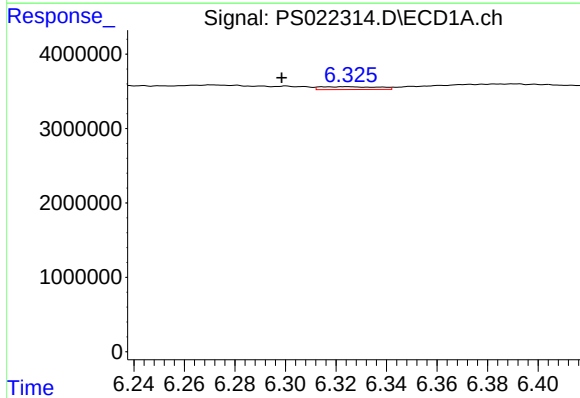

#4 2,4-DCAA

R.T.: 6.324 min
Delta R.T.: 0.025 min
Response: 603759
Conc: N.D.

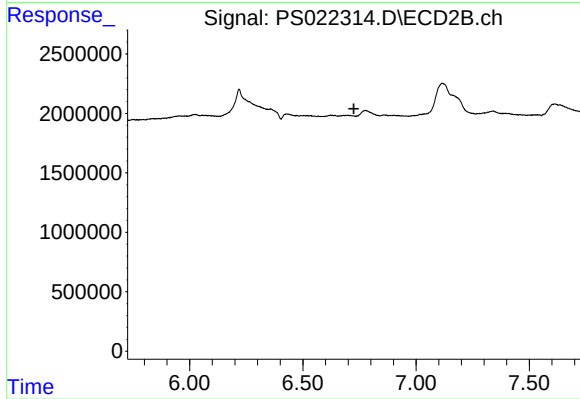

#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.726 min
Response: 0
Conc: N.D.