

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030325\
 Data File : PS029326.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2025 08:42
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 01:16:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
 Quant Title : 8080.M
 QLast Update : Sat Feb 22 01:02:20 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.158	7.625	1967.0E6	442.2E6	477.358	470.280
Target Compounds							
1) T	Dalapon	2.637f	2.684f	38412986	13545345	6.959	6.398
2) T	3,5-DICHL...	6.331	0.000	182650	0	<MDL	N.D. #
3) T	4-Nitroph...	6.953	0.000	8268158	0	3.533	N.D. #
7) T	MCPA	7.694	0.000	659269	0	<MDL	N.D. #
8) T	DICHLORPROP	8.037	8.580f	4240127	3840947	<MDL	3.004 #
10) T	Pentachlo...	8.563	9.372	6651346	18262773	<MDL	<MDL #
11) T	2,4,5-TP ...	9.107f	9.751	11040937	10996739	<MDL	1.217 #
12) T	2,4,5-T	9.453	0.000	6707939	0	<MDL	N.D. #
13) T	2,4-DB	10.001	0.000	1280405	0	<MDL	N.D. #
14) T	DINOSEB	11.192	0.000	695345	0	<MDL	N.D. #
15) T	Picloram	11.048f	12.199	14979487	3714153	<MDL	<MDL #
16) T	DCPA	11.486	0.000	4143260	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030325\
Data File : PS029326.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2025 08:42
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 01:16:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022125.M
Quant Title : 8080.M
QLast Update : Sat Feb 22 01:02:20 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

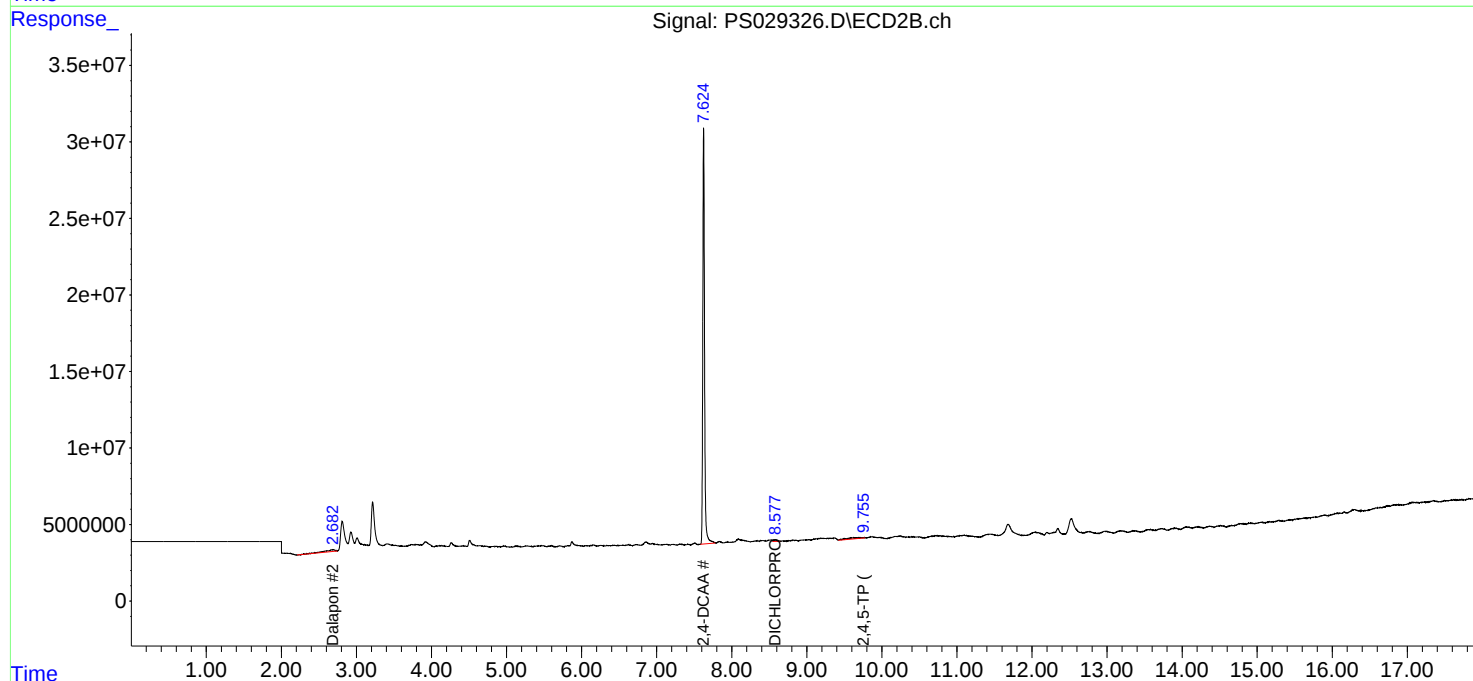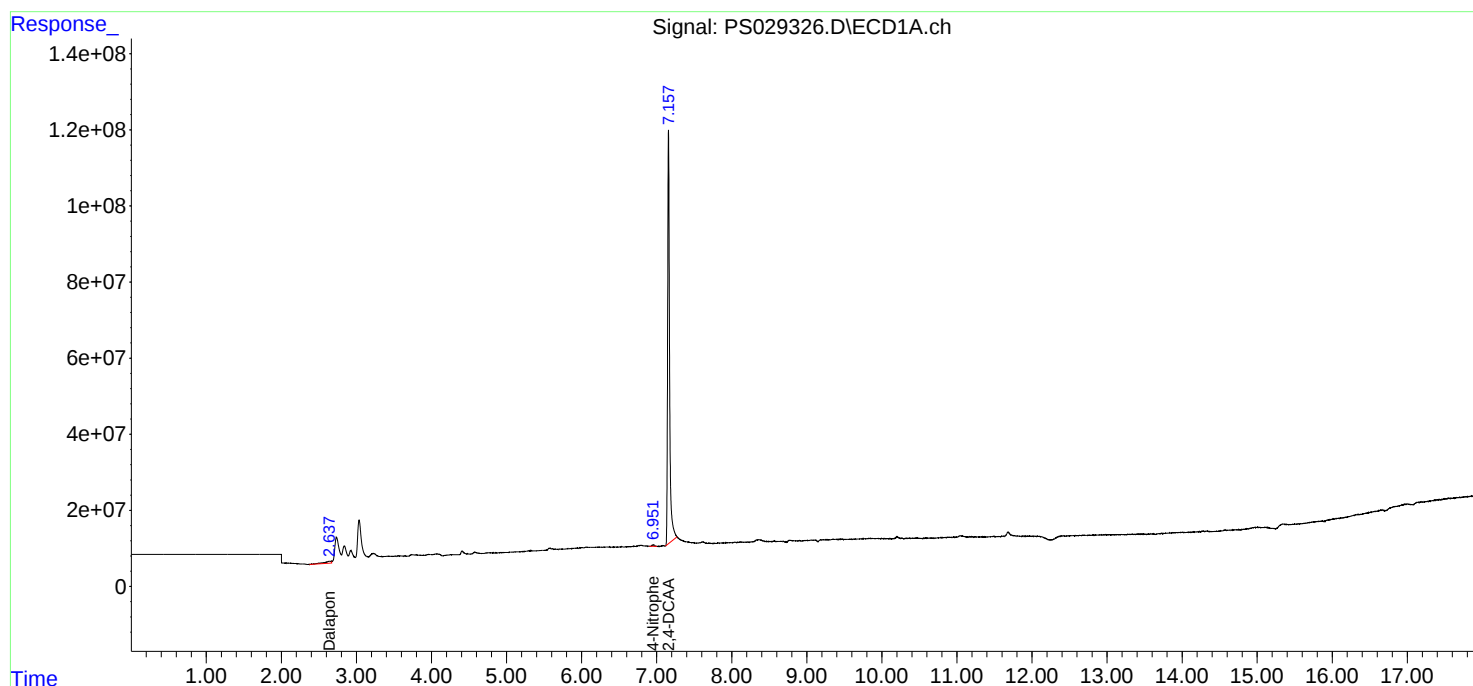


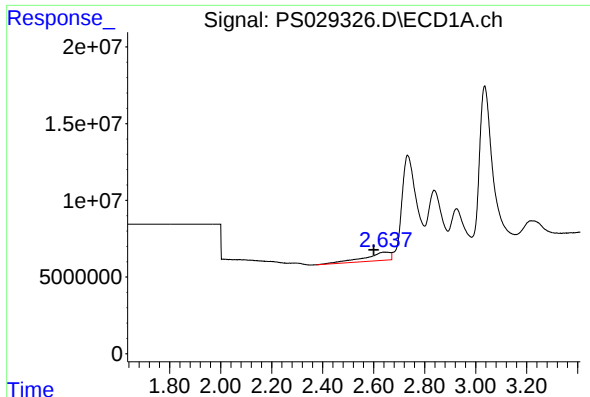

#1 Dalapon


R.T.: 2.637 min
Delta R.T.: 0.037 min
Response: 38412986
Conc: 6.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

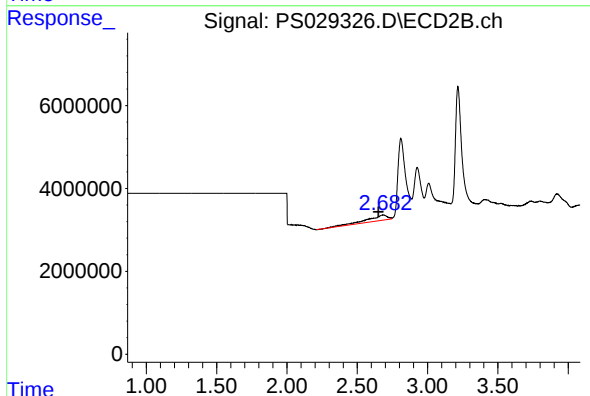


#1 Dalapon

R.T.: 2.684 min
Delta R.T.: 0.033 min
Response: 13545345
Conc: 6.40 ng/ml

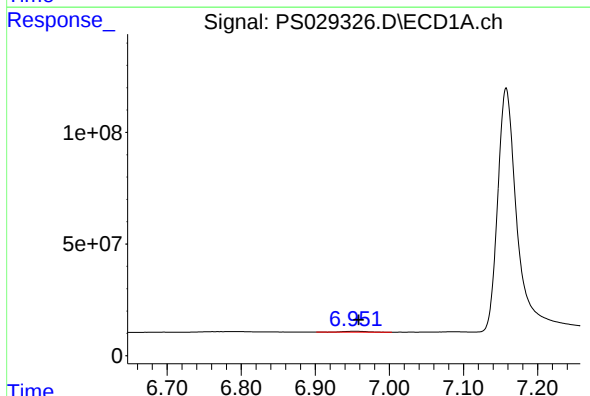


#3 4-Nitrophenol

R.T.: 6.953 min
Delta R.T.: -0.005 min
Response: 8268158
Conc: 3.53 ng/ml

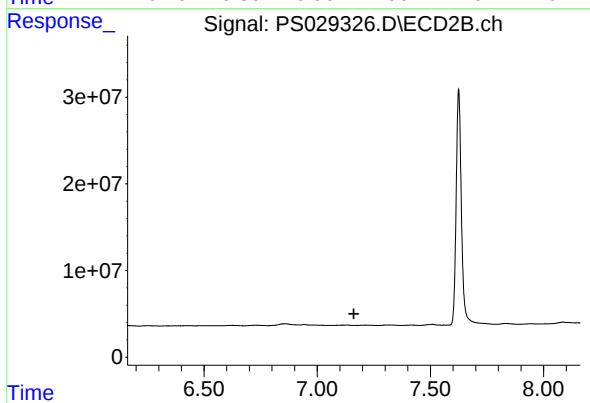

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.162 min
Response: 0
Conc: N.D.

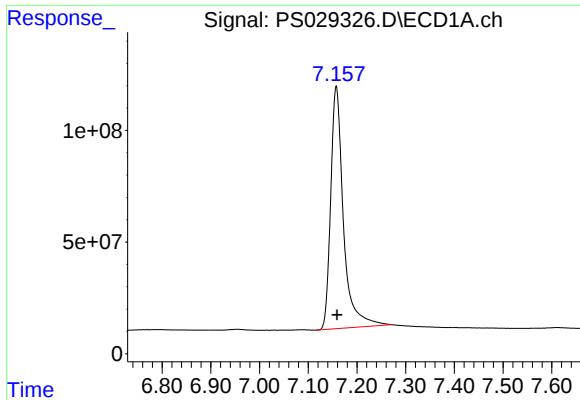

#4 2,4-DCAA


R.T.: 7.158 min
Delta R.T.: -0.002 min
Response: 1966990435
Conc: 477.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

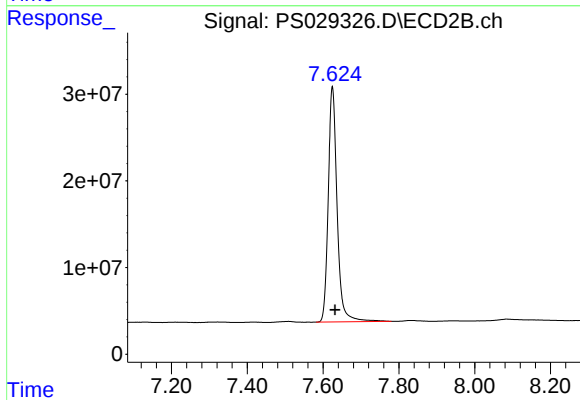


#4 2,4-DCAA

R.T.: 7.625 min
Delta R.T.: -0.007 min
Response: 442219967
Conc: 470.28 ng/ml

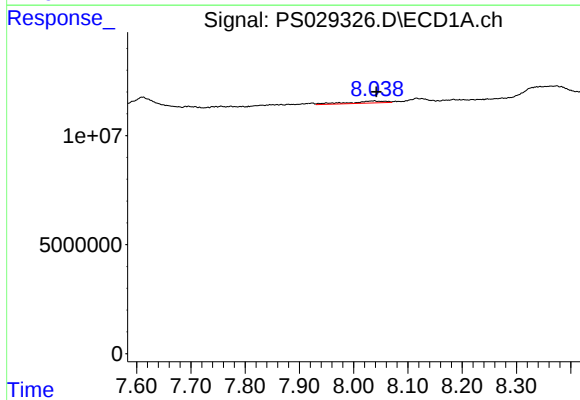


#8 DICHLORPROP

R.T.: 8.037 min
Delta R.T.: -0.005 min
Response: 4240127
Conc: N.D.

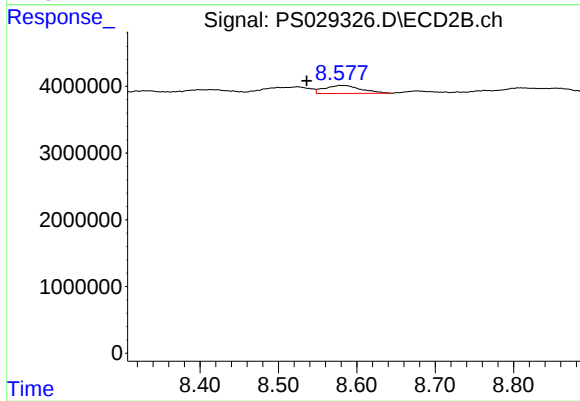

#8 DICHLORPROP


R.T.: 8.580 min
Delta R.T.: 0.044 min
Response: 3840947
Conc: 3.00 ng/ml

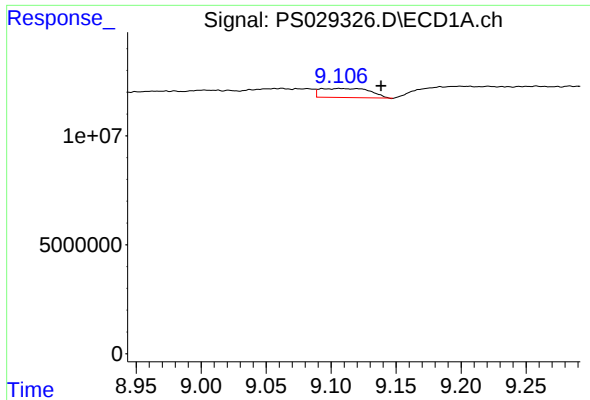

#11 2,4,5-TP (SILVEX)

R.T.: 9.107 min
Delta R.T.: -0.031 min
Response: 11040937
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

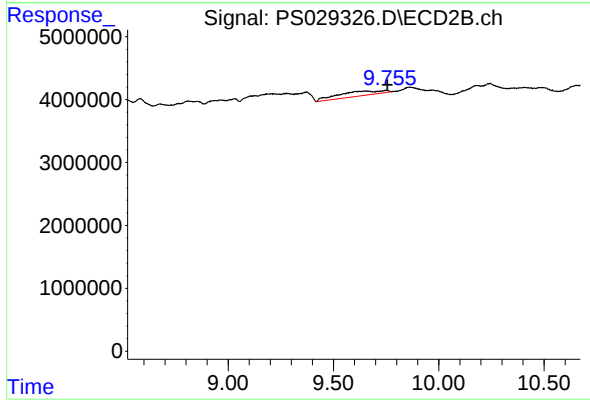

#11 2,4,5-TP (SILVEX)

R.T.: 9.751 min
Delta R.T.: -0.005 min
Response: 10996739
Conc: 1.22 ng/ml