

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030419\
 Data File : PS003403.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2019 09:39
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 00:01:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.313	10.809	212.1E6	204.6E6	483.223	435.699
Target Compounds							
3) T	4-Nitroph...	0.000	9.982	0	142789	N.D.	0.635 #
7) T	MCPA	0.000	11.701	0	290150	N.D.	0.168 #
8) T	DICHLORPROP	0.000	12.240	0	262090	N.D.	0.634 #
10) T	Pentachlo...	0.000	13.228	0	1052838	N.D.	0.160 #
11) T	2,4,5-TP ...	0.000	13.808	0	940692	N.D.	0.369 #
14) T	DINOSEB	0.000	15.495	0	527195	N.D.	0.295 #
15) T	Picloram	0.000	16.663	0	1040900	N.D.	0.410 #
16) T	DCPA	0.000	16.663	0	1040900	N.D.	0.335 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030419\
Data File : PS003403.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2019 09:39
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 00:01:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

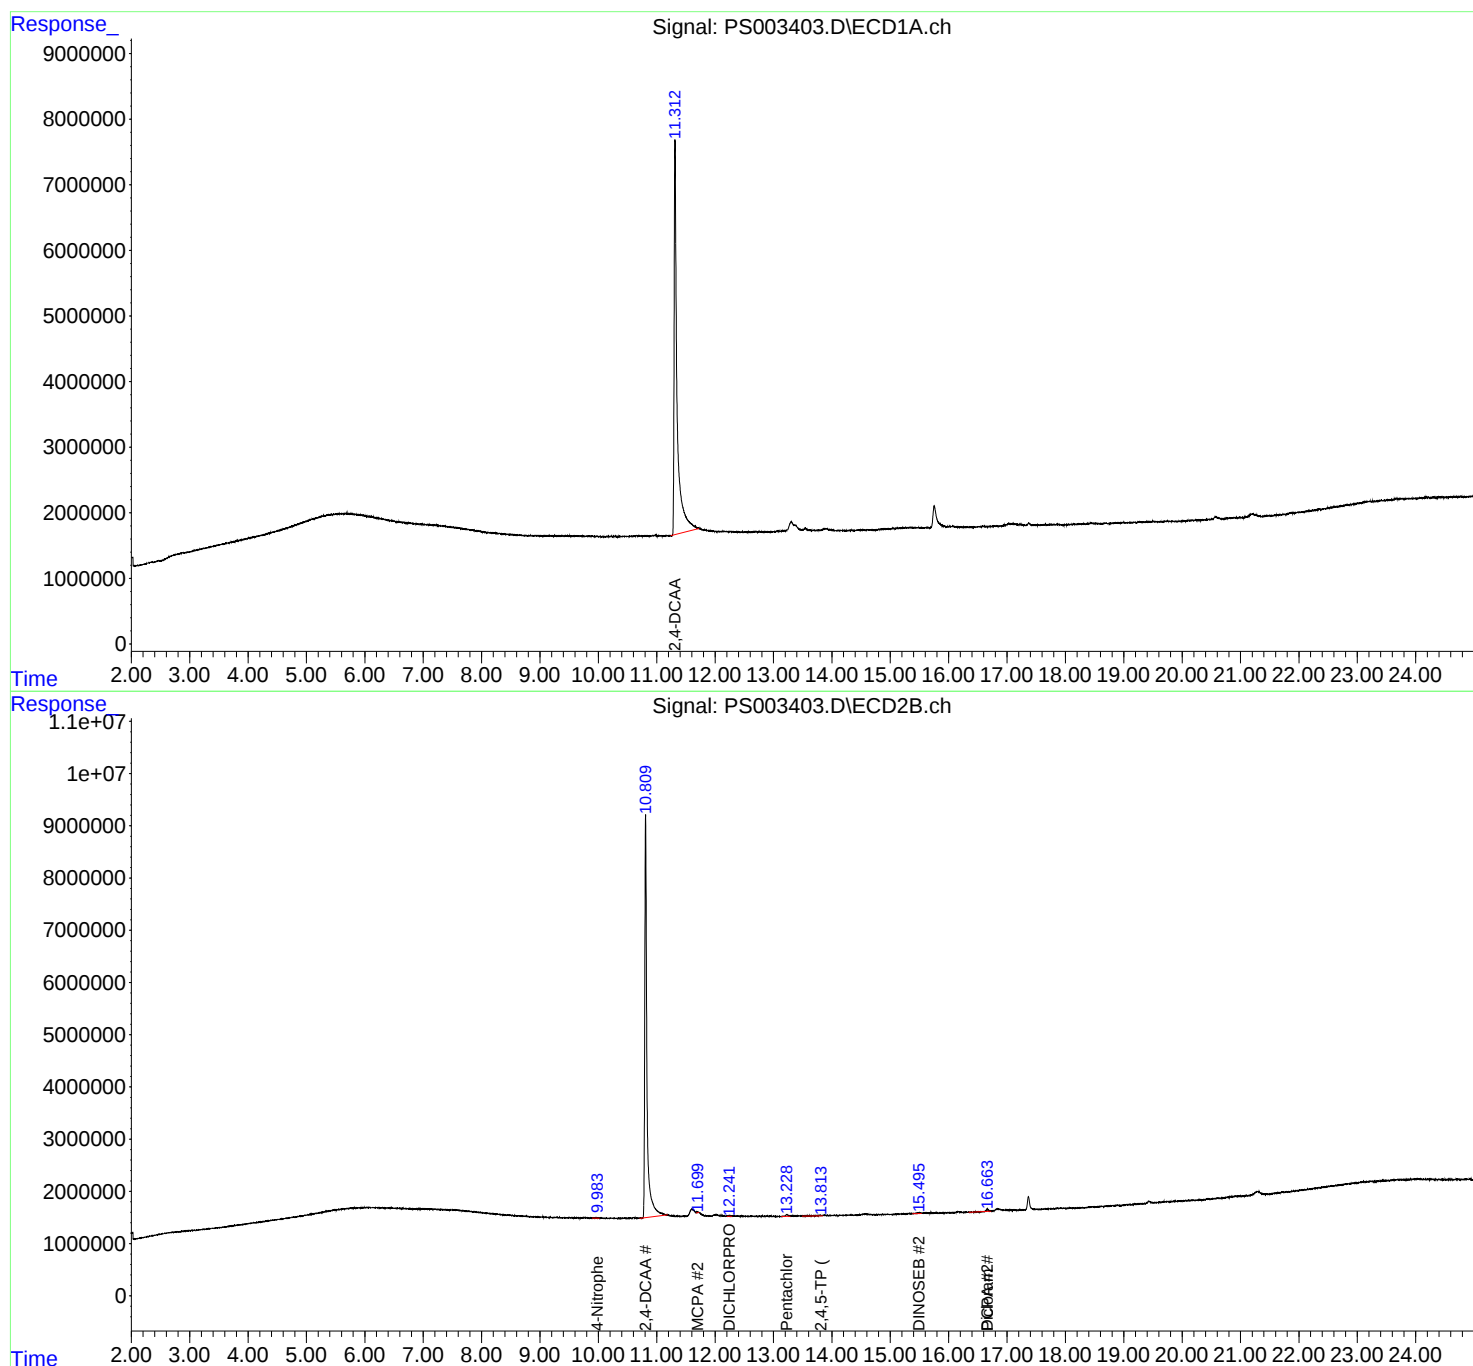


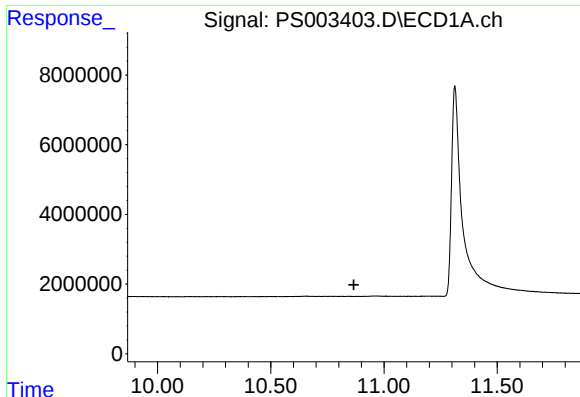

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

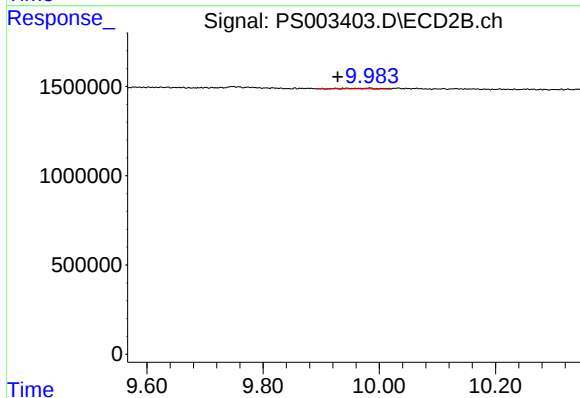


#3 4-Nitrophenol

R.T.: 9.982 min
Delta R.T.: 0.053 min
Response: 142789
Conc: 0.64 ng/ml

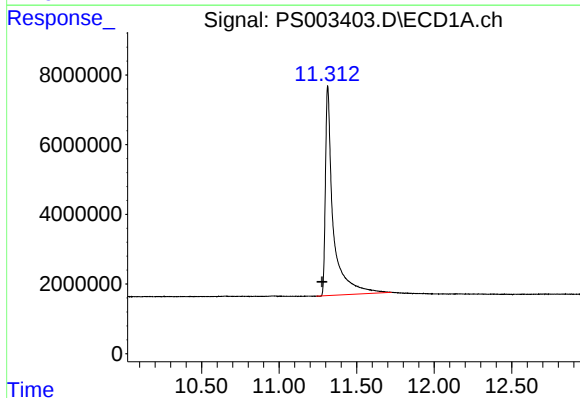


#4 2,4-DCAA

R.T.: 11.313 min
Delta R.T.: 0.035 min
Response: 212146945
Conc: 483.22 ng/ml

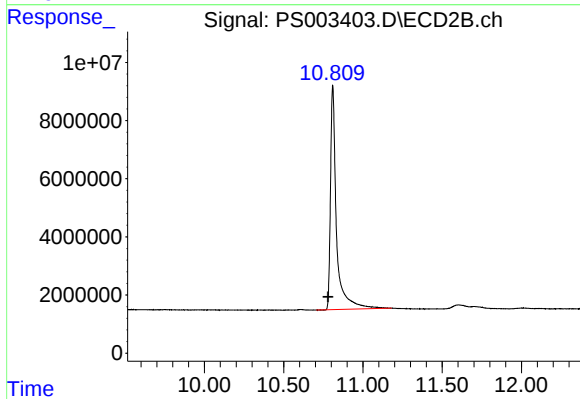

#4 2,4-DCAA


R.T.: 10.809 min
Delta R.T.: 0.030 min
Response: 204591017
Conc: 435.70 ng/ml

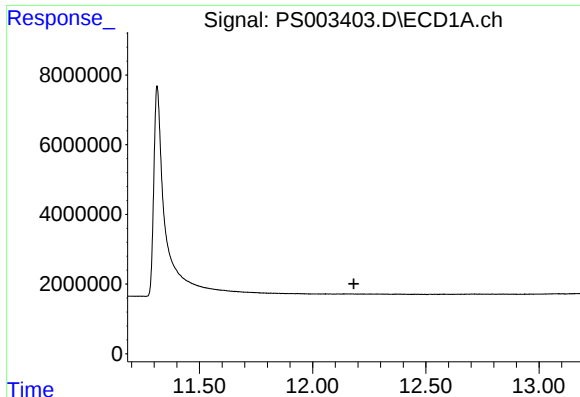

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

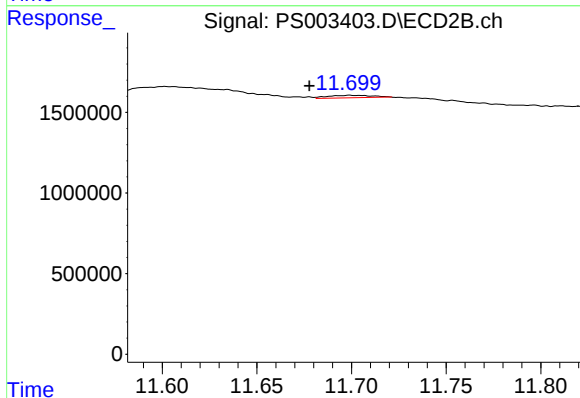


#7 MCPA

R.T.: 11.701 min
Delta R.T.: 0.023 min
Response: 290150
Conc: 0.17 ug/ml

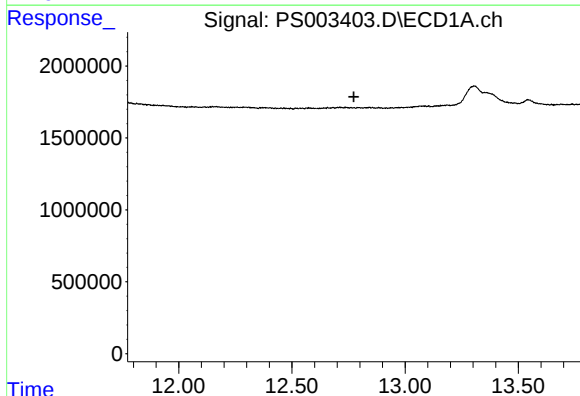


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.773 min
Response: 0
Conc: N.D.

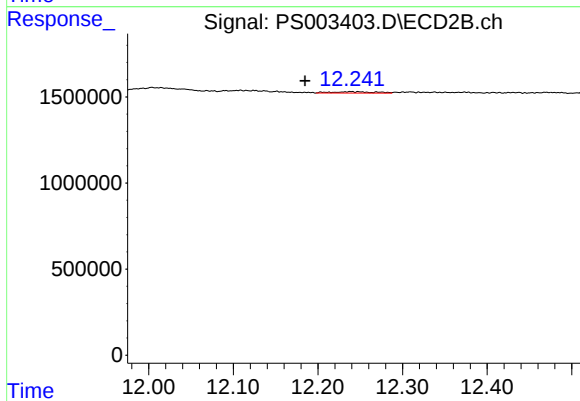

#8 DICHLORPROP


R.T.: 12.240 min
Delta R.T.: 0.055 min
Response: 262090
Conc: 0.63 ng/ml

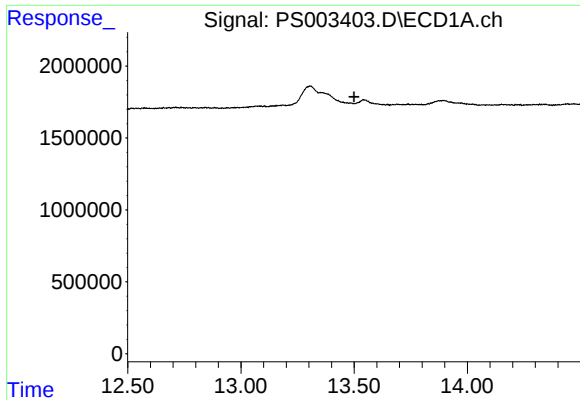

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

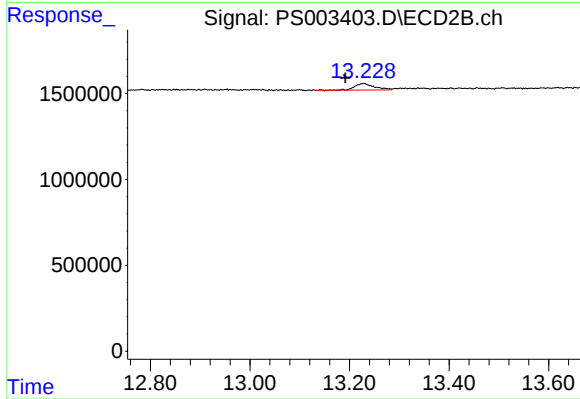


#10 Pentachlorophenol

R.T.: 13.228 min
Delta R.T.: 0.036 min
Response: 1052838
Conc: 0.16 ng/ml

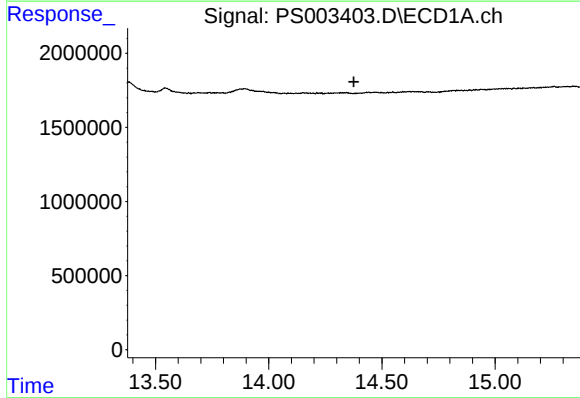


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.376 min
Response: 0
Conc: N.D.

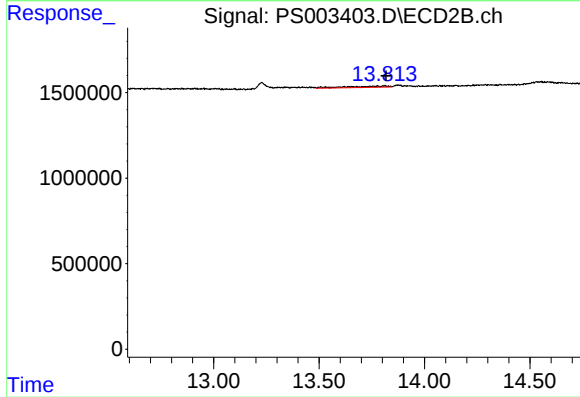

#11 2,4,5-TP (SILVEX)


R.T.: 13.808 min
Delta R.T.: -0.009 min
Response: 940692
Conc: 0.37 ng/ml

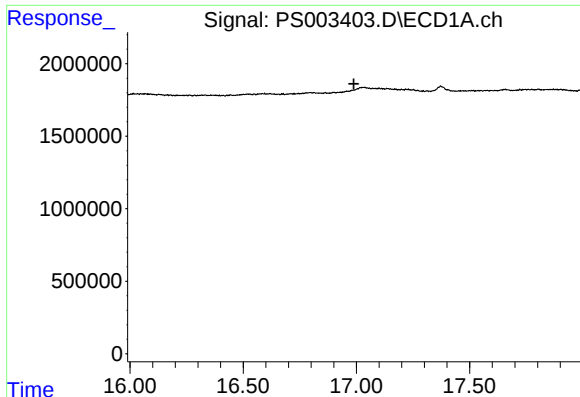

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

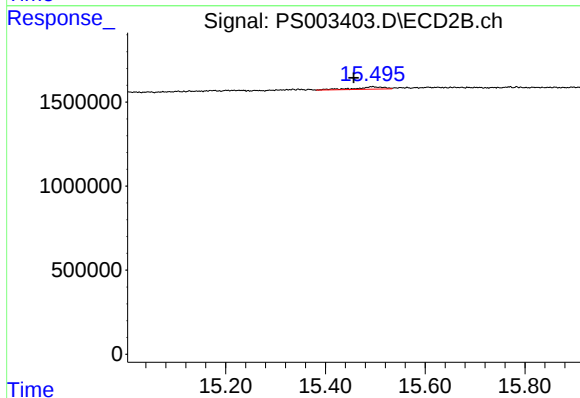


#14 DINOSEB

R.T.: 15.495 min
Delta R.T.: 0.038 min
Response: 527195
Conc: 0.30 ng/ml

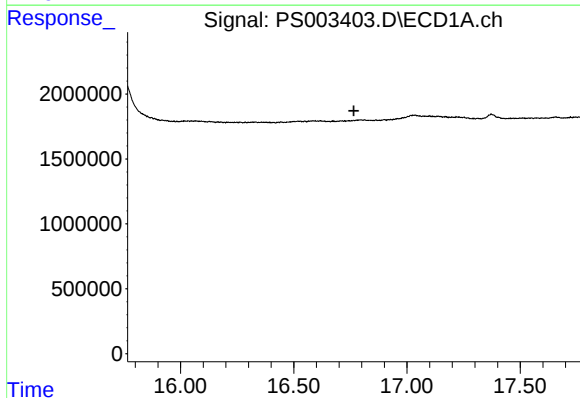


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.765 min
Response: 0
Conc: N.D.

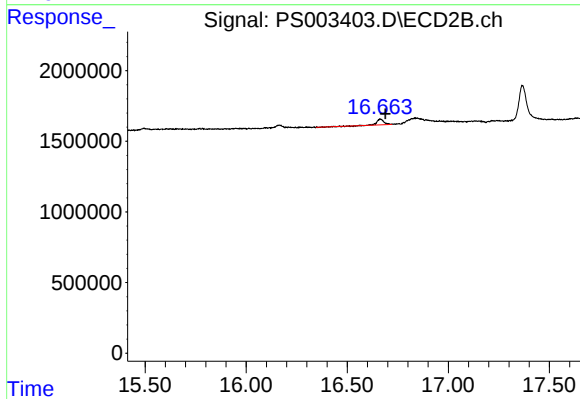

#15 Picloram


R.T.: 16.663 min
Delta R.T.: -0.025 min
Response: 1040900
Conc: 0.41 ng/ml

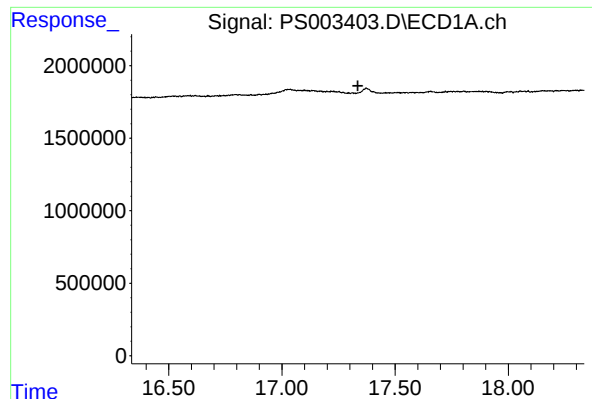

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

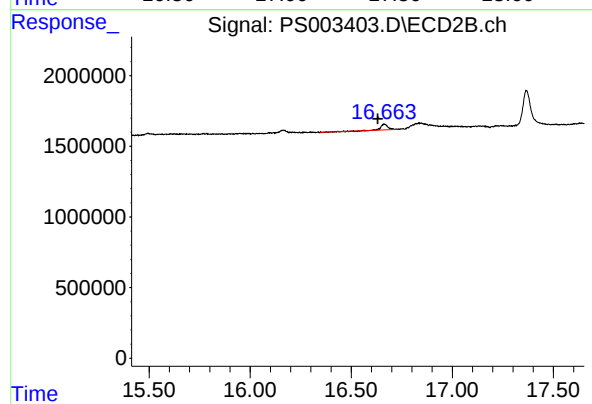

#16 DCPA

R.T.: 16.663 min
Delta R.T.: 0.031 min
Response: 1040900
Conc: 0.33 ng/ml