

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030419\
 Data File : PS003412.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2019 14:42
 Operator : EI\SJ
 Sample : K1665-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 200053

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 00:04:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.281	10.780	205.5E6	206.9E6	468.031	440.557
Target Compounds							
1) T	Dalapon	2.798	2.289	54471352	87317954	83.809	137.903 #
5) T	DICAMBA	0.000	11.020	0	9731748	N.D.	5.825 #
6) T	MCPD	11.974	11.319	4396194	-56506	3.348	N.D. #
9) T	2,4-D	13.135	12.684	3158234	1008415	6.809	1.921 #
10) T	Pentachlo...	13.503	13.191	38543797	37856364	5.456	5.748
12) T	2,4,5-T	0.000	14.384	0	13752861	N.D.	6.819 #
13) T	2,4-DB	15.559	0.000	4237980	0	17.897	N.D. #
15) T	Picloram	16.765	16.718	5303701	30679495	2.155	12.087 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030419\
Data File : PS003412.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2019 14:42
Operator : EI\SJ
Sample : K1665-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
200053

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 00:04:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

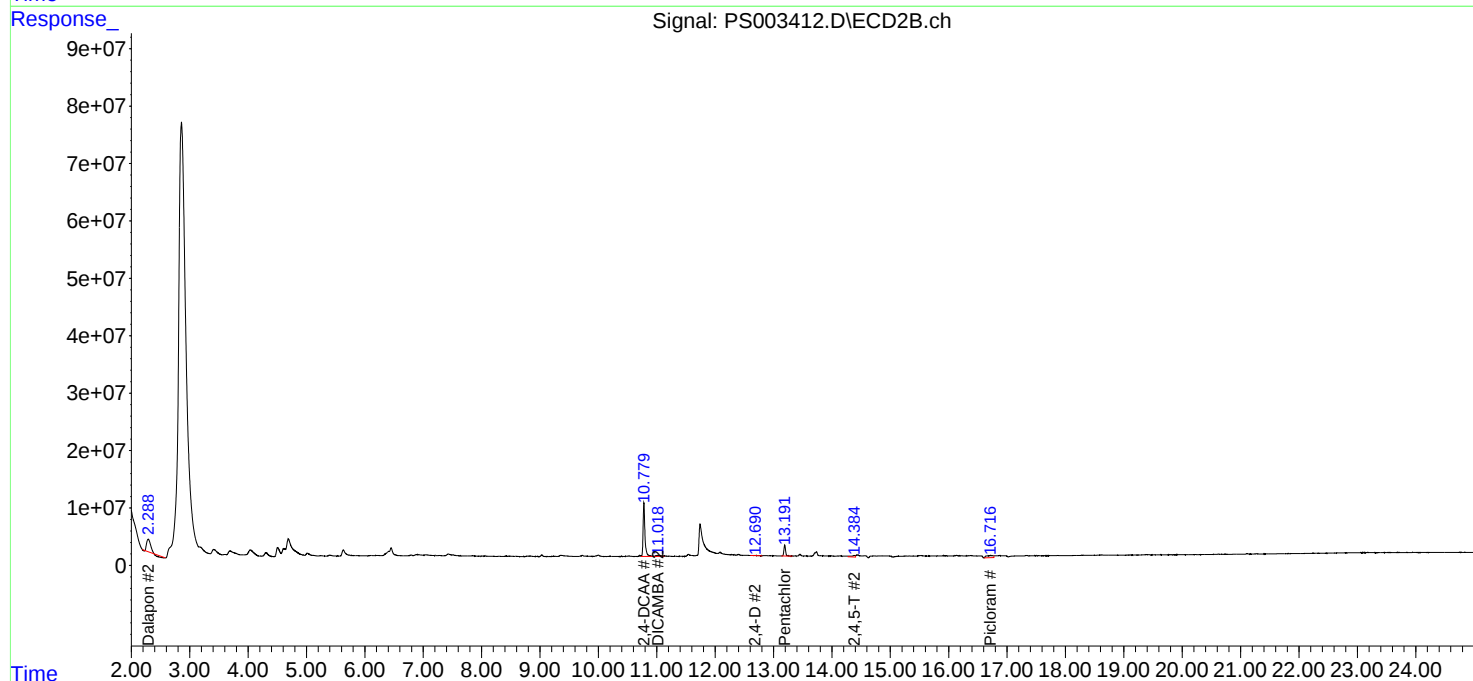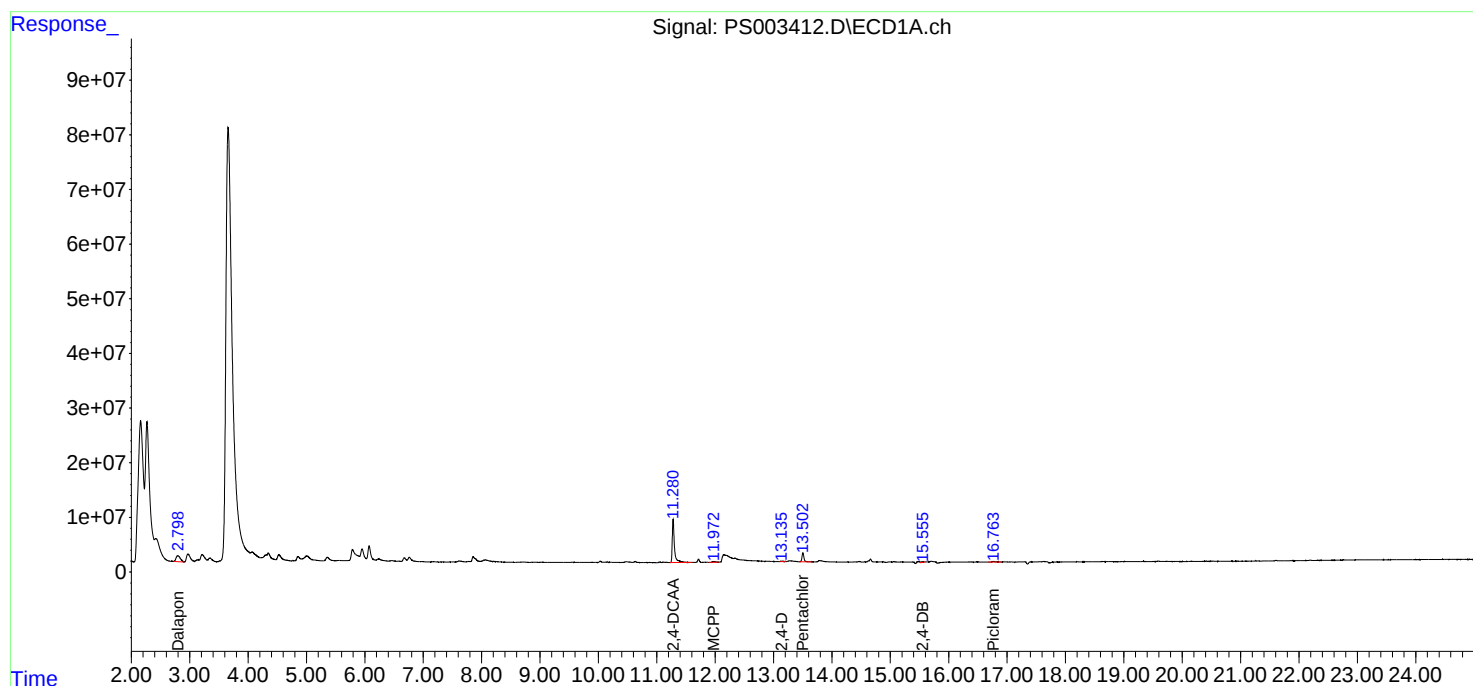


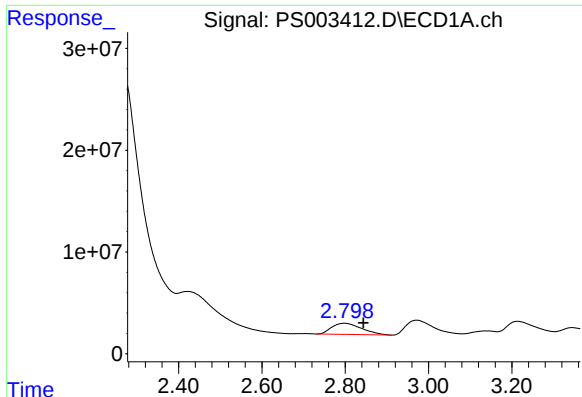

#1 Dalapon


R.T.: 2.798 min
Delta R.T.: -0.046 min
Response: 54471352
Conc: 83.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
200053

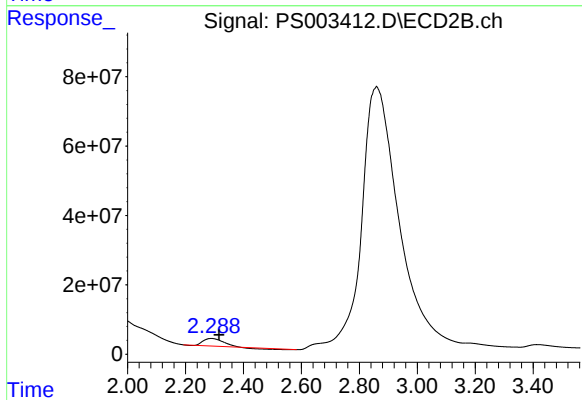


#1 Dalapon

R.T.: 2.289 min
Delta R.T.: -0.028 min
Response: 87317954
Conc: 137.90 ng/ml

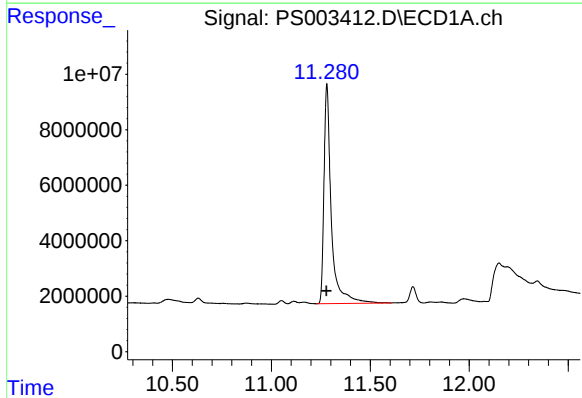


#4 2,4-DCAA

R.T.: 11.281 min
Delta R.T.: 0.003 min
Response: 205476926
Conc: 468.03 ng/ml

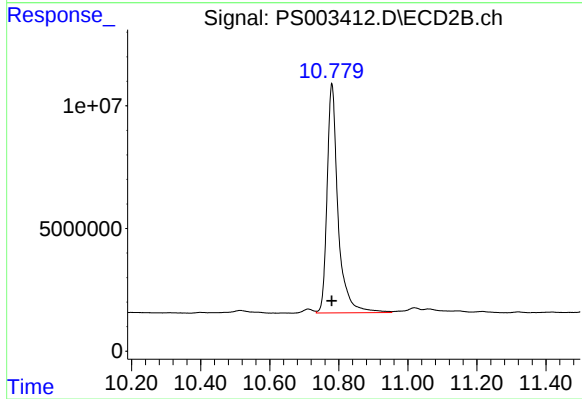

#4 2,4-DCAA


R.T.: 10.780 min
Delta R.T.: 0.000 min
Response: 206872029
Conc: 440.56 ng/ml

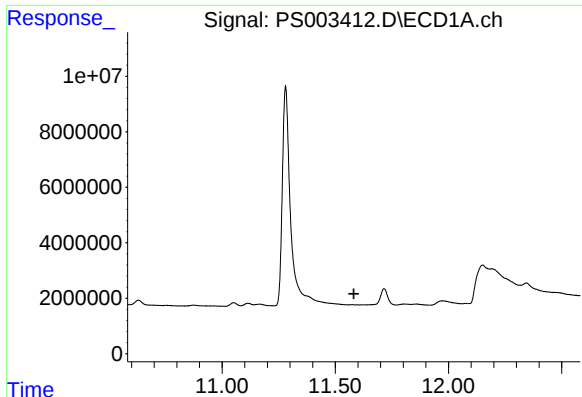

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
200053

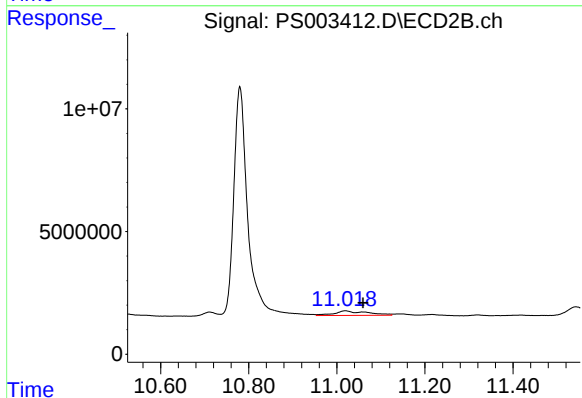


#5 DICAMBA

R.T.: 11.020 min
Delta R.T.: -0.040 min
Response: 9731748
Conc: 5.83 ng/ml

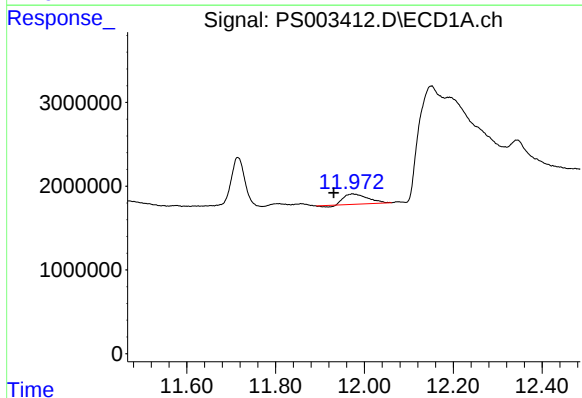


#6 MCP

R.T.: 11.974 min
Delta R.T.: 0.043 min
Response: 4396194
Conc: 3.35 ug/ml

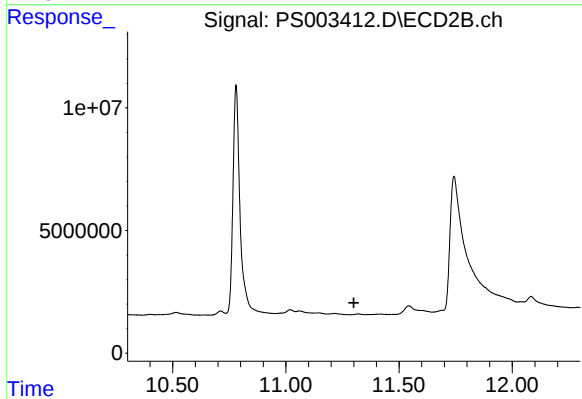

#6 MCP


R.T.: 11.319 min
Delta R.T.: 0.019 min
Response: -56506
Conc: N.D.

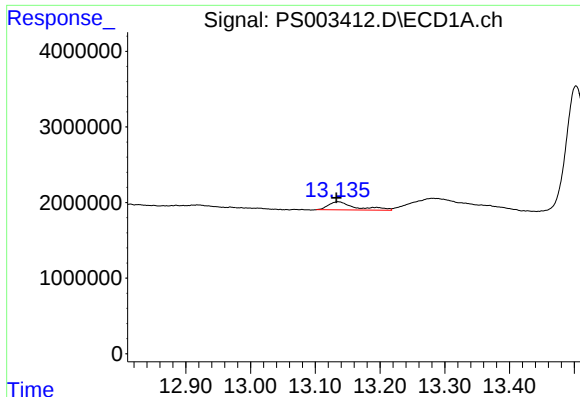

#9 2,4-D


R.T.: 13.135 min
Delta R.T.: 0.003 min
Response: 3158234
Conc: 6.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
200053

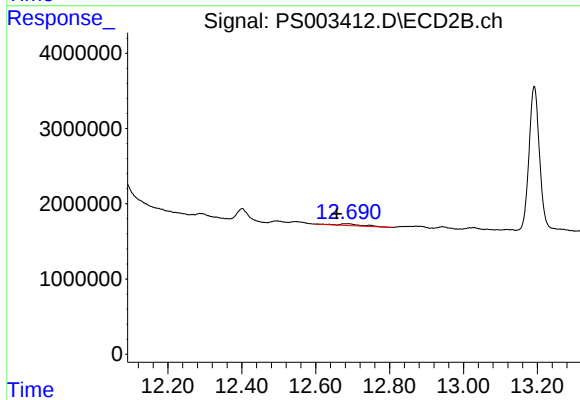


#9 2,4-D

R.T.: 12.684 min
Delta R.T.: 0.027 min
Response: 1008415
Conc: 1.92 ng/ml

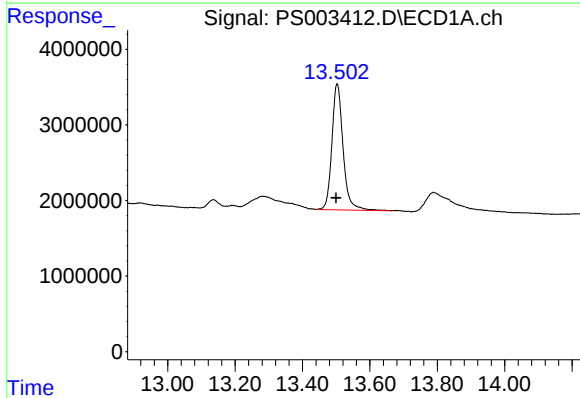


#10 Pentachlorophenol

R.T.: 13.503 min
Delta R.T.: 0.004 min
Response: 38543797
Conc: 5.46 ng/ml

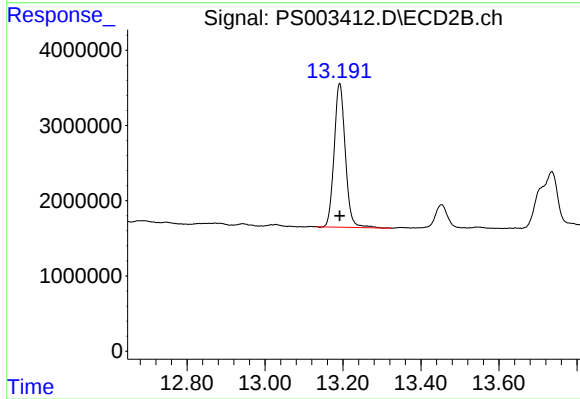

#10 Pentachlorophenol


R.T.: 13.191 min
Delta R.T.: 0.000 min
Response: 37856364
Conc: 5.75 ng/ml

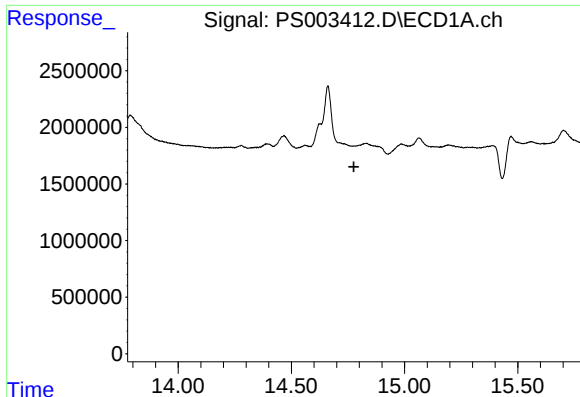

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
200053

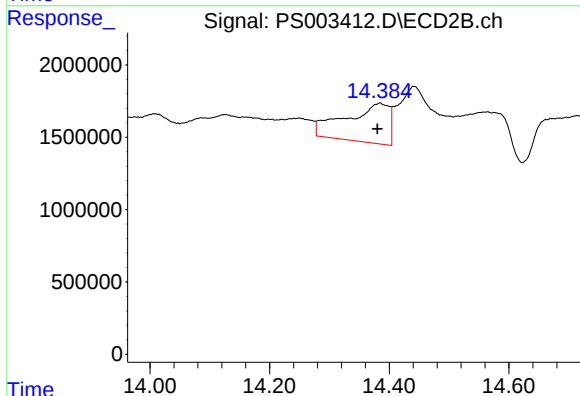


#12 2,4,5-T

R.T.: 14.384 min
Delta R.T.: 0.004 min
Response: 13752861
Conc: 6.82 ng/ml

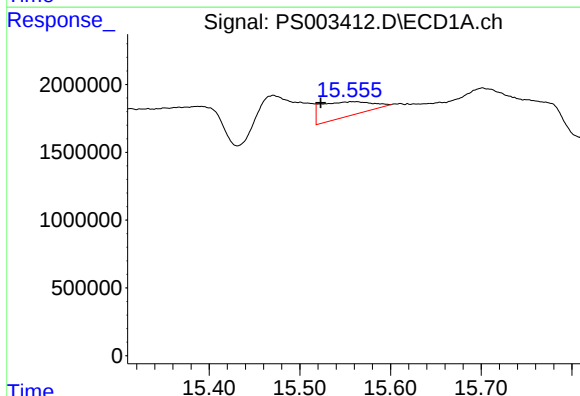


#13 2,4-DB

R.T.: 15.559 min
Delta R.T.: 0.036 min
Response: 4237980
Conc: 17.90 ng/ml

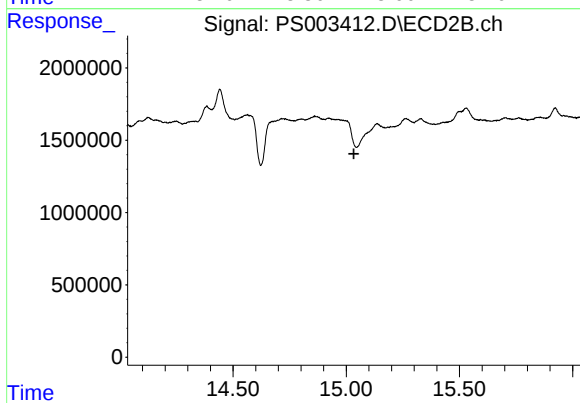

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.033 min
Response: 0
Conc: N.D.

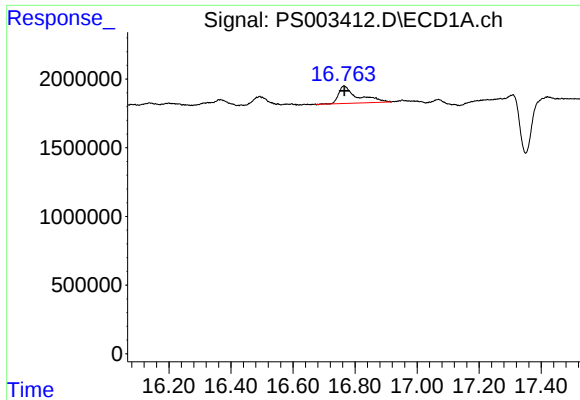

#15 Picloram

R.T.: 16.765 min
Delta R.T.: 0.000 min
Response: 5303701
Conc: 2.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
200053

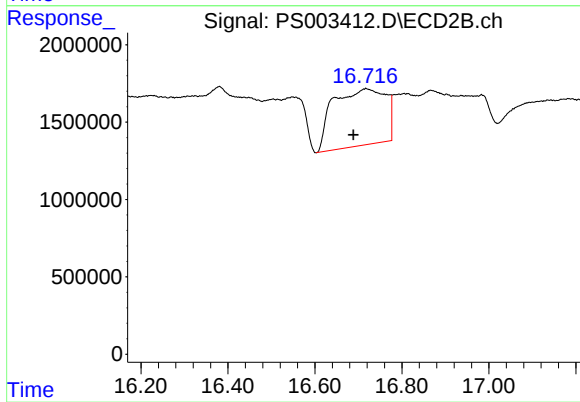

#15 Picloram

R.T.: 16.718 min
Delta R.T.: 0.030 min
Response: 30679495
Conc: 12.09 ng/ml