

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030419\
 Data File : PS003414.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2019 15:44
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 00:04:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.283	10.781	218.8E6	193.7E6	498.364	412.406
Target Compounds							
7) T	MCPA	0.000	11.667	0	362214	N.D.	0.210 #
8) T	DICHLORPROP	0.000	12.211	0	584913	N.D.	1.415 #
9) T	2,4-D	0.000	12.668	0	163277	N.D.	0.311 #
10) T	Pentachlo...	0.000	13.200	0	1051572	N.D.	0.160 #
11) T	2,4,5-TP ...	0.000	13.847	0	261282	N.D.	0.103 #
14) T	DINOSEB	0.000	15.502	0	708407	N.D.	0.397 #
15) T	Picloram	0.000	16.637	0	464050	N.D.	0.183 #
16) T	DCPA	0.000	16.637	0	464050	N.D.	0.149 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030419\
Data File : PS003414.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2019 15:44
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 00:04:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

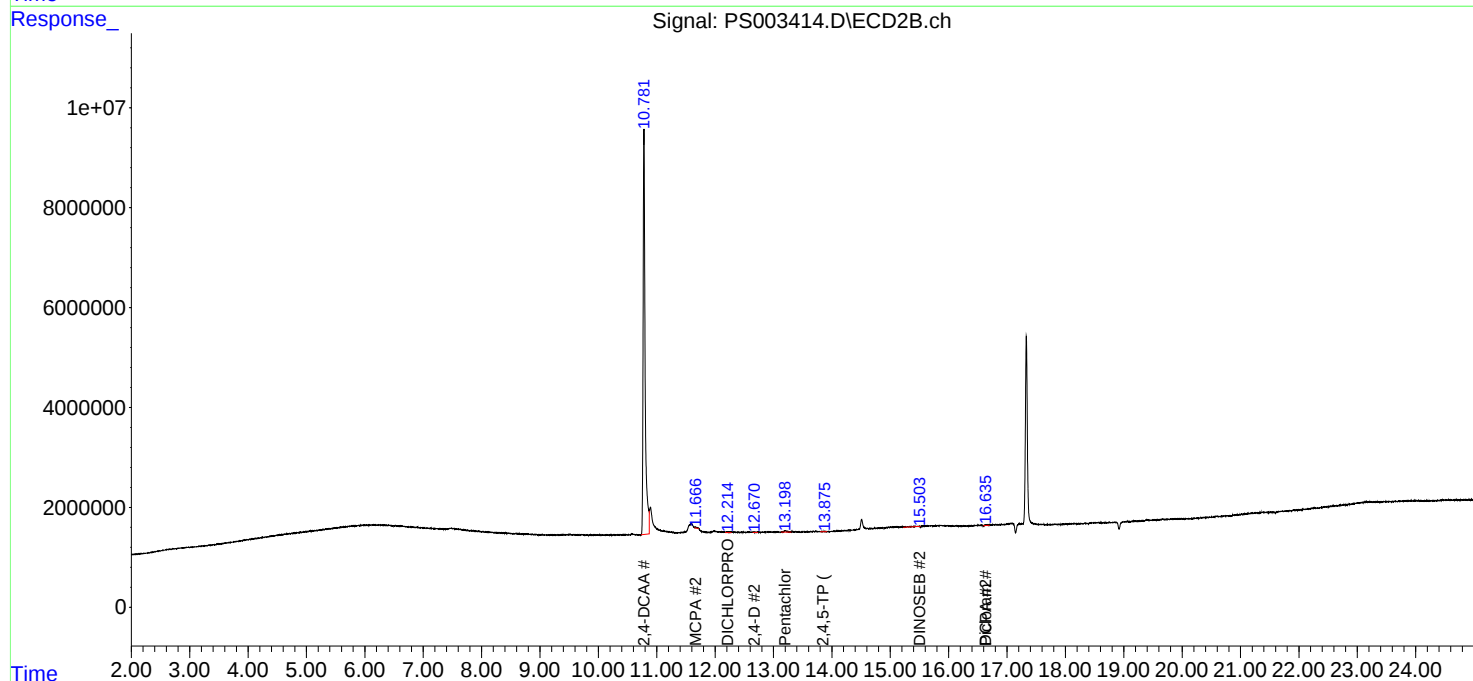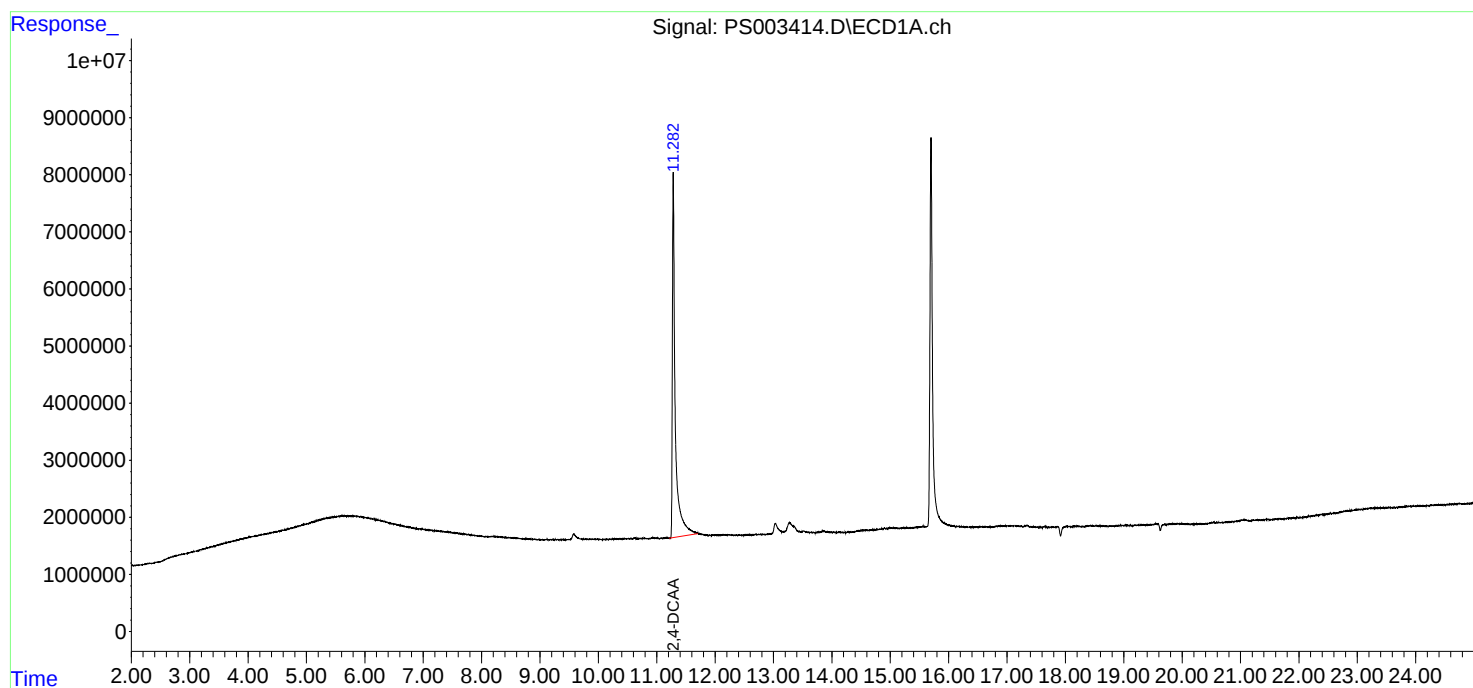


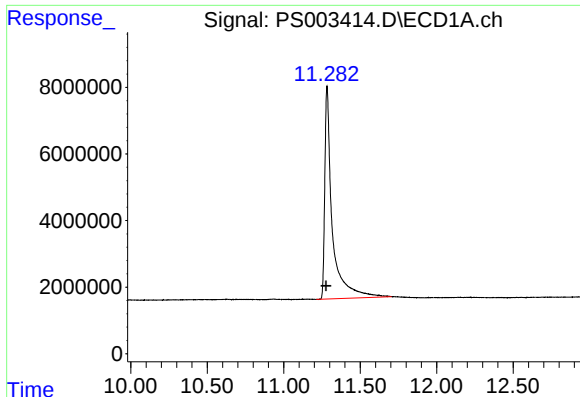

#4 2,4-DCAA


R.T.: 11.283 min
Delta R.T.: 0.005 min
Response: 218793861
Conc: 498.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

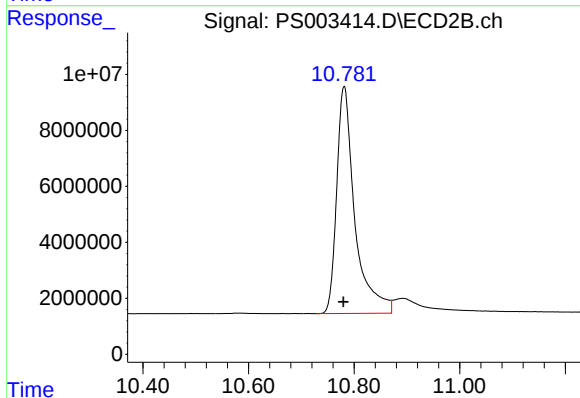


#4 2,4-DCAA

R.T.: 10.781 min
Delta R.T.: 0.001 min
Response: 193653109
Conc: 412.41 ng/ml

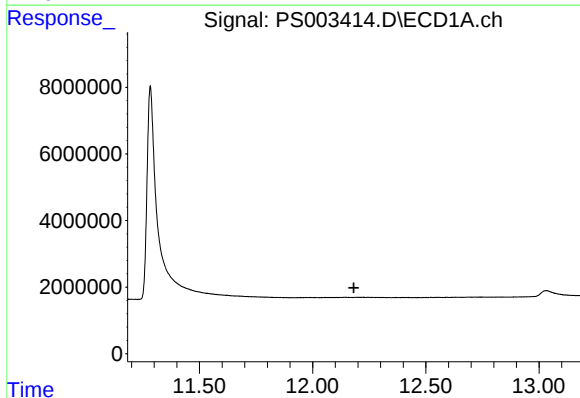


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

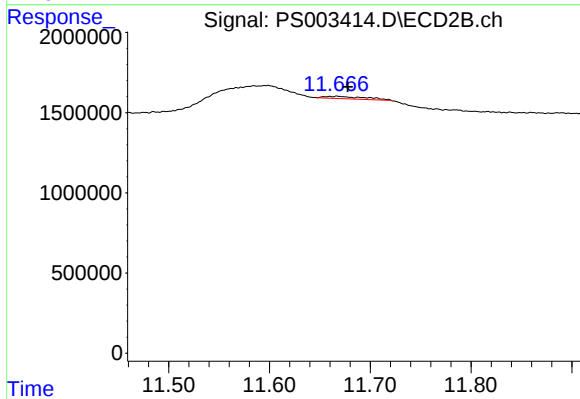

#7 MCPA


R.T.: 11.667 min
Delta R.T.: -0.010 min
Response: 362214
Conc: 0.21 ug/ml

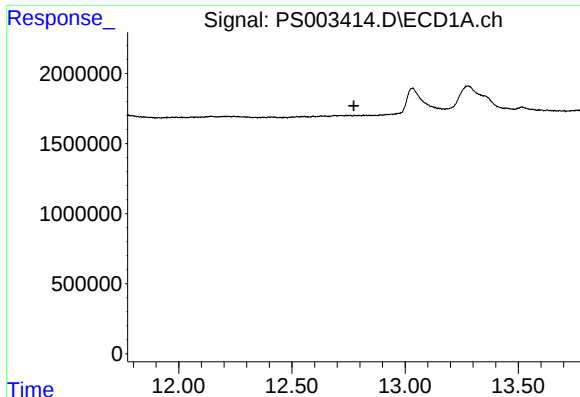

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

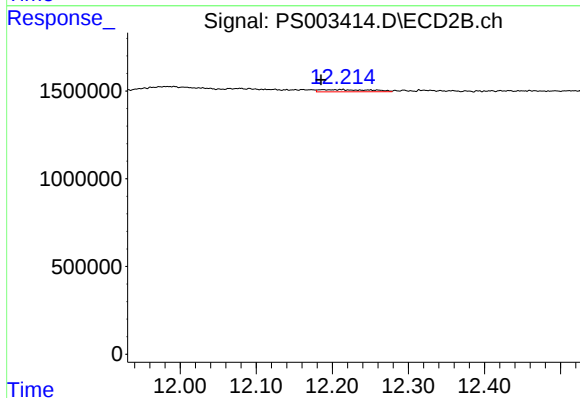


#8 DICHLORPROP

R.T.: 12.211 min
Delta R.T.: 0.026 min
Response: 584913
Conc: 1.42 ng/ml

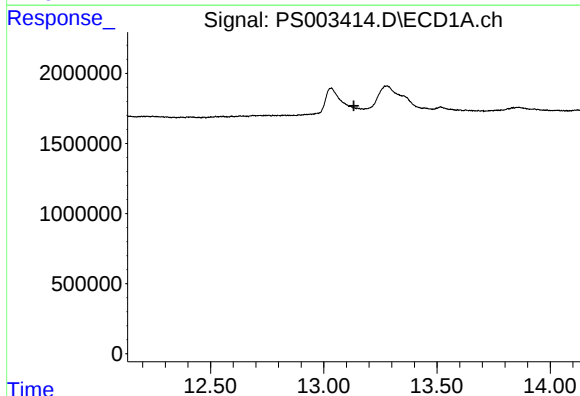


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.133 min
Response: 0
Conc: N.D.

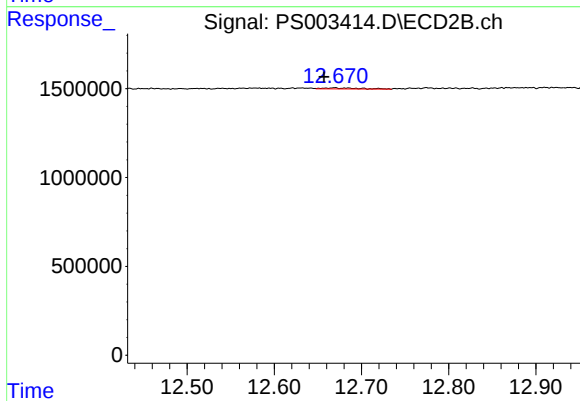

#9 2,4-D


R.T.: 12.668 min
Delta R.T.: 0.011 min
Response: 163277
Conc: 0.31 ng/ml

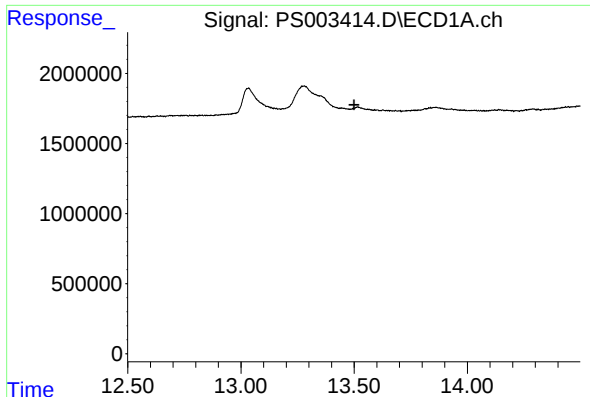

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

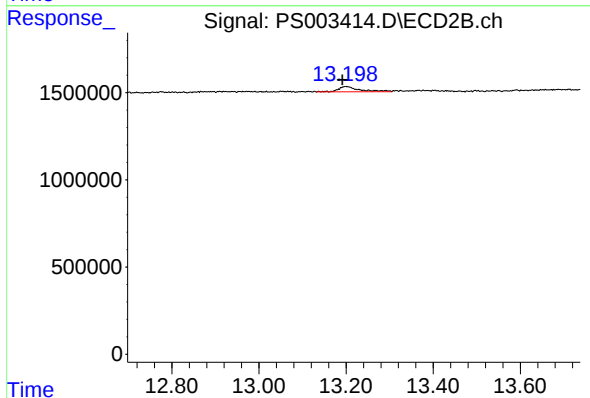


#10 Pentachlorophenol

R.T.: 13.200 min
Delta R.T.: 0.008 min
Response: 1051572
Conc: 0.16 ng/ml

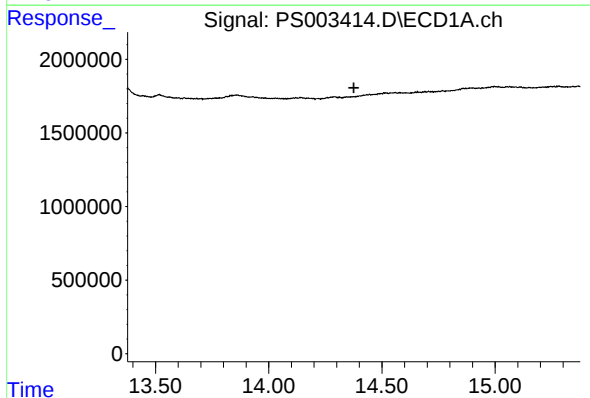


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

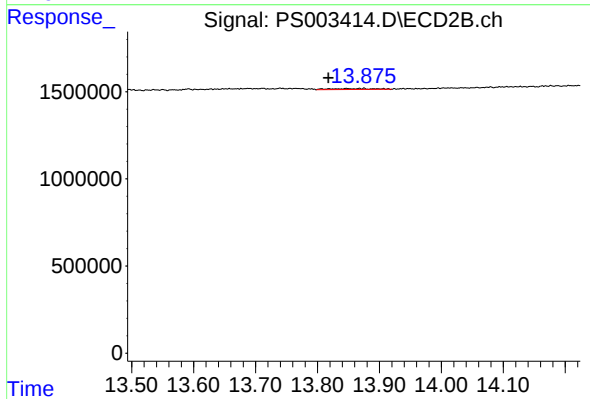

#11 2,4,5-TP (SILVEX)


R.T.: 13.847 min
Delta R.T.: 0.030 min
Response: 261282
Conc: 0.10 ng/ml

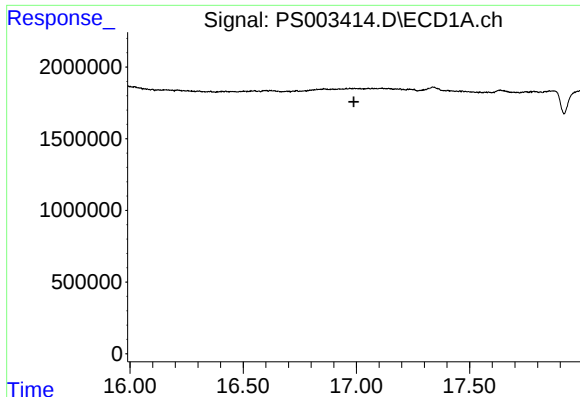

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

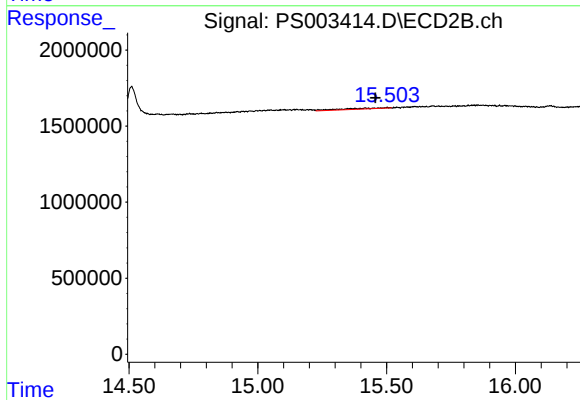


#14 DINOSEB

R.T.: 15.502 min
Delta R.T.: 0.046 min
Response: 708407
Conc: 0.40 ng/ml

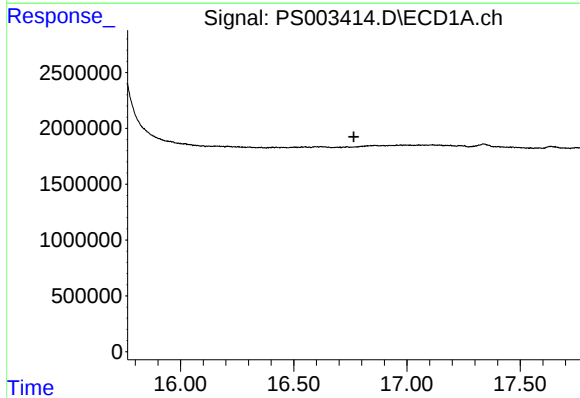


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.765 min
Response: 0
Conc: N.D.

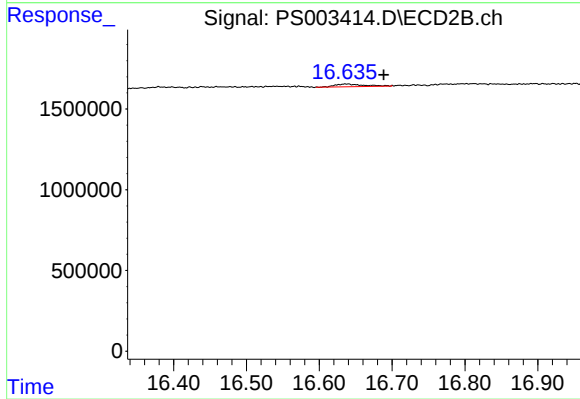

#15 Picloram


R.T.: 16.637 min
Delta R.T.: -0.051 min
Response: 464050
Conc: 0.18 ng/ml

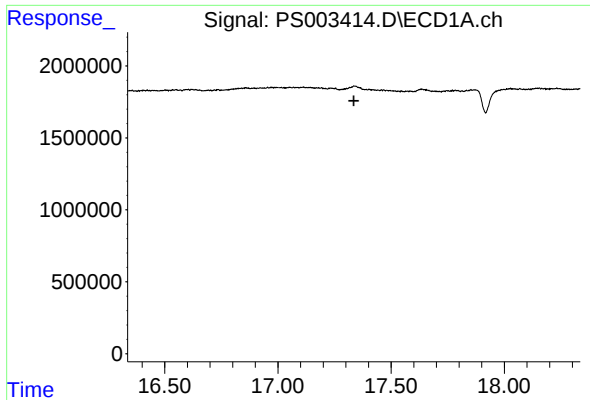

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

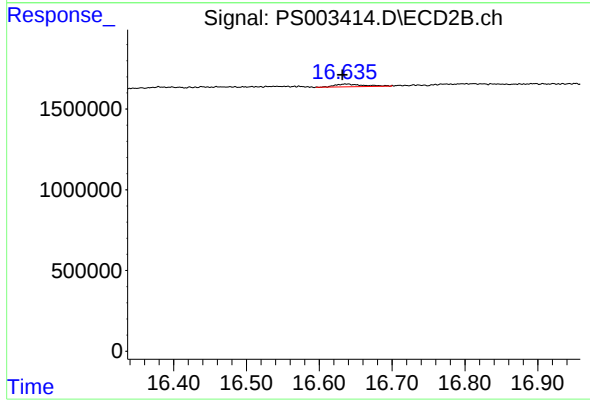

#16 DCPA

R.T.: 16.637 min
Delta R.T.: 0.005 min
Response: 464050
Conc: 0.15 ng/ml