

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030419\
 Data File : PS003424.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2019 21:06
 Operator : EI\SJ
 Sample : K1688-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 JC-03-030119-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 00:07:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.305	10.806	259.6E6	275.3E6	591.365	586.374
Target Compounds							
1) T	Dalapon	2.824	2.314	48026784	102.3E6	73.894	161.627 #
2) T	3,5-DICHL...	0.000	8.973	0	3768101	N.D.	6.103 #
5) T	DICAMBA	0.000	11.046	0	5487850	N.D.	3.285 #
6) T	MCP	0.000	11.296	0	372737	N.D.	0.316 #
7) T	MCPA	12.243	0.000	42596890	0	21.475	N.D. #
11) T	2,4,5-TP ...	0.000	13.763	0	18961064	N.D.	7.446 #
12) T	2,4,5-T	0.000	14.408	0	18310005	N.D.	9.079 #
13) T	2,4-DB	15.503	0.000	19624617	0	82.876	N.D. #
14) T	DINOSEB	0.000	15.525	0	12708806	N.D.	7.120 #
15) T	Picloram	16.787	0.000	5926090	0	2.408	N.D. #
16) T	DCPA	0.000	16.577	0	23432420	N.D.	7.534 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030419\
Data File : PS003424.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2019 21:06
Operator : EI\SJ
Sample : K1688-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
JC-03-030119-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 00:07:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

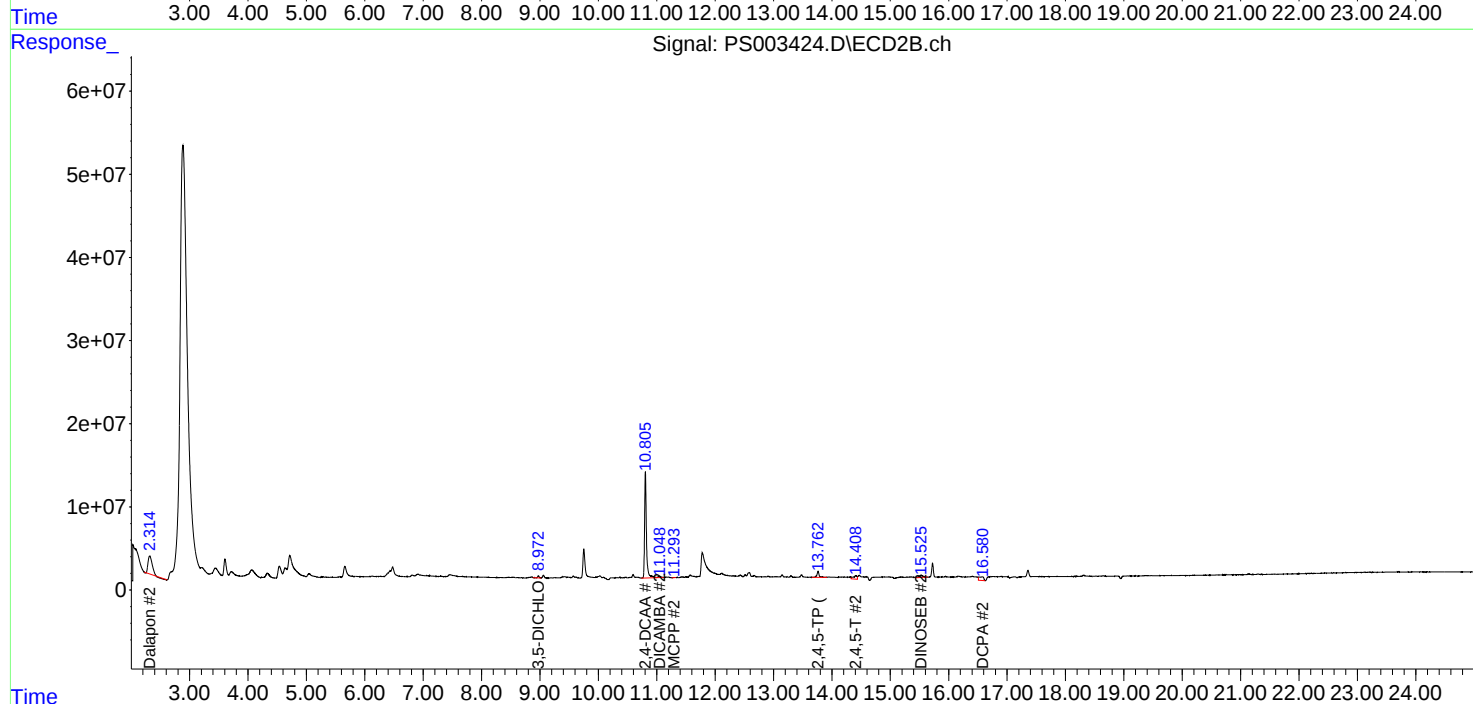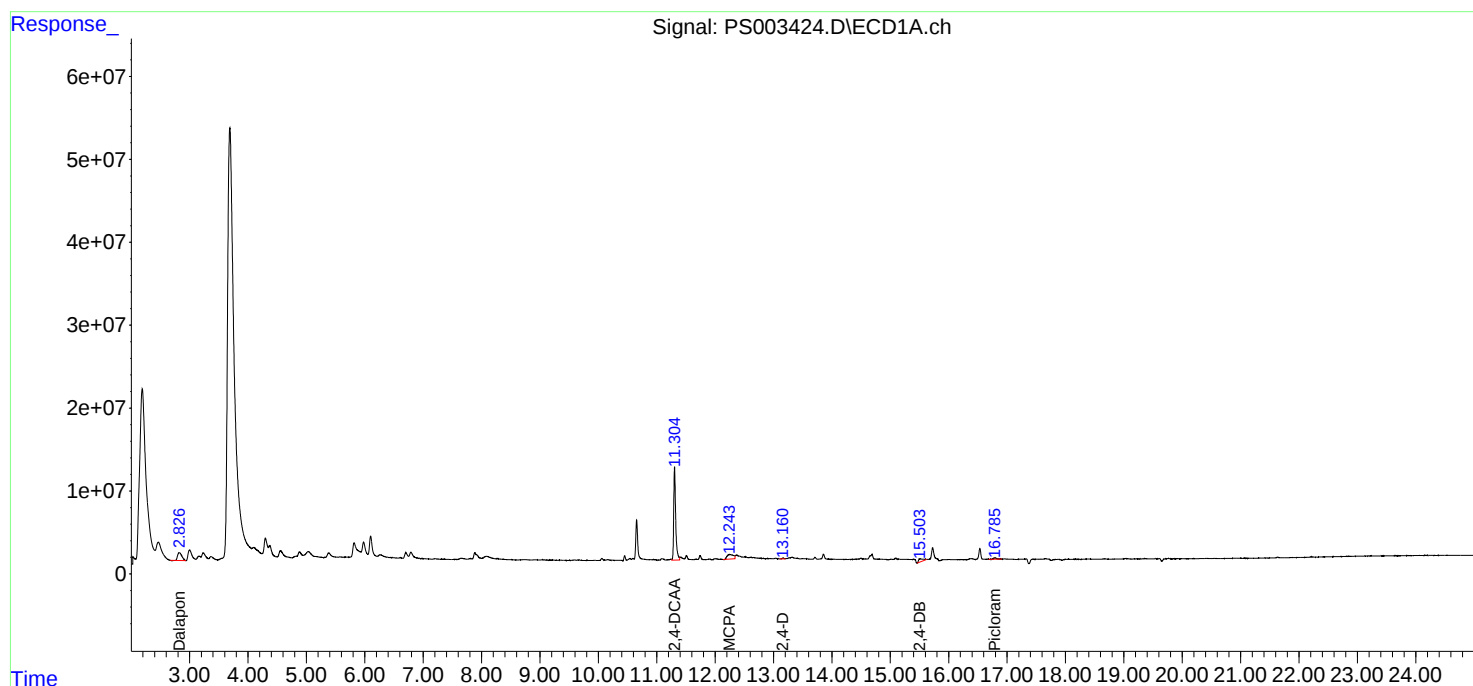


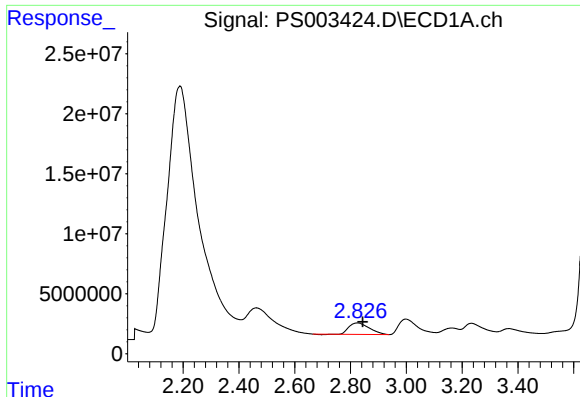

#1 Dalapon


R.T.: 2.824 min
Delta R.T.: -0.020 min
Response: 48026784
Conc: 73.89 ng/ml

Instrument :
ECD_S
ClientSampleId :
JC-03-030119-D

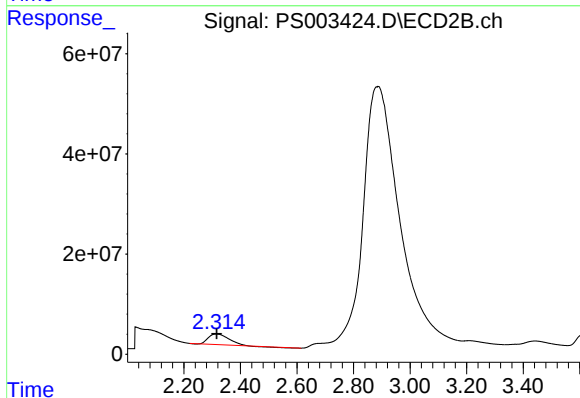


#1 Dalapon

R.T.: 2.314 min
Delta R.T.: -0.003 min
Response: 102339986
Conc: 161.63 ng/ml

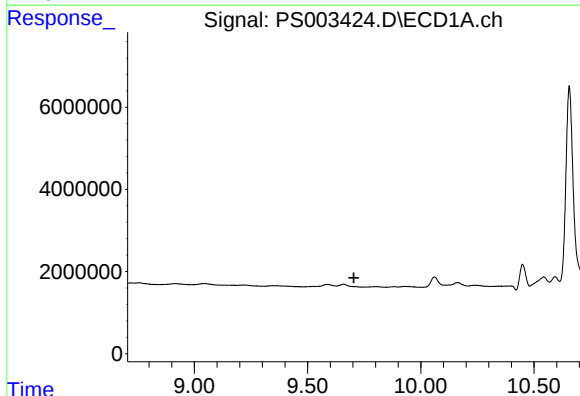


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

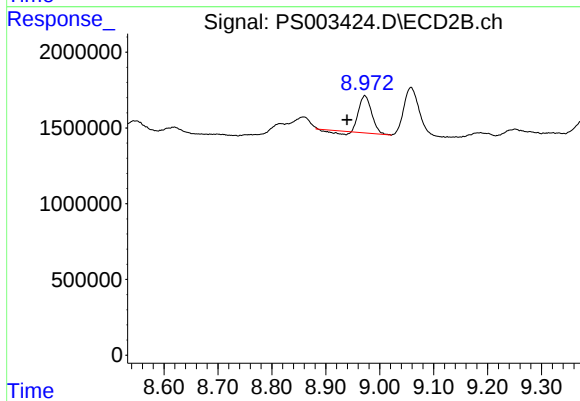

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.973 min
Delta R.T.: 0.033 min
Response: 3768101
Conc: 6.10 ng/ml

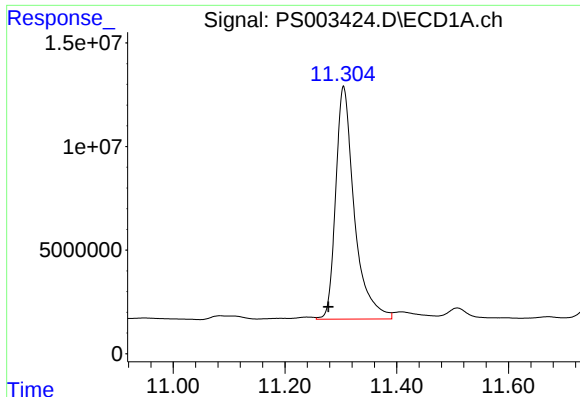

#4 2,4-DCAA


R.T.: 11.305 min
Delta R.T.: 0.027 min
Response: 259623664
Conc: 591.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
JC-03-030119-D

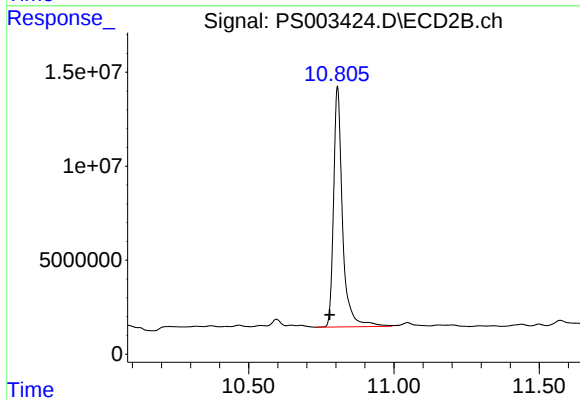


#4 2,4-DCAA

R.T.: 10.806 min
Delta R.T.: 0.026 min
Response: 275343076
Conc: 586.37 ng/ml

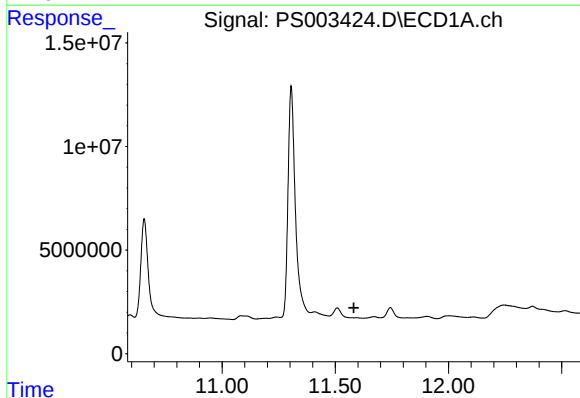


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

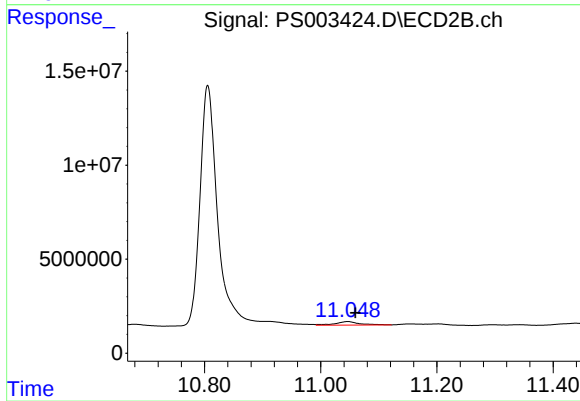

#5 DICAMBA


R.T.: 11.046 min
Delta R.T.: -0.013 min
Response: 5487850
Conc: 3.28 ng/ml

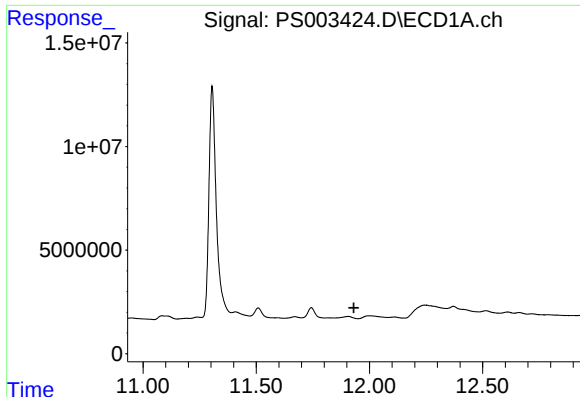

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
JC-03-030119-D

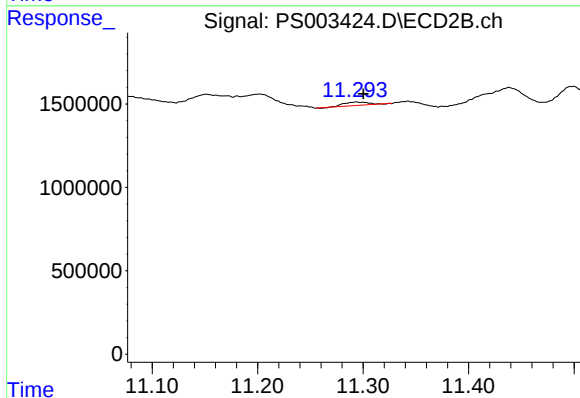


#6 MCPP

R.T.: 11.296 min
Delta R.T.: -0.005 min
Response: 372737
Conc: 0.32 ug/ml

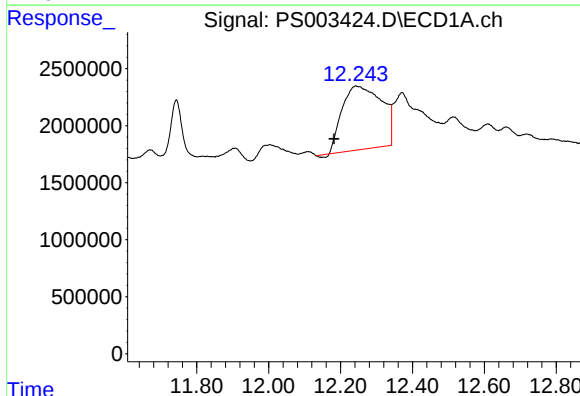


#7 MCPA

R.T.: 12.243 min
Delta R.T.: 0.060 min
Response: 42596890
Conc: 21.48 ug/ml

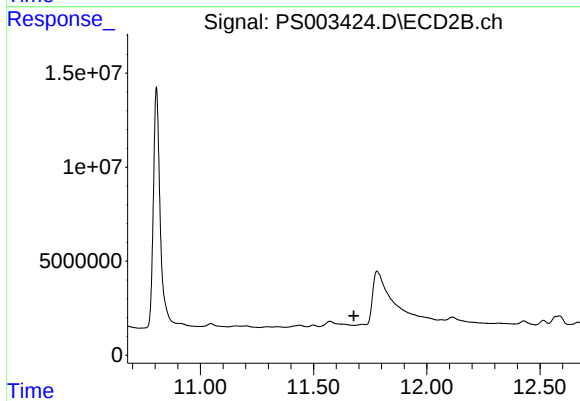

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 11.678 min
Response: 0
Conc: N.D.

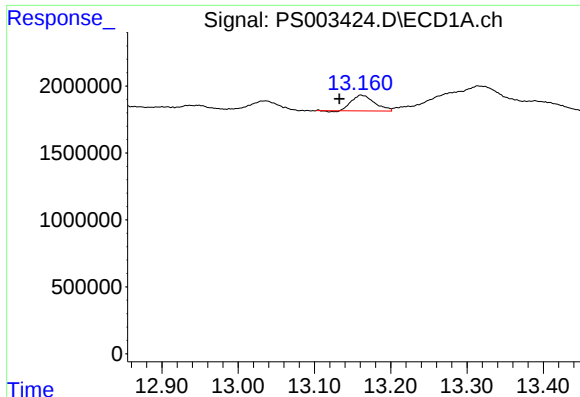

#9 2,4-D


R.T.: 13.162 min
Delta R.T.: 0.029 min
Response: 2444758
Conc: 5.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
JC-03-030119-D

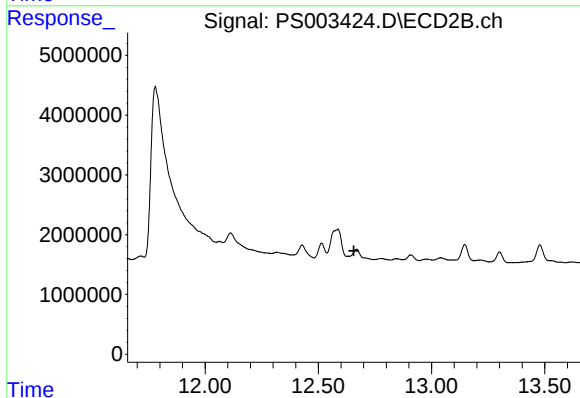


#9 2,4-D

R.T.: 12.668 min
Delta R.T.: 0.011 min
Response: -6693008
Conc: N.D.

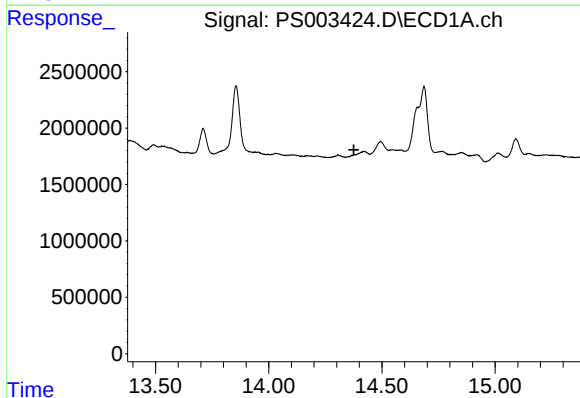


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.376 min
Response: 0
Conc: N.D.

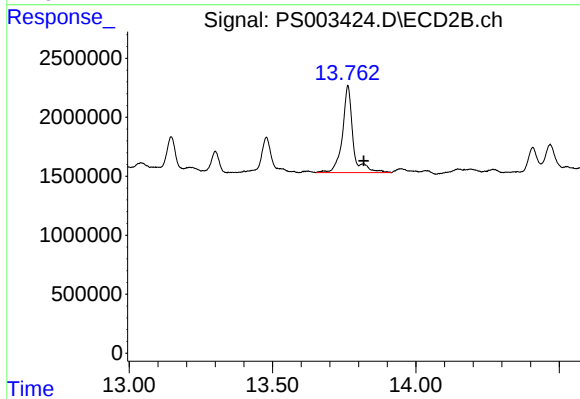

#11 2,4,5-TP (SILVEX)


R.T.: 13.763 min
Delta R.T.: -0.055 min
Response: 18961064
Conc: 7.45 ng/ml

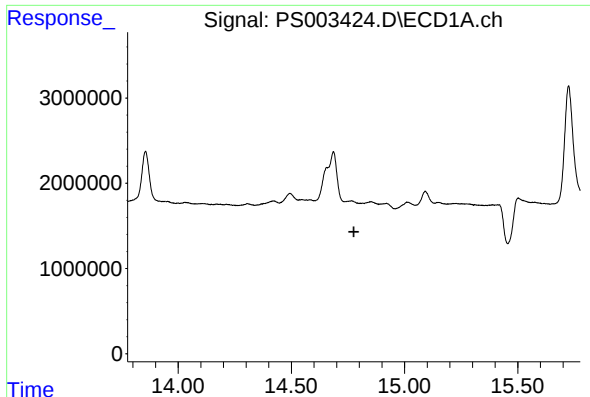

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
JC-03-030119-D

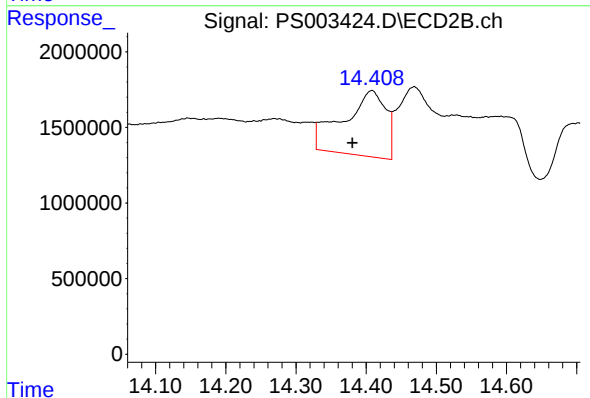


#12 2,4,5-T

R.T.: 14.408 min
Delta R.T.: 0.027 min
Response: 18310005
Conc: 9.08 ng/ml

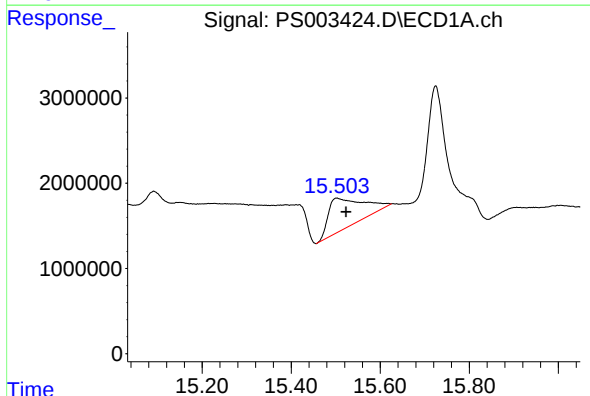


#13 2,4-DB

R.T.: 15.503 min
Delta R.T.: -0.021 min
Response: 19624617
Conc: 82.88 ng/ml

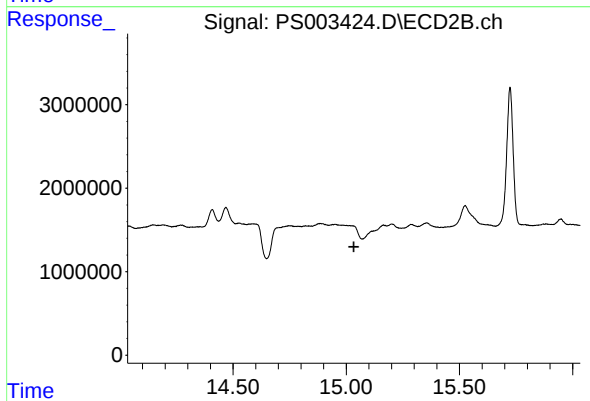

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.033 min
Response: 0
Conc: N.D.

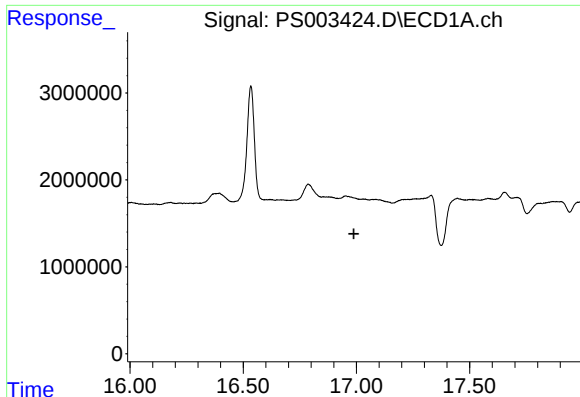

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
JC-03-030119-D

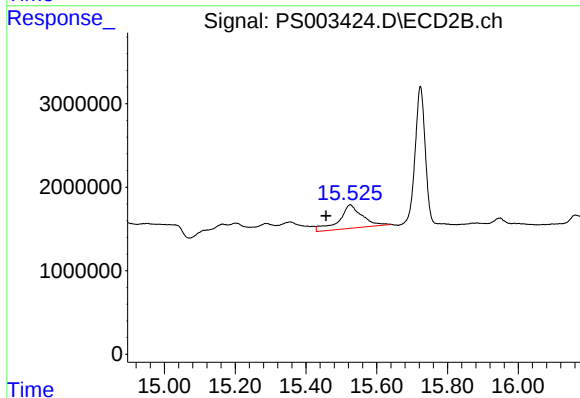


#14 DINOSEB

R.T.: 15.525 min
Delta R.T.: 0.068 min
Response: 12708806
Conc: 7.12 ng/ml

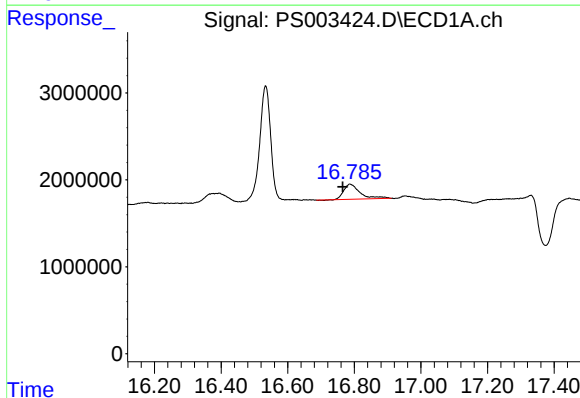


#15 Picloram

R.T.: 16.787 min
Delta R.T.: 0.022 min
Response: 5926090
Conc: 2.41 ng/ml

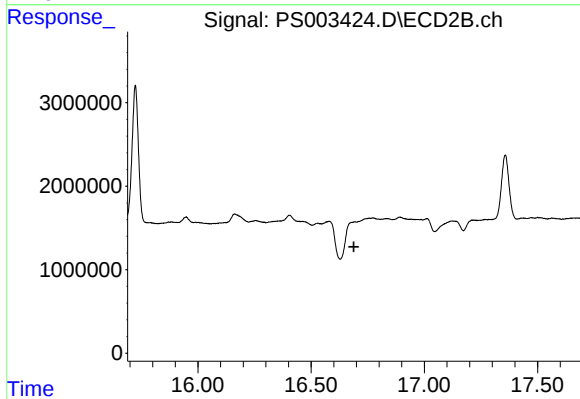

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.688 min
Response: 0
Conc: N.D.

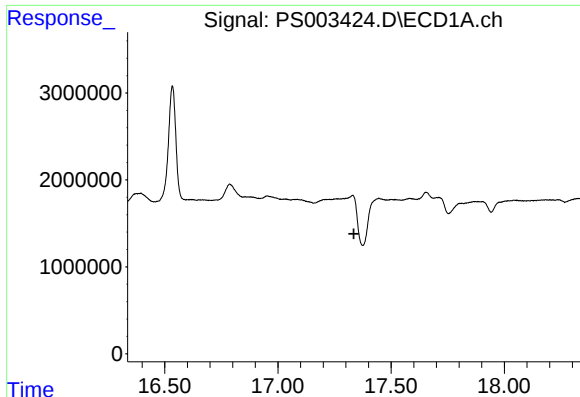

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
JC-03-030119-D

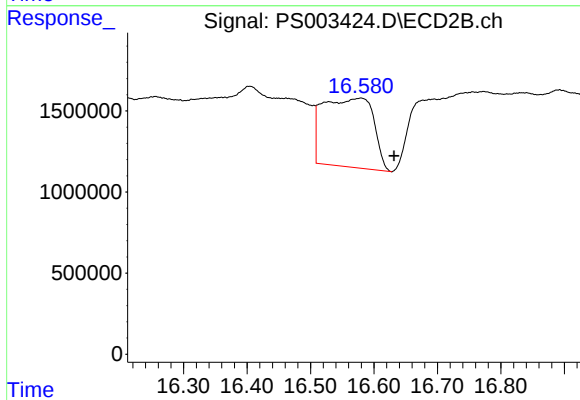

#16 DCPA

R.T.: 16.577 min
Delta R.T.: -0.055 min
Response: 23432420
Conc: 7.53 ng/ml