

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030419\
 Data File : PS003425.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2019 21:37
 Operator : EI\SJ
 Sample : K1688-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 JC-03-030119-E

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 00:08:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.306	10.806	259.6E6	264.4E6	591.379	562.995
Target Compounds							
1) T	Dalapon	2.826	2.315	42026712	95568583	64.662	150.933 #
2) T	3,5-DICHL...	0.000	8.973	0	4608928	N.D.	7.464 #
5) T	DICAMBA	0.000	11.046	0	4298750	N.D.	2.573 #
6) T	MCP	0.000	11.293	0	428922	N.D.	0.363 #
11) T	2,4,5-TP ...	0.000	13.817	0	1730030	N.D.	0.679 #
12) T	2,4,5-T	0.000	14.408	0	13734197	N.D.	6.810 #
15) T	Picloram	16.791	0.000	6755025	0	2.745	N.D. #
16) T	DCPA	0.000	16.577	0	13759160	N.D.	4.424 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030419\
Data File : PS003425.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2019 21:37
Operator : EI\SJ
Sample : K1688-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
JC-03-030119-E

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 00:08:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

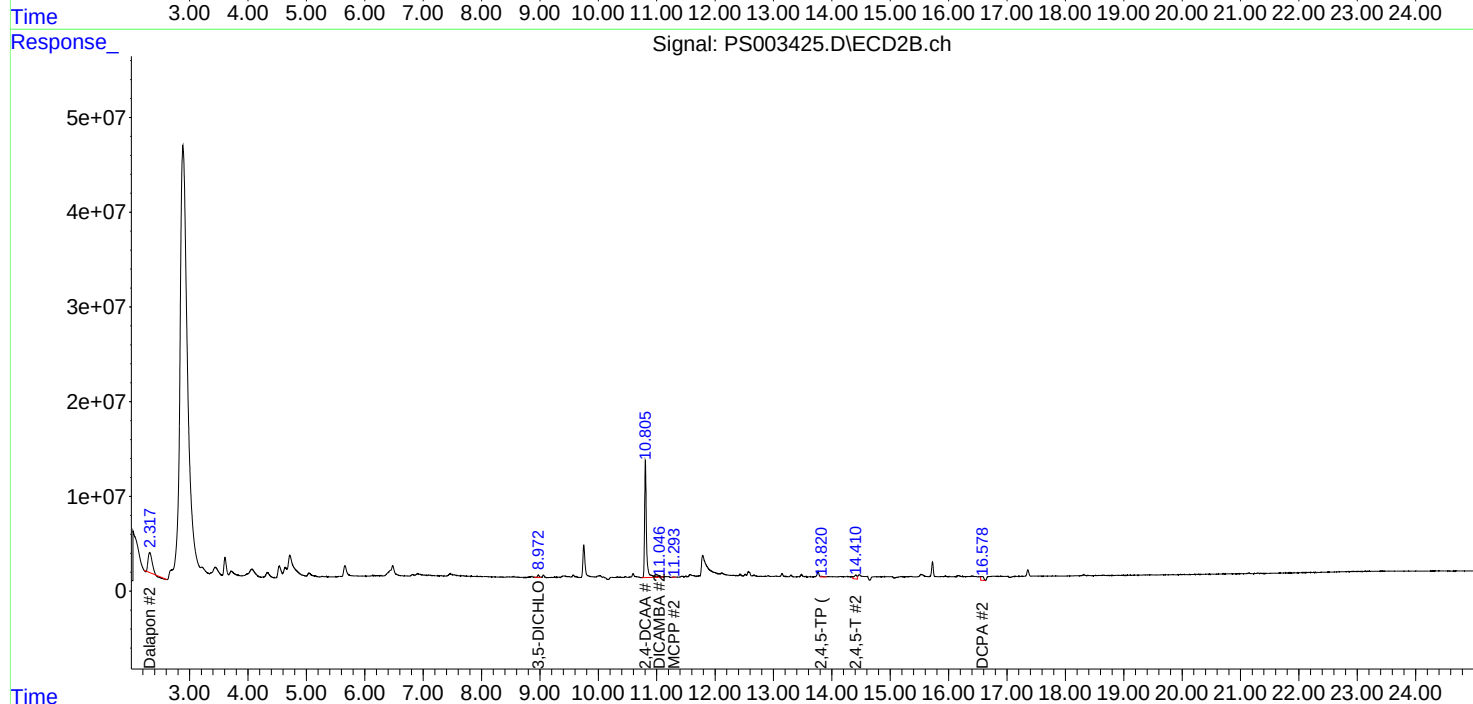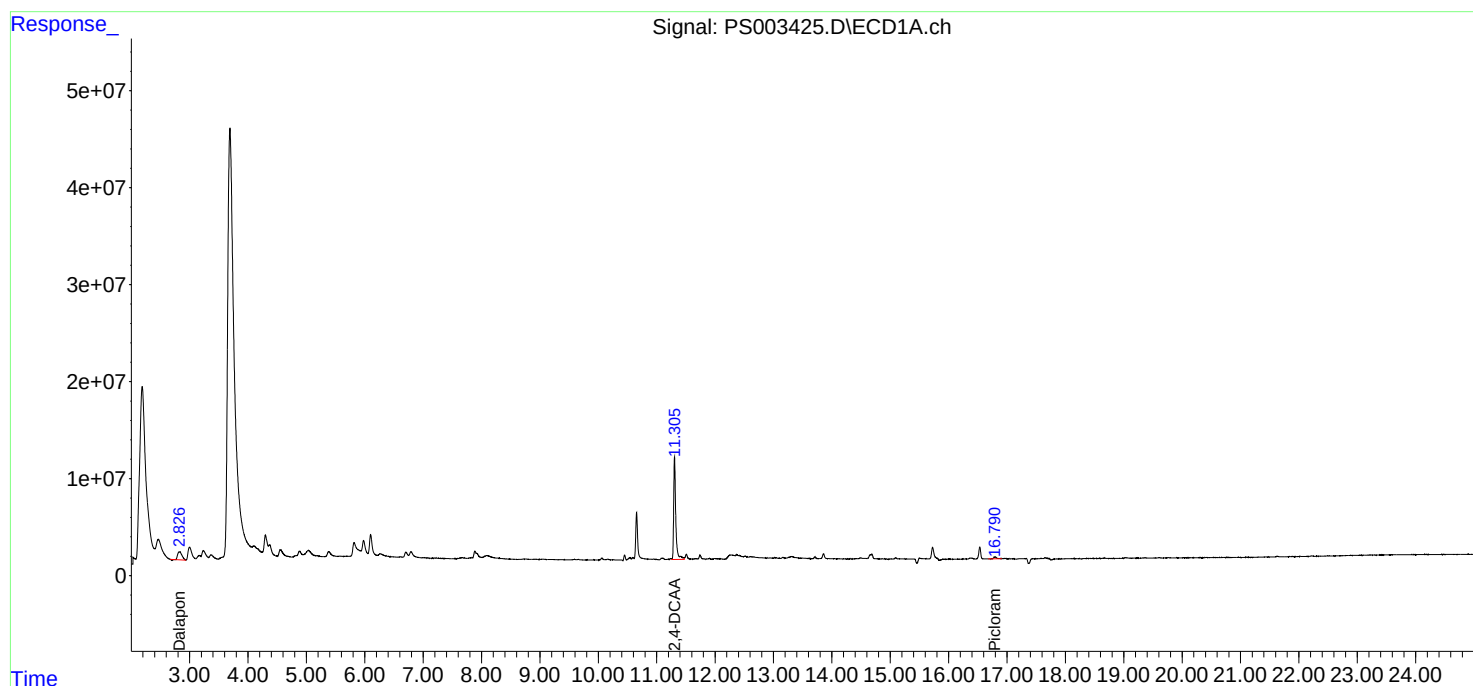


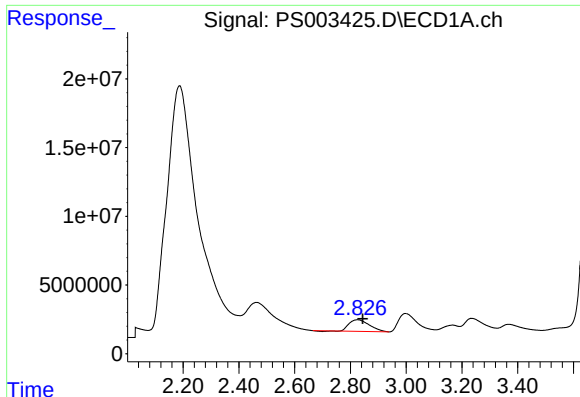

#1 Dalapon


R.T.: 2.826 min
Delta R.T.: -0.018 min
Response: 42026712
Conc: 64.66 ng/ml

Instrument :
ECD_S
ClientSampleId :
JC-03-030119-E

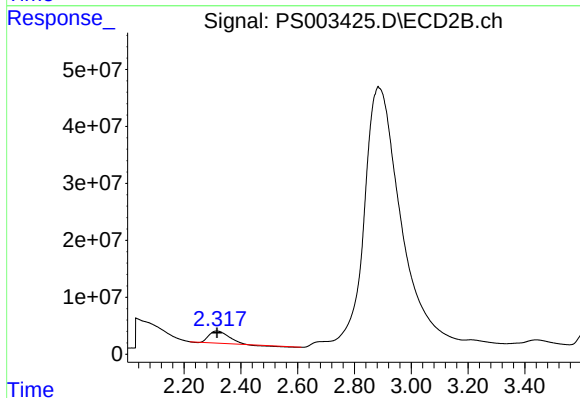


#1 Dalapon

R.T.: 2.315 min
Delta R.T.: -0.001 min
Response: 95568583
Conc: 150.93 ng/ml

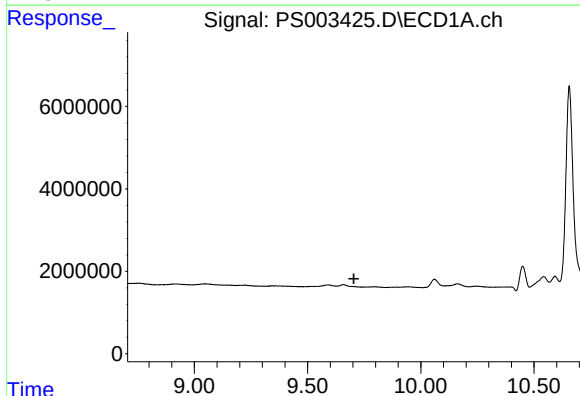


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.705 min
Response: 0
Conc: N.D.

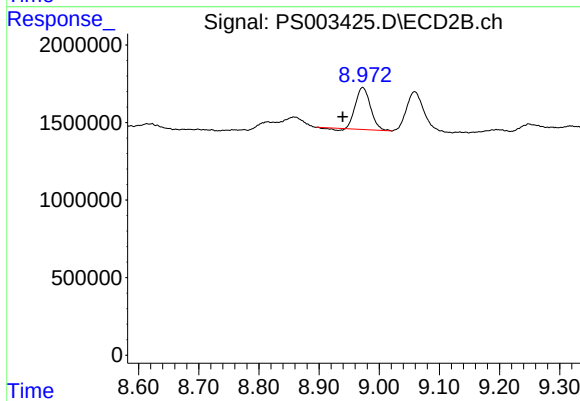

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.973 min
Delta R.T.: 0.033 min
Response: 4608928
Conc: 7.46 ng/ml

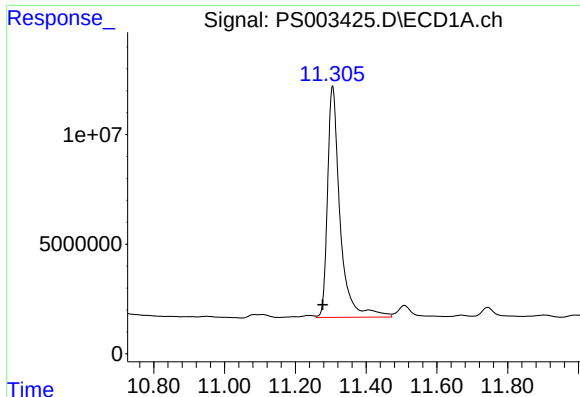

#4 2,4-DCAA


R.T.: 11.306 min
Delta R.T.: 0.028 min
Response: 259629975
Conc: 591.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
JC-03-030119-E

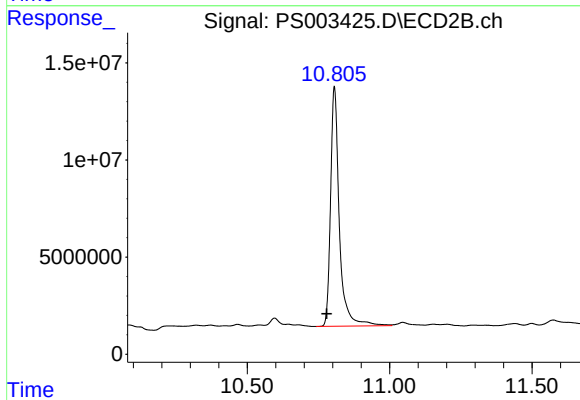


#4 2,4-DCAA

R.T.: 10.806 min
Delta R.T.: 0.026 min
Response: 264364874
Conc: 562.99 ng/ml

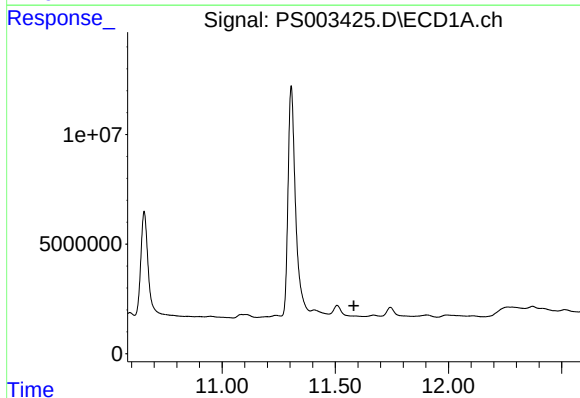


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.582 min
Response: 0
Conc: N.D.

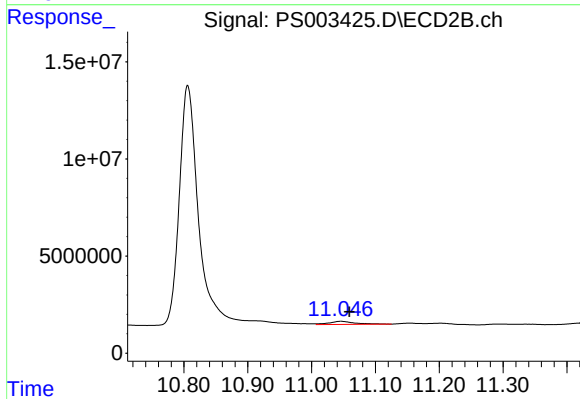

#5 DICAMBA


R.T.: 11.046 min
Delta R.T.: -0.014 min
Response: 4298750
Conc: 2.57 ng/ml

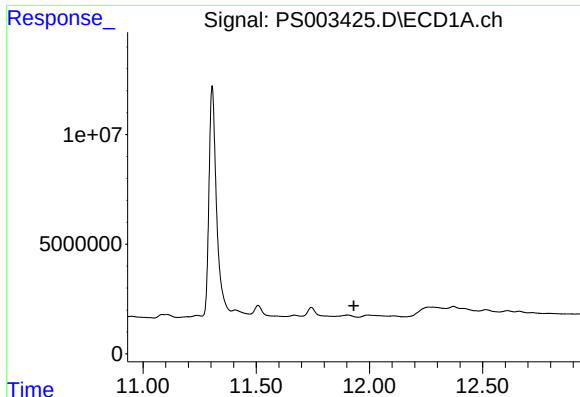

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
JC-03-030119-E

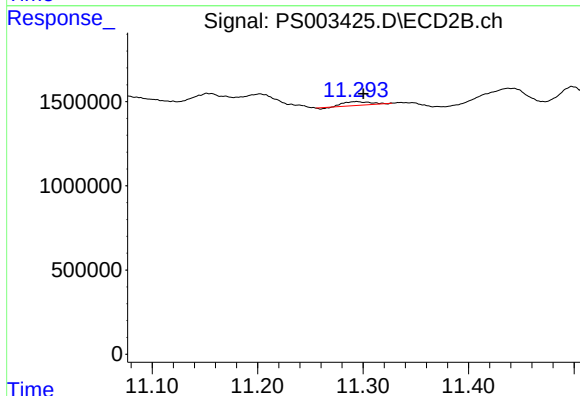


#6 MCP

R.T.: 11.293 min
Delta R.T.: -0.007 min
Response: 428922
Conc: 0.36 ug/ml

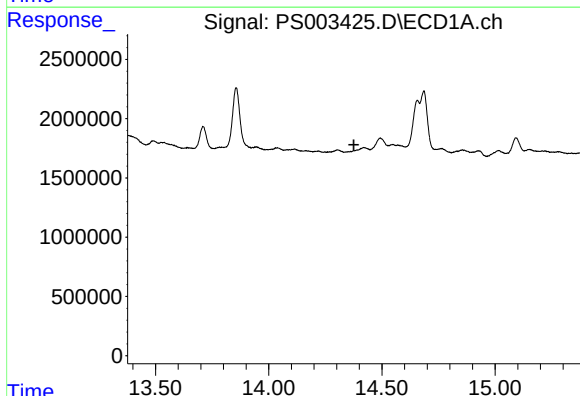


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

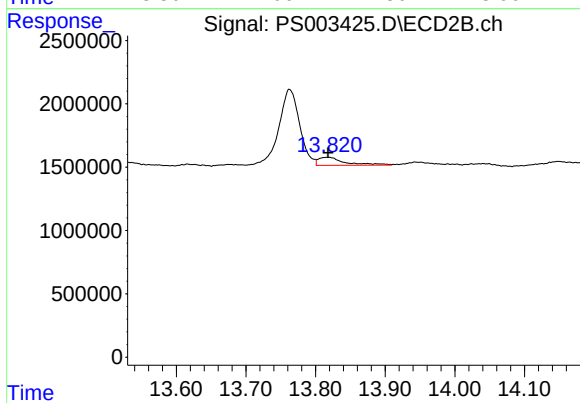

#11 2,4,5-TP (SILVEX)


R.T.: 13.817 min
Delta R.T.: 0.000 min
Response: 1730030
Conc: 0.68 ng/ml

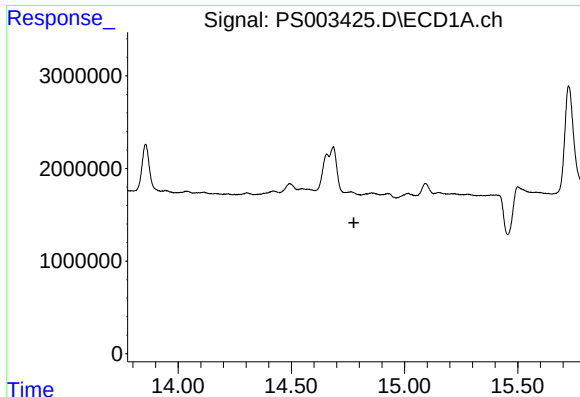

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.776 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
JC-03-030119-E

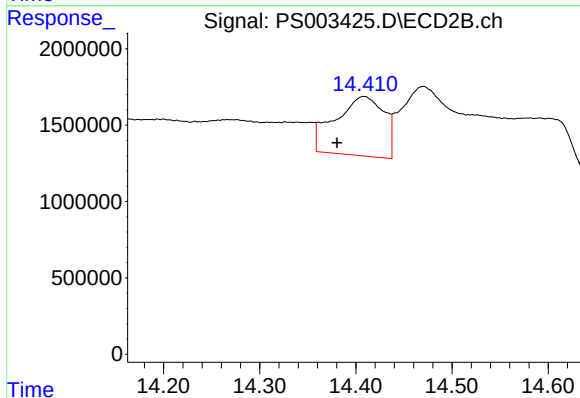


#12 2,4,5-T

R.T.: 14.408 min
Delta R.T.: 0.028 min
Response: 13734197
Conc: 6.81 ng/ml

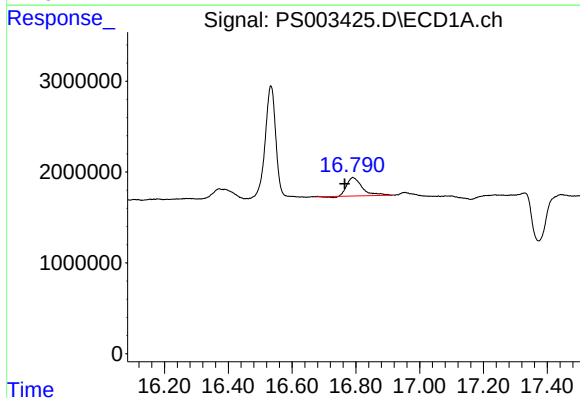


#15 Picloram

R.T.: 16.791 min
Delta R.T.: 0.026 min
Response: 6755025
Conc: 2.74 ng/ml

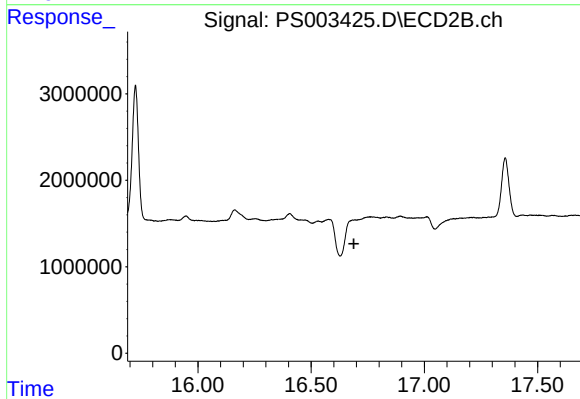

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.688 min
Response: 0
Conc: N.D.

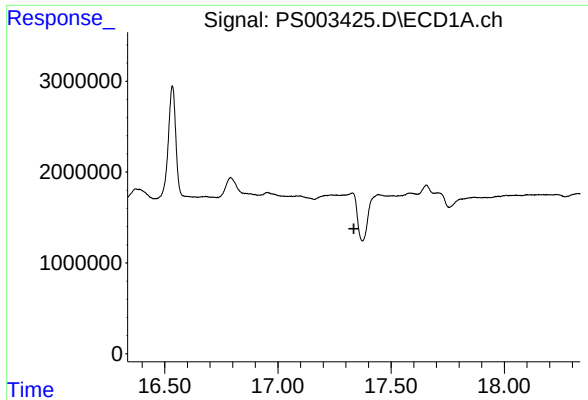

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
JC-03-030119-E

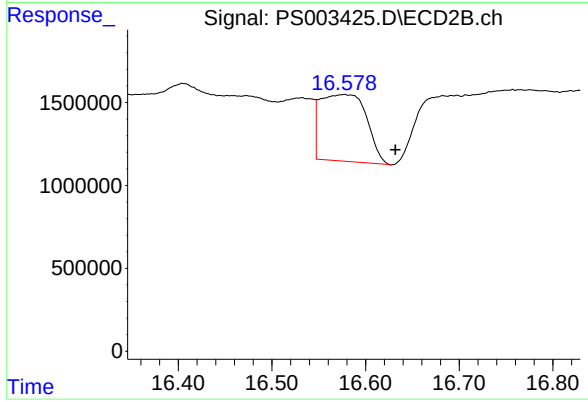

#16 DCPA

R.T.: 16.577 min
Delta R.T.: -0.055 min
Response: 13759160
Conc: 4.42 ng/ml