

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030420\
 Data File : PS009083.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2020 08:43
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 14:09:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	6.938	939.5E6	478.3E6	429.660	496.428
Target Compounds							
12) T	2,4,5-T	9.512	0.000	11584198	0	1.083	N.D. #
15) T	Picloram	11.046	0.000	23519197	0	1.718	N.D. #
16) T	DCPA	11.496	0.000	7806097	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030420\
Data File : PS009083.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2020 08:43
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 14:09:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

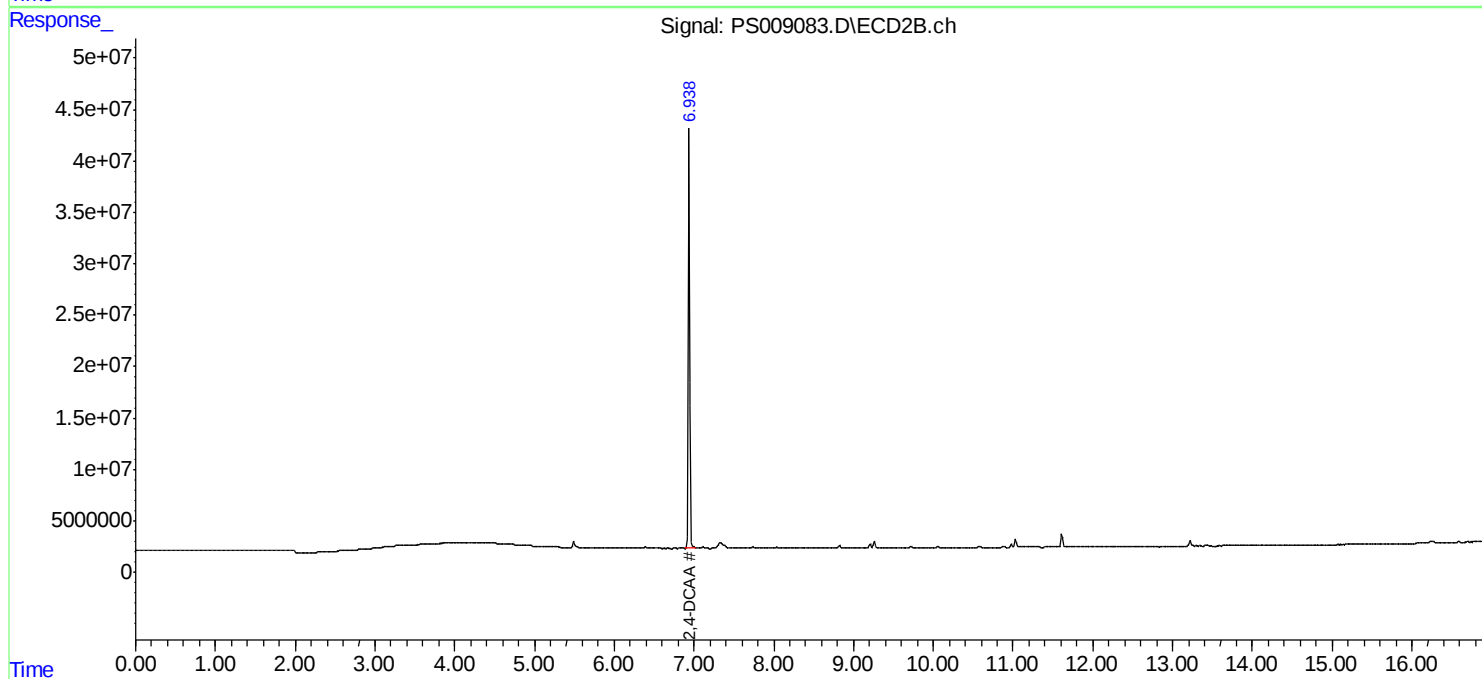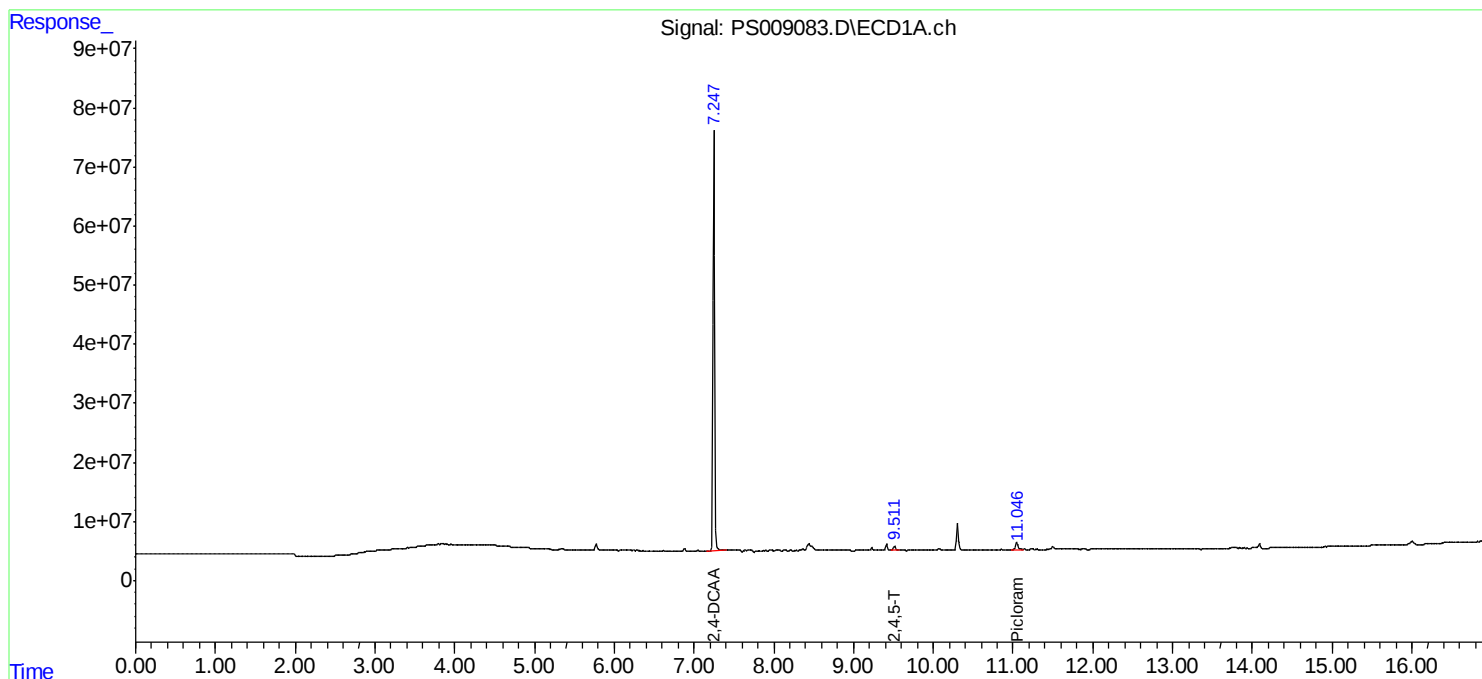


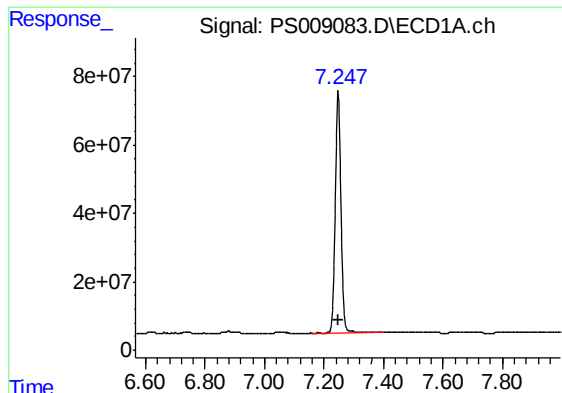

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: 0.000 min
Response: 939491010
Conc: 429.66 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

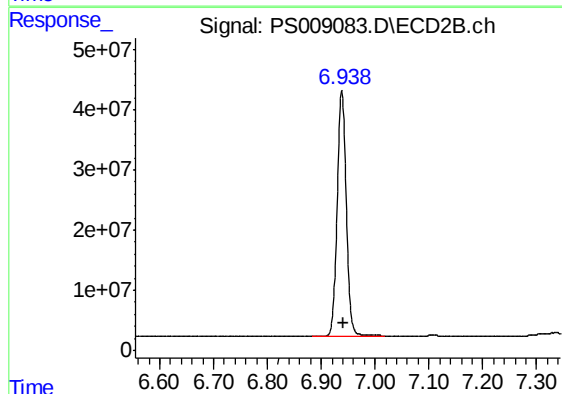


#4 2,4-DCAA

R.T.: 6.938 min
Delta R.T.: -0.002 min
Response: 478336161
Conc: 496.43 ng/ml

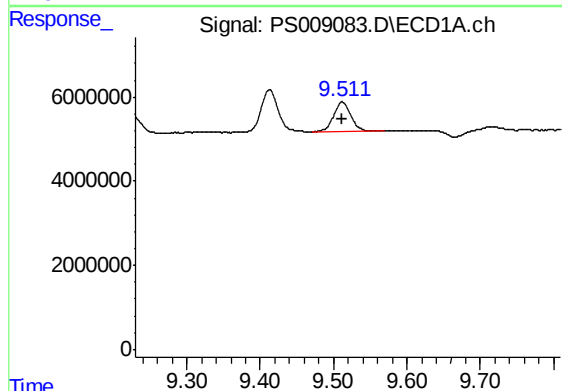


#12 2,4,5-T

R.T.: 9.512 min
Delta R.T.: 0.000 min
Response: 11584198
Conc: 1.08 ng/ml

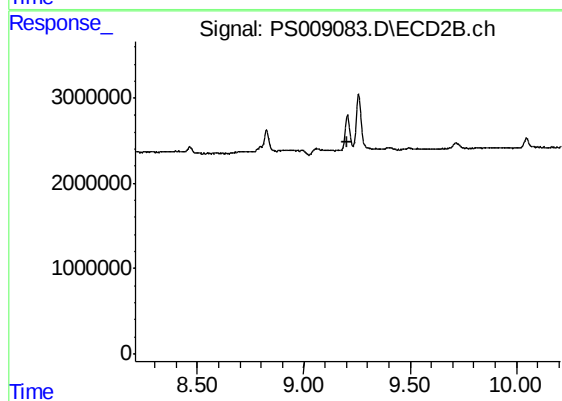

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.208 min
Response: 0
Conc: N.D.

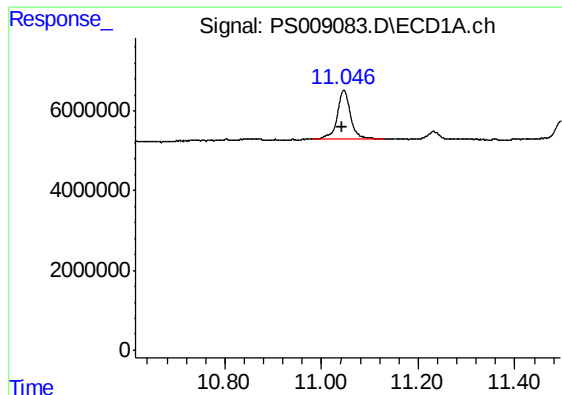

#15 Picloram

R.T.: 11.046 min
Delta R.T.: 0.003 min
Response: 23519197
Conc: 1.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

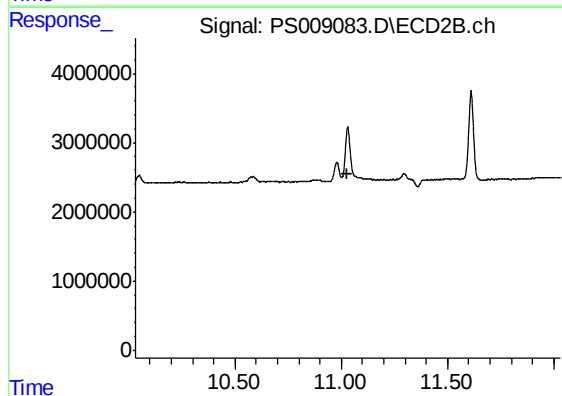

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.031 min
Response: 0
Conc: N.D.