

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030420\
 Data File : PS009107.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2020 18:48
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 01:14:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.246	6.938	917.7E6	501.1E6	419.678	520.006
Target Compounds							
11) T	2,4,5-TP ...	9.224	0.000	8646957	0	<MDL	N.D. #
12) T	2,4,5-T	9.509	9.259	18574965	17162546	1.737	3.171 #
15) T	Picloram	11.043	10.979	25948916	11798850	1.895	1.624
16) T	DCPA	11.493	10.979	22905908	11798850	1.667	1.705



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030420\
Data File : PS009107.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2020 18:48
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 01:14:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

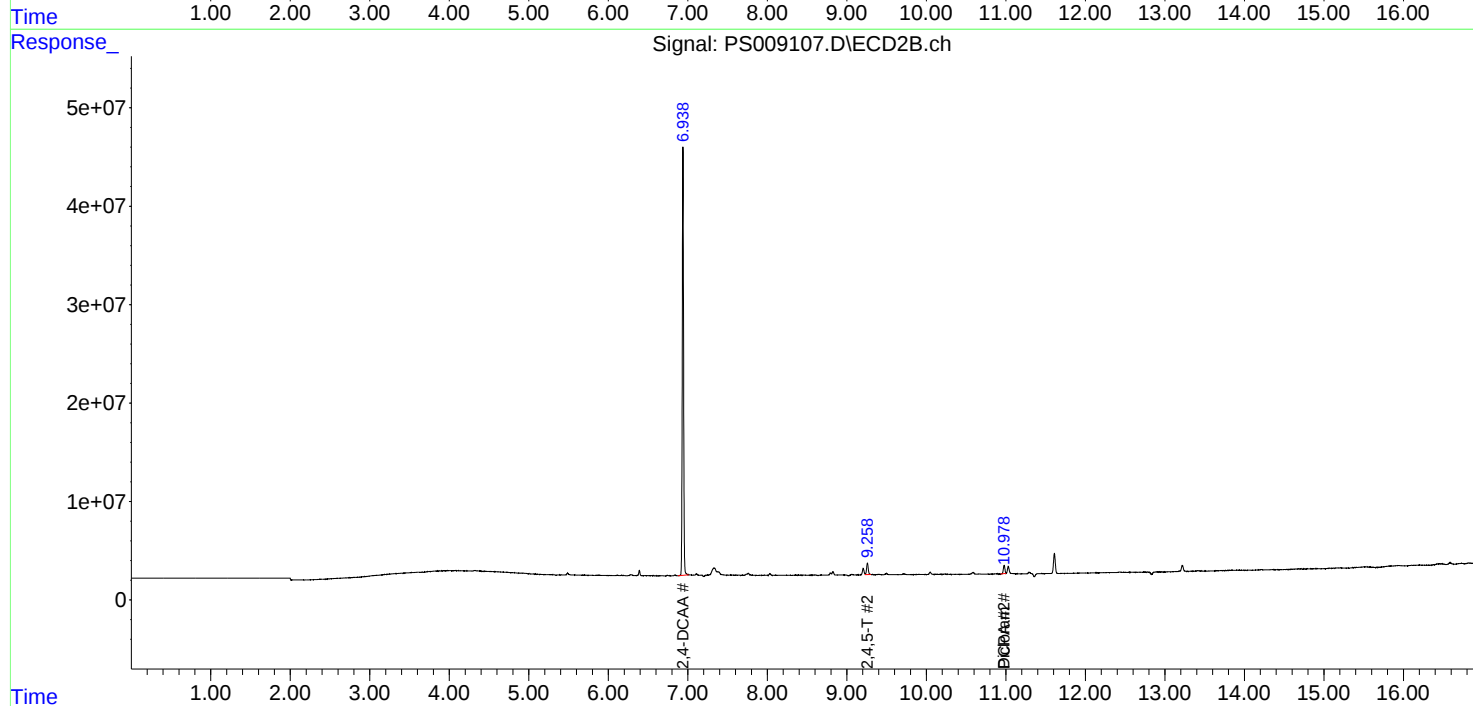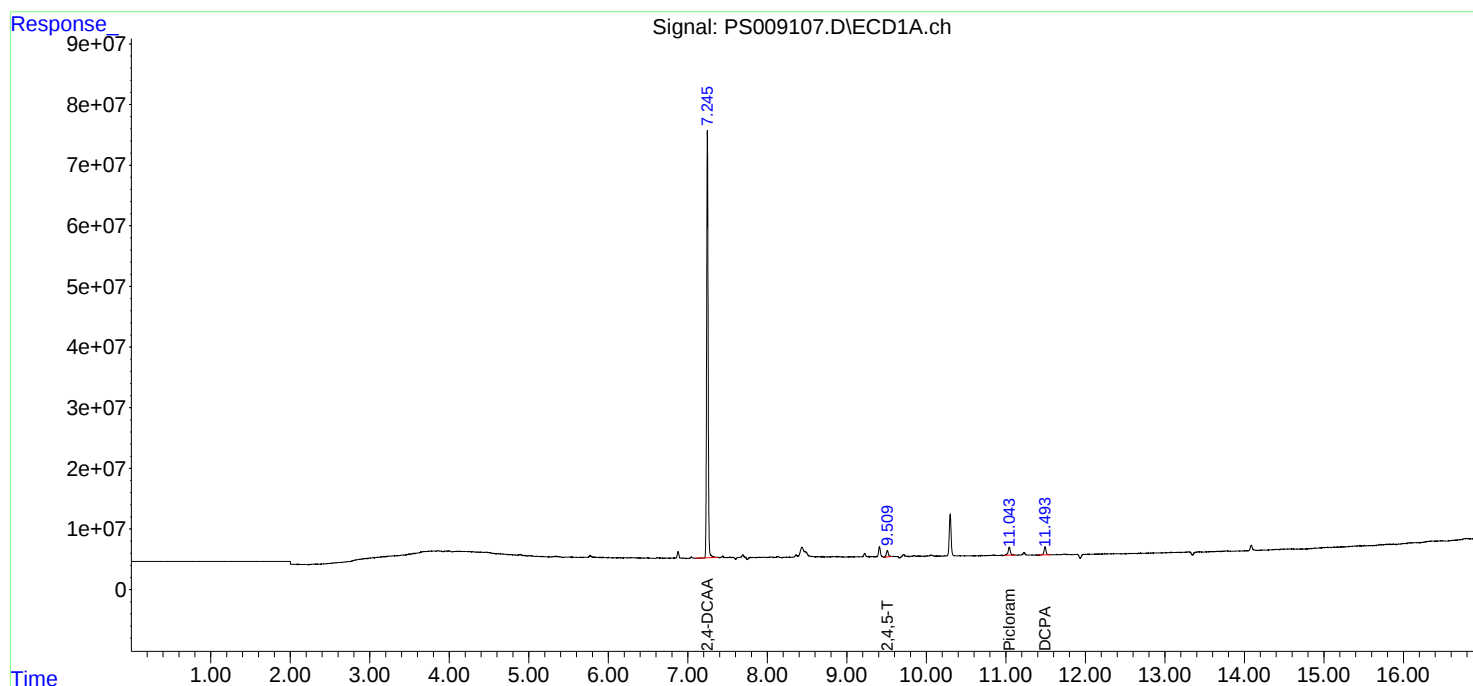


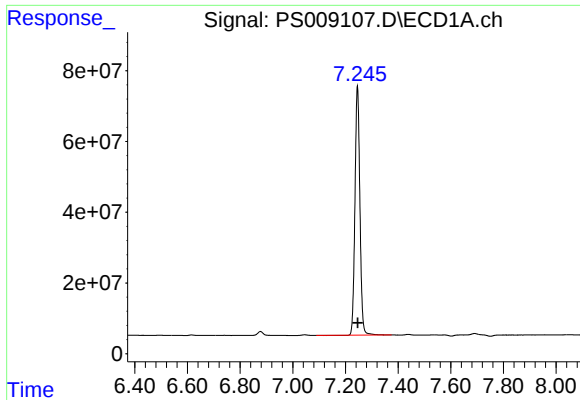

#4 2,4-DCAA


R.T.: 7.246 min
Delta R.T.: -0.001 min
Response: 917665641
Conc: 419.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

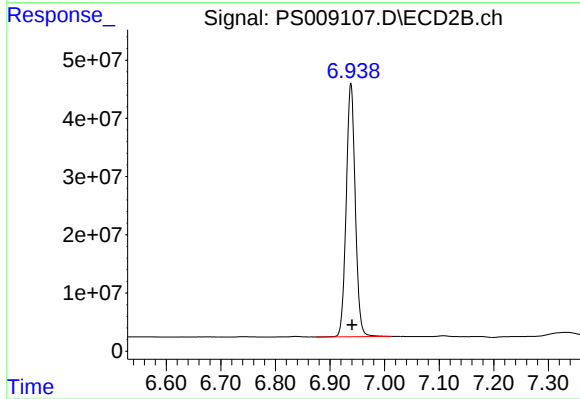


#4 2,4-DCAA

R.T.: 6.938 min
Delta R.T.: -0.002 min
Response: 501054952
Conc: 520.01 ng/ml

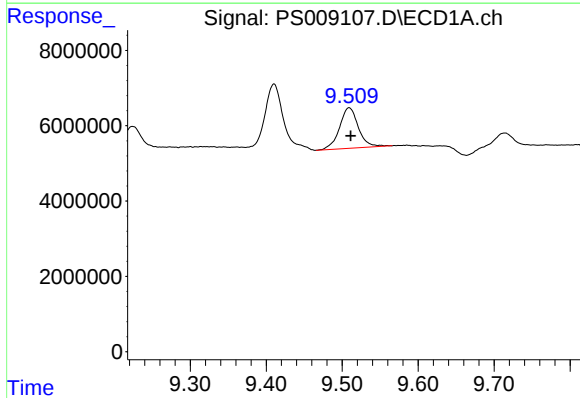


#12 2,4,5-T

R.T.: 9.509 min
Delta R.T.: -0.002 min
Response: 18574965
Conc: 1.74 ng/ml

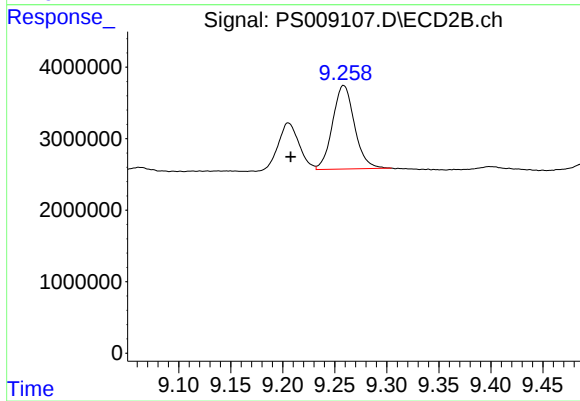

#12 2,4,5-T


R.T.: 9.259 min
Delta R.T.: 0.051 min
Response: 17162546
Conc: 3.17 ng/ml

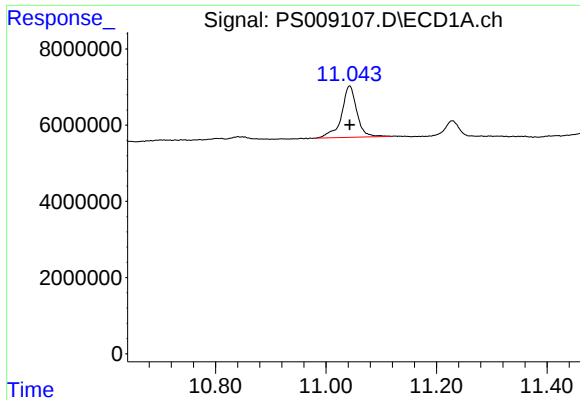

#15 Picloram


R.T.: 11.043 min
Delta R.T.: 0.000 min
Response: 25948916
Conc: 1.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

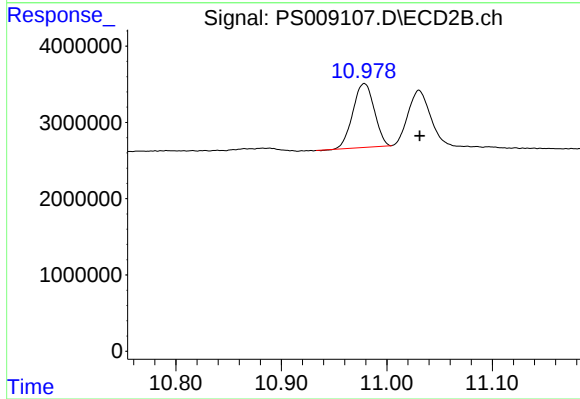


#15 Picloram

R.T.: 10.979 min
Delta R.T.: -0.052 min
Response: 11798850
Conc: 1.62 ng/ml

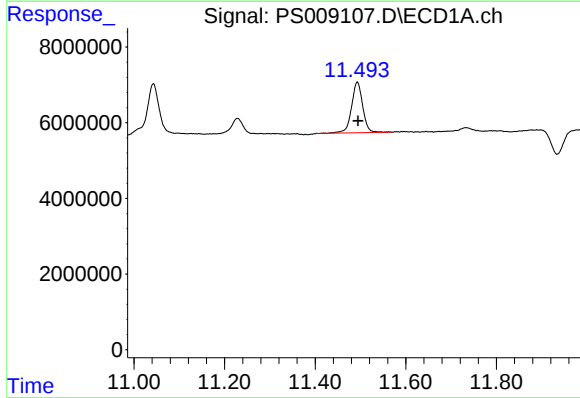

#16 DCPA

R.T.: 11.493 min
Delta R.T.: -0.002 min
Response: 22905908
Conc: 1.67 ng/ml

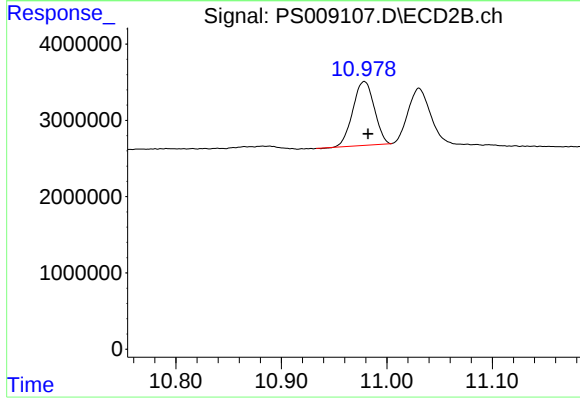

#16 DCPA

R.T.: 10.979 min
Delta R.T.: -0.004 min
Response: 11798850
Conc: 1.71 ng/ml