

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030420\
 Data File : PS009119.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2020 23:46
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 01:16:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.245	6.938	927.6E6	502.5E6	424.228	521.472
Target Compounds							
9) T	2,4-D	8.362	0.000	7118241	0	3.435	N.D. #
11) T	2,4,5-TP ...	9.225	0.000	10042036	0	<MDL	N.D. #
12) T	2,4,5-T	9.509	9.205	24311748	12129905	2.274	2.241
15) T	Picloram	11.043	11.030	45438873	23693597	3.319	3.261
16) T	DCPA	11.493	11.030	14693452	23693597	1.069	3.424 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030420\
Data File : PS009119.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2020 23:46
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 01:16:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

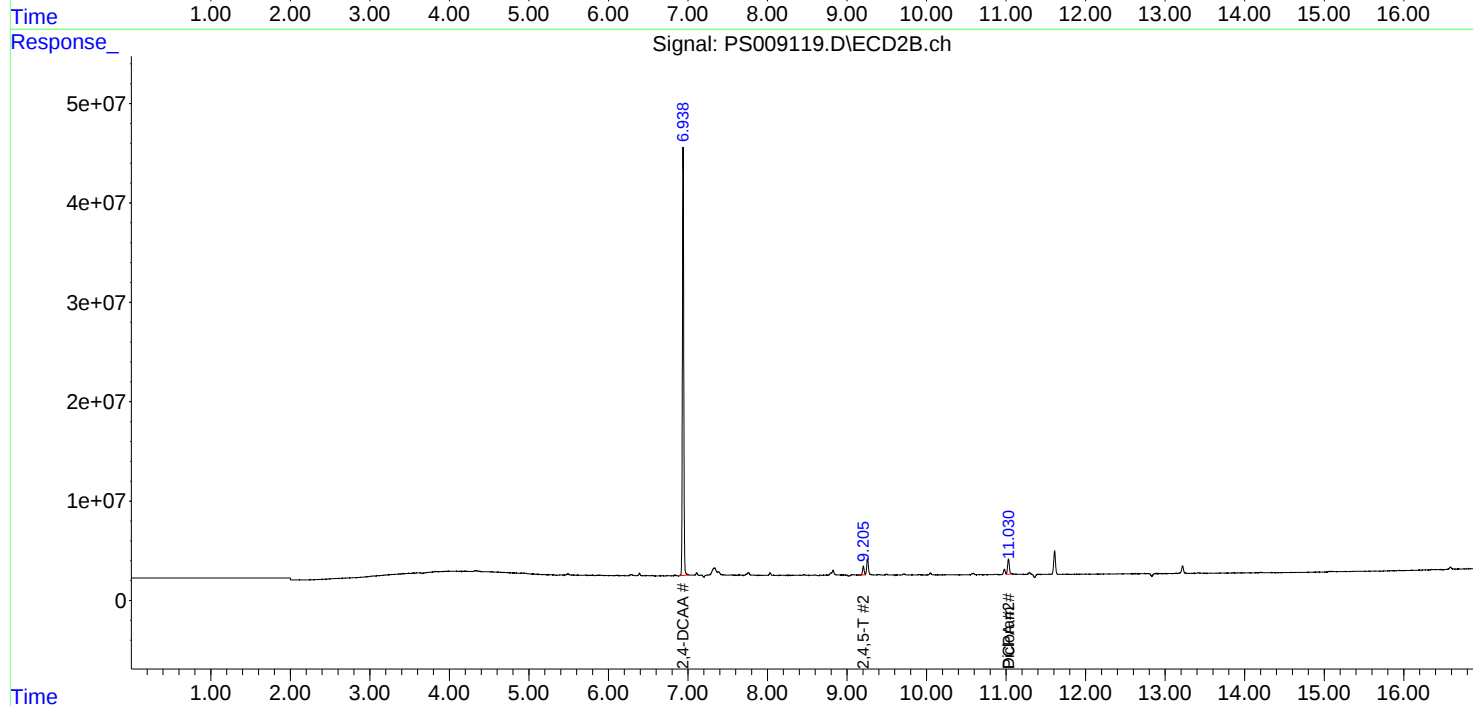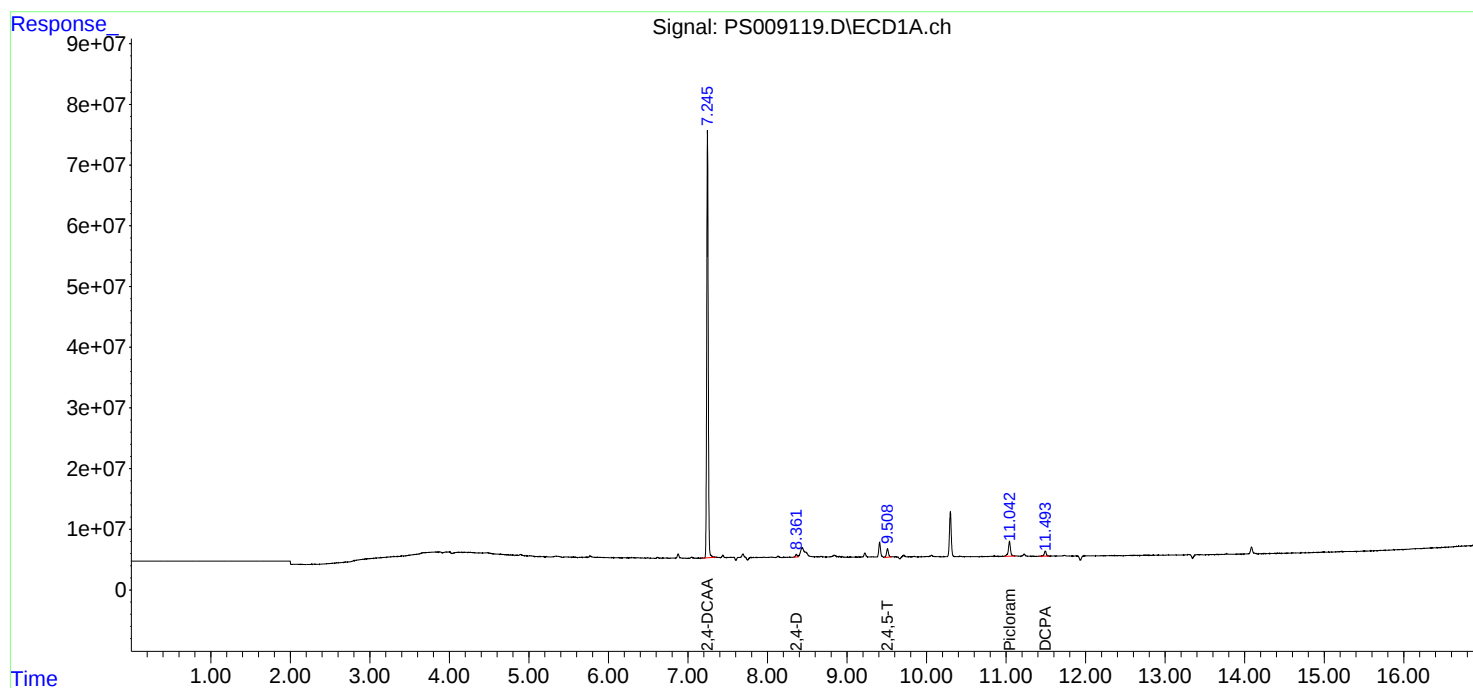


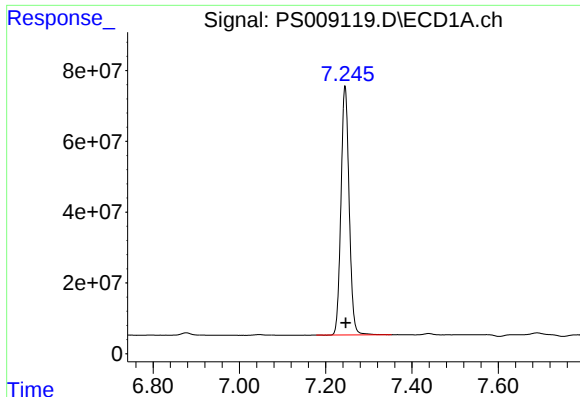

#4 2,4-DCAA


R.T.: 7.245 min
Delta R.T.: -0.002 min
Response: 927613908
Conc: 424.23 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

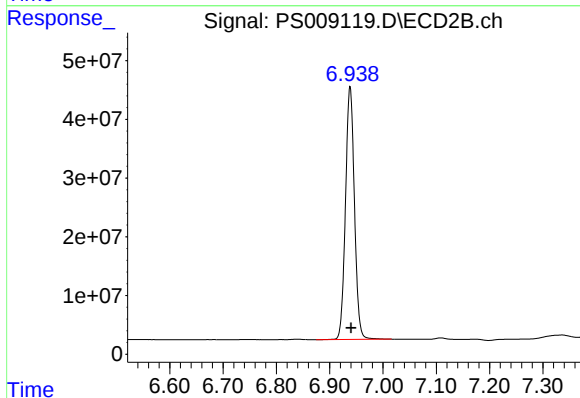


#4 2,4-DCAA

R.T.: 6.938 min
Delta R.T.: -0.002 min
Response: 502467362
Conc: 521.47 ng/ml

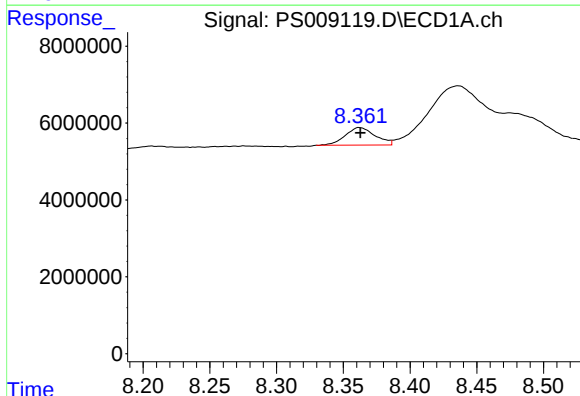


#9 2,4-D

R.T.: 8.362 min
Delta R.T.: 0.000 min
Response: 7118241
Conc: 3.43 ng/ml

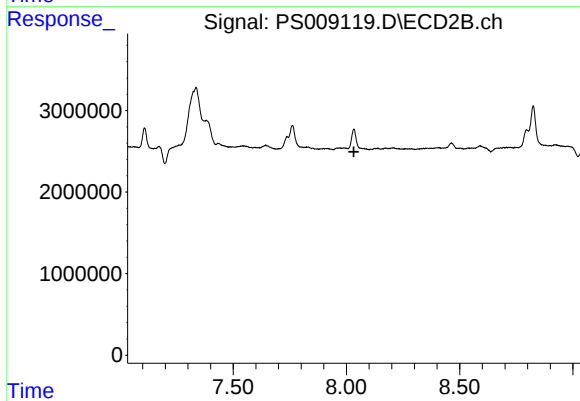

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.033 min
Response: 0
Conc: N.D.

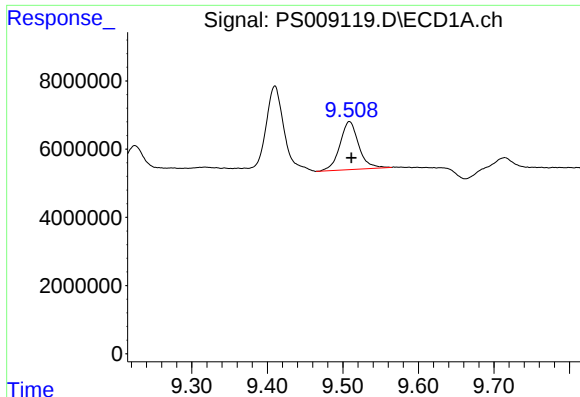

#12 2,4,5-T


R.T.: 9.509 min
Delta R.T.: -0.002 min
Response: 24311748
Conc: 2.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

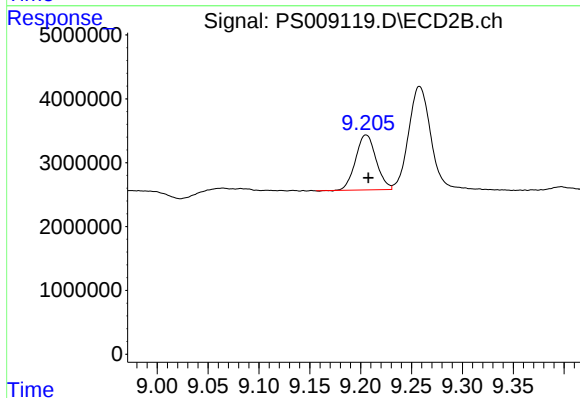


#12 2,4,5-T

R.T.: 9.205 min
Delta R.T.: -0.002 min
Response: 12129905
Conc: 2.24 ng/ml

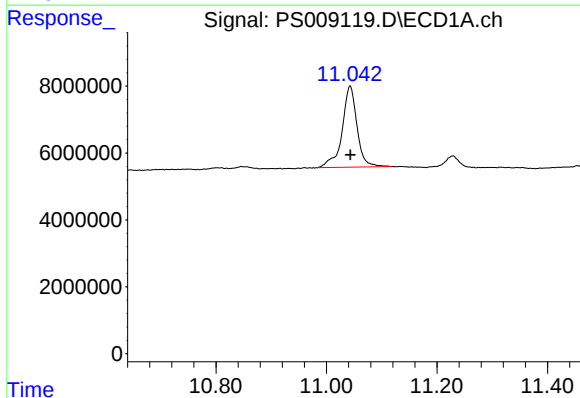


#15 Picloram

R.T.: 11.043 min
Delta R.T.: 0.000 min
Response: 45438873
Conc: 3.32 ng/ml

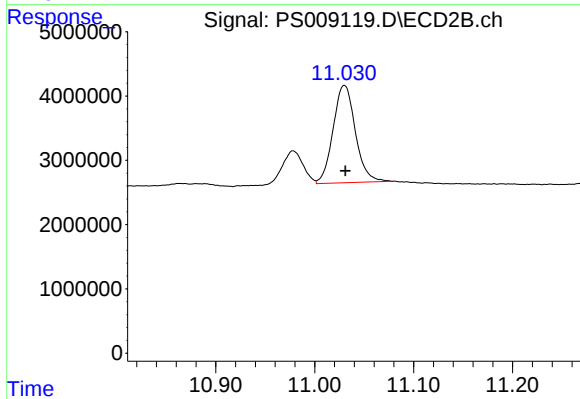

#15 Picloram


R.T.: 11.030 min
Delta R.T.: -0.001 min
Response: 23693597
Conc: 3.26 ng/ml

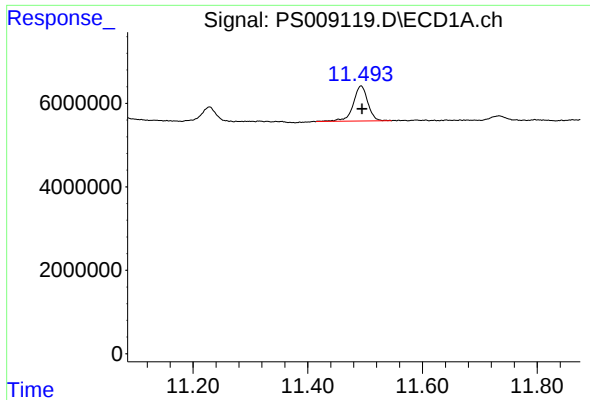

#16 DCPA

R.T.: 11.493 min
Delta R.T.: -0.002 min
Response: 14693452
Conc: 1.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

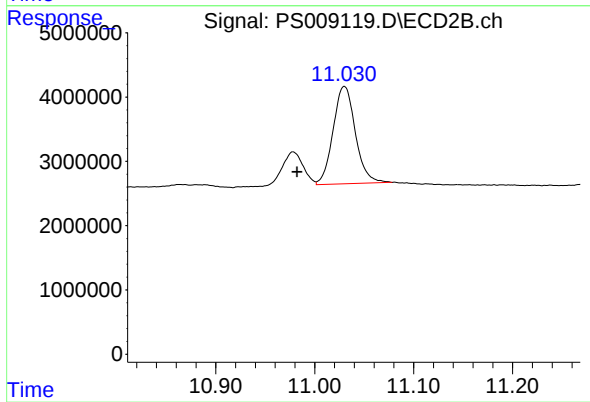

#16 DCPA

R.T.: 11.030 min
Delta R.T.: 0.048 min
Response: 23693597
Conc: 3.42 ng/ml