

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030420\
 Data File : PS009126.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2020 02:49
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 04:07:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.245	6.938	919.5E6	499.5E6	420.513	518.368
Target Compounds							
11) T	2,4,5-TP ...	9.223	0.000	7108802	0	<MDL	N.D. #
12) T	2,4,5-T	9.508	9.258	16558027	15016242	1.549	2.774 #
15) T	Picloram	11.042	11.029	31843705	15030148	2.326	2.068
16) T	DCPA	11.492	11.029	9641501	15030148	<MDL	2.172 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030420\
Data File : PS009126.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2020 02:49
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 04:07:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

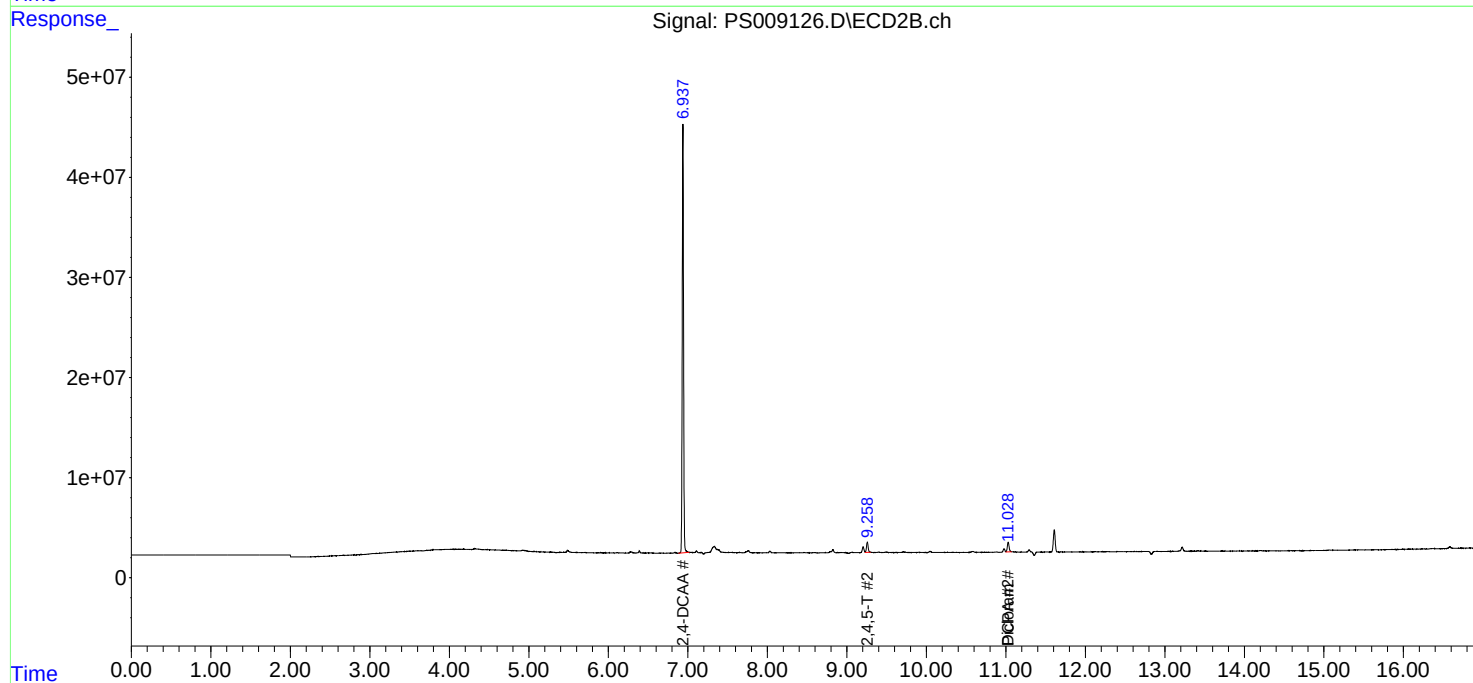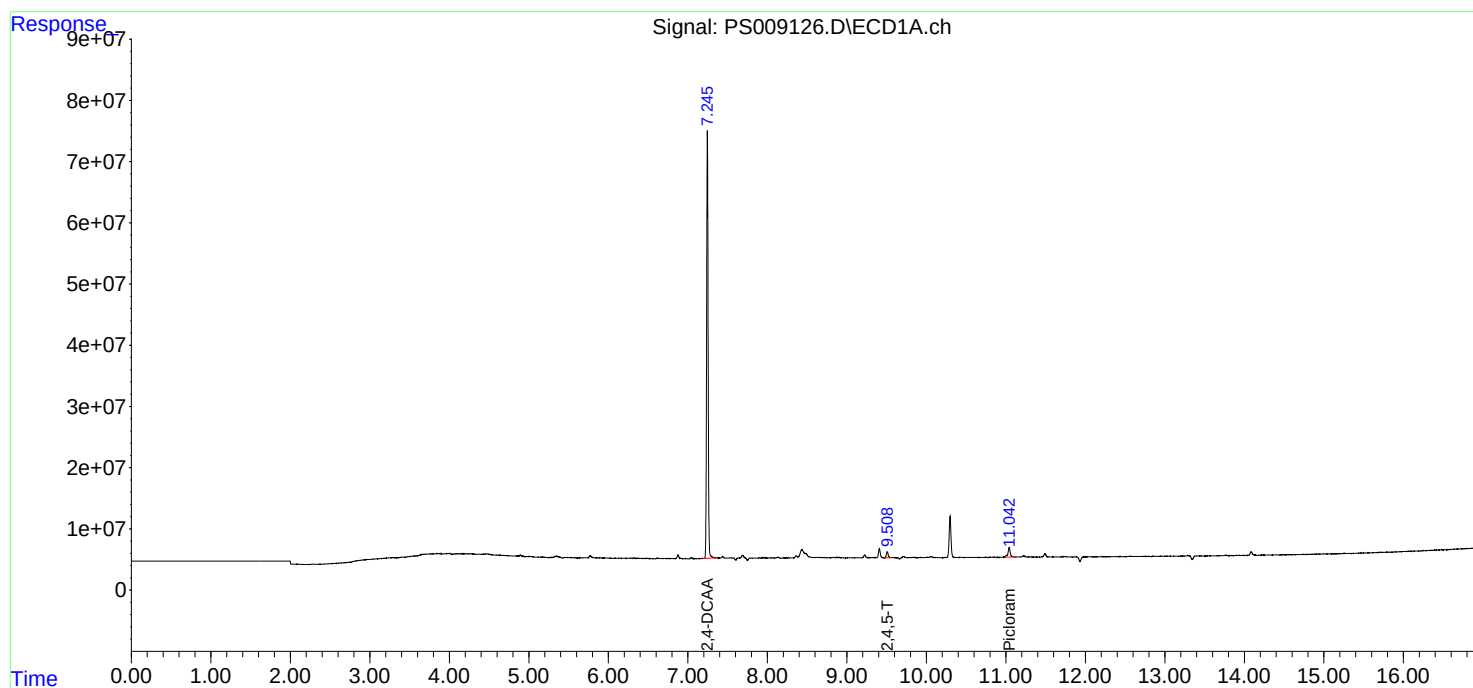


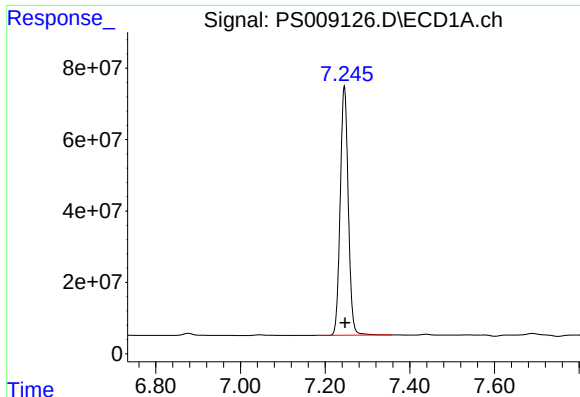

#4 2,4-DCAA


R.T.: 7.245 min
Delta R.T.: -0.002 min
Response: 919490613
Conc: 420.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

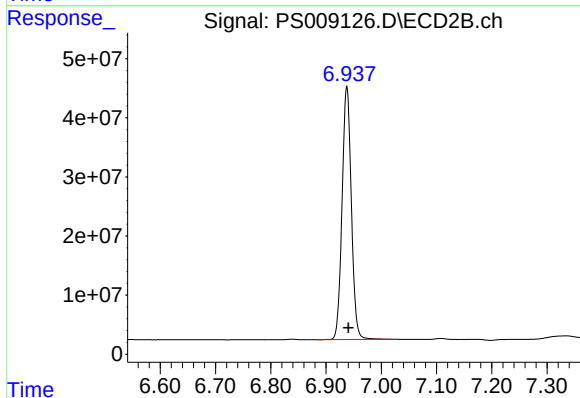


#4 2,4-DCAA

R.T.: 6.938 min
Delta R.T.: -0.003 min
Response: 499476442
Conc: 518.37 ng/ml

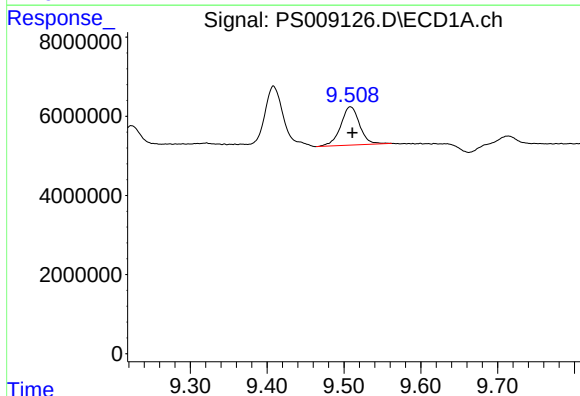


#12 2,4,5-T

R.T.: 9.508 min
Delta R.T.: -0.003 min
Response: 16558027
Conc: 1.55 ng/ml

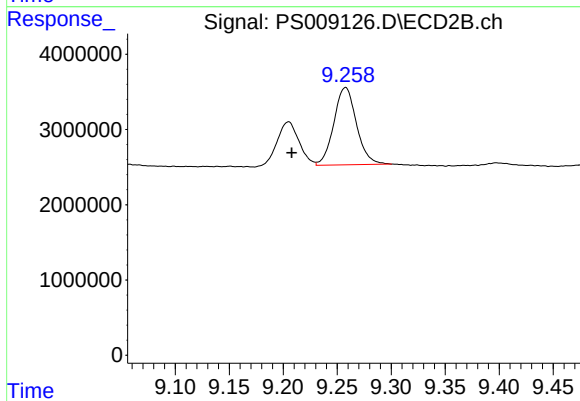

#12 2,4,5-T


R.T.: 9.258 min
Delta R.T.: 0.050 min
Response: 15016242
Conc: 2.77 ng/ml

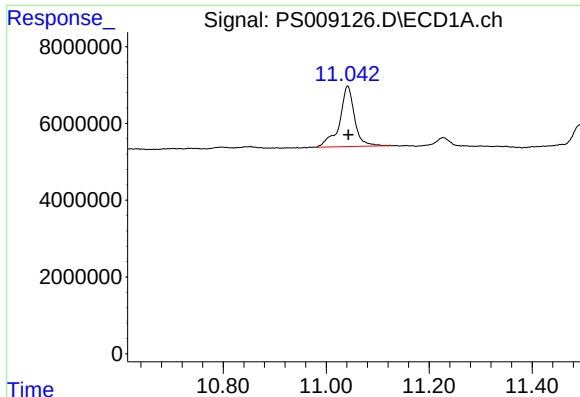

#15 Picloram


R.T.: 11.042 min
Delta R.T.: -0.002 min
Response: 31843705
Conc: 2.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

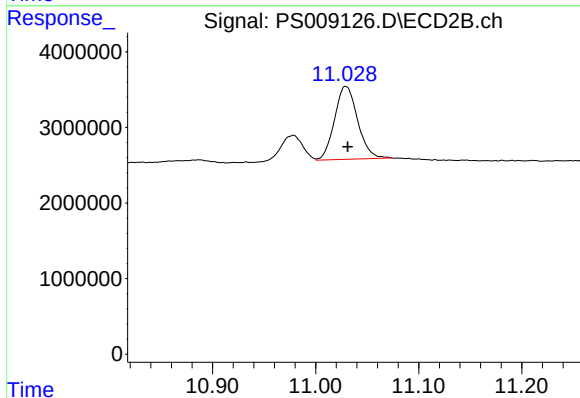


#15 Picloram

R.T.: 11.029 min
Delta R.T.: -0.002 min
Response: 15030148
Conc: 2.07 ng/ml

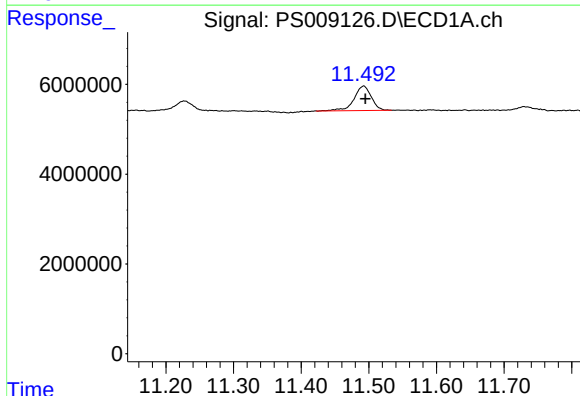

#16 DCPA

R.T.: 11.492 min
Delta R.T.: -0.002 min
Response: 9641501
Conc: N.D.

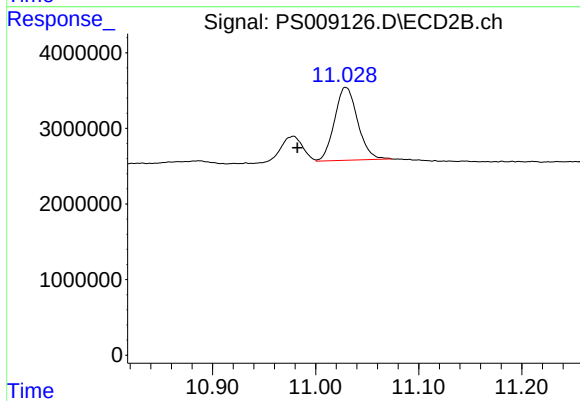

#16 DCPA

R.T.: 11.029 min
Delta R.T.: 0.047 min
Response: 15030148
Conc: 2.17 ng/ml