

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030421\
 Data File : PS014123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2021 10:11
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 14:50:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030421.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 04 14:50:18 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.462f	0.000	1018.8E6	0	735.336	N.D. #
5) T	DICAMBA	0.000	7.132f	0	454.3E6	N.D.	278.867
6) T	MCP	0.000	7.132	0	454.3E6	N.D.	340.862
15) T	Picloram	10.964	11.046f	78223409	5311400	9.264	1.546 #
16) T	DCPA	0.000	10.849f	0	4640228	N.D.	1.355



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030421\
Data File : PS014123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2021 10:11
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 14:50:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030421.M
Quant Title : 8080.M
QLast Update : Thu Mar 04 14:50:18 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

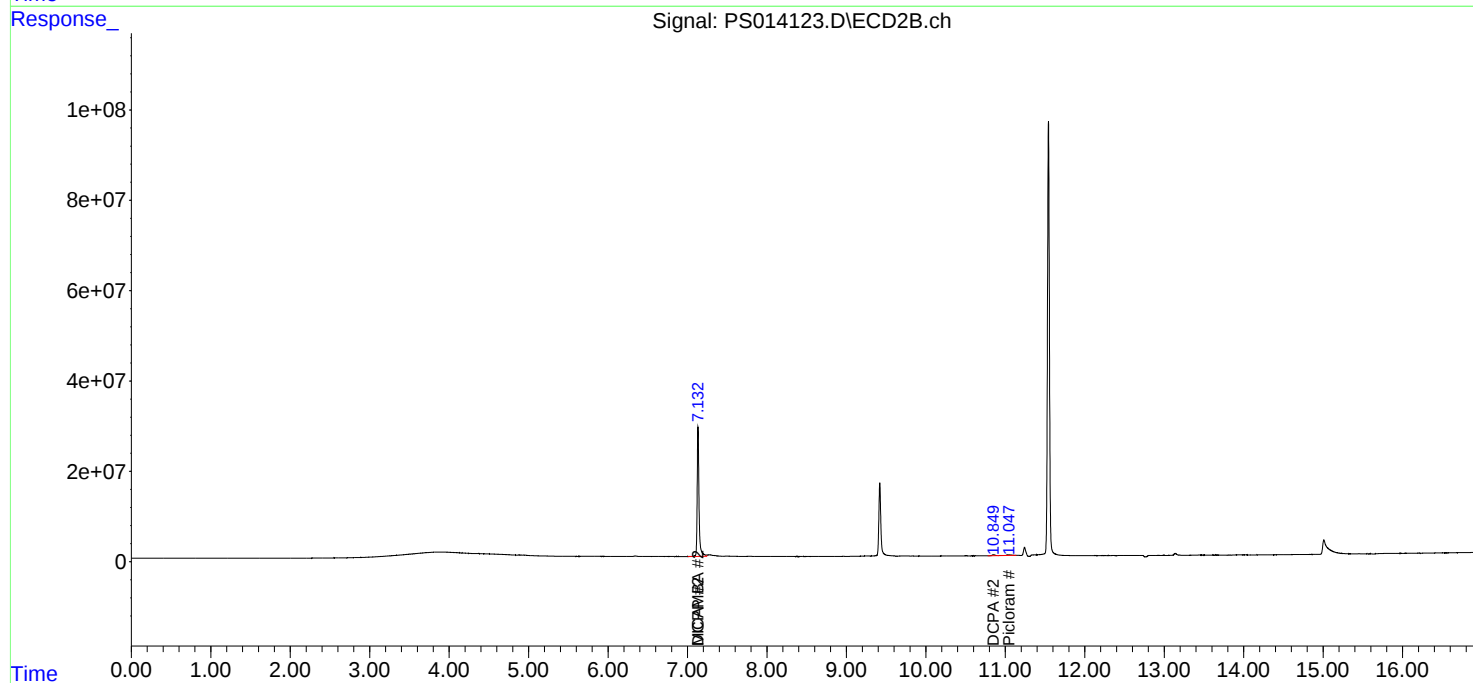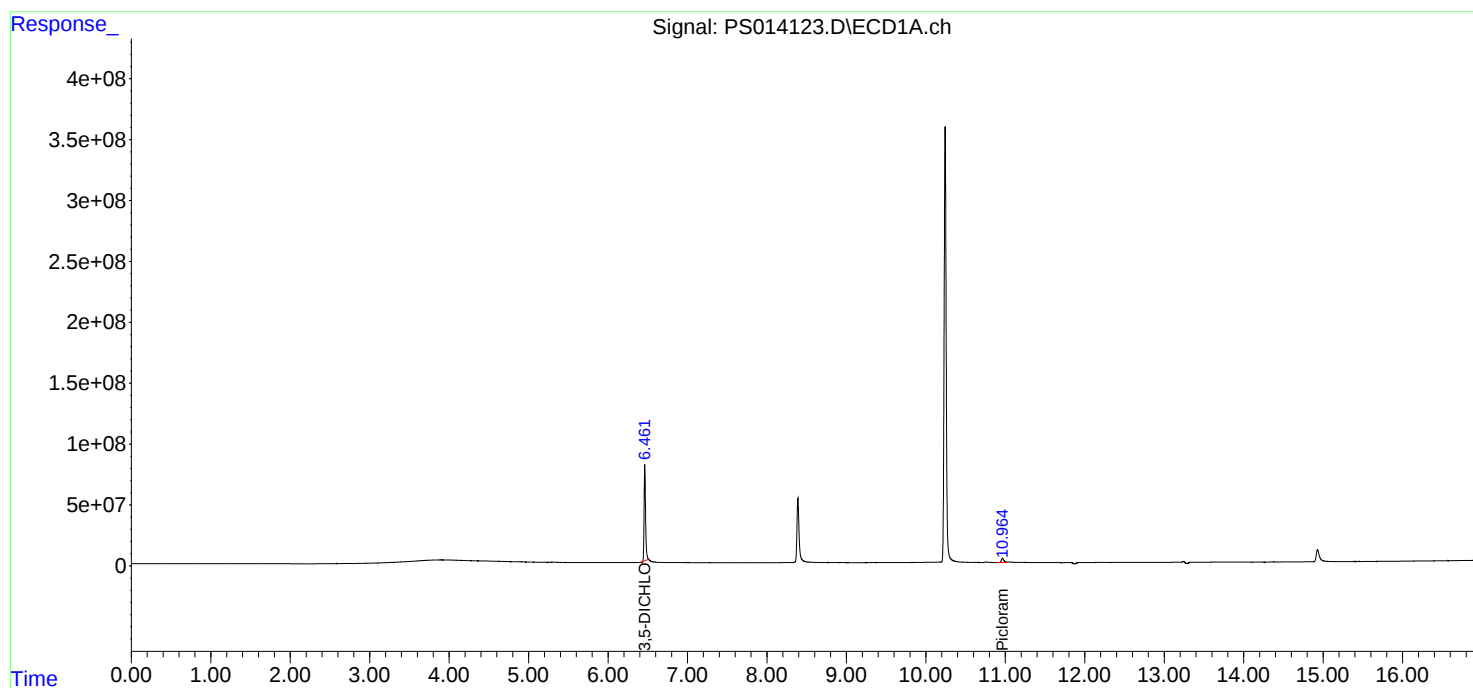


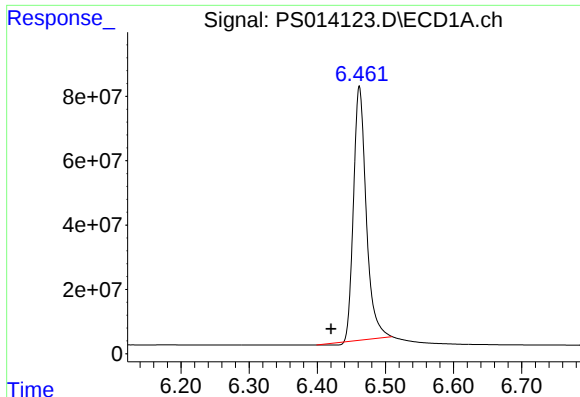

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.462 min
Delta R.T.: 0.042 min
Response: 1018791590
Conc: 735.34 ng/ml

Instrument :
ECD_S
ClientSampleId :

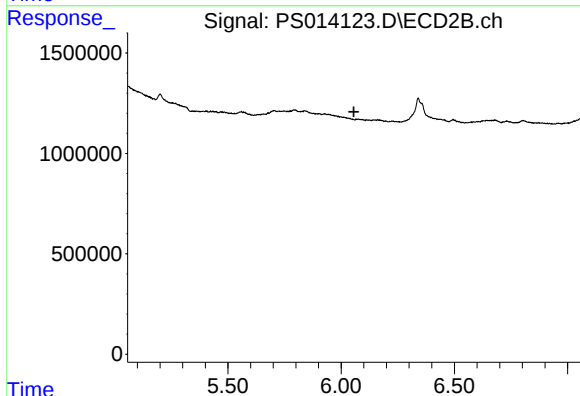


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.056 min
Response: 0
Conc: N.D.

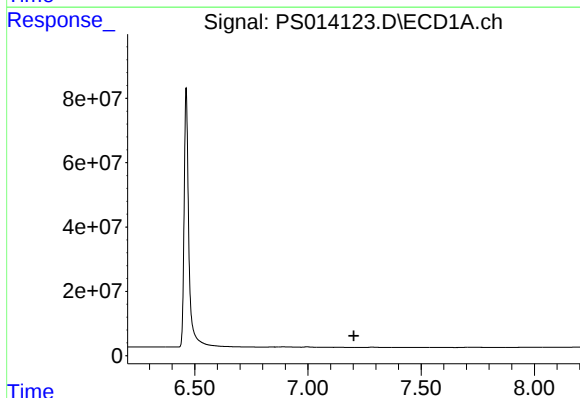


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.203 min
Response: 0
Conc: N.D.

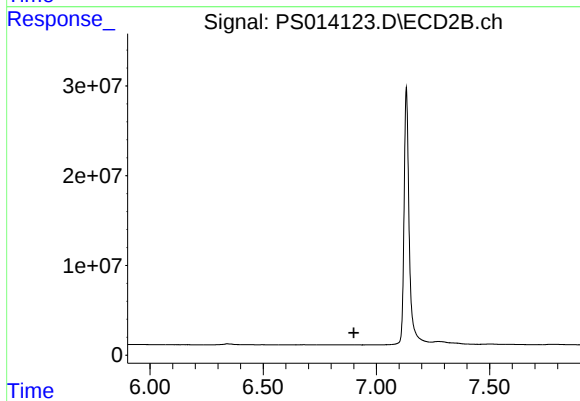

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.900 min
Response: 0
Conc: N.D.

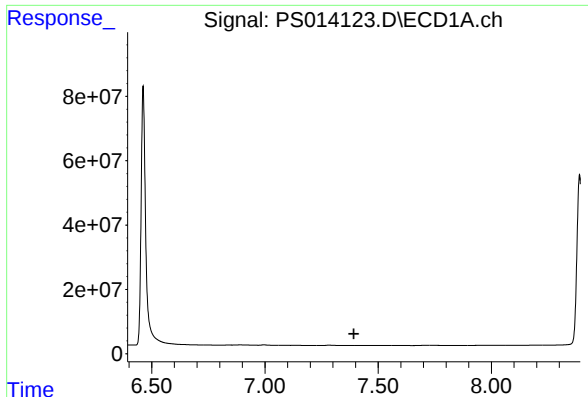

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.393 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

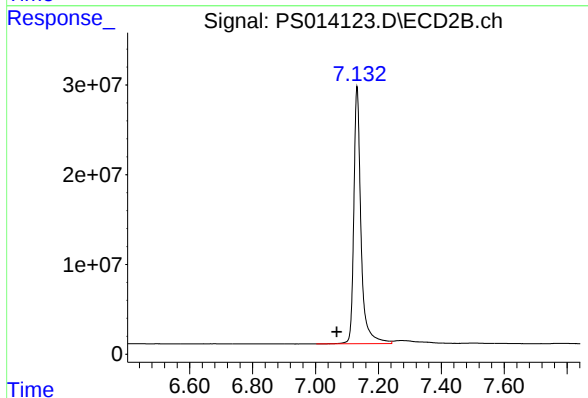


#5 DICAMBA

R.T.: 7.132 min
Delta R.T.: 0.065 min
Response: 454260939
Conc: 278.87 ng/ml

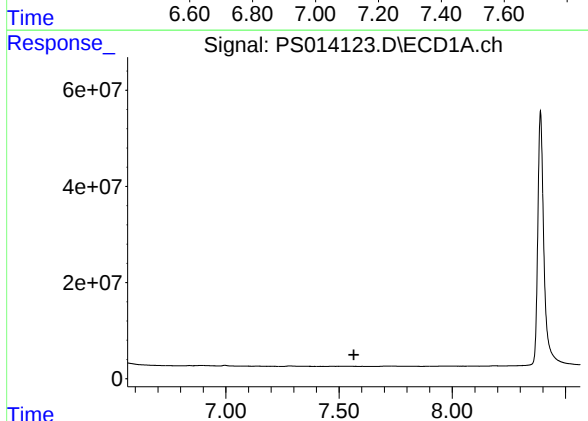


#6 MCP

R.T.: 0.000 min
Exp R.T.: 7.565 min
Response: 0
Conc: N.D.

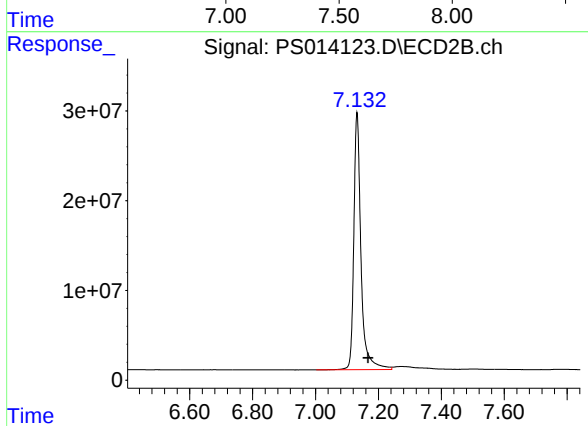

#6 MCP


R.T.: 7.132 min
Delta R.T.: -0.035 min
Response: 454260939
Conc: 340.86 ug/ml

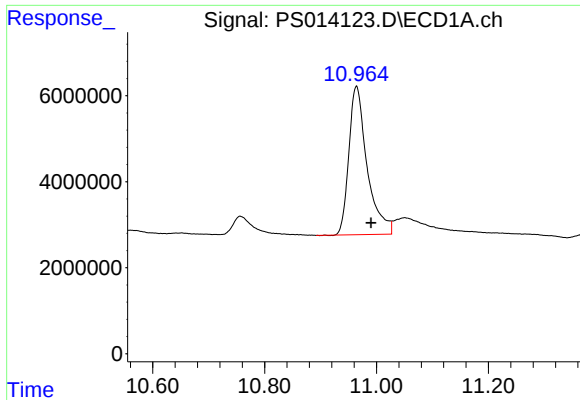

#15 Picloram


R.T.: 10.964 min
Delta R.T.: -0.026 min
Response: 78223409
Conc: 9.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

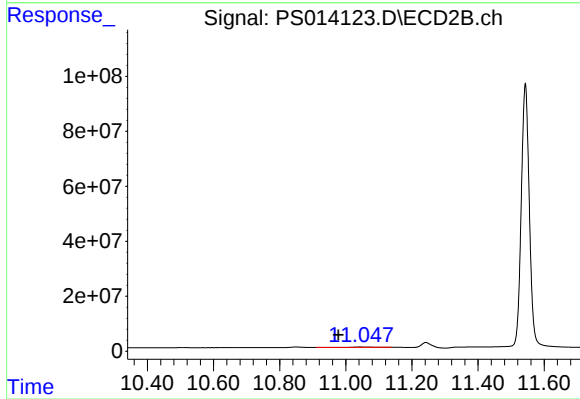


#15 Picloram

R.T.: 11.046 min
Delta R.T.: 0.069 min
Response: 5311400
Conc: 1.55 ng/ml

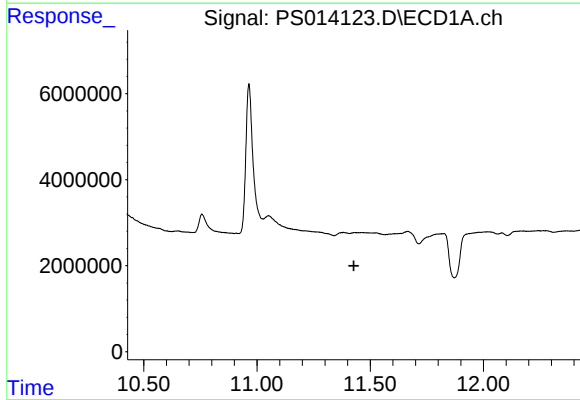

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.428 min
Response: 0
Conc: N.D.

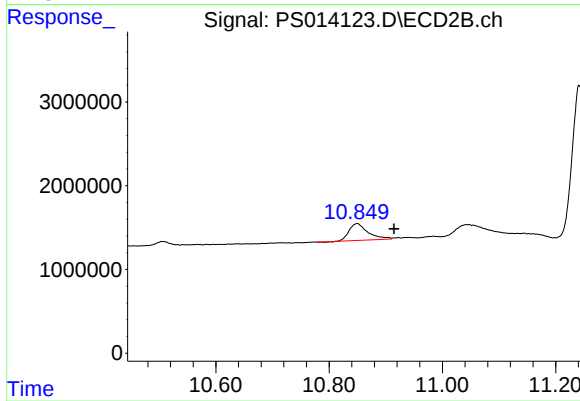

#16 DCPA

R.T.: 10.849 min
Delta R.T.: -0.066 min
Response: 4640228
Conc: 1.35 ng/ml