

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030421\
 Data File : PS014131.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2021 14:43
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 15:27:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030421.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 04 14:50:18 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.208	6.905	442.9E6	200.7E6	435.640	522.793
Target Compounds							
5) T	DICAMBA	7.396	7.071	4494330	6982431	1.118	4.286 #
10) T	Pentachlo...	8.629	8.421	11735188	5241380	<MDL	<MDL #
11) T	2,4,5-TP ...	9.187	8.793	6522654	3454895	1.123	1.529 #
12) T	2,4,5-T	9.433	9.212f	24561944	4103690	4.018	1.851 #
14) T	DINOSEB	11.167	10.002	21098427	2358151	4.471	1.461 #
15) T	Picloram	0.000	10.922f	0	5642809	N.D.	1.643
16) T	DCPA	11.433	10.922	12041641	5642809	1.394	1.648



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030421\
Data File : PS014131.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2021 14:43
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 15:27:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030421.M
Quant Title : 8080.M
QLast Update : Thu Mar 04 14:50:18 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

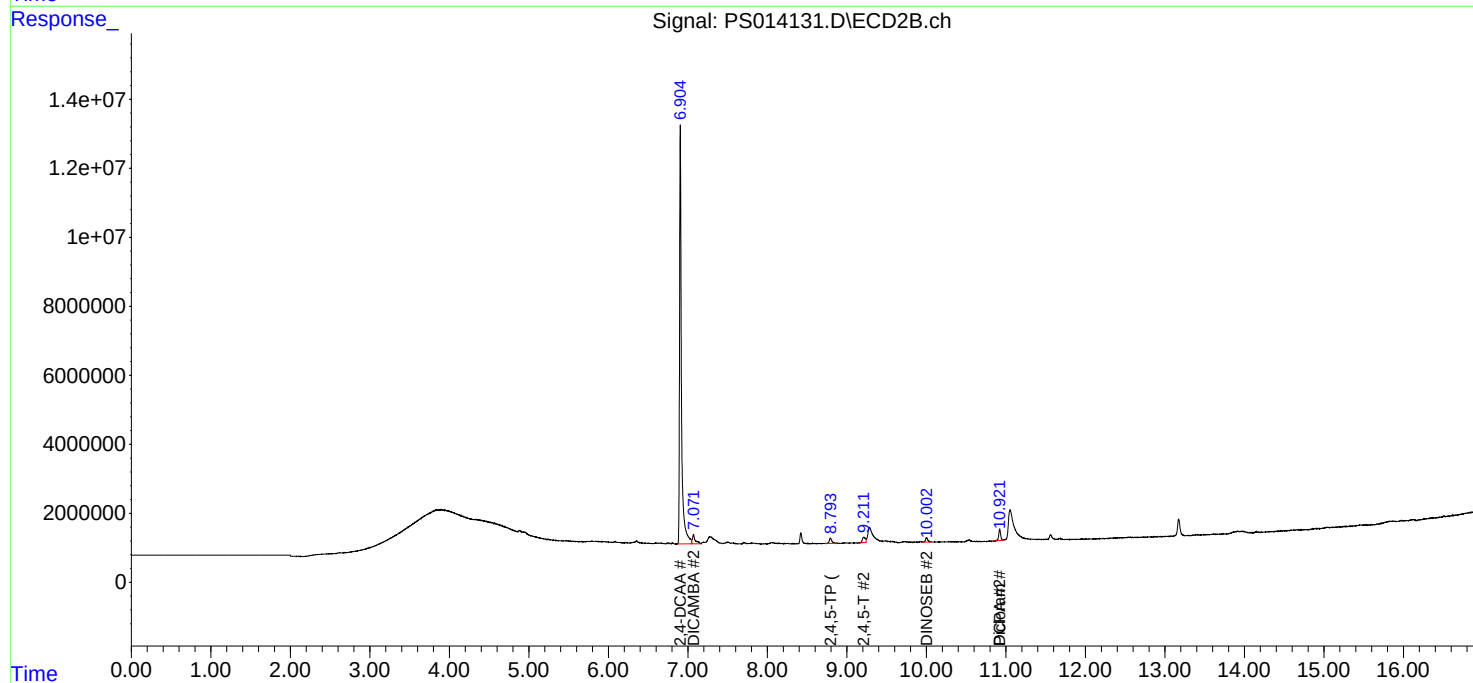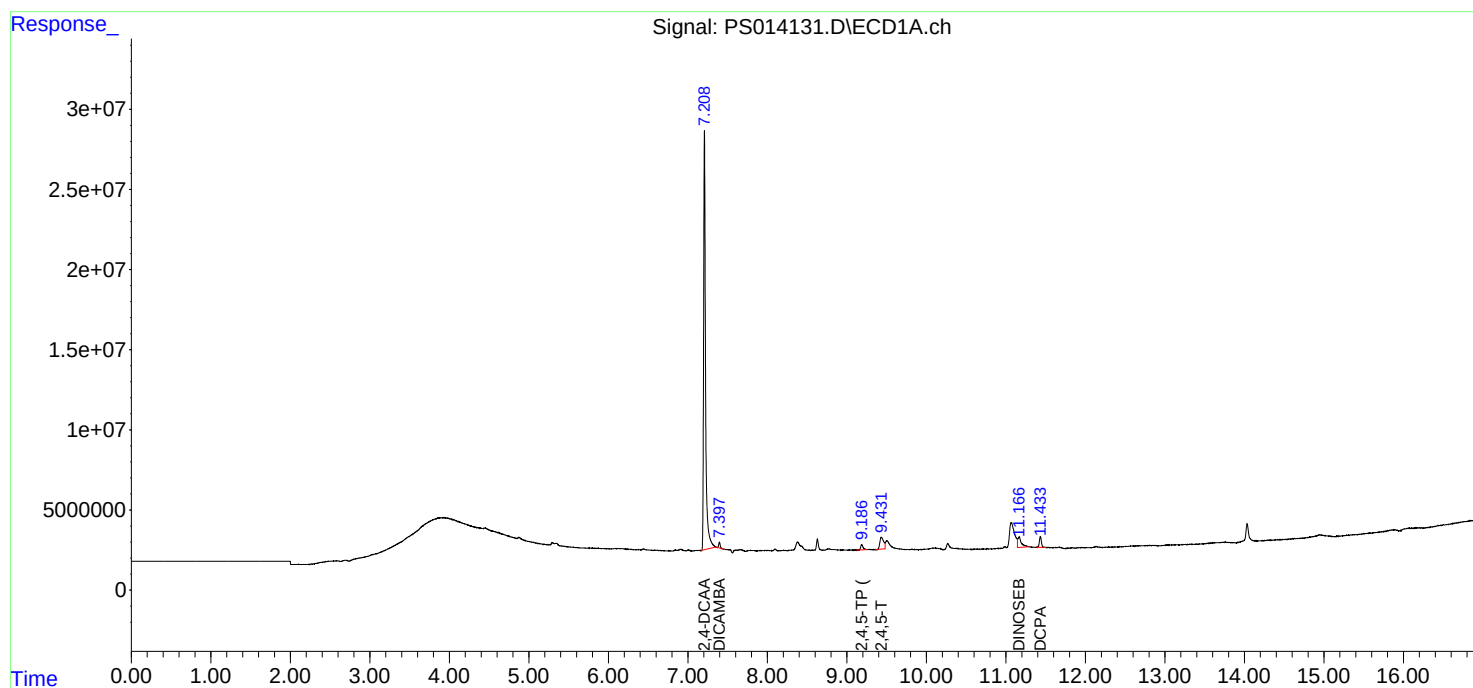


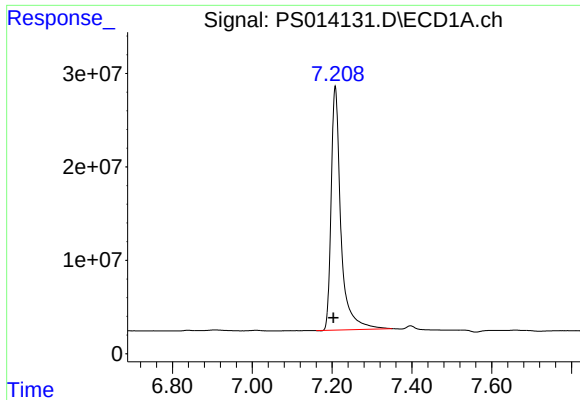

#4 2,4-DCAA


R.T.: 7.208 min
Delta R.T.: 0.005 min
Response: 442906822
Conc: 435.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

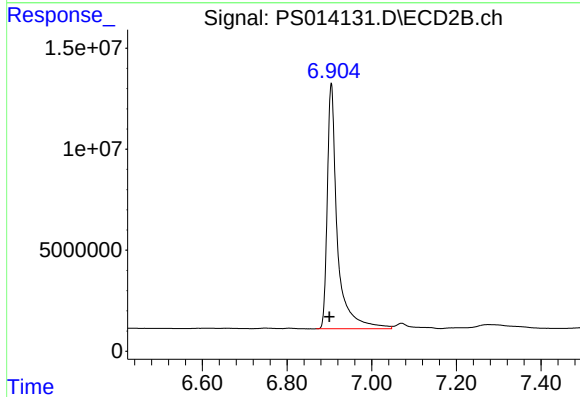


#4 2,4-DCAA

R.T.: 6.905 min
Delta R.T.: 0.004 min
Response: 200722928
Conc: 522.79 ng/ml

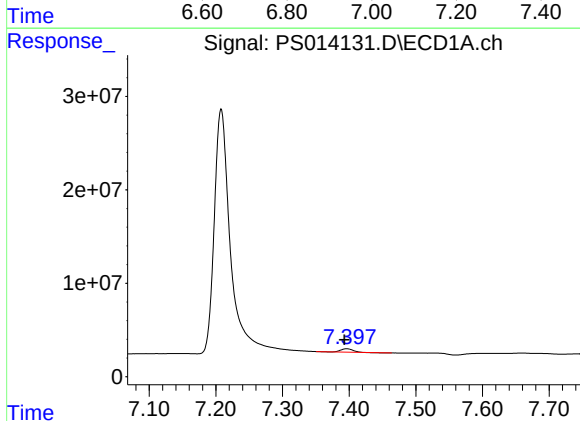


#5 DICAMBA

R.T.: 7.396 min
Delta R.T.: 0.003 min
Response: 4494330
Conc: 1.12 ng/ml

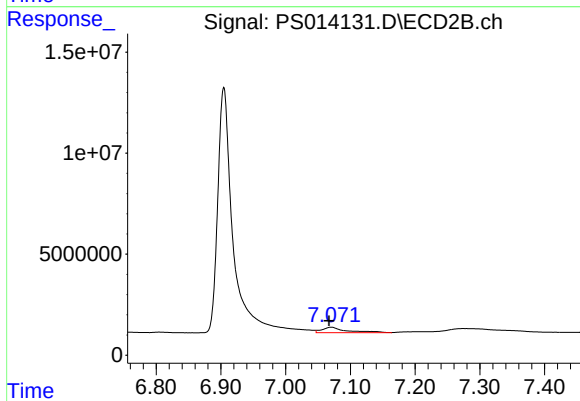

#5 DICAMBA


R.T.: 7.071 min
Delta R.T.: 0.003 min
Response: 6982431
Conc: 4.29 ng/ml

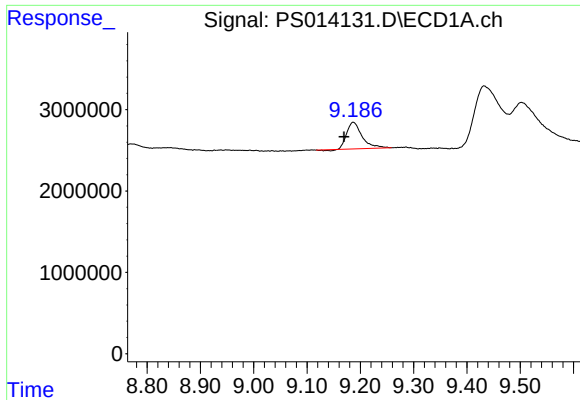

#11 2,4,5-TP (SILVEX)


R.T.: 9.187 min
Delta R.T.: 0.017 min
Response: 6522654
Conc: 1.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

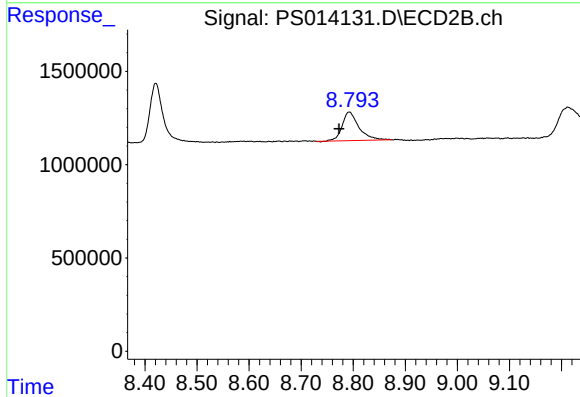


#11 2,4,5-TP (SILVEX)

R.T.: 8.793 min
Delta R.T.: 0.020 min
Response: 3454895
Conc: 1.53 ng/ml

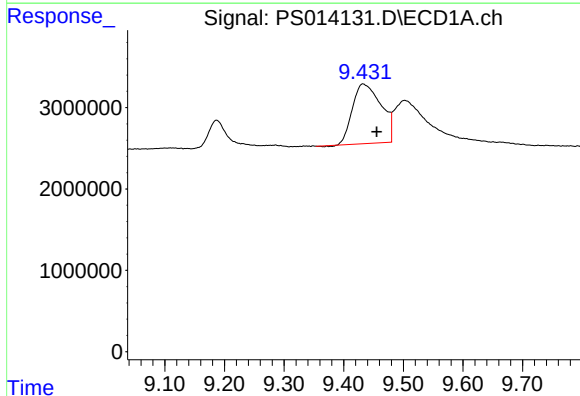


#12 2,4,5-T

R.T.: 9.433 min
Delta R.T.: -0.023 min
Response: 24561944
Conc: 4.02 ng/ml

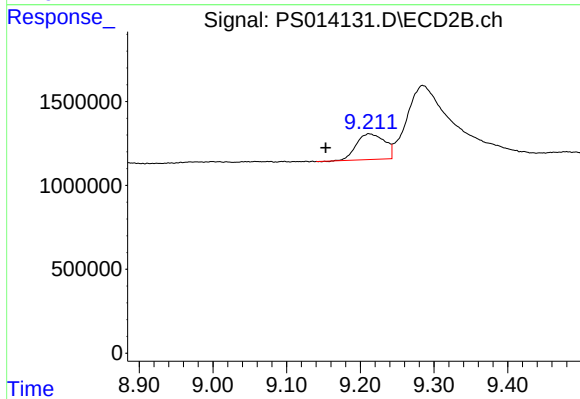

#12 2,4,5-T


R.T.: 9.212 min
Delta R.T.: 0.059 min
Response: 4103690
Conc: 1.85 ng/ml

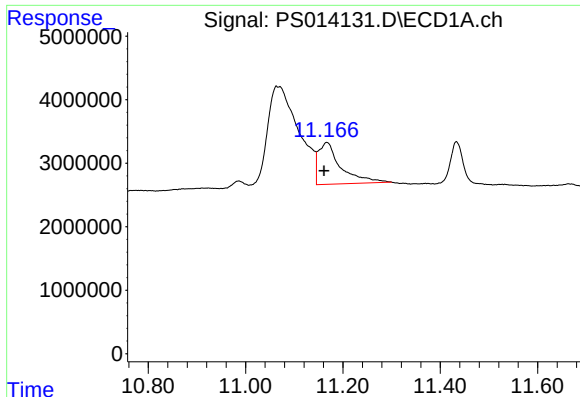

#14 DINOSEB


R.T.: 11.167 min
Delta R.T.: 0.006 min
Response: 21098427
Conc: 4.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

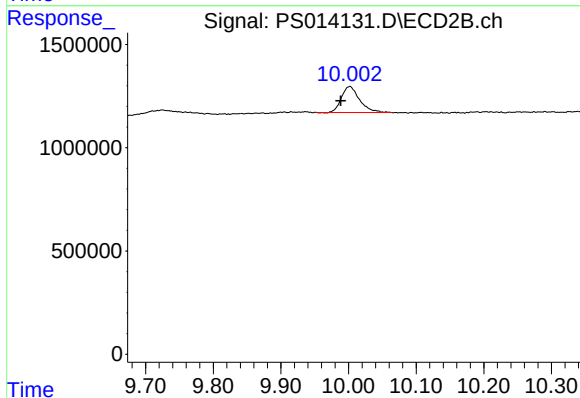


#14 DINOSEB

R.T.: 10.002 min
Delta R.T.: 0.013 min
Response: 2358151
Conc: 1.46 ng/ml

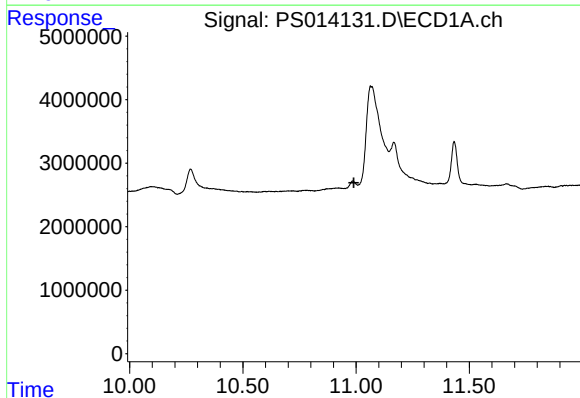


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.990 min
Response: 0
Conc: N.D.

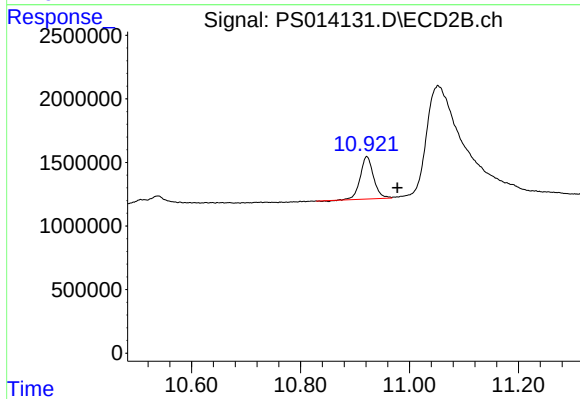

#15 Picloram


R.T.: 10.922 min
Delta R.T.: -0.056 min
Response: 5642809
Conc: 1.64 ng/ml

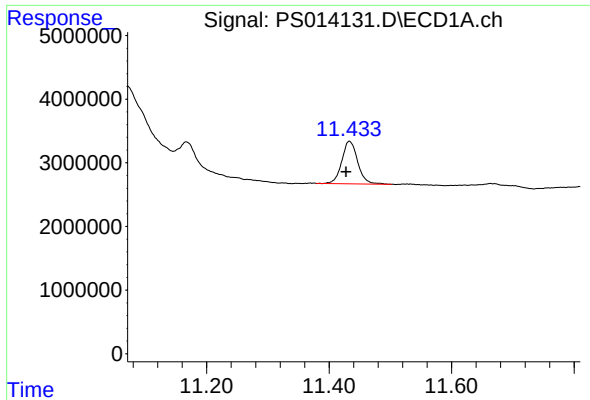

#16 DCPA

R.T.: 11.433 min
Delta R.T.: 0.005 min
Response: 12041641
Conc: 1.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

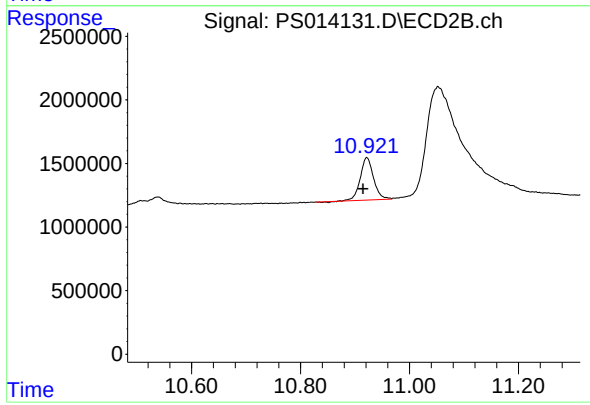

#16 DCPA

R.T.: 10.922 min
Delta R.T.: 0.007 min
Response: 5642809
Conc: 1.65 ng/ml