

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030422\
 Data File : PS018497.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2022 10:04
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 21:44:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.026	6.638	620.7E6	325.0E6	372.998	487.716 #
Target Compounds							
5) T	DICAMBA	0.000	6.793	0	2366144	N.D.	<MDL
10) T	Pentachlo...	0.000	8.105	0	1765021	N.D.	<MDL
11) T	2,4,5-TP ...	8.970	8.428	2892819	16310322	<MDL	3.951 #
12) T	2,4,5-T	9.271	8.872	15165268	3820353	1.508	<MDL #
14) T	DINOSEB	0.000	9.666	0	3073138	N.D.	1.057
15) T	Picloram	10.755	10.672	5382419	126.0E6	<MDL	21.791 #
16) T	DCPA	11.203	10.581	3805184	2255771	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030422\
Data File : PS018497.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2022 10:04
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 21:44:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

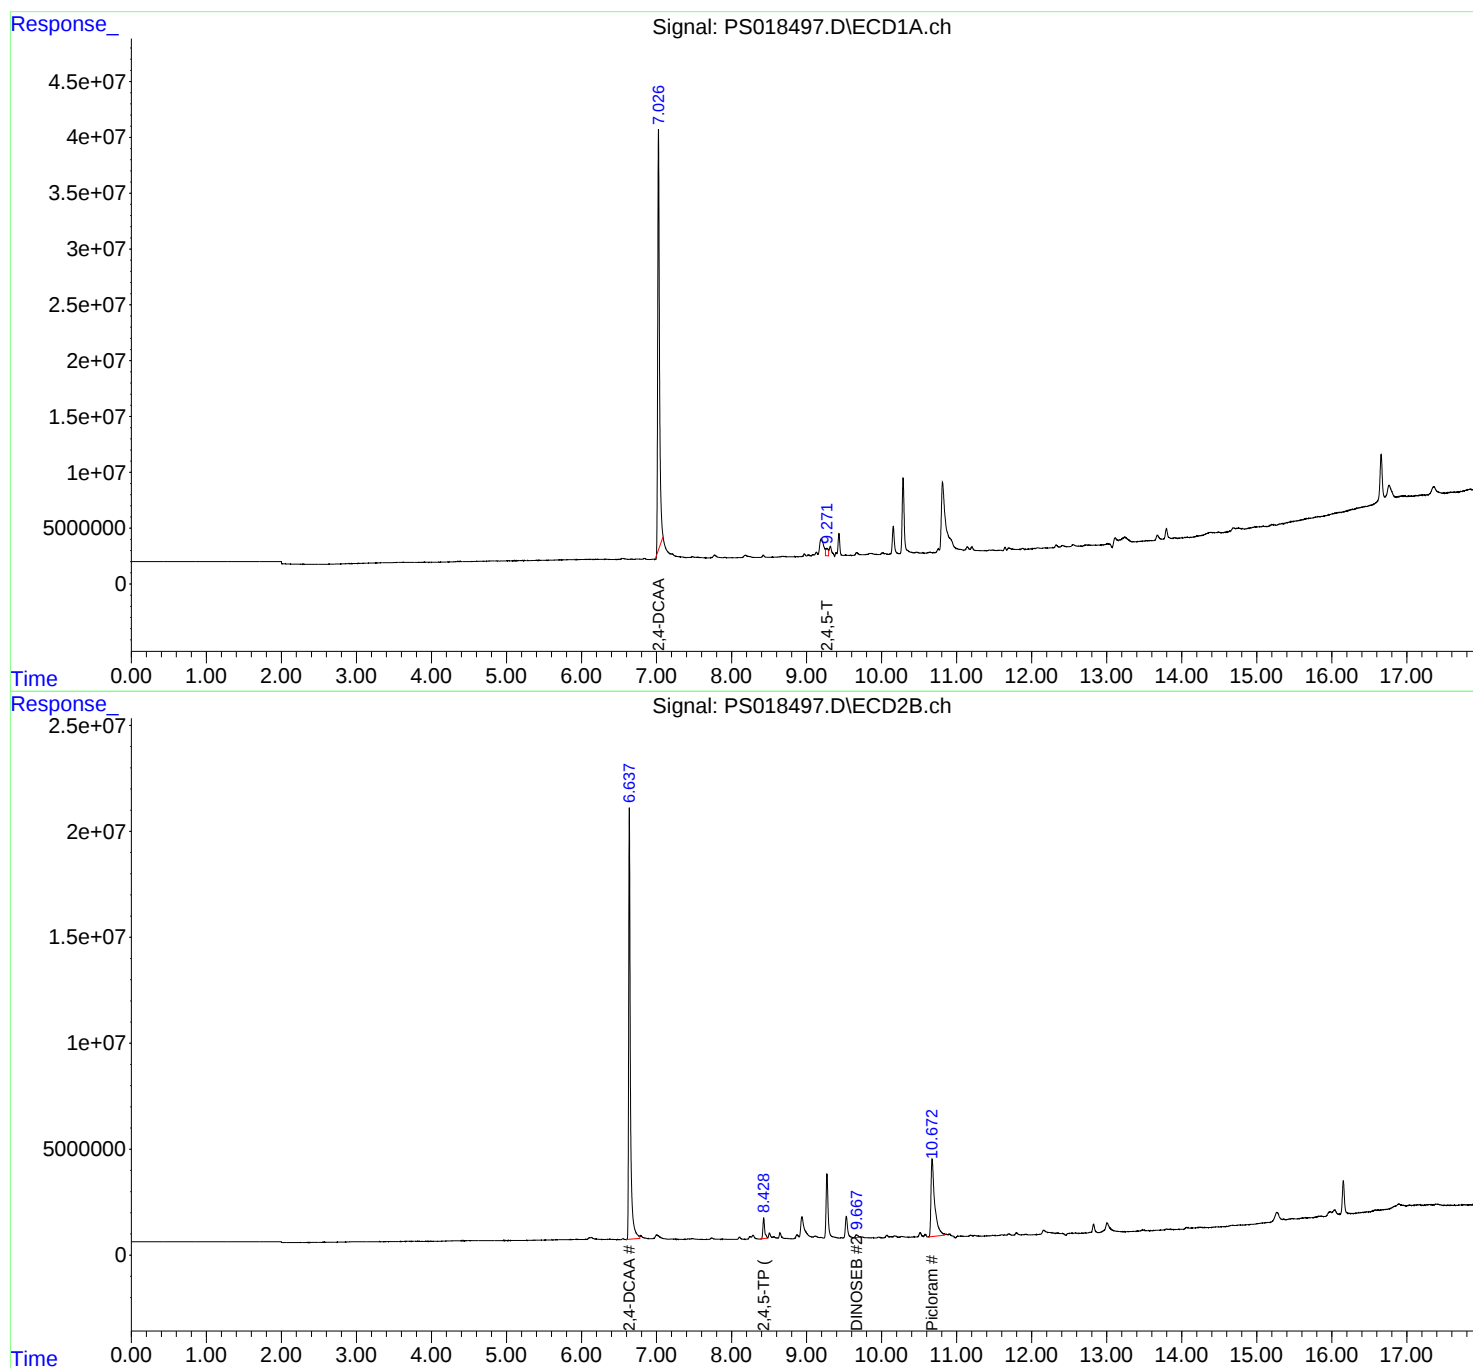


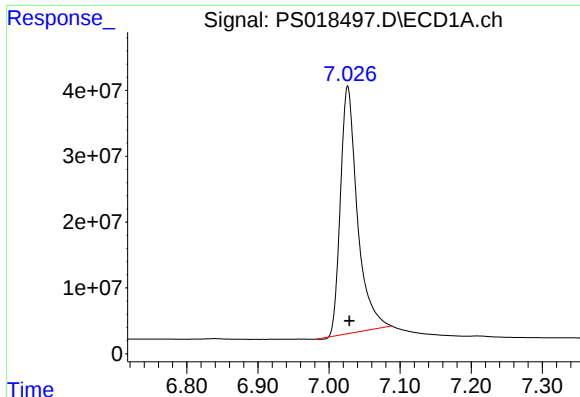

#4 2,4-DCAA


R.T.: 7.026 min
Delta R.T.: -0.002 min
Response: 620687299
Conc: 373.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

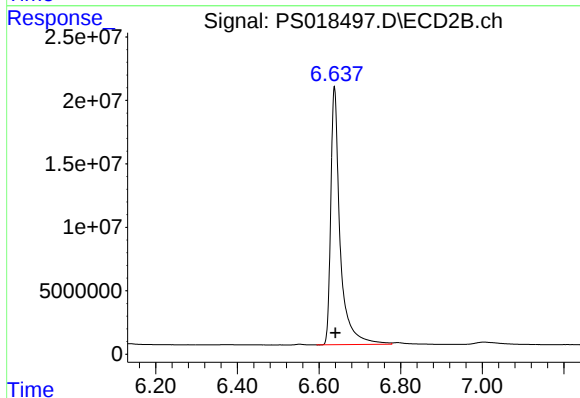


#4 2,4-DCAA

R.T.: 6.638 min
Delta R.T.: -0.002 min
Response: 324985976
Conc: 487.72 ng/ml

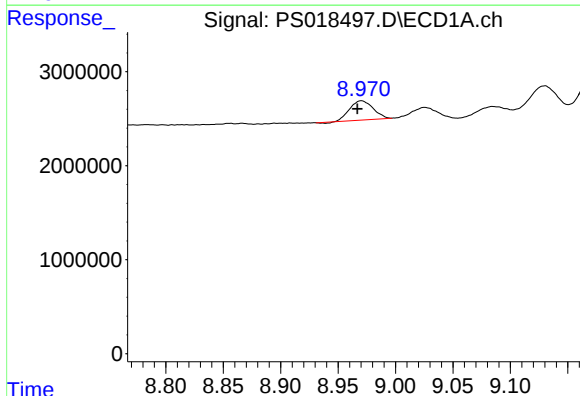


#11 2,4,5-TP (SILVEX)

R.T.: 8.970 min
Delta R.T.: 0.003 min
Response: 2892819
Conc: N.D.

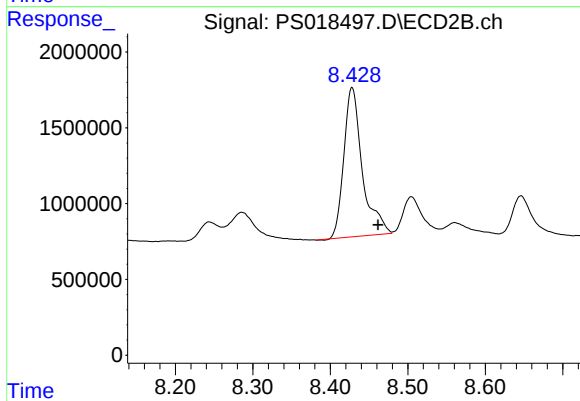

#11 2,4,5-TP (SILVEX)


R.T.: 8.428 min
Delta R.T.: -0.034 min
Response: 16310322
Conc: 3.95 ng/ml

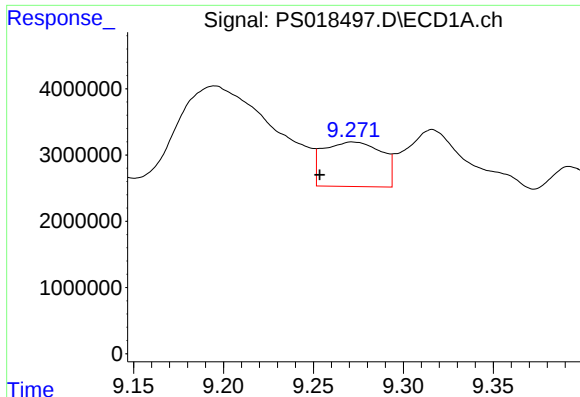

#12 2,4,5-T


R.T.: 9.271 min
Delta R.T.: 0.018 min
Response: 15165268
Conc: 1.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

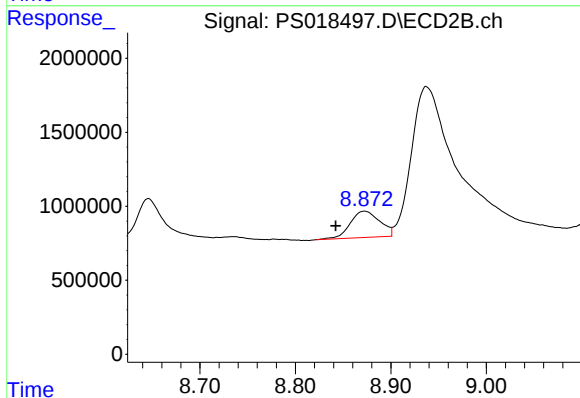


#12 2,4,5-T

R.T.: 8.872 min
Delta R.T.: 0.030 min
Response: 3820353
Conc: N.D.

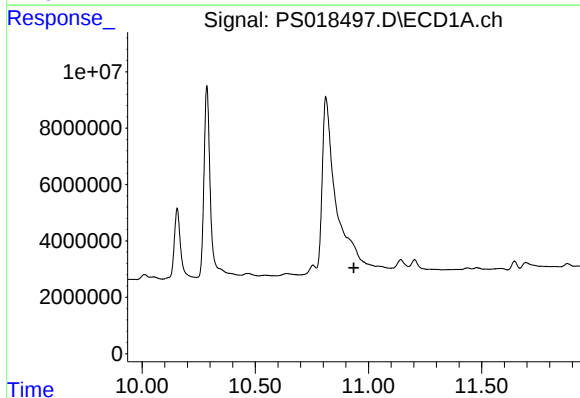


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 10.936 min
Response: 0
Conc: N.D.

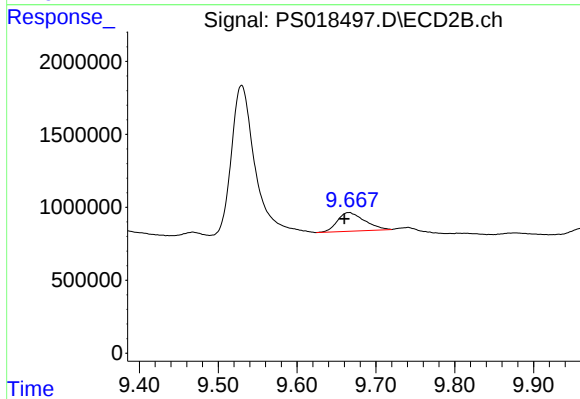

#14 DINOSEB


R.T.: 9.666 min
Delta R.T.: 0.006 min
Response: 3073138
Conc: 1.06 ng/ml

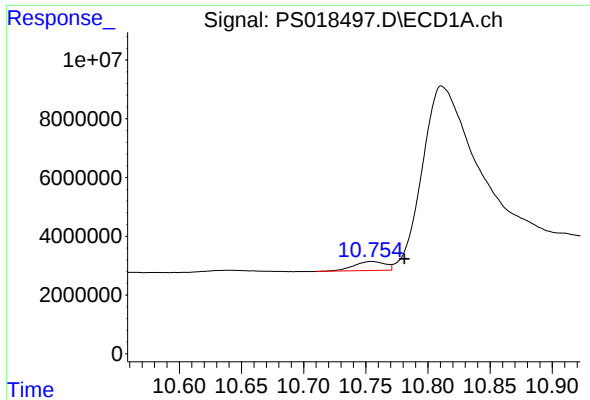

#15 Picloram

R.T.: 10.755 min
Delta R.T.: -0.026 min
Response: 5382419
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

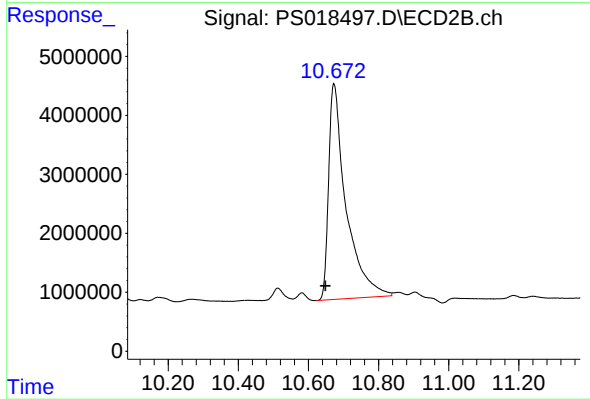

#15 Picloram

R.T.: 10.672 min
Delta R.T.: 0.024 min
Response: 126018156
Conc: 21.79 ng/ml