

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030422\
 Data File : PS018504.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2022 16:01
 Operator : AJ\MA
 Sample : N1726-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 21:46:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
 Quant Title : 8080.M
 QLast Update : Tue Feb 22 00:27:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.021	6.627	585.2E6	398.7E6	351.668	598.309 #
Target Compounds							
1) T	Dalapon	2.944f	2.411	1953708	213.1E6	<MDL	249.378 #
2) T	3,5-DICHL...	6.280	5.872	4271110	215.6E6	1.798	211.524 #
3) T	4-Nitroph...	6.865	6.311	1396.2E6	43140739	1621.805	98.751 #
5) T	DICAMBA	7.176	6.747f	21611465	114.9E6	3.287	40.912 #
6) T	MCP	7.413f	6.860	28205162	36886506	5.827	16.213 #
7) T	MCPA	7.510	7.070	22855043	35303739	3.250	10.540 #
8) T	DICHLORPROP	7.950f	7.409	184.9E6	43900557	109.345	59.624 #
10) T	Pentachlo...	8.418	8.092	1734.5E6	467.0E6	73.251	49.002 #
11) T	2,4,5-TP ...	9.021f	8.412f	3864.8E6	11001.6E6	405.932	2664.729 #
12) T	2,4,5-T	9.291	8.832	186.6E6	877.2E6	18.555	222.851 #
13) T	2,4-DB	9.773	9.354	1333.1E6	4648.3E6	767.127	8603.560 #
14) T	DINOSEB	10.874f	9.657	44452.6E6	1649.9E6	5721.697	567.563 #
15) T	Picloram	10.740f	10.655	20010.1E6	5159.9E6	1574.852	892.261 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030422\
Data File : PS018504.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2022 16:01
Operator : AJ\MA
Sample : N1726-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 21:46:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022122.M
Quant Title : 8080.M
QLast Update : Tue Feb 22 00:27:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

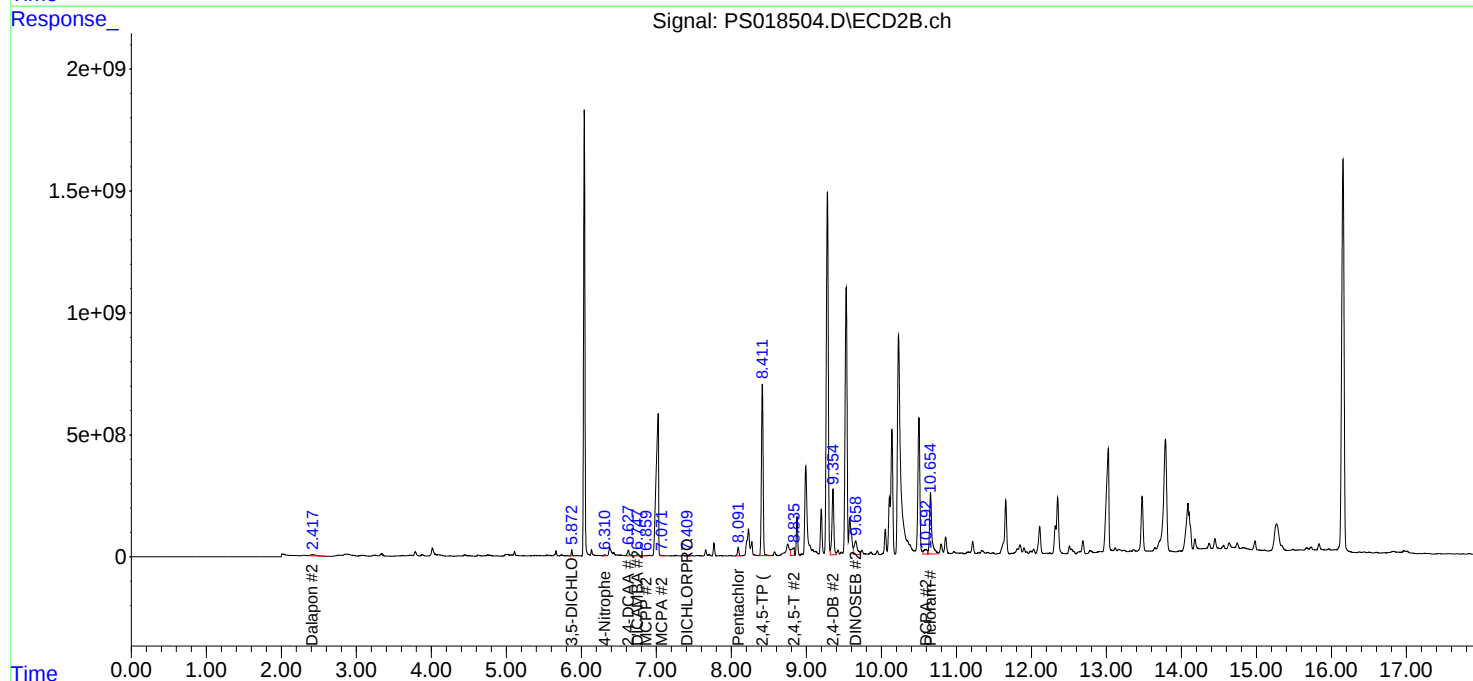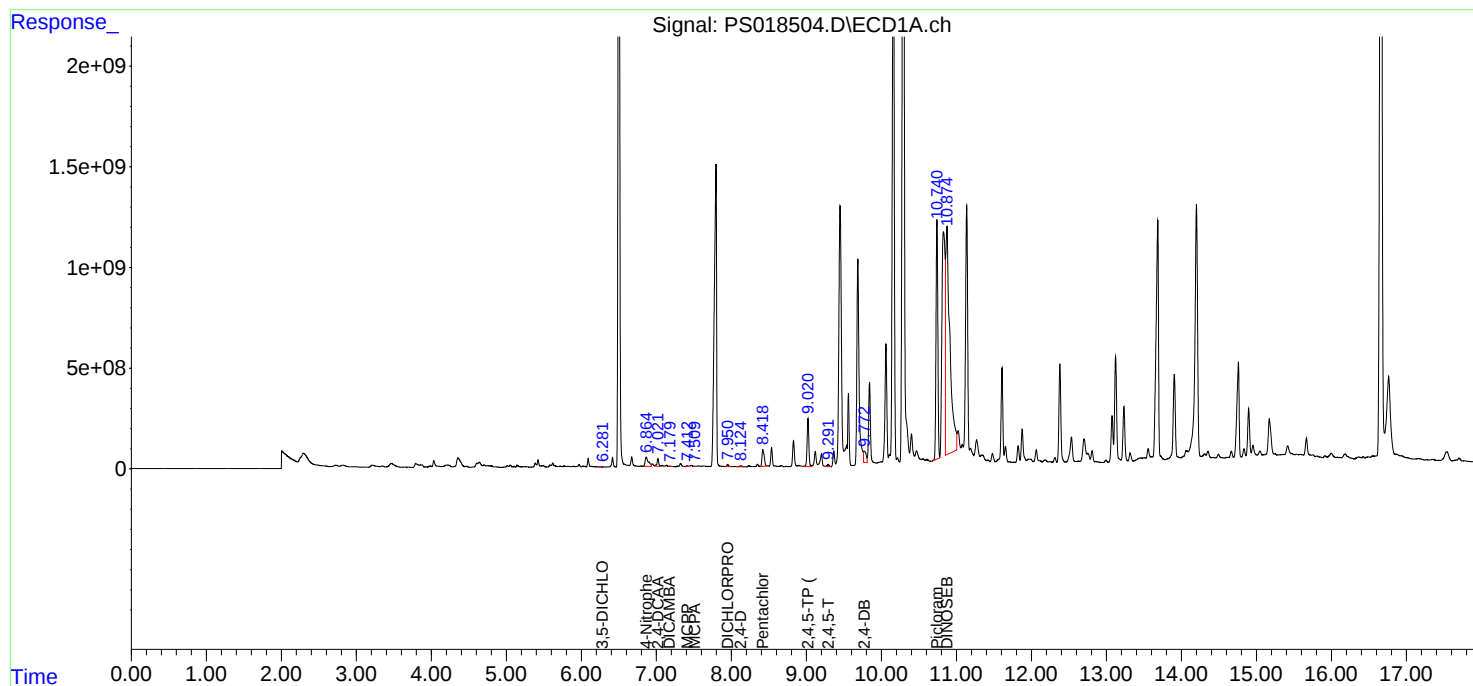


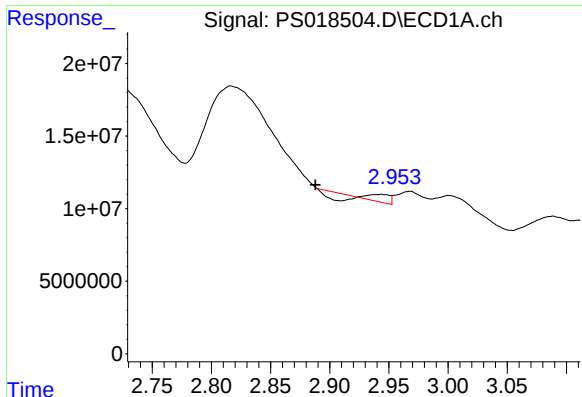

#1 Dalapon


R.T.: 2.944 min
Delta R.T.: 0.056 min
Response: 1953708
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

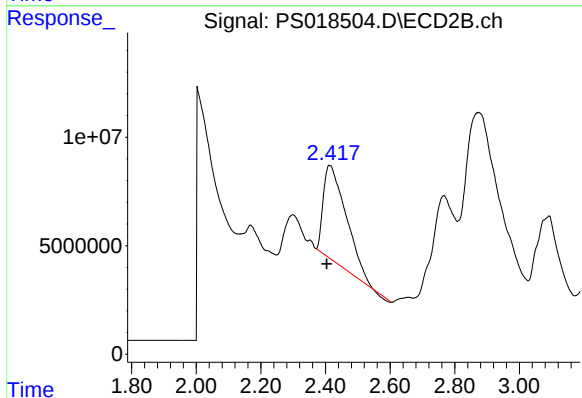


#1 Dalapon

R.T.: 2.411 min
Delta R.T.: 0.007 min
Response: 213078985
Conc: 249.38 ng/ml

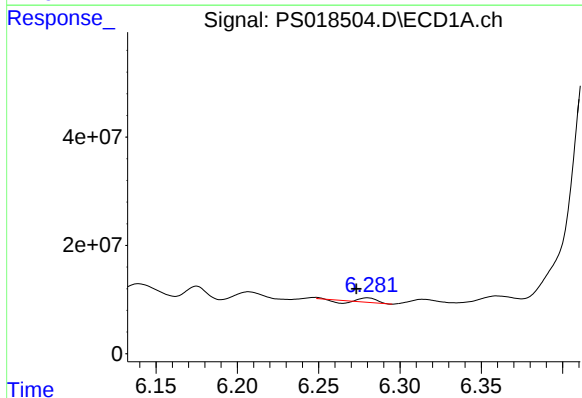


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.280 min
Delta R.T.: 0.007 min
Response: 4271110
Conc: 1.80 ng/ml

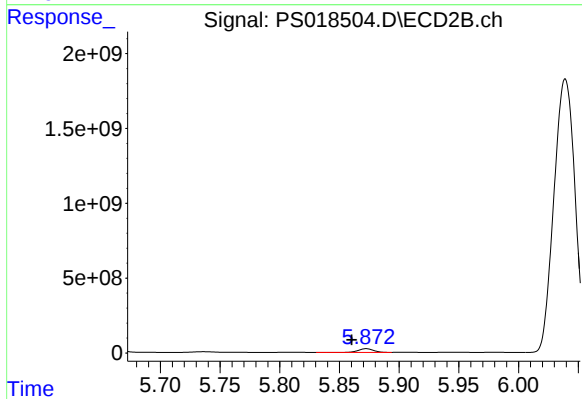

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.872 min
Delta R.T.: 0.012 min
Response: 215645800
Conc: 211.52 ng/ml

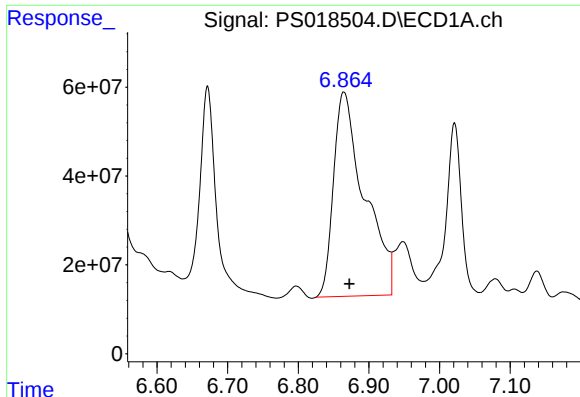

#3 4-Nitrophenol


R.T.: 6.865 min
Delta R.T.: -0.008 min
Response: 1396189155
Conc: 1621.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

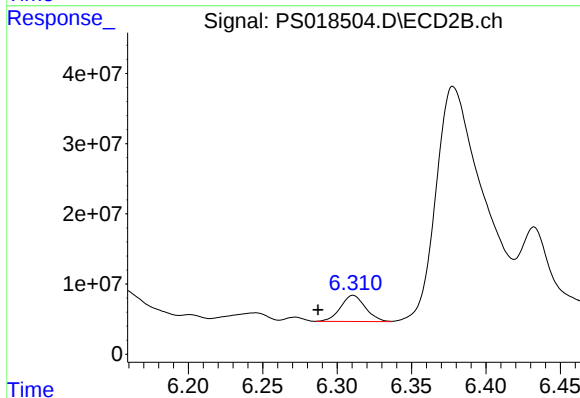


#3 4-Nitrophenol

R.T.: 6.311 min
Delta R.T.: 0.024 min
Response: 43140739
Conc: 98.75 ng/ml

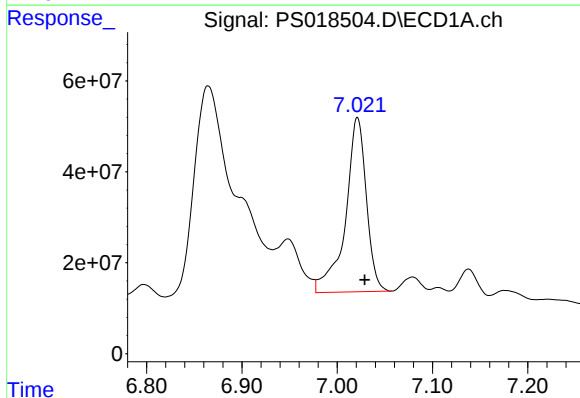


#4 2,4-DCAA

R.T.: 7.021 min
Delta R.T.: -0.007 min
Response: 585193711
Conc: 351.67 ng/ml

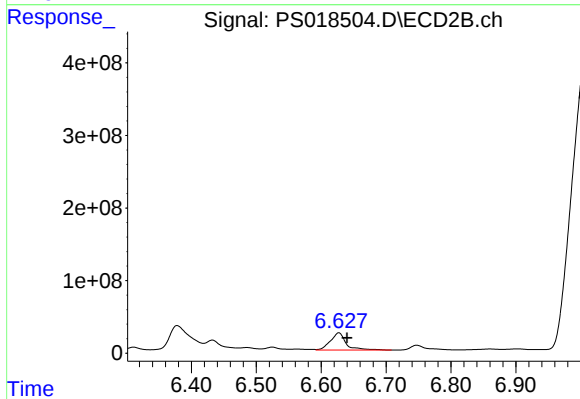

#4 2,4-DCAA


R.T.: 6.627 min
Delta R.T.: -0.013 min
Response: 398678404
Conc: 598.31 ng/ml

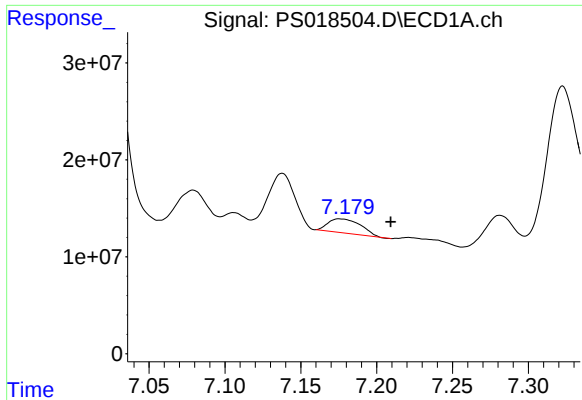

#5 DICAMBA


R.T.: 7.176 min
Delta R.T.: -0.034 min
Response: 21611465
Conc: 3.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

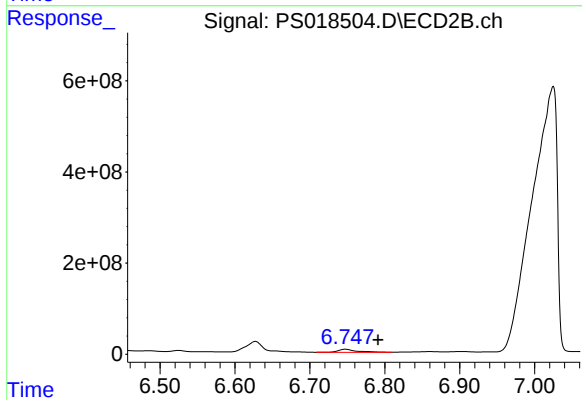


#5 DICAMBA

R.T.: 6.747 min
Delta R.T.: -0.044 min
Response: 114880774
Conc: 40.91 ng/ml

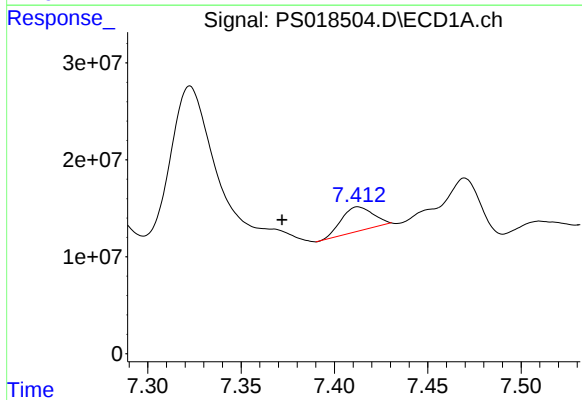


#6 MCP

R.T.: 7.413 min
Delta R.T.: 0.041 min
Response: 28205162
Conc: 5.83 ug/ml

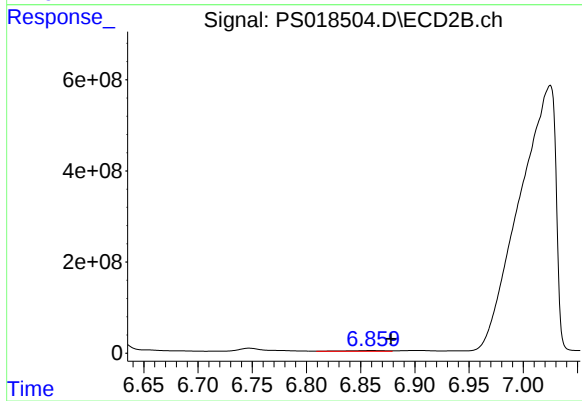

#6 MCP


R.T.: 6.860 min
Delta R.T.: -0.018 min
Response: 36886506
Conc: 16.21 ug/ml

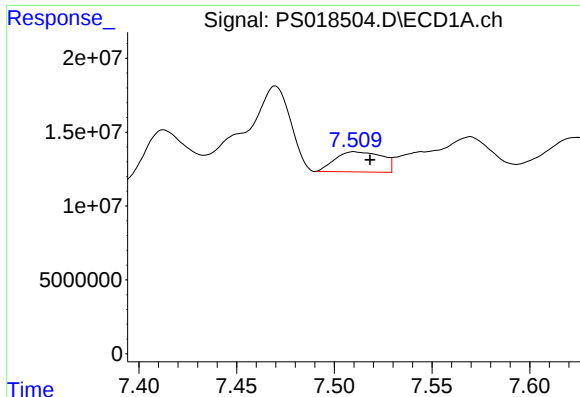

#7 MCPA


R.T.: 7.510 min
Delta R.T.: -0.008 min
Response: 22855043
Conc: 3.25 ug/ml

Instrument :
ECD_S
ClientSampleId :

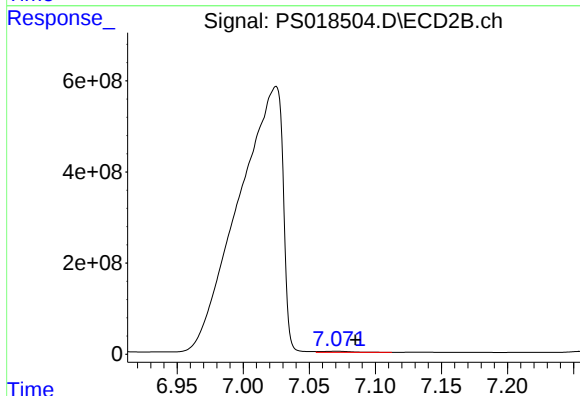


#7 MCPA

R.T.: 7.070 min
Delta R.T.: -0.015 min
Response: 35303739
Conc: 10.54 ug/ml

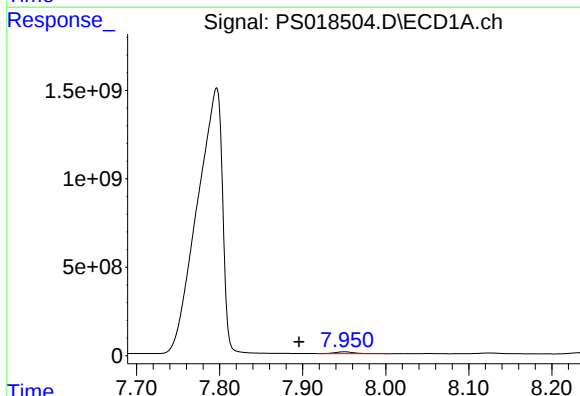


#8 DICHLORPROP

R.T.: 7.950 min
Delta R.T.: 0.054 min
Response: 184927912
Conc: 109.34 ng/ml

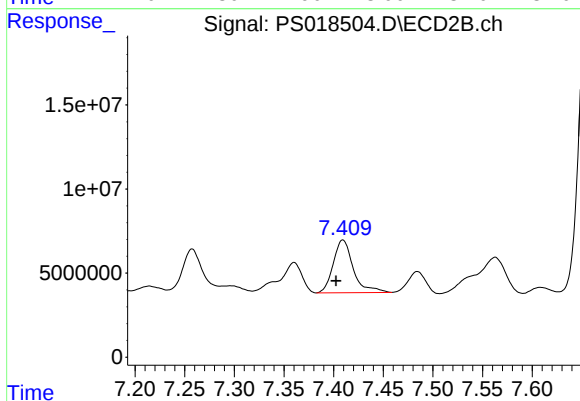

#8 DICHLORPROP


R.T.: 7.409 min
Delta R.T.: 0.007 min
Response: 43900557
Conc: 59.62 ng/ml

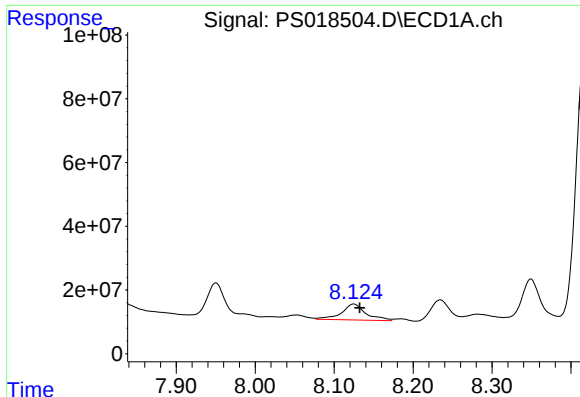

#9 2,4-D


R.T.: 8.125 min
Delta R.T.: -0.008 min
Response: 107344624
Conc: 52.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

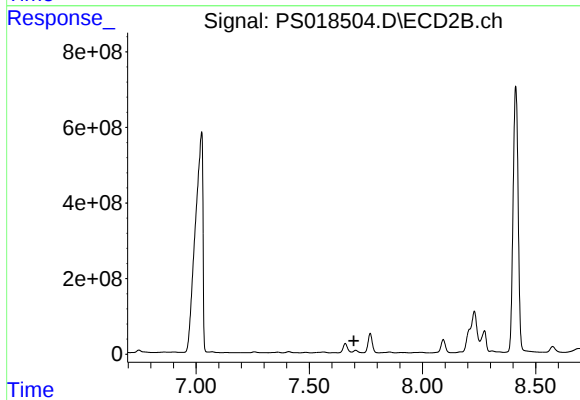


#9 2,4-D

R.T.: 7.705 min
Delta R.T.: 0.007 min
Response: -236069968
Conc: N.D.

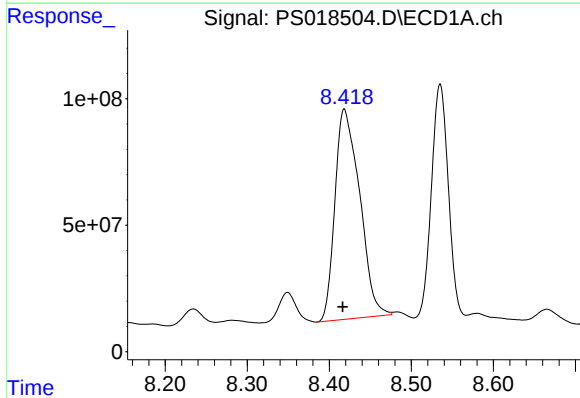


#10 Pentachlorophenol

R.T.: 8.418 min
Delta R.T.: 0.002 min
Response: 1734485792
Conc: 73.25 ng/ml

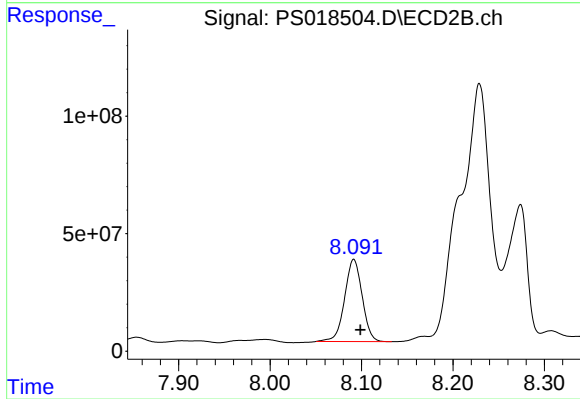

#10 Pentachlorophenol


R.T.: 8.092 min
Delta R.T.: -0.007 min
Response: 467044520
Conc: 49.00 ng/ml

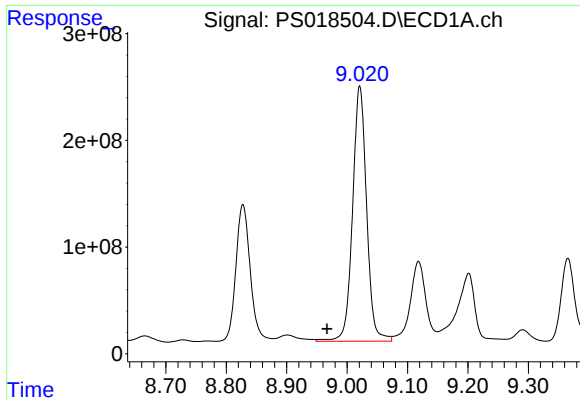

#11 2,4,5-TP (SILVEX)


R.T.: 9.021 min
Delta R.T.: 0.054 min
Response: 3864811633
Conc: 405.93 ng/ml

Instrument :
ECD_S
ClientSampleId :

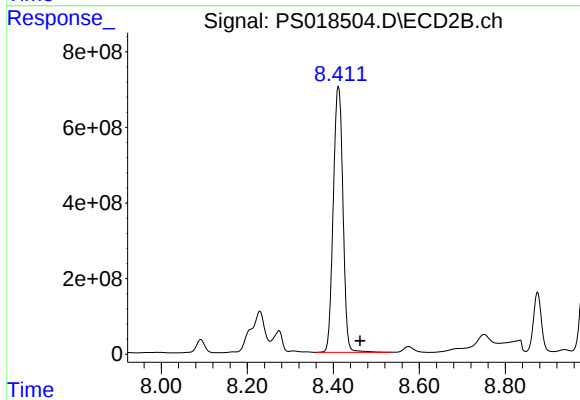


#11 2,4,5-TP (SILVEX)

R.T.: 8.412 min
Delta R.T.: -0.050 min
Response: 11001578328
Conc: 2664.73 ng/ml

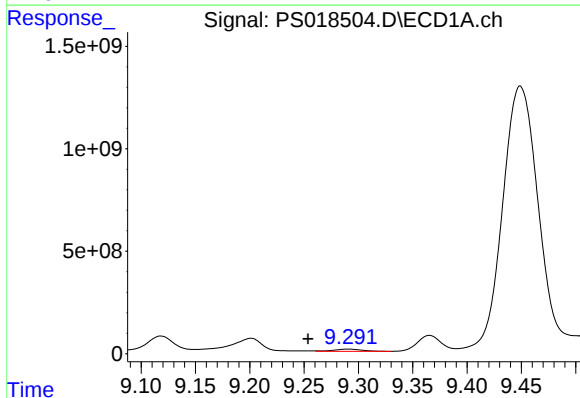


#12 2,4,5-T

R.T.: 9.291 min
Delta R.T.: 0.037 min
Response: 186649586
Conc: 18.56 ng/ml

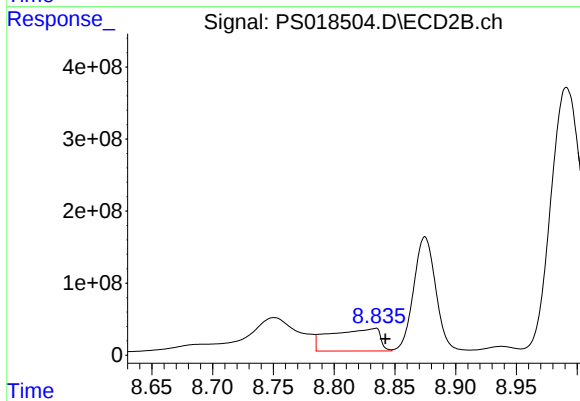

#12 2,4,5-T


R.T.: 8.832 min
Delta R.T.: -0.010 min
Response: 877197932
Conc: 222.85 ng/ml

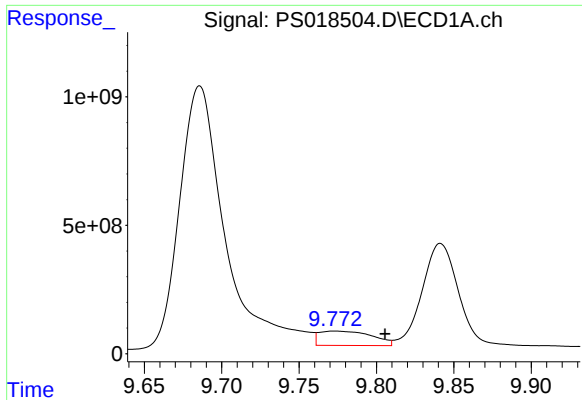

#13 2,4-DB


R.T.: 9.773 min
Delta R.T.: -0.032 min
Response: 1333118258
Conc: 767.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

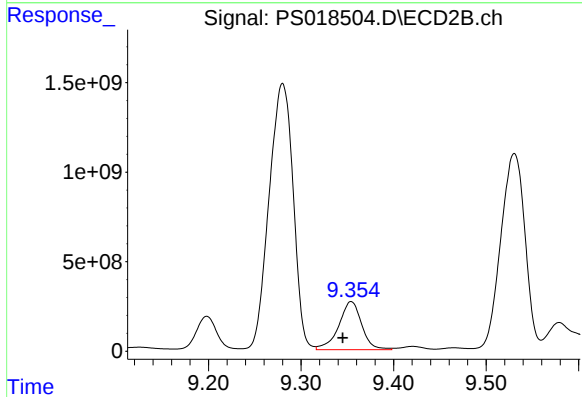


#13 2,4-DB

R.T.: 9.354 min
Delta R.T.: 0.009 min
Response: 4648253486
Conc: 8603.56 ng/ml

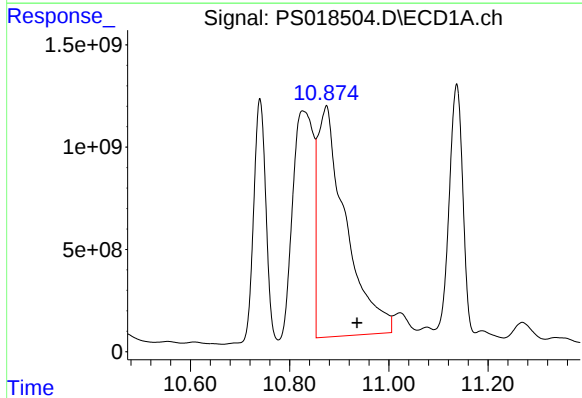


#14 DINOSEB

R.T.: 10.874 min
Delta R.T.: -0.062 min
Response: 44452585260
Conc: 5721.70 ng/ml

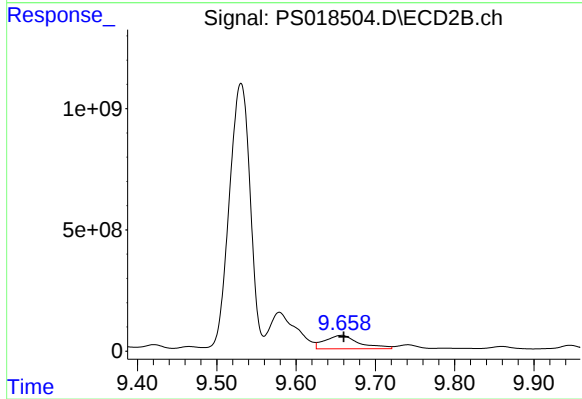

#14 DINOSEB


R.T.: 9.657 min
Delta R.T.: -0.003 min
Response: 1649905200
Conc: 567.56 ng/ml

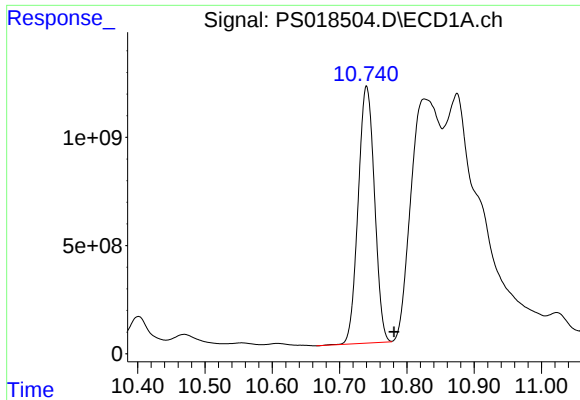

#15 Picloram


R.T.: 10.740 min
Delta R.T.: -0.041 min
Response: 20010134673
Conc: 1574.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

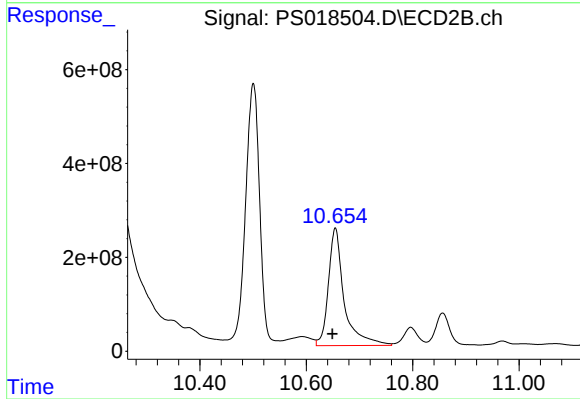


#15 Picloram

R.T.: 10.655 min
Delta R.T.: 0.006 min
Response: 5159911248
Conc: 892.26 ng/ml

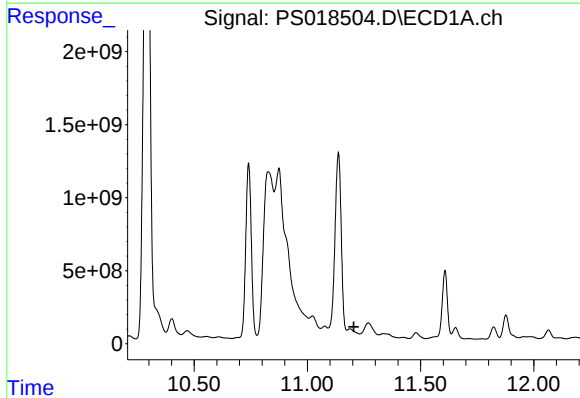

#16 DCPA

R.T.: 11.188 min
Delta R.T.: -0.017 min
Response: -7486804796
Conc: N.D.

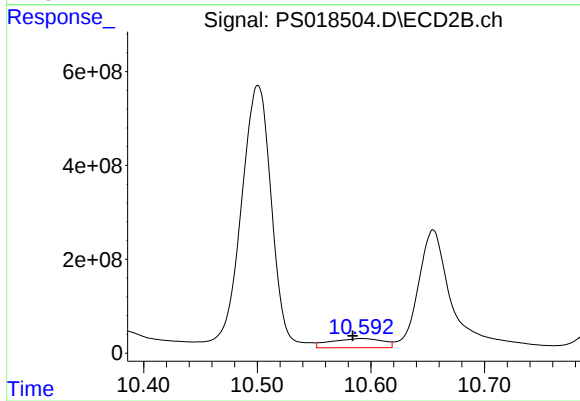

#16 DCPA

R.T.: 10.592 min
Delta R.T.: 0.008 min
Response: 620890445
Conc: 125.05 ng/ml