

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030520\
 Data File : PS009131.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2020 12:49
 Operator : DD\AJ
 Sample : L1775-05RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 CR-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 13:55:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 20 11:30:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.249	6.936	796.2E6	432.8E6	364.136	449.157
Target Compounds							
2) T	3,5-DICHL...	0.000	6.111	0	122.3E6	N.D.	83.808
5) T	DICAMBA	0.000	7.071	0	26803785	N.D.	6.475
8) T	DICHLORPROP	0.000	7.757	0	87387417	N.D.	87.219
9) T	2,4-D	8.304	0.000	133.3E6	0	64.321	N.D. #
11) T	2,4,5-TP ...	0.000	8.790	0	93961284	N.D.	17.346
12) T	2,4,5-T	9.455	9.204	79924758	13142885	7.475	2.428 #
15) T	Picloram	11.046	11.027	520.9E6	310.9E6	38.046	42.783
16) T	DCPA	0.000	10.978	0	21654718	N.D.	3.130



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030520\
Data File : PS009131.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2020 12:49
Operator : DD\AJ
Sample : L1775-05RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
CR-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 13:55:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022020.M
Quant Title : 8080.M
QLast Update : Thu Feb 20 11:30:26 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

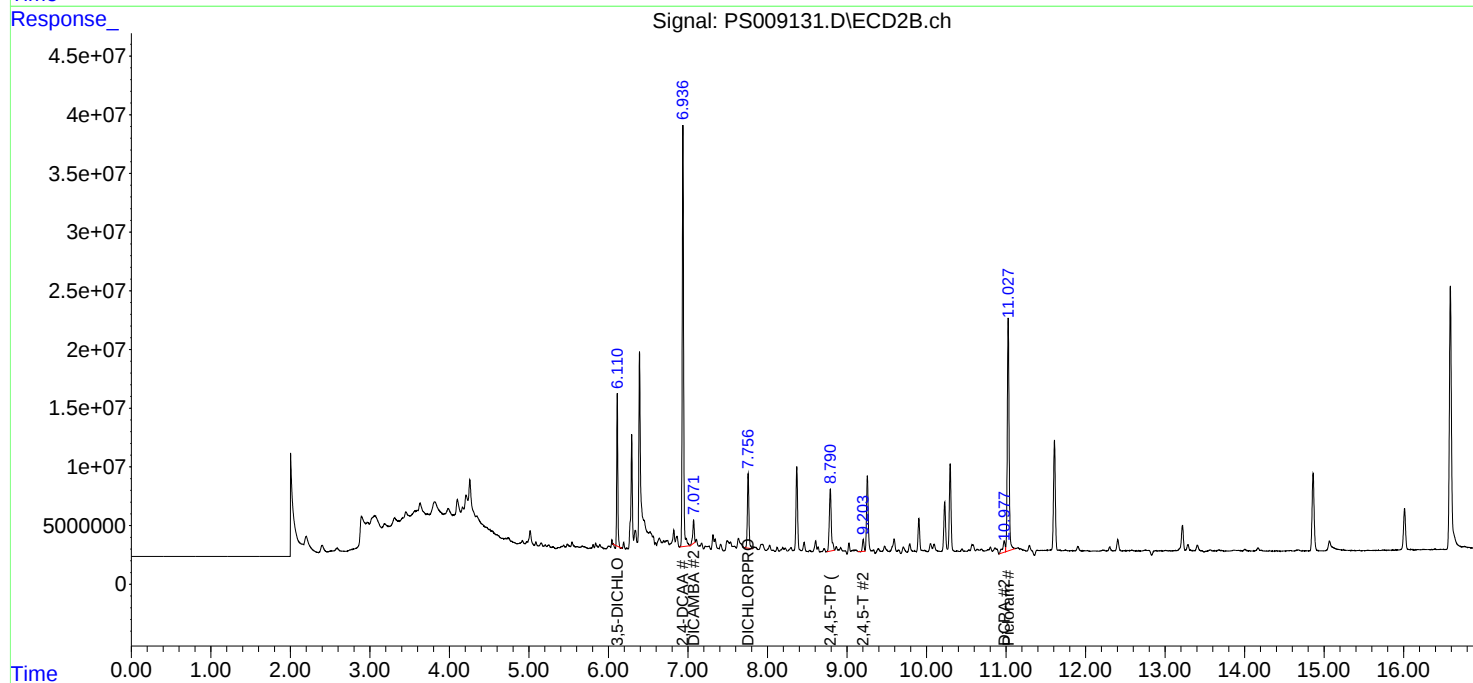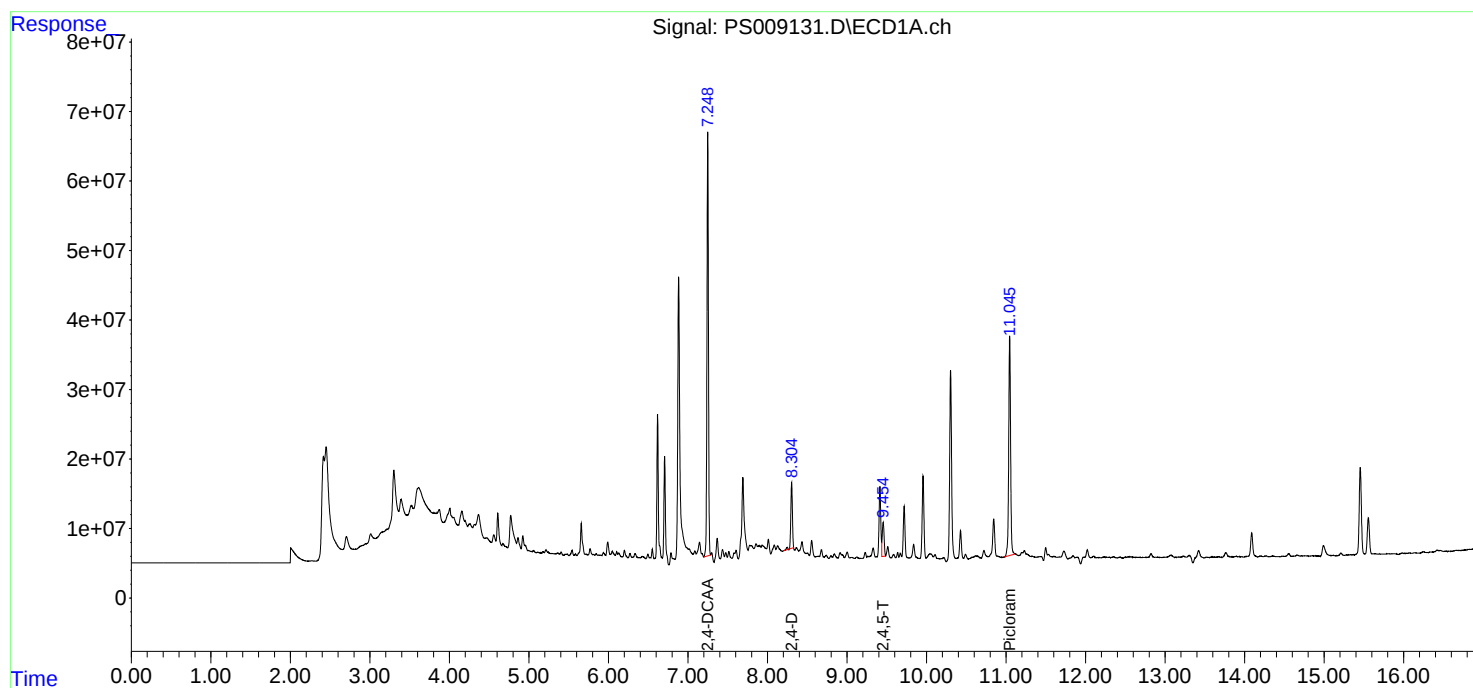


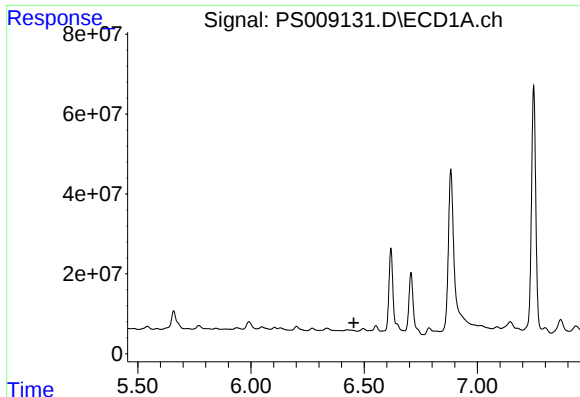

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.455 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CR-1

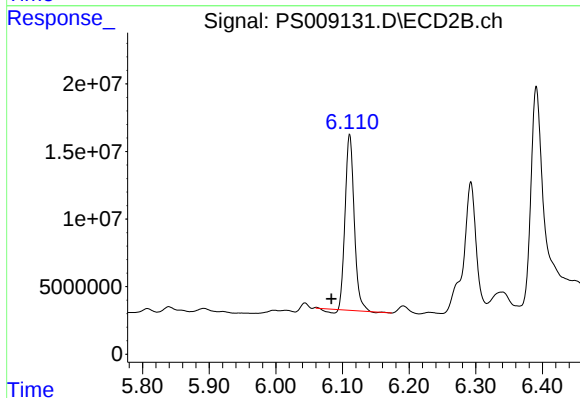


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.111 min
Delta R.T.: 0.027 min
Response: 122298079
Conc: 83.81 ng/ml

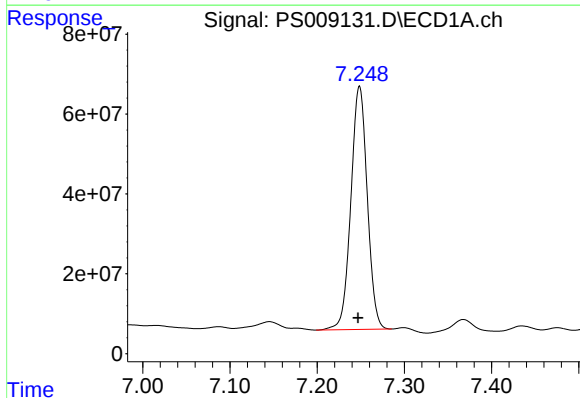


#4 2,4-DCAA

R.T.: 7.249 min
Delta R.T.: 0.002 min
Response: 796217093
Conc: 364.14 ng/ml

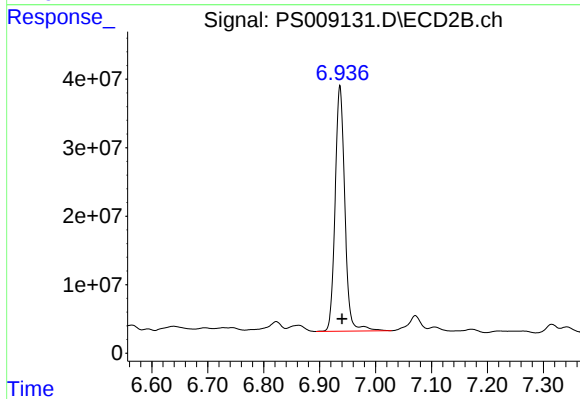

#4 2,4-DCAA


R.T.: 6.936 min
Delta R.T.: -0.004 min
Response: 432787778
Conc: 449.16 ng/ml

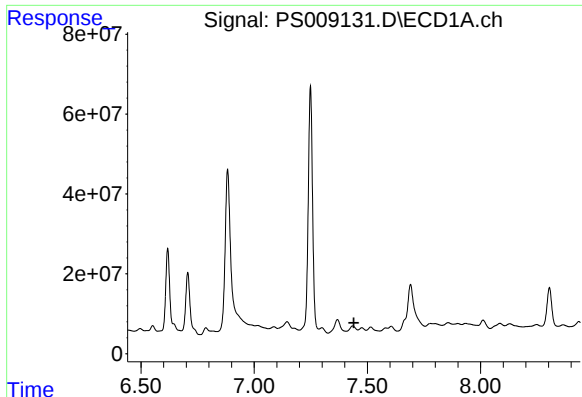

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.440 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CR-1

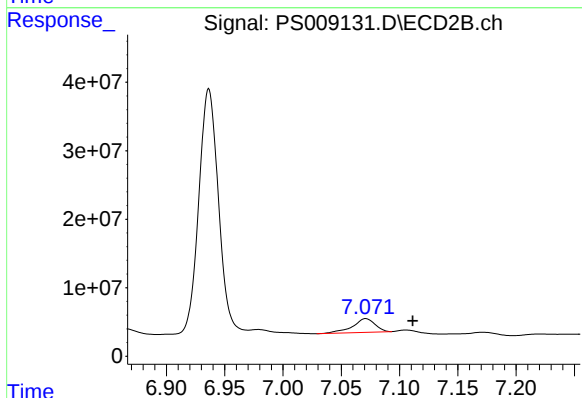


#5 DICAMBA

R.T.: 7.071 min
Delta R.T.: -0.040 min
Response: 26803785
Conc: 6.48 ng/ml

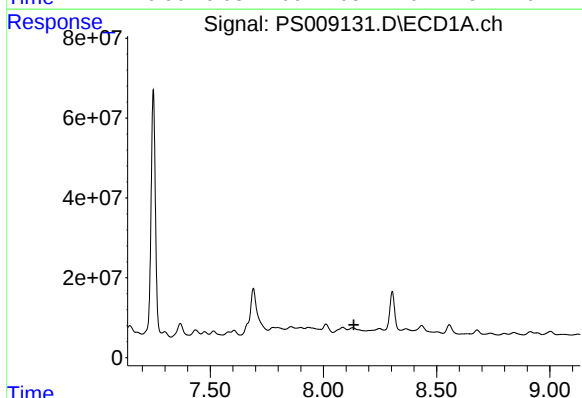


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.135 min
Response: 0
Conc: N.D.

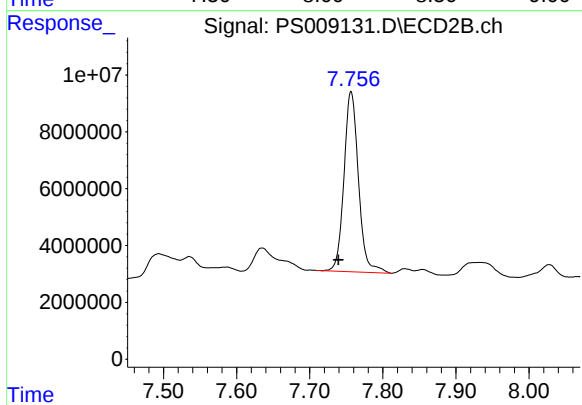

#8 DICHLORPROP


R.T.: 7.757 min
Delta R.T.: 0.018 min
Response: 87387417
Conc: 87.22 ng/ml

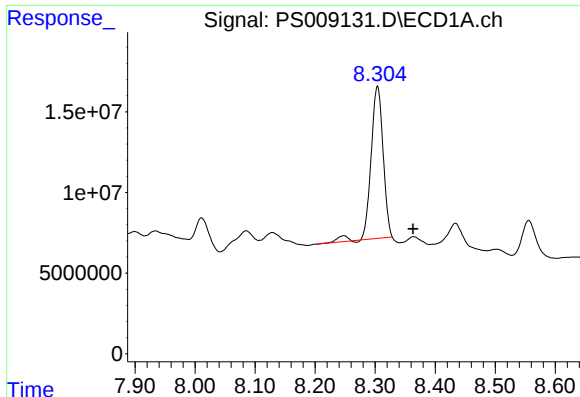

#9 2,4-D


R.T.: 8.304 min
Delta R.T.: -0.059 min
Response: 133294547
Conc: 64.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
CR-1

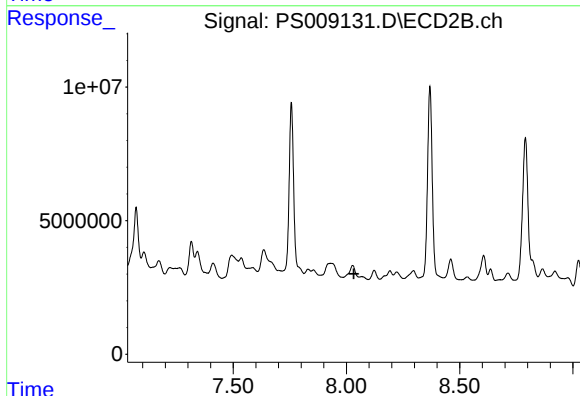


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.033 min
Response: 0
Conc: N.D.

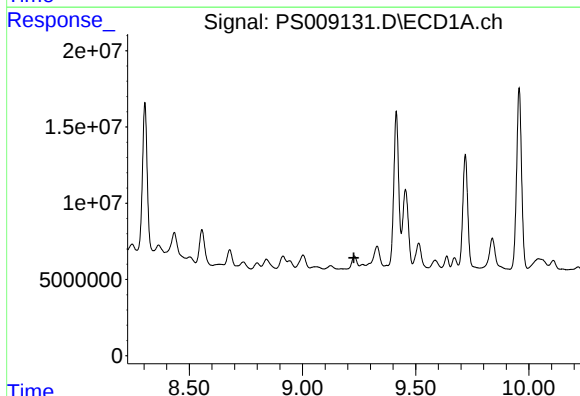


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.227 min
Response: 0
Conc: N.D.

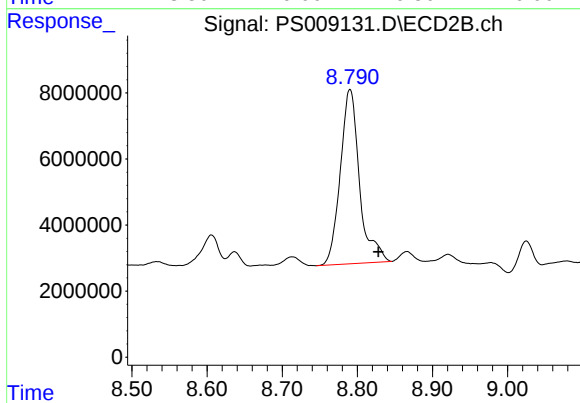

#11 2,4,5-TP (SILVEX)


R.T.: 8.790 min
Delta R.T.: -0.038 min
Response: 93961284
Conc: 17.35 ng/ml

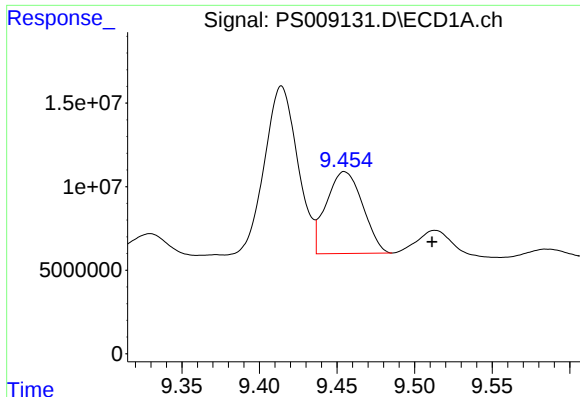

#12 2,4,5-T


R.T.: 9.455 min
Delta R.T.: -0.056 min
Response: 79924758
Conc: 7.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
CR-1

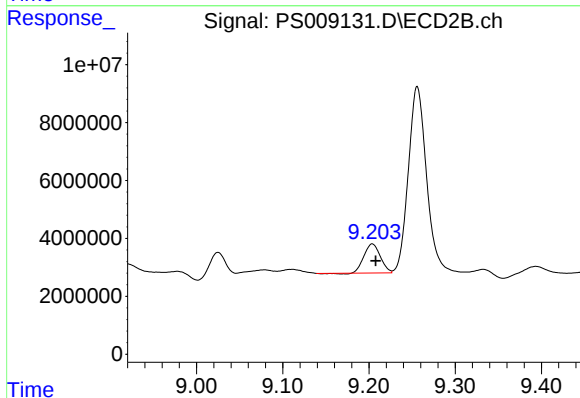


#12 2,4,5-T

R.T.: 9.204 min
Delta R.T.: -0.004 min
Response: 13142885
Conc: 2.43 ng/ml

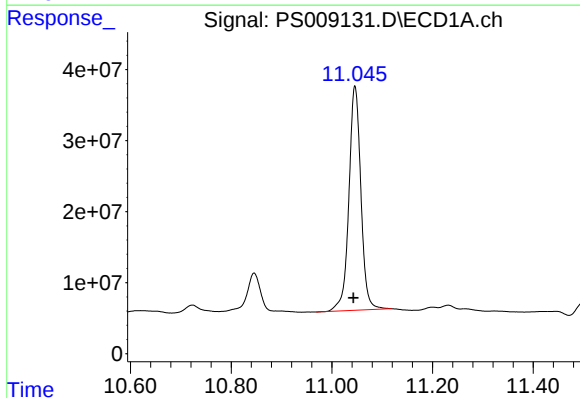


#15 Picloram

R.T.: 11.046 min
Delta R.T.: 0.003 min
Response: 520887573
Conc: 38.05 ng/ml

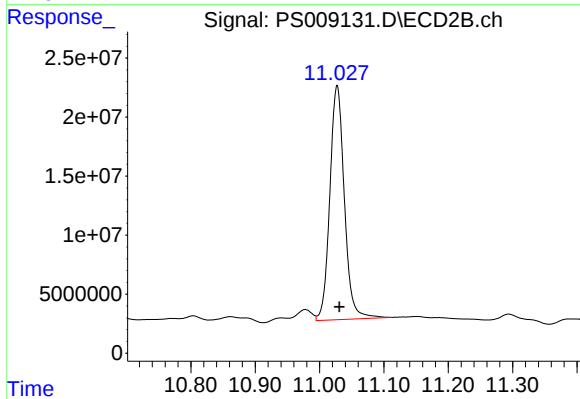

#15 Picloram


R.T.: 11.027 min
Delta R.T.: -0.004 min
Response: 310885211
Conc: 42.78 ng/ml

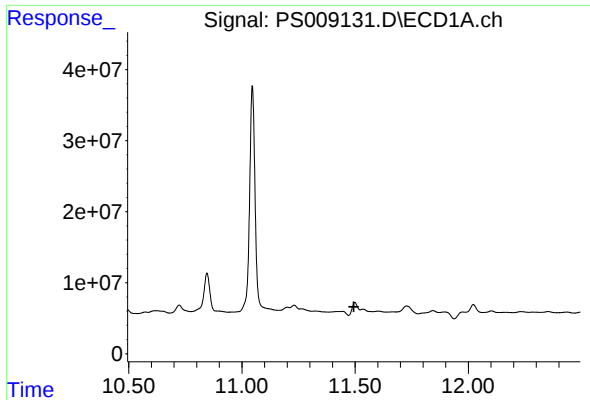

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.495 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
CR-1

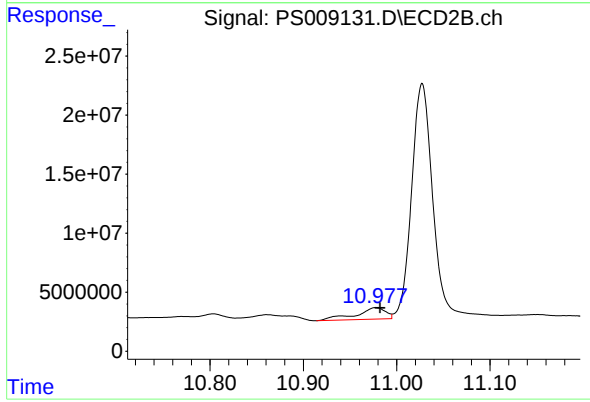

#16 DCPA

R.T.: 10.978 min
Delta R.T.: -0.005 min
Response: 21654718
Conc: 3.13 ng/ml