

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030521\
 Data File : PS014144.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2021 11:31
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 13:19:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030521.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 05 11:52:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.208	6.905	441.1E6	204.8E6	438.028	538.439
Target Compounds							
5) T	DICAMBA	0.000	7.135f	0	1364794	N.D.	<MDL
6) T	MCP	0.000	7.135	0	1364794	N.D.	1.030
12) T	2,4,5-T	9.447	0.000	11381508	0	1.899	N.D. #
15) T	Picloram	0.000	10.922f	0	1910703	N.D.	<MDL
16) T	DCPA	0.000	10.922	0	1910703	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS030521\
Data File : PS014144.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2021 11:31
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 13:19:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS030521.M
Quant Title : 8080.M
QLast Update : Fri Mar 05 11:52:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

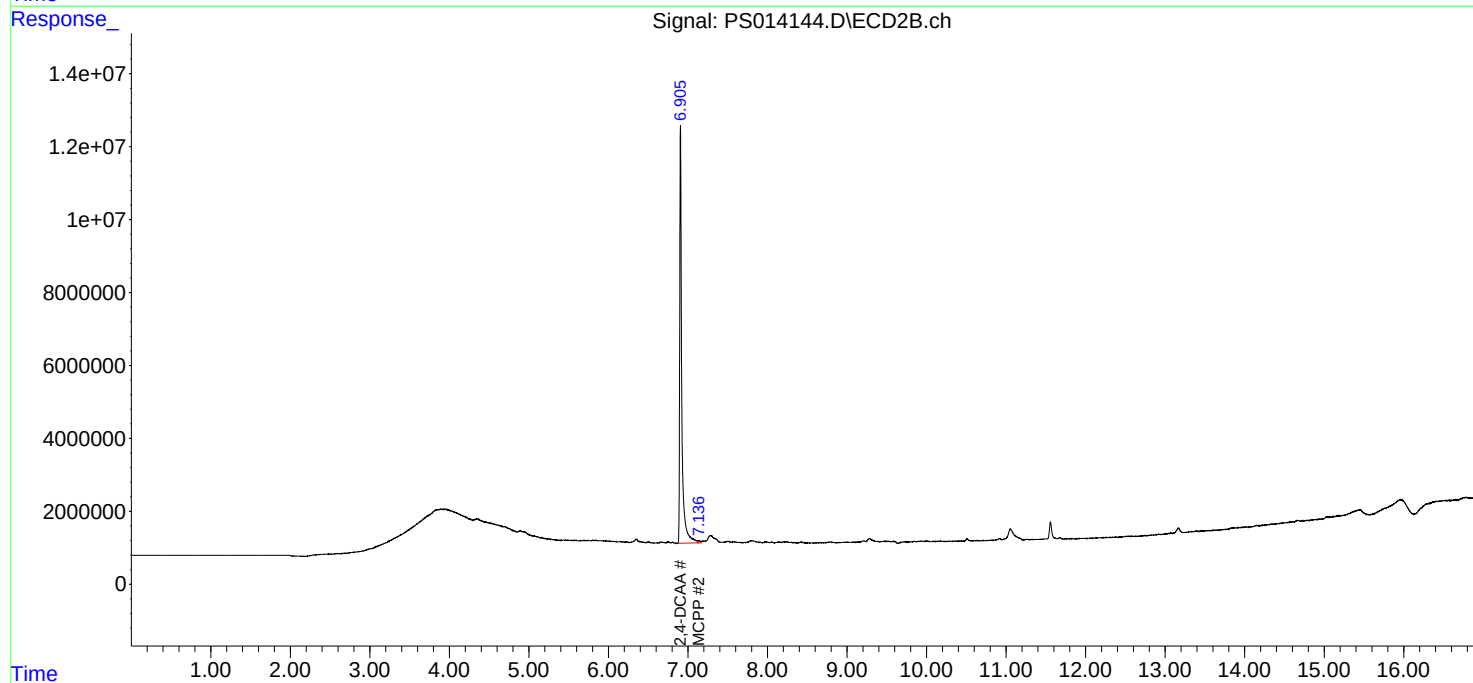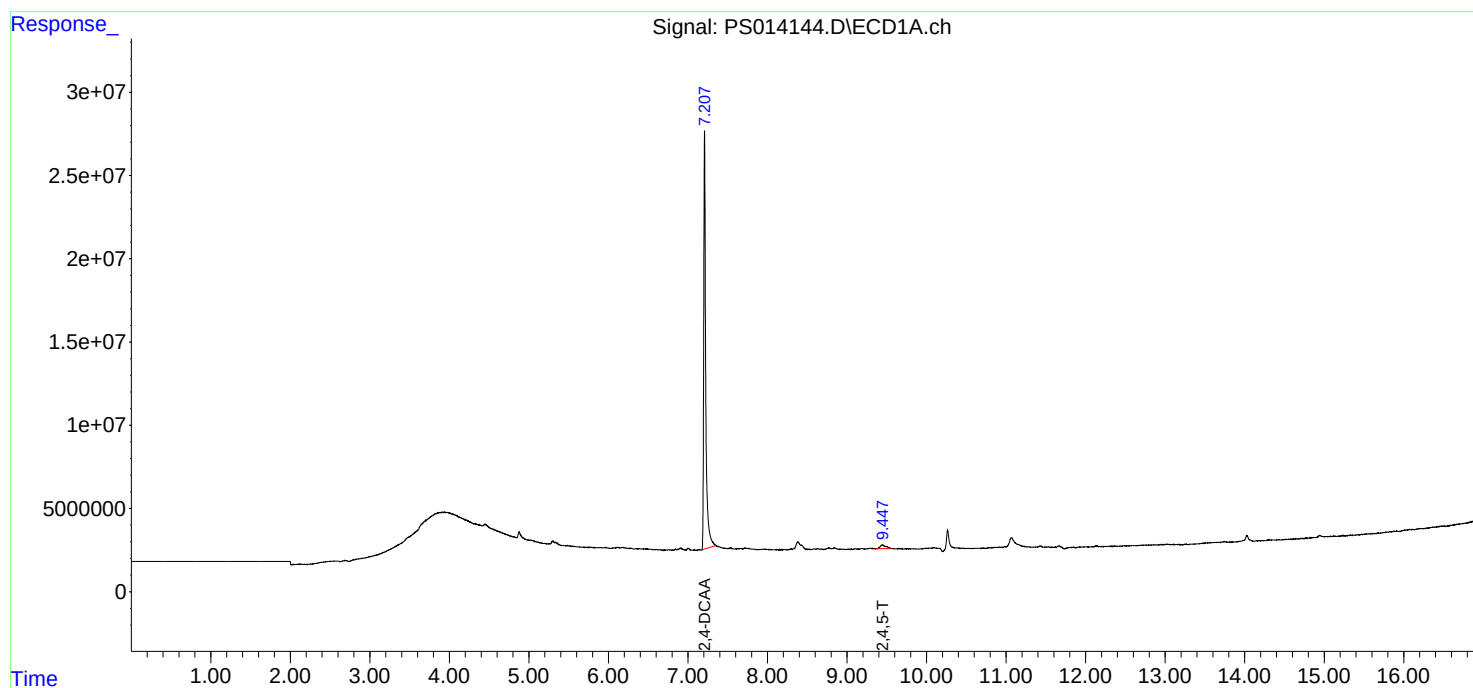


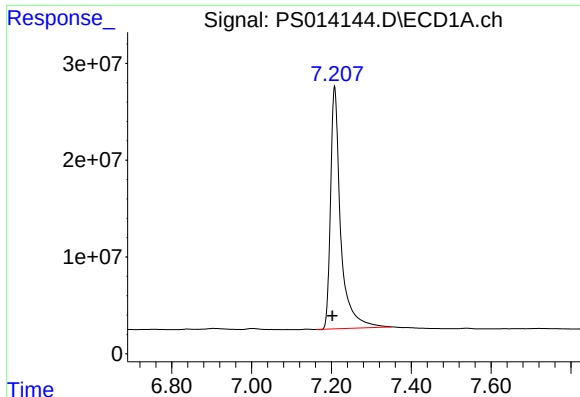

#4 2,4-DCAA


R.T.: 7.208 min
Delta R.T.: 0.006 min
Response: 441083284
Conc: 438.03 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

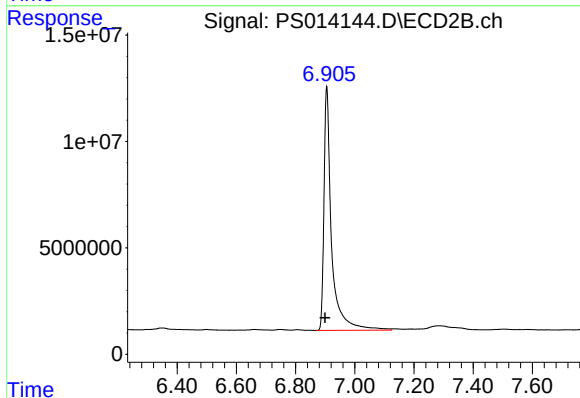


#4 2,4-DCAA

R.T.: 6.905 min
Delta R.T.: 0.006 min
Response: 204847442
Conc: 538.44 ng/ml

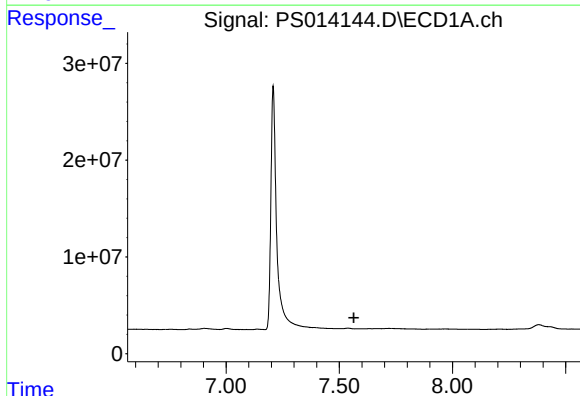


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.565 min
Response: 0
Conc: N.D.

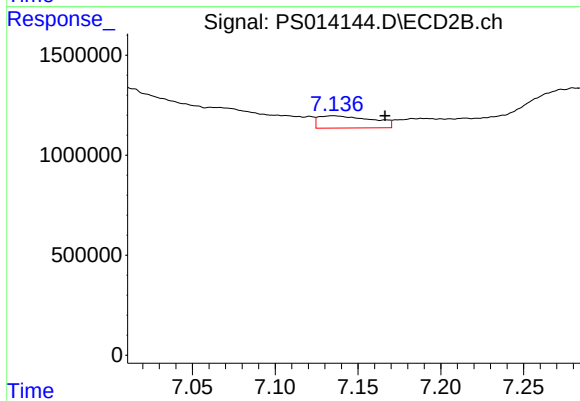

#6 MCP


R.T.: 7.135 min
Delta R.T.: -0.031 min
Response: 1364794
Conc: 1.03 ug/ml

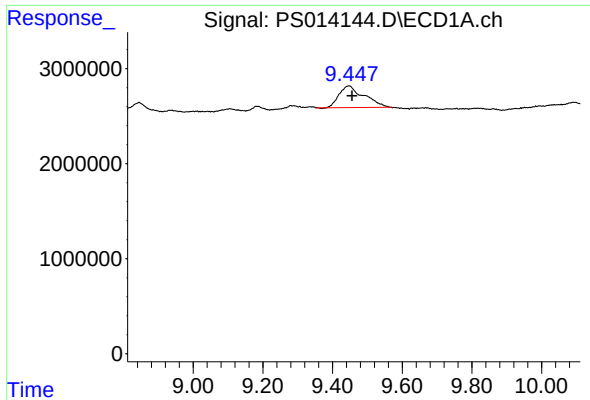

#12 2,4,5-T

R.T.: 9.447 min
Delta R.T.: -0.009 min
Response: 11381508
Conc: 1.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

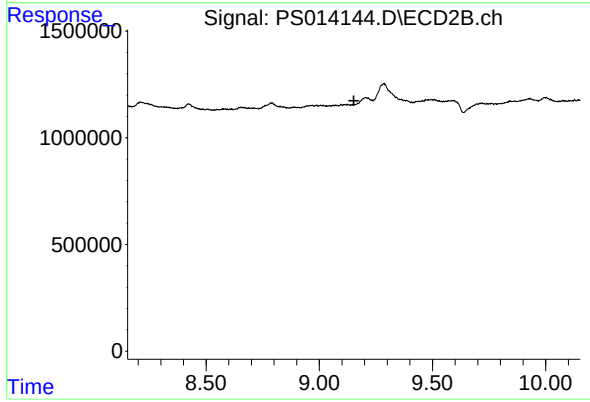

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.152 min
Response: 0
Conc: N.D.